


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041223\
Data File : VN077305.D
Acq On : 12 Apr 2023 09:46
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N040523W.M
Title : SW846 8260
Last Update : Thu Apr 06 08:27:03 2023

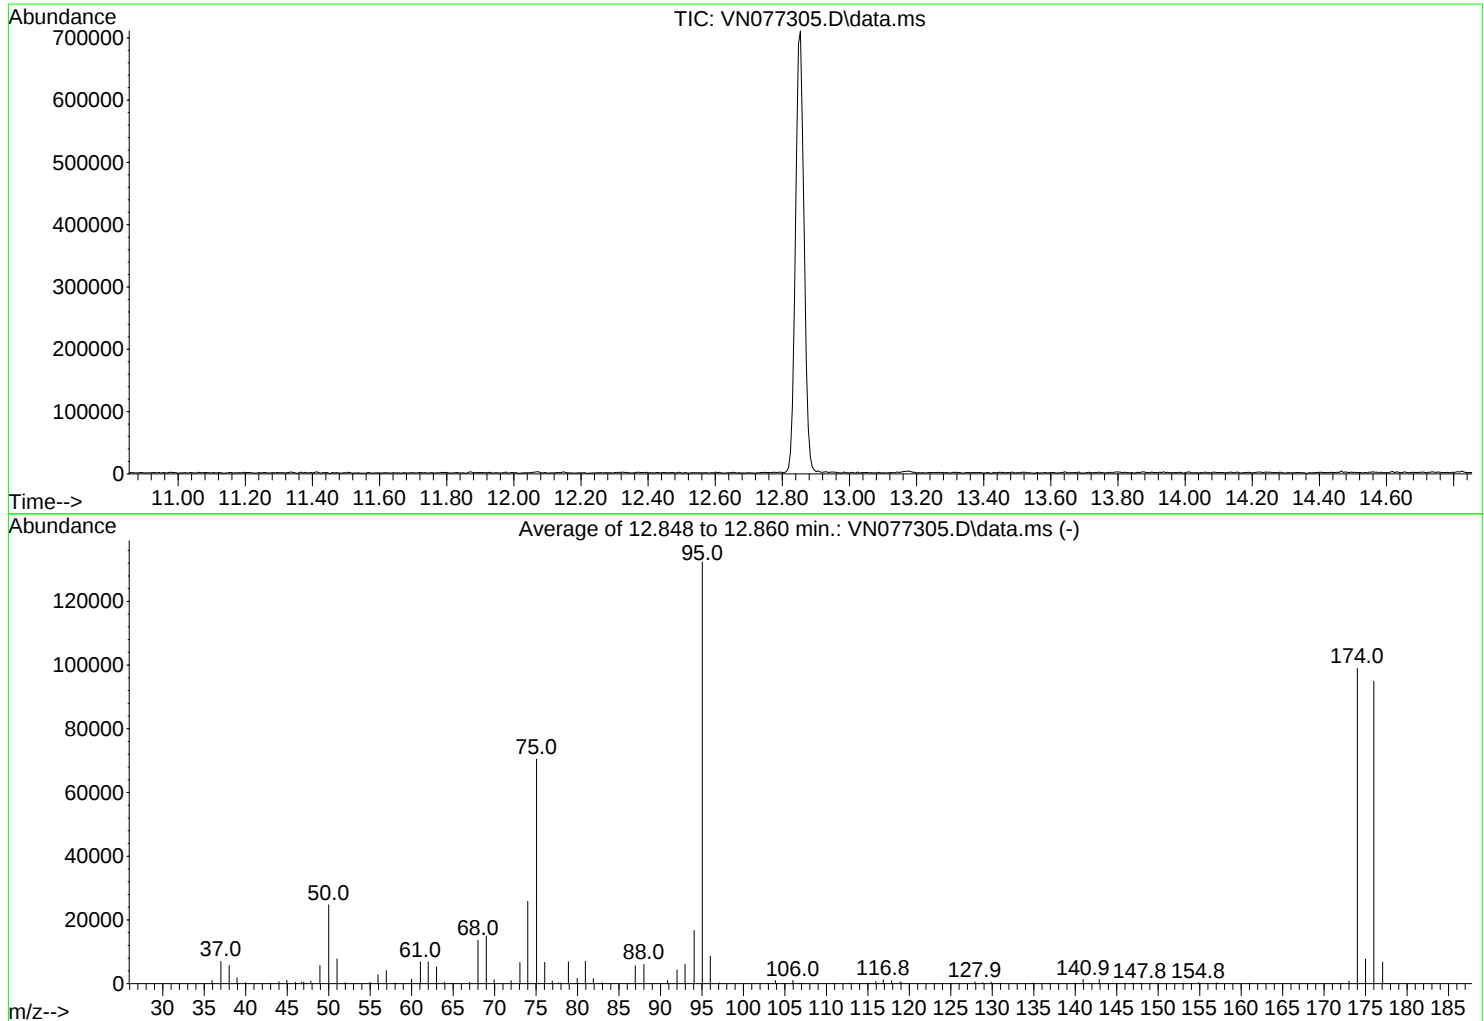

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1846

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.7	24755	PASS
75	95	30	60	53.2	70459	PASS
95	95	100	100	100.0	132405	PASS
96	95	5	9	6.5	8605	PASS
173	174	0.00	2	0.8	800	PASS
174	95	50	100	74.8	98992	PASS
175	174	5	9	7.8	7674	PASS
176	174	95	101	95.9	94933	PASS
177	176	5	9	7.1	6766	PASS

Average of 12.848 to 12.860 min.: VN077305.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	1036	47.00	505	57.95	158	69.95	123
37.00	7013	47.30	142	58.20	55	70.90	5
38.00	5738	47.85	801	60.00	1442	72.00	95
38.95	1867	48.95	5755	61.05	6835	73.05	665
39.95	381	50.00	24755	62.00	6835	74.00	25867
42.70	68	51.00	7713	63.00	5256	75.05	70459
43.00	102	51.90	255	63.95	453	76.05	6686
44.00	607	52.20	139	64.70	128	76.95	853
44.95	1129	55.00	449	67.00	455	77.70	283
46.00	444	55.95	2799	68.00	13650	78.00	199
46.75	547	56.95	4128	69.00	14992	78.90	6890

Average of 12.848 to 12.860 min.: VN077305.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.95	1648	94.05	16732	112.75	133	127.90	602
80.95	7026	95.05	132405	113.05	151	128.85	267
81.90	1598	96.00	8605	114.90	66	129.85	557
82.90	234	97.10	240	115.10	100	130.95	160
83.10	88	102.90	91	115.95	652	134.70	103
86.10	77	103.85	948	116.85	1173	134.95	227
86.95	5626	104.80	113	117.85	919	136.10	93
88.00	6044	105.95	984	118.90	609	136.80	114
90.85	1030	106.80	143	119.10	321	139.95	136
92.00	4304	107.20	136	123.20	80	140.95	1336
92.95	6064	110.80	81	123.95	145	141.75	203

Average of 12.848 to 12.860 min.: VN077305.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
142.90	1315	160.90	57				
145.90	116	171.60	61				
146.90	131	172.20	177				
147.80	183	173.00	800				
147.95	138	174.00	98992				
149.10	90	175.00	7674				
151.90	63	176.00	94933				
152.60	50	177.05	6766				
152.90	54	177.80	59				
154.85	361						
157.10	286						

Instrument :

MSVOA_N

ClientSampleId :

BFB