


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041224\
Data File : VN081705.D
Acq On : 12 Apr 2024 08:23
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Title : SW846 8260
Last Update : Tue Mar 19 06:00:00 2024

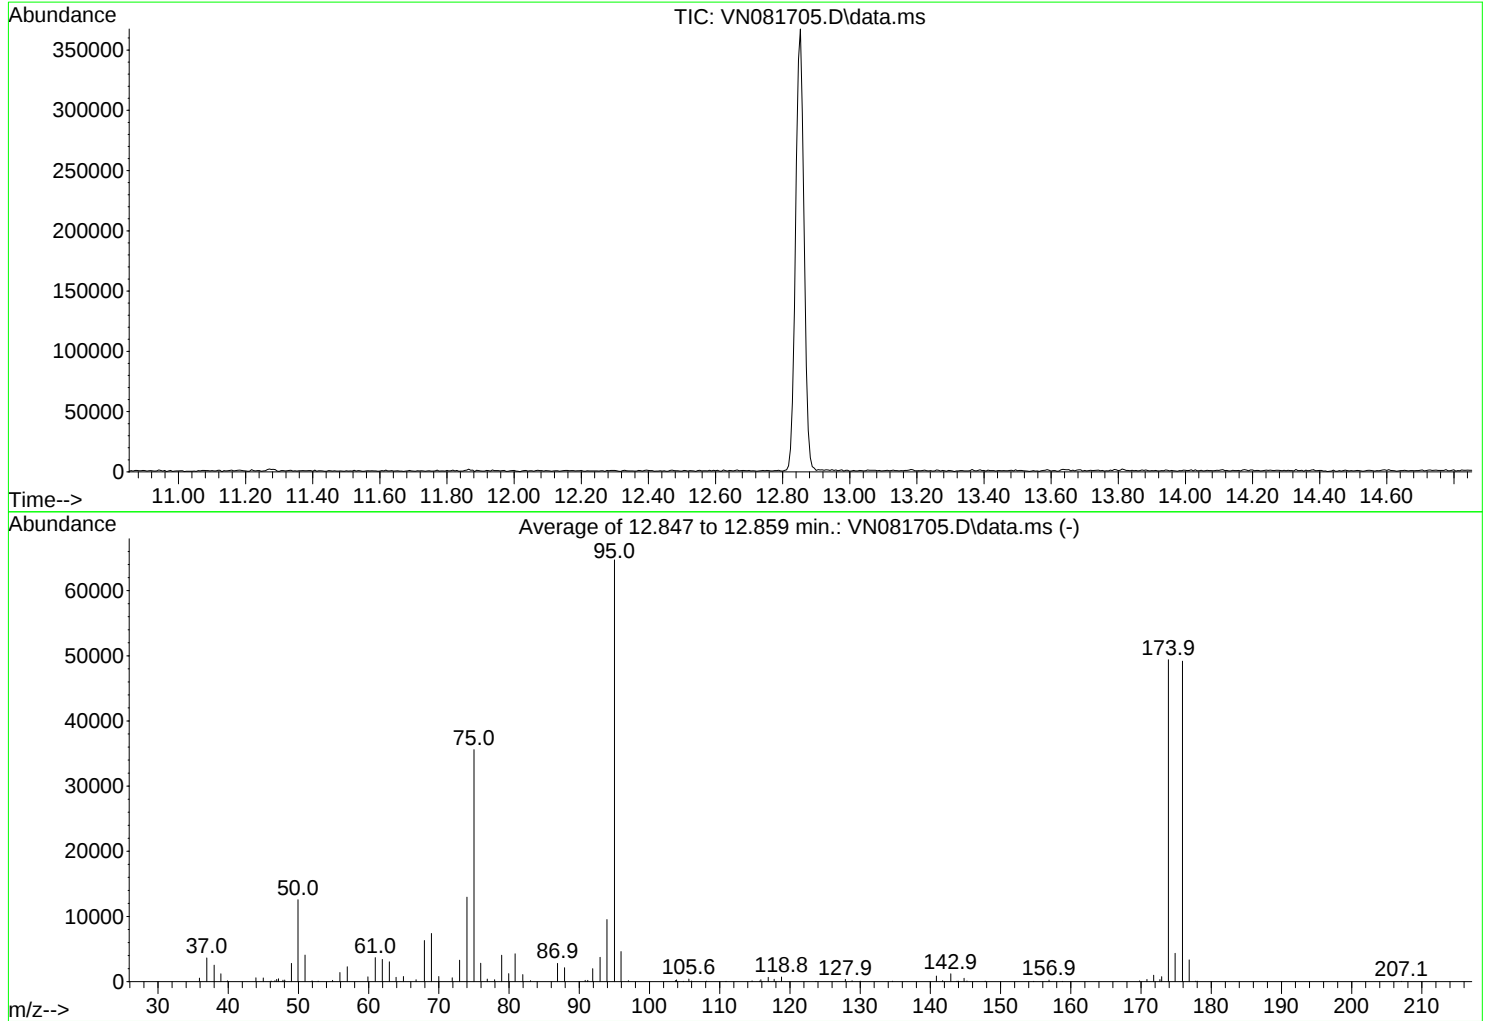

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	12585	PASS
75	95	30	60	55.0	35592	PASS
95	95	100	100	100.0	64728	PASS
96	95	5	9	7.1	4622	PASS
173	174	0.00	2	1.5	758	PASS
174	95	50	100	76.3	49395	PASS
175	174	5	9	8.8	4355	PASS
176	174	95	101	99.6	49195	PASS
177	176	5	9	6.8	3352	PASS

Average of 12.847 to 12.859 min.: VN081705.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	552	47.80	227	60.95	3681	74.00	1297
36.95	3628	48.05	238	61.95	3406	75.00	3559
38.00	2534	49.00	2808	62.95	3054	75.95	283
38.95	1207	49.95	12585	63.90	664	76.90	40
39.90	116	50.95	4088	64.95	785	77.95	285
43.95	594	51.95	116	66.75	285	78.95	4065
45.00	568	52.80	77	67.95	6301	79.95	1240
46.10	92	54.85	202	68.95	7380	80.85	4286
46.65	160	55.90	1401	70.00	777	81.95	1089
46.90	340	56.95	2294	71.90	592	83.05	151
47.15	445	59.90	737	72.95	3284	86.90	2815

Average of 12.847 to 12.859 min.: VN081705.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.90	2143	104.80	63	118.80	707	144.80	522
90.85	204	105.60	399	123.70	60	145.20	98
91.20	211	106.00	103	127.90	340	147.80	75
91.90	1995	108.10	67	128.85	161	154.70	56
92.95	3730	110.90	53	130.00	71	156.90	240
93.95	9537	114.60	120	134.60	81	158.80	55
95.00	64728	115.70	93	140.85	866	169.80	113
95.95	4622	115.85	284	141.75	158	170.85	340
97.00	143	116.90	662	142.90	1201	171.80	987
103.70	164	117.75	369	143.80	65	172.70	314
103.85	277	118.00	63	144.00	70	172.95	758

Average of 12.847 to 12.859 min.: VN081705.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
173.90	49395						
174.85	4355						
175.90	49195						
176.85	3352						
177.80	77						
178.00	82						
207.10	52						

Instrument :

MSVOA_N

ClientSampleId :

BFB