


Methylene Chloride

Response Ratio

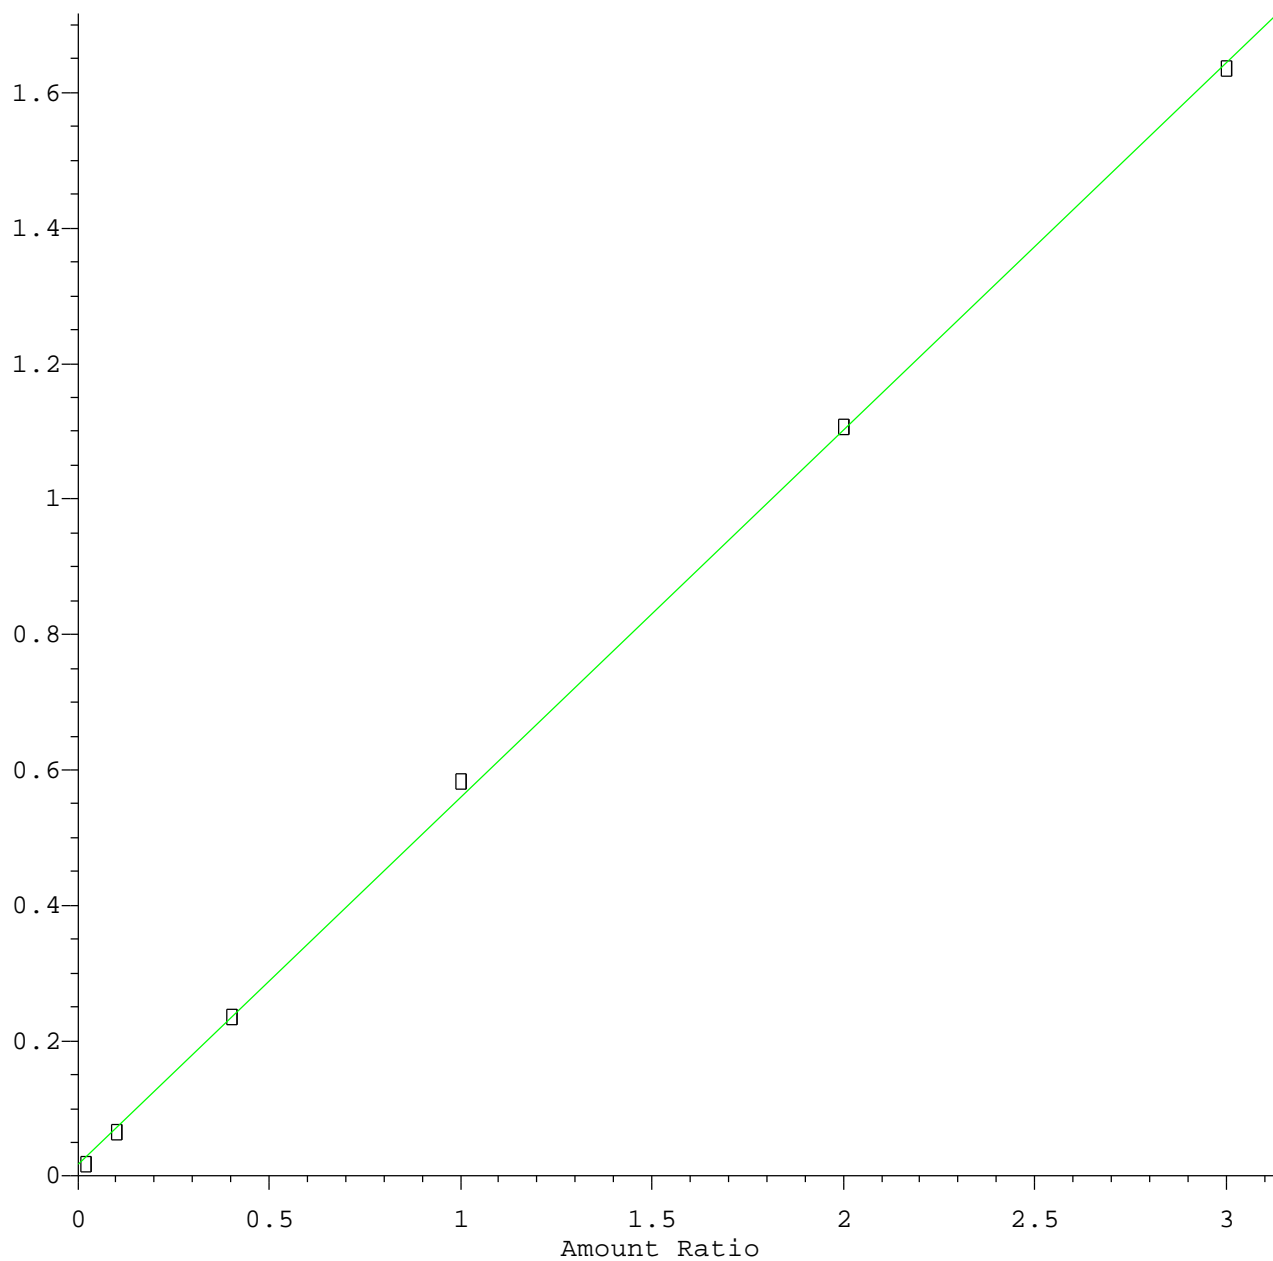


Resp Ratio = 5.43e-001 \* Amt + 1.69e-002  
Coef of Det (r<sup>2</sup>) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N041319W.M  
Calibration Table Last Updated: Sat Apr 13 03:34:24 2019

Cyclohexane

Response Ratio

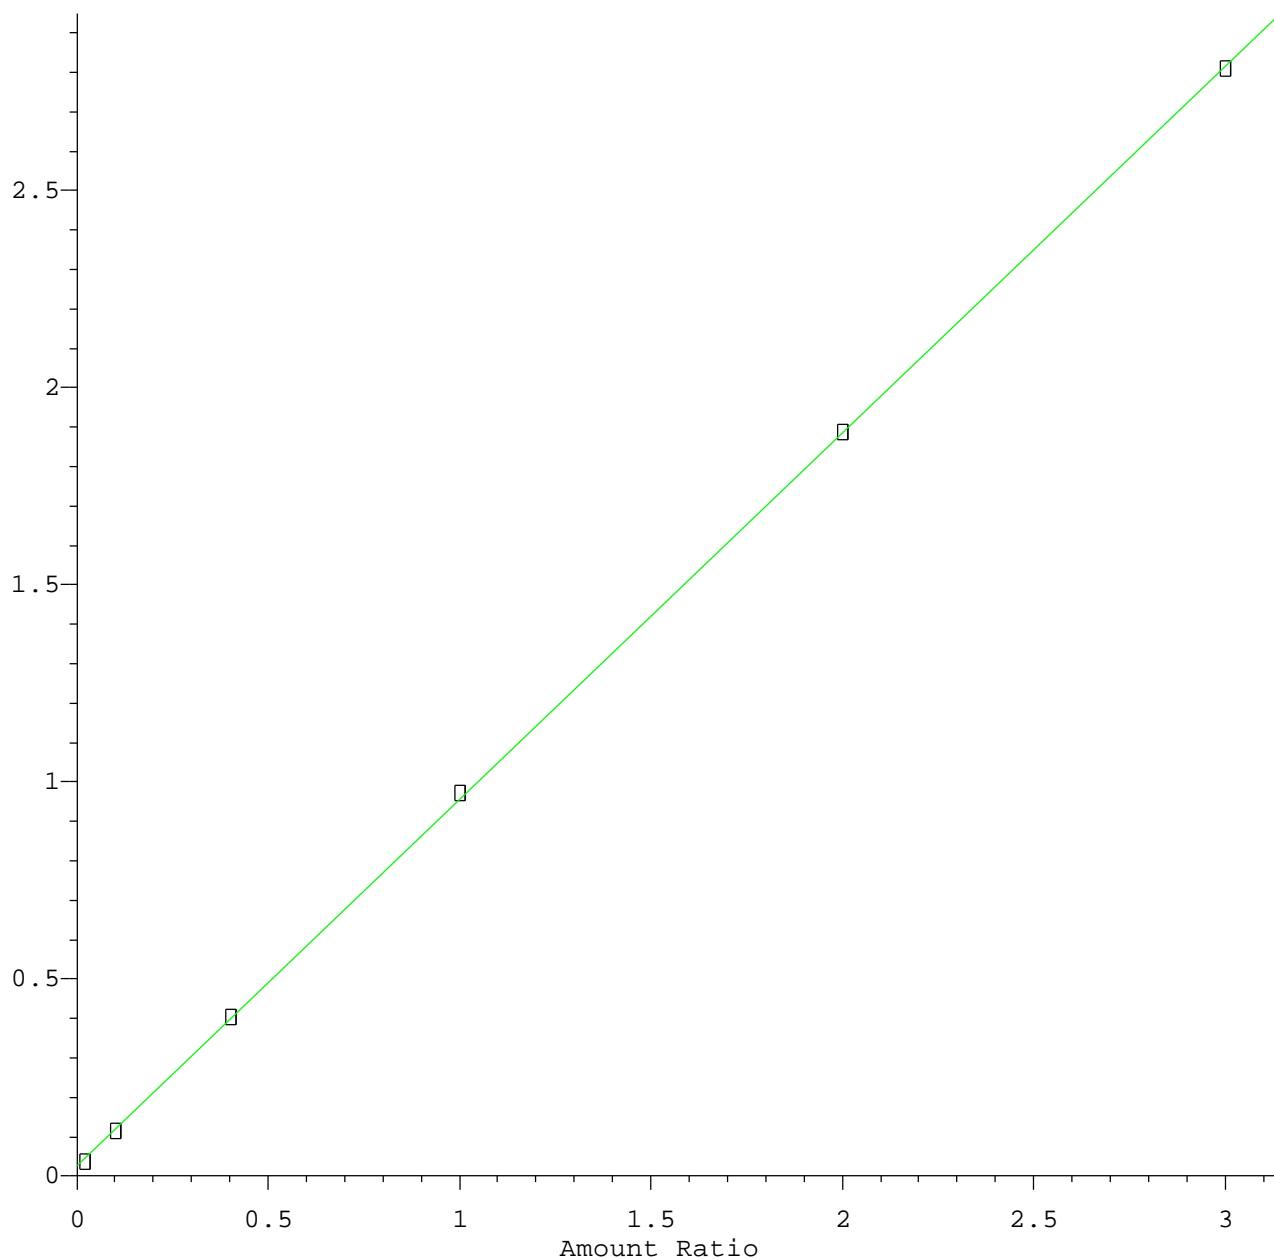


Resp Ratio = 9.29e-001 \* Amt + 2.66e-002  
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N041319W.M  
Calibration Table Last Updated: Sat Apr 13 03:34:24 2019

2-Chloroethyl Vinyl ether

Response Ratio

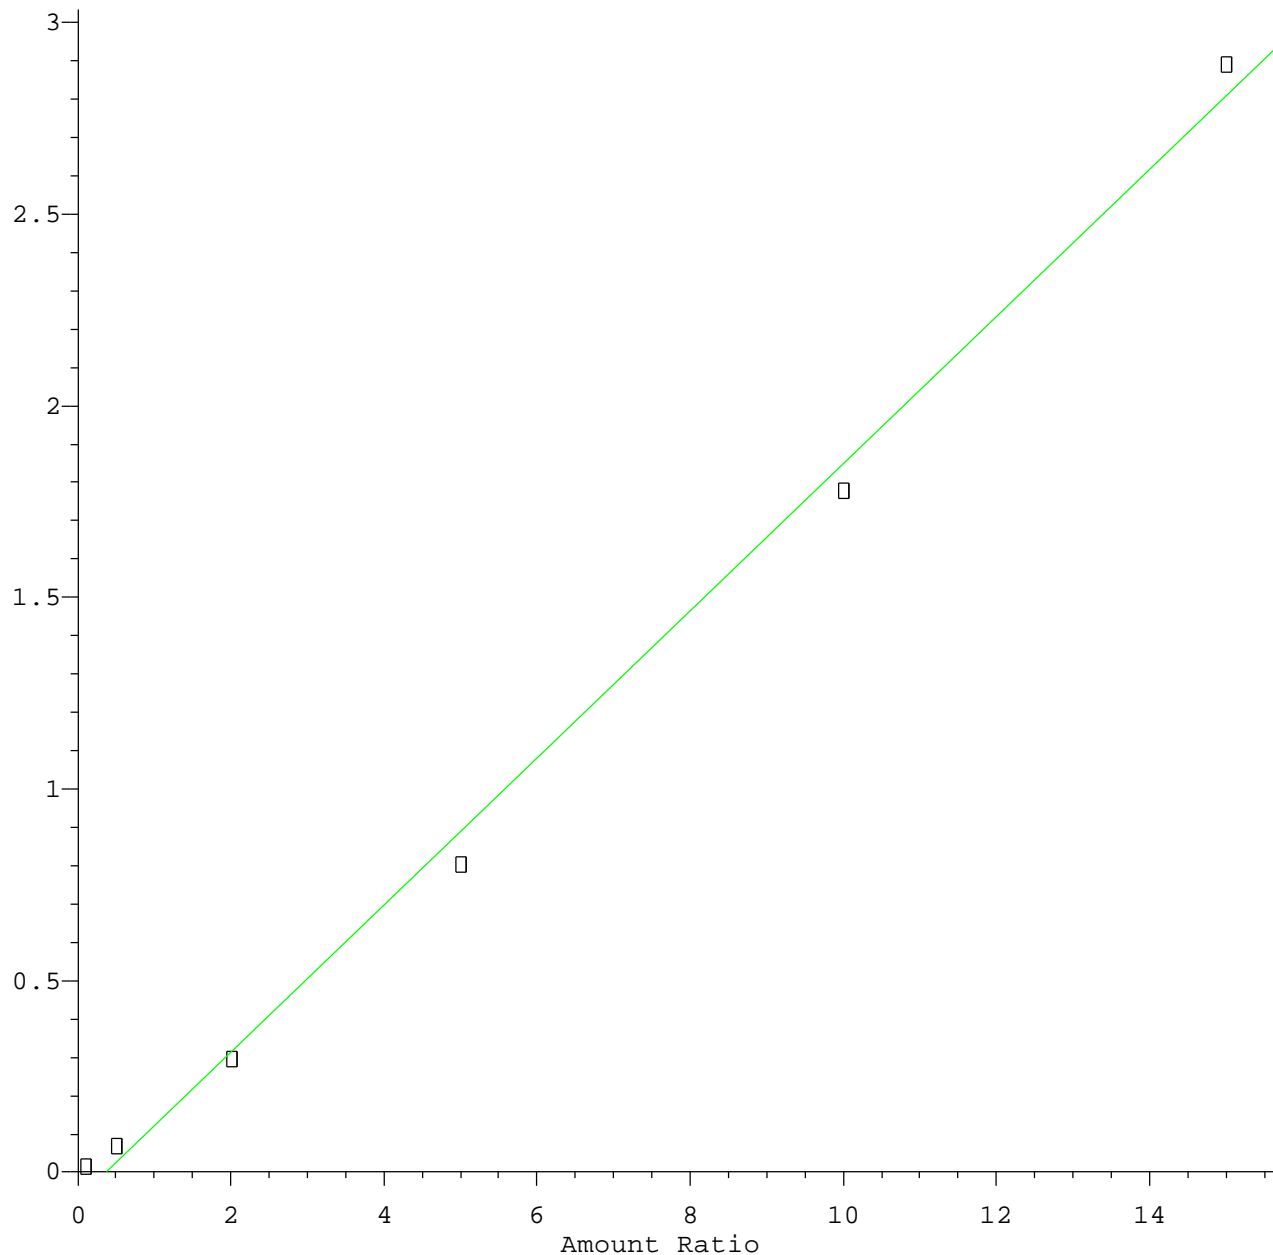


Resp Ratio = 1.92e-001 \* Amt - 6.99e-002  
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N041319W.M  
Calibration Table Last Updated: Sat Apr 13 03:34:24 2019

Bromoform

Response Ratio

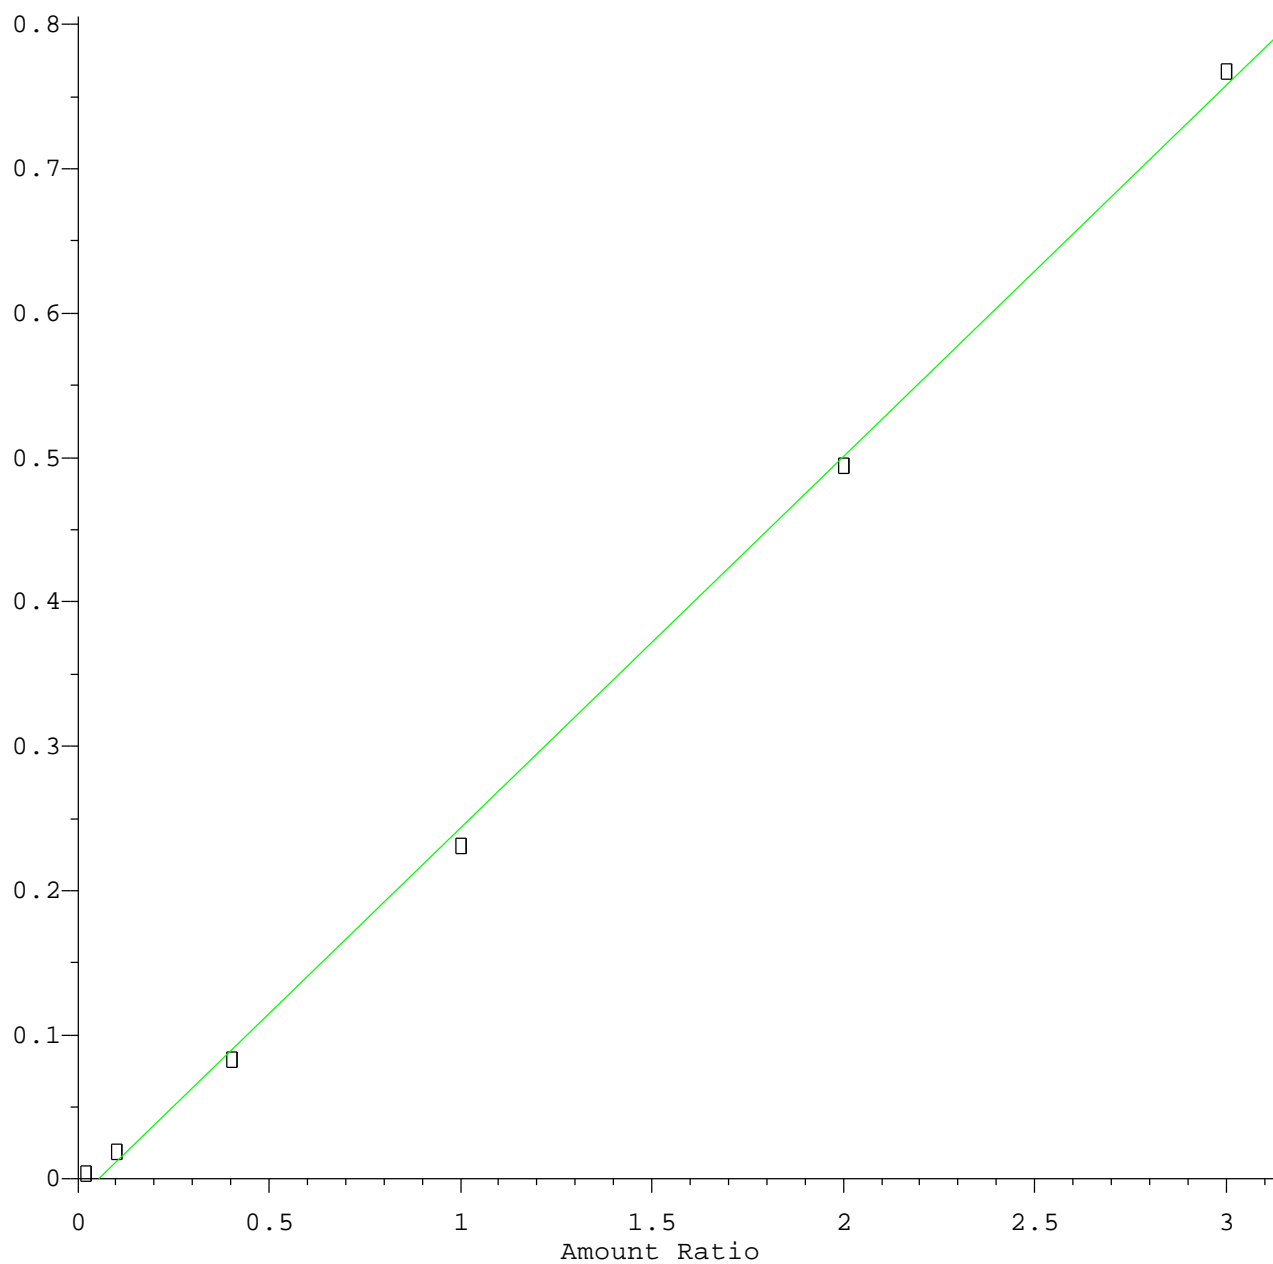


Resp Ratio = 2.57e-001 \* Amt - 1.33e-002  
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N041319W.M  
Calibration Table Last Updated: Sat Apr 13 03:34:24 2019

Bromobenzene

Response Ratio

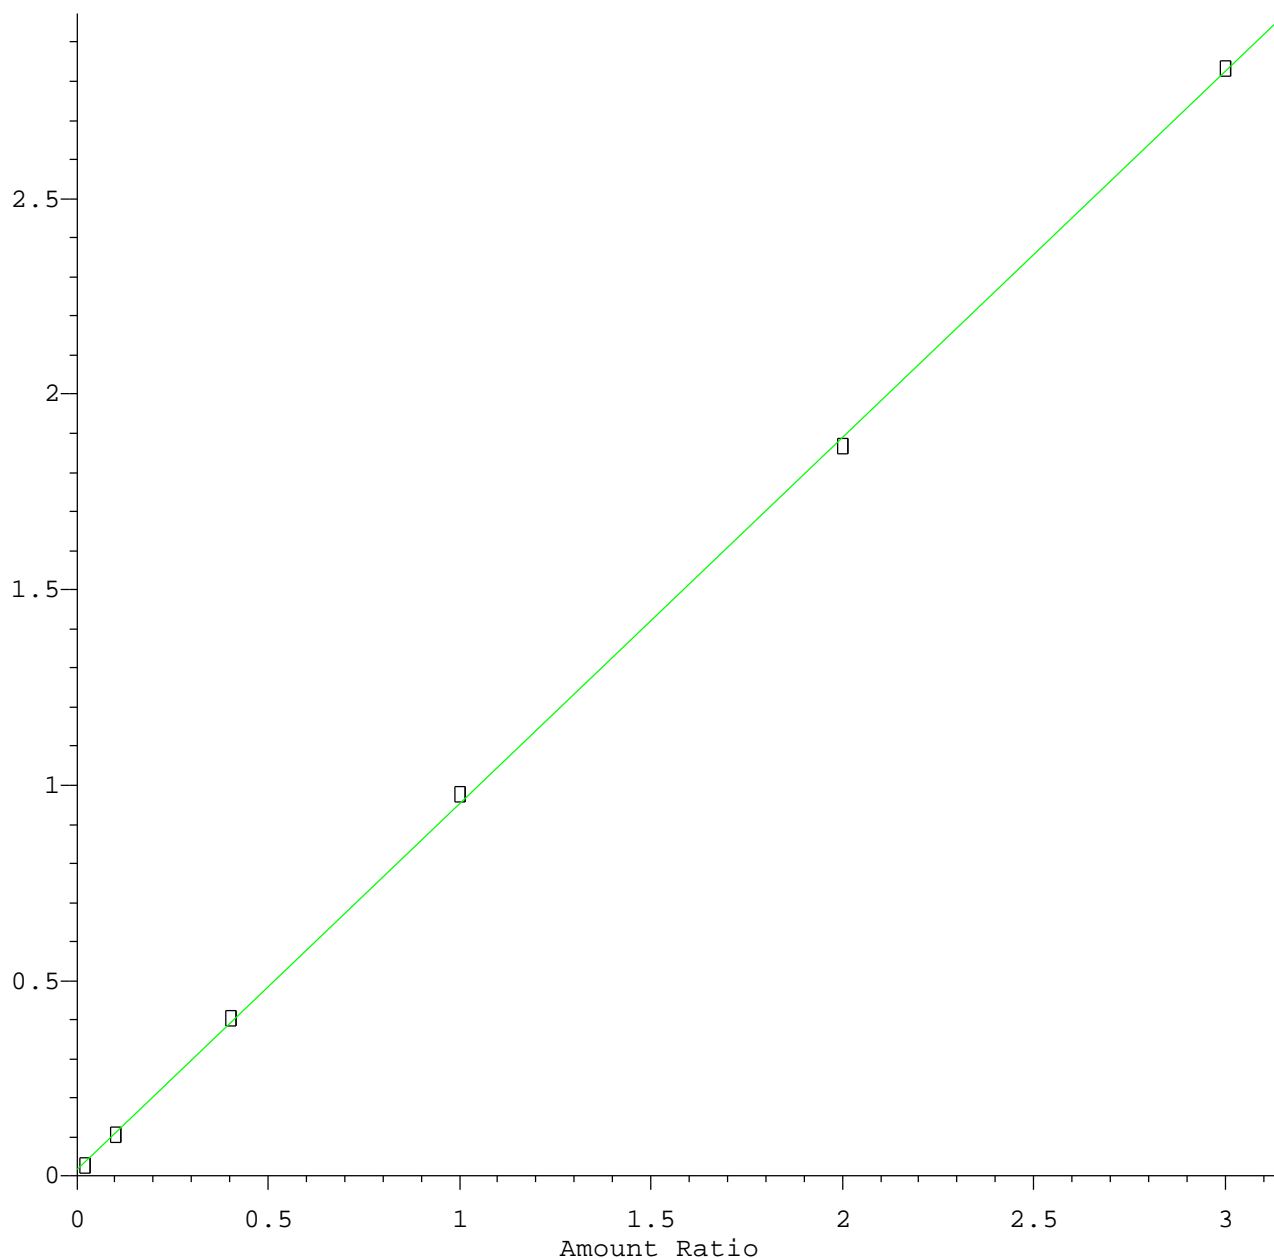


Resp Ratio = 9.35e-001 \* Amt + 1.77e-002  
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N041319W.M  
Calibration Table Last Updated: Sat Apr 13 03:34:24 2019

1,2,4-Trichlorobenzene

Response Ratio

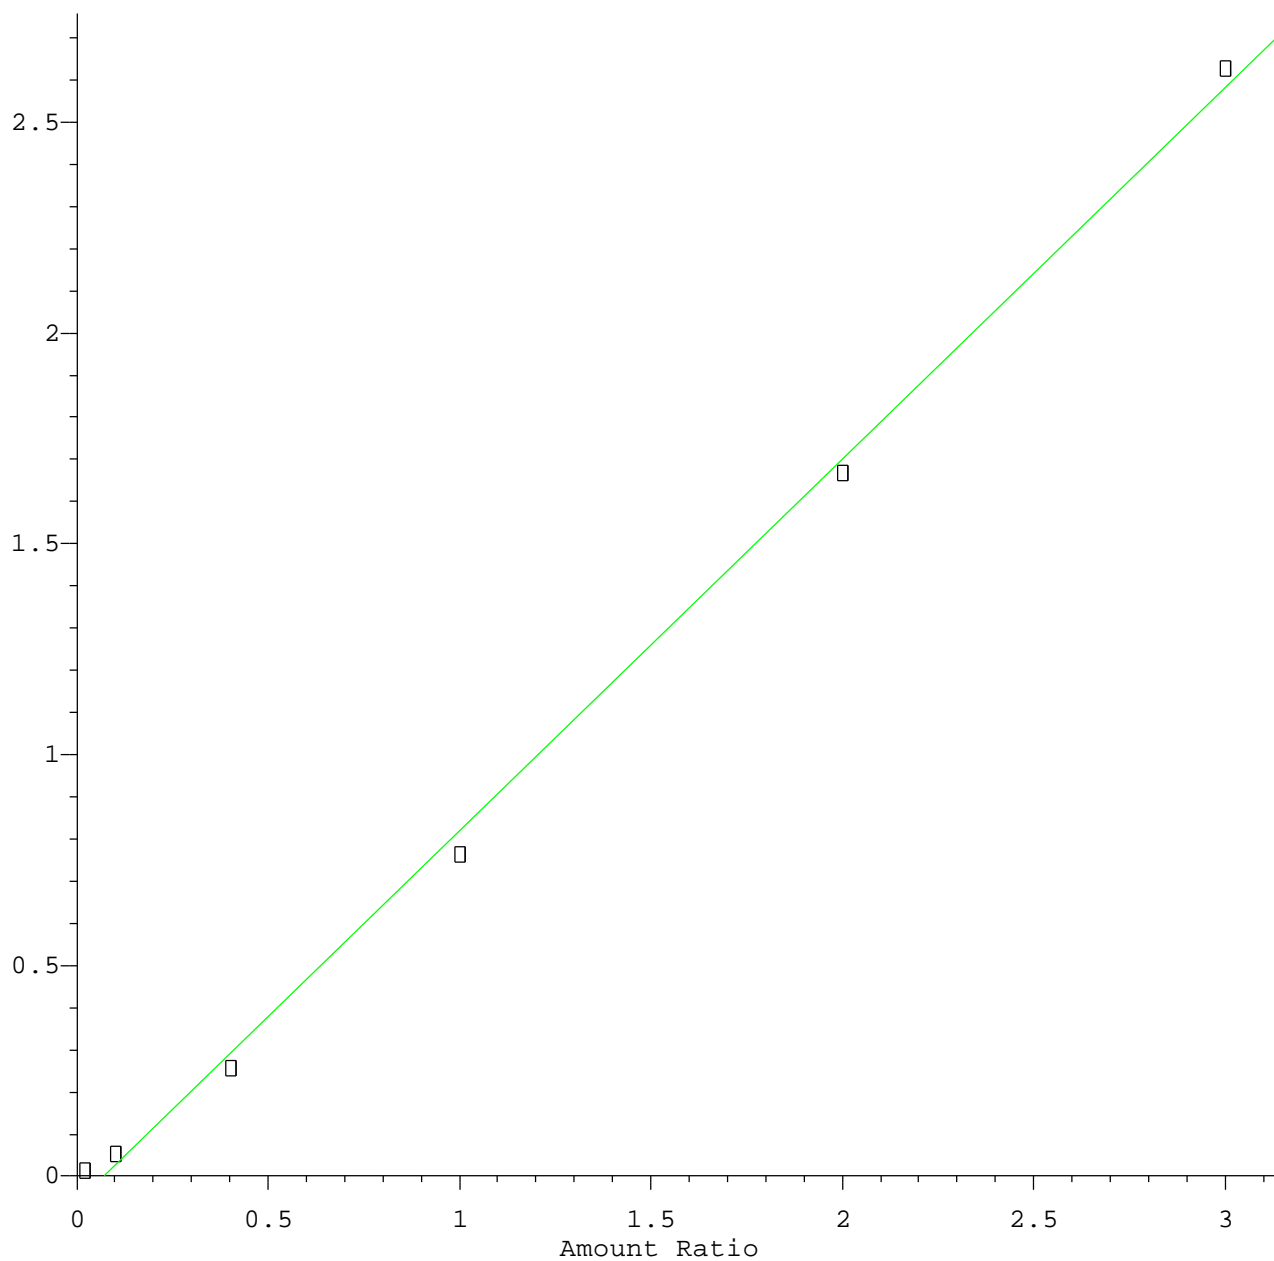


Resp Ratio =  $8.81e-001 * Amt - 6.22e-002$   
Coef of Det ( $r^2$ ) = 0.998    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N041319W.M  
Calibration Table Last Updated: Sat Apr 13 03:34:24 2019

Hexachlorobutadiene

Response Ratio

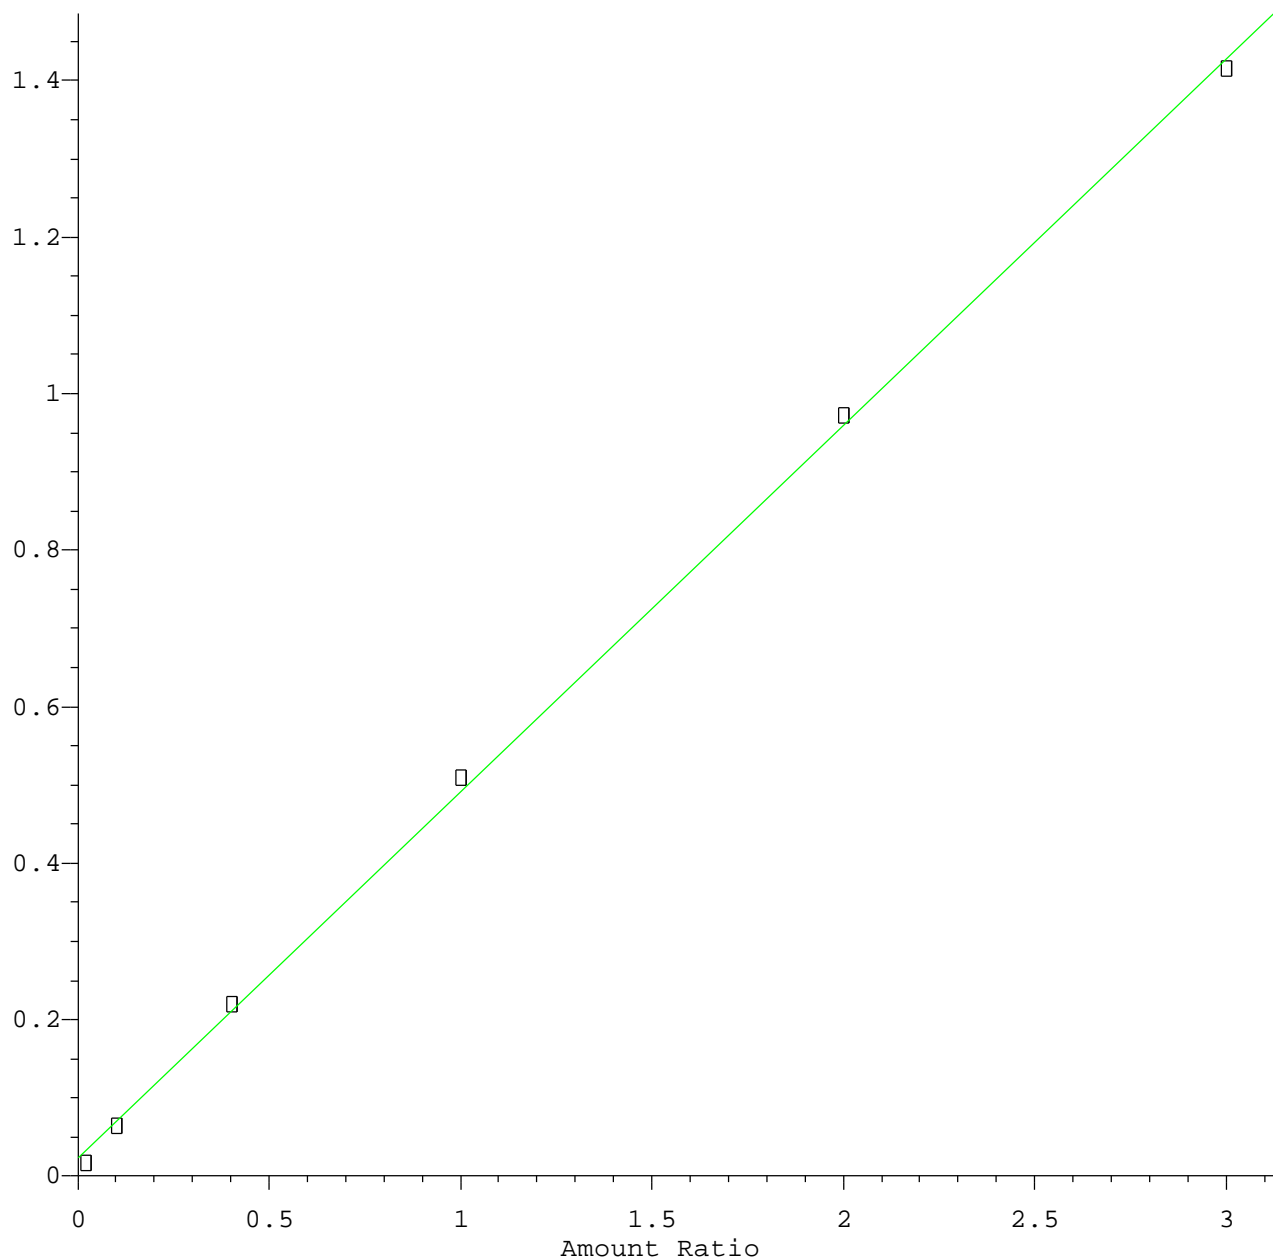


Resp Ratio = 4.68e-001 \* Amt + 2.31e-002  
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N041319W.M  
Calibration Table Last Updated: Sat Apr 13 03:34:24 2019

Naphthalene

Response Ratio

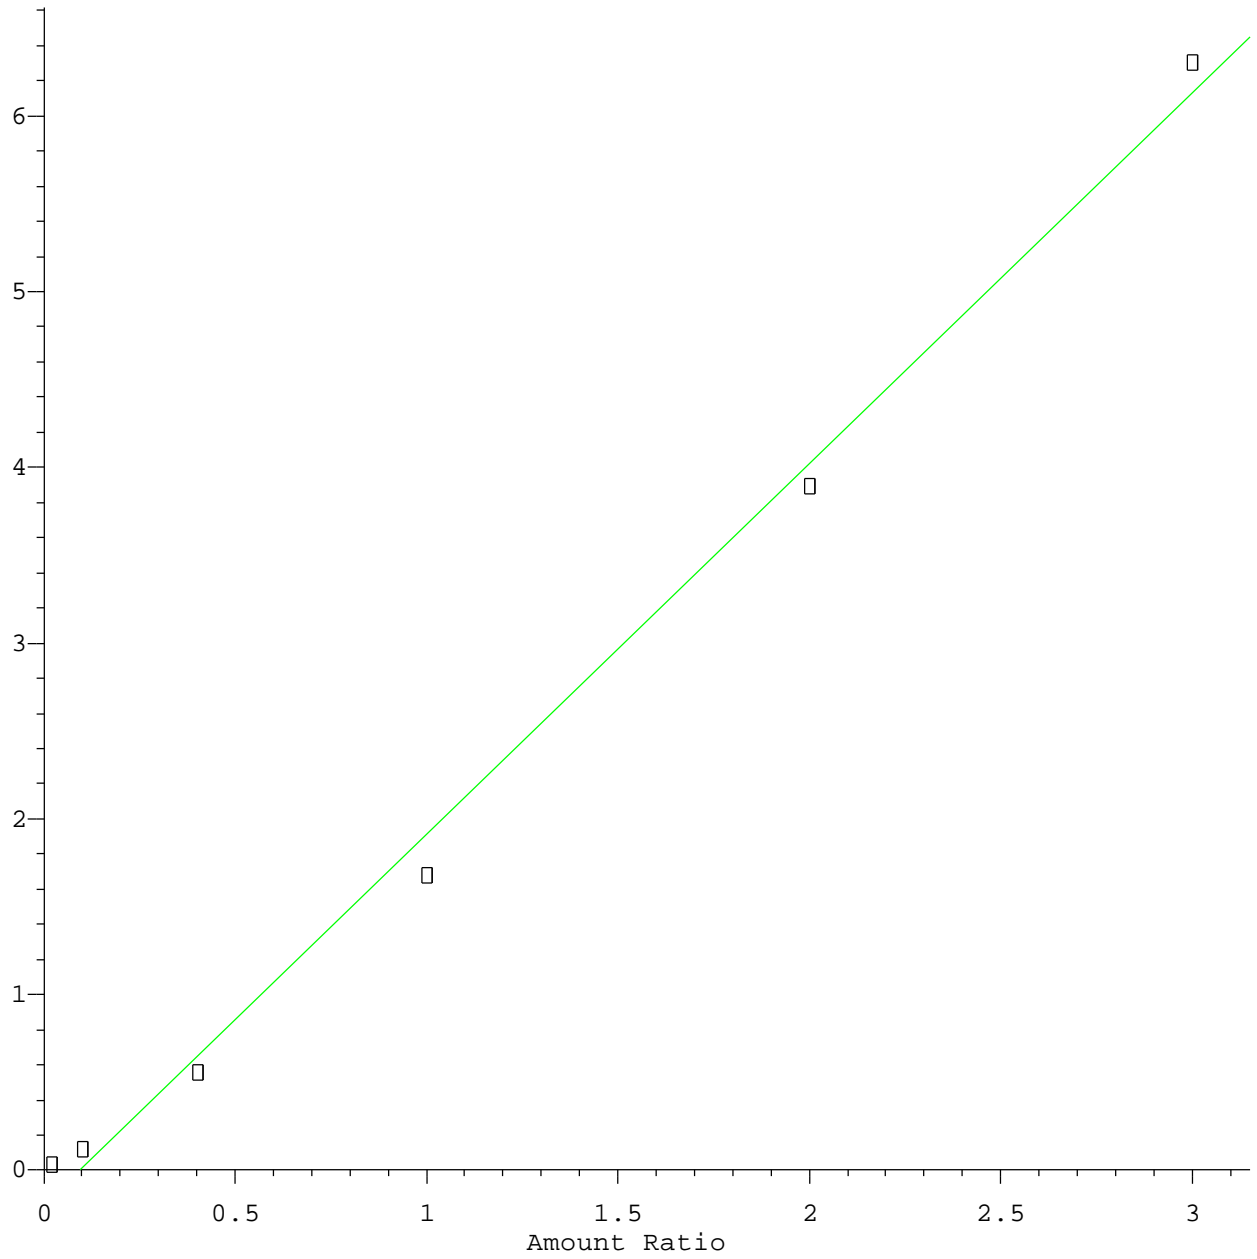

Resp Ratio = 2.11e+000 \* Amt - 1.97e-001  
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N041319W.M  
Calibration Table Last Updated: Sat Apr 13 03:34:24 2019