


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041321\
 Data File : VN066570.D
 Acq On : 13 Apr 2021 9:47
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N041321W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Apr 15 19:20:03 2021

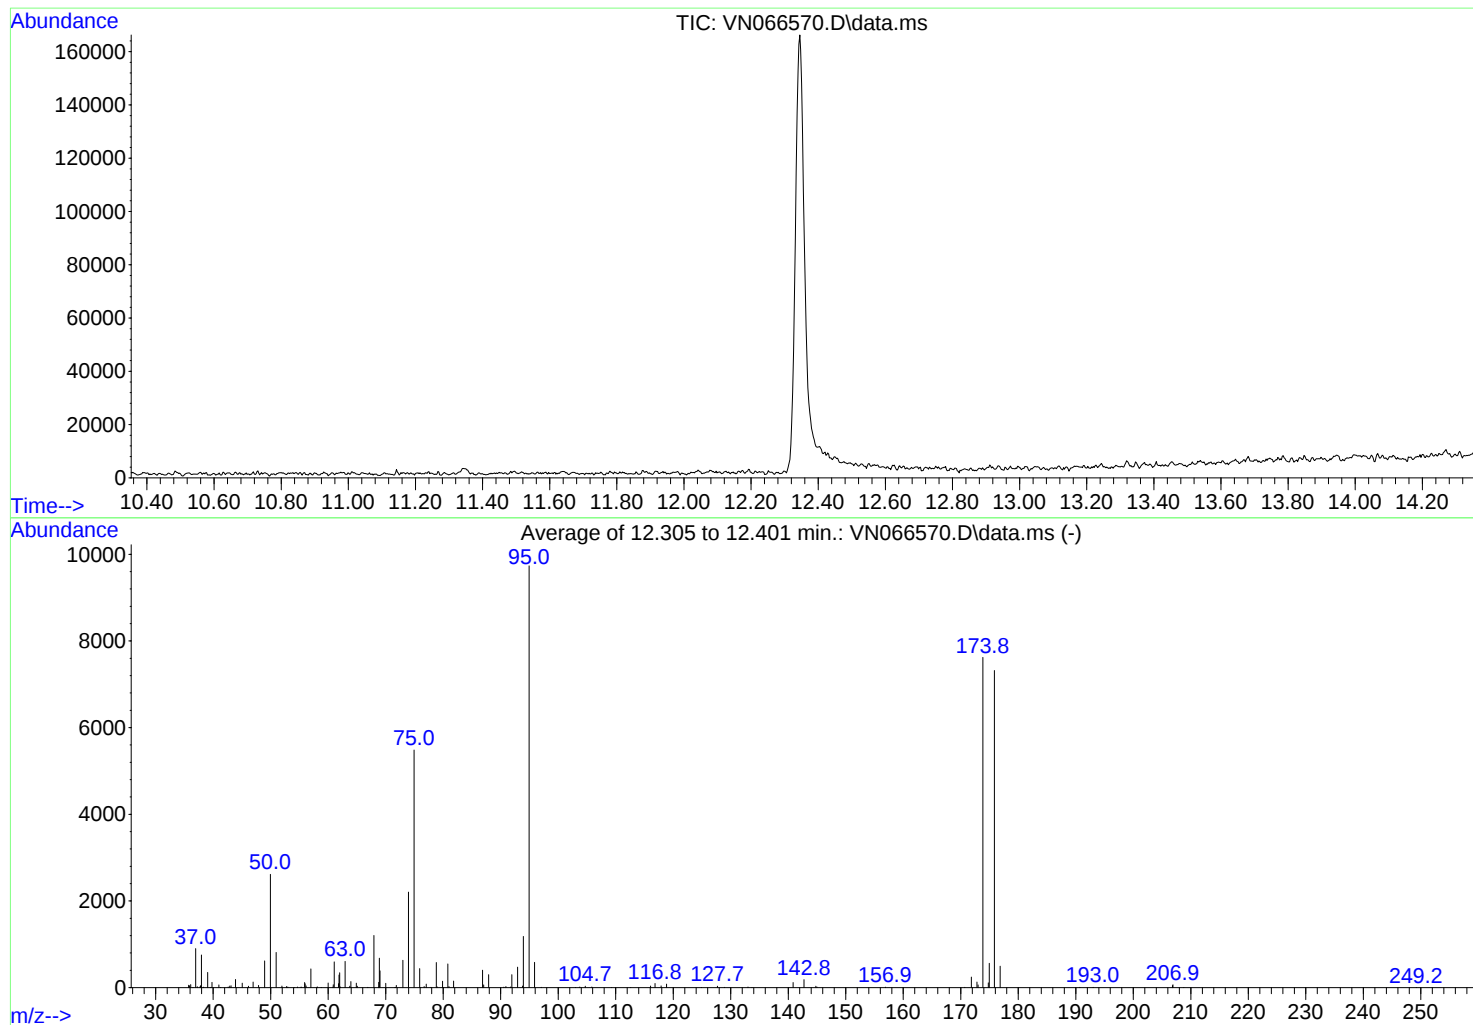

AutoFind: Averaged scan 3958 to 3994; Bkg corrected with scan 3957

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.9	2616	PASS
75	95	30	60	56.3	5482	PASS
95	95	100	100	100.0	9733	PASS
96	95	5	9	6.0	582	PASS
173	174	0.00	2	1.7	129	PASS
174	95	50	100	78.3	7620	PASS
175	174	5	9	7.3	560	PASS
176	174	95	101	96.0	7319	PASS
177	176	5	9	6.7	494	PASS