

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041323\
 Data File : VN077337.D
 Acq On : 13 Apr 2023 18:42
 Operator : JC\MD
 Sample : 02295-01 500X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SEW-30994

Quant Time: Apr 14 07:25:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N040523W.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 06 08:27:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.231	168	534997	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.107	114	1020427	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.872	117	907250	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.801	152	434345	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.589	65	329097	45.008	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	90.020%		
35) Dibromofluoromethane	8.172	113	302339	46.283	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	92.560%		
50) Toluene-d8	10.572	98	1265109	48.108	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	96.220%		
62) 4-Bromofluorobenzene	12.854	95	445282	50.911	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	101.820%		
Target Compounds						Qvalue
11) Tert butyl alcohol	5.513	59	2187	1.466	ug/l #	72
16) Acetone	4.443	43	142226	52.755	ug/l	95
18) Methyl Acetate	5.054	43	7506	0.731	ug/l	100
20) Methylene Chloride	5.278	84	1543	0.203	ug/l #	80
25) 2-Butanone	7.490	43	913	0.209	ug/l	91
26) 2,2-Dichloropropane	7.437	77	2624	0.234	ug/l #	51
31) Cyclohexane	8.231	56	13965	1.229	ug/l #	26
36) 1,1-Dichloropropene	8.237	75	46203	4.782	ug/l #	49
38) Carbon Tetrachloride	8.237	117	57514	5.810	ug/l #	15
43) Isopropyl Acetate	8.701	43	37248	2.335	ug/l #	56
48) Methyl methacrylate	9.654	41	2172	0.319	ug/l #	27
55) 1,1,2-Trichloroethane	11.007	97	5121	0.661	ug/l #	15
59) 2-Hexanone	11.178	43	6631	0.965	ug/l #	40
71) Bromoform	12.854	173	2081	0.391	ug/l #	1
73) Isopropylbenzene	12.713	105	174148	4.128	ug/l #	57
74) N-amyl acetate	12.483	43	23274	1.456	ug/l #	56
75) 1,1,2,2-Tetrachloroethane	12.913	83	3083	0.233	ug/l #	25
76) 1,2,3-Trichloropropane	12.854	75	245001	23.688	ug/l #	1
78) n-propylbenzene	13.060	91	16509	0.354	ug/l #	69
79) 2-Chlorotoluene	13.189	91	483688	17.233	ug/l #	41
81) trans-1,4-Dichloro-2-b...	12.854	75	245001	53.305	ug/l #	13
82) 4-Chlorotoluene	13.189	91	483688	18.278	ug/l #	41
83) tert-Butylbenzene	13.601	119	94186	3.140	ug/l #	1
84) 1,2,4-Trimethylbenzene	13.601	105	169318	5.086	ug/l #	48
85) sec-Butylbenzene	13.601	105	169318	4.051	ug/l #	57
86) p-Isopropyltoluene	13.730	119	3101392	94.410	ug/l #	69
89) n-Butylbenzene	13.954	91	1788829	65.594	ug/l #	74
90) Hexachloroethane	14.283	117	3154	0.439	ug/l #	21
96) 1,2,3-Trichlorobenzene	15.777	180	1443	0.263	ug/l #	31


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041323\
Data File : VN077337.D
Acq On : 13 Apr 2023 18:42
Operator : JC\MD
Sample : 02295-01 500X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SEW-30994

Quant Time: Apr 14 07:25:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N040523W.M
Quant Title : SW846 8260
QLast Update : Thu Apr 06 08:27:03 2023
Response via : Initial Calibration




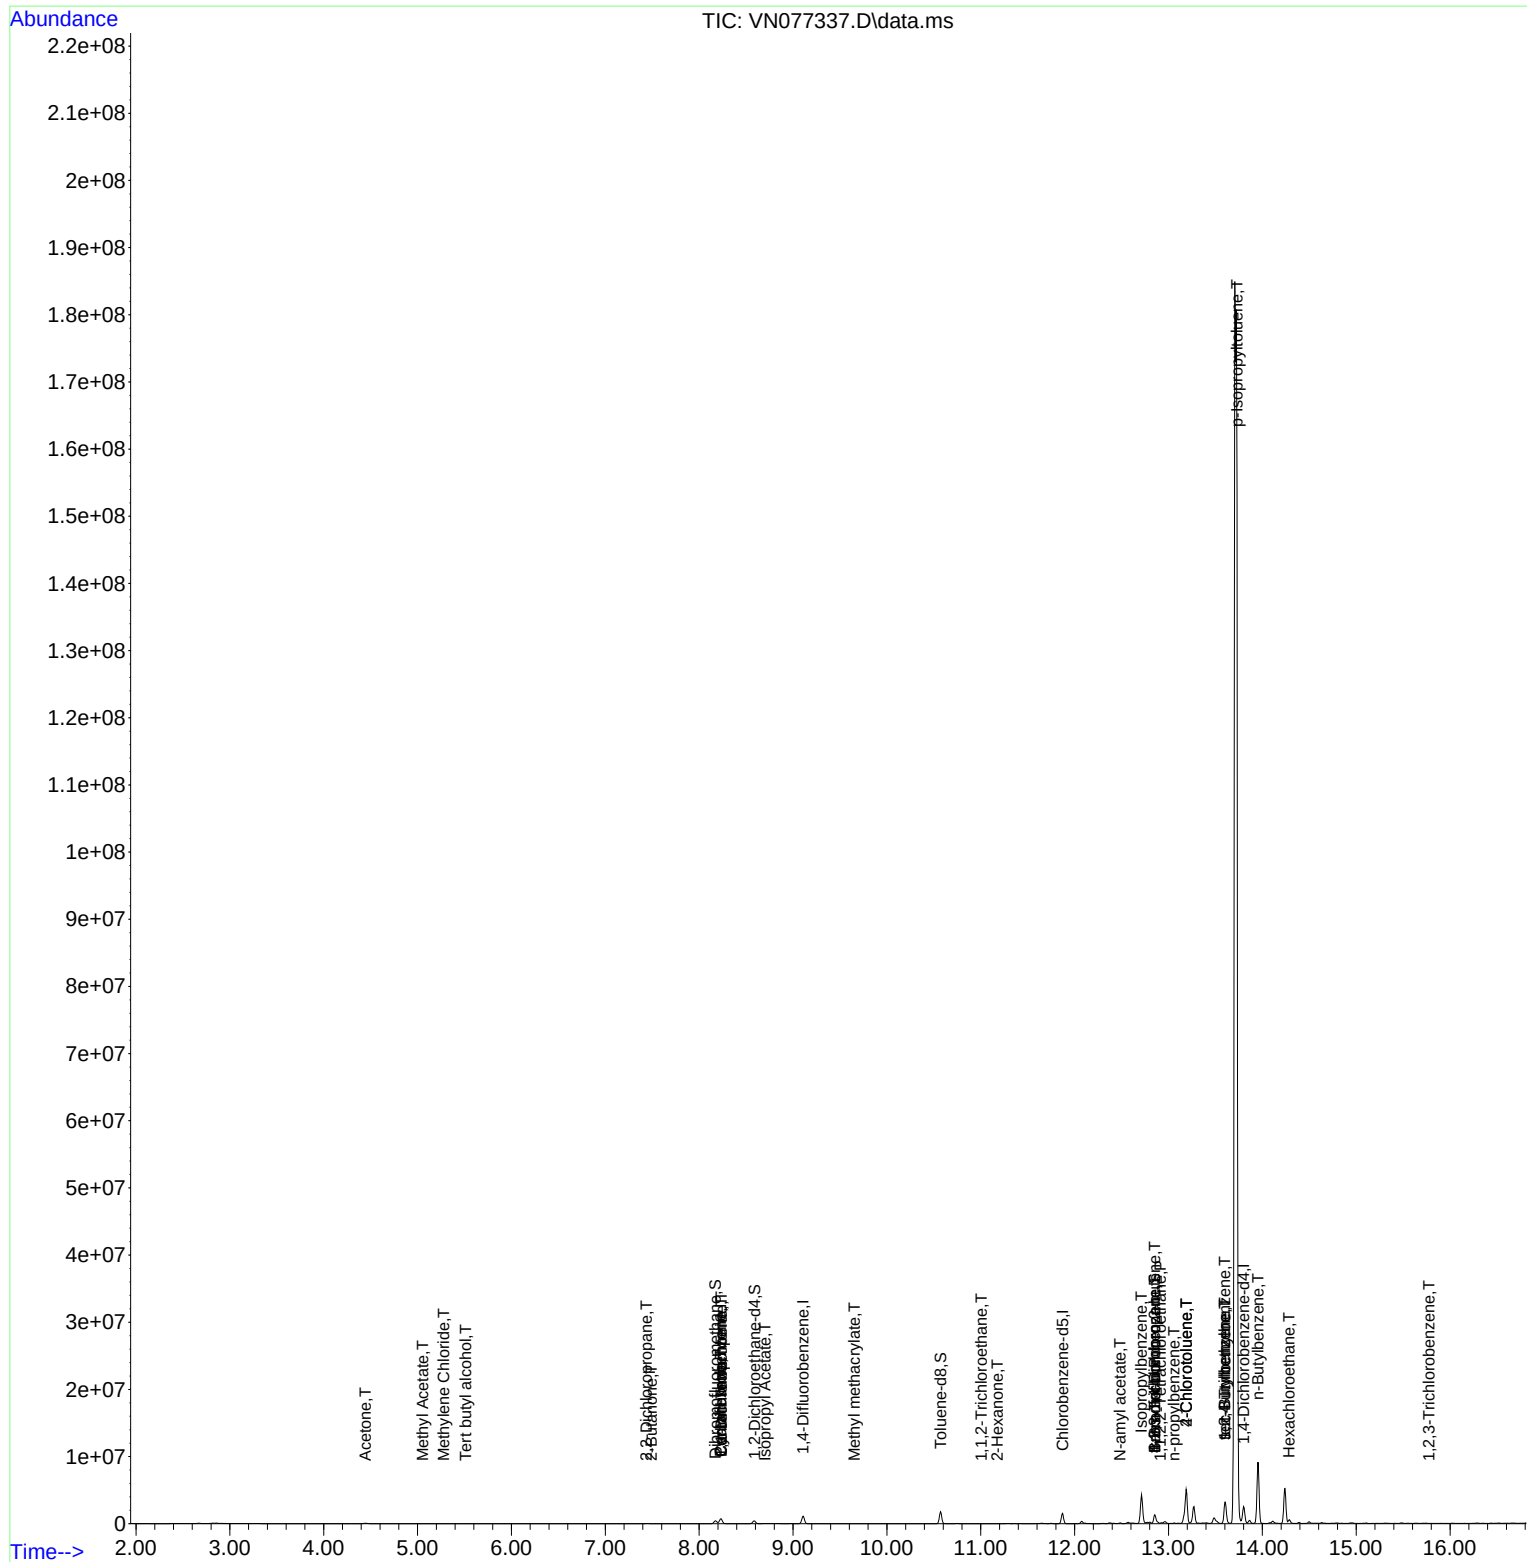




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.231 min Scan# 1070
Delta R.T. -0.000 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42




Instrument :
MSVOA_N
ClientSampleId :
SEW-30994


Tgt Ion:168 Resp: 534997
Ion Ratio Lower Upper
168 100
99 64.8 50.6 75.8

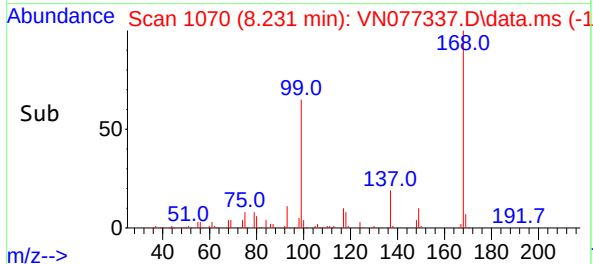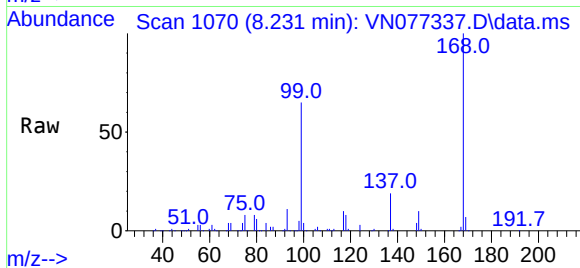

#11
Tert butyl alcohol
Concen: 1.466 ug/l
RT: 5.513 min Scan# 608
Delta R.T. -0.024 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42

Tgt Ion: 59 Resp: 2187
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#


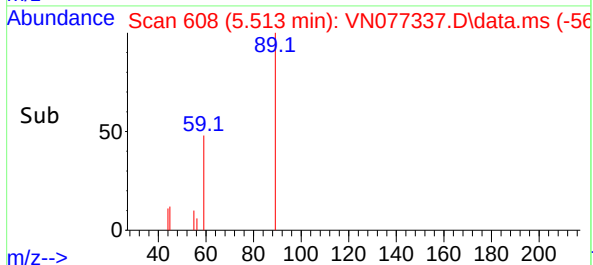

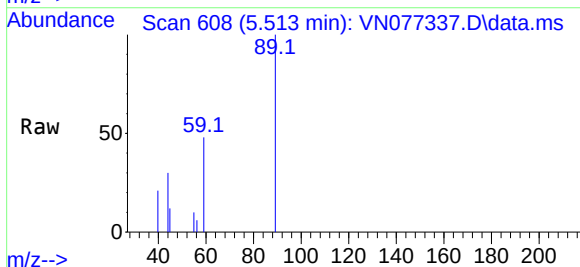




#16
Acetone
Concen: 52.755 ug/l
RT: 4.443 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42




Instrument :
MSVOA_N
ClientSampleId :
SEW-30994


Tgt Ion: 43 Resp: 142226
Ion Ratio Lower Upper
43 100
58 33.2 29.0 43.6



#18
Methyl Acetate
Concen: 0.731 ug/l
RT: 5.054 min Scan# 530
Delta R.T. 0.017 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42

Tgt Ion: 43 Resp: 7506
Ion Ratio Lower Upper
43 100
74 29.2 23.4 35.2


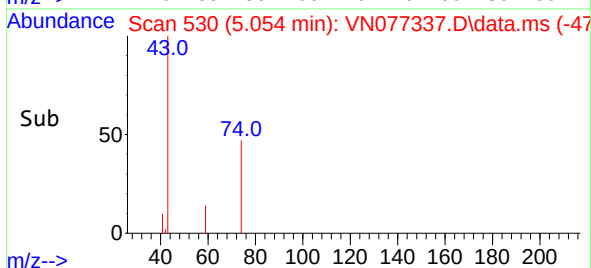
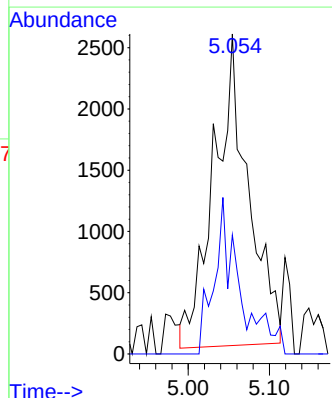





#20
Methylene Chloride
Concen: 0.203 ug/l
RT: 5.278 min Scan# 51
Delta R.T. -0.012 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42




Instrument :
MSVOA_N
ClientSampleId :
SEW-30994


Tgt Ion:	84	Resp:	1543
Ion	Ratio	Lower	Upper
84	100		
49	81.0	80.6	121.0
51	21.2	24.4	36.6#
86	76.5	47.0	70.6#

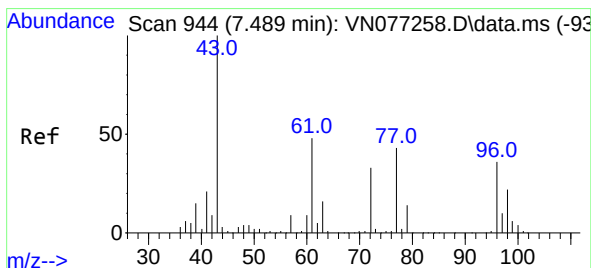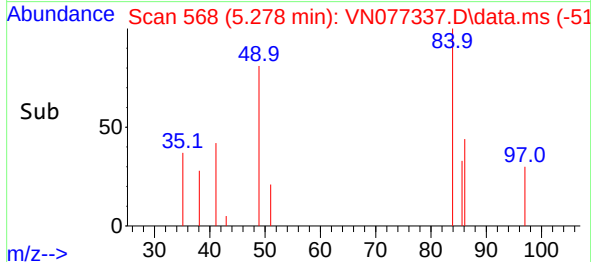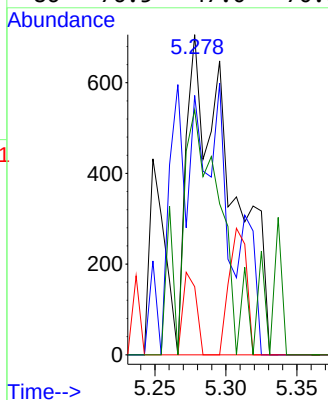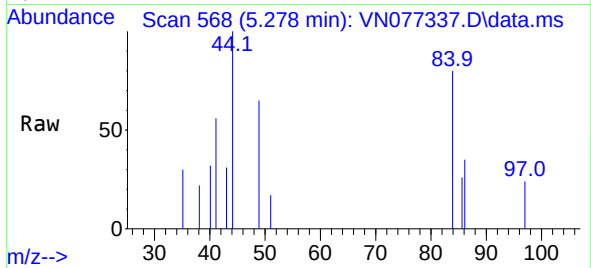

#25
2-Butanone
Concen: 0.209 ug/l
RT: 7.490 min Scan# 944
Delta R.T. 0.001 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42

Tgt Ion:	43	Resp:	913
Ion	Ratio	Lower	Upper
43	100		
72	38.5	26.6	39.8


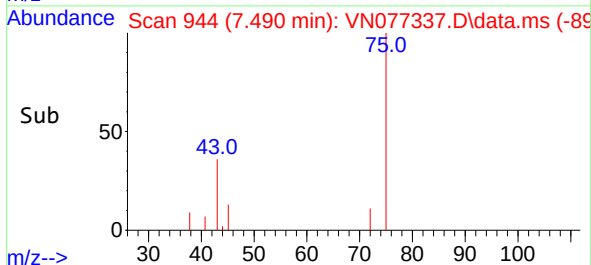
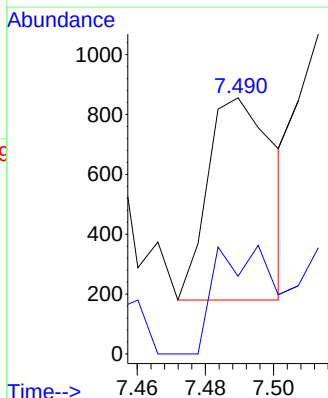
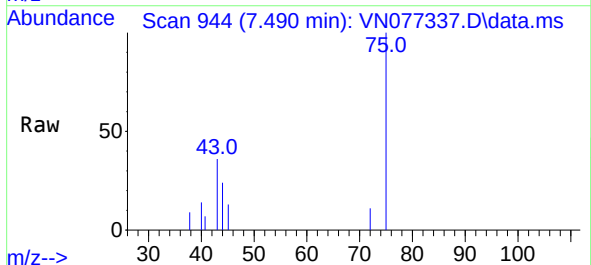




#26
2,2-Dichloropropane
Concen: 0.234 ug/l
RT: 7.437 min Scan# 91
Delta R.T. -0.058 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42




Instrument :
MSVOA_N
ClientSampleId :
SEW-30994


Tgt Ion: 77 Resp: 2624
Ion Ratio Lower Upper
77 100
97 0.0 12.0 36.1#

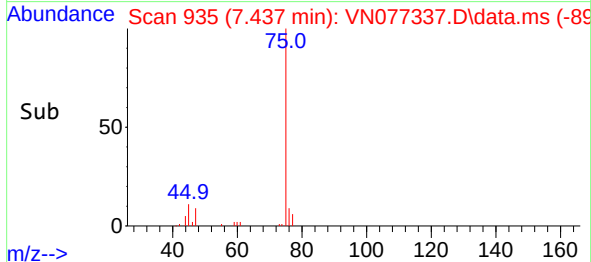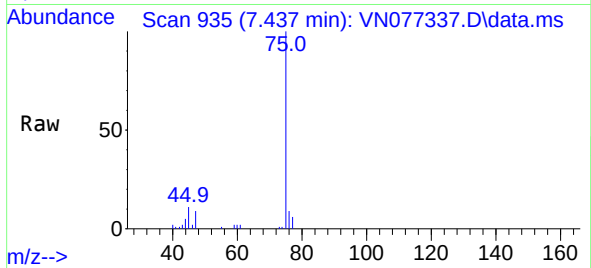

#31
Cyclohexane
Concen: 1.229 ug/l
RT: 8.231 min Scan# 1070
Delta R.T. -0.029 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42

Tgt Ion: 56 Resp: 13965
Ion Ratio Lower Upper
56 100
69 127.0 26.6 40.0#
84 147.2 81.8 122.8#


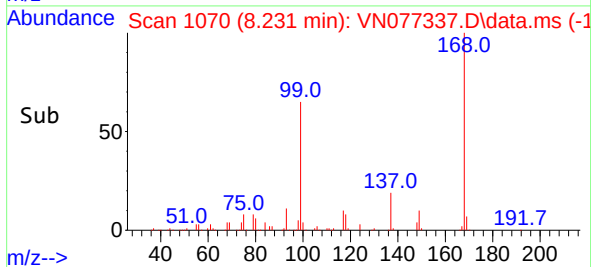

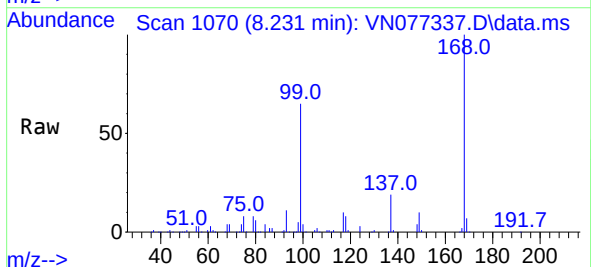




#33
1,2-Dichloroethane-d4
Concen: 45.008 ug/l
RT: 8.589 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42




Instrument :
MSVOA_N
ClientSampleId :
SEW-30994


Tgt Ion: 65 Resp: 329097
Ion Ratio Lower Upper
65 100
67 54.1 0.0 108.8

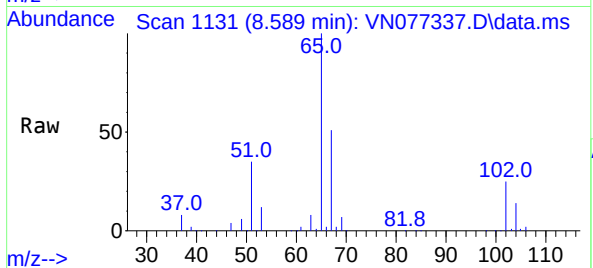

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.107 min Scan# 1219
Delta R.T. 0.000 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42

Tgt Ion: 114 Resp: 1020427
Ion Ratio Lower Upper
114 100
63 18.3 0.0 37.8
88 15.0 0.0 29.4


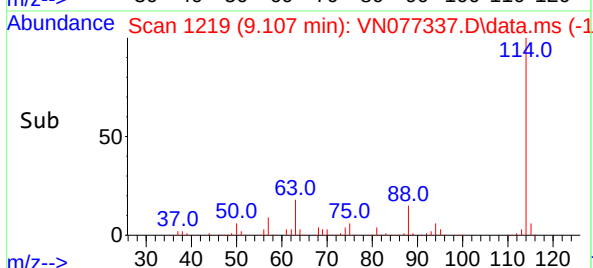






#35
Dibromofluoromethane
Concen: 46.283 ug/l
RT: 8.172 min Scan# 1071
Delta R.T. -0.000 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42




Instrument :
MSVOA_N
ClientSampleId :
SEW-30994


Tgt Ion:113 Resp: 302339
Ion Ratio Lower Upper
113 100
111 103.8 83.4 125.0
192 16.0 13.5 20.3

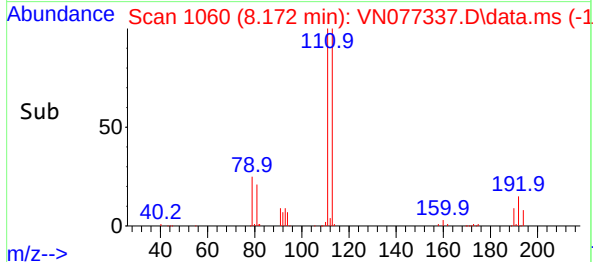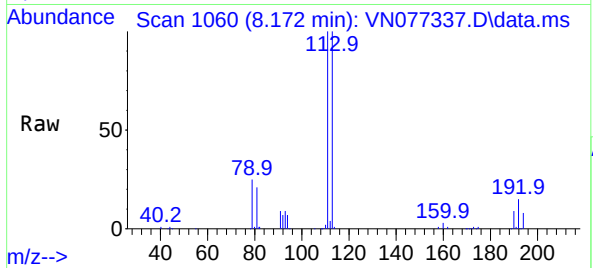

#36
1,1-Dichloropropene
Concen: 4.782 ug/l
RT: 8.237 min Scan# 1071
Delta R.T. -0.141 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42

Tgt Ion: 75 Resp: 46203
Ion Ratio Lower Upper
75 100
110 8.7 17.8 53.5#
77 0.0 25.0 37.4#


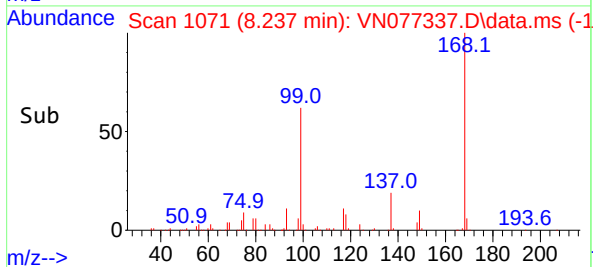

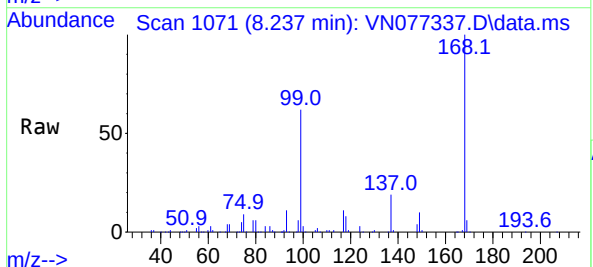




#38
Carbon Tetrachloride
Concen: 5.810 ug/l
RT: 8.237 min Scan# 1107
Delta R.T. -0.129 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42




Instrument :
MSVOA_N
ClientSampleId :
SEW-30994


Tgt Ion:117 Resp: 57514
Ion Ratio Lower Upper
117 100
119 4.8 78.5 117.7#
121 0.0 26.6 40.0#

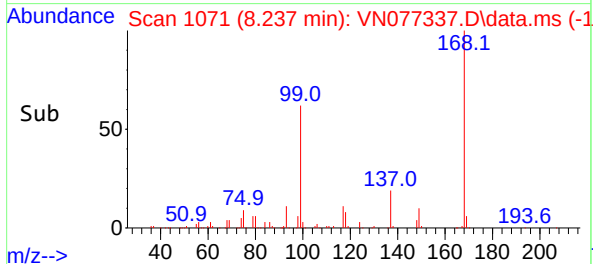

#43
Isopropyl Acetate
Concen: 2.335 ug/l
RT: 8.701 min Scan# 1150
Delta R.T. 0.006 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42

Tgt Ion: 43 Resp: 37248
Ion Ratio Lower Upper
43 100
61 3.3 22.7 34.1#
87 0.1 13.6 20.4#


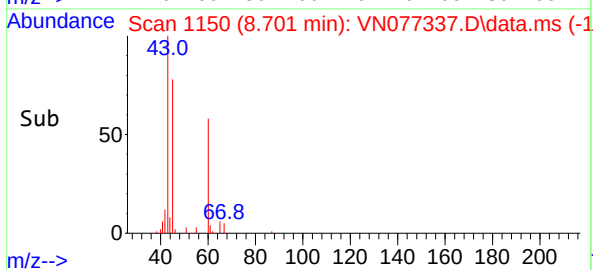

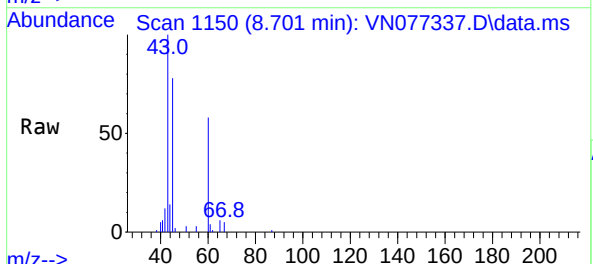




#48
Methyl methacrylate
Concen: 0.319 ug/l
RT: 9.654 min Scan# 11
Delta R.T. -0.029 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42




Instrument :
MSVOA_N
ClientSampleId :
SEW-30994


Tgt Ion: 41 Resp: 2172
Ion Ratio Lower Upper
41 100
69 0.0 85.0 127.6#
39 46.7 53.5 80.3#

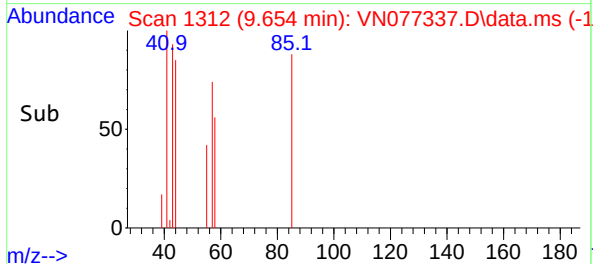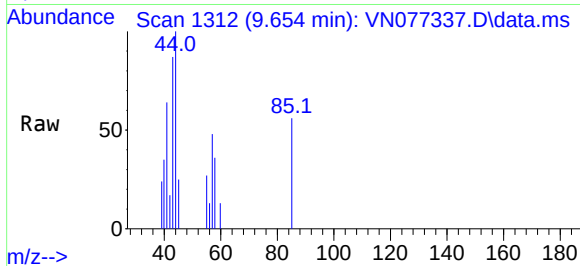

#50
Toluene-d8
Concen: 48.108 ug/l
RT: 10.572 min Scan# 1468
Delta R.T. -0.000 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42

Tgt Ion: 98 Resp: 1265109
Ion Ratio Lower Upper
98 100
100 64.6 51.3 76.9


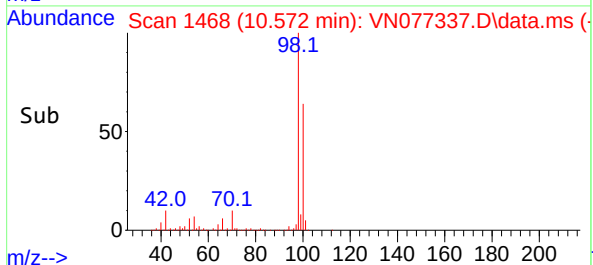

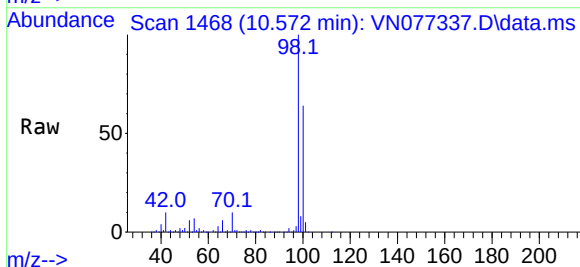




#55
1,1,2-Trichloroethane
Concen: 0.661 ug/l
RT: 11.007 min Scan# 11
Delta R.T. -0.012 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42




Instrument :
MSVOA_N
ClientSampleId :
SEW-30994


Tgt Ion: 97	Resp: 5121
Ion Ratio	Lower Upper
97 100	
83 0.0	67.4 101.2#
85 0.0	44.1 66.1#
99 0.0	49.8 74.6#

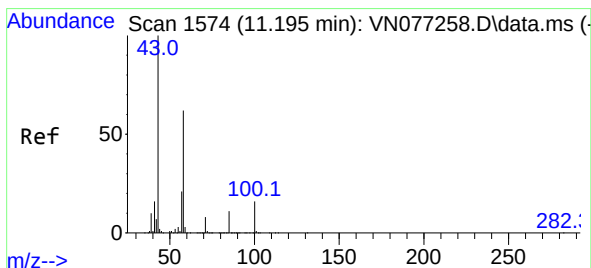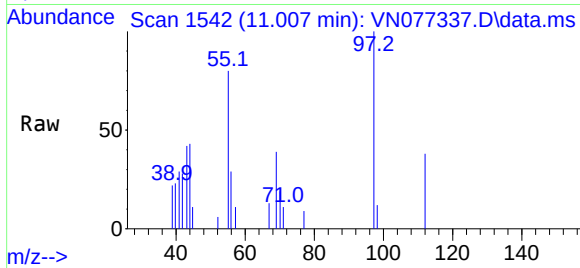

#59
2-Hexanone
Concen: 0.965 ug/l
RT: 11.178 min Scan# 1571
Delta R.T. -0.017 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42

Tgt Ion: 43	Resp: 6631		
Ion Ratio	Lower	Upper	
43 100			
58 15.6	30.9	92.5#	


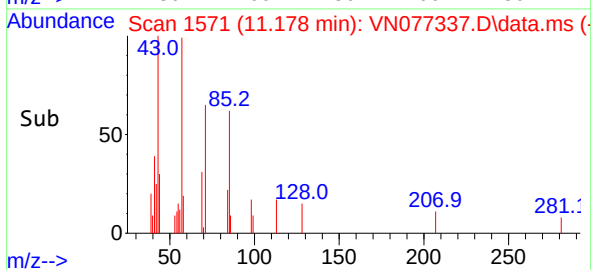

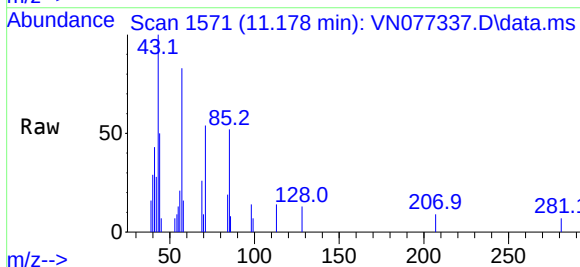




#62
4-Bromofluorobenzene
Concen: 50.911 ug/l
RT: 12.854 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42




Instrument :
MSVOA_N
ClientSampleId :
SEW-30994


Tgt Ion: 95 Resp: 445282
Ion Ratio Lower Upper
95 100
174 71.4 0.0 146.8
176 70.0 0.0 139.6



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.872 min Scan# 1689
Delta R.T. 0.001 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42

Tgt Ion: 117 Resp: 907250
Ion Ratio Lower Upper
117 100
82 55.1 42.9 64.3
119 34.2 26.2 39.4


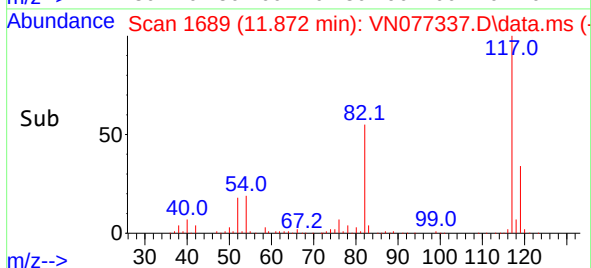
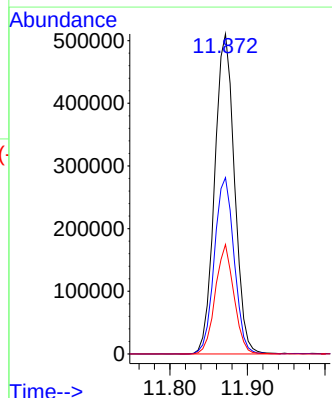





#71
Bromoform
Concen: 0.391 ug/l
RT: 12.854 min Scan# 1810
Delta R.T. 0.271 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42




Instrument :
MSVOA_N
ClientSampleId :
SEW-30994


Tgt Ion:173 Resp: 2081
Ion Ratio Lower Upper
173 100
175 820.8 24.1 72.4#
254 0.0 0.1 0.1#

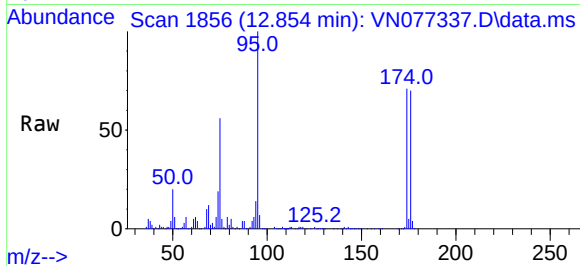

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.801 min Scan# 2017
Delta R.T. 0.006 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42

Tgt Ion:152 Resp: 434345
Ion Ratio Lower Upper
152 100
115 63.1 32.1 96.3
150 157.7 0.0 354.8


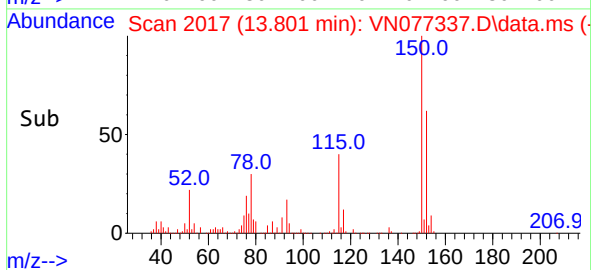

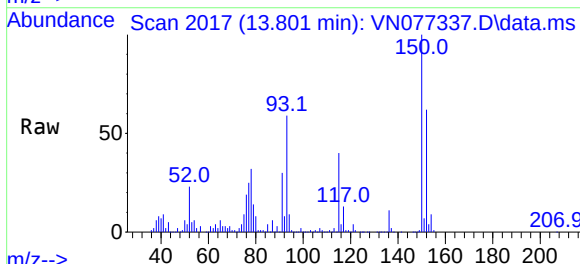




#73
Isopropylbenzene
Concen: 4.128 ug/l
RT: 12.713 min Scan# 1832
Delta R.T. 0.012 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42




Instrument :
MSVOA_N
ClientSampleId :
SEW-30994


Tgt Ion:105 Resp: 174148
Ion Ratio Lower Upper
105 100
120 4.4 13.2 39.6#



#74
N-ethyl acetate
Concen: 1.456 ug/l
RT: 12.483 min Scan# 1793
Delta R.T. -0.012 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42

Tgt Ion: 43 Resp: 23274
Ion Ratio Lower Upper
43 100
70 18.8 41.0 61.6#
55 38.4 19.3 28.9#
61 0.0 22.0 33.0#


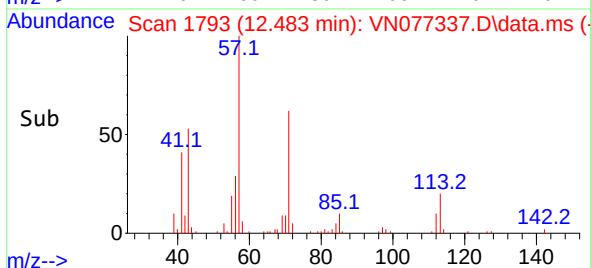
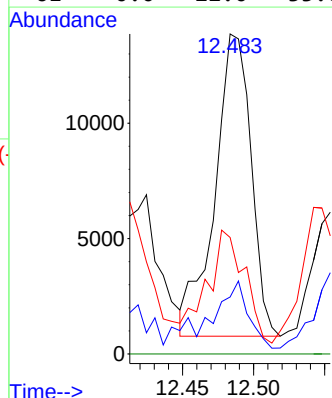





#75
1,1,2,2-Tetrachloroethane
Concen: 0.233 ug/l
RT: 12.913 min Scan# 1866
Delta R.T. -0.029 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42




Instrument :
MSVOA_N
ClientSampleId :
SEW-30994


Tgt Ion: 83 Resp: 3083
Ion Ratio Lower Upper
83 100
131 0.0 4.9 14.6#
85 0.0 32.1 96.3#

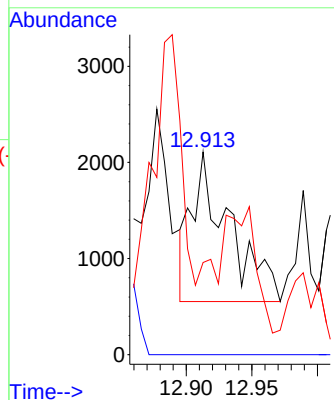

#76
1,2,3-Trichloropropane
Concen: 23.688 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. -0.141 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42

Tgt Ion: 75 Resp: 245001
Ion Ratio Lower Upper
75 100
77 0.0 88.3 264.9#


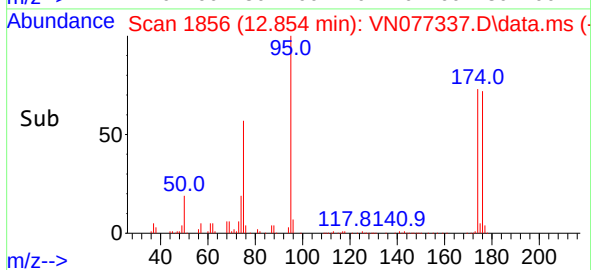
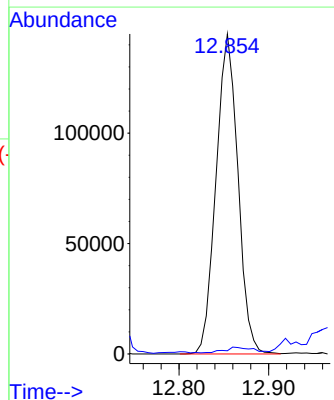





#78
n-propylbenzene
Concen: 0.354 ug/l
RT: 13.060 min Scan# 1888
Delta R.T. 0.018 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42




Instrument :
MSVOA_N
ClientSampleId :
SEW-30994


Tgt Ion: 91 Resp: 16509
Ion Ratio Lower Upper
91 100
120 7.8 11.5 34.5#

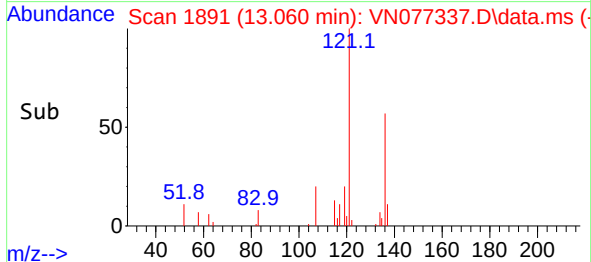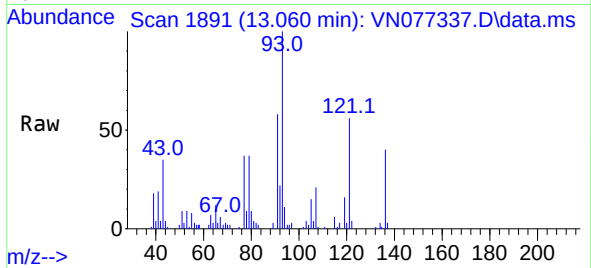

#79
2-Chlorotoluene
Concen: 17.233 ug/l
RT: 13.189 min Scan# 1913
Delta R.T. 0.059 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42

Tgt Ion: 91 Resp: 483688
Ion Ratio Lower Upper
91 100
126 0.1 16.8 50.4#


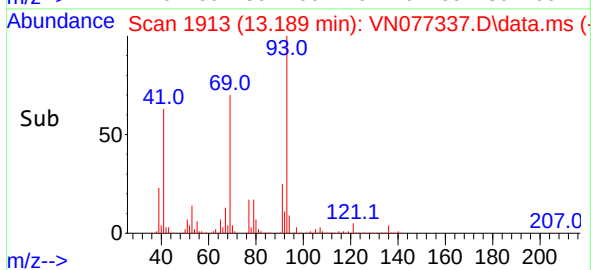






#81
trans-1,4-Dichloro-2-butene
Concen: 53.305 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. 0.112 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42




Instrument :
MSVOA_N
ClientSampleId :
SEW-30994


Tgt Ion: 75 Resp: 245001
Ion Ratio Lower Upper
75 100
53 0.0 72.8 109.2#
89 0.0 37.4 56.2#



#82
4-Chlorotoluene
Concen: 18.278 ug/l
RT: 13.189 min Scan# 1913
Delta R.T. -0.035 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42

Tgt Ion: 91 Resp: 483688
Ion Ratio Lower Upper
91 100
126 0.1 16.9 50.7#


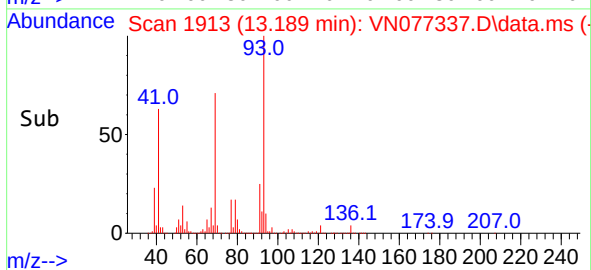






#83
tert-Butylbenzene
Concen: 3.140 ug/l
RT: 13.601 min Scan# 1956
Delta R.T. 0.159 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42




Instrument :
MSVOA_N
ClientSampleId :
SEW-30994


Tgt Ion:119 Resp: 94186
Ion Ratio Lower Upper
119 100
91 506.3 33.5 100.4#
134 18.8 13.3 39.9



#84
1,2,4-Trimethylbenzene
Concen: 5.086 ug/l
RT: 13.601 min Scan# 1983
Delta R.T. 0.118 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42

Tgt Ion:105 Resp: 169318
Ion Ratio Lower Upper
105 100
120 11.1 22.5 67.5#


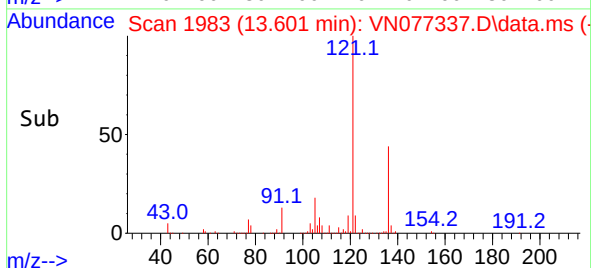
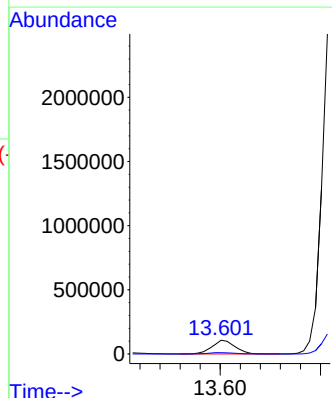





#85
 sec-Butylbenzene
 Concen: 4.051 ug/l
 RT: 13.601 min Scan# 1983
 Delta R.T. -0.017 min
 Lab File: VN077337.D
 Acq: 13 Apr 2023 18:42




Instrument :
 MSVOA_N
 ClientSampleId :
 SEW-30994


Tgt Ion:105 Resp: 169318
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.8 29.4#

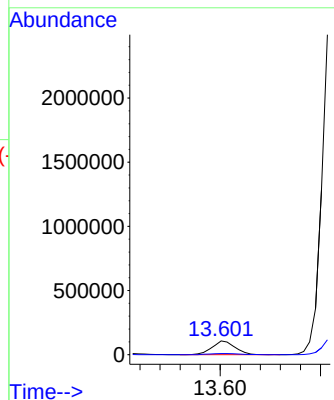

#86
 p-Isopropyltoluene
 Concen: 94.410 ug/l
 RT: 13.730 min Scan# 2005
 Delta R.T. 0.000 min
 Lab File: VN077337.D
 Acq: 13 Apr 2023 18:42

Tgt Ion:119 Resp: 3101392
 Ion Ratio Lower Upper
 119 100
 134 19.2 12.9 38.6
 91 0.0 12.3 36.8#


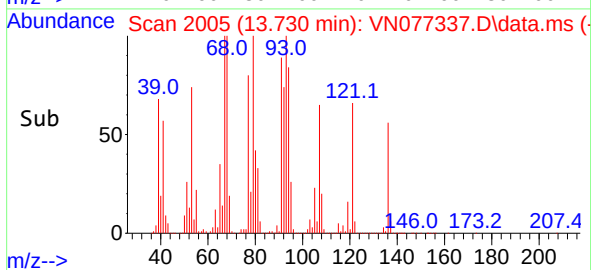
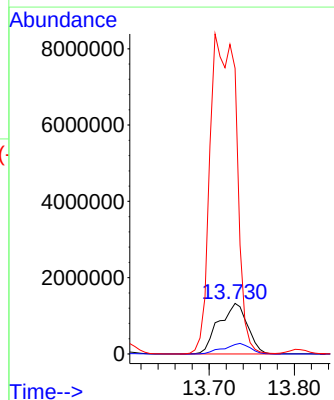





#89
n-Butylbenzene
Concen: 65.594 ug/l
RT: 13.954 min Scan# 2061
Delta R.T. -0.106 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42




Instrument :
MSVOA_N
ClientSampleId :
SEW-30994


Tgt Ion: 91 Resp: 1788829
Ion Ratio Lower Upper
91 100
92 41.2 26.7 80.0
134 2.1 12.8 38.3#



#90
Hexachloroethane
Concen: 0.439 ug/l
RT: 14.283 min Scan# 2099
Delta R.T. -0.053 min
Lab File: VN077337.D
Acq: 13 Apr 2023 18:42

Tgt Ion: 117 Resp: 3154
Ion Ratio Lower Upper
117 100
201 0.0 29.8 89.5#

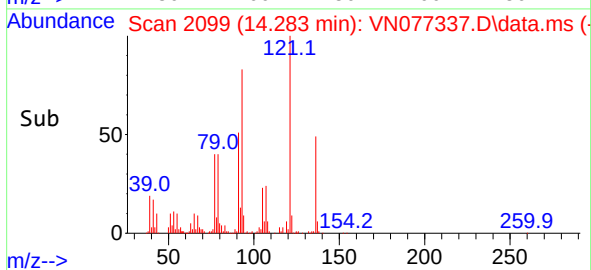



#96
 1,2,3-Trichlorobenzene
 Concen: 0.263 ug/l
 RT: 15.777 min Scan# 21
 Delta R.T. 0.023 min
 Lab File: VN077337.D
 Acq: 13 Apr 2023 18:42

Instrument :
 MSVOA_N
 ClientSampleId :
 SEW-30994

Tgt Ion	Ratio	Lower	Upper
180	100		
182	8.3	46.9	140.8#
145	44.0	17.6	52.8

