
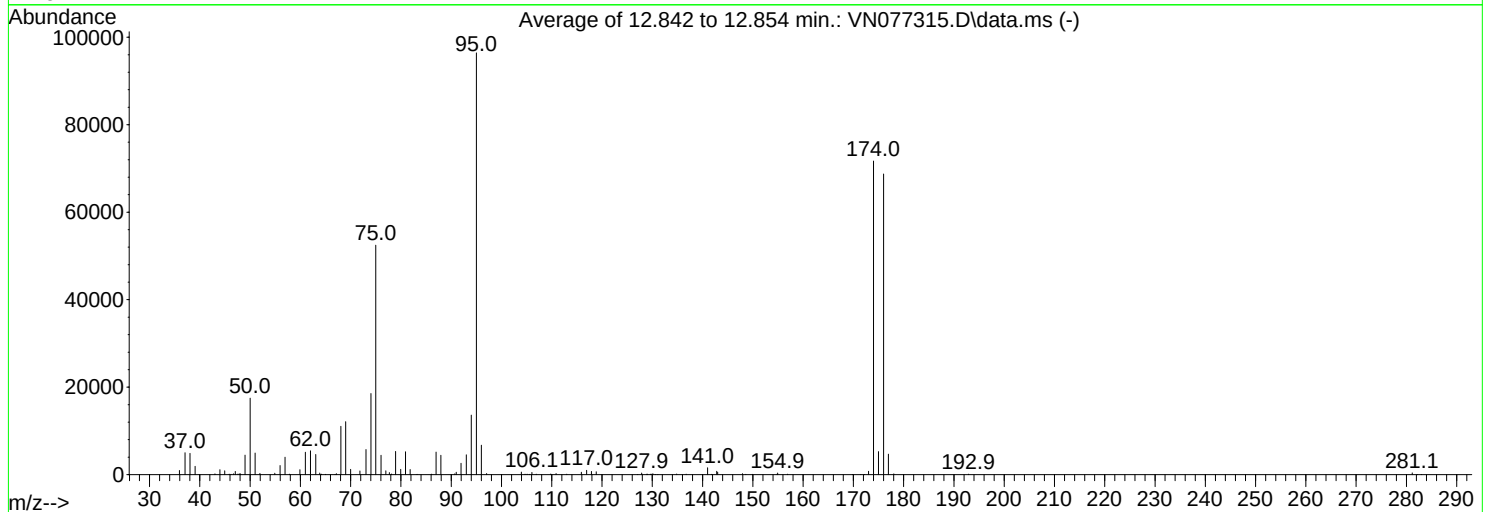


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041323\
Data File : VN077315.D
Acq On : 13 Apr 2023 08:32
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N040523W.M
Title : SW846 8260
Last Update : Thu Apr 06 08:27:03 2023

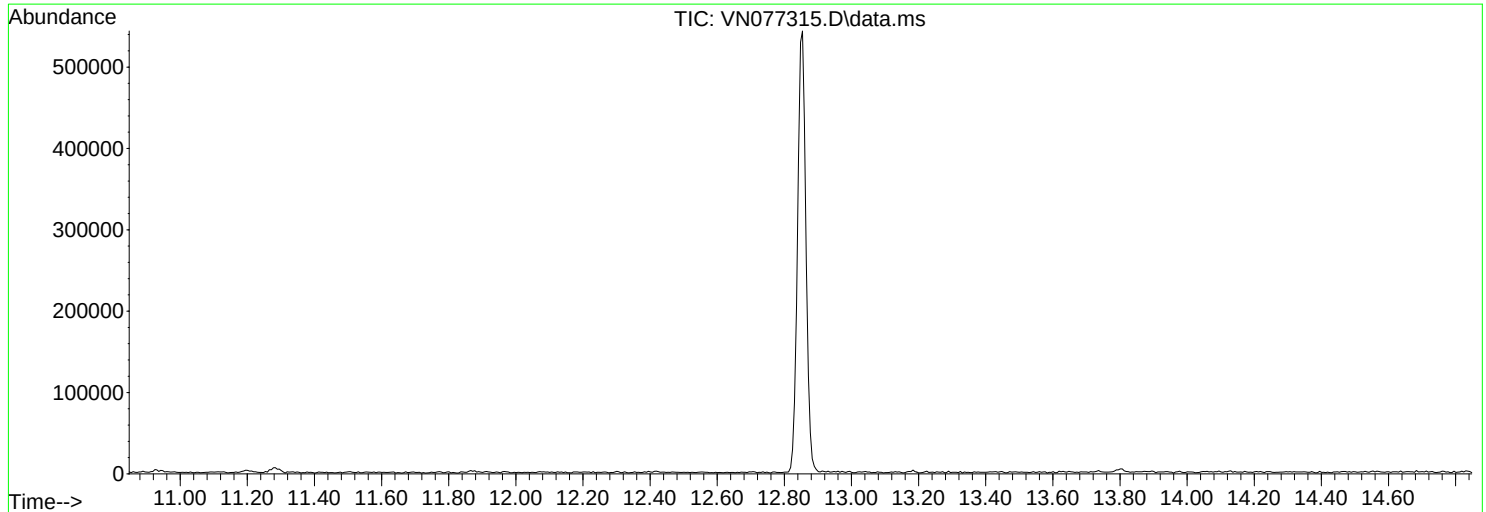

AutoFind: Scans 1854, 1855, 1856; Background Corrected with Scan 1847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	17488	PASS
75	95	30	60	54.4	52461	PASS
95	95	100	100	100.0	96429	PASS
96	95	5	9	7.0	6742	PASS
173	174	0.00	2	1.1	753	PASS
174	95	50	100	74.4	71712	PASS
175	174	5	9	7.3	5267	PASS
176	174	95	101	95.8	68725	PASS
177	176	5	9	6.8	4683	PASS

Average of 12.842 to 12.854 min.: VN077315.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	936	47.05	747	57.85	127	69.00	1209
37.05	5000	47.60	152	59.90	1122	70.00	122
38.05	4850	47.90	203	61.00	5117	71.85	83
39.05	1901	48.10	203	62.00	5453	73.05	574
39.90	33	49.00	4466	63.05	4595	74.05	18551
43.00	201	50.00	17488	63.85	375	75.00	52461
44.00	1128	51.00	4926	64.20	97	76.05	4430
44.95	864	51.95	286	65.00	61	77.00	886
45.85	115	54.90	317	66.90	88	77.70	468
46.20	69	55.95	2091	67.15	221	78.10	149
46.70	175	56.95	3976	68.05	11038	78.95	5318

Average of 12.842 to 12.854 min.: VN077315.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.95	1195	94.00	13601	110.85	260	129.90	102
80.90	5245	95.00	96429	113.00	103	130.10	230
81.85	1180	96.00	6742	115.90	557	130.60	51
83.20	79	97.05	264	116.95	989	131.10	52
86.10	113	103.95	607	117.90	740	134.85	154
87.00	5166	104.70	129	118.85	671	136.75	125
87.95	4417	105.10	103	127.10	55	141.00	1588
90.70	175	105.60	69	127.90	376	141.80	69
91.00	543	106.05	528	128.90	126	142.80	762
91.95	2592	106.90	103	129.05	102	143.00	540
93.00	4551	109.80	135	129.60	111	147.95	232

Average of 12.842 to 12.854 min.: VN077315.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
148.60	67	176.00	68725				
149.90	62	176.95	4683				
154.80	97	178.05	175				
154.95	363	192.90	105				
156.90	101	281.15	411				
169.80	58	282.20	54				
171.50	53	283.00	58				
172.20	55						
173.00	753						
174.00	71712						
175.00	5267						

Instrument :

MSVOA_N

ClientSampleId :

BFB