


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN041419\
 Data File : VN055021.D
 Acq On : 13 Apr 2019 10:02
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N041319W.M
 Title : SW846 8260
 Last Update : Sat Apr 13 03:34:24 2019

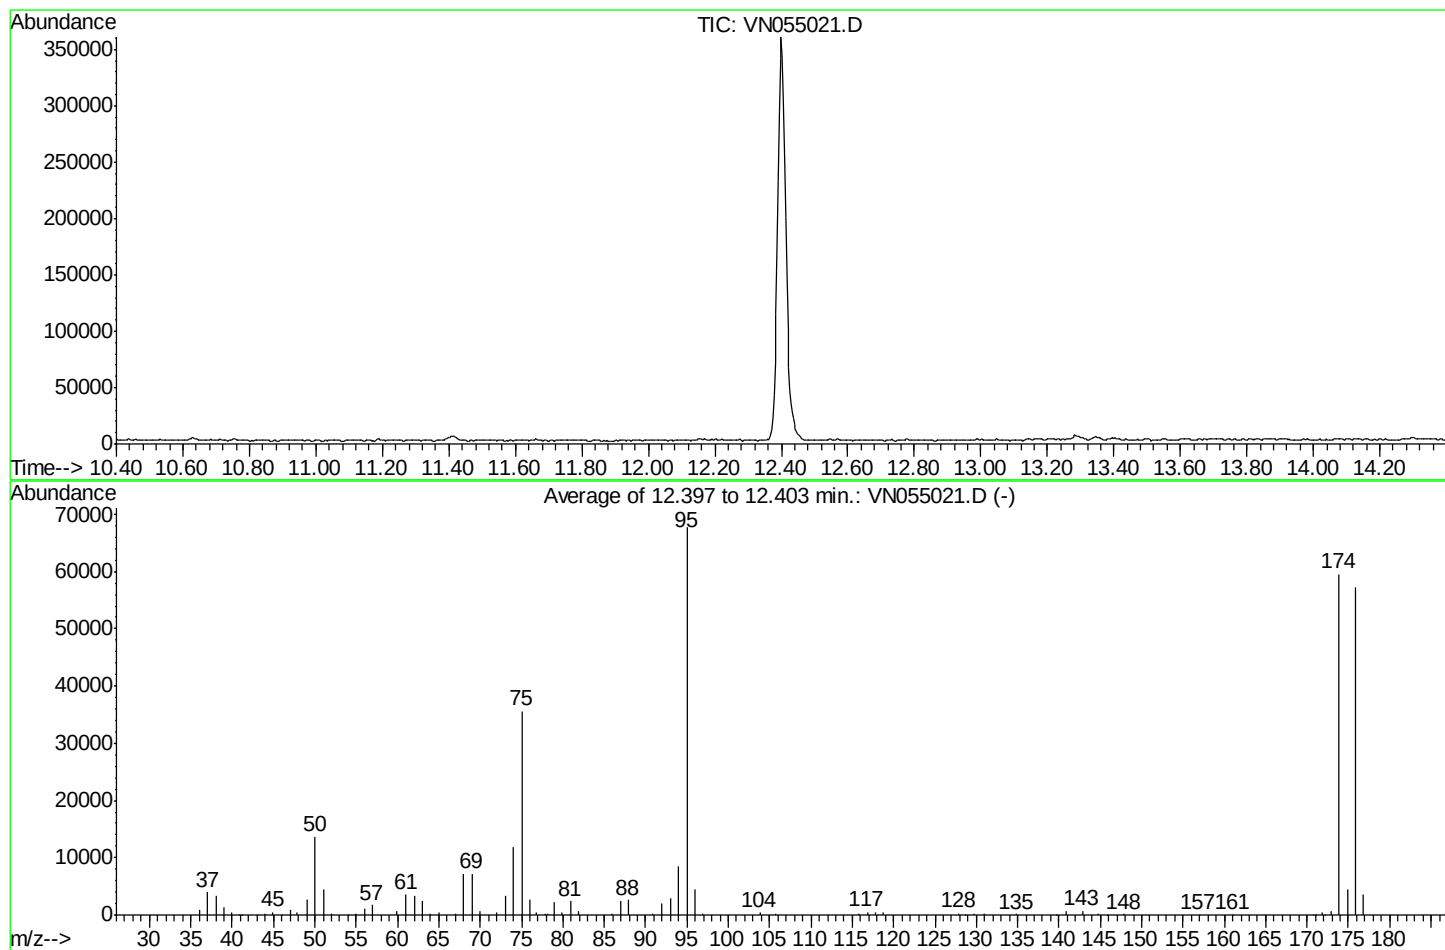

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	13678	PASS
75	95	30	60	52.6	35600	PASS
95	95	100	100	100.0	67720	PASS
96	95	5	9	6.7	4558	PASS
173	174	0.00	2	1.1	665	PASS
174	95	50	100	87.8	59480	PASS
175	174	5	9	7.5	4479	PASS
176	174	95	101	96.1	57184	PASS
177	176	5	9	6.3	3629	PASS