
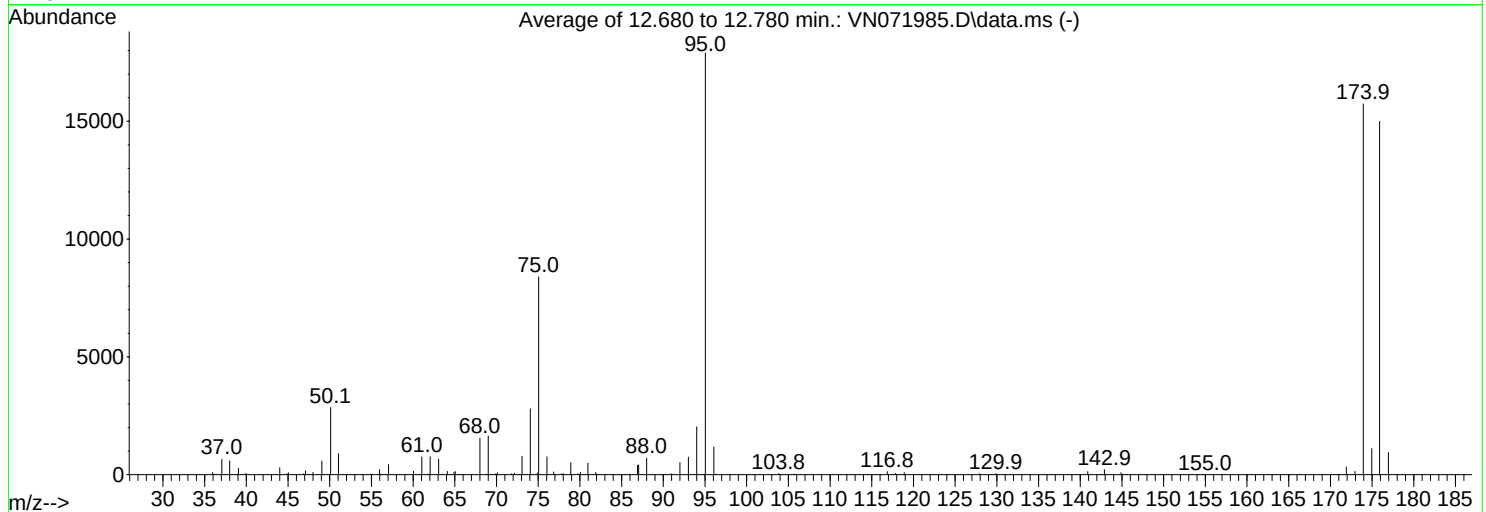


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041422\
Data File : VN071985.D
Acq On : 14 Apr 2022 09:13
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N032422W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Mar 24 12:03:44 2022

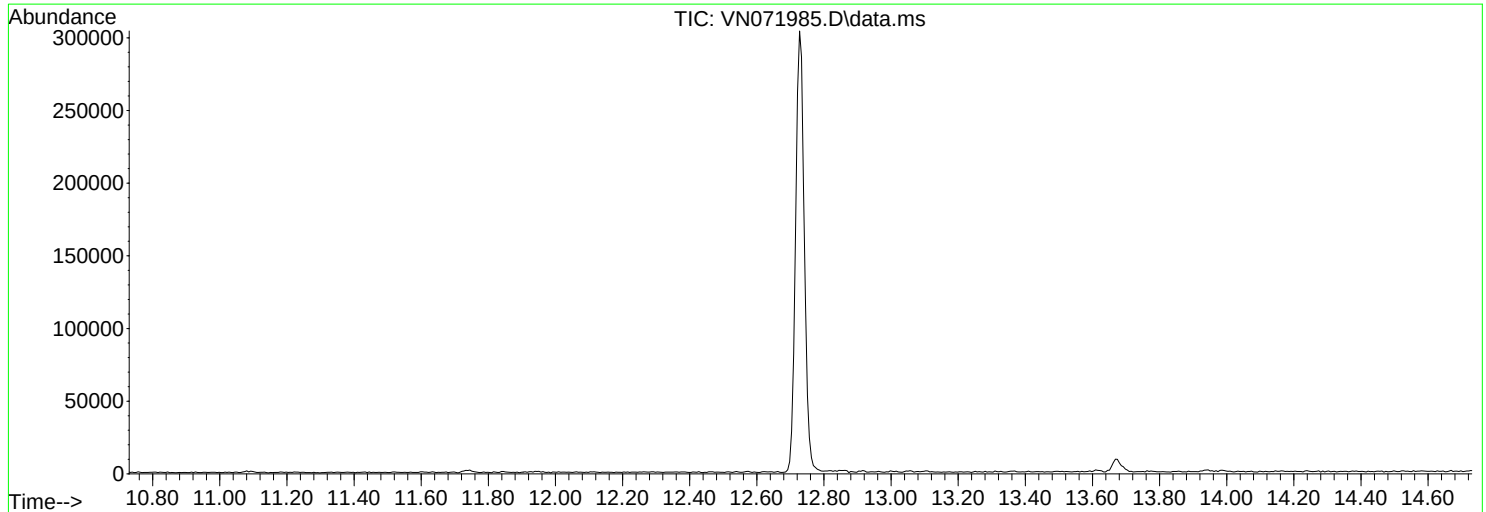

AutoFind: Averaged scan 1818 to 1835; Bkg corrected with scan 1817

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.9	2844	PASS
75	95	30	60	46.9	8393	PASS
95	95	100	100	100.0	17903	PASS
96	95	5	9	6.6	1175	PASS
173	174	0.00	2	0.9	139	PASS
174	95	50	100	87.9	15738	PASS
175	174	5	9	7.0	1105	PASS
176	174	95	101	95.3	14998	PASS
177	176	5	9	6.3	940	PASS