
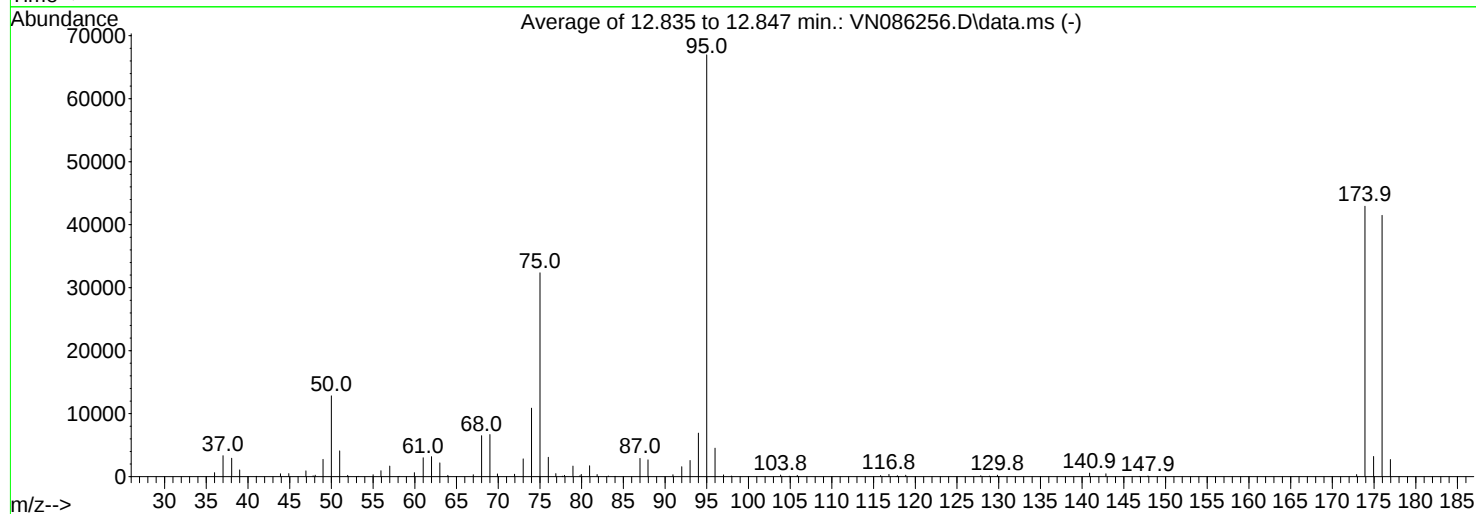


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041425\
Data File : VN086256.D
Acq On : 14 Apr 2025 08:59
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N041125W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Sat Apr 12 01:21:52 2025

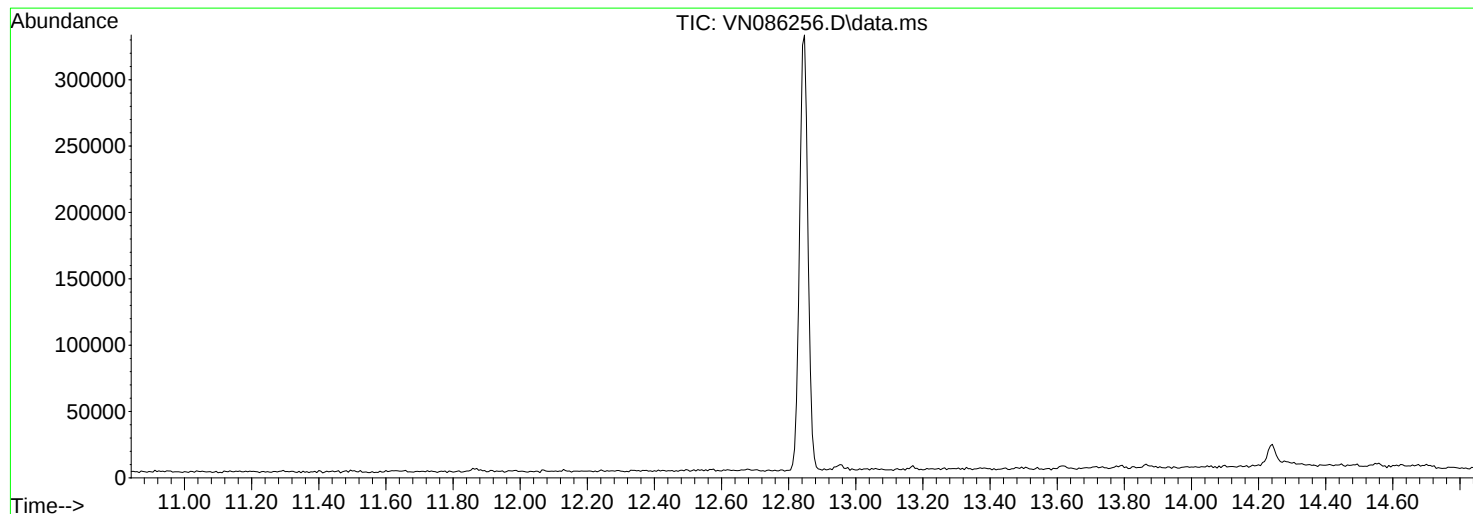

AutoFind: Scans 1850, 1851, 1852; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	12839	PASS
75	95	30	60	48.3	32352	PASS
95	95	100	100	100.0	66968	PASS
96	95	5	9	6.8	4521	PASS
173	174	0.00	2	0.8	342	PASS
174	95	50	100	64.1	42933	PASS
175	174	5	9	7.5	3209	PASS
176	174	95	101	96.7	41499	PASS
177	176	5	9	6.6	2730	PASS