


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN041519\
 Data File : VN055033.D
 Acq On : 15 Apr 2019 8:40
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N041519W.M
 Title : SW846 8260
 Last Update : Mon Apr 15 12:28:28 2019

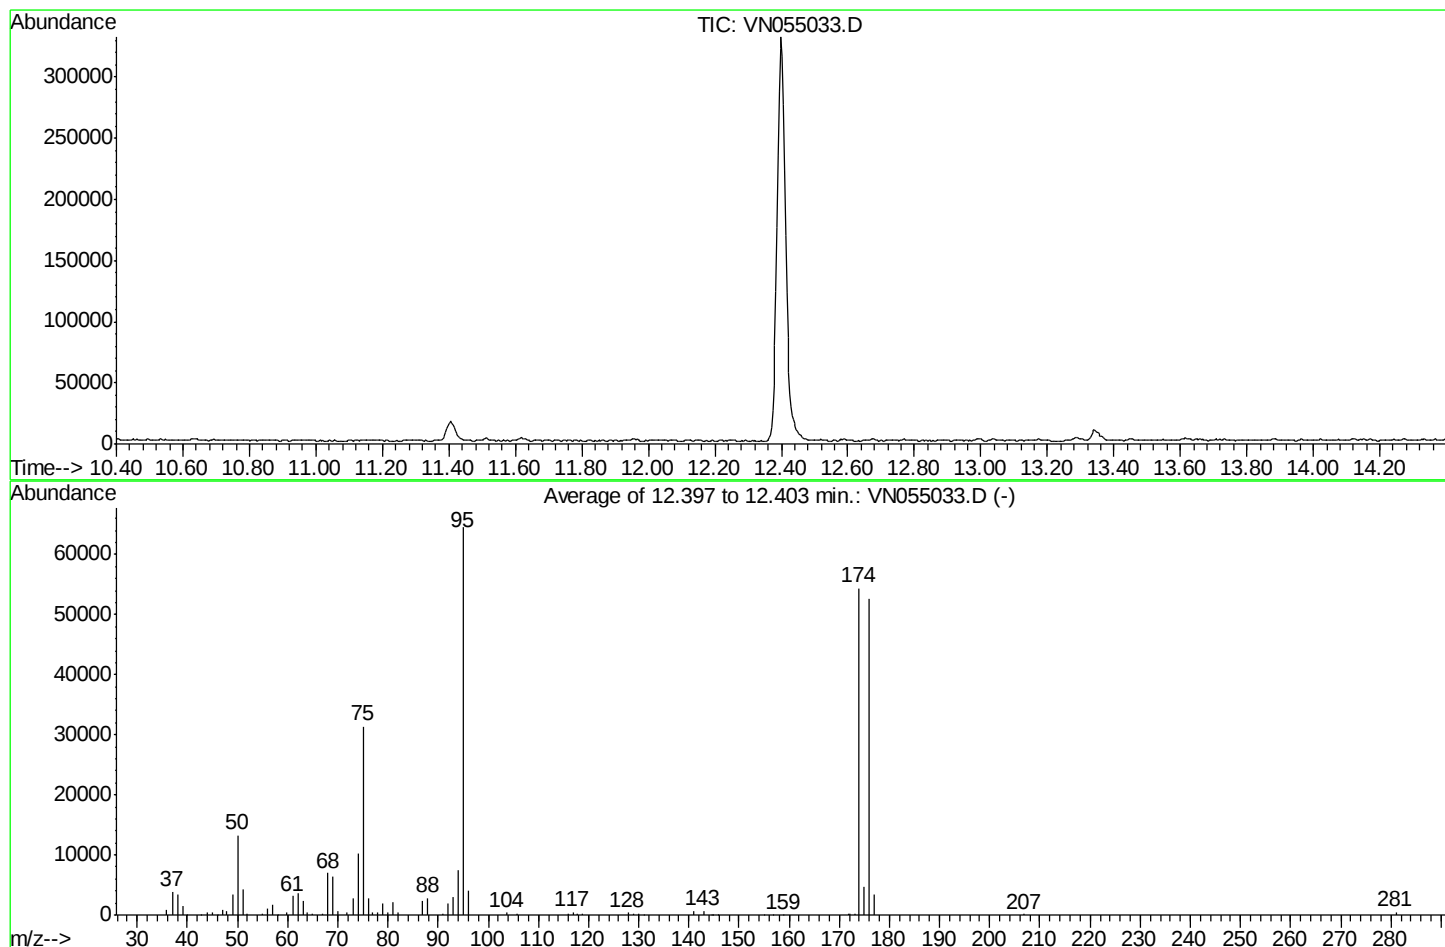

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	13248	PASS
75	95	30	60	48.6	31352	PASS
95	95	100	100	100.0	64536	PASS
96	95	5	9	6.4	4157	PASS
173	174	0.00	2	0.5	274	PASS
174	95	50	100	84.2	54341	PASS
175	174	5	9	8.7	4728	PASS
176	174	95	101	96.8	52592	PASS
177	176	5	9	6.5	3443	PASS