


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN041519\
 Data File : VN055046.D
 Acq On : 15 Apr 2019 16:23
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N041519W.M
 Title : SW846 8260
 Last Update : Mon Apr 15 12:28:28 2019

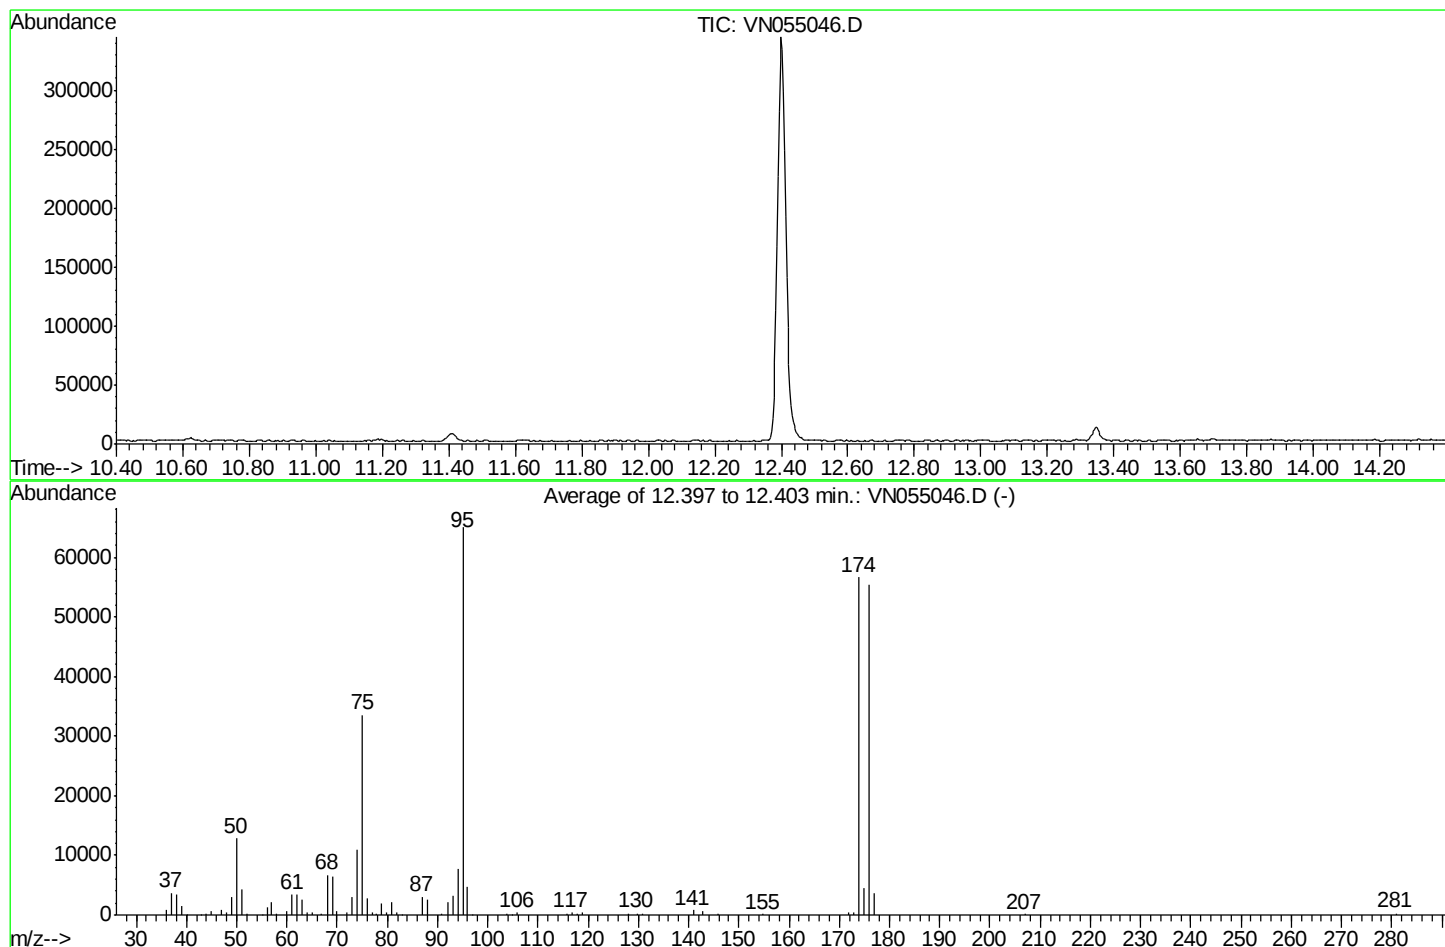

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	12799	PASS
75	95	30	60	51.7	33602	PASS
95	95	100	100	100.0	65032	PASS
96	95	5	9	7.3	4778	PASS
173	174	0.00	2	0.8	478	PASS
174	95	50	100	87.1	56621	PASS
175	174	5	9	7.9	4465	PASS
176	174	95	101	98.0	55496	PASS
177	176	5	9	6.5	3608	PASS