


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN041520\
Data File : VN060949.D
Acq On : 15 Apr 2020 9:42
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031820W.M
Title : SW846 8260
Last Update : Wed Mar 18 08:49:09 2020

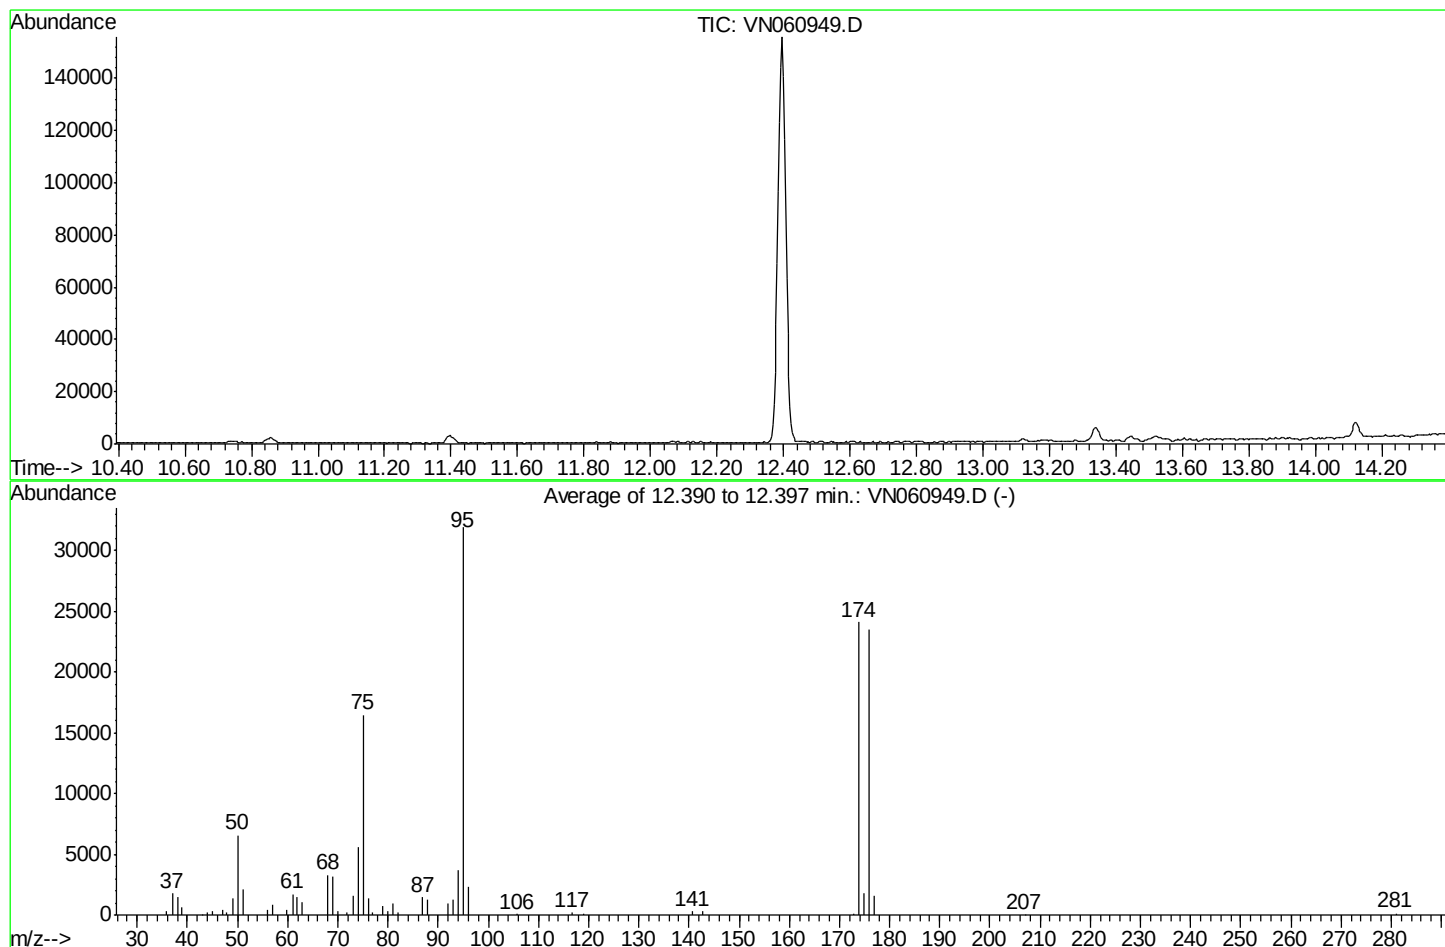

AutoFind: Scans 3302, 3303, 3304; Background Corrected with Scan 3289

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	6570	PASS
75	95	30	60	51.6	16469	PASS
95	95	100	100	100.0	31912	PASS
96	95	5	9	7.2	2289	PASS
173	174	0.00	2	0.3	81	PASS
174	95	50	100	75.5	24096	PASS
175	174	5	9	7.5	1801	PASS
176	174	95	101	97.5	23504	PASS
177	176	5	9	6.9	1613	PASS