

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041521\
 Data File : VN066623.D
 Acq On : 15 Apr 2021 19:53
 Operator : JC/MD
 Sample : M2030-04
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Apr 16 07:54:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041521W.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 15 19:16:35 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.588	168	239775	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.516	114	376469	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.348	117	377985	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.290	152	158545	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.950	65	178674	49.40	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	98.80%		
35) Dibromofluoromethane	7.510	113	137806	52.78	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	105.56%		
50) Toluene-d8	10.029	98	564806	55.20	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	110.40%		
62) 4-Bromofluorobenzene	12.346	95	192541	53.51	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	107.02%		
Target Compounds						Qvalue
3) Chloromethane	2.034	50	1370	0.32	ug/l #	84
11) Tert butyl alcohol	4.708	59	186	0.32	ug/l #	73
13) Acrolein	3.538	56	947	3.06	ug/l	98
14) Allyl chloride	4.453	41	227	0.21	ug/l #	25
16) Acetone	3.756	43	16749	4.61	ug/l	93
18) Methyl Acetate	4.257	43	5137	1.32	ug/l #	66
20) Methylene Chloride	4.466	84	14211	4.16	ug/l	88
25) 2-Butanone	6.757	43	2189	1.03	ug/l	89
31) Cyclohexane	7.586	56	5062	0.97	ug/l #	1
36) 1,1-Dichloropropene	7.588	75	18359	4.84	ug/l #	47
37) Ethyl Acetate	6.757	43	2189	0.51	ug/l #	68
38) Carbon Tetrachloride	7.586	117	21486	6.04	ug/l #	17
39) Methylcyclohexane	9.181	83	1109	0.26	ug/l #	20
43) Isopropyl Acetate	8.095	43	23694	3.30	ug/l #	86
45) 1,2-Dichloropropane	9.200	63	1966	0.58	ug/l #	44
47) Bromodichloromethane	9.181	83	1109	0.27	ug/l #	50
48) Methyl methacrylate	9.112	41	6747	2.09	ug/l #	10
51) 4-Methyl-2-Pentanone	9.924	43	5399	1.28	ug/l	88
54) cis-1,3-Dichloropropene	9.844	75	36808	7.43	ug/l #	63
56) Ethyl methacrylate	10.294	69	113	0.92	ug/l #	27
57) 1,3-Dichloropropane	10.705	76	21155	4.27	ug/l #	43
59) 2-Hexanone	10.707	43	323910	110.27	ug/l #	50
71) Bromoform	12.346	173	1295	0.58	ug/l #	1
74) N-amyl acetate	12.030	43	73	9.74	ug/l #	1
76) 1,2,3-Trichloropropane	12.346	75	95172	25.67	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.346	75	95172	79.21	ug/l #	12
84) 1,2,4-Trimethylbenzene	12.992	105	2857	0.30	ug/l	90
88) 1,4-Dichlorobenzene	13.312	146	52	Below Cal	#	25
90) Hexachloroethane	13.843	117	584	0.28	ug/l #	12
95) Naphthalene	15.076	128	50754	6.27	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041521\
Data File : VN066623.D
Acq On : 15 Apr 2021 19:53
Operator : JC/MD
Sample : M2030-04
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Apr 16 07:54:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041521W.M
Quant Title : SW846 8260
QLast Update : Thu Apr 15 19:16:35 2021
Response via : Initial Calibration




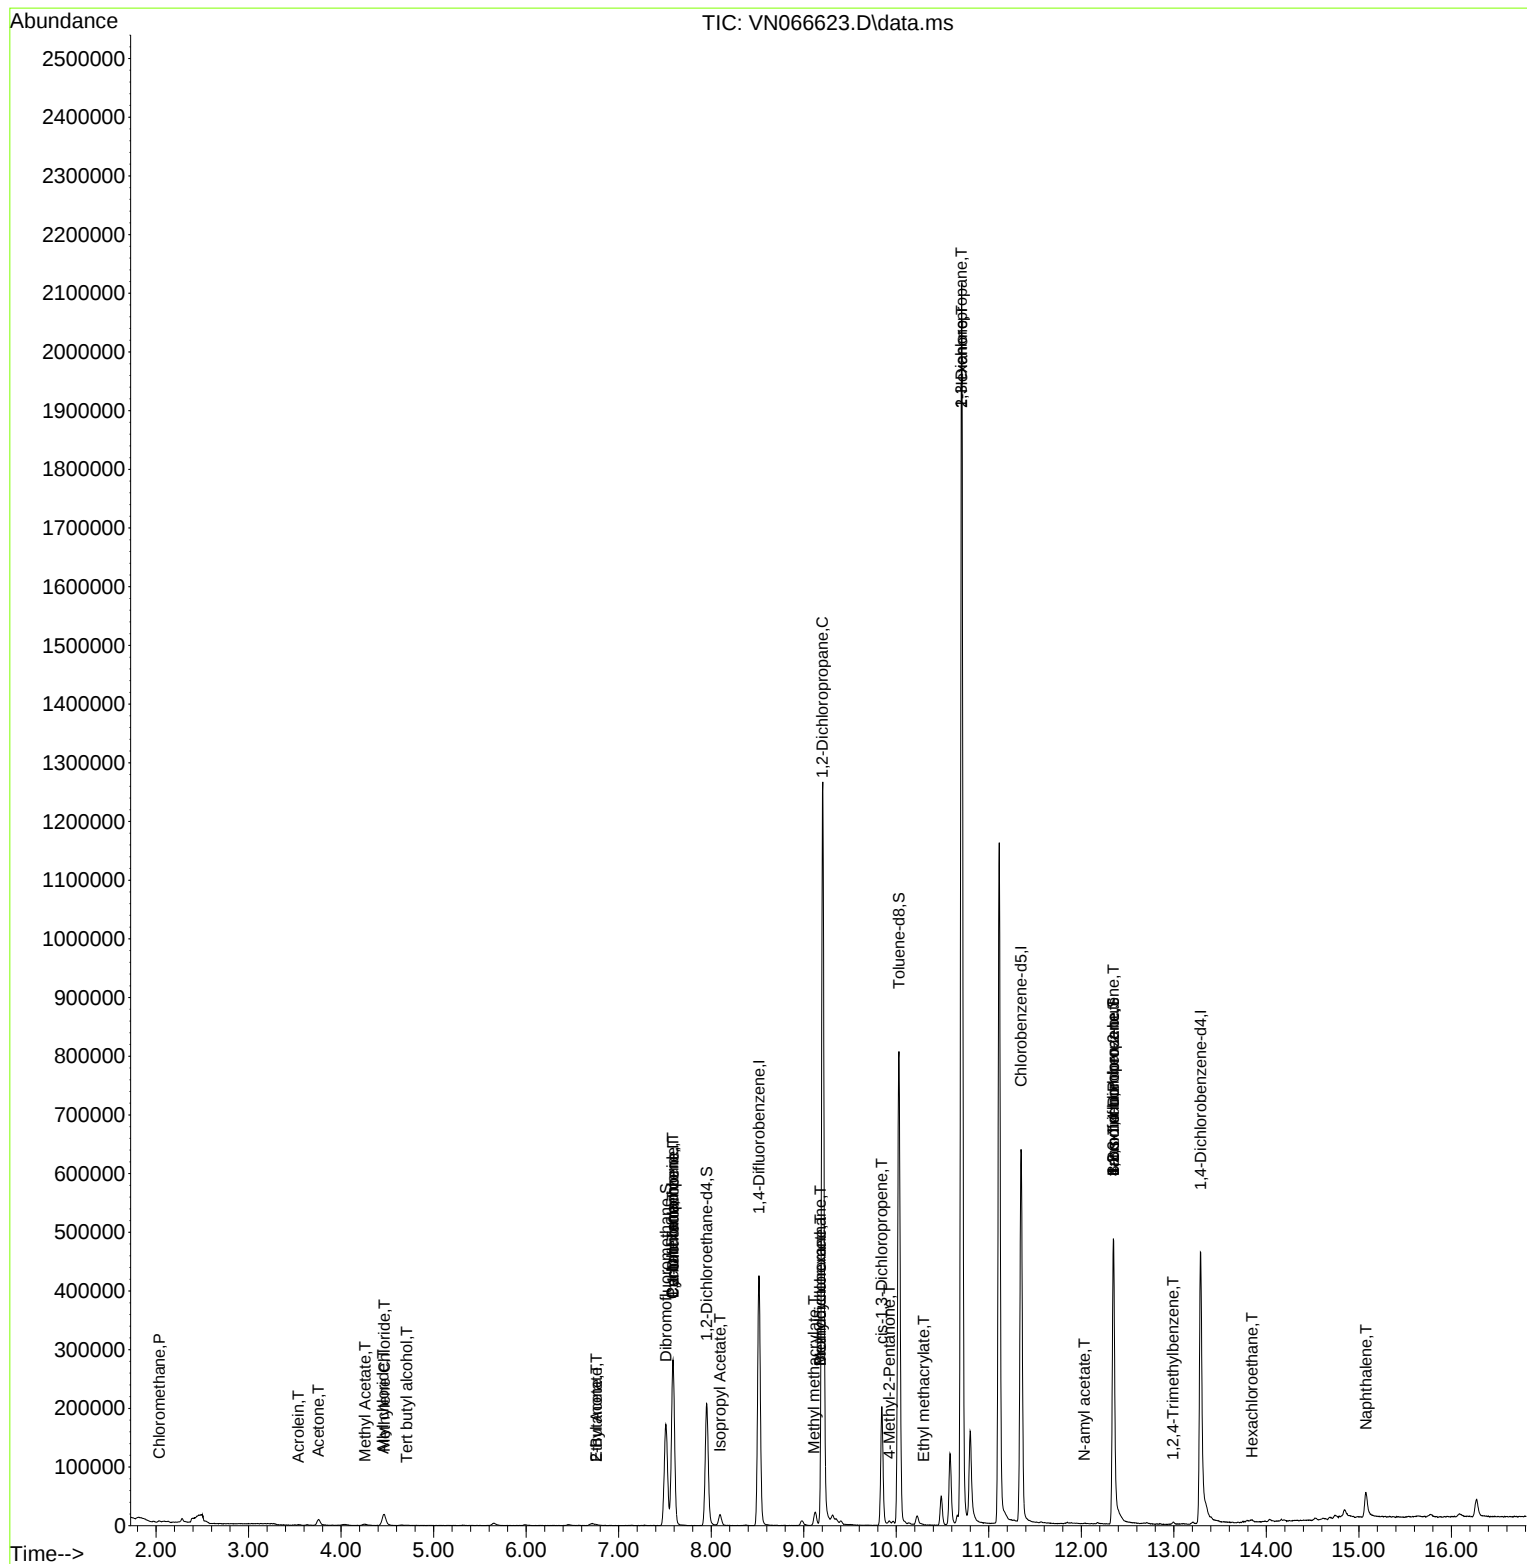




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.588 min Scan# 2187
Delta R.T. 0.000 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 239775
Ion Ratio Lower Upper
168 100
99 53.1 42.6 63.8

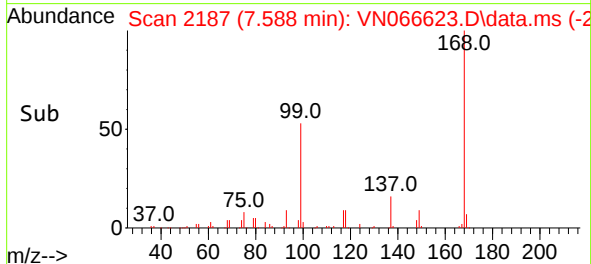

#3
Chloromethane
Concen: 0.32 ug/l
RT: 2.034 min Scan# 116
Delta R.T. 0.003 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53

Tgt Ion: 50 Resp: 1370
Ion Ratio Lower Upper
50 100
52 41.4 25.8 38.8#

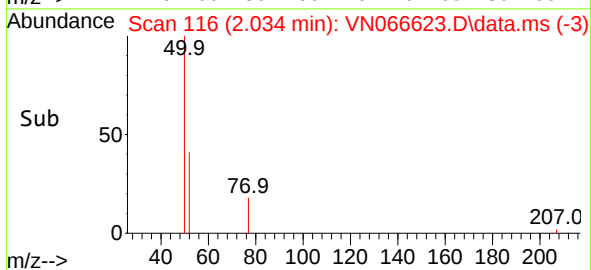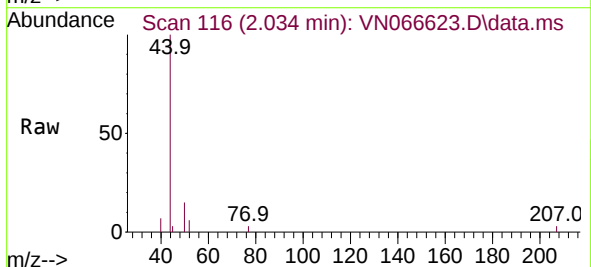




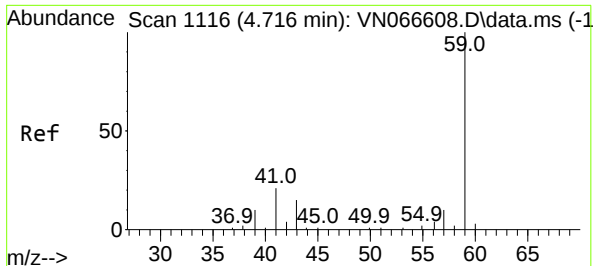


#11

Tert butyl alcohol
Concen: 0.32 ug/l
RT: 4.708 min Scan# 1113
Delta R.T. -0.008 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion: 59 Resp: 186
Ion Ratio Lower Upper
59 100
57 0.0 8.0 12.0#

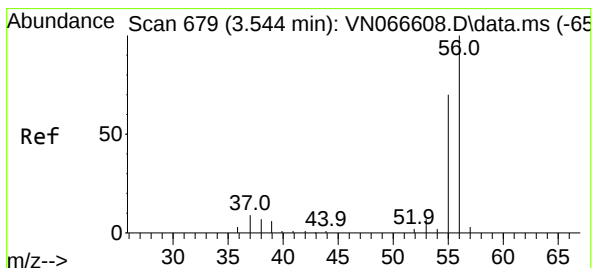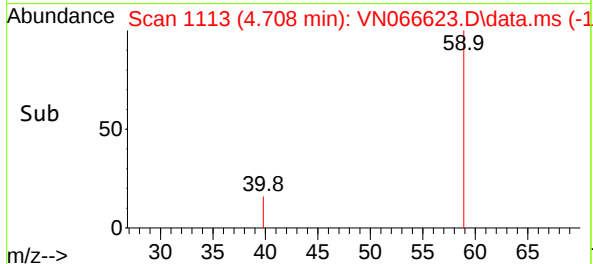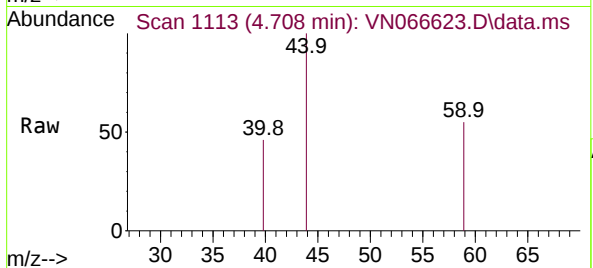


#13

Acrolein
Concen: 3.06 ug/l
RT: 3.538 min Scan# 677
Delta R.T. -0.006 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53


Tgt Ion: 56 Resp: 947
Ion Ratio Lower Upper
56 100
55 72.0 56.0 84.0

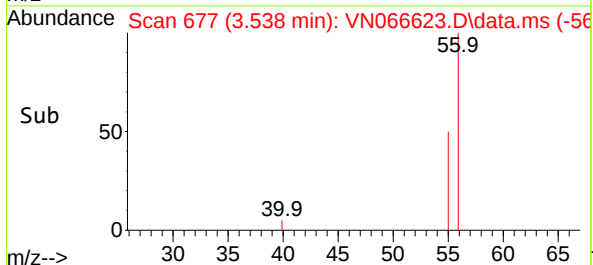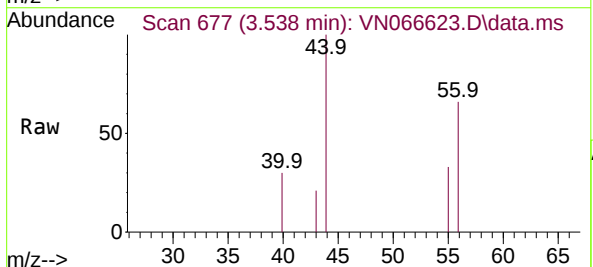






#14
Allyl chloride
Concen: 0.21 ug/l
RT: 4.453 min Scan# 1018
Delta R.T. 0.209 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53


Instrument :
MSVOA_N
ClientSampled :





Tgt Ion: 41 Resp: 227
Ion Ratio Lower Upper
41 100
39 0.0 53.0 79.4#
76 0.0 28.9 43.3#




#16
Acetone
Concen: 4.61 ug/l
RT: 3.756 min Scan# 758
Delta R.T. 0.003 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53

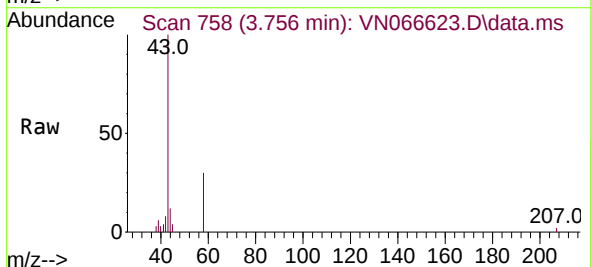


Tgt Ion: 43 Resp: 16749
Ion Ratio Lower Upper
43 100
58 30.0 27.0 40.6








#18
Methyl Acetate
Concen: 1.32 ug/l
RT: 4.257 min Scan# 945
Delta R.T. 0.008 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion: 43 Resp: 5137
Ion Ratio Lower Upper
43 100
74 7.3 19.5 29.3#

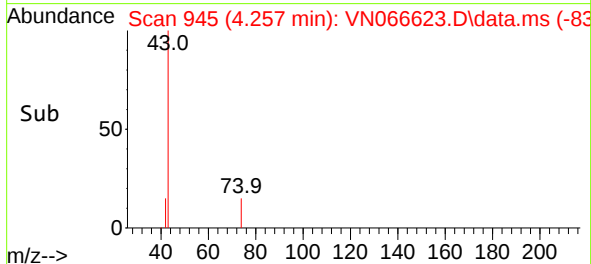

#20
Methylene Chloride
Concen: 4.16 ug/l
RT: 4.466 min Scan# 1023
Delta R.T. -0.001 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53

Tgt Ion: 84 Resp: 14211
Ion Ratio Lower Upper
84 100
49 136.9 94.6 141.8
51 42.2 29.9 44.9
86 67.8 51.4 77.2


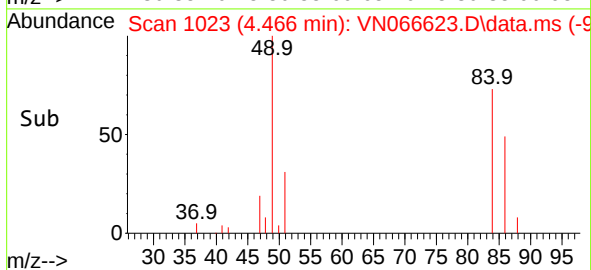

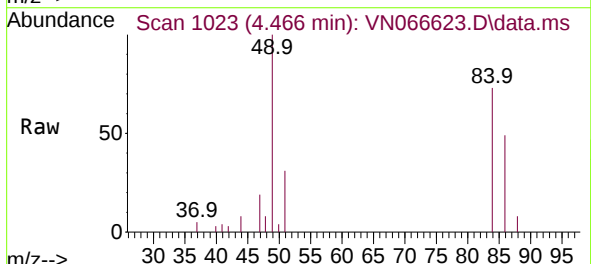


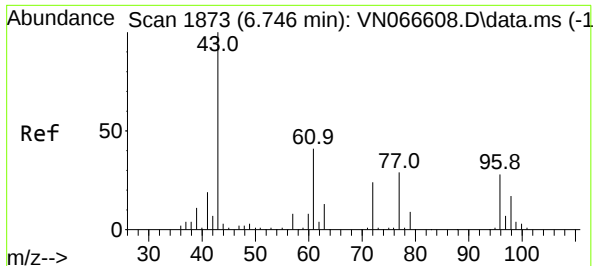

#25
2-Butanone
Concen: 1.03 ug/l
RT: 6.757 min Scan# 1877
Delta R.T. 0.011 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 2189
Ion Ratio Lower Upper
43 100
72 23.2 23.1 34.7

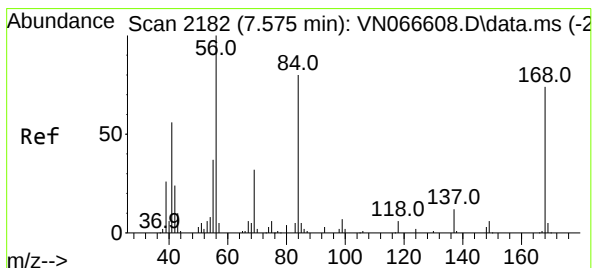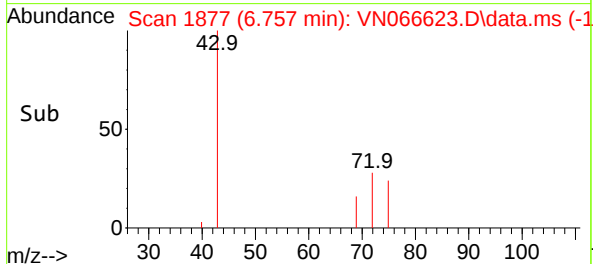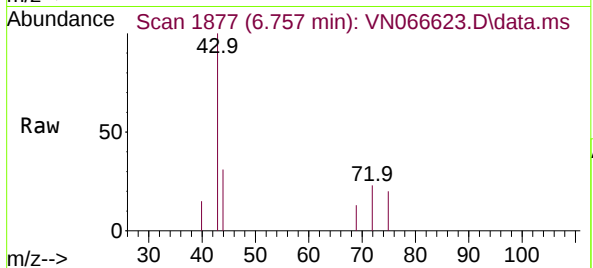

#31
Cyclohexane
Concen: 0.97 ug/l
RT: 7.586 min Scan# 2186
Delta R.T. 0.011 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53

Tgt Ion: 56 Resp: 5062
Ion Ratio Lower Upper
56 100
69 161.6 26.6 39.8#
84 141.9 70.4 105.6#


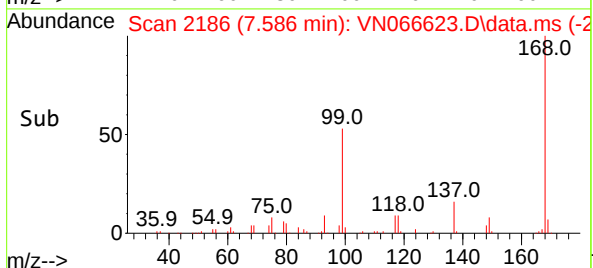

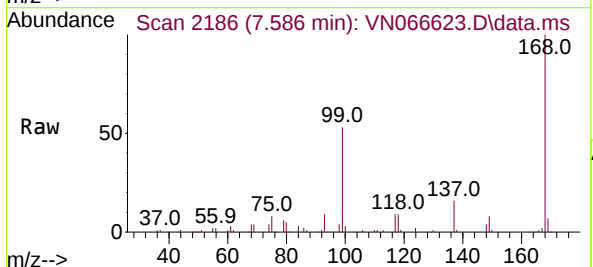




#33
 1,2-Dichloroethane-d4
 Concen: 49.40 ug/l
 RT: 7.950 min Scan# 2322
 Delta R.T. -0.003 min
 Lab File: VN066623.D
 Acq: 15 Apr 2021 19:53




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 65 Resp: 178674
 Ion Ratio Lower Upper
 65 100
 67 54.1 0.0 107.2

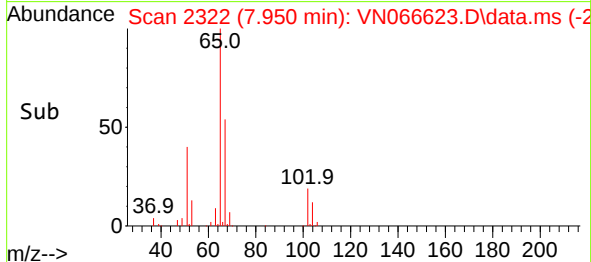

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.516 min Scan# 2533
 Delta R.T. -0.003 min
 Lab File: VN066623.D
 Acq: 15 Apr 2021 19:53

Tgt Ion: 114 Resp: 376469
 Ion Ratio Lower Upper
 114 100
 63 22.4 0.0 38.6
 88 15.7 0.0 30.6

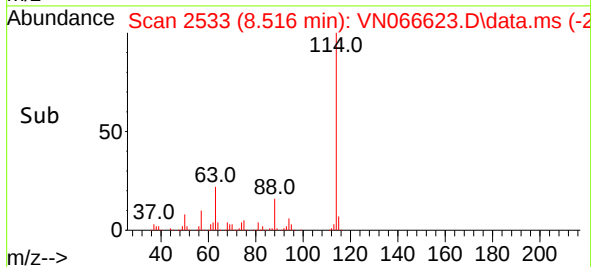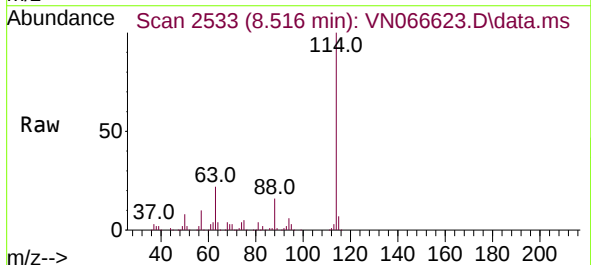

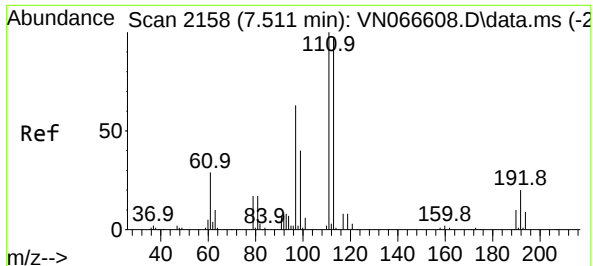

#35

Dibromofluoromethane

Concen: 52.78 ug/l

RT: 7.510 min Scan# 2158

Delta R.T. -0.001 min

Lab File: VN066623.D

Acq: 15 Apr 2021 19:53





Tgt Ion: 113 Resp: 137806

Ion Ratio Lower Upper

113 100

111 102.8 82.2 123.2

192 20.5 15.4 23.0

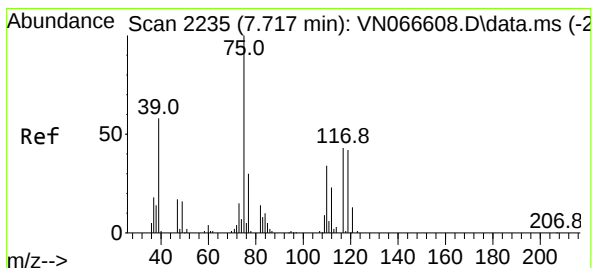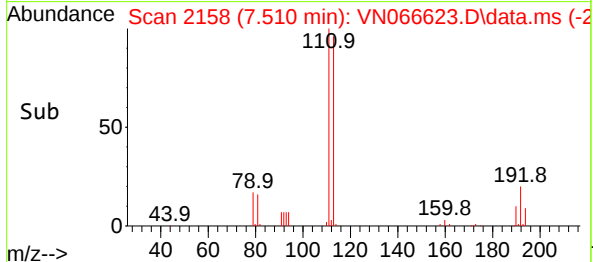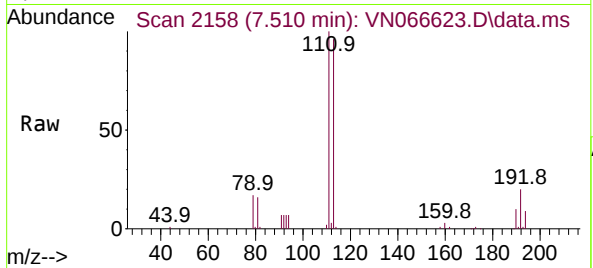

#36

1,1-Dichloropropene

Concen: 4.84 ug/l

RT: 7.588 min Scan# 2187

Delta R.T. -0.129 min

Lab File: VN066623.D

Acq: 15 Apr 2021 19:53




Tgt Ion: 75 Resp: 18359


Ion Ratio Lower Upper

75 100

110 6.5 18.2 54.6#

77 0.0 24.9 37.3#

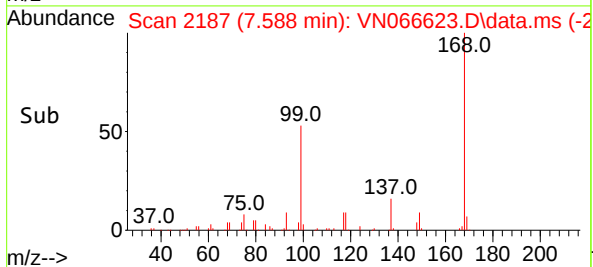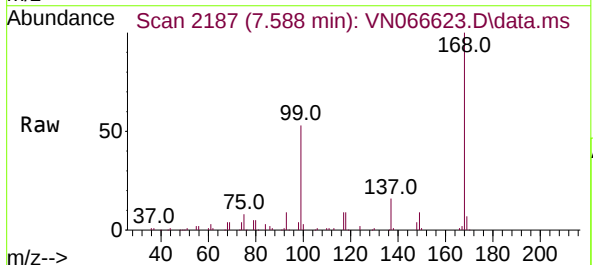

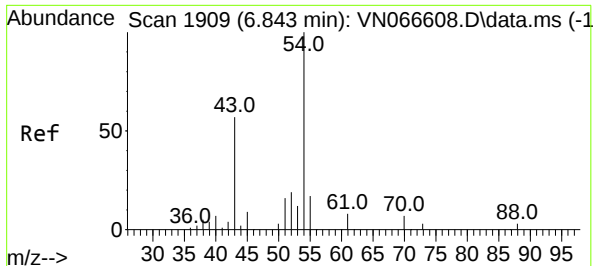

#37

Ethyl Acetate

Concen: 0.51 ug/l

RT: 6.757 min Scan# 1877





Delta R.T. -0.086 min

Lab File: VN066623.D

Acq: 15 Apr 2021 19:53

Tgt Ion:	43	Resp:	2189
Ion	Ratio	Lower	Upper
43	100		
61	0.0	11.6	17.4#
70	0.0	8.6	13.0#

Instrument :
MSVOA_N
ClientSampled :

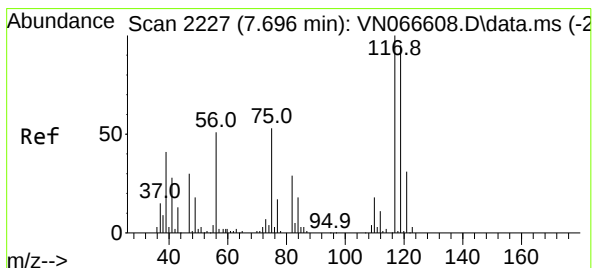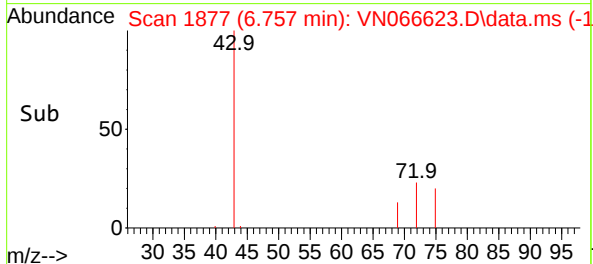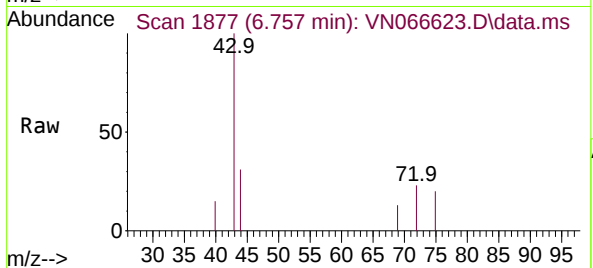

#38

Carbon Tetrachloride

Concen: 6.04 ug/l




RT: 7.586 min Scan# 2186


Delta R.T. -0.110 min

Lab File: VN066623.D

Acq: 15 Apr 2021 19:53

Tgt Ion:	117	Resp:	21486
Ion	Ratio	Lower	Upper
117	100		
119	6.0	76.0	114.0#
121	0.0	24.5	36.7#


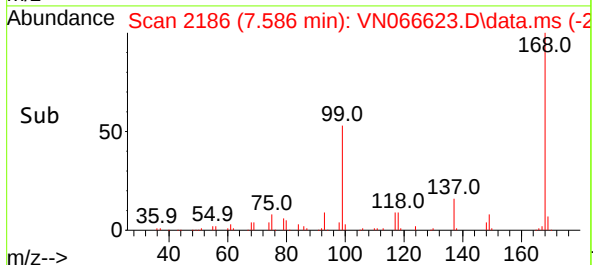
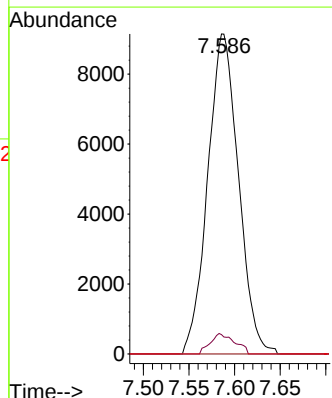
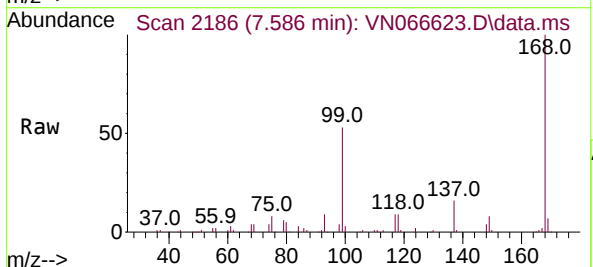




#39
Methylcyclohexane
Concen: 0.26 ug/l
RT: 9.181 min Scan# 2781
Delta R.T. 0.166 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 83 Resp: 1109
Ion Ratio Lower Upper
83 100
55 0.0 58.9 88.3#
98 0.0 35.9 53.9#

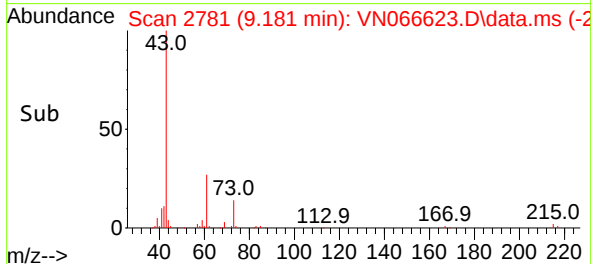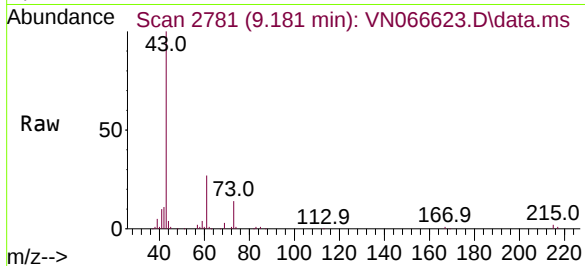

#43
Isopropyl Acetate
Concen: 3.30 ug/l
RT: 8.095 min Scan# 2376
Delta R.T. 0.000 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53

Tgt Ion: 43 Resp: 23694
Ion Ratio Lower Upper
43 100
61 18.7 22.5 33.7#
87 11.2 11.1 16.7

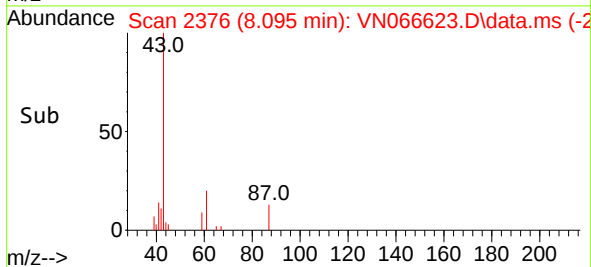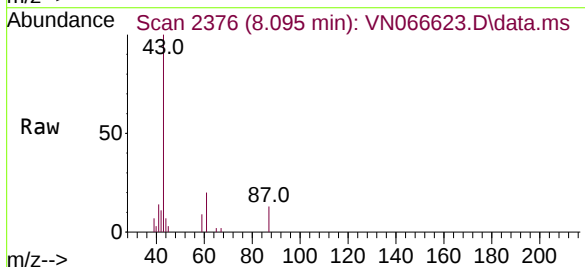



#45

1,2-Dichloropropane

Concen: 0.58 ug/l

RT: 9.200 min Scan# 2788

Delta R.T. 0.147 min

Lab File: VN066623.D

Acq: 15 Apr 2021 19:53

Tgt Ion: 63 Resp: 1966

Ion Ratio Lower Upper





63 100

65 0.0 24.9 37.3#

Instrument :

MSVOA_N

ClientSampled :

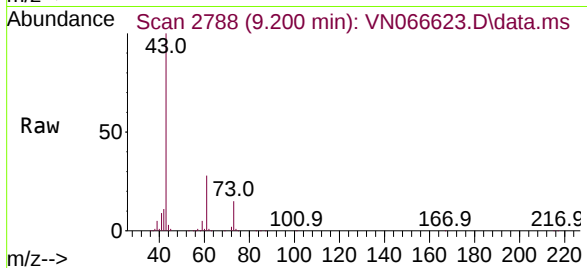

#47

Bromodichloromethane

Concen: 0.27 ug/l

RT: 9.181 min Scan# 2781

Delta R.T. -0.156 min

Lab File: VN066623.D

Acq: 15 Apr 2021 19:53




Tgt Ion: 83 Resp: 1109


Ion Ratio Lower Upper

83 100

85 105.7 51.0 76.4#

127 0.0 7.0 10.6#


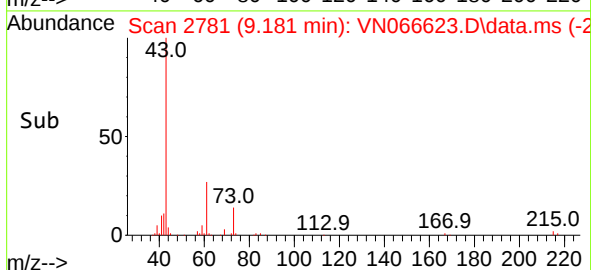

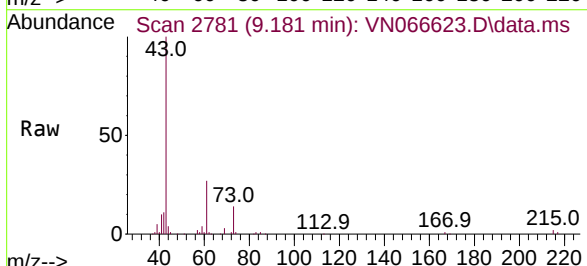


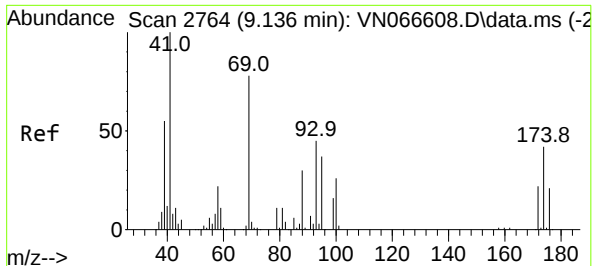

#48
Methyl methacrylate
Concen: 2.09 ug/l
RT: 9.112 min Scan# 2755
Delta R.T. -0.024 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 41 Resp: 6747
Ion Ratio Lower Upper
41 100
69 0.0 75.9 113.9#
39 0.0 46.6 69.8#

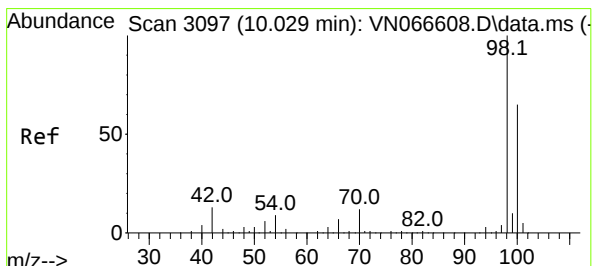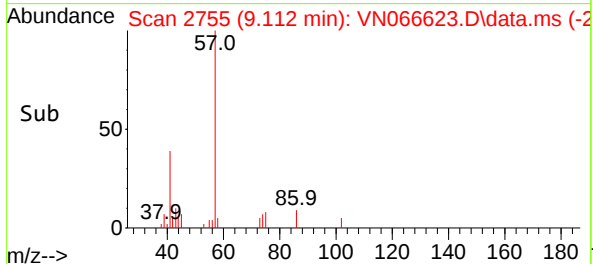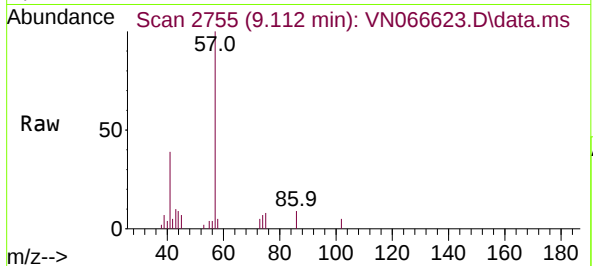

#50
Toluene-d8
Concen: 55.20 ug/l
RT: 10.029 min Scan# 3097
Delta R.T. -0.000 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53

Tgt Ion: 98 Resp: 564806
Ion Ratio Lower Upper
98 100
100 64.4 50.5 75.7


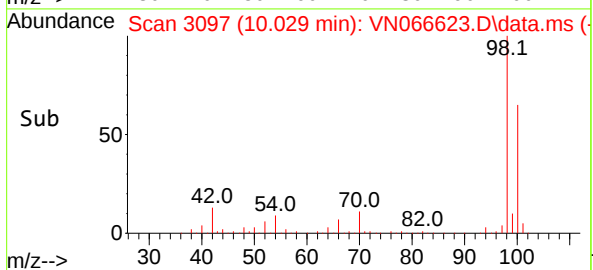

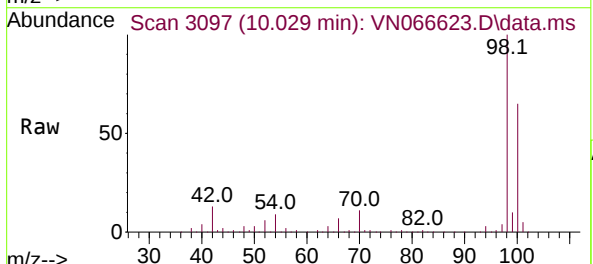




#51
4-Methyl-2-Pentanone
Concen: 1.28 ug/l
RT: 9.924 min Scan# 3058
Delta R.T. 0.002 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 5399
Ion Ratio Lower Upper
43 100
58 33.2 32.5 48.7

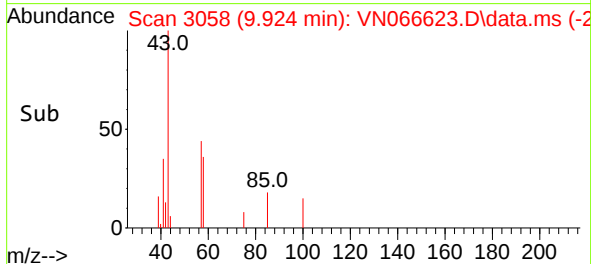

#54
cis-1,3-Dichloropropene
Concen: 7.43 ug/l
RT: 9.844 min Scan# 3028
Delta R.T. 0.067 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53


Tgt Ion: 75 Resp: 36808
Ion Ratio Lower Upper
75 100
77 0.0 24.9 37.3#
39 29.9 36.2 54.4#

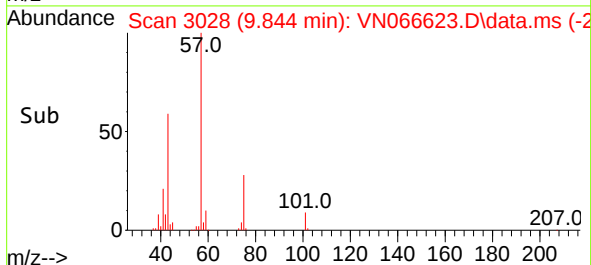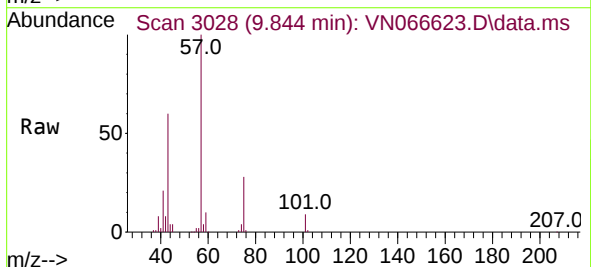



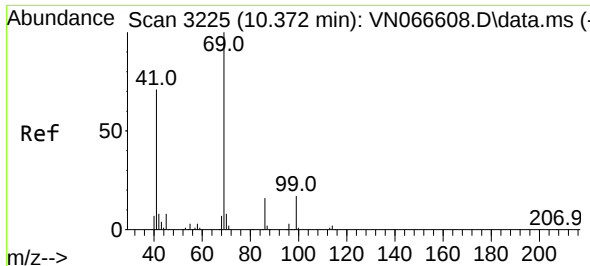


#56
Ethyl methacrylate
Concen: 0.92 ug/l
RT: 10.294 min Scan# 3196
Delta R.T. -0.078 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 69 Resp: 113
Ion Ratio Lower Upper
69 100
41 0.0 49.6 74.4#
39 0.0 28.0 42.0#

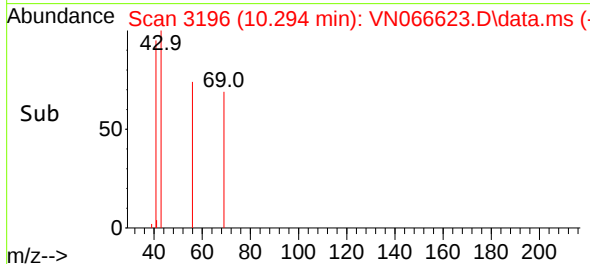

#57
1,3-Dichloropropane
Concen: 4.27 ug/l
RT: 10.705 min Scan# 3349
Delta R.T. 0.059 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53

Tgt Ion: 76 Resp: 21155
Ion Ratio Lower Upper
76 100
78 0.0 25.7 38.5#


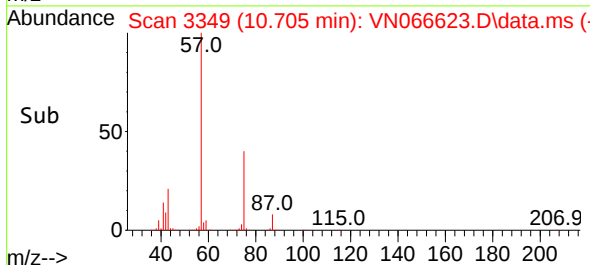
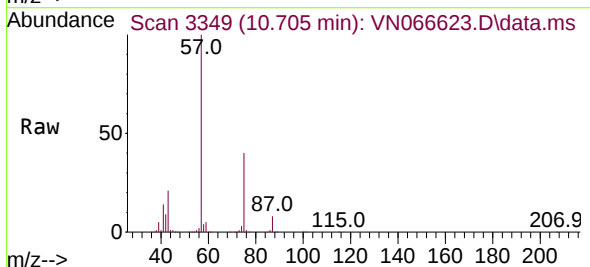



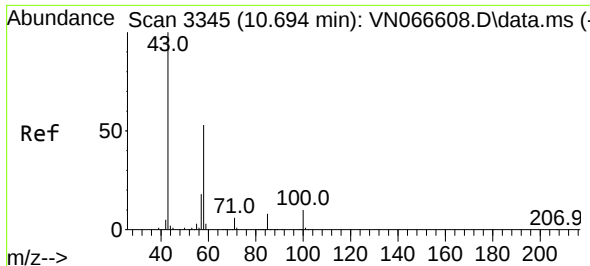

#59
2-Hexanone
Concen: 110.27 ug/l
RT: 10.707 min Scan# 3350
Delta R.T. 0.013 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 323910
Ion Ratio Lower Upper
43 100
58 19.5 28.1 84.3#

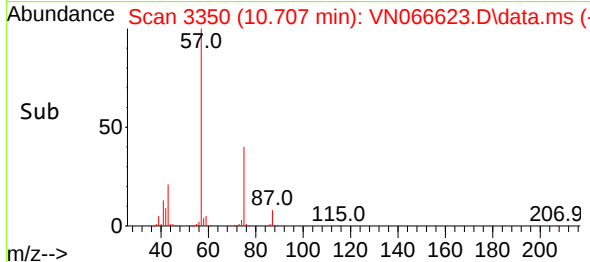

#62
4-Bromofluorobenzene
Concen: 53.51 ug/l
RT: 12.346 min Scan# 3961
Delta R.T. 0.002 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53


Tgt Ion: 95 Resp: 192541
Ion Ratio Lower Upper
95 100
174 83.6 0.0 169.0
176 79.9 0.0 162.4

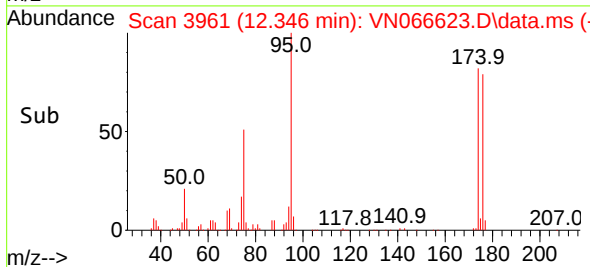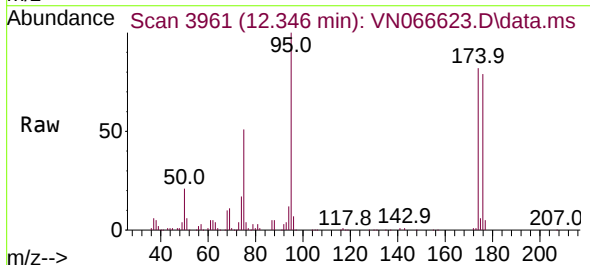



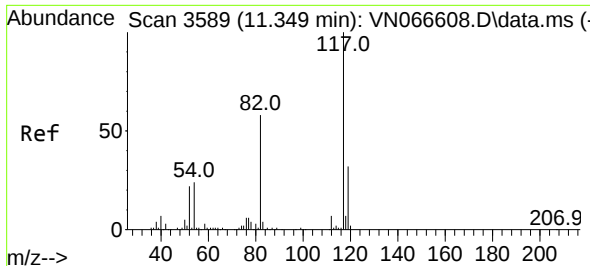


#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.348 min Scan# 3589
Delta R.T. -0.001 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:117 Resp: 377985
Ion Ratio Lower Upper
117 100
82 57.9 43.7 65.5
119 32.0 26.1 39.1

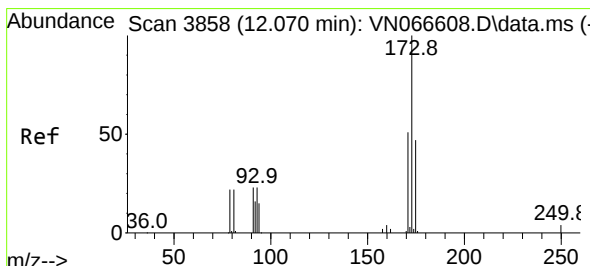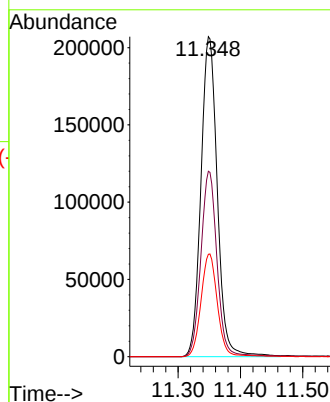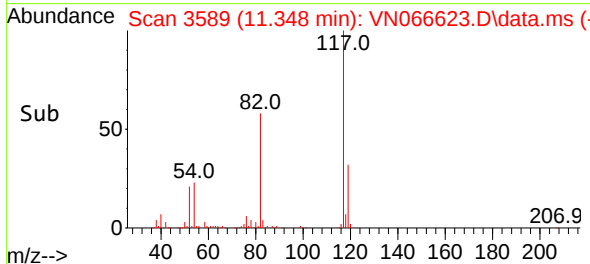


#71
Bromoform
Concen: 0.58 ug/l
RT: 12.346 min Scan# 3961
Delta R.T. 0.276 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53

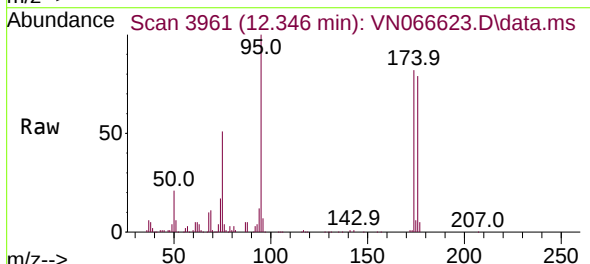

Tgt Ion:173 Resp: 1295
Ion Ratio Lower Upper
173 100
175 682.8 23.8 71.2#
254 0.0 0.0 0.0







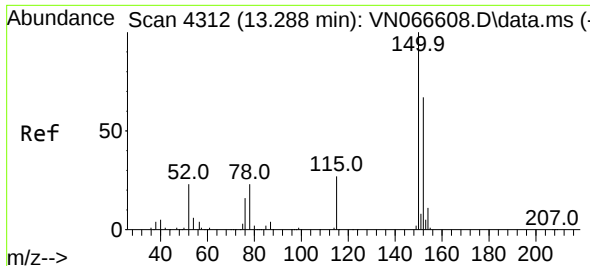

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.290 min Scan# 4313
Delta R.T. 0.002 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:152 Resp: 158545
Ion Ratio Lower Upper
152 100
115 57.3 28.5 85.6
150 157.7 0.0 347.6

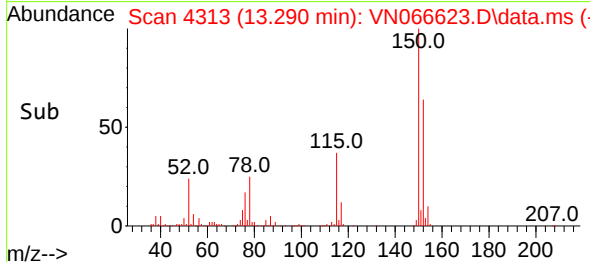

#74
N-ethyl acetate
Concen: 9.74 ug/l
RT: 12.030 min Scan# 3843
Delta R.T. 0.011 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53

Tgt Ion: 43 Resp: 73
Ion Ratio Lower Upper
43 100
70 0.0 34.4 51.6#
55 447.9 20.7 31.1#
61 0.0 19.1 28.7#


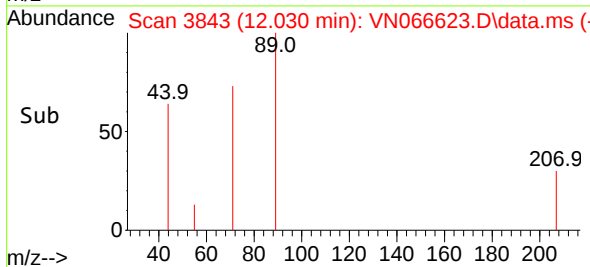
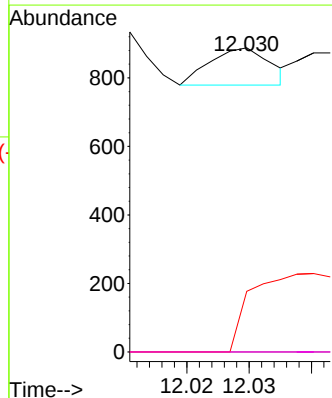
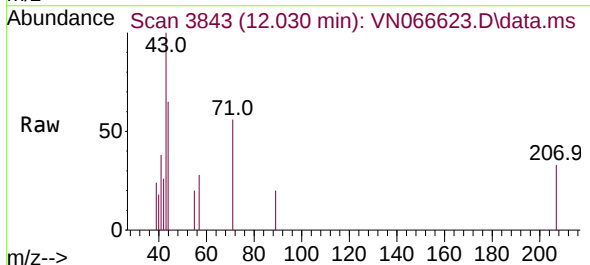


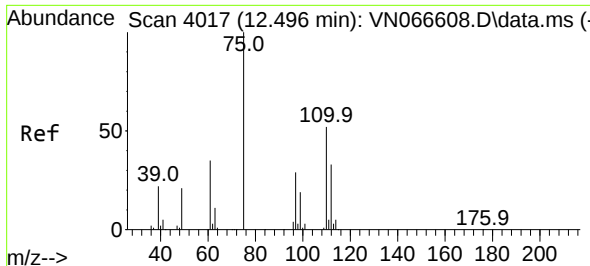

#76
1,2,3-Trichloropropane
Concen: 25.67 ug/l
RT: 12.346 min Scan# 3961
Delta R.T. -0.150 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 95172
Ion Ratio Lower Upper
75 100
77 1.3 0.0 0.0#

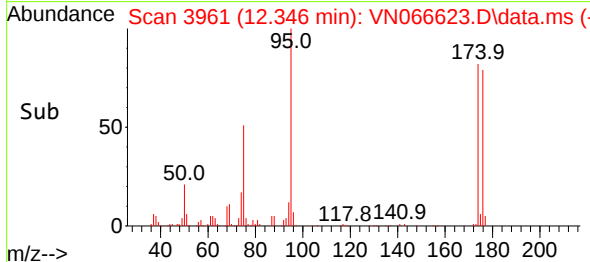

#81
trans-1,4-Dichloro-2-butene
Concen: 79.21 ug/l
RT: 12.346 min Scan# 3961
Delta R.T. 0.102 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53

Tgt Ion: 75 Resp: 95172
Ion Ratio Lower Upper
75 100
53 0.0 74.6 111.8#
89 0.2 35.8 53.8#


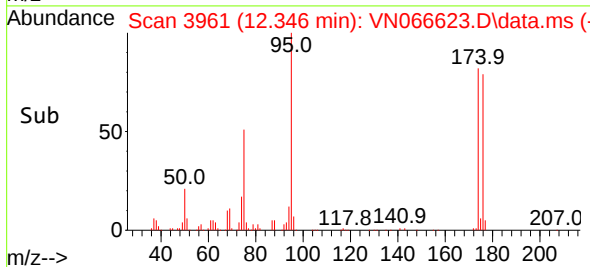

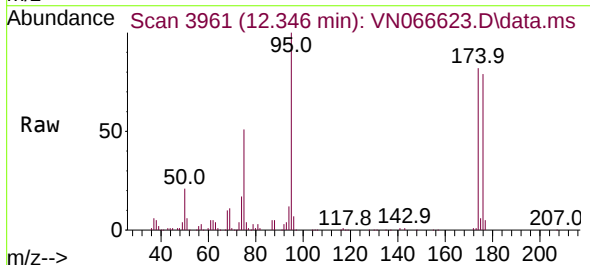




#84
1,2,4-Trimethylbenzene
Concen: 0.30 ug/l
RT: 12.992 min Scan# 4202
Delta R.T. 0.010 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:105 Resp: 2857
Ion Ratio Lower Upper
105 100
120 37.9 22.4 67.0

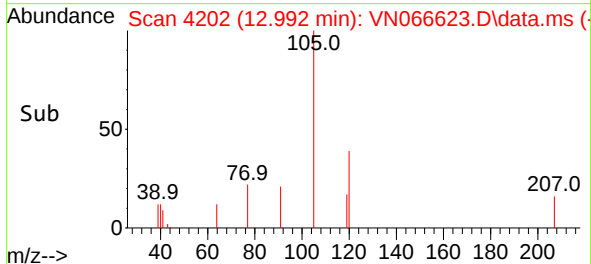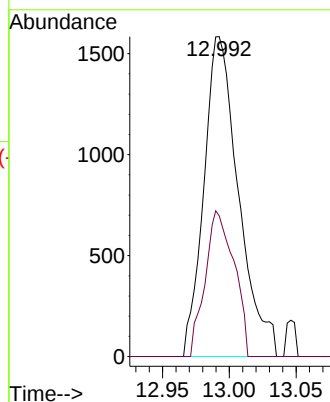

#88
1,4-Dichlorobenzene
Concen: Below Cal
RT: 13.312 min Scan# 4321
Delta R.T. 0.006 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53

Tgt Ion:146 Resp: 52
Ion Ratio Lower Upper
146 100
111 0.0 19.0 57.0#
148 0.0 31.8 95.3#


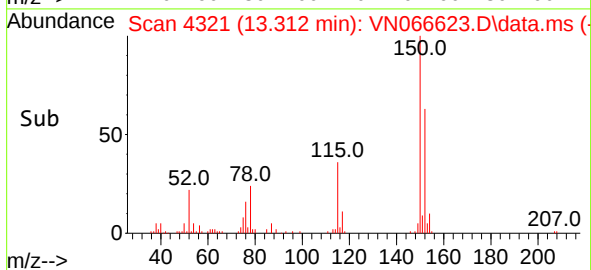
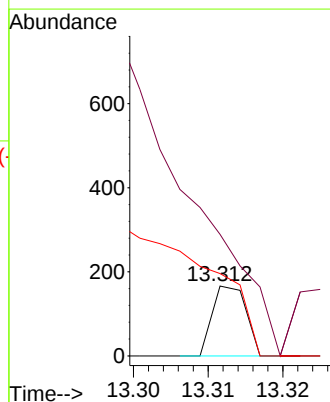
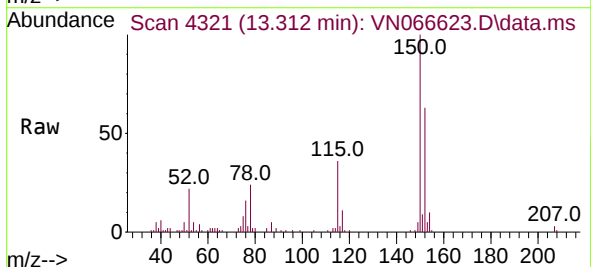




#90
Hexachloroethane
Concen: 0.28 ug/l
RT: 13.843 min Scan# 4519
Delta R.T. 0.030 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion:117 Resp: 584
Ion Ratio Lower Upper
117 100
201 0.0 37.8 113.3#

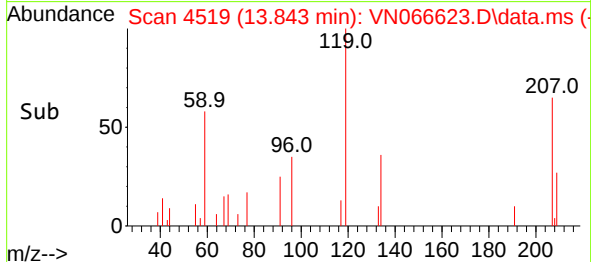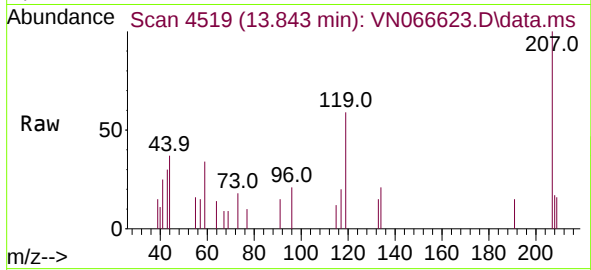

#95
Naphthalene
Concen: 6.27 ug/l
RT: 15.076 min Scan# 4979
Delta R.T. 0.005 min
Lab File: VN066623.D
Acq: 15 Apr 2021 19:53

Tgt Ion:128 Resp: 50754
Ion Ratio Lower Upper
128 100
127 12.1 10.2 15.2
129 10.2 8.6 13.0

