


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041521\
 Data File : VN066602.D
 Acq On : 15 Apr 2021 8:51
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041521W.M
 Title : SW846 8260
 Last Update : Thu Apr 15 19:16:35 2021

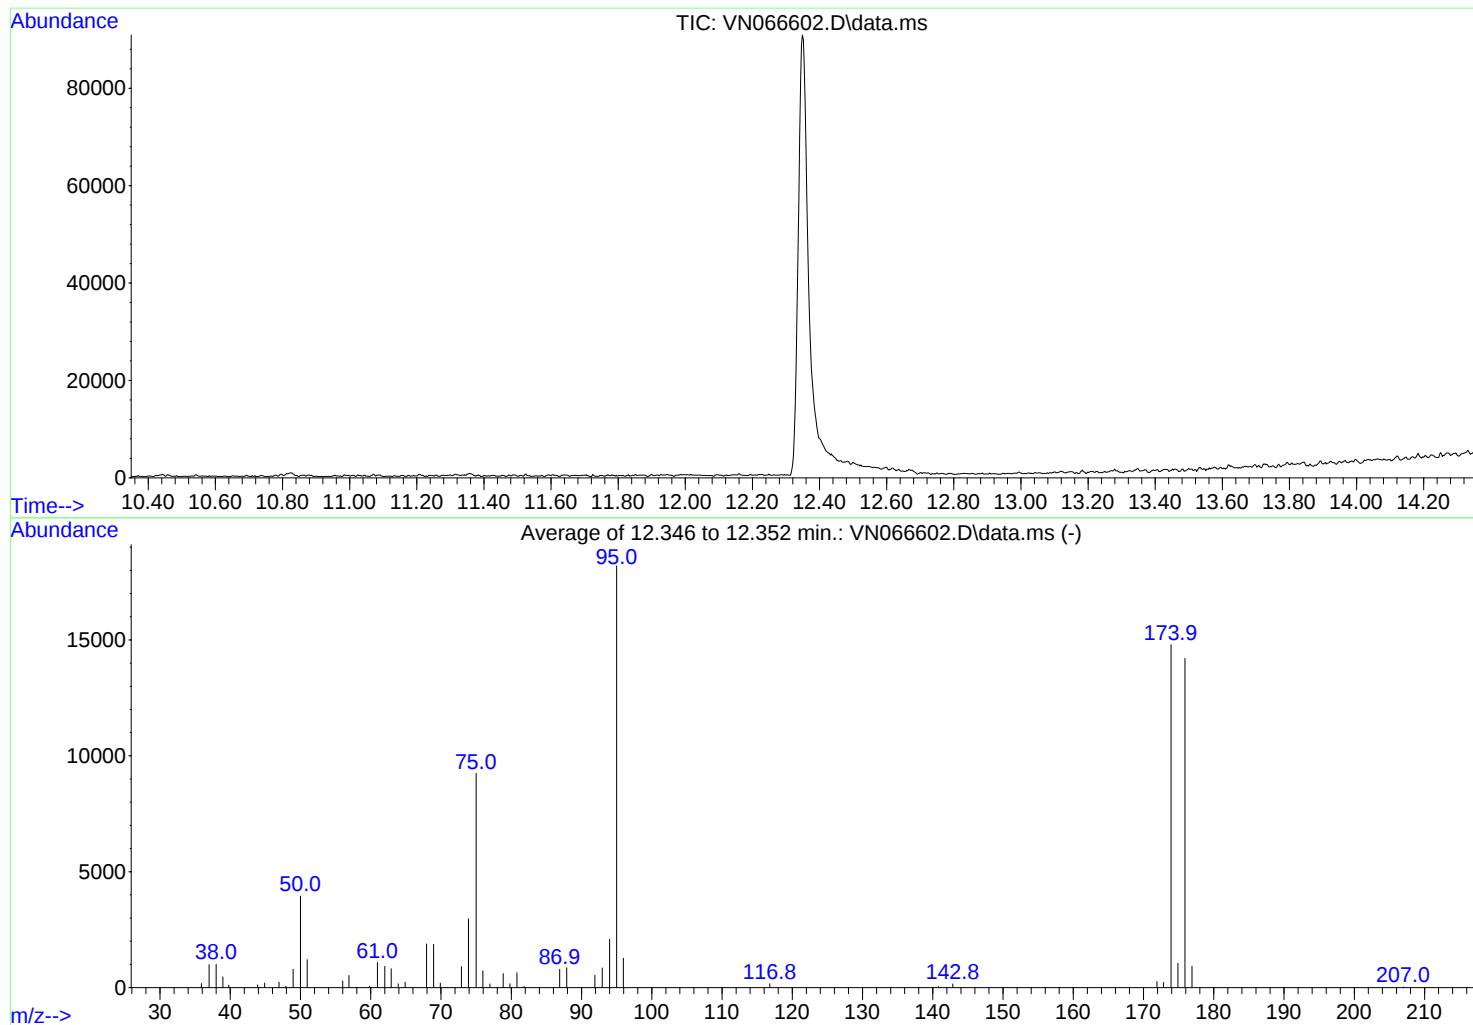

AutoFind: Scans 3961, 3962, 3963; Background Corrected with Scan 3947

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	3948	PASS
75	95	30	60	50.8	9241	PASS
95	95	100	100	100.0	18195	PASS
96	95	5	9	7.0	1269	PASS
173	174	0.00	2	1.5	220	PASS
174	95	50	100	81.3	14796	PASS
175	174	5	9	7.1	1048	PASS
176	174	95	101	96.0	14206	PASS
177	176	5	9	6.5	925	PASS