
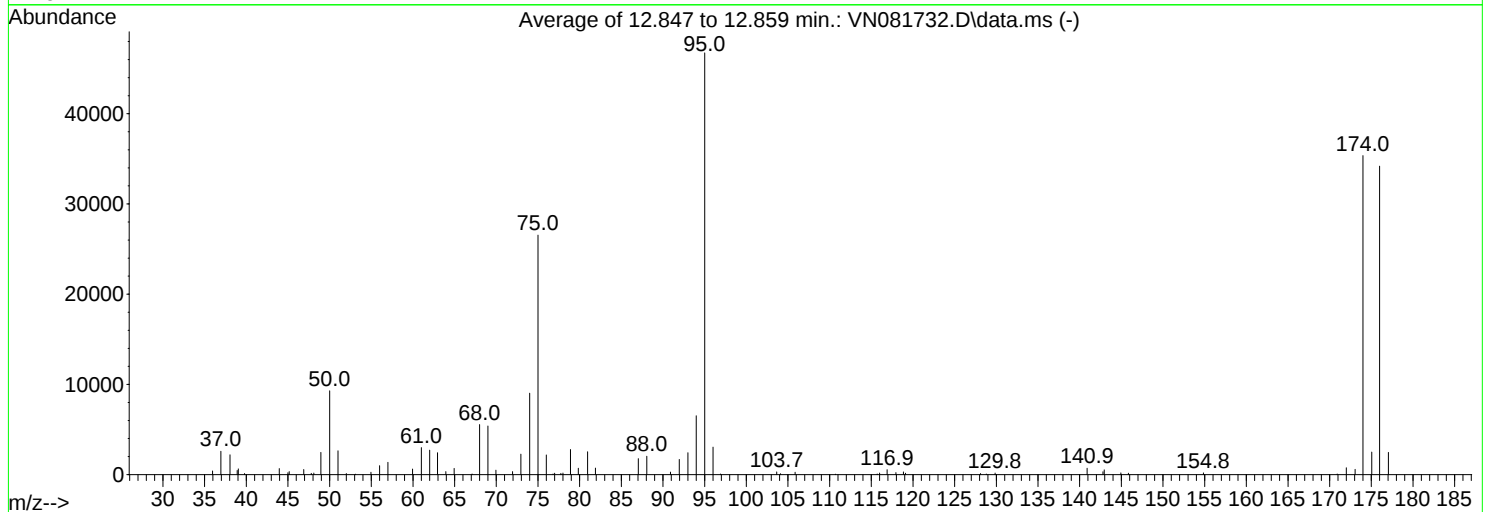


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041524\
Data File : VN081732.D
Acq On : 15 Apr 2024 11:38
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041524W.M
Title : SW846 8260
Last Update : Mon Apr 15 15:37:39 2024

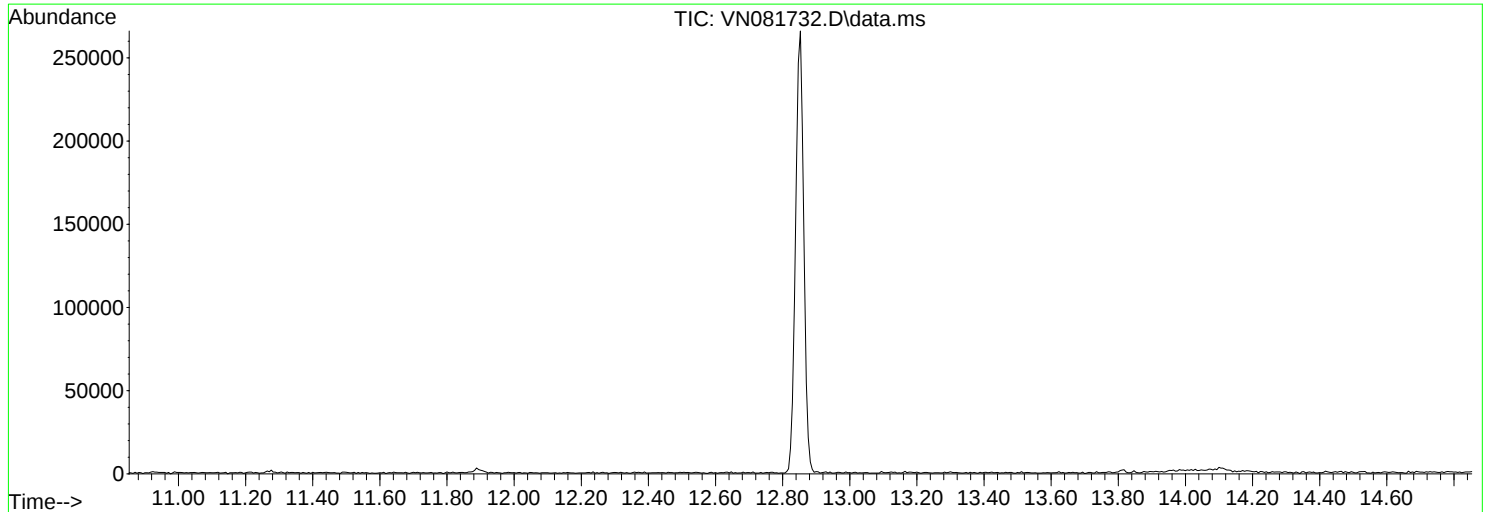

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.9	9288	PASS
75	95	30	60	56.8	26541	PASS
95	95	100	100	100.0	46747	PASS
96	95	5	9	6.5	3047	PASS
173	174	0.00	2	1.7	584	PASS
174	95	50	100	75.6	35352	PASS
175	174	5	9	7.1	2498	PASS
176	174	95	101	96.7	34189	PASS
177	176	5	9	7.2	2460	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	407	48.10	172	62.00	2706	75.00	2654
36.95	2582	48.95	2469	62.95	2435	76.00	2191
38.05	2203	50.00	9288	63.95	330	76.80	8
38.90	462	51.00	2646	64.95	687	77.00	15
39.05	637	52.00	129	67.10	65	77.75	145
39.80	121	53.10	60	68.00	5544	78.00	173
43.95	666	54.95	259	69.00	5398	78.90	2778
45.00	215	56.00	1003	69.95	494	79.85	715
45.15	334	57.00	1365	71.95	344	80.95	2545
46.90	574	59.95	616	72.95	2262	81.90	729
47.80	151	61.00	2997	74.00	9035	87.05	1777

Average of 12.847 to 12.859 min.: VN081732.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
88.05	2044	110.70	60	142.80	314	177.05	2460
90.90	293	115.70	66	142.95	535		
91.95	1682	116.00	185	144.95	204		
93.00	2433	116.90	542	145.85	166		
94.00	6526	117.95	225	154.85	201		
95.00	46747	118.85	297	170.90	70		
96.00	3047	119.10	157	172.00	765		
96.90	69	128.10	119	173.05	584		
103.65	306	128.80	79	174.00	35352		
104.10	104	129.85	173	175.05	2498		
105.85	268	140.90	703	176.00	34189		

Instrument :

MSVOA_N

ClientSampleId :

BFB