


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041525\
Data File : VN086276.D
Acq On : 15 Apr 2025 10:47
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Title : SW846 8260
Last Update : Wed Apr 16 04:19:23 2025

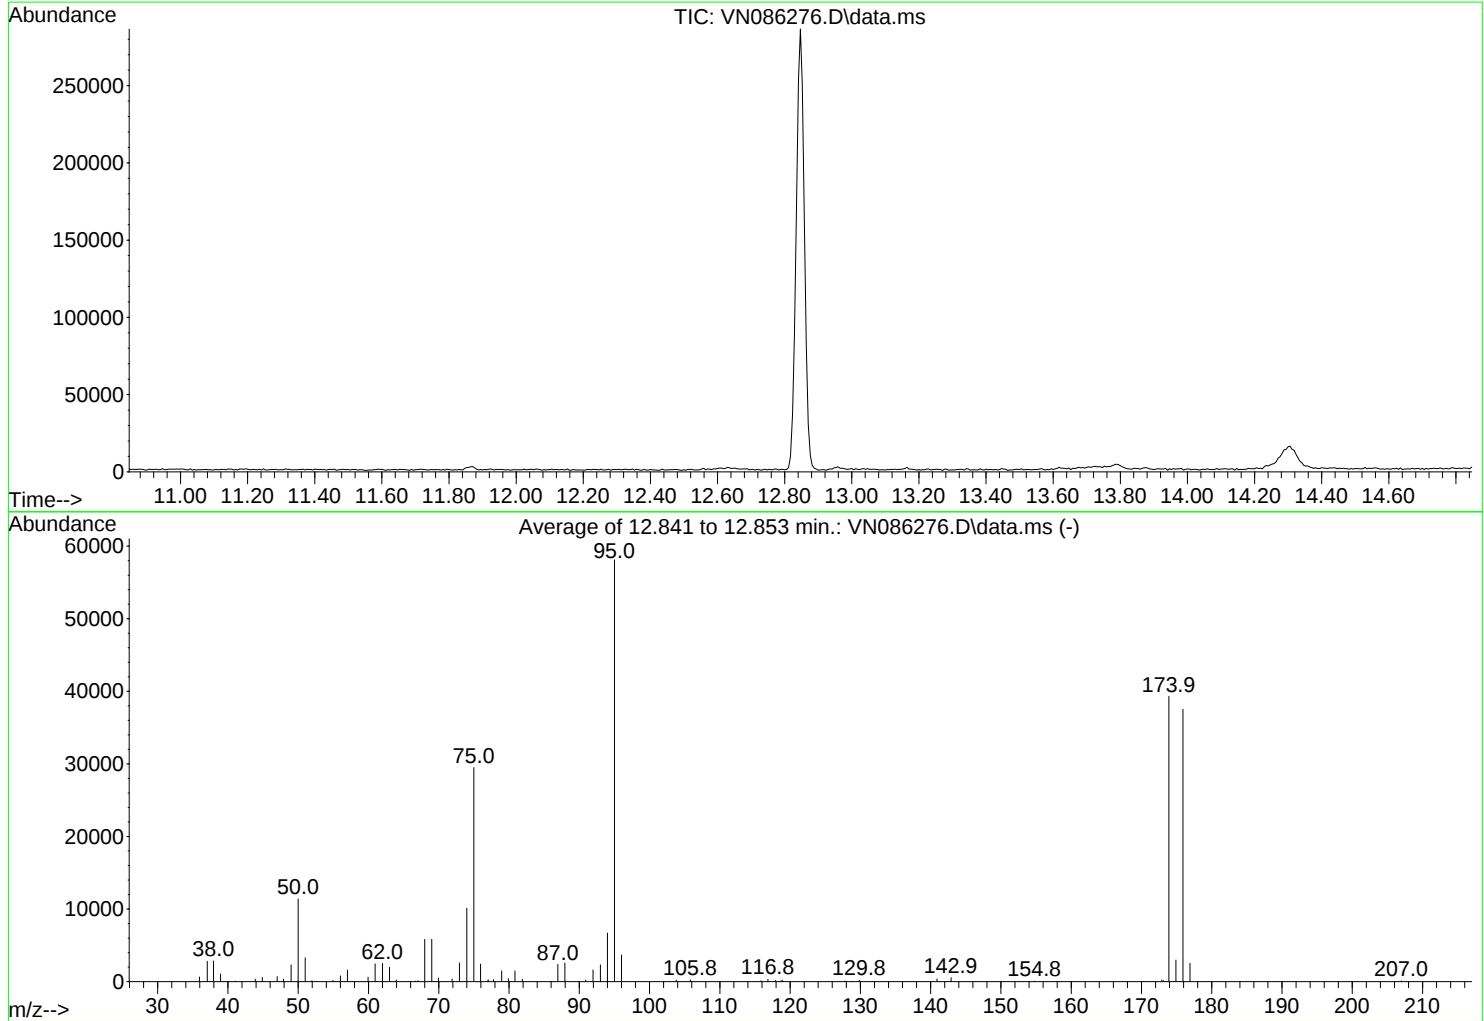

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	11398	PASS
75	95	30	60	50.8	29499	PASS
95	95	100	100	100.0	58112	PASS
96	95	5	9	6.3	3682	PASS
173	174	0.00	2	0.6	240	PASS
174	95	50	100	67.6	39296	PASS
175	174	5	9	7.6	2977	PASS
176	174	95	101	95.5	37528	PASS
177	176	5	9	6.7	2533	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	635	51.00	3286	67.05	140	77.80	271
37.05	2796	51.95	128	68.00	5813	78.95	147
37.95	2853	54.95	179	69.00	5847	79.90	39
38.95	1053	56.00	804	69.95	514	80.85	148
41.10	67	57.00	1592	71.90	363	81.90	335
43.90	345	59.95	619	72.95	2581	85.90	51
44.90	579	60.95	2450	74.00	10128	86.95	2372
47.00	701	62.00	2513	75.00	29499	87.95	2557
47.90	354	63.00	1986	75.95	2430	90.90	233
49.00	2323	63.95	246	76.90	99	91.95	1612
50.00	11398	66.70	59	77.05	268	93.00	2327

Average of 12.841 to 12.853 min.: VN086276.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.00	6693	128.90	53	207.00	112		
95.00	58112	129.85	189				
96.00	3682	140.90	380				
103.80	224	142.90	552				
105.80	239	154.80	75				
115.85	118	172.90	240				
116.85	326	173.10	131				
117.90	152	173.90	39296				
118.70	112	174.90	2977				
118.90	196	175.90	37528				
127.80	80	176.90	2533				

Instrument :

MSVOA_N

ClientSampleId :

BFB