


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041619\
 Data File : VN055067.D
 Acq On : 16 Apr 2019 9:08
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N041119W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Apr 12 07:55:25 2019

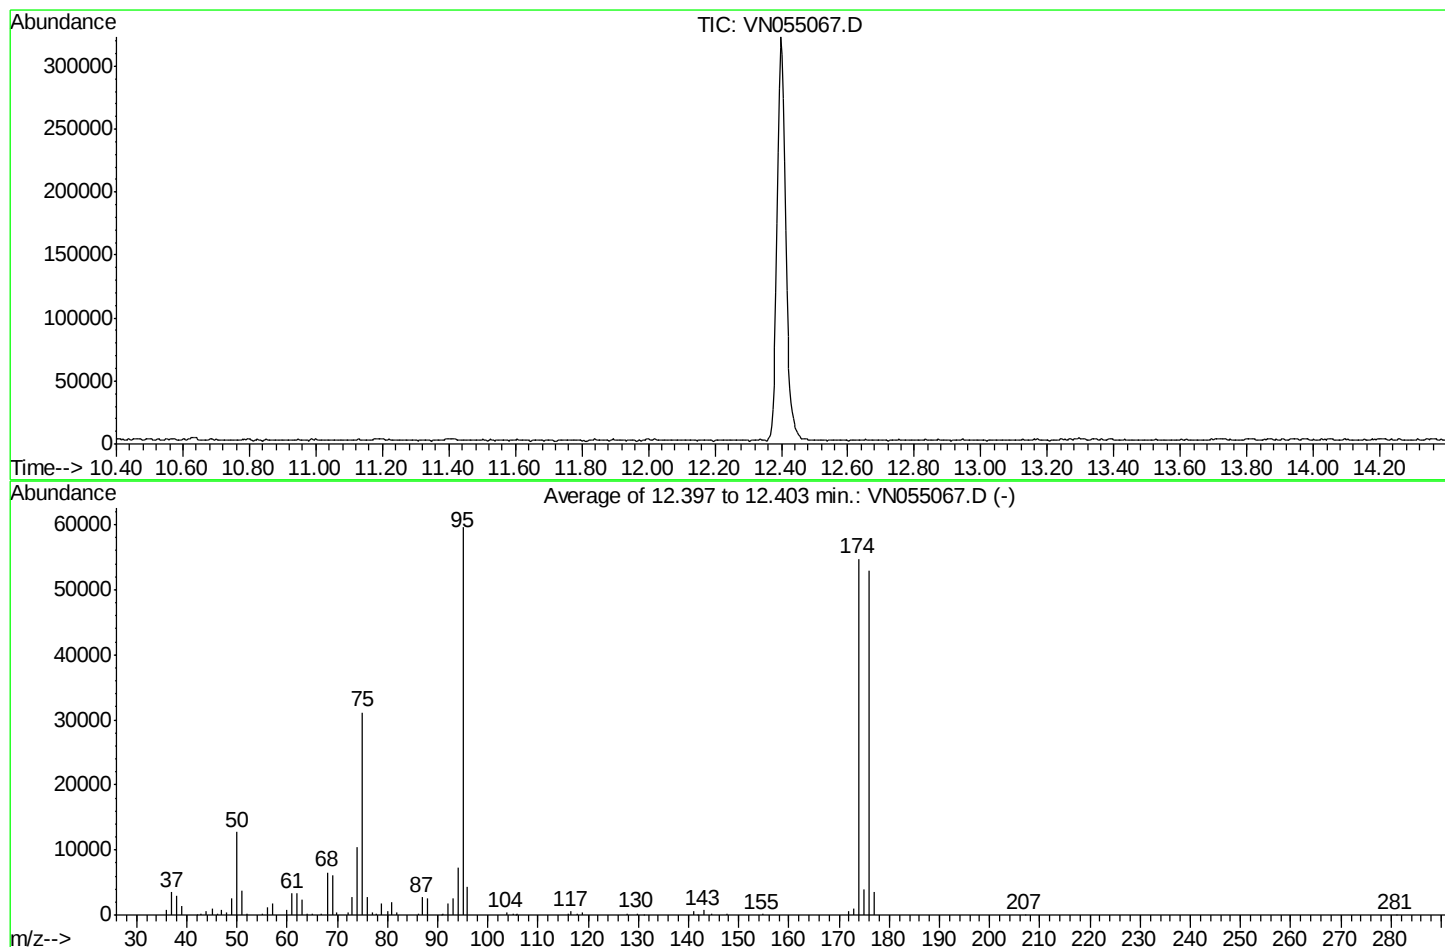

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	12731	PASS
75	95	30	60	52.3	31170	PASS
95	95	100	100	100.0	59586	PASS
96	95	5	9	7.2	4313	PASS
173	174	0.00	2	1.8	965	PASS
174	95	50	100	91.9	54744	PASS
175	174	5	9	7.1	3884	PASS
176	174	95	101	96.8	52978	PASS
177	176	5	9	6.5	3454	PASS