


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN041620\
 Data File : VN061002.D
 Acq On : 16 Apr 2020 10:37
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N041620W.M
 Title : SW846 8260
 Last Update : Fri Apr 17 03:49:39 2020

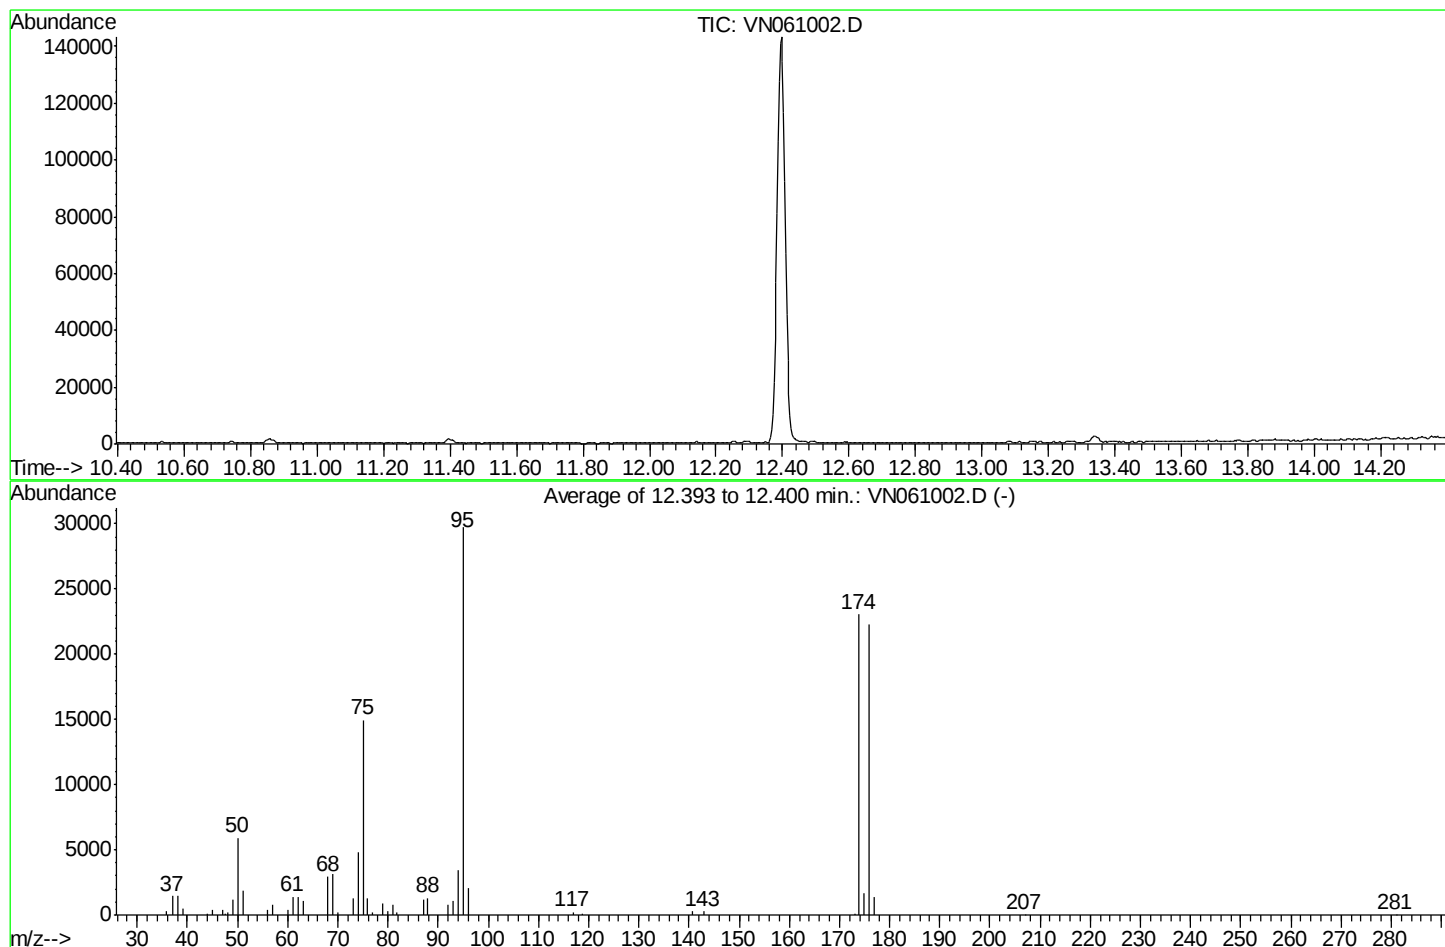

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	5909	PASS
75	95	30	60	50.3	14958	PASS
95	95	100	100	100.0	29725	PASS
96	95	5	9	6.8	2032	PASS
173	174	0.00	2	0.5	105	PASS
174	95	50	100	77.6	23056	PASS
175	174	5	9	7.4	1704	PASS
176	174	95	101	96.5	22245	PASS
177	176	5	9	6.1	1349	PASS