


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN041620\
Data File : VN061010.D
Acq On : 16 Apr 2020 14:29
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N041620W.M
Title : SW846 8260
Last Update : Fri Apr 17 03:49:39 2020

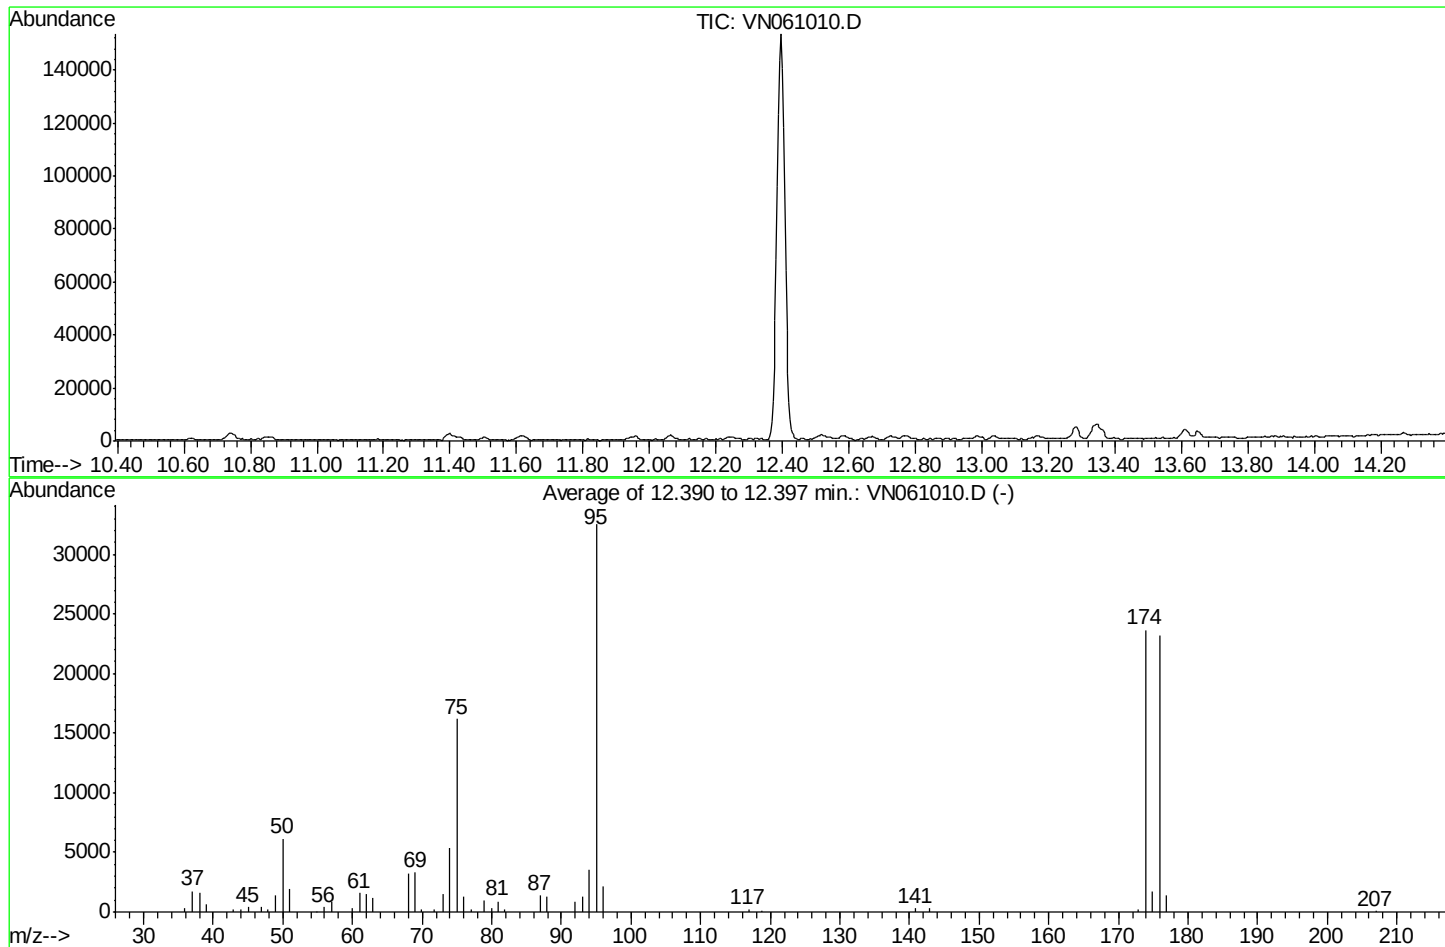

AutoFind: Scans 3302, 3303, 3304; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	6152	PASS
75	95	30	60	49.8	16190	PASS
95	95	100	100	100.0	32517	PASS
96	95	5	9	6.7	2167	PASS
173	174	0.00	2	1.1	265	PASS
174	95	50	100	72.7	23650	PASS
175	174	5	9	7.2	1701	PASS
176	174	95	101	98.2	23216	PASS
177	176	5	9	6.1	1426	PASS