
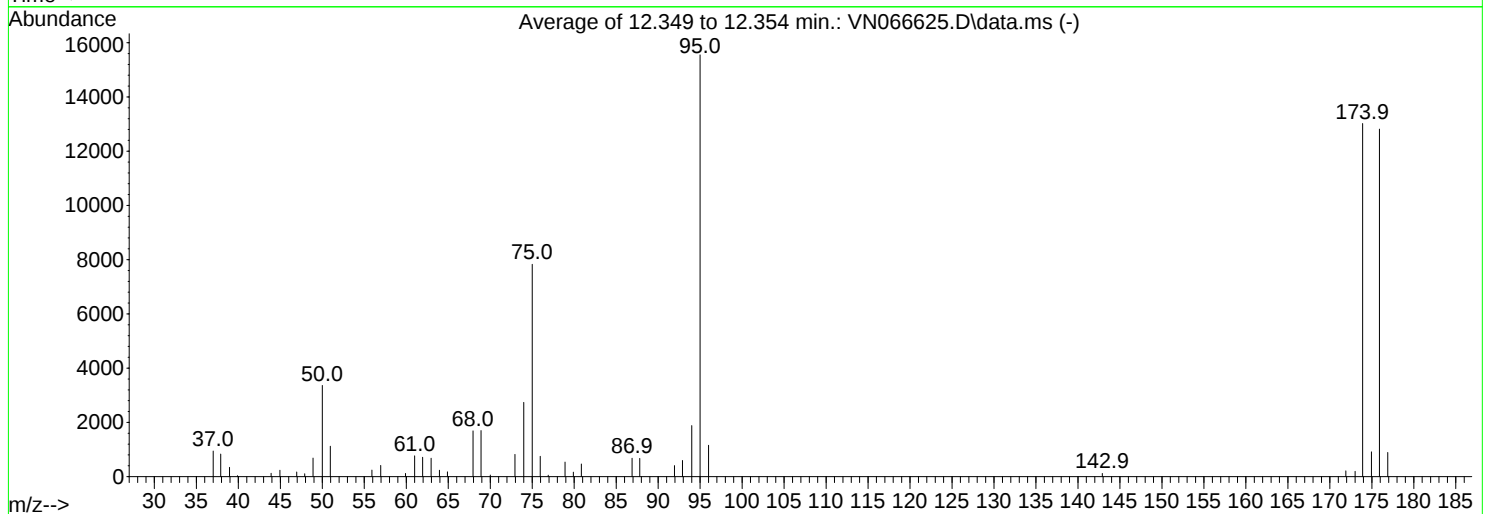


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041621\
Data File : VN066625.D
Acq On : 16 Apr 2021 13:54
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041521W.M
Title : SW846 8260
Last Update : Thu Apr 15 19:16:35 2021

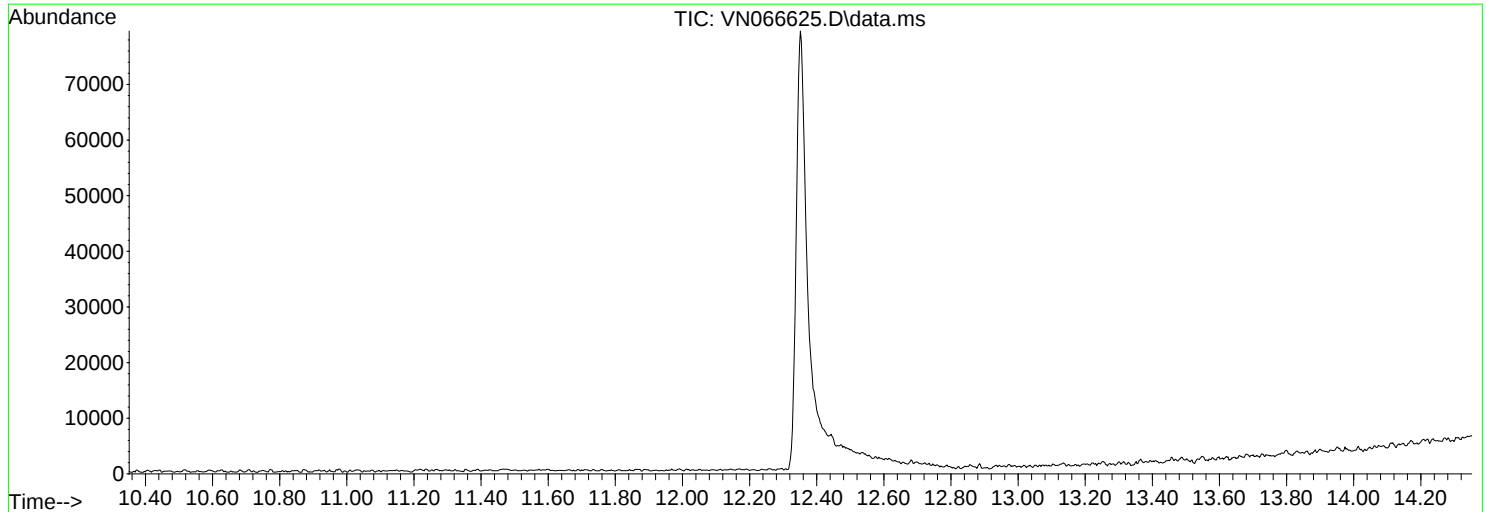

AutoFind: Scans 3962, 3963, 3964; Background Corrected with Scan 3947

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	3362	PASS
75	95	30	60	50.3	7830	PASS
95	95	100	100	100.0	15552	PASS
96	95	5	9	7.4	1156	PASS
173	174	0.00	2	1.5	192	PASS
174	95	50	100	83.7	13018	PASS
175	174	5	9	7.0	914	PASS
176	174	95	101	98.4	12815	PASS
177	176	5	9	6.9	890	PASS