

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041624\
 Data File : VN081761.D
 Acq On : 16 Apr 2024 16:03
 Operator : JC\MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Apr 17 03:27:18 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041524W.M
 Quant Title : SW846 8260
 QLast Update : Mon Apr 15 15:37:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.229	168	241235	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	444448	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	389448	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	161456	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	171745	50.594	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 101.180%	
35) Dibromofluoromethane	8.171	113	142067	48.406	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 96.820%	
50) Toluene-d8	10.565	98	530376	49.054	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 98.100%	
62) 4-Bromofluorobenzene	12.853	95	171259	46.352	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	= 92.700%	
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	2.118	85	677	0.222	ug/l #	43
3) Chloromethane	2.359	50	578	Below Cal		92
5) Bromomethane	2.971	94	2498	1.106	ug/l #	31
6) Chloroethane	3.112	64	197	Below Cal	#	44
9) 1,1,2-Trichlorotrifluo...	4.377	101	2487	0.822	ug/l	88
10) Methyl Iodide	4.589	142	487	0.300	ug/l #	40
13) Acrolein	4.165	56	104	0.211	ug/l #	15
15) Acrylonitrile	5.730	53	661	0.517	ug/l #	57
16) Acetone	4.424	43	936	0.991	ug/l	97
17) Carbon Disulfide	4.706	76	4999	0.600	ug/l	98
20) Methylene Chloride	5.277	84	726	Below Cal	#	22
21) trans-1,2-Dichloroethene	5.800	96	861	0.299	ug/l #	27
31) Cyclohexane	8.224	56	6455	1.386	ug/l #	32
36) 1,1-Dichloropropene	8.224	75	22233	5.437	ug/l #	48
38) Carbon Tetrachloride	8.224	117	26881	5.650	ug/l #	18
43) Isopropyl Acetate	8.677	43	11872	1.894	ug/l #	54
44) Trichloroethene	9.353	130	38391	11.590	ug/l	95
49) 1,4-Dioxane	9.700	88	74	1.155	ug/l #	28
59) 2-Hexanone	11.200	43	529	0.210	ug/l #	23
64) Tetrachloroethene	11.100	164	2032	0.615	ug/l #	72
68) m/p-Xylenes	12.082	106	1239	0.226	ug/l	100
76) 1,2,3-Trichloropropane	12.853	75	95905	31.232	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	95905	72.681	ug/l #	12
82) 4-Chlorotoluene	13.223	91	2065	0.239	ug/l	81
87) 1,3-Dichlorobenzene	13.729	146	2033	0.352	ug/l	87
88) 1,4-Dichlorobenzene	13.729	146	2033	0.346	ug/l	90
89) n-Butylbenzene	14.064	91	2047	0.236	ug/l	86
93) 1,2,4-Trichlorobenzene	15.400	180	1883	0.640	ug/l	97
94) Hexachlorobutadiene	15.506	225	1296	1.022	ug/l	84
95) Naphthalene	15.647	128	5996	0.638	ug/l #	87
96) 1,2,3-Trichlorobenzene	15.853	180	2509	0.834	ug/l	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041624\
Data File : VN081761.D
Acq On : 16 Apr 2024 16:03
Operator : JC\MD
Sample : IBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Apr 17 03:27:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041524W.M
Quant Title : SW846 8260
QLast Update : Mon Apr 15 15:37:39 2024
Response via : Initial Calibration

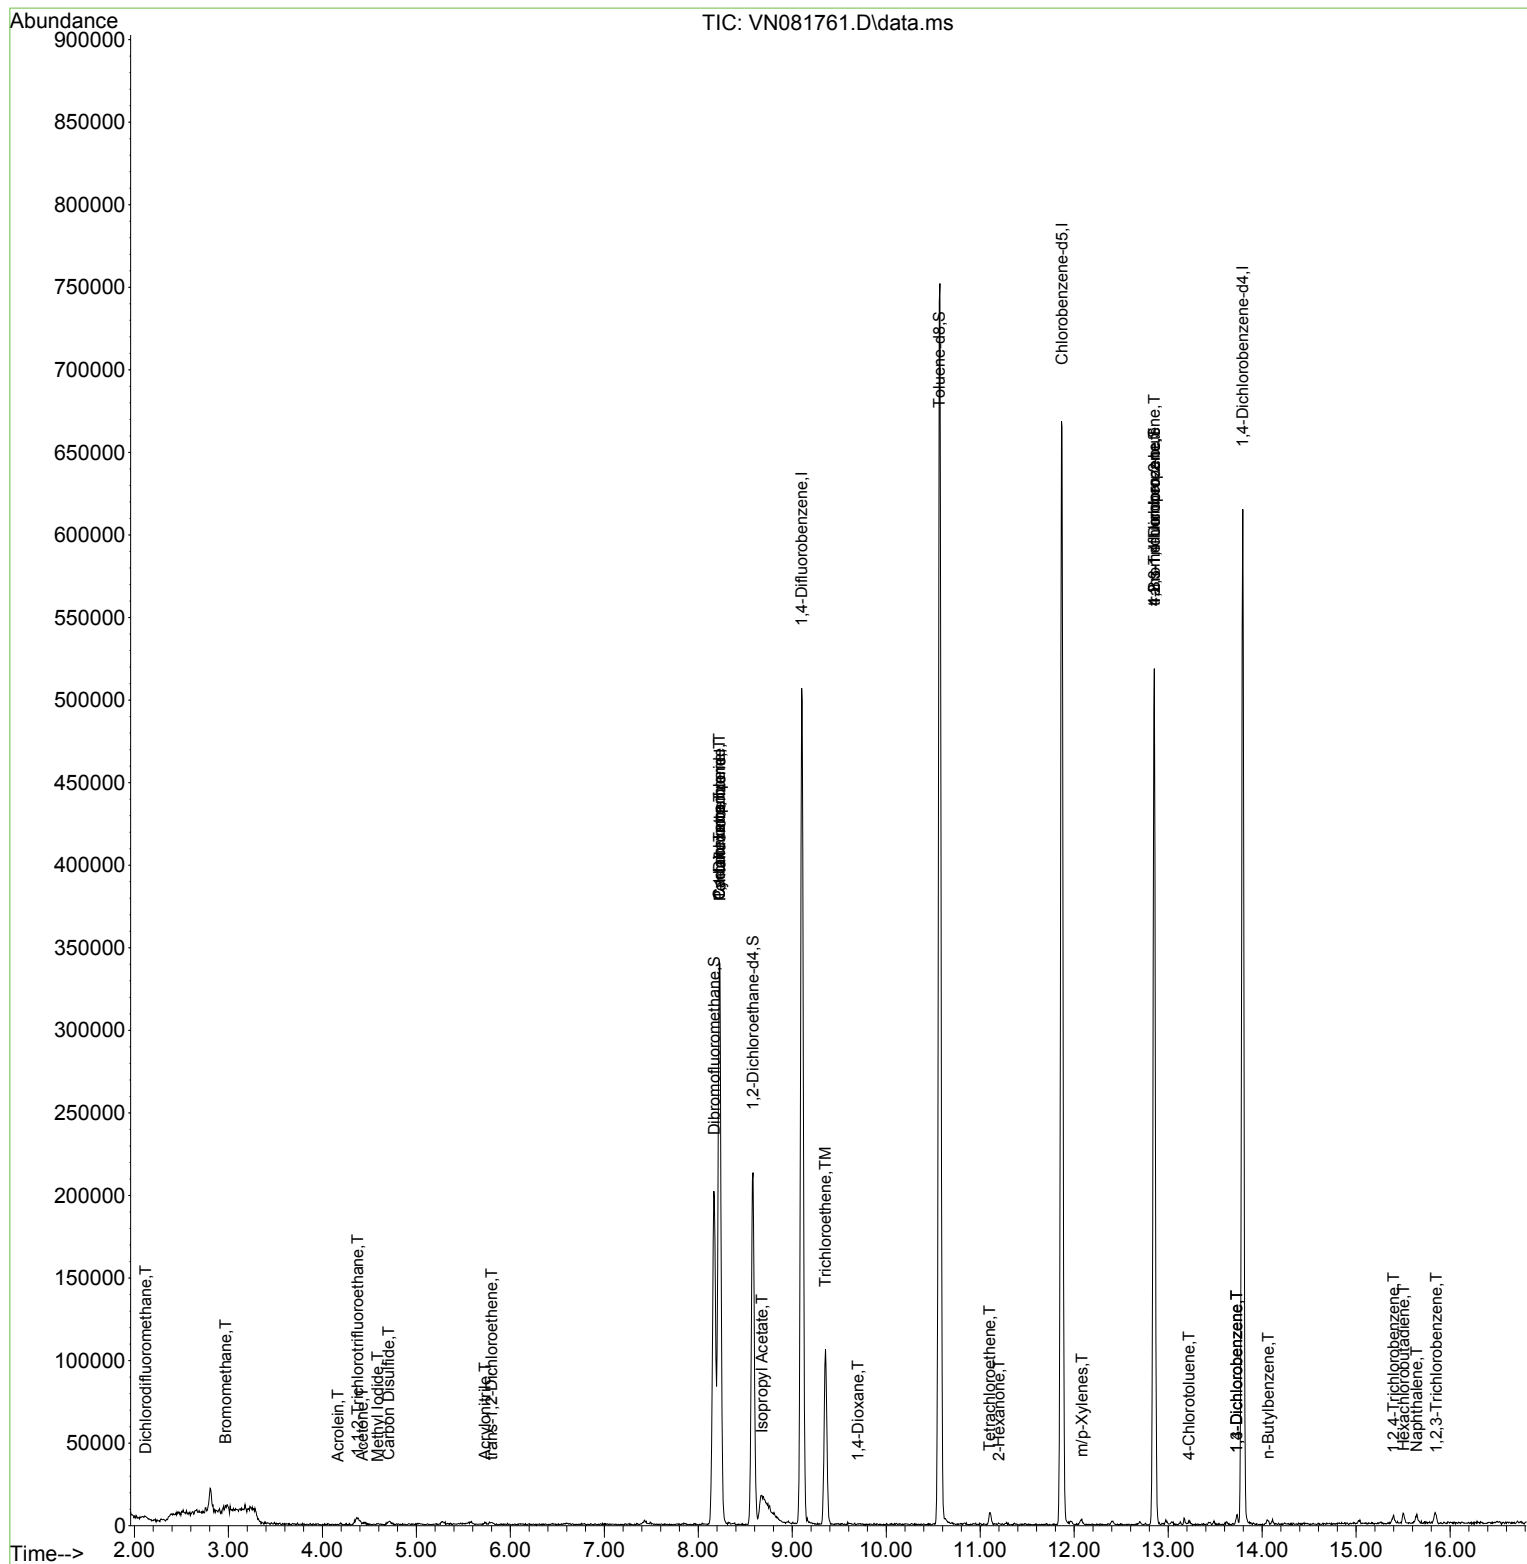






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.229 min Scan# 10
Delta R.T. 0.005 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:168 Resp: 241235
Ion Ratio Lower Upper
168 100
99 65.7 48.2 72.4



#2
Dichlorodifluoromethane
Concen: 0.222 ug/l
RT: 2.118 min Scan# 28
Delta R.T. -0.006 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03

Tgt Ion: 85 Resp: 677
Ion Ratio Lower Upper
85 100
87 0.0 15.8 47.4#







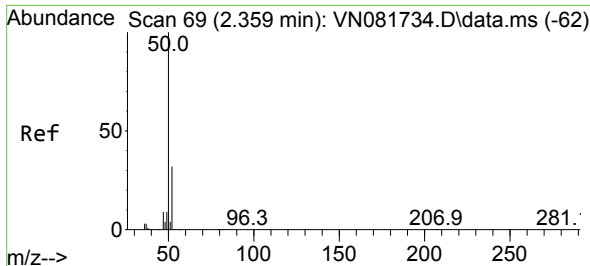

#3
Chloromethane
Concen: Below Cal
RT: 2.359 min Scan# 69
Delta R.T. 0.000 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 50 Resp: 578
Ion Ratio Lower Upper
50 100
52 27.7 25.5 38.3

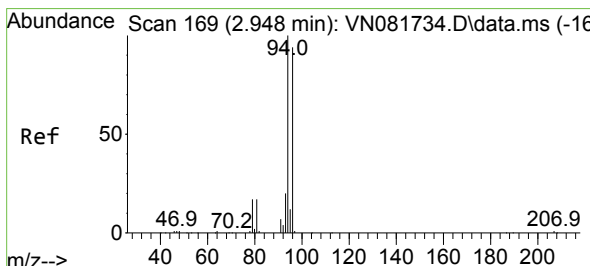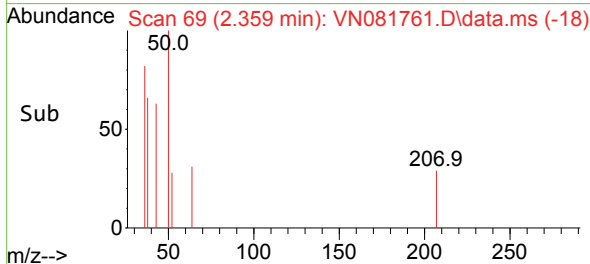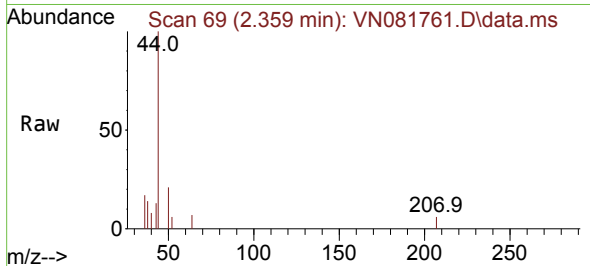

#5
Bromomethane
Concen: 1.106 ug/l
RT: 2.971 min Scan# 173
Delta R.T. 0.023 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03

Tgt Ion: 94 Resp: 2498
Ion Ratio Lower Upper
94 100
96 159.8 74.8 112.2#


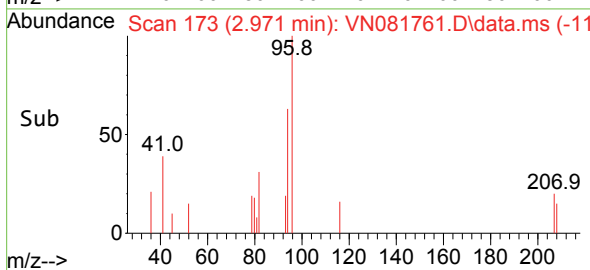

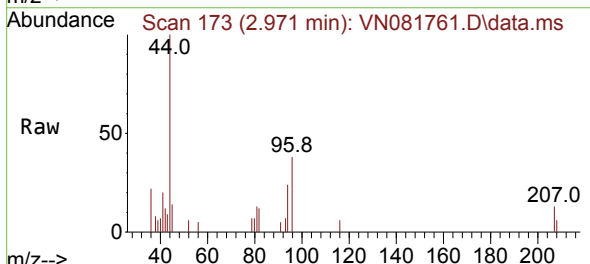


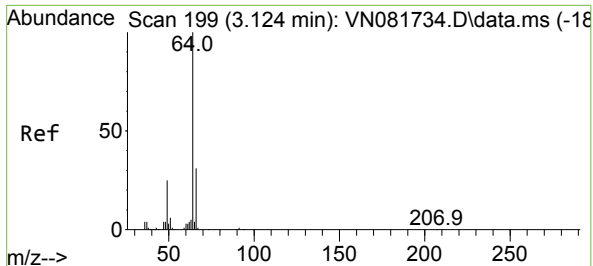

#6
Chloroethane
Concen: Below Cal
RT: 3.112 min Scan# 197
Delta R.T. -0.012 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 64 Resp: 197
Ion Ratio Lower Upper
64 100
66 0.0 24.7 37.1#

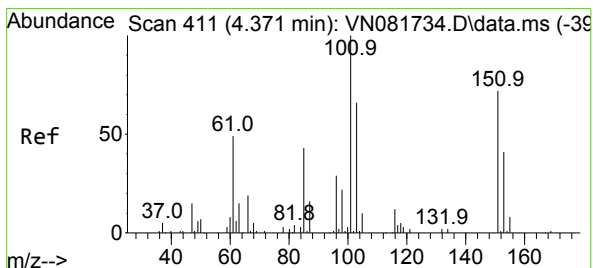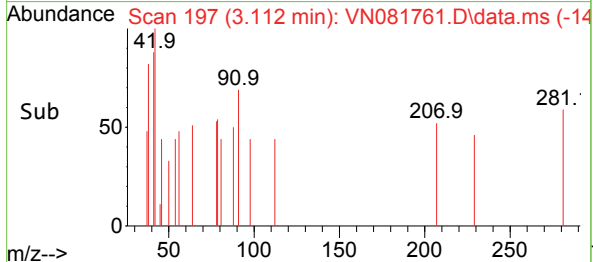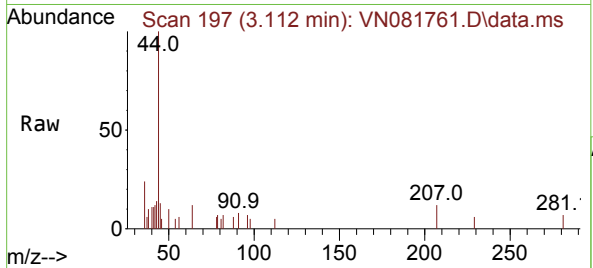

#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.822 ug/l
RT: 4.377 min Scan# 412
Delta R.T. 0.006 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03


Tgt Ion: 101 Resp: 2487
Ion Ratio Lower Upper
101 100
85 39.0 37.3 55.9
151 63.4 59.2 88.8

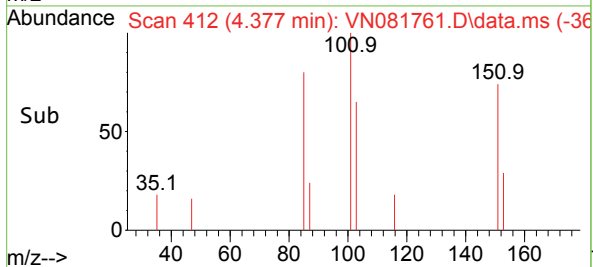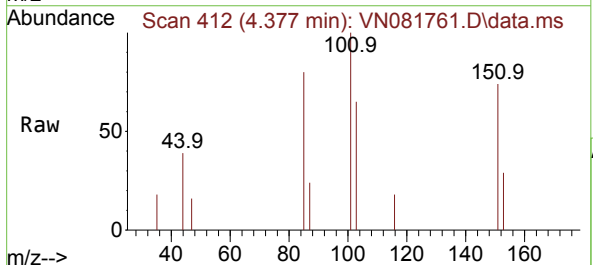



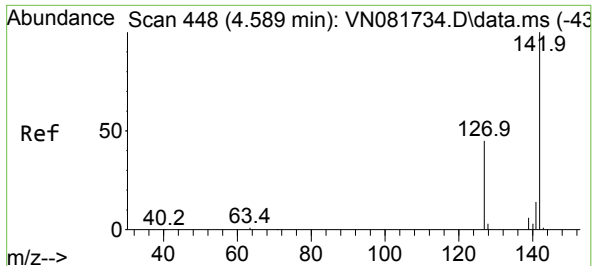


#10
Methyl Iodide
Concen: 0.300 ug/l
RT: 4.589 min Scan# 448
Delta R.T. -0.000 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03

Instrument :
MSVOA_N
ClientSampleId :



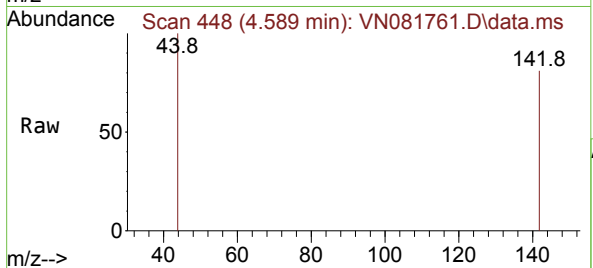



Tgt Ion:142 Resp: 487
Ion Ratio Lower Upper
142 100
127 0.0 35.8 53.6#
141 0.0 11.4 17.2#

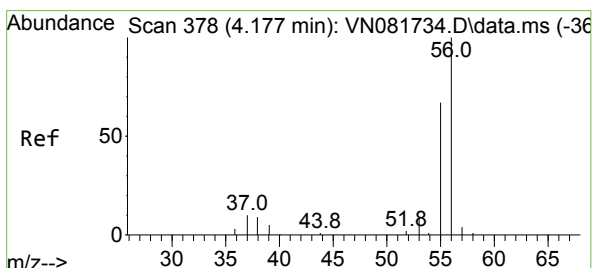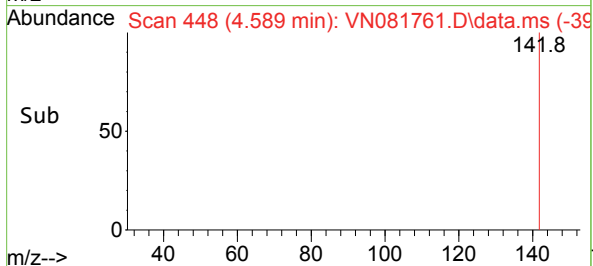

#13
Acrolein
Concen: 0.211 ug/l
RT: 4.165 min Scan# 376
Delta R.T. -0.012 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03


Tgt Ion: 56 Resp: 104
Ion Ratio Lower Upper
56 100
55 0.0 55.8 83.8#

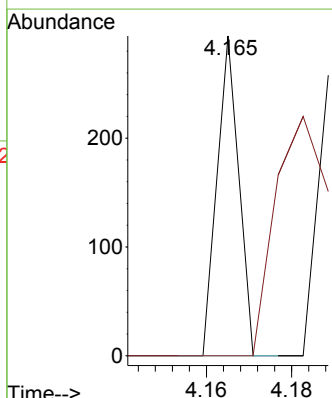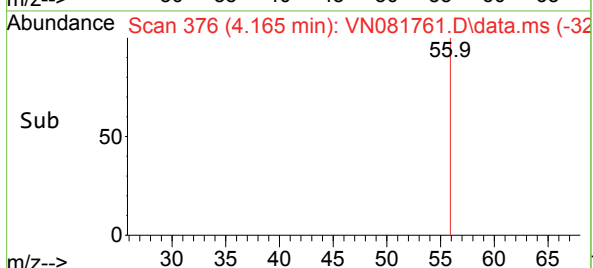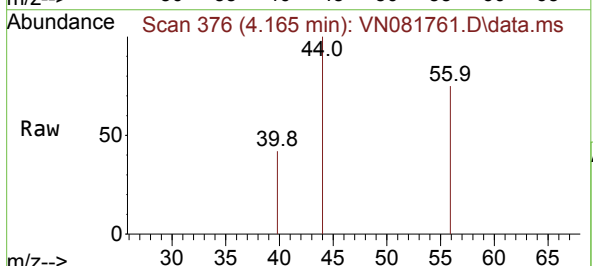






#15
Acrylonitrile
Concen: 0.517 ug/l
RT: 5.730 min Scan# 641
Delta R.T. 0.012 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 53 Resp: 661
Ion Ratio Lower Upper
53 100
52 46.3 66.1 99.1#
51 8.5 29.4 44.2#

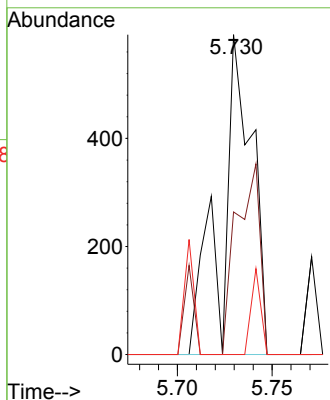


#16
Acetone
Concen: 0.991 ug/l
RT: 4.424 min Scan# 420
Delta R.T. -0.000 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03




Tgt Ion: 43 Resp: 936
Ion Ratio Lower Upper
43 100
58 33.0 25.2 37.8

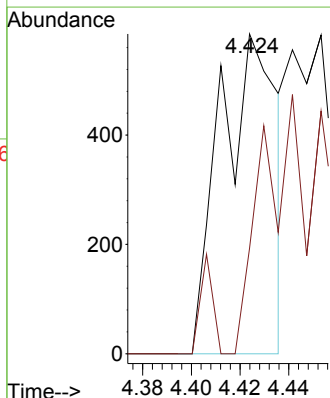






#17
Carbon Disulfide
Concen: 0.600 ug/l
RT: 4.706 min Scan# 41
Delta R.T. -0.006 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 76 Resp: 4999
Ion Ratio Lower Upper
76 100
78 10.0 7.5 11.3



#20
Methylene Chloride
Concen: Below Cal
RT: 5.277 min Scan# 565
Delta R.T. -0.000 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03


Tgt Ion: 84 Resp: 726
Ion Ratio Lower Upper
84 100
49 0.0 84.9 127.3#
51 0.0 27.0 40.6#
86 26.5 52.3 78.5#

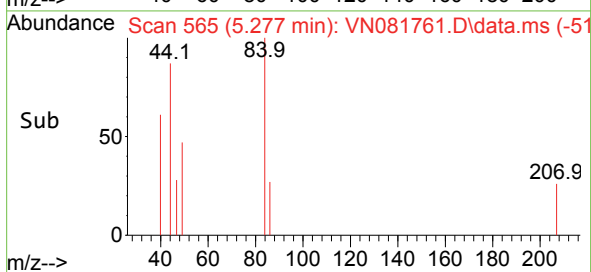






#21
trans-1,2-Dichloroethene
Concen: 0.299 ug/l
RT: 5.800 min Scan# 61
Delta R.T. 0.017 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 96 Resp: 861
Ion Ratio Lower Upper
96 100
61 0.0 96.5 144.7#
98 68.3 51.3 76.9

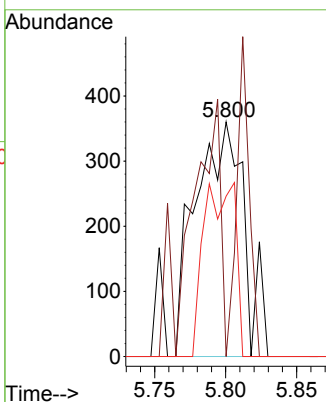


#31
Cyclohexane
Concen: 1.386 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.035 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03



Tgt Ion: 56 Resp: 6455
Ion Ratio Lower Upper
56 100
69 165.5 24.4 36.6#
84 106.6 77.0 115.4

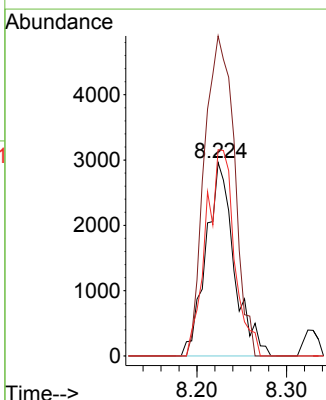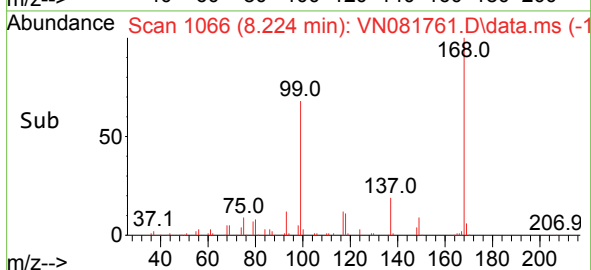



#33

1,2-Dichloroethane-d4

Concen: 50.594 ug/l

RT: 8.582 min Scan# 1126

Delta R.T. 0.005 min

Lab File: VN081761.D

Acq: 16 Apr 2024 16:03

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 171745

Ion Ratio Lower Upper

65 100

67 52.4 0.0 103.0



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1215

Delta R.T. 0.000 min

Lab File: VN081761.D

Acq: 16 Apr 2024 16:03




Tgt Ion: 114 Resp: 444448


Ion Ratio Lower Upper

114 100

63 18.4 0.0 41.0


88 15.0 0.0 31.4

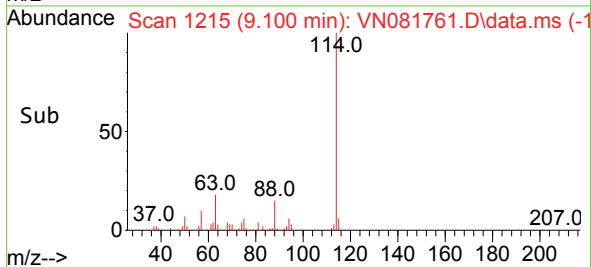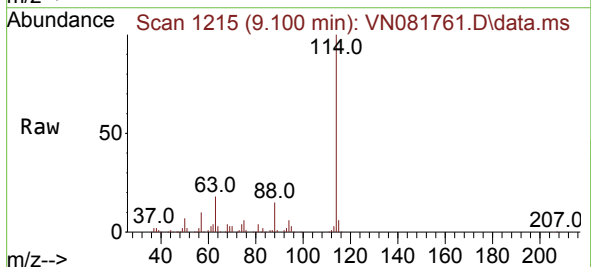






#35
Dibromofluoromethane
Concen: 48.406 ug/l
RT: 8.171 min Scan# 1056
Delta R.T. 0.006 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 113 Resp: 142067
Ion Ratio Lower Upper
113 100
111 103.6 83.4 125.2
192 17.0 14.0 21.0



#36
1,1-Dichloropropene
Concen: 5.437 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.153 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03

Tgt Ion: 75 Resp: 22233
Ion Ratio Lower Upper
75 100
110 7.4 17.8 53.5#
77 0.0 25.0 37.4#

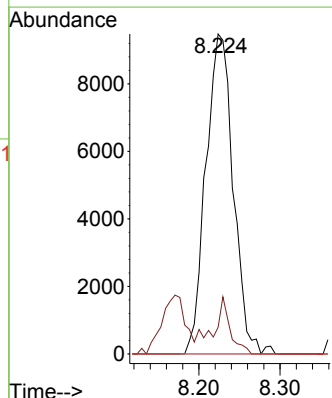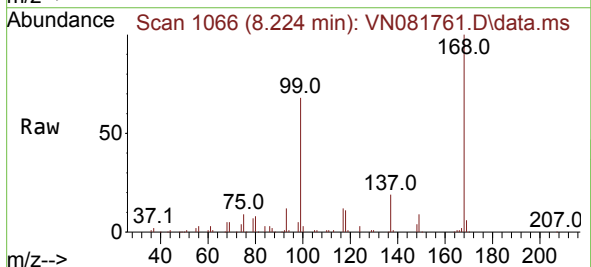



#38

Carbon Tetrachloride

Concen: 5.650 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.141 min


Lab File: VN081761.D

Acq: 16 Apr 2024 16:03

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion:117 Resp: 26881

Ion Ratio Lower Upper

117 100

119 7.6 76.5 114.7#

121 0.0 23.9 35.9#



#43

Isopropyl Acetate

Concen: 1.894 ug/l

RT: 8.677 min Scan# 1143

Delta R.T. -0.011 min

Lab File: VN081761.D

Acq: 16 Apr 2024 16:03




Tgt Ion: 43 Resp: 11872


Ion Ratio Lower Upper

43 100

61 1.5 22.8 34.2#

87 0.0 12.0 18.0#

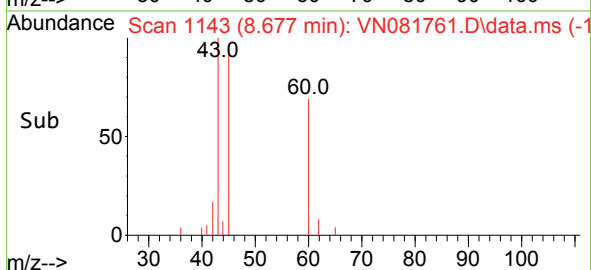



#44

Trichloroethene

Concen: 11.590 ug/l

RT: 9.353 min Scan# 11

Delta R.T. -0.000 min

Lab File: VN081761.D

Acq: 16 Apr 2024 16:03

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:130 Resp: 38391

Ion Ratio Lower Upper

130 100

95 102.7 0.0 195.4

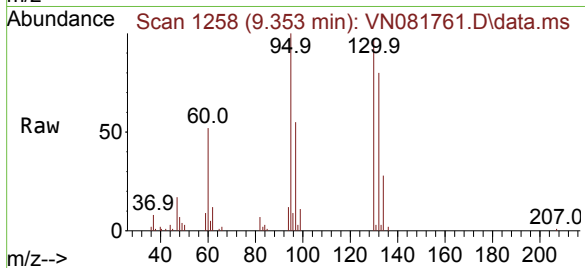

#49

1,4-Dioxane

Concen: 1.155 ug/l

RT: 9.700 min Scan# 1317

Delta R.T. -0.000 min

Lab File: VN081761.D

Acq: 16 Apr 2024 16:03




Tgt Ion: 88 Resp: 74


Ion Ratio Lower Upper

88 100

43 0.0 19.0 28.6#


58 0.0 50.6 76.0#

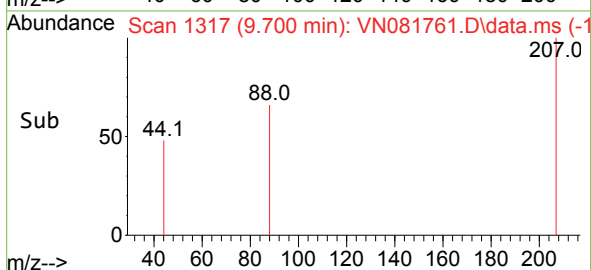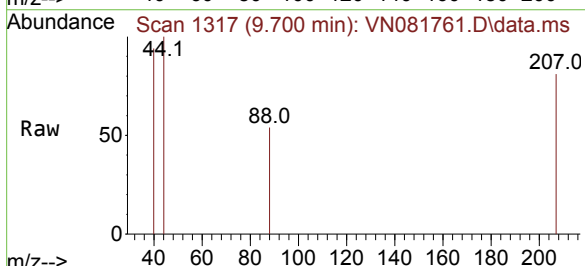






#50
Toluene-d8
Concen: 49.054 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.006 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 98 Resp: 530376
Ion Ratio Lower Upper
98 100
100 63.8 51.8 77.6



#59
2-Hexanone
Concen: 0.210 ug/l
RT: 11.200 min Scan# 1572
Delta R.T. 0.006 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03

Tgt Ion: 43 Resp: 529
Ion Ratio Lower Upper
43 100
58 0.0 28.3 84.9#


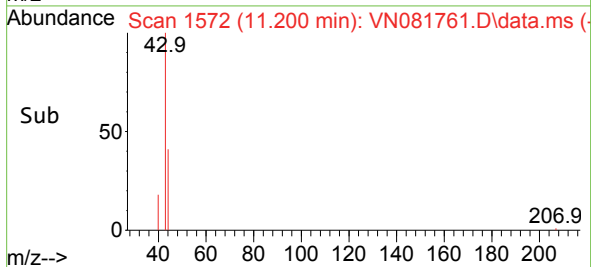

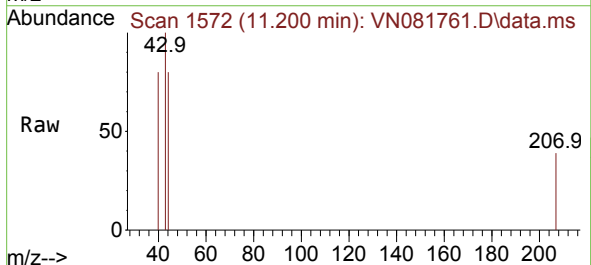


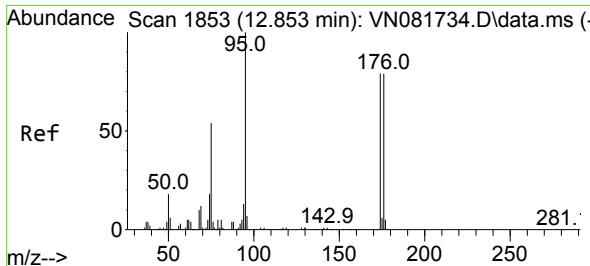

#62
4-Bromofluorobenzene
Concen: 46.352 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 171259
Ion Ratio Lower Upper
95 100
174 78.2 0.0 160.6
176 71.1 0.0 152.8

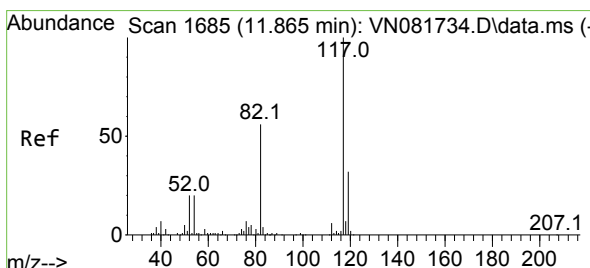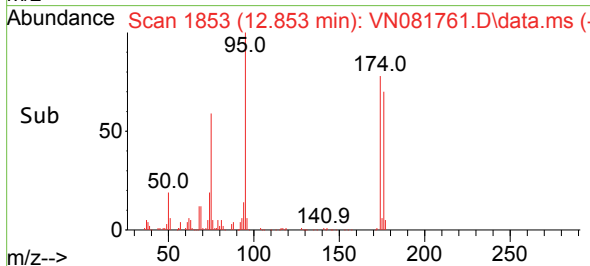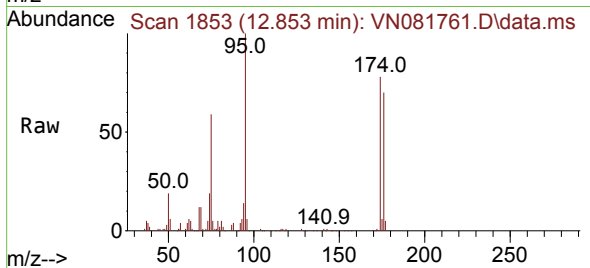

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1686
Delta R.T. 0.005 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03

Tgt Ion: 117 Resp: 389448
Ion Ratio Lower Upper
117 100
82 56.8 44.6 66.8
119 32.7 25.9 38.9

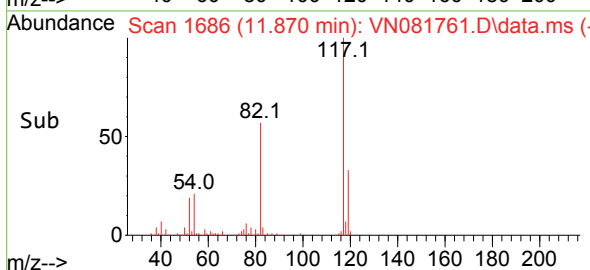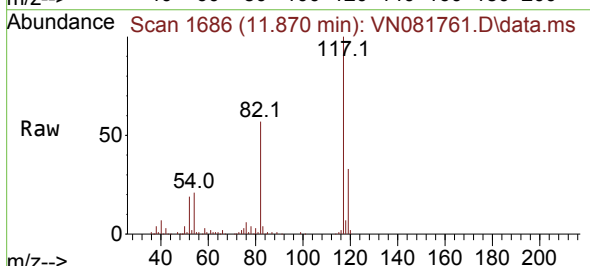



#64

Tetrachloroethene

Concen: 0.615 ug/l

RT: 11.100 min Scan# 1555

Delta R.T. -0.006 min


Lab File: VN081761.D

Acq: 16 Apr 2024 16:03

Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion:164 Resp: 2032




Ion Ratio Lower Upper

164 100

166 82.2 97.6 146.4#

129 94.2 73.7 110.5

131 51.7 75.8 113.6#

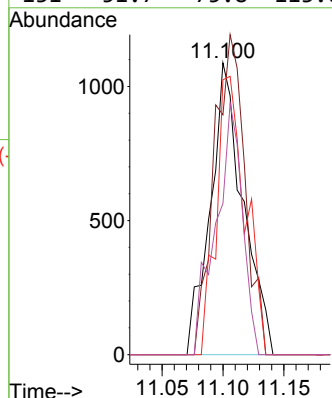

#68

m/p-Xylenes

Concen: 0.226 ug/l

RT: 12.082 min Scan# 1722

Delta R.T. 0.011 min

Lab File: VN081761.D




Acq: 16 Apr 2024 16:03


Tgt Ion:106 Resp: 1239

Ion Ratio Lower Upper

106 100


91 199.3 159.4 239.0

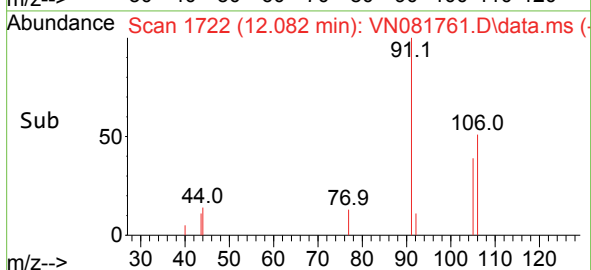



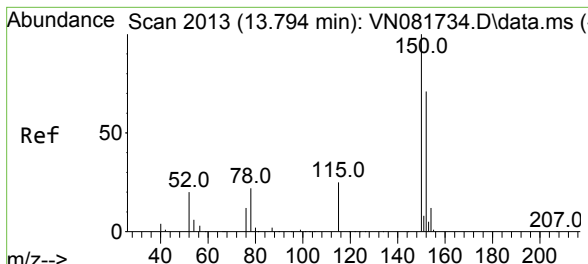


#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.794 min Scan# 2013
 Delta R.T. -0.000 min
 Lab File: VN081761.D
 Acq: 16 Apr 2024 16:03

Instrument :
 MSVOA_N
 ClientSampleId :



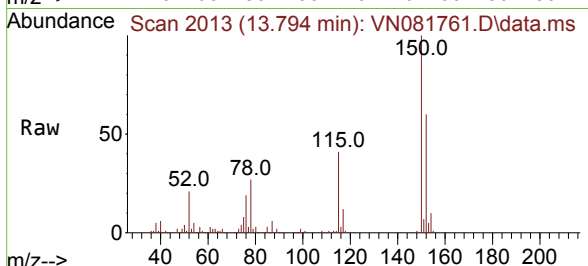



Tgt Ion:152 Resp: 161456
 Ion Ratio Lower Upper
 152 100
 115 63.6 30.4 91.3
 150 159.3 0.0 353.2

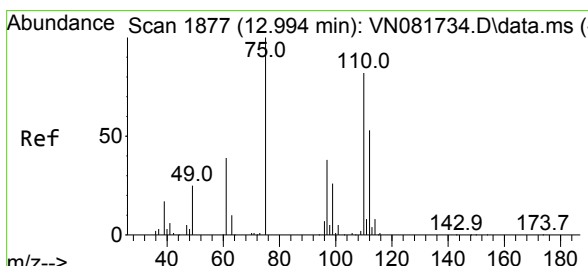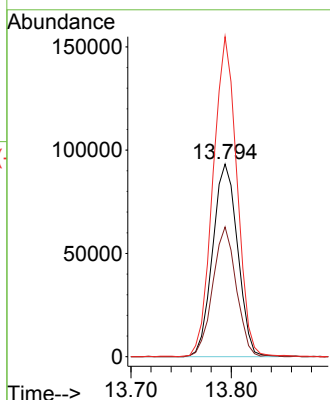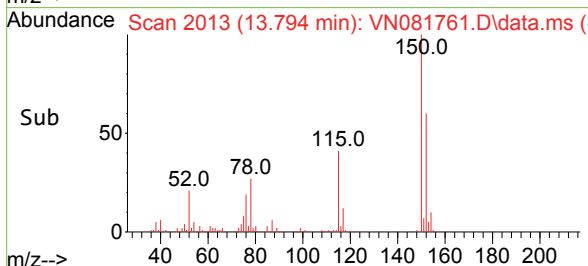

#76
 1,2,3-Trichloropropane
 Concen: 31.232 ug/l
 RT: 12.853 min Scan# 1853
 Delta R.T. -0.141 min
 Lab File: VN081761.D
 Acq: 16 Apr 2024 16:03


Tgt Ion: 75 Resp: 95905
 Ion Ratio Lower Upper
 75 100
 77 1.2 90.5 271.3#

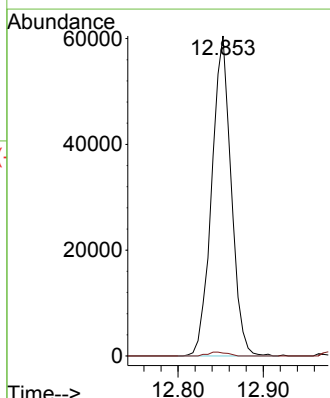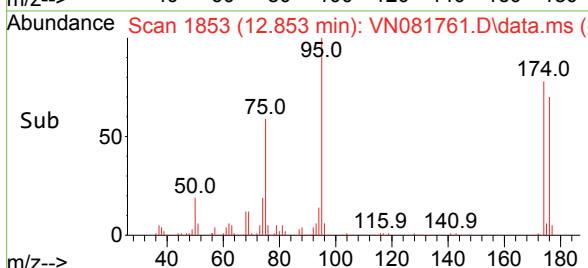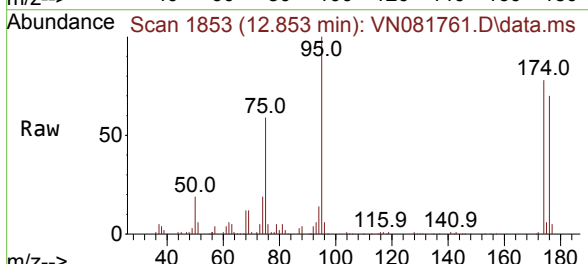






#81
trans-1,4-Dichloro-2-butene
Concen: 72.681 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.118 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 75 Resp: 95905
Ion Ratio Lower Upper
75 100
53 0.1 72.9 109.3#
89 0.0 39.1 58.7#

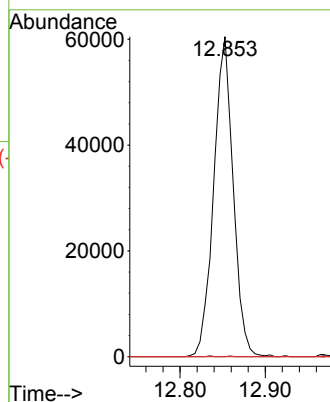

#82
4-Chlorotoluene
Concen: 0.239 ug/l
RT: 13.223 min Scan# 1916
Delta R.T. 0.000 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03


Tgt Ion: 91 Resp: 2065
Ion Ratio Lower Upper
91 100
126 23.8 17.4 52.3

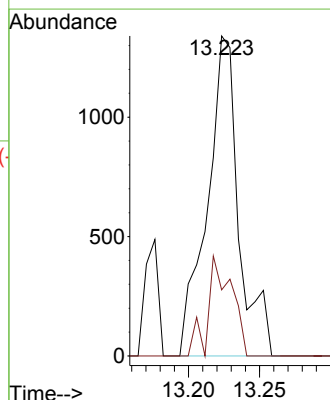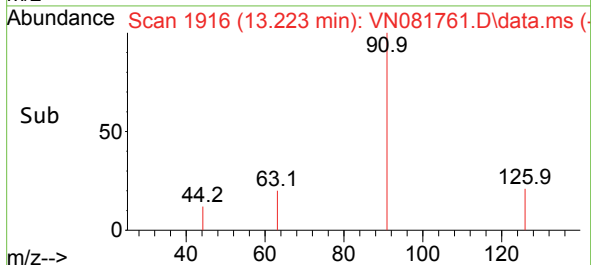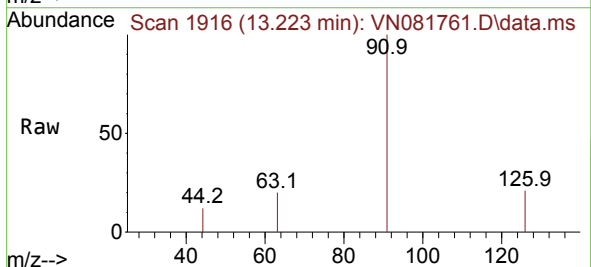






#87
1,3-Dichlorobenzene
Concen: 0.352 ug/l
RT: 13.729 min Scan# 2002
Delta R.T. -0.006 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:146 Resp: 2033
Ion Ratio Lower Upper
146 100
111 37.5 20.8 62.5
148 50.7 32.1 96.3

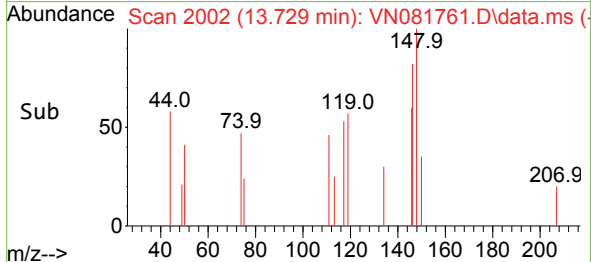

#88
1,4-Dichlorobenzene
Concen: 0.346 ug/l
RT: 13.729 min Scan# 2002
Delta R.T. -0.083 min
Lab File: VN081761.D
Acq: 16 Apr 2024 16:03

Tgt Ion:146 Resp: 2033
Ion Ratio Lower Upper
146 100
111 37.5 19.3 57.9
148 50.7 31.3 93.9

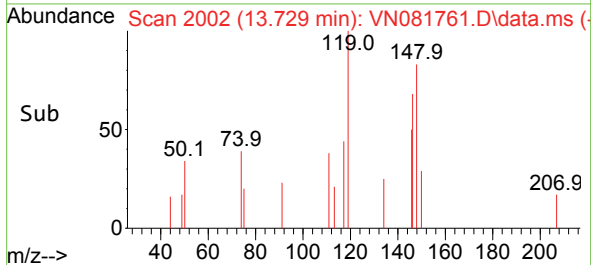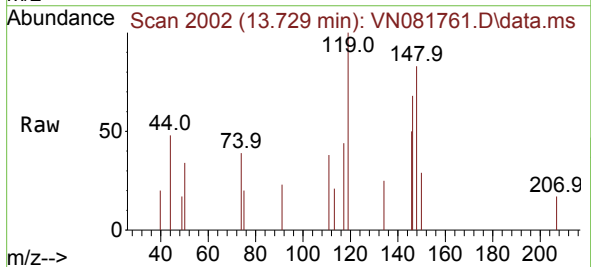



#89

n-Butylbenzene

Concen: 0.236 ug/l

RT: 14.064 min Scan# 2059

Delta R.T. 0.005 min

Lab File: VN081761.D





Acq: 16 Apr 2024 16:03

Instrument :

MSVOA_N

ClientSampleId :

Tgt Ion:	91	Resp:	2047
Ion	Ratio	Lower	Upper
91	100		
92	38.6	26.2	78.5
134	27.8	13.2	39.5

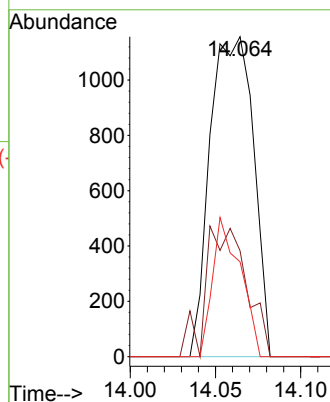

#93

1,2,4-Trichlorobenzene

Concen: 0.640 ug/l




RT: 15.400 min Scan# 2286


Delta R.T. 0.006 min

Lab File: VN081761.D

Acq: 16 Apr 2024 16:03

Tgt Ion:	180	Resp:	1883
Ion	Ratio	Lower	Upper
180	100		
182	89.9	46.7	140.0
145	31.1	16.2	48.6

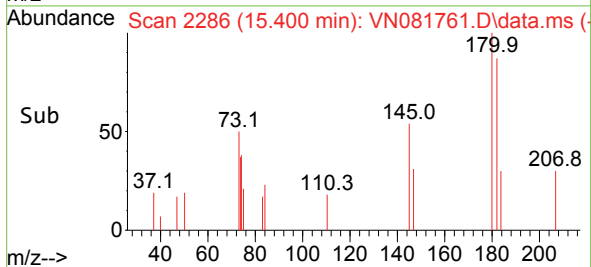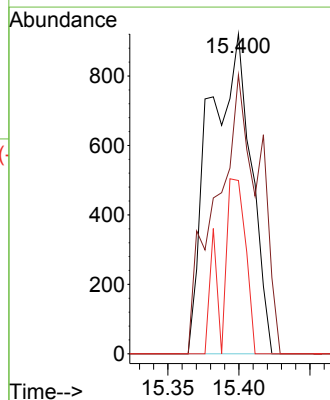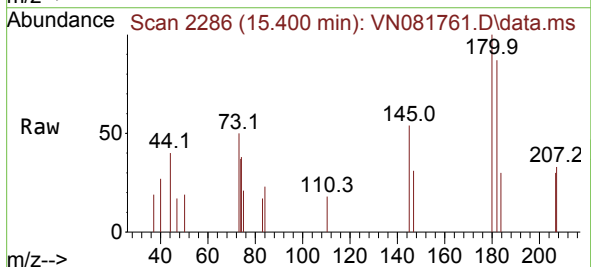



#94

Hexachlorobutadiene

Concen: 1.022 ug/l

RT: 15.506 min Scan# 21

Delta R.T. -0.001 min


Lab File: VN081761.D

Acq: 16 Apr 2024 16:03




Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion:	225	Resp:	1296
Ion	Ratio	Lower	Upper
225	100		
223	54.9	31.1	93.2
227	43.9	30.6	91.6

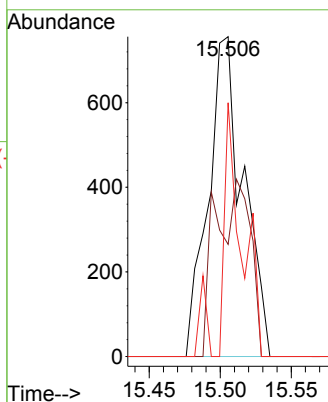

#95

Naphthalene

Concen: 0.638 ug/l




RT: 15.647 min Scan# 2328


Delta R.T. 0.006 min

Lab File: VN081761.D

Acq: 16 Apr 2024 16:03


Tgt Ion:	128	Resp:	5996
Ion	Ratio	Lower	Upper
128	100		
127	11.5	10.1	15.1
129	1.5	8.9	13.3

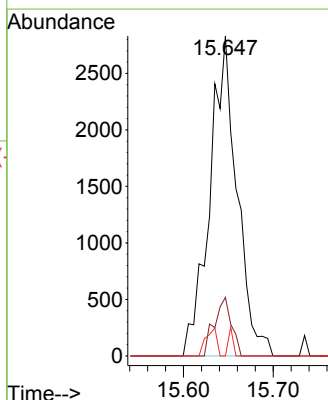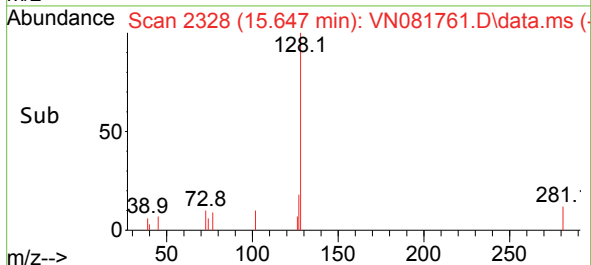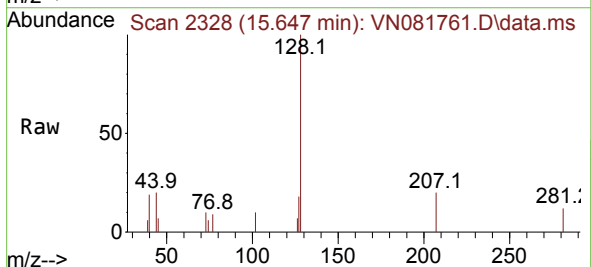



#96
 1,2,3-Trichlorobenzene
 Concen: 0.834 ug/l
 RT: 15.853 min Scan# 21
 Delta R.T. 0.012 min
 Lab File: VN081761.D
 Acq: 16 Apr 2024 16:03

Instrument :
 MSVOA_N
 ClientSampleId :

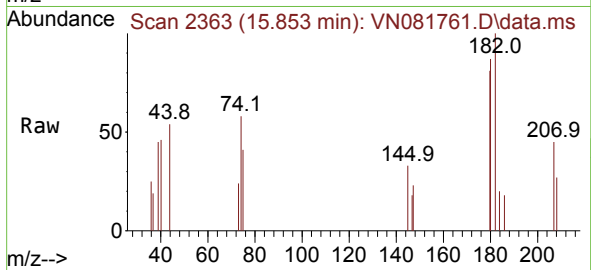

Tgt Ion:180 Resp: 2509
 Ion Ratio Lower Upper
 180 100
 182 90.7 46.0 137.8
 145 21.1 17.1 51.3

