
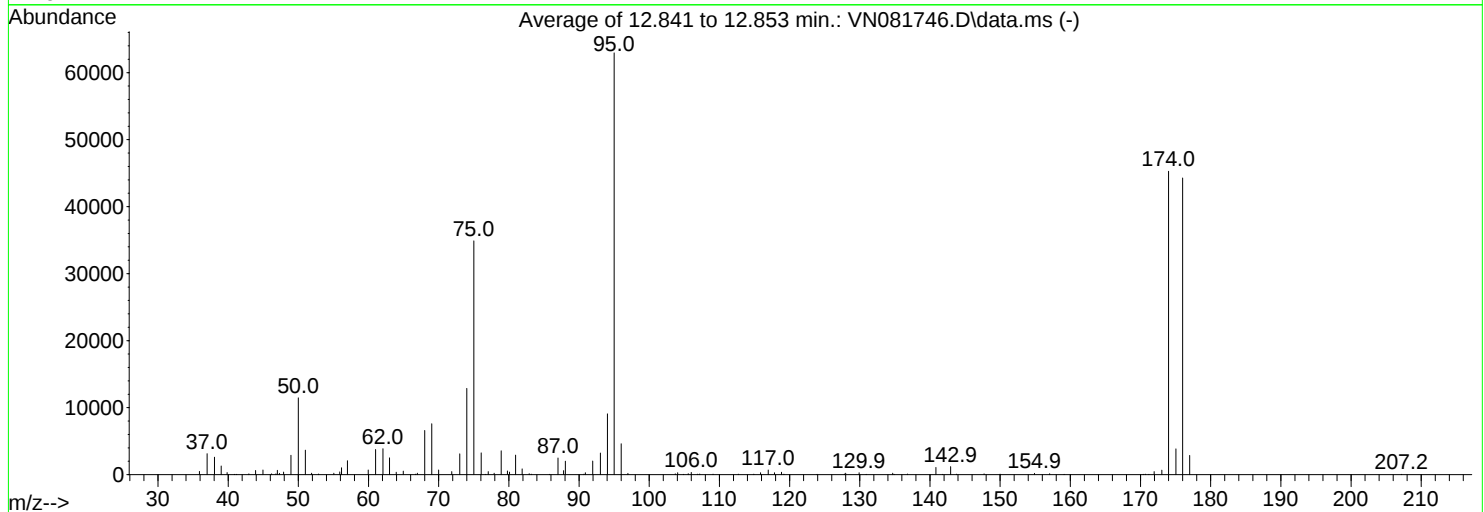


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041624\
Data File : VN081746.D
Acq On : 16 Apr 2024 08:44
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041524W.M
Title : SW846 8260
Last Update : Mon Apr 15 15:37:39 2024

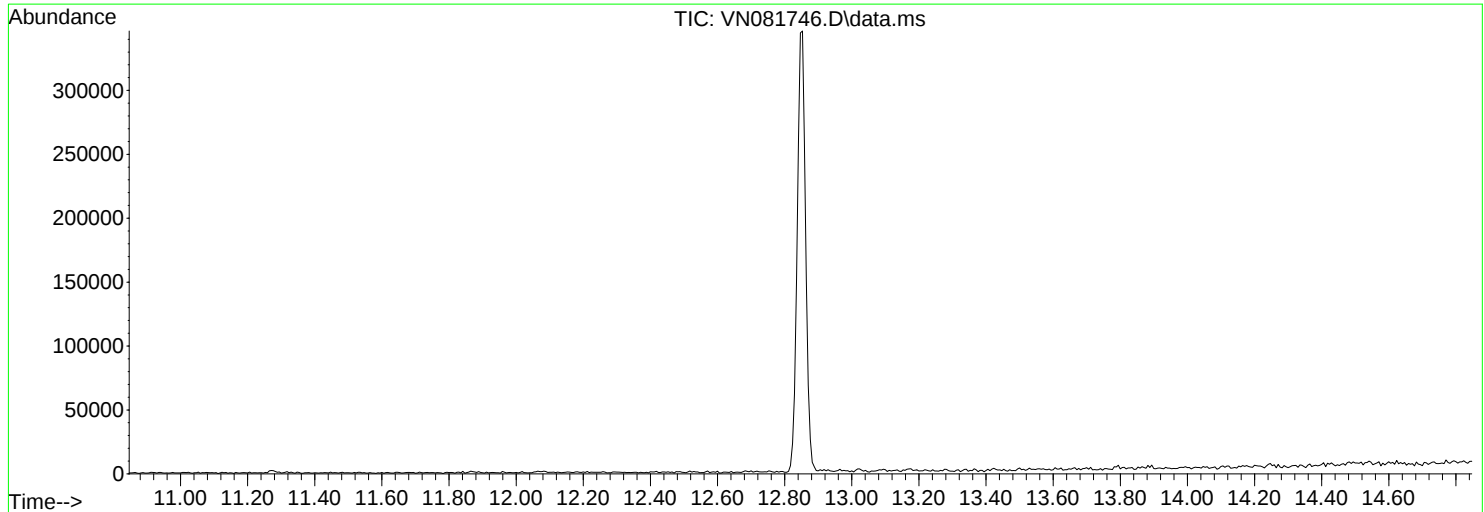

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	11458	PASS
75	95	30	60	55.4	34891	PASS
95	95	100	100	100.0	62957	PASS
96	95	5	9	7.3	4610	PASS
173	174	0.00	2	1.5	667	PASS
174	95	50	100	71.9	45288	PASS
175	174	5	9	8.5	3855	PASS
176	174	95	101	97.8	44285	PASS
177	176	5	9	6.5	2859	PASS

Average of 12.841 to 12.853 min.: VN081746.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	481	46.80	134	56.15	1034	69.00	758
37.00	3122	47.00	643	57.00	2075	70.00	701
38.05	2607	47.30	193	59.95	699	71.85	45
39.00	1300	47.90	373	61.00	3761	73.00	311
39.85	300	48.95	2893	62.05	3883	74.00	12865
40.90	56	50.00	11458	63.00	2510	75.00	34891
41.20	56	51.00	3667	63.95	369	76.05	3253
42.95	134	51.90	210	64.95	537	76.70	53
43.90	617	52.90	104	66.70	67	77.05	454
44.95	687	55.05	226	66.95	219	77.90	227
46.20	127	55.90	411	68.00	6586	78.90	3556

Average of 12.841 to 12.853 min.: VN081746.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.80	545	90.90	280	106.00	342	123.90	52
80.10	380	91.95	2043	106.90	73	127.80	98
80.95	2921	93.05	3222	107.20	91	128.00	212
81.90	868	94.05	9075	109.10	64	129.90	283
82.90	143	95.00	62957	112.70	79	130.90	53
83.20	68	96.00	4610	114.90	74	134.70	204
85.80	63	96.95	198	115.85	284	134.90	55
87.00	2493	103.70	122	116.95	696	136.80	99
87.80	611	104.05	291	117.85	296	140.85	1069
88.05	2008	104.90	51	118.85	357	141.80	57
90.70	75	105.55	151	119.20	78	142.95	1195

Average of 12.841 to 12.853 min.: VN081746.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
143.80	65	174.00	45288				
147.70	123	175.05	3855				
150.00	64	176.00	44285				
154.90	203	177.00	2859				
157.05	154	207.20	60				
159.10	62						
170.40	54						
170.70	78						
171.20	55						
171.95	454						
173.05	667						

Instrument :

MSVOA_N

ClientSampleId :

BFB