

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041625\
 Data File : VN086301.D
 Acq On : 16 Apr 2025 16:51
 Operator : JC\MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Quant Time: Apr 17 03:07:58 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 16 04:19:23 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	194380	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.094	114	369447	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	344478	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	156273	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	138602	49.173	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	98.340%
35) Dibromofluoromethane	8.165	113	94390	55.049	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	110.100%
50) Toluene-d8	10.565	98	470129	51.302	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	102.600%
62) 4-Bromofluorobenzene	12.847	95	174493	52.205	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	104.400%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041625\
Data File : VN086301.D
Acq On : 16 Apr 2025 16:51
Operator : JC\MD
Sample : IBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Time: Apr 17 03:07:58 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 16 04:19:23 2025
Response via : Initial Calibration




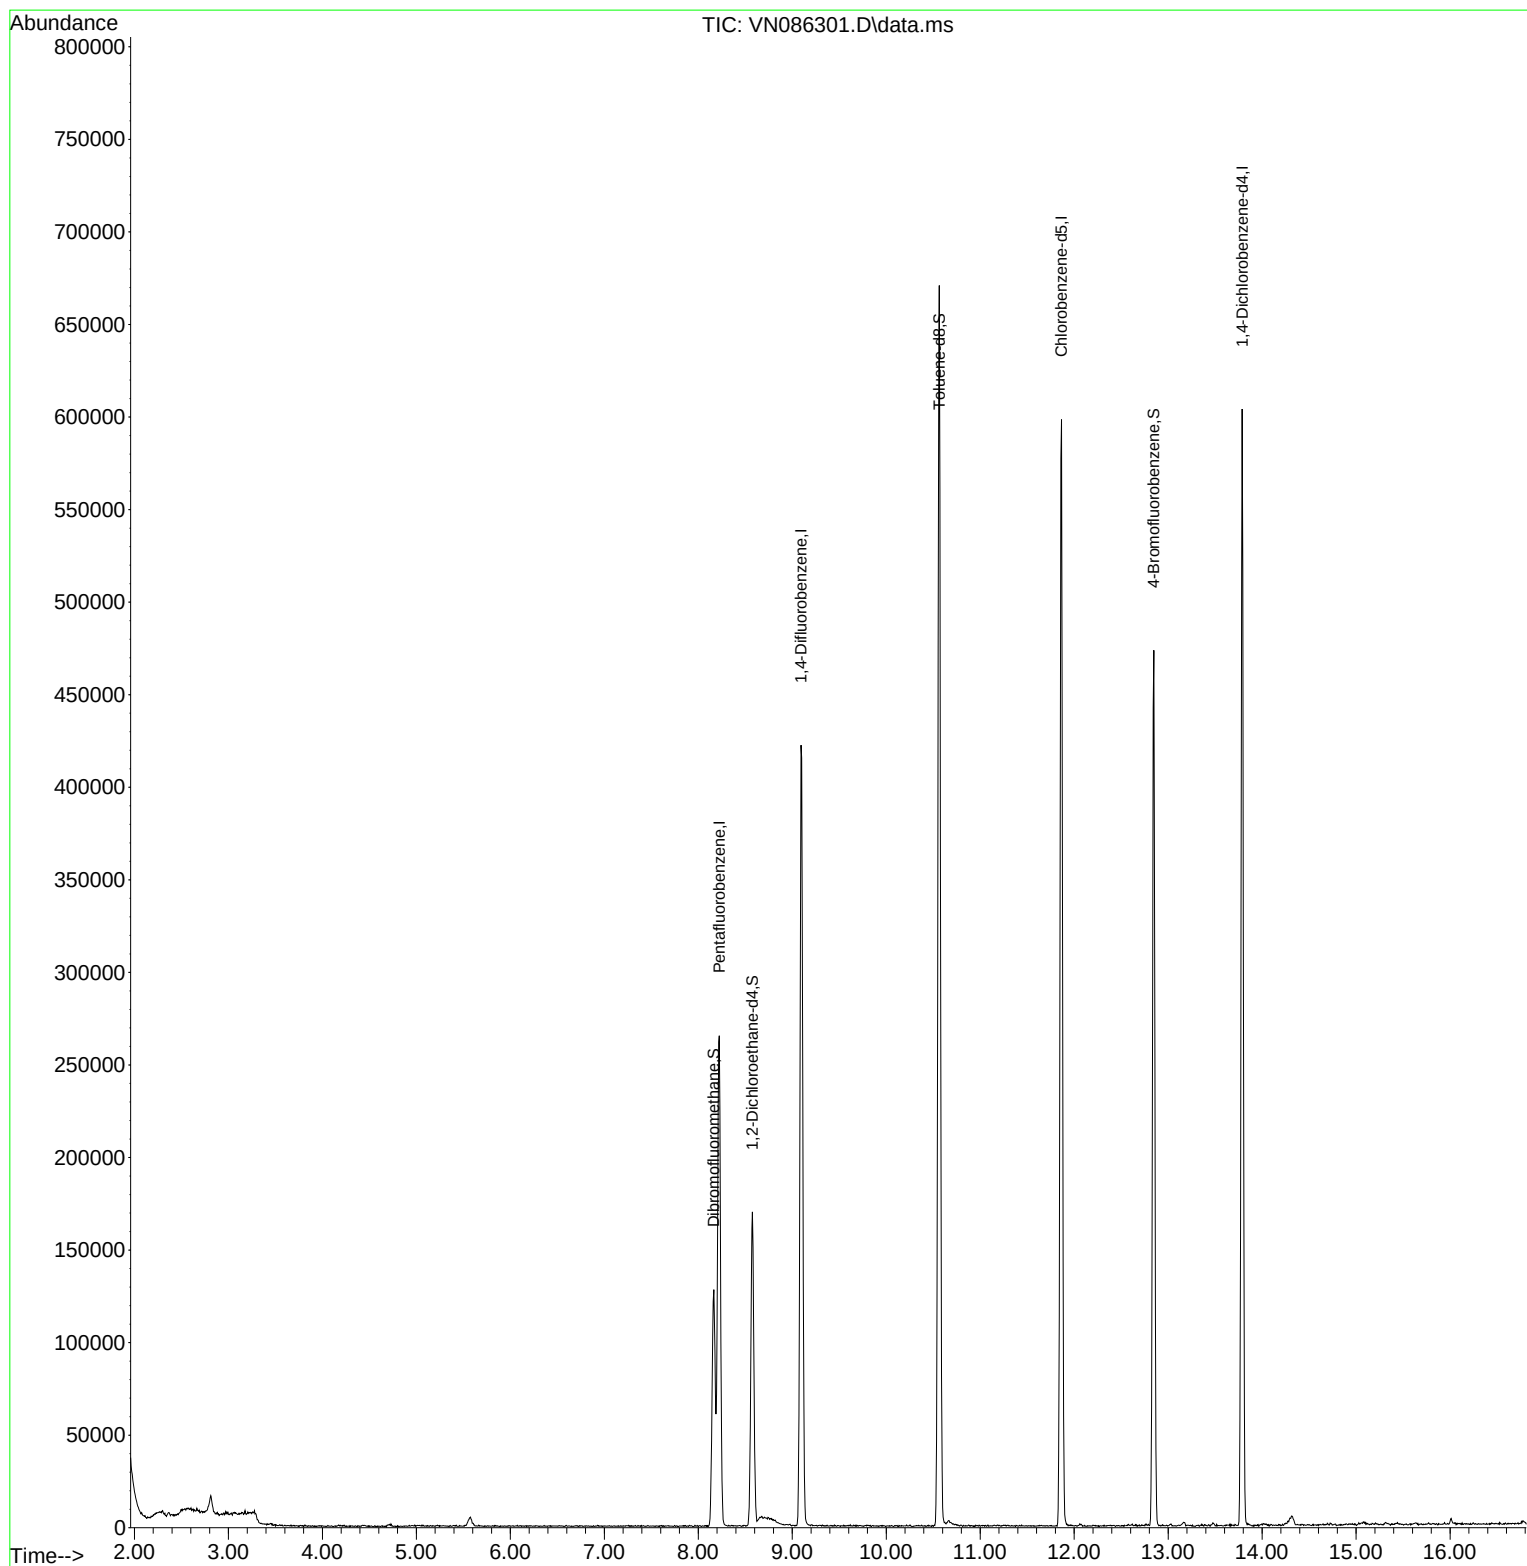


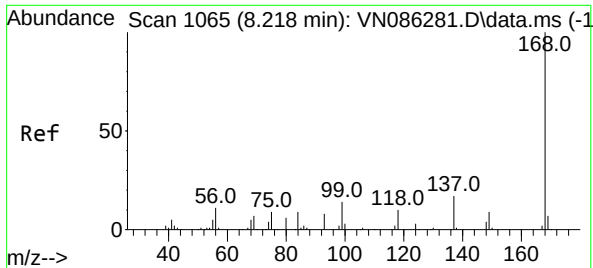

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1065
Delta R.T. 0.006 min
Lab File: VN086301.D
Acq: 16 Apr 2025 16:51




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 194380
Ion Ratio Lower Upper
168 100
99 62.3 52.5 78.7

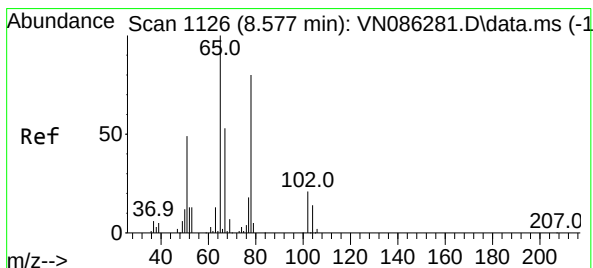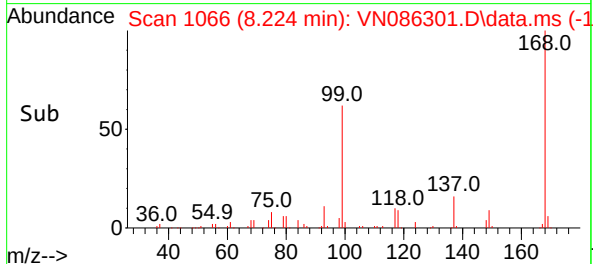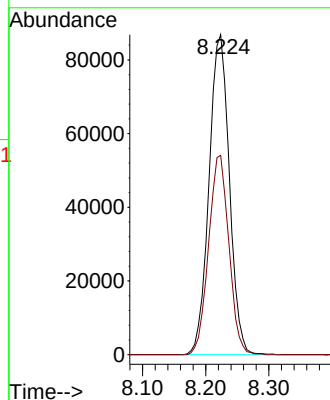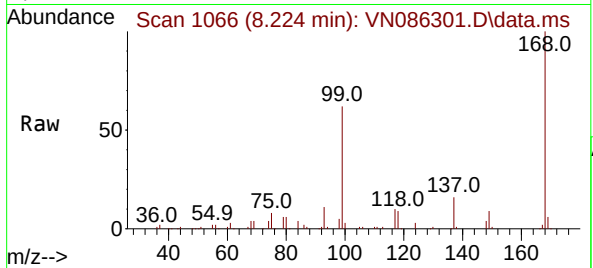

#33
1,2-Dichloroethane-d4
Concen: 49.173 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VN086301.D
Acq: 16 Apr 2025 16:51

Tgt Ion: 65 Resp: 138602
Ion Ratio Lower Upper
65 100
67 52.6 0.0 106.0

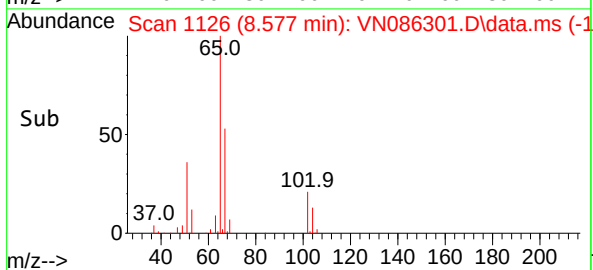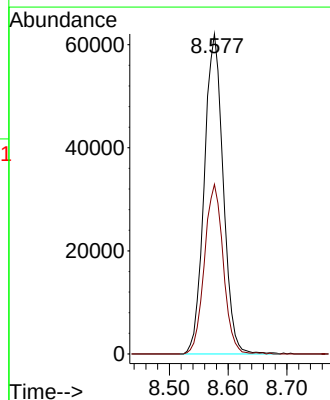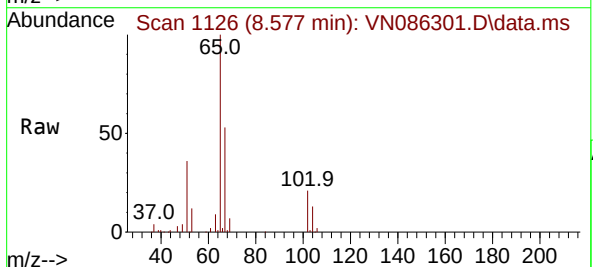

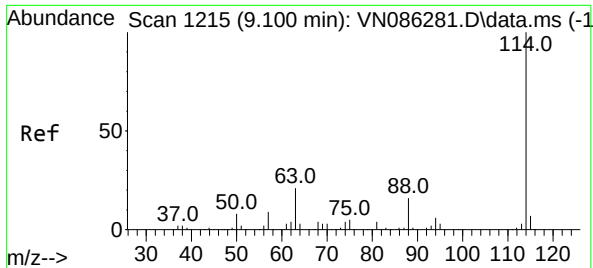

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.094 min Scan# 11

Delta R.T. -0.006 min

Lab File: VN086301.D

Acq: 16 Apr 2025 16:51

Instrument :

MSVOA_N

ClientSampleId :

IBLK





Tgt Ion:114 Resp: 369447

Ion Ratio Lower Upper

114 100

63 21.2 0.0 42.6

88 16.3 0.0 31.8

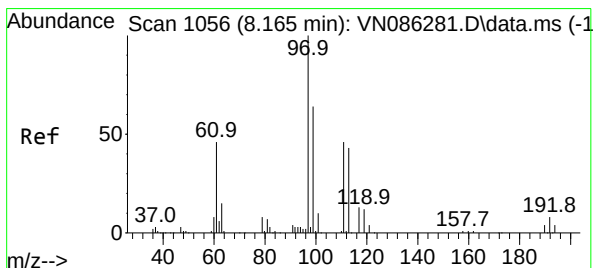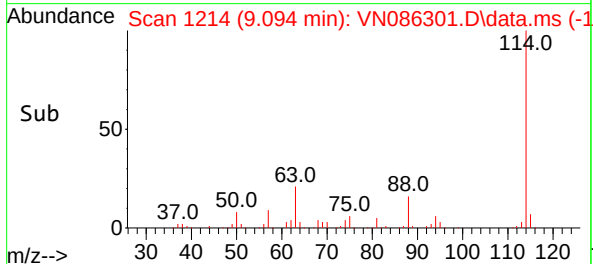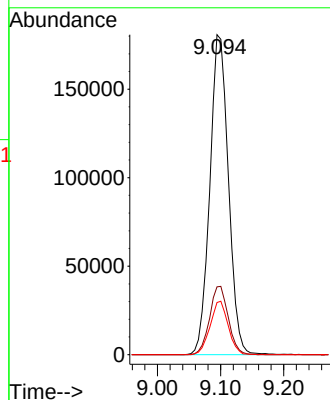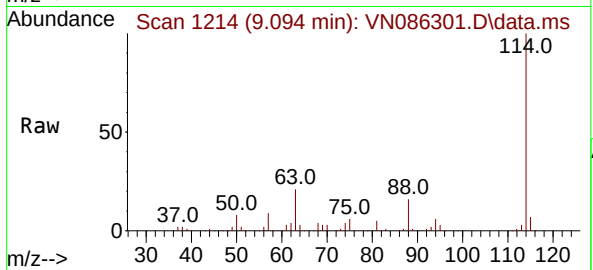

#35

Dibromofluoromethane

Concen: 55.049 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.000 min

Lab File: VN086301.D

Acq: 16 Apr 2025 16:51




Tgt Ion:113 Resp: 94390


Ion Ratio Lower Upper

113 100

111 105.7 83.4 125.0

192 17.2 13.7 20.5


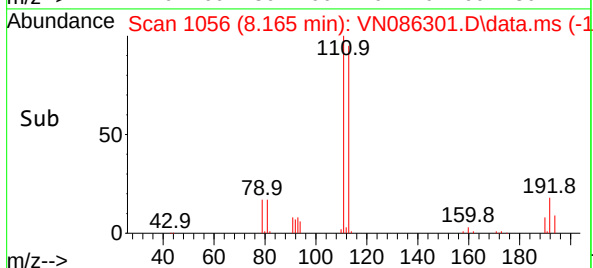
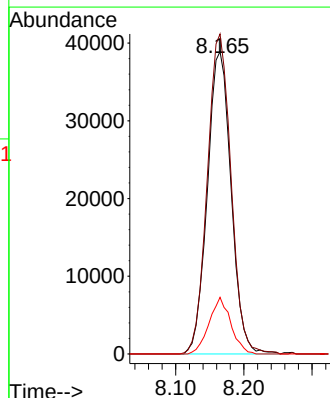
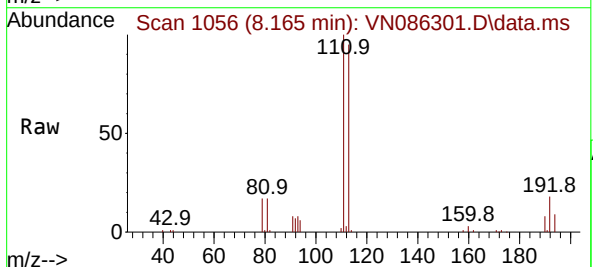


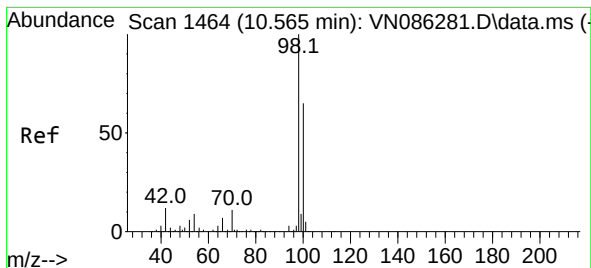

#50
Toluene-d8
Concen: 51.302 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.000 min
Lab File: VN086301.D
Acq: 16 Apr 2025 16:51




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 470129
Ion Ratio Lower Upper
98 100
100 65.7 52.5 78.7

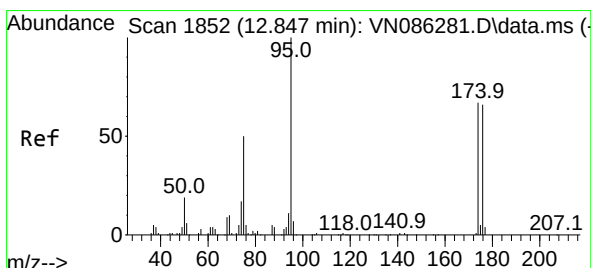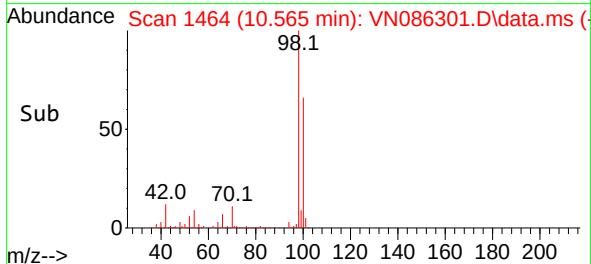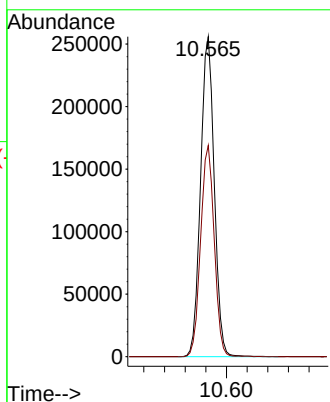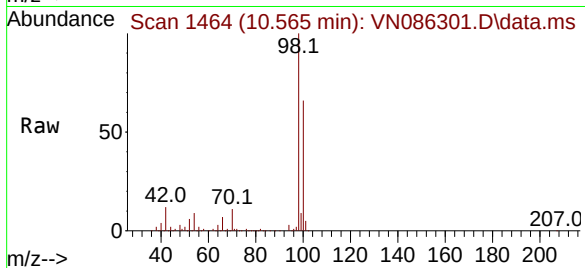

#62
4-Bromofluorobenzene
Concen: 52.205 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN086301.D
Acq: 16 Apr 2025 16:51

Tgt Ion: 95 Resp: 174493
Ion Ratio Lower Upper
95 100
174 68.9 0.0 133.4
176 66.4 0.0 129.2


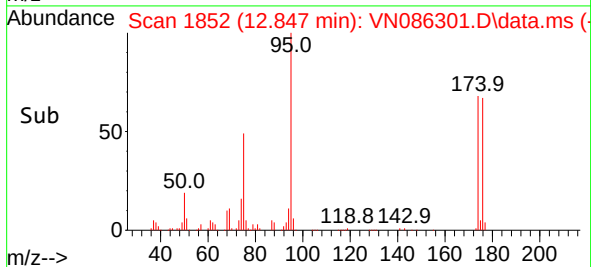
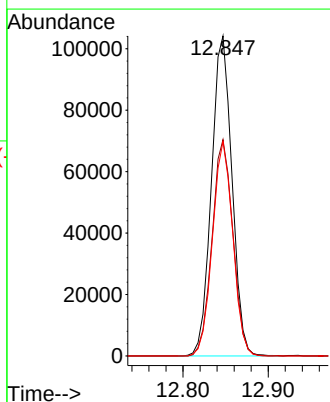
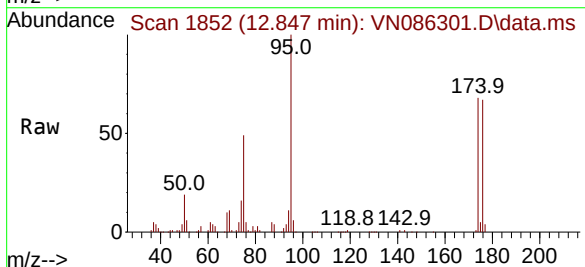


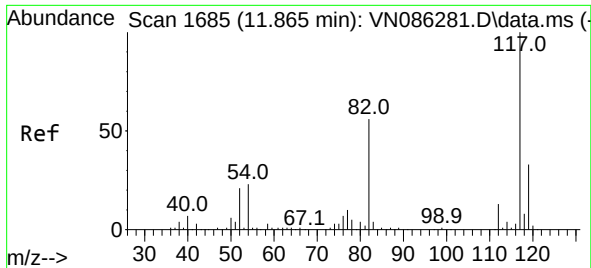

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN086301.D
Acq: 16 Apr 2025 16:51

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Tgt Ion:117 Resp: 344478
Ion Ratio Lower Upper
117 100
82 57.3 44.7 67.1
119 33.6 26.4 39.6

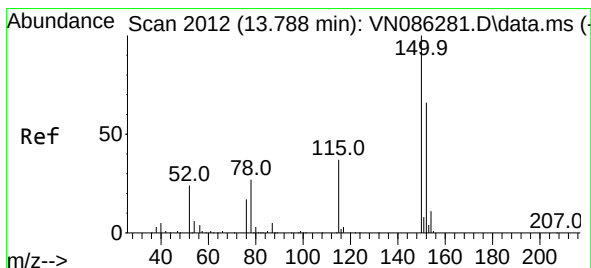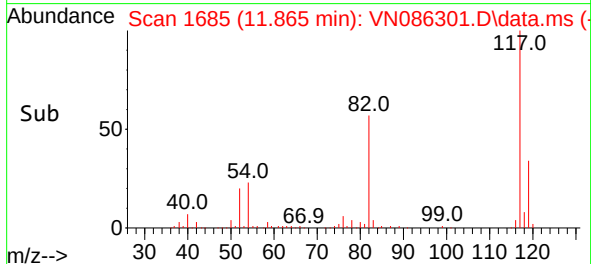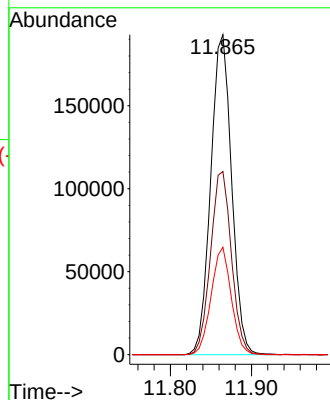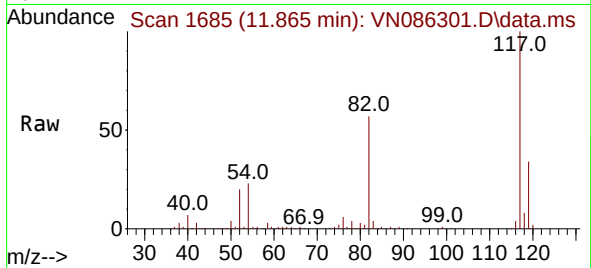

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. 0.000 min
Lab File: VN086301.D
Acq: 16 Apr 2025 16:51

Tgt Ion:152 Resp: 156273
Ion Ratio Lower Upper
152 100
115 62.7 31.9 95.9
150 158.0 0.0 352.0

