
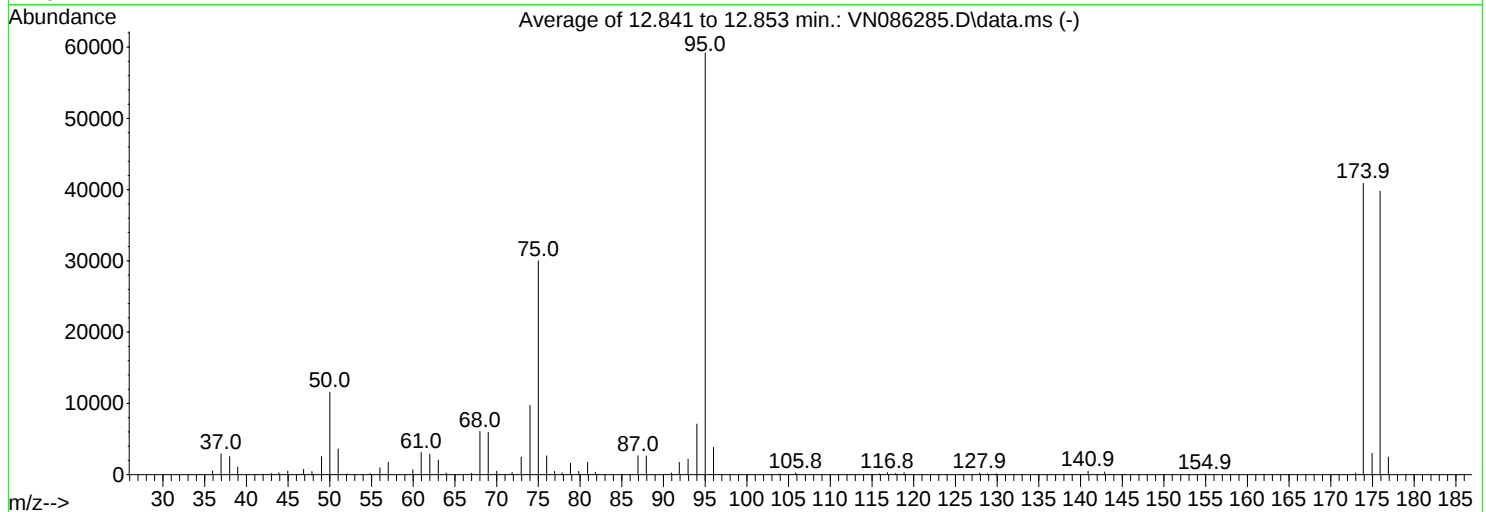


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041625\
Data File : VN086285.D
Acq On : 16 Apr 2025 08:38
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Title : SW846 8260
Last Update : Wed Apr 16 04:19:23 2025

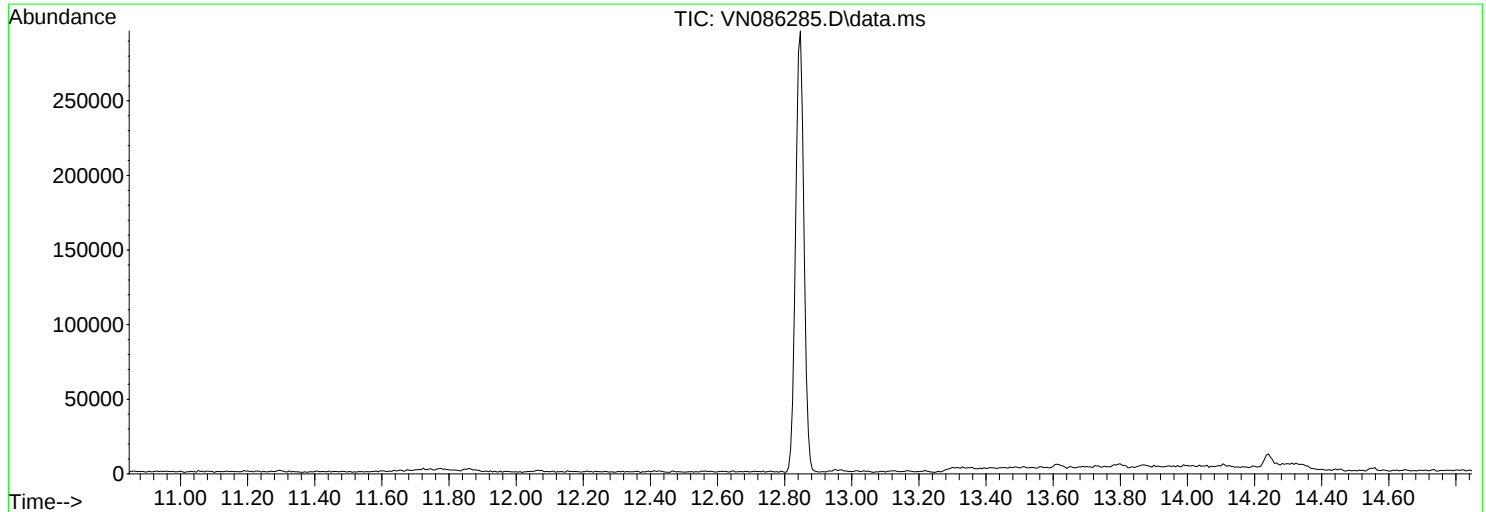

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	11559	PASS
75	95	30	60	50.7	30005	PASS
95	95	100	100	100.0	59203	PASS
96	95	5	9	6.5	3819	PASS
173	174	0.00	2	0.6	241	PASS
174	95	50	100	69.1	40880	PASS
175	174	5	9	7.4	3011	PASS
176	174	95	101	97.3	39787	PASS
177	176	5	9	6.2	2465	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	525	49.00	2548	63.95	244	77.85	244
36.95	2913	50.00	11559	66.95	198	78.85	1591
38.00	2541	51.00	3615	68.00	6055	79.85	46
38.95	1065	52.05	115	69.00	5936	80.90	1730
39.90	41	54.85	151	70.00	495	81.85	336
42.00	61	56.00	963	71.85	288	86.95	2654
43.00	153	57.00	1730	72.95	2481	87.95	2625
43.90	274	59.95	690	74.00	9726	90.95	232
44.95	516	60.95	3100	75.00	30005	91.90	1720
46.85	741	62.00	2878	76.00	2633	92.95	2175
47.85	420	63.00	2054	76.95	454	94.00	7091

Average of 12.841 to 12.853 min.: VN086285.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.00	59203	129.90	136				
96.00	3819	140.90	482				
103.80	73	142.90	387				
104.00	124	154.90	82				
105.85	219	172.95	241				
115.90	128	173.90	40880				
116.85	302	174.95	3011				
117.85	183	175.90	39787				
118.85	271	176.90	2465				
127.90	204						
128.85	127						

Instrument :

MSVOA_N

ClientSampleId :

BFB