

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN041720\
 Data File : VN061077.D
 Acq On : 18 Apr 2020 1:59
 Operator : JC/MD
 Sample : L2338-07
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BP-MW202S-20200414

Quant Time: Apr 20 01:40:42 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N041620W.M
 Quant Title : SW846 8260
 QLast Update : Fri Apr 17 03:49:39 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.64	168	142354	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.56	114	243263	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.40	117	228978	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	101148	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.00	65	97804	53.70	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	107.40%	
35) Dibromofluoromethane	7.56	113	73563	51.78	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	103.56%	
50) Toluene-d8	10.08	98	302254	56.30	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	112.60%	
62) 4-Bromofluorobenzene	12.39	95	110765	52.65	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	105.30%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
14) Allyl chloride	4.02	41	1313	0.445	ug/l #	68
16) Acetone	3.79	43	1110	1.385	ug/l #	44
18) Methyl Acetate	4.01	43	3744	1.489	ug/l #	54
31) Cyclohexane	7.64	56	3220	0.949	ug/l #	1
36) 1,1-Dichloropropene	7.64	75	11866	4.727	ug/l #	49
38) Carbon Tetrachloride	7.64	117	13794	6.602	ug/l #	15
71) Bromoform	12.40	173	381	0.302	ug/l #	1
76) 1,2,3-Trichloropropane	12.39	75	56951	25.598	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.39	75	56951	63.139	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN041720\
Data File : VN061077.D
Acq On : 18 Apr 2020 1:59
Operator : JC/MD
Sample : L2338-07
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BP-MW202S-20200414

Quant Time: Apr 20 01:40:42 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N041620W.M
Quant Title : SW846 8260
QLast Update : Fri Apr 17 03:49:39 2020
Response via : Initial Calibration

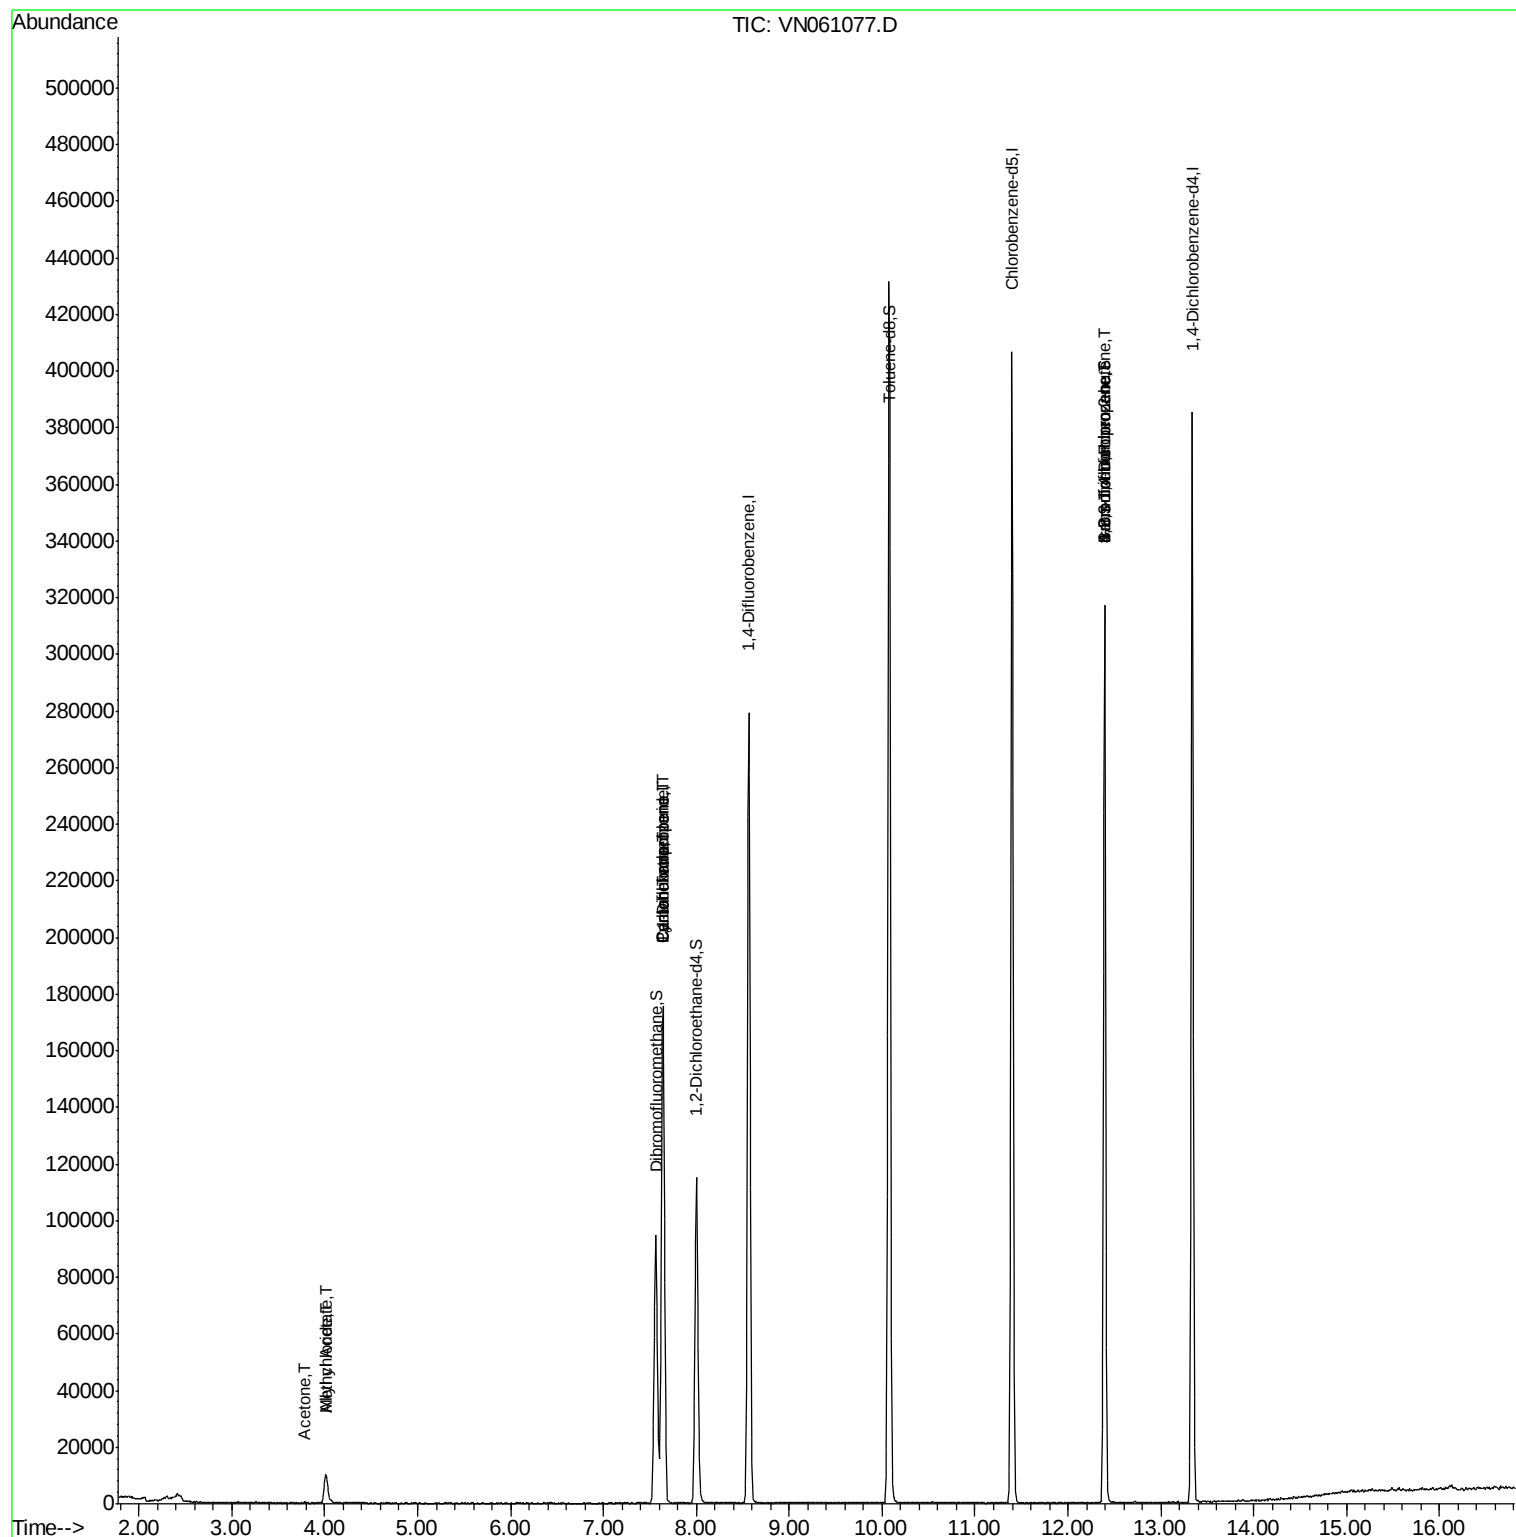



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.64 min Scan# 1825

Delta R.T. 0.00 min

Lab File: VN061077.D

Acq: 18 Apr 2020 1:59

Instrument :

MSVOA_N

ClientSampleId :


BP-MW202S-20200414

Tot Ion:168 Resp: 142354




Ion Ratio Lower Upper

168 100

99 58.5 47.4 71.2

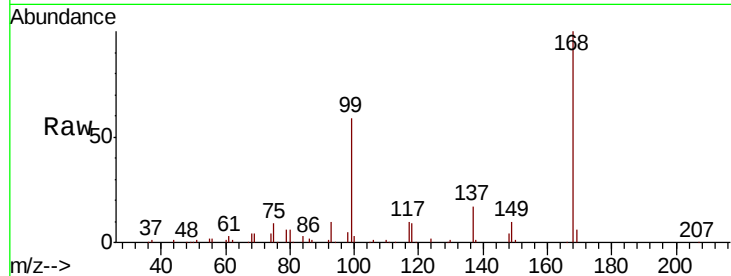

Abundance Ion 167.90 (167.60 to 168.60): VN061077.D (-1732) (-)

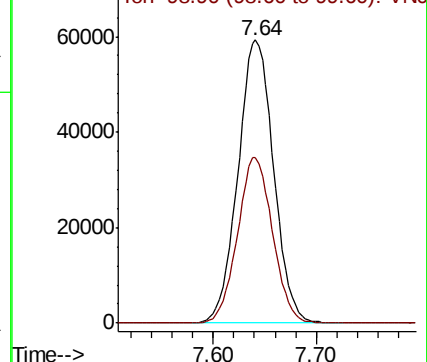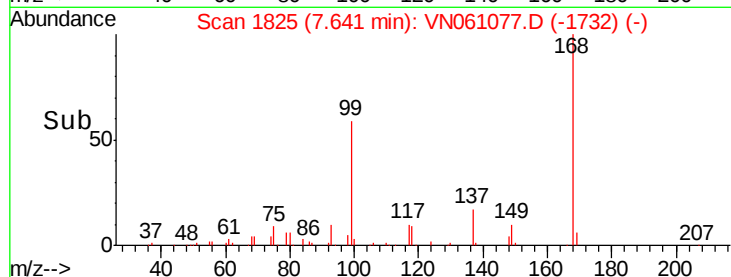

#14

Allyl chloride

Concen: 0.445 ug/l

RT: 4.02 min Scan# 698

Delta R.T. -0.27 min

Lab File: VN061077.D

Acq: 18 Apr 2020 1:59


Tgt Ion: 41 Resp: 1313

Ion Ratio Lower Upper



41 100


39 84.8 56.3 84.5#

76 0.0 27.7 41.5#



Abundance Ion 41.00 (40.70 to 41.70): VN061077.D (-690) (-)

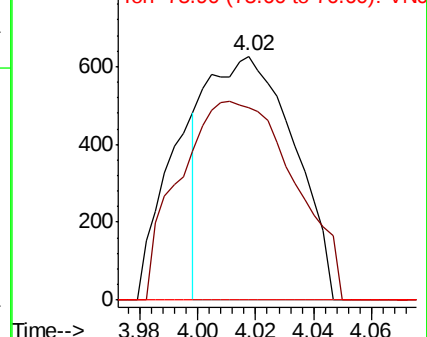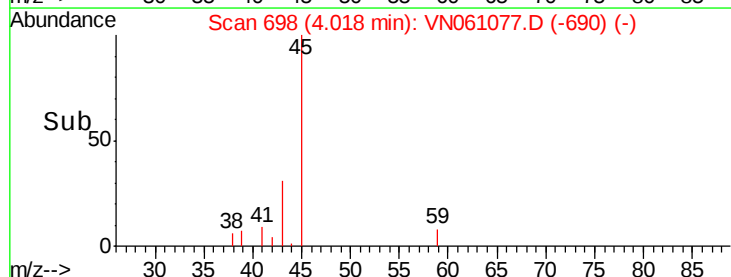

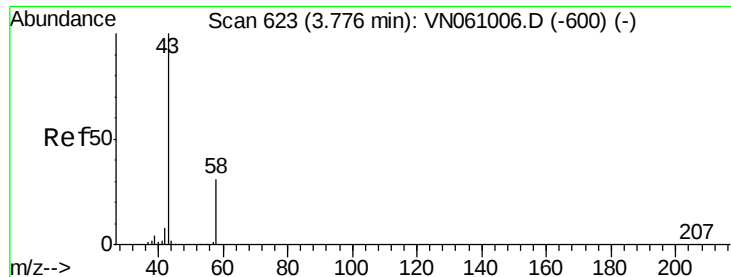

#16

Acetone

Concen: 1.385 ug/l

RT: 3.79 min Scan# 627

Delta R.T. 0.01 min

Lab File: VN061077.D

Acq: 18 Apr 2020 1:59

Instrument :

MSVOA_N

ClientSampleId :


BP-MW202S-20200414

Tot Ion: 43 Resp: 1110




Ion Ratio Lower Upper

43 100

58 0.0 24.6 37.0#



Abundance Ion 43.00 (42.70 to 43.70): VN061006.D (-600) (-)

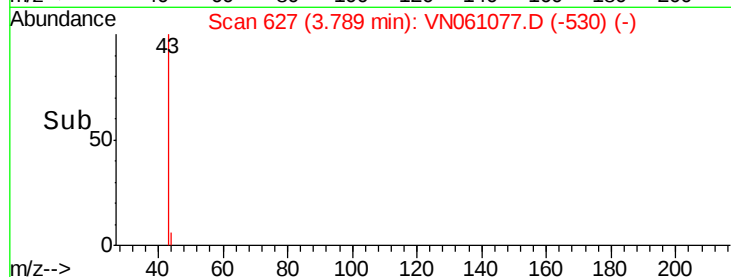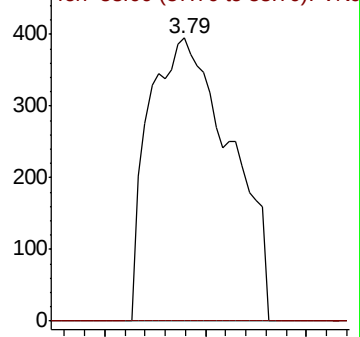

#18

Methyl Acetate

Concen: 1.489 ug/l

RT: 4.01 min Scan# 697

Delta R.T. -0.27 min

Lab File: VN061077.D


Acq: 18 Apr 2020 1:59

Tgt Ion: 43 Resp: 3744



Ion Ratio Lower Upper


43 100

74 0.0 17.4 26.0#



Abundance Ion 43.00 (42.70 to 43.70): VN061006.D (-759) (-)

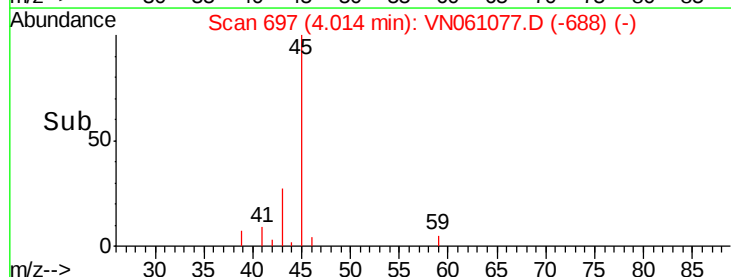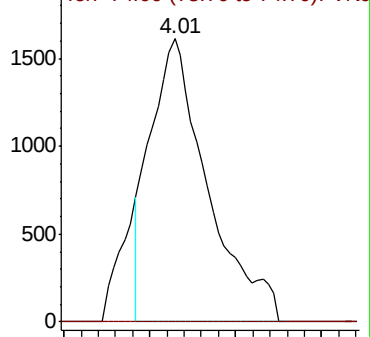







#31
Cyclohexane
Concen: 0.949 ug/l
RT: 7.64 min Scan# 1826
Delta R.T. 0.02 min
Lab File: VN061077.D
Acq: 18 Apr 2020 1:59

Instrument :
MSVOA_N
ClientSampleId :
BP-MW202S-20200414

Tot Ion: 56 Resp: 3220
Ion Ratio Lower Upper
56 100
69 166.9 25.6 38.4#
84 130.3 63.4 95.2#

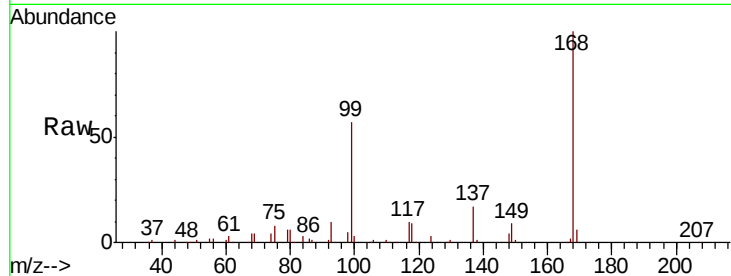


Abundance Ion 56.00 (55.70 to 56.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 84.00 (83.70 to 84.70): VN0

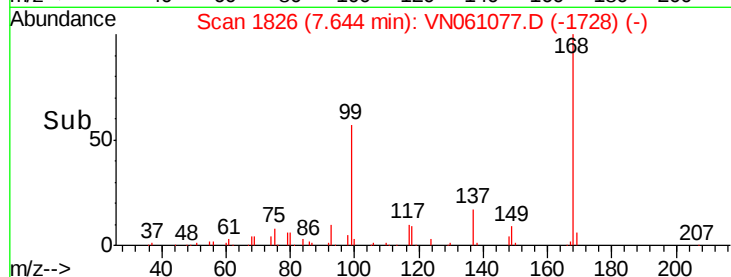
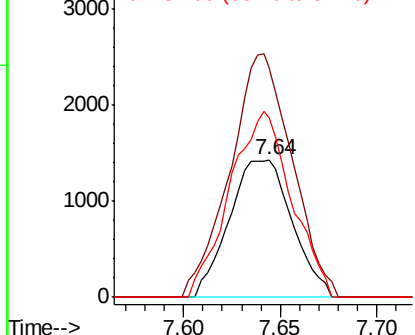



#33
1,2-Dichloroethane-d4
Concen: 53.699 ug/l
RT: 8.00 min Scan# 1937
Delta R.T. 0.00 min
Lab File: VN061077.D
Acq: 18 Apr 2020 1:59

Tgt Ion: 65 Resp: 97804
Ion Ratio Lower Upper
65 100
67 53.8 0.0 107.0



Abundance Ion 64.90 (64.60 to 65.60): VN0
Ion 66.90 (66.60 to 67.60): VN0

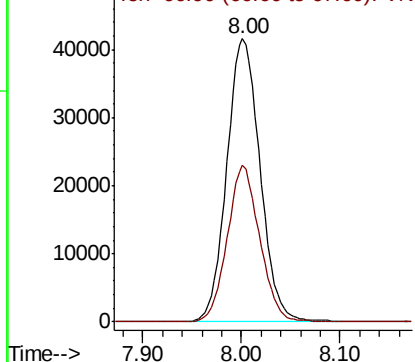



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.56 min Scan# 2112

Delta R.T. 0.00 min

Lab File: VN061077.D

Acq: 18 Apr 2020 1:59

Instrument :

MSVOA_N

ClientSampleId :

BP-MW202S-20200414


Tot Ion:114 Resp: 243263

Ion Ratio Lower Upper

114 100

63 22.3 0.0 46.2




88 16.9 0.0 33.4



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

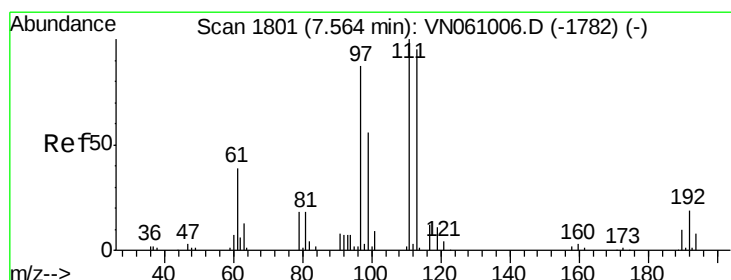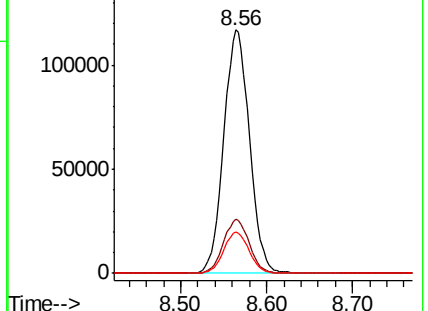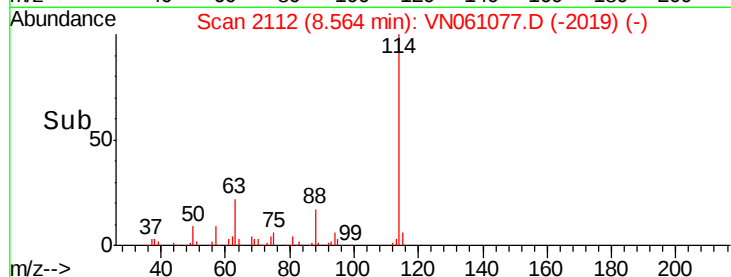

#35

Dibromofluoromethane

Concen: 51.782 ug/l

RT: 7.56 min Scan# 1801

Delta R.T. 0.00 min

Lab File: VN061077.D

Acq: 18 Apr 2020 1:59


Tgt Ion:113 Resp: 73563

Ion Ratio Lower Upper

113 100

111 103.0 83.4 125.2



192 19.4 15.5 23.3




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



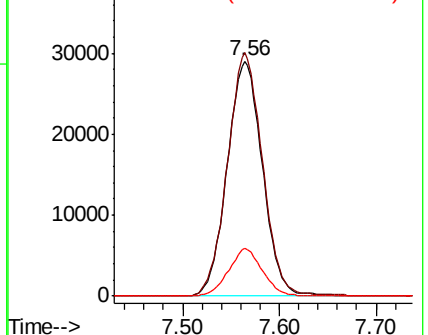





#36
 1,1-Dichloropropene
 Concen: 4.727 ug/l
 RT: 7.64 min Scan# 1824
 Delta R.T. -0.13 min
 Lab File: VN061077.D
 Acq: 18 Apr 2020 1:59




Instrument :
 MSVOA_N
 ClientSampleId :
 BP-MW202S-20200414


Tot Ion	Ratio	Lower	Upper
75	100		
110	7.7	16.8	50.3#
77	0.0	24.7	37.1#

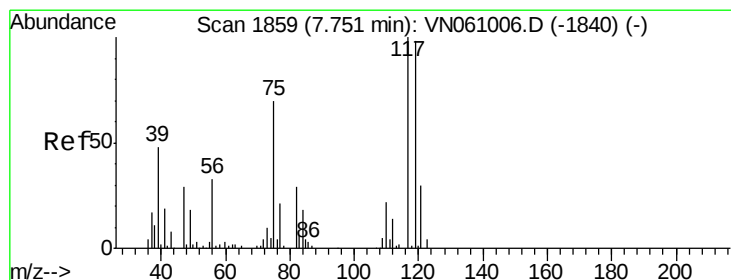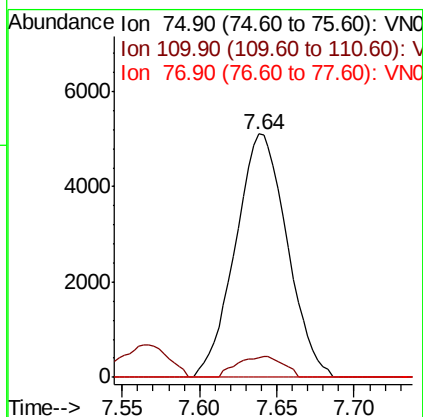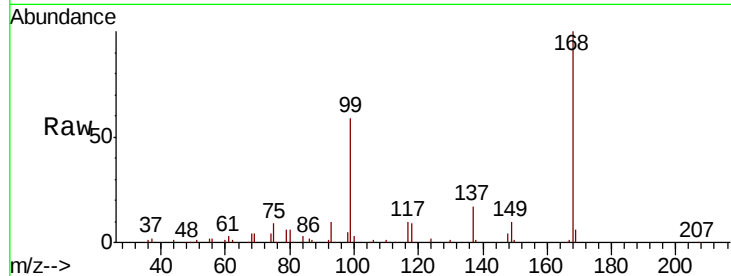

#38
 Carbon Tetrachloride
 Concen: 6.602 ug/l
 RT: 7.64 min Scan# 1825
 Delta R.T. -0.11 min
 Lab File: VN061077.D
 Acq: 18 Apr 2020 1:59

Tgt Ion	Ratio	Lower	Upper
117	100		
119	4.3	78.1	117.1#
121	0.0	24.0	36.0#

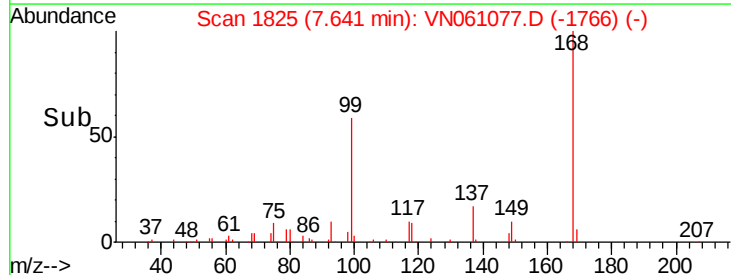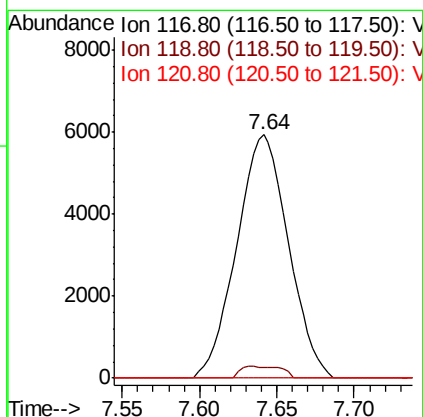



#50

Toluene-d8

Concen: 56.304 ug/l

RT: 10.08 min Scan# 2582

Delta R.T. 0.00 min

Lab File: VN061077.D

Acq: 18 Apr 2020 1:59

Instrument :

MSVOA_N

ClientSampleId :





BP-MW202S-20200414

Tot Ion: 98 Resp: 302254

Ion Ratio Lower Upper

98 100

100 64.6 51.9 77.9

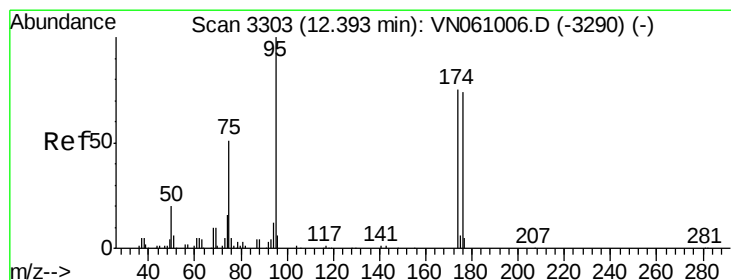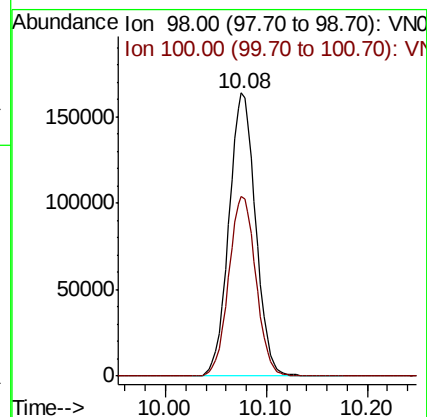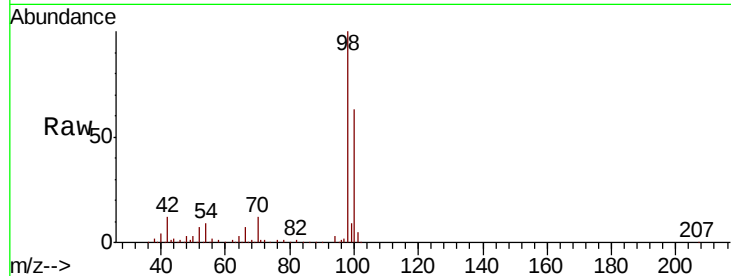

#62

4-Bromofluorobenzene

Concen: 52.646 ug/l

RT: 12.39 min Scan# 3303

Delta R.T. 0.00 min

Lab File: VN061077.D

Acq: 18 Apr 2020 1:59




Tgt Ion: 95 Resp: 110765


Ion Ratio Lower Upper

95 100

174 77.3 0.0 151.2

176 74.1 0.0 148.2



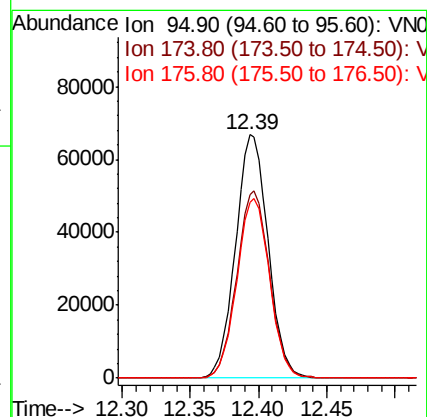
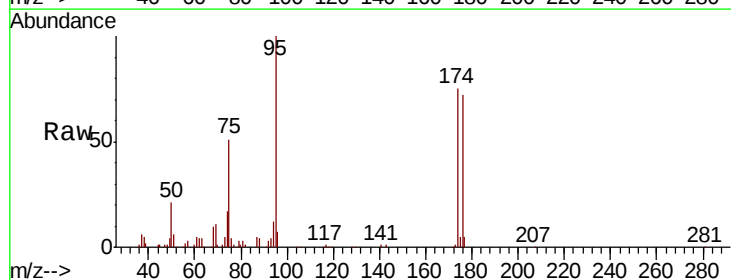




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.40 min Scan# 2993
Delta R.T. 0.00 min
Lab File: VN061077.D
Acq: 18 Apr 2020 1:59




Instrument :
MSVOA_N
ClientSampleId :
BP-MW202S-20200414


Tot Ion:117 Resp: 228978
Ion Ratio Lower Upper
117 100
82 58.5 47.1 70.7
119 31.8 25.7 38.5

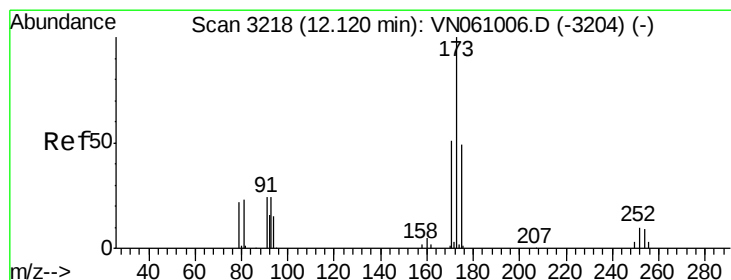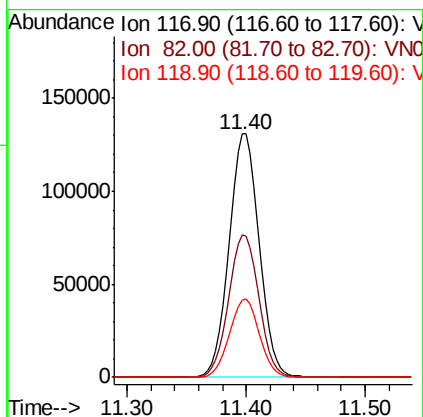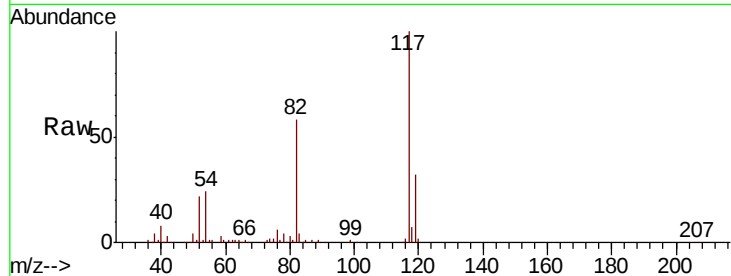

#71
Bromoform
Concen: 0.302 ug/l
RT: 12.40 min Scan# 3305
Delta R.T. 0.28 min
Lab File: VN061077.D
Acq: 18 Apr 2020 1:59

Tgt Ion:173 Resp: 381
Ion Ratio Lower Upper
173 100
175 1380.3 24.5 73.5#
254 0.0 0.0 0.0

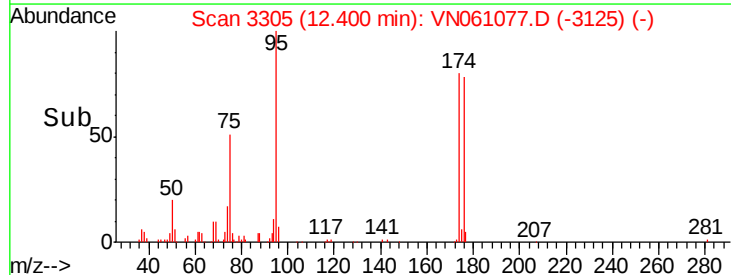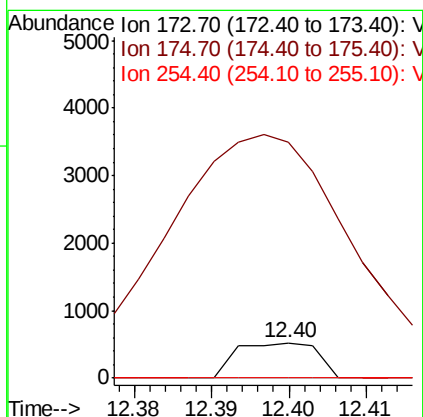



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.34 min Scan# 3597

Delta R.T. 0.00 min

Lab File: VN061077.D

Acq: 18 Apr 2020 1:59

Instrument :

MSVOA_N

ClientSampleId :

BP-MW202S-20200414


Tot Ion:152 Resp: 101148

Ion Ratio Lower Upper

152 100

115 59.6 30.8 92.4




150 154.9 0.0 349.0



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

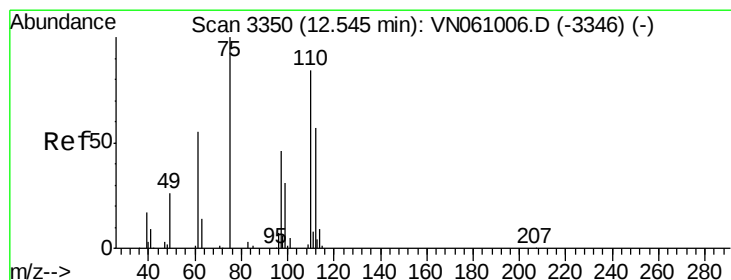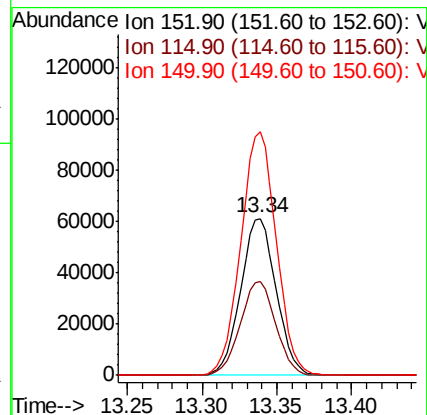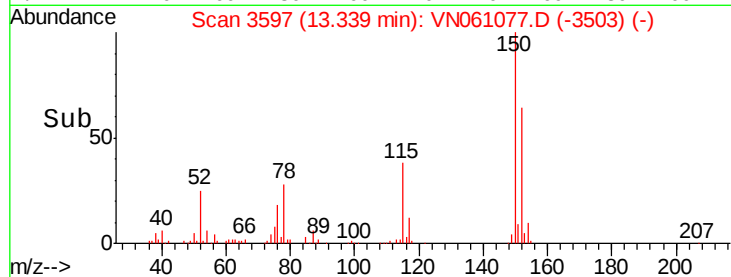

#76

1,2,3-Trichloropropane

Concen: 25.598 ug/l

RT: 12.39 min Scan# 3303

Delta R.T. -0.15 min

Lab File: VN061077.D


Acq: 18 Apr 2020 1:59

Tgt Ion: 75 Resp: 56951

Ion Ratio Lower Upper



75 100


77 1.1 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): V

Ion 77.00 (76.70 to 77.70): V

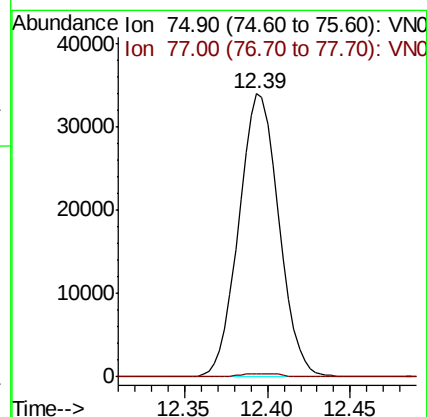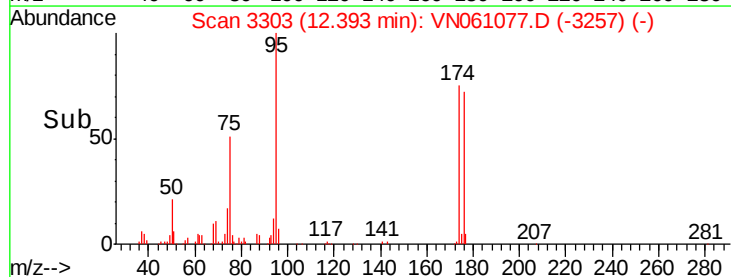

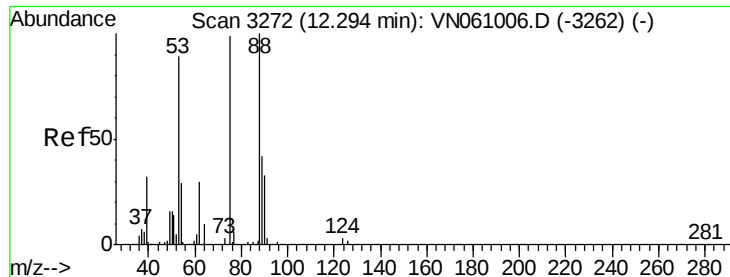

#81

trans-1,4-Dichloro-2-butene

Concen: 63.139 ug/l

RT: 12.39 min Scan# 3303

Delta R.T. 0.10 min

Lab File: VN061077.D

Acq: 18 Apr 2020 1:59

Instrument :

MSVOA_N

ClientSampleId :

BP-MW202S-20200414


Tot Ion: 75 Resp: 56951

Ion Ratio Lower Upper

75 100

53 0.0 74.7 112.1#

89 0.0 34.6 52.0#

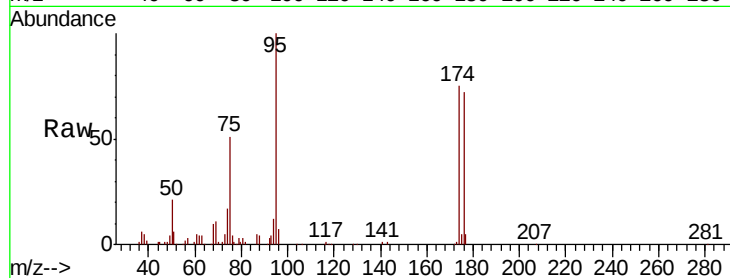

Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 53.00 (52.70 to 53.70): VN0

Ion 88.90 (88.60 to 89.60): VN0

