
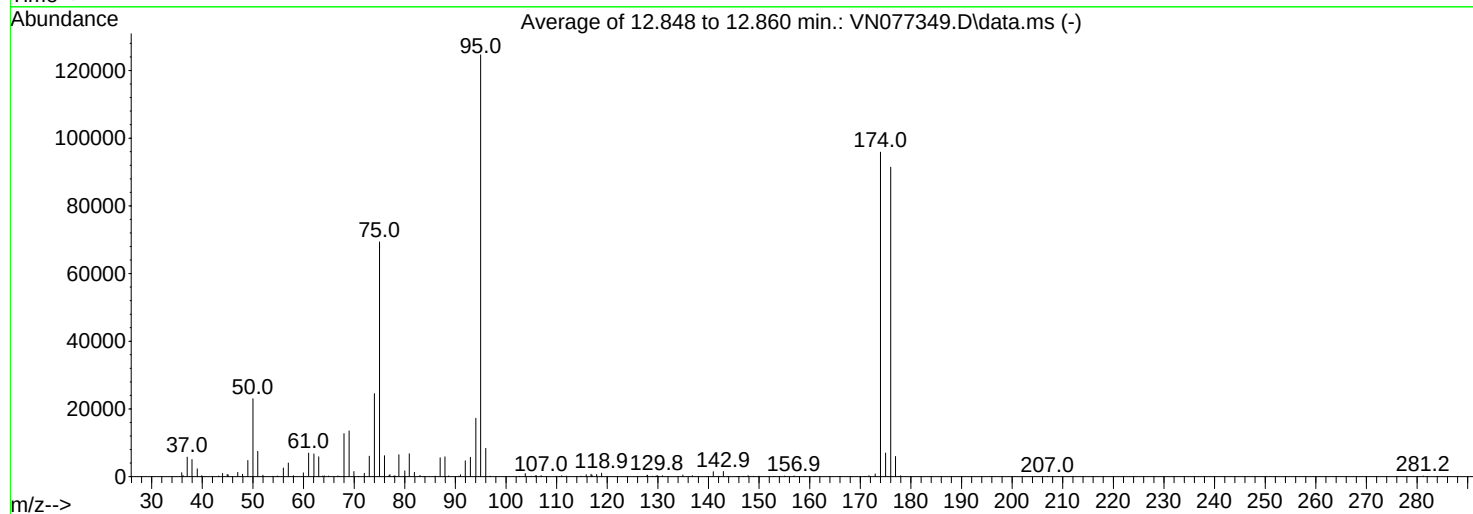


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041723\
Data File : VN077349.D
Acq On : 17 Apr 2023 10:14
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N040523W.M
Title : SW846 8260
Last Update : Thu Apr 06 08:27:03 2023

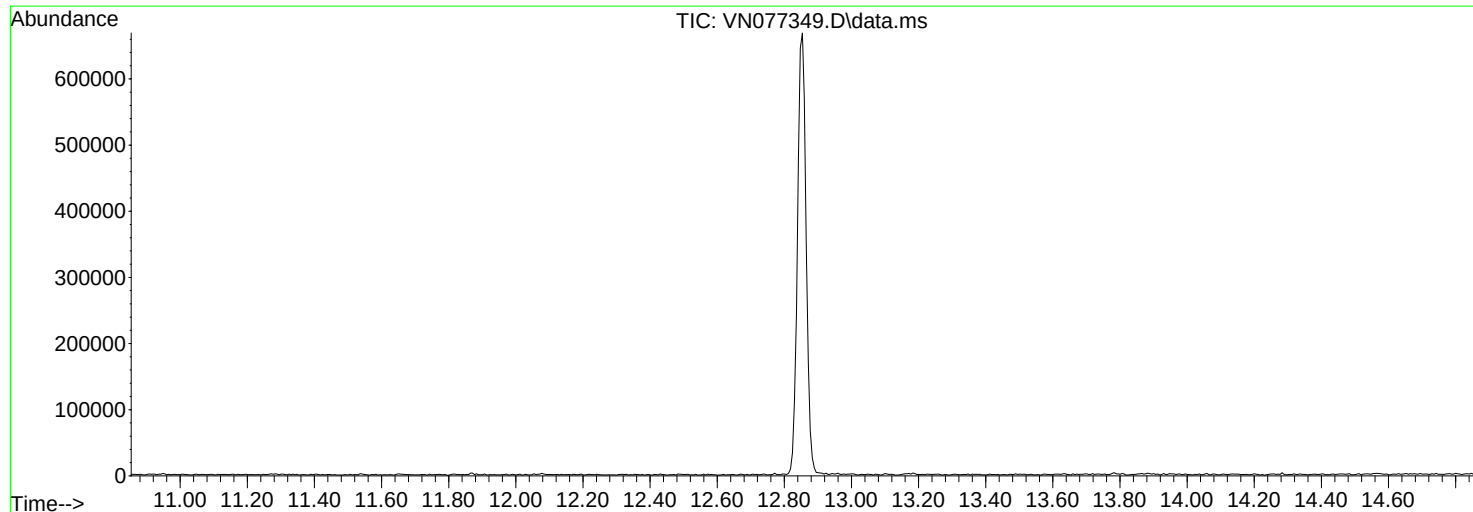

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1846

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.5	23043	PASS
75	95	30	60	55.7	69365	PASS
95	95	100	100	100.0	124624	PASS
96	95	5	9	6.7	8375	PASS
173	174	0.00	2	0.9	820	PASS
174	95	50	100	76.9	95893	PASS
175	174	5	9	7.3	7015	PASS
176	174	95	101	95.3	91419	PASS
177	176	5	9	6.5	5964	PASS

Average of 12.848 to 12.860 min.: VN077349.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	1172	45.90	68	56.00	2536	67.00	121
36.20	348	47.00	1302	57.00	4029	68.00	1272
37.00	5773	47.95	703	58.00	306	69.00	1354
37.95	5065	49.00	4799	59.95	1152	69.95	152
39.00	2302	50.00	23043	61.00	6952	70.90	75
39.90	265	50.95	7481	62.05	6700	72.00	989
40.60	63	51.95	429	63.00	5847	73.00	6043
43.25	180	53.80	85	63.80	211	74.00	24528
44.00	940	54.60	69	64.10	255	75.00	69365
44.90	645	54.85	205	64.95	186	76.00	6200
45.10	528	55.10	71	66.75	199	76.90	420

Average of 12.848 to 12.860 min.: VN077349.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.05	577	87.95	5882	103.80	901	116.80	696
77.80	144	88.70	231	104.95	156	117.00	455
78.05	275	90.70	162	105.80	250	117.90	637
78.85	6464	91.00	568	105.95	352	118.90	1049
80.00	1710	91.95	4697	106.95	353	123.90	61
80.90	6754	92.95	5703	109.90	85	127.80	229
81.90	1263	94.05	17240	110.60	55	127.95	430
83.00	367	95.00	124624	111.00	296	129.00	148
83.80	94	96.00	8375	111.90	157	129.60	156
86.00	160	96.85	146	114.80	150	129.85	394
87.00	5564	102.70	77	115.85	565	130.10	113

Average of 12.848 to 12.860 min.: VN077349.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
130.90	268	147.85	306	172.95	820		
134.95	494	148.90	91	174.00	95893		
136.80	297	149.95	137	175.00	7015		
139.60	73	152.80	68	176.00	91419		
140.95	1458	155.05	169	176.95	5964		
142.05	107	156.90	260	177.95	221		
142.95	1519	158.90	85	207.00	70		
143.80	69	161.00	55	281.20	207		
145.70	69	168.40	55				
146.00	80	170.90	60				
147.00	119	171.70	266				