
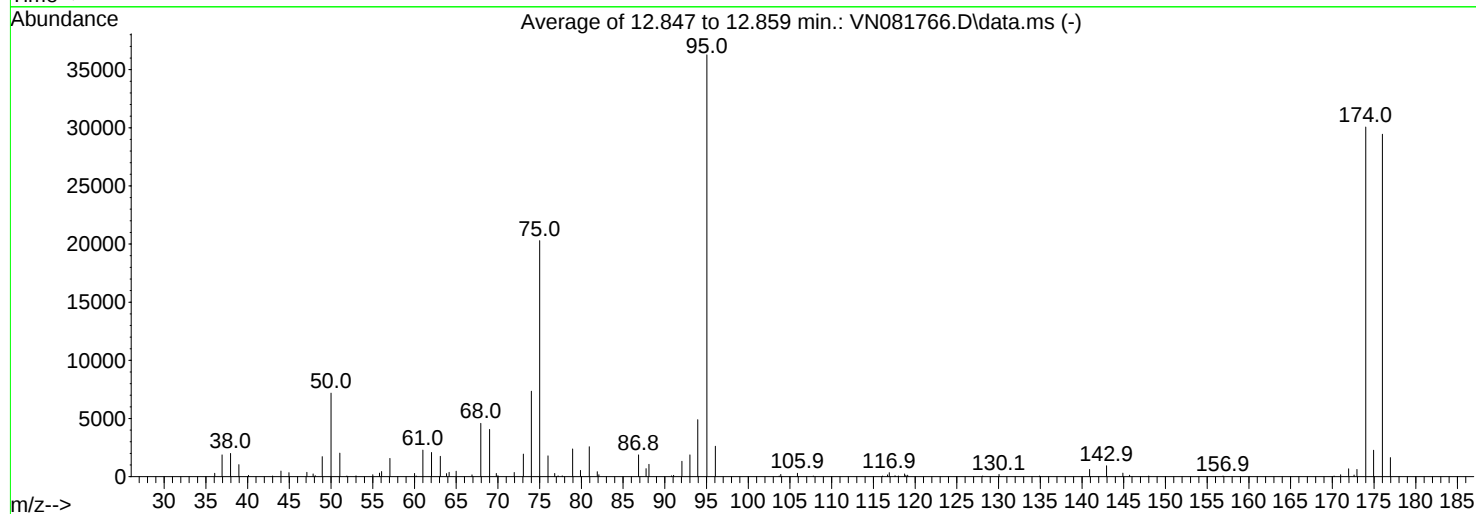


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041724\
Data File : VN081766.D
Acq On : 17 Apr 2024 10:49
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N041024W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Apr 11 09:25:01 2024

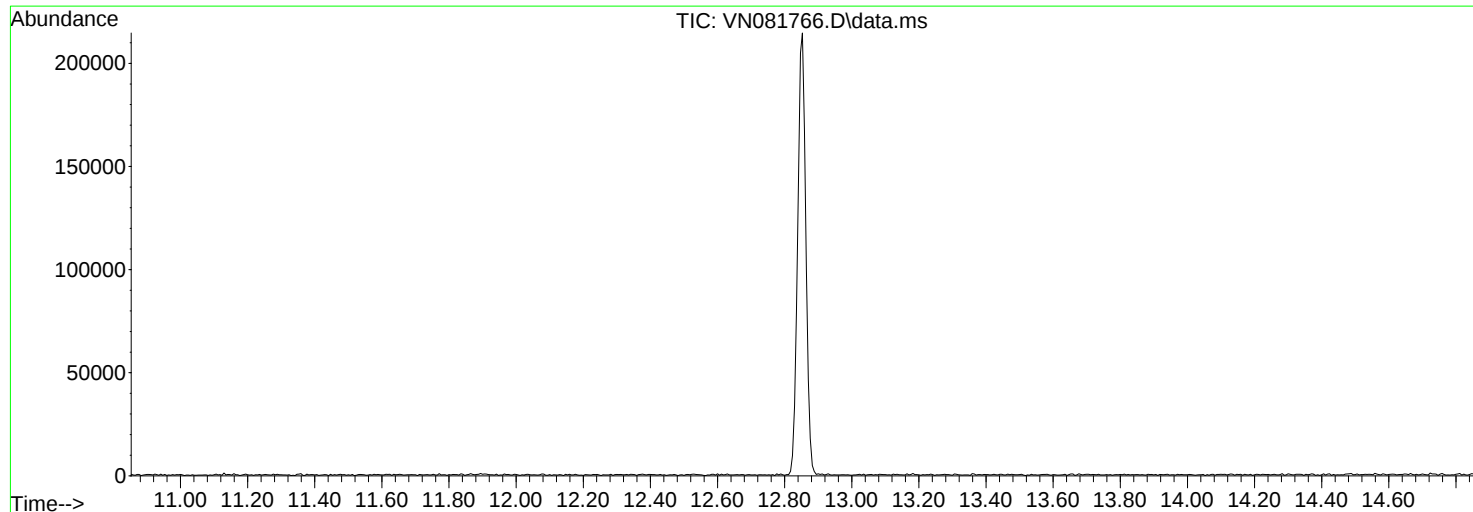

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	7176	PASS
75	95	30	60	55.9	20293	PASS
95	95	100	100	100.0	36272	PASS
96	95	5	9	7.2	2619	PASS
173	174	0.00	2	2.0	615	FAIL*
174	95	50	100	82.9	30067	PASS
175	174	5	9	7.5	2268	PASS
176	174	95	101	97.9	29445	PASS
177	176	5	9	5.6	1645	PASS