
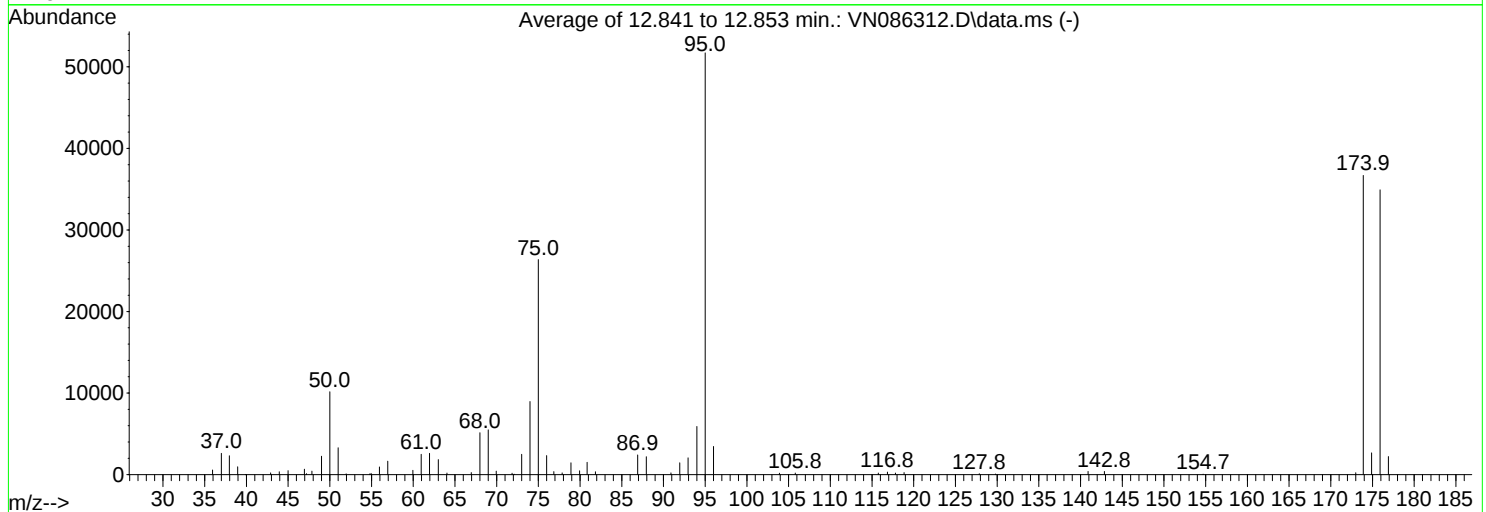


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041725\
Data File : VN086312.D
Acq On : 17 Apr 2025 08:56
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Title : SW846 8260
Last Update : Wed Apr 16 04:19:23 2025

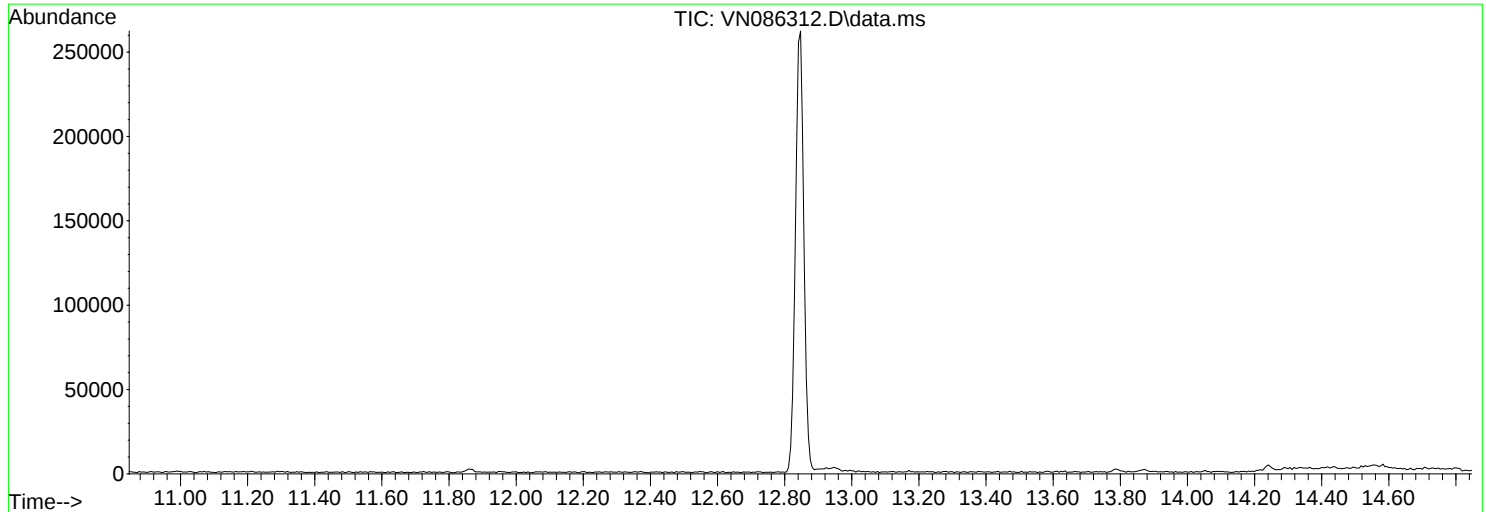

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	10167	PASS
75	95	30	60	51.0	26368	PASS
95	95	100	100	100.0	51715	PASS
96	95	5	9	6.7	3445	PASS
173	174	0.00	2	0.6	230	PASS
174	95	50	100	70.9	36691	PASS
175	174	5	9	7.3	2666	PASS
176	174	95	101	95.2	34923	PASS
177	176	5	9	6.4	2224	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	575	49.00	2249	63.00	1852	76.00	2334
37.00	2617	50.00	10167	64.05	195	76.85	381
37.95	2319	51.00	3307	66.95	246	77.85	21
38.95	969	51.95	105	68.00	5143	78.90	144
39.90	9	54.80	92	69.00	5501	79.95	478
42.90	213	54.95	151	69.95	427	80.85	1504
43.95	361	55.95	945	71.85	185	81.85	346
45.00	497	56.95	1642	72.10	51	86.90	2419
46.95	676	59.95	536	73.00	2488	87.95	2194
47.20	112	60.95	2500	74.00	8960	90.90	215
47.85	431	61.95	2603	75.00	26368	91.95	1447

Average of 12.841 to 12.853 min.: VN086312.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.95	2068	129.80	82				
94.00	5915	140.90	388				
95.00	51715	142.85	393				
96.00	3445	154.70	51				
103.90	168	173.00	230				
105.80	200	173.90	36691				
115.75	196	174.90	2666				
116.85	311	175.90	34923				
117.80	194	176.90	2224				
118.85	256						
127.85	115						

Instrument :

MSVOA_N

ClientSampleId :

BFB