


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN041819\  
 Data File : VN055112.D  
 Acq On : 18 Apr 2019 8:33  
 Operator : JC/SP  
 Sample : BFB  
 Misc : 5.00mL/MSVOA N/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N041519W.M  
 Title : SW846 8260  
 Last Update : Mon Apr 15 12:28:28 2019

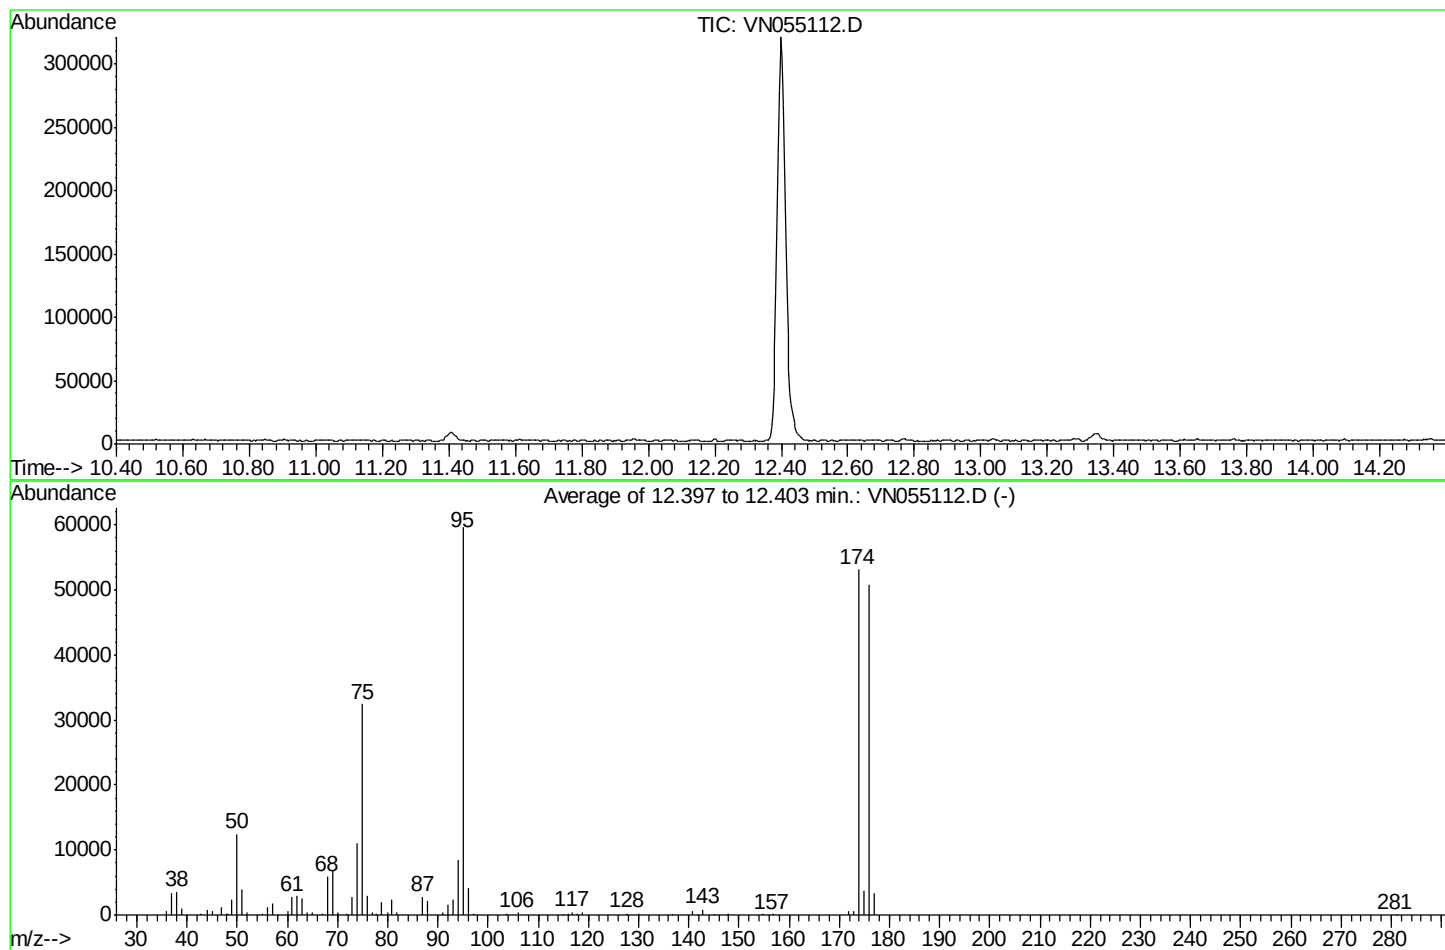

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 20.9      | 12464   | PASS             |
| 75          | 95           | 30           | 60           | 54.5      | 32480   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 59634   | PASS             |
| 96          | 95           | 5            | 9            | 6.8       | 4069    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.2       | 654     | PASS             |
| 174         | 95           | 50           | 100          | 89.0      | 53090   | PASS             |
| 175         | 174          | 5            | 9            | 7.1       | 3790    | PASS             |
| 176         | 174          | 95           | 101          | 95.6      | 50752   | PASS             |
| 177         | 176          | 5            | 9            | 6.5       | 3293    | PASS             |