

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041824\
 Data File : VN081796.D
 Acq On : 18 Apr 2024 18:42
 Operator : JC\MD
 Sample : P2121-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Apr 19 02:11:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041524W.M
 Quant Title : SW846 8260
 QLast Update : Mon Apr 15 15:37:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	263082	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	456356	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	459959	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	212851	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	174588	47.161	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	94.320%		
35) Dibromofluoromethane	8.165	113	141279	46.882	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	93.760%		
50) Toluene-d8	10.565	98	588498	53.010	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	106.020%		
62) 4-Bromofluorobenzene	12.847	95	220086	58.013	ug/l	0.00
Spiked Amount 50.000	Range 64 - 133		Recovery =	116.020%		
Target Compounds						
					Qvalue	
3) Chloromethane	2.353	50	2015	Below Cal	#	43
5) Bromomethane	2.971	94	824	0.334	ug/l #	78
6) Chloroethane	3.118	64	1194	Below Cal	#	63
11) Tert butyl alcohol	5.518	59	192	0.380	ug/l #	1
13) Acrolein	4.171	56	284	0.529	ug/l #	15
16) Acetone	4.430	43	54042	52.450	ug/l	98
18) Methyl Acetate	5.018	43	1270	0.441	ug/l #	67
20) Methylene Chloride	5.265	84	733	Below Cal	#	68
25) 2-Butanone	7.488	43	4573	2.692	ug/l #	75
31) Cyclohexane	8.218	56	6258	1.232	ug/l #	40
36) 1,1-Dichloropropene	8.224	75	22935	5.463	ug/l #	53
38) Carbon Tetrachloride	8.224	117	28741	5.884	ug/l #	15
41) Methacrylonitrile	7.783	41	414	0.221	ug/l #	25
43) Isopropyl Acetate	8.706	43	1302	0.202	ug/l #	52
49) 1,4-Dioxane	9.688	88	79	1.201	ug/l #	1
51) 4-Methyl-2-Pentanone	10.441	43	794	0.222	ug/l #	56
52) Toluene	10.629	92	1954	0.235	ug/l	100
60) Dibromochloromethane	11.570	129	1164	0.309	ug/l	84
68) m/p-Xylenes	12.076	106	2087	0.322	ug/l #	1
71) Bromoform	12.594	173	1850	0.664	ug/l #	61
76) 1,2,3-Trichloropropane	12.847	75	120792	29.659	ug/l #	1
77) Bromobenzene	12.976	156	1422	0.349	ug/l #	1
79) 2-Chlorotoluene	13.047	91	5076	0.440	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.847	75	120792	69.438	ug/l #	13
82) 4-Chlorotoluene	13.206	91	10091	0.885	ug/l	85
84) 1,2,4-Trimethylbenzene	13.482	105	12303	0.935	ug/l	90
85) sec-Butylbenzene	13.588	105	8268	0.519	ug/l #	67
86) p-Isopropyltoluene	13.735	119	9197	0.704	ug/l #	66
87) 1,3-Dichlorobenzene	13.735	146	2102	0.276	ug/l #	51
92) 1,2-Dibromo-3-Chloropr...	14.729	75	257	Below Cal	#	2
95) Naphthalene	15.635	128	10699	0.864	ug/l #	19


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041824\
Data File : VN081796.D
Acq On : 18 Apr 2024 18:42
Operator : JC\MD
Sample : P2121-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Apr 19 02:11:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041524W.M
Quant Title : SW846 8260
QLast Update : Mon Apr 15 15:37:39 2024
Response via : Initial Calibration

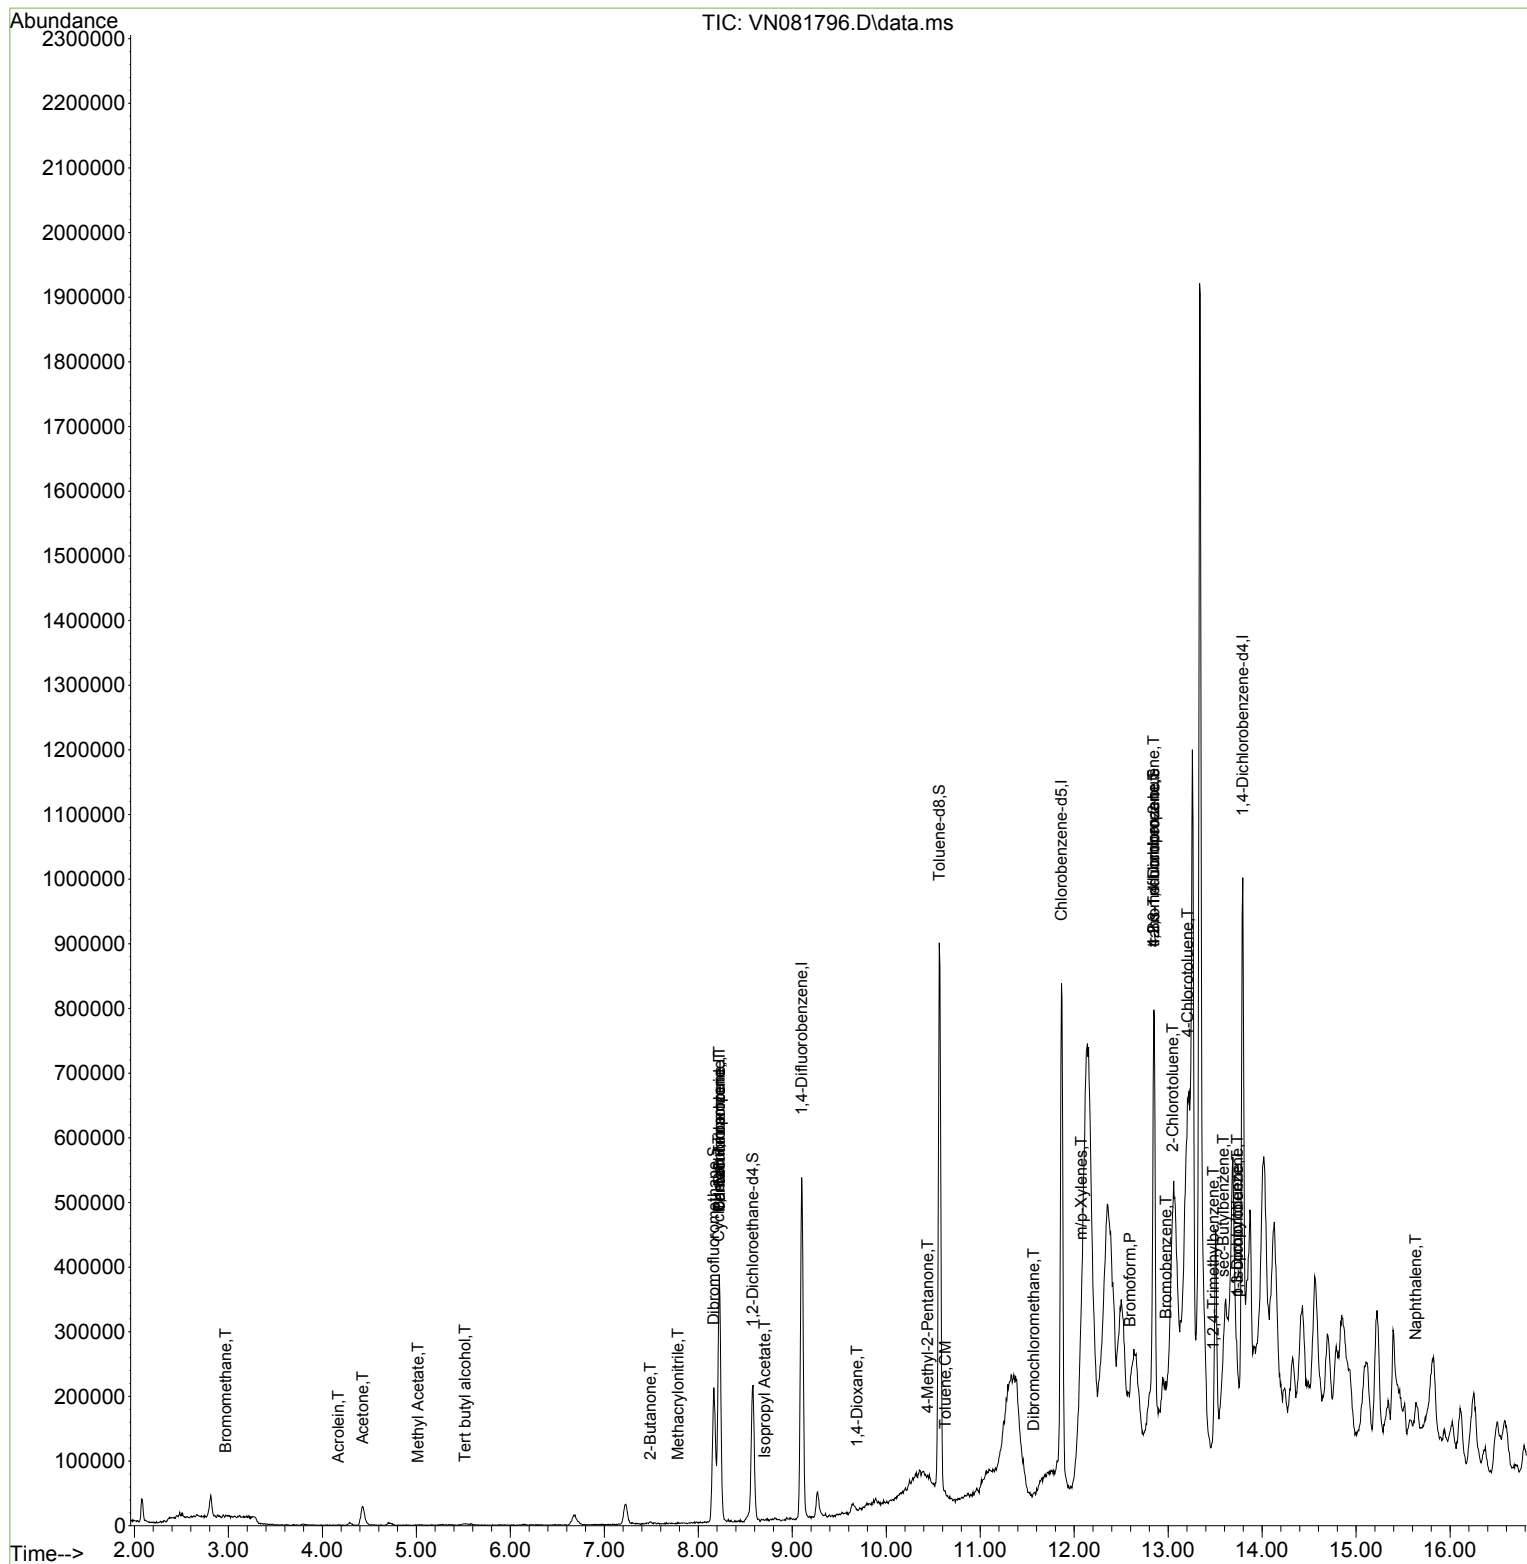



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.000 min

Lab File: VN081796.D

Acq: 18 Apr 2024 18:42

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:168 Resp: 263082

Ion Ratio Lower Upper

168 100

99 63.3 48.2 72.4



#3

Chloromethane

Concen: Below Cal

RT: 2.353 min Scan# 68

Delta R.T. -0.006 min

Lab File: VN081796.D




Acq: 18 Apr 2024 18:42


Tgt Ion: 50 Resp: 2015

Ion Ratio Lower Upper

50 100

52 0.0 25.5 38.3#




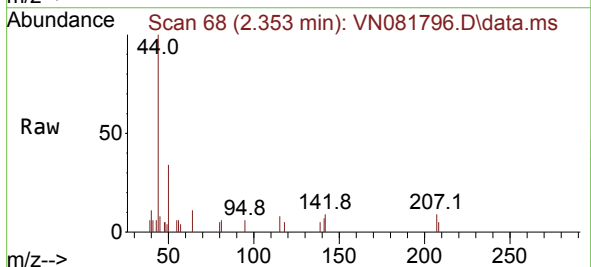




#5
Bromomethane
Concen: 0.334 ug/l
RT: 2.971 min Scan# 11
Delta R.T. 0.023 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 94 Resp: 824
Ion Ratio Lower Upper
94 100
96 72.5 74.8 112.2#



#6
Chloroethane
Concen: Below Cal
RT: 3.118 min Scan# 198
Delta R.T. -0.006 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42

Tgt Ion: 64 Resp: 1194
Ion Ratio Lower Upper
64 100
66 51.0 24.7 37.1#





#11

Tert butyl alcohol

Concen: 0.380 ug/l

RT: 5.518 min Scan# 605

Delta R.T. 0.006 min


Lab File: VN081796.D

Acq: 18 Apr 2024 18:42

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 59 Resp: 192

Ion Ratio Lower Upper

59 100

57 190.6 8.9 13.3#



#13

Acrolein

Concen: 0.529 ug/l

RT: 4.171 min Scan# 377

Delta R.T. -0.006 min

Lab File: VN081796.D




Acq: 18 Apr 2024 18:42


Tgt Ion: 56 Resp: 284

Ion Ratio Lower Upper

56 100

55 0.0 55.8 83.8#









#16
Acetone
Concen: 52.450 ug/l
RT: 4.430 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 54042
Ion Ratio Lower Upper
43 100
58 32.6 25.2 37.8



#18
Methyl Acetate
Concen: 0.441 ug/l
RT: 5.018 min Scan# 521
Delta R.T. -0.006 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42


Tgt Ion: 43 Resp: 1270
Ion Ratio Lower Upper
43 100
74 10.5 22.2 33.2#

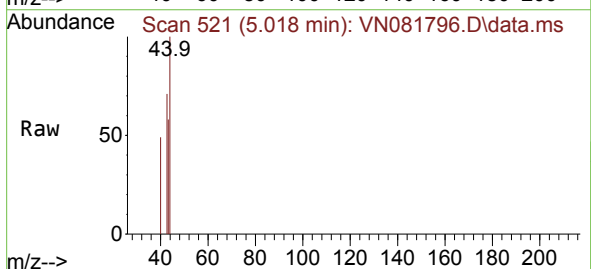






#20
Methylene Chloride
Concen: Below Cal
RT: 5.265 min Scan# 51
Delta R.T. -0.012 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 84	Resp: 733
Ion Ratio	Lower Upper
84 100	
49 68.8	84.9 127.3#
51 0.0	27.0 40.6#
86 55.9	52.3 78.5

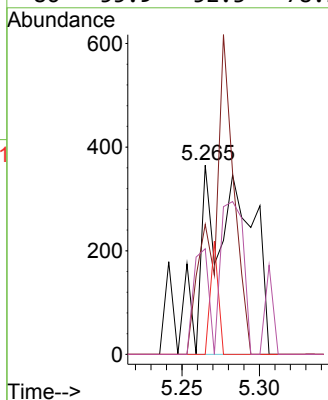

#25
2-Butanone
Concen: 2.692 ug/l
RT: 7.488 min Scan# 941
Delta R.T. 0.005 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42


Tgt Ion: 43	Resp: 4573
Ion Ratio	Lower Upper
43 100	
72 17.8	25.3 37.9#

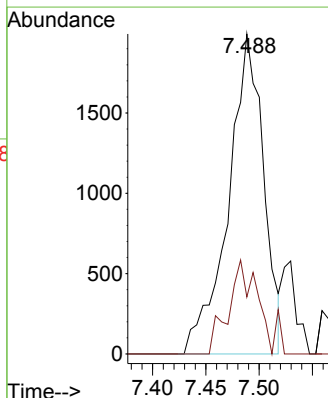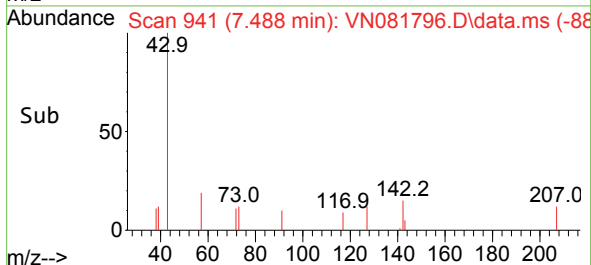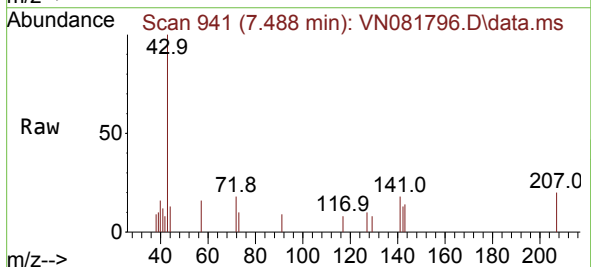






#31
Cyclohexane
Concen: 1.232 ug/l
RT: 8.218 min Scan# 1065
Delta R.T. -0.041 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 6258
Ion Ratio Lower Upper
56 100
69 158.8 24.4 36.6#
84 91.6 77.0 115.4



#33
1,2-Dichloroethane-d4
Concen: 47.161 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42

Tgt Ion: 65 Resp: 174588
Ion Ratio Lower Upper
65 100
67 51.3 0.0 103.0

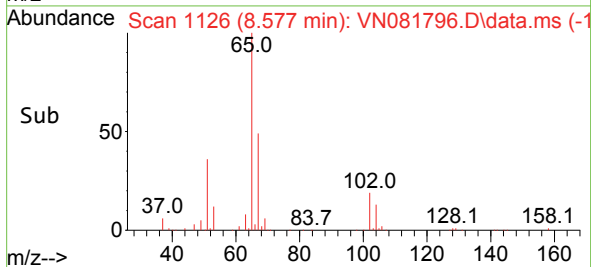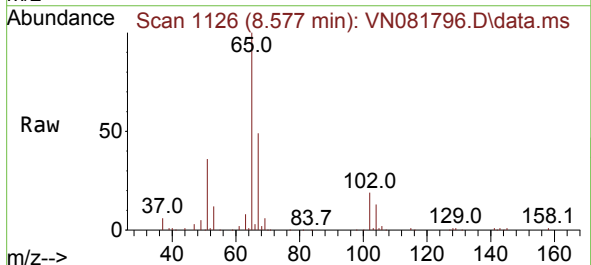



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. 0.000 min


Lab File: VN081796.D

Acq: 18 Apr 2024 18:42

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion:114 Resp: 456356

Ion Ratio Lower Upper

114 100

63 20.7 0.0 41.0

88 15.6 0.0 31.4



#35

Dibromofluoromethane

Concen: 46.882 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN081796.D

Acq: 18 Apr 2024 18:42




Tgt Ion:113 Resp: 141279


Ion Ratio Lower Upper

113 100

111 105.6 83.4 125.2

192 17.8 14.0 21.0





#36

1,1-Dichloropropene

Concen: 5.463 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.153 min


Lab File: VN081796.D

Acq: 18 Apr 2024 18:42

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 75 Resp: 22935

Ion Ratio Lower Upper

75 100

110 11.6 17.8 53.5#

77 1.3 25.0 37.4#



#38

Carbon Tetrachloride

Concen: 5.884 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.141 min

Lab File: VN081796.D

Acq: 18 Apr 2024 18:42




Tgt Ion: 117 Resp: 28741


Ion Ratio Lower Upper

117 100

119 4.0 76.5 114.7#


121 0.0 23.9 35.9#








#41
Methacrylonitrile
Concen: 0.221 ug/l
RT: 7.783 min Scan# 991
Delta R.T. 0.006 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 41	Resp: 414
Ion Ratio	Lower Upper
41 100	
39 15.0	46.6 69.8#
67 0.0	67.3 100.9#
52 0.0	27.3 40.9#

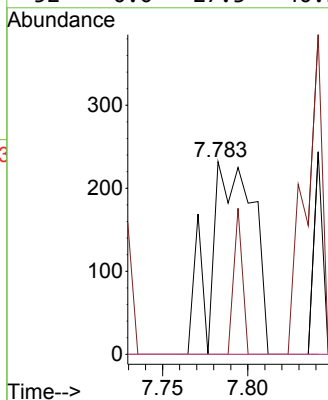

#43
Isopropyl Acetate
Concen: 0.202 ug/l
RT: 8.706 min Scan# 1148
Delta R.T. 0.018 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42

Tgt Ion: 43	Resp: 1302
Ion Ratio	Lower Upper
43 100	
61 0.0	22.8 34.2#
87 0.0	12.0 18.0#

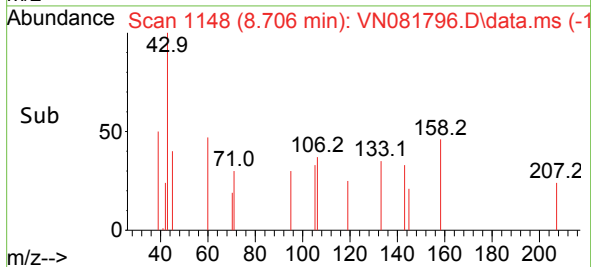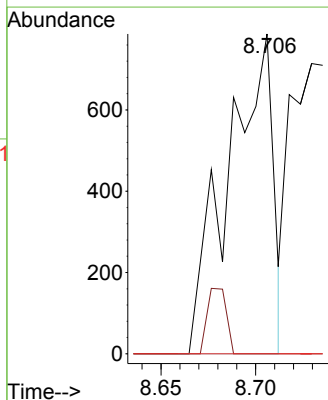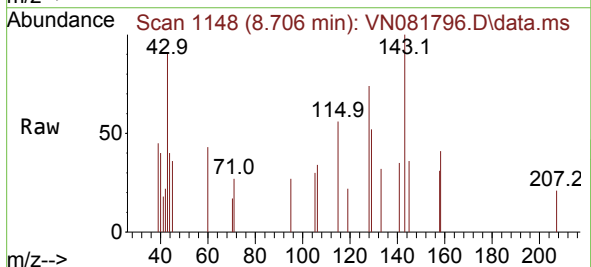



#49

1,4-Dioxane

Concen: 1.201 ug/l

RT: 9.688 min Scan# 11

Delta R.T. -0.012 min


Lab File: VN081796.D

Acq: 18 Apr 2024 18:42

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 88 Resp: 79

Ion Ratio Lower Upper

88 100

43 0.0 19.0 28.6#

58 398.7 50.6 76.0#

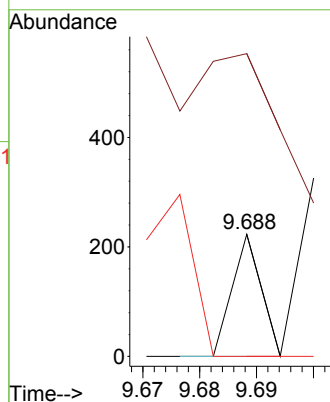

#50

Toluene-d8

Concen: 53.010 ug/l

RT: 10.565 min Scan# 1464

Delta R.T. -0.006 min

Lab File: VN081796.D




Acq: 18 Apr 2024 18:42


Tgt Ion: 98 Resp: 588498

Ion Ratio Lower Upper

98 100

100 65.3 51.8 77.6

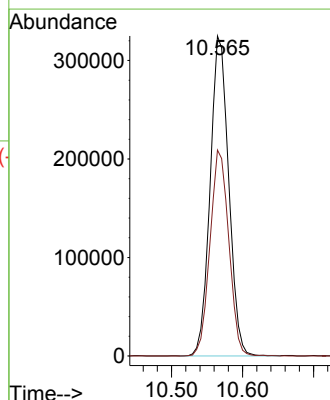



#51

4-Methyl-2-Pentanone

Concen: 0.222 ug/l

RT: 10.441 min Scan# 1444

Delta R.T. -0.006 min

Lab File: VN081796.D

Acq: 18 Apr 2024 18:42

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 43 Resp: 794

Ion Ratio Lower Upper

43 100

58 69.4 33.2 49.8#



#52

Toluene

Concen: 0.235 ug/l

RT: 10.629 min Scan# 1475

Delta R.T. 0.000 min

Lab File: VN081796.D




Acq: 18 Apr 2024 18:42


Tgt Ion: 92 Resp: 1954

Ion Ratio Lower Upper

92 100

91 171.5 136.7 205.1









#60
Dibromochloromethane
Concen: 0.309 ug/l
RT: 11.570 min Scan# 1164
Delta R.T. 0.211 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:129 Resp: 1164
Ion Ratio Lower Upper
129 100
127 63.0 38.3 114.8

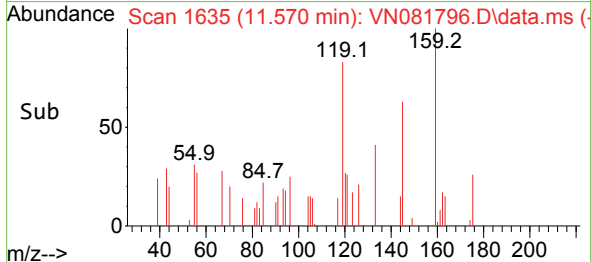

#62
4-Bromofluorobenzene
Concen: 58.013 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.006 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42


Tgt Ion: 95 Resp: 220086
Ion Ratio Lower Upper
95 100
174 74.1 0.0 160.6
176 73.2 0.0 152.8





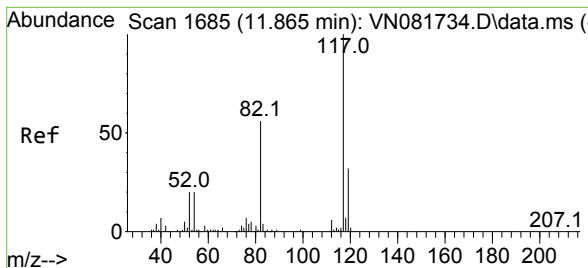


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42

Instrument :
MSVOA_N
ClientSampleId :



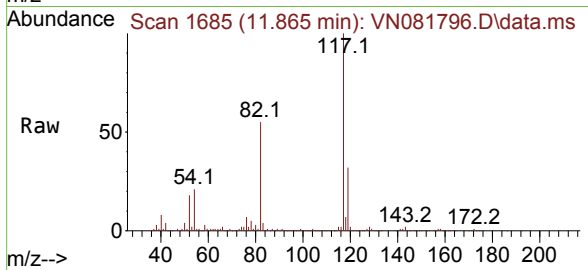



Tgt Ion:117 Resp: 459959
Ion Ratio Lower Upper
117 100
82 54.6 44.6 66.8
119 31.5 25.9 38.9

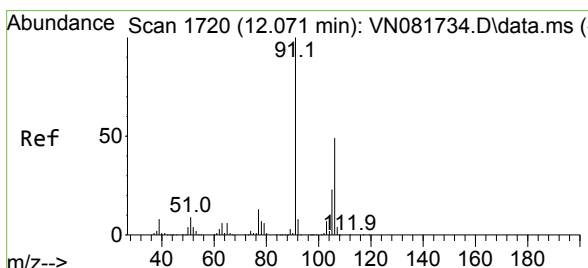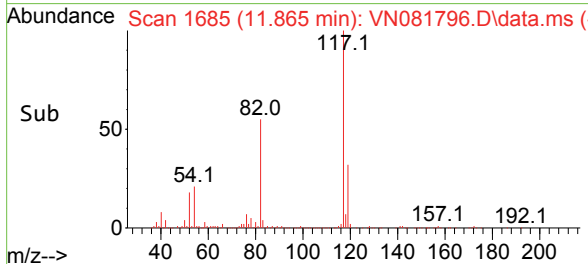

#68
m/p-Xylenes
Concen: 0.322 ug/l
RT: 12.076 min Scan# 1721
Delta R.T. 0.005 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42

Tgt Ion:106 Resp: 2087
Ion Ratio Lower Upper
106 100
91 0.0 159.4 239.0#



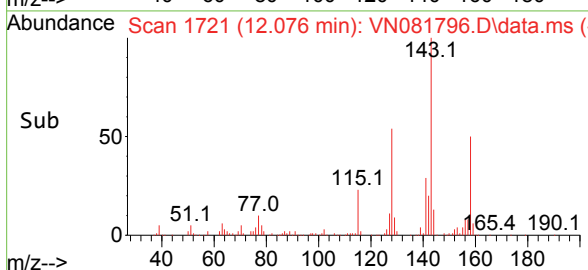
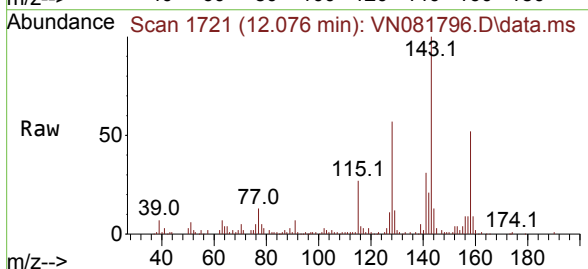




#71
Bromoform
Concen: 0.664 ug/l
RT: 12.594 min Scan# 1809
Delta R.T. 0.012 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:173 Resp: 1850
Ion Ratio Lower Upper
173 100
175 22.6 24.6 74.0#
254 0.0 0.0 0.0



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42

Tgt Ion:152 Resp: 212851
Ion Ratio Lower Upper
152 100
115 64.0 30.4 91.3
150 160.2 0.0 353.2


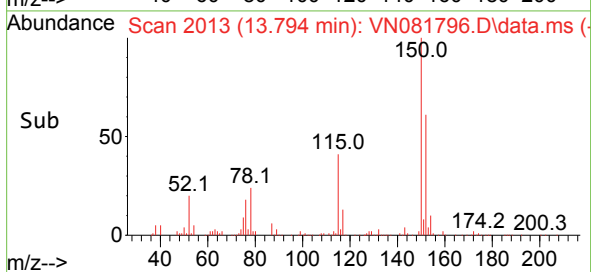




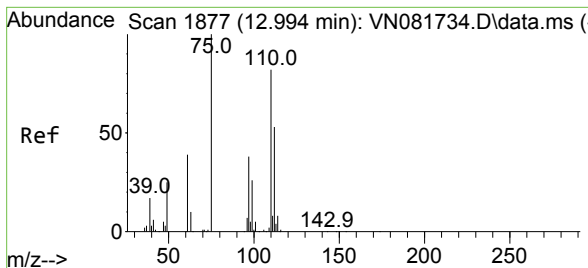

#76
1,2,3-Trichloropropane
Concen: 29.659 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.147 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 120792
Ion Ratio Lower Upper
75 100
77 3.9 90.5 271.3#

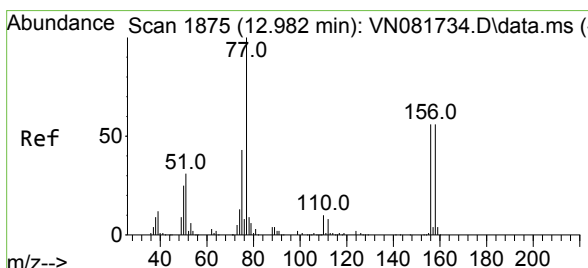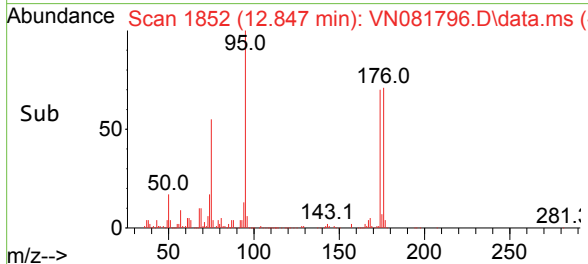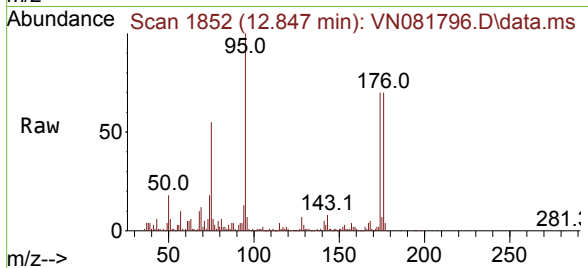

#77
Bromobenzene
Concen: 0.349 ug/l
RT: 12.976 min Scan# 1874
Delta R.T. -0.006 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42

Tgt Ion:156 Resp: 1422
Ion Ratio Lower Upper
156 100
77 42.5 100.2 300.6#
158 0.0 49.1 147.3#


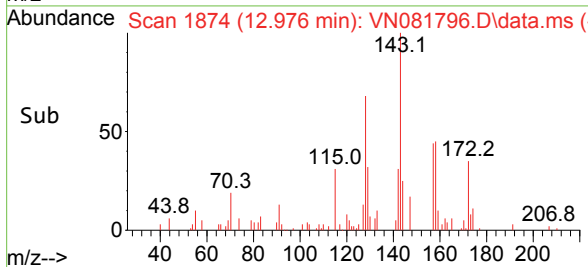

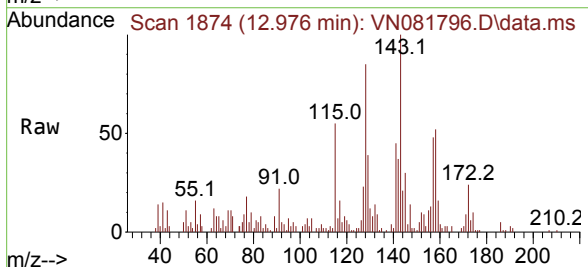


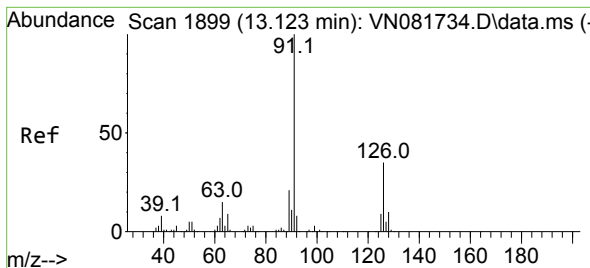

#79
2-Chlorotoluene
Concen: 0.440 ug/l
RT: 13.047 min Scan# 11
Delta R.T. -0.076 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 5076
Ion Ratio Lower Upper
91 100
126 34.0 17.5 52.5

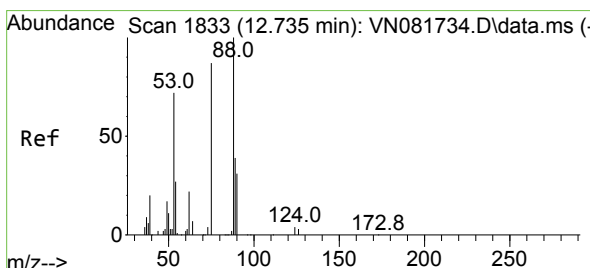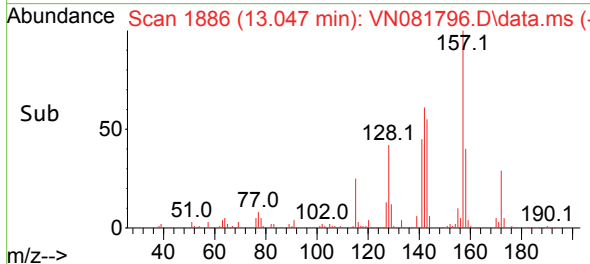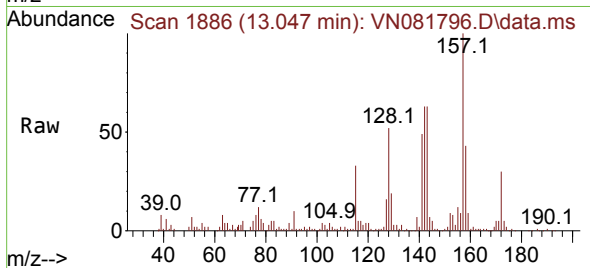

#81
trans-1,4-Dichloro-2-butene
Concen: 69.438 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.112 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42

Tgt Ion: 75 Resp: 120792
Ion Ratio Lower Upper
75 100
53 0.7 72.9 109.3#
89 0.0 39.1 58.7#


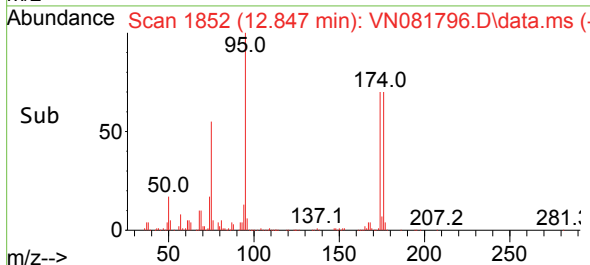

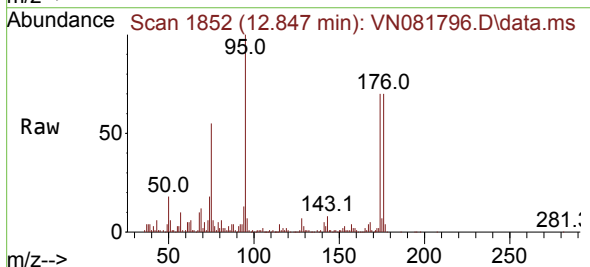




#82
4-Chlorotoluene
Concen: 0.885 ug/l
RT: 13.206 min Scan# 1916
Delta R.T. -0.017 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 10091
Ion Ratio Lower Upper
91 100
126 43.7 17.4 52.3

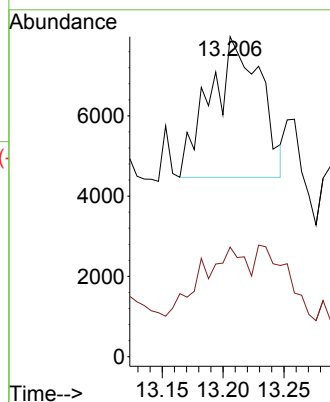

#84
1,2,4-Trimethylbenzene
Concen: 0.935 ug/l
RT: 13.482 min Scan# 1960
Delta R.T. 0.000 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42

Tgt Ion: 105 Resp: 12303
Ion Ratio Lower Upper
105 100
120 52.7 22.9 68.7

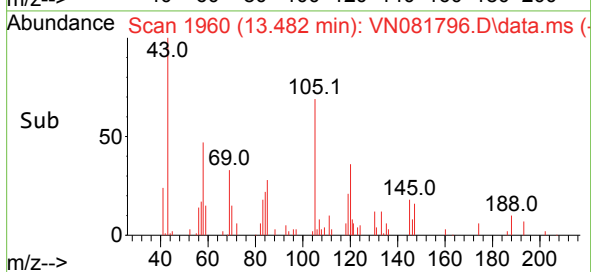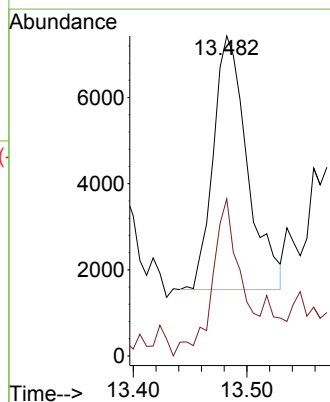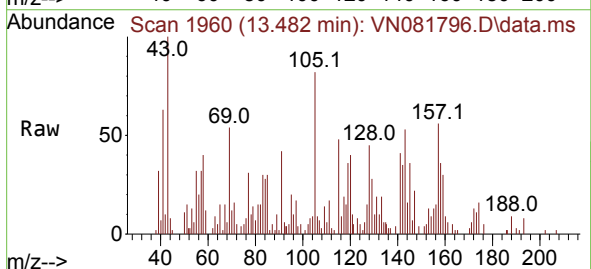

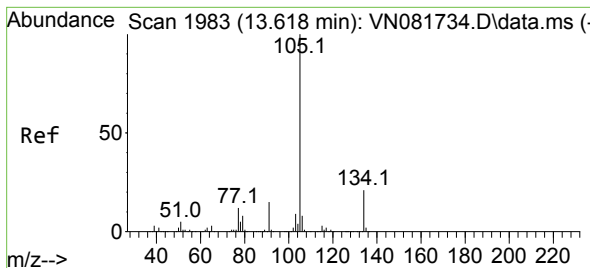

#85

sec-Butylbenzene

Concen: 0.519 ug/l

RT: 13.588 min Scan# 1983

Delta R.T. -0.030 min

Lab File: VN081796.D

Acq: 18 Apr 2024 18:42

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:105 Resp: 8268

Ion Ratio Lower Upper

105 100

134 4.9 10.2 30.4#

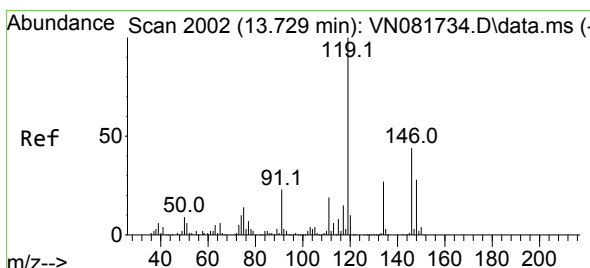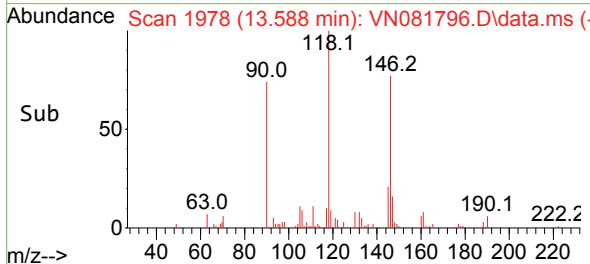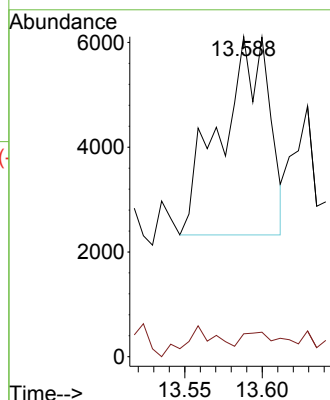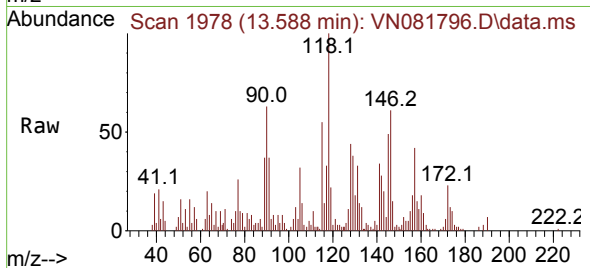

#86

p-Isopropyltoluene

Concen: 0.704 ug/l

RT: 13.735 min Scan# 2003

Delta R.T. 0.006 min

Lab File: VN081796.D

Acq: 18 Apr 2024 18:42




Tgt Ion:119 Resp: 9197


Ion Ratio Lower Upper

119 100

134 15.4 13.2 39.5


91 0.0 11.8 35.3#

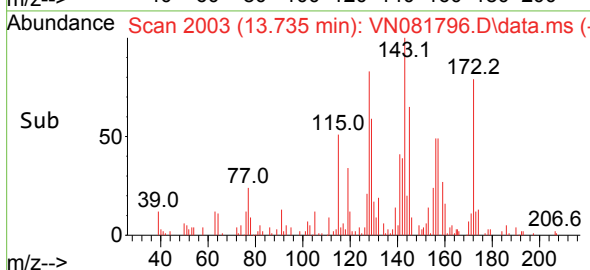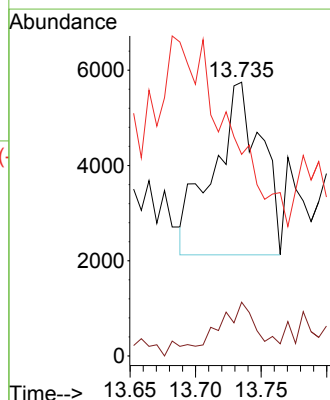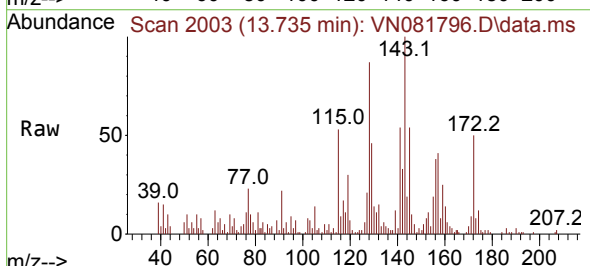



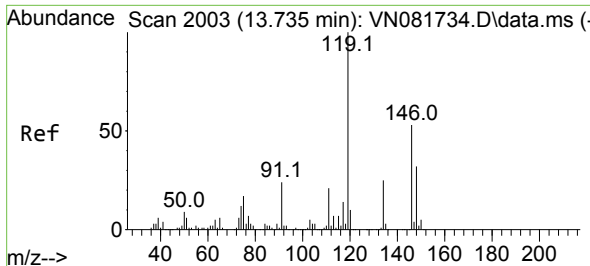


#87
1,3-Dichlorobenzene
Concen: 0.276 ug/l
RT: 13.735 min Scan# 2003
Delta R.T. 0.000 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42


Instrument :
MSVOA_N
ClientSampleId :

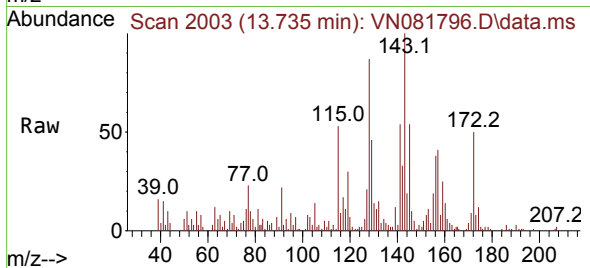



Tgt Ion:146 Resp: 2102
Ion Ratio Lower Upper
146 100
111 23.8 20.8 62.5
148 15.3 32.1 96.3#

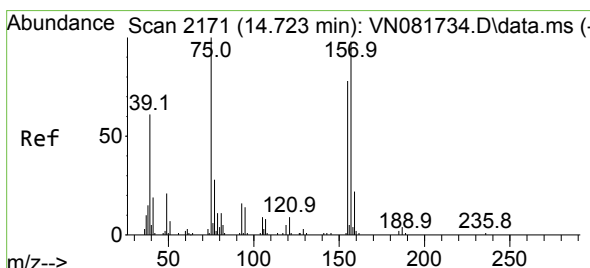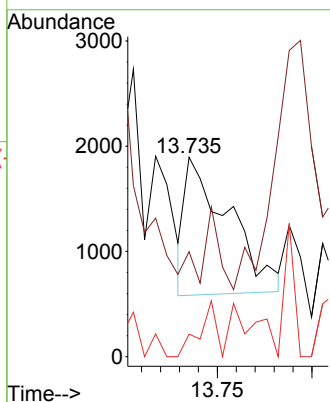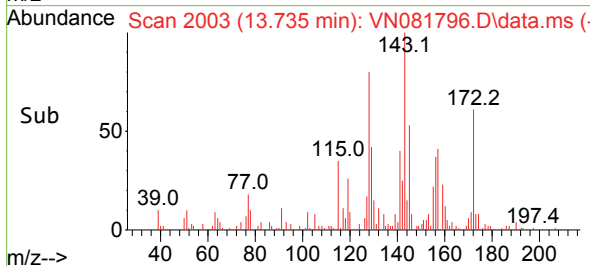


#92
1,2-Dibromo-3-Chloropropane
Concen: Below Cal
RT: 14.729 min Scan# 2172
Delta R.T. 0.006 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42

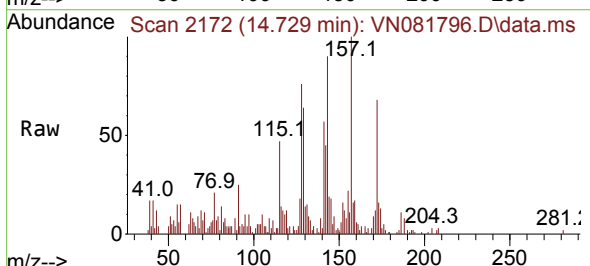


Tgt Ion: 75 Resp: 257
Ion Ratio Lower Upper
75 100
155 0.0 42.6 128.0#
157 0.0 53.0 159.0#

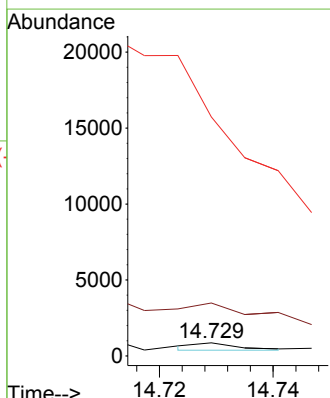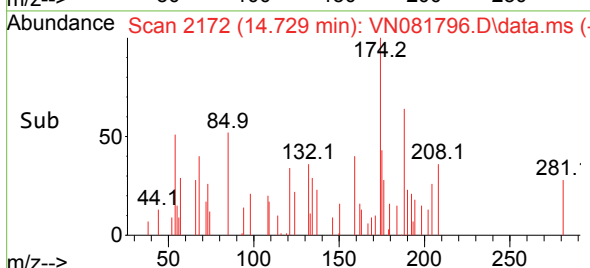

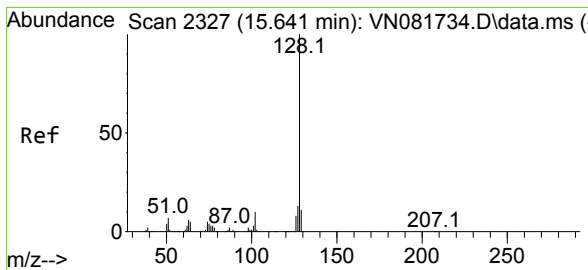

#95
Naphthalene
Concen: 0.864 ug/l
RT: 15.635 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN081796.D
Acq: 18 Apr 2024 18:42

Instrument :
MSVOA_N
ClientSampleId :

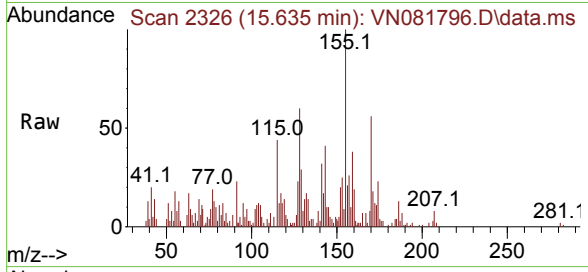

Tgt Ion:	128	Resp:	10699
Ion	Ratio	Lower	Upper
128	100		
127	38.1	10.1	15.1#
129	48.6	8.9	13.3#

