
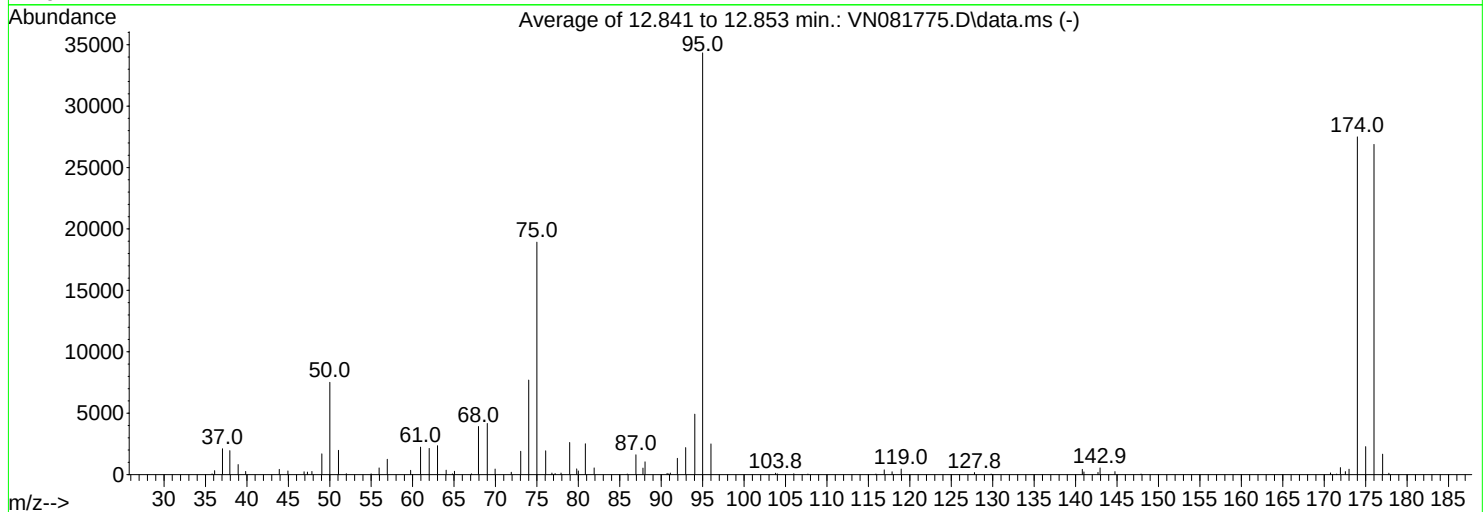


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041824\
Data File : VN081775.D
Acq On : 18 Apr 2024 08:44
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041524W.M
Title : SW846 8260
Last Update : Mon Apr 15 15:37:39 2024

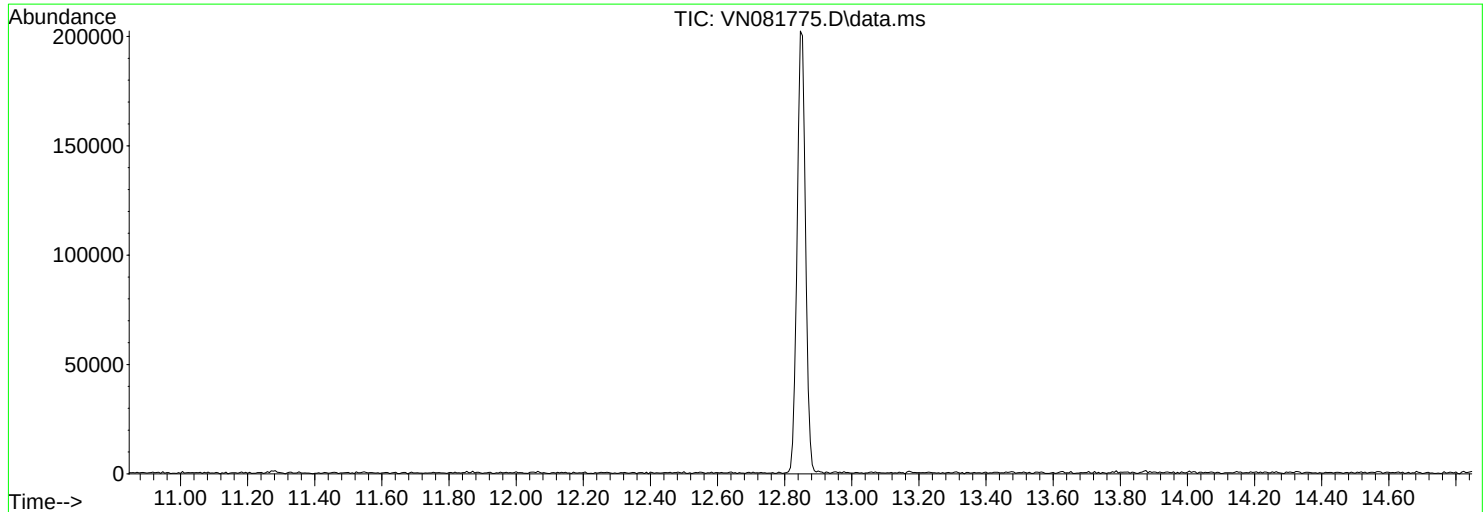

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.9	7523	PASS
75	95	30	60	55.1	18925	PASS
95	95	100	100	100.0	34336	PASS
96	95	5	9	7.3	2497	PASS
173	174	0.00	2	1.6	447	PASS
174	95	50	100	80.1	27493	PASS
175	174	5	9	8.3	2282	PASS
176	174	95	101	97.8	26888	PASS
177	176	5	9	6.2	1674	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	73	49.05	1699	64.05	368	76.05	1941
36.10	325	50.00	7523	64.80	72	76.80	134
37.05	2104	51.05	1982	65.05	276	77.20	9
37.95	1959	52.00	79	67.10	60	77.90	12
38.95	822	55.00	62	67.95	3921	78.95	2617
39.85	258	55.95	553	69.00	4171	79.80	464
43.90	430	56.95	1256	69.95	452	80.00	307
44.95	301	59.75	353	71.90	193	80.85	2514
46.90	230	60.95	2238	73.05	1901	81.90	542
47.30	204	62.00	2136	74.00	7695	85.90	53
47.85	265	63.00	2355	75.00	18925	86.95	1614

Average of 12.841 to 12.853 min.: VN081775.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.80	532	104.00	68	142.70	180	176.00	26888
88.05	1039	106.00	78	142.95	549	177.05	1674
90.70	101	107.70	59	144.75	248	177.80	118
90.90	64	115.90	51	147.90	56		
91.10	126	116.90	387	170.75	141		
91.95	1328	117.85	240	171.50	53		
92.95	2201	118.95	455	171.95	576		
94.05	4919	127.80	165	172.55	248		
95.00	34336	129.80	57	173.00	447		
96.00	2497	140.80	430	174.00	27493		
103.80	125	141.00	217	175.00	2282		

Instrument :

MSVOA_N

ClientSampleId :

BFB