


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041825\
Data File : VN086330.D
Acq On : 18 Apr 2025 08:13
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Title : SW846 8260
Last Update : Wed Apr 16 04:19:23 2025

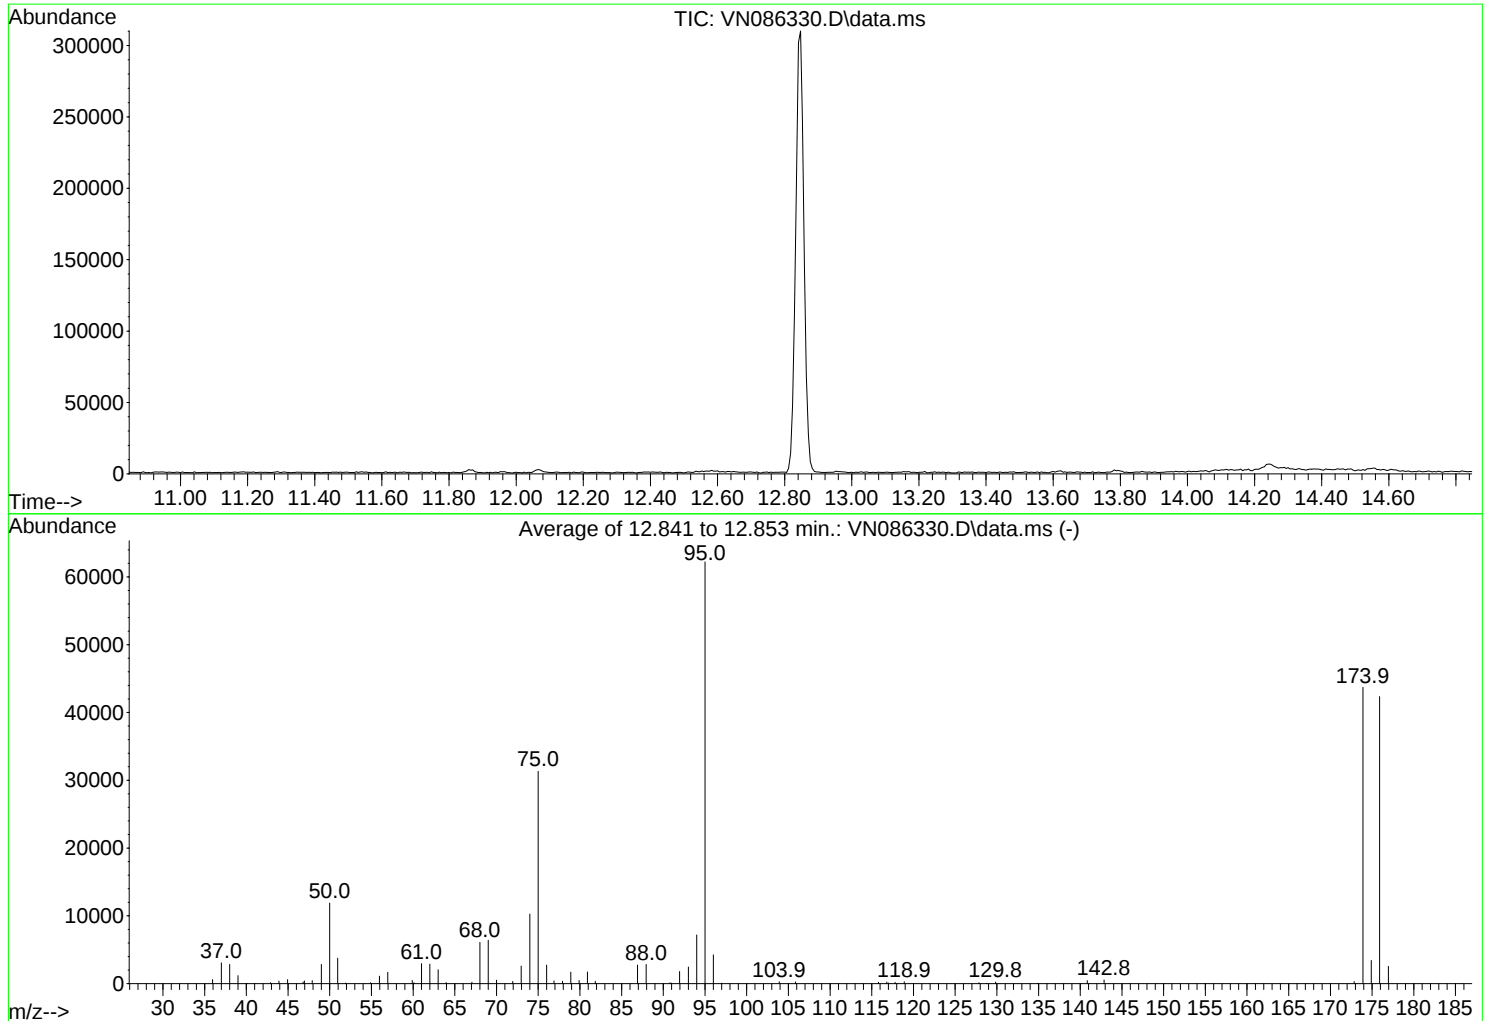

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.1	11907	PASS
75	95	30	60	50.3	31328	PASS
95	95	100	100	100.0	62224	PASS
96	95	5	9	6.8	4257	PASS
173	174	0.00	2	0.7	305	PASS
174	95	50	100	70.2	43712	PASS
175	174	5	9	7.8	3422	PASS
176	174	95	101	96.9	42347	PASS
177	176	5	9	6.0	2549	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	586	47.90	443	62.00	2870	76.00	2744
37.00	3065	49.00	2833	63.00	2064	76.90	4081
38.00	2838	50.00	11907	63.95	163	77.90	351
39.00	1170	50.95	3742	67.05	220	78.90	170
39.95	4	51.90	96	68.00	6102	79.90	466
41.00	52	54.90	150	69.00	6404	80.90	1716
42.90	138	55.95	1103	70.00	526	81.85	362
43.90	378	56.95	1682	71.95	339	86.90	2734
44.95	584	59.90	470	72.95	2599	87.95	2832
46.80	243	60.10	153	74.00	10269	90.80	147
46.95	396	61.00	2951	75.00	31328	91.00	83

Average of 12.841 to 12.853 min.: VN086330.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.95	1789	117.80	179	175.90	42347		
93.00	2466	118.90	274	176.95	2549		
94.00	7187	127.85	139				
95.00	62224	128.80	57				
96.00	4257	129.85	242				
97.00	73	134.90	51				
103.90	285	140.85	440				
105.85	267	142.85	534				
115.80	220	172.85	305				
116.80	234	173.90	43712				
117.00	100	174.90	3422				

Instrument :

MSVOA_N

ClientSampleId :

BFB