


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN041919\
Data File : VN055144.D
Acq On : 19 Apr 2019 16:11
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N041519W.M
Title : SW846 8260
Last Update : Mon Apr 15 12:28:28 2019

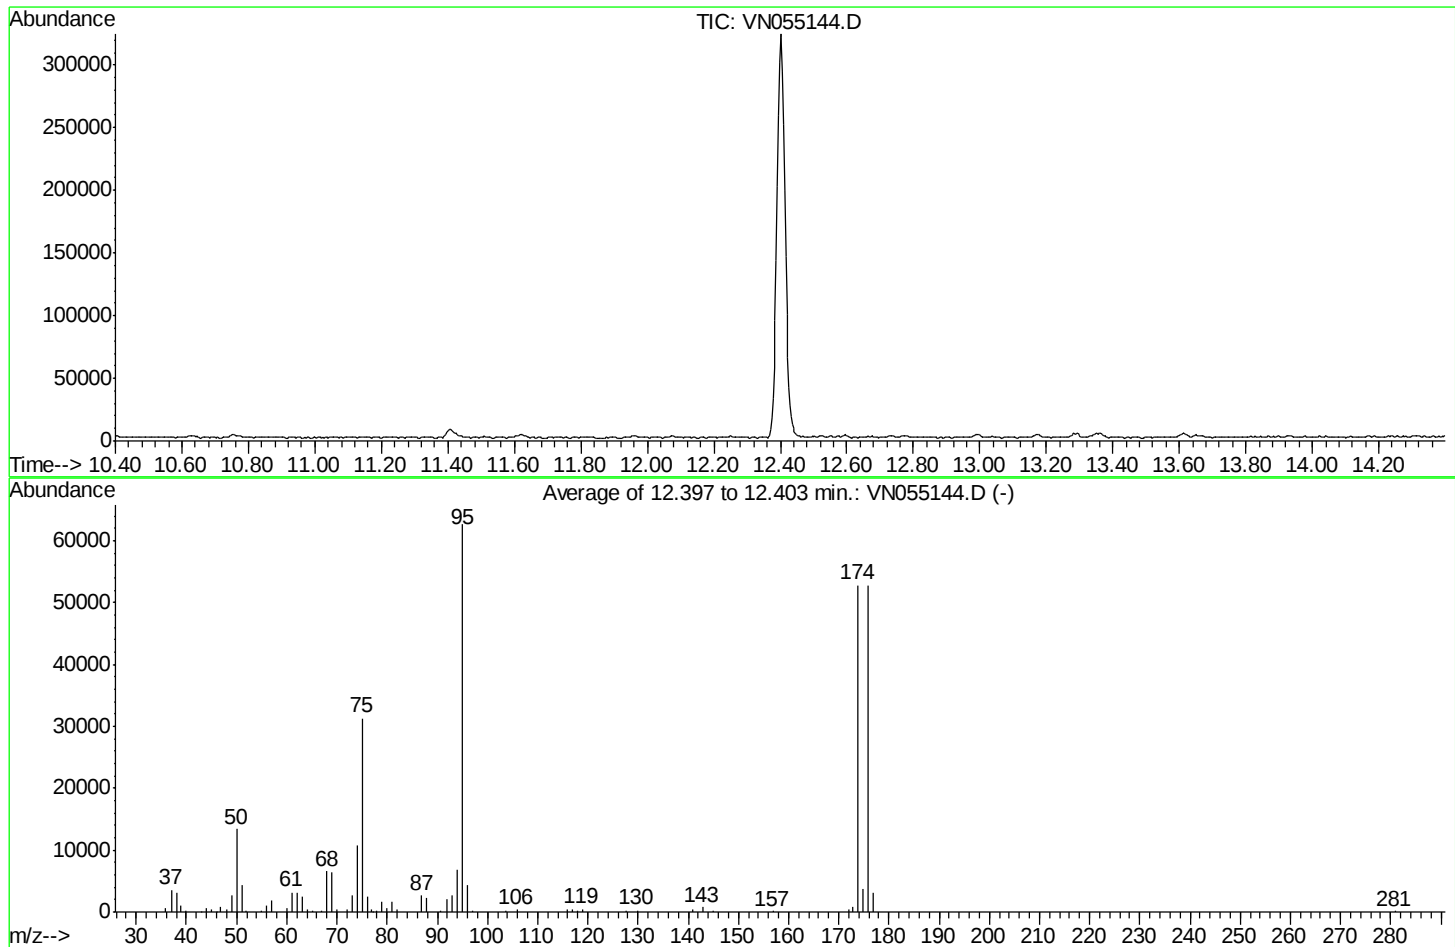

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	13393	PASS
75	95	30	60	50.0	31298	PASS
95	95	100	100	100.0	62624	PASS
96	95	5	9	7.1	4426	PASS
173	174	0.00	2	1.7	880	PASS
174	95	50	100	84.3	52816	PASS
175	174	5	9	7.1	3751	PASS
176	174	95	101	99.9	52765	PASS
177	176	5	9	5.9	3094	PASS