

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041921\
 Data File : VN066658.D
 Acq On : 19 Apr 2021 13:31
 Operator : JC/MD
 Sample : M2075-05
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Apr 20 04:55:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041521W.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 15 19:16:35 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.591	168	280471	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.519	114	443913	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.348	117	427470	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.290	152	178224	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.953	65	208042	49.17	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	98.34%
35) Dibromofluoromethane	7.513	113	162634	52.83	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	105.66%
50) Toluene-d8	10.029	98	651140	53.97	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	107.94%
62) 4-Bromofluorobenzene	12.346	95	212012	49.97	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	99.94%


Target Compounds					Qvalue	
3) Chloromethane	2.037	50	1535	0.31	ug/l	98
11) Tert butyl alcohol	4.708	59	380	0.56	ug/l #	73
13) Acrolein	3.555	56	1045	2.89	ug/l	93
16) Acetone	3.756	43	35862	15.75	ug/l	97
18) Methyl Acetate	4.260	43	4305	0.94	ug/l #	79
20) Methylene Chloride	4.474	84	9878	2.47	ug/l	97
25) 2-Butanone	6.757	43	10837	4.35	ug/l #	89
29) Tetrahydrofuran	7.143	42	1506	0.90	ug/l #	53
31) Cyclohexane	7.591	56	5433	0.89	ug/l #	1
36) 1,1-Dichloropropene	7.591	75	21091	4.71	ug/l #	48
38) Carbon Tetrachloride	7.591	117	24982	5.96	ug/l #	18
43) Isopropyl Acetate	8.095	43	26902	3.17	ug/l #	86
45) 1,2-Dichloropropane	9.203	63	1612	0.40	ug/l #	44
48) Methyl methacrylate	9.117	41	6542	1.72	ug/l #	10
51) 4-Methyl-2-Pentanone	9.924	43	11297	2.27	ug/l	94
54) cis-1,3-Dichloropropene	9.844	75	42815	7.32	ug/l #	63
56) Ethyl methacrylate	10.380	69	153	0.92	ug/l #	27
57) 1,3-Dichloropropane	10.705	76	24584	4.20	ug/l #	43
59) 2-Hexanone	10.707	43	361818	104.72	ug/l #	50
71) Bromoform	12.346	173	1353	0.53	ug/l #	1
74) N-amyl acetate	12.008	43	185	9.76	ug/l #	50
76) 1,2,3-Trichloropropane	12.346	75	105959	25.42	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.346	75	105959	78.47	ug/l #	12
86) p-Isopropyltoluene	13.239	119	2976	0.28	ug/l	84
87) 1,3-Dichlorobenzene	13.234	146	1211	0.20	ug/l	93
88) 1,4-Dichlorobenzene	13.234	146	1211	Below	Cal	94
89) n-Butylbenzene	13.582	91	2098	0.23	ug/l #	73
91) 1,2-Dichlorobenzene	13.609	146	1264	0.22	ug/l #	75
92) 1,2-Dibromo-3-Chloropr...	14.226	75	250	0.29	ug/l #	1
93) 1,2,4-Trichlorobenzene	14.862	180	2970	0.90	ug/l	86
95) Naphthalene	15.082	128	17625	1.94	ug/l	95
96) 1,2,3-Trichlorobenzene	15.253	180	4341	1.28	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041921\
Data File : VN066658.D
Acq On : 19 Apr 2021 13:31
Operator : JC/MD
Sample : M2075-05
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Apr 20 04:55:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041521W.M
Quant Title : SW846 8260
QLast Update : Thu Apr 15 19:16:35 2021
Response via : Initial Calibration




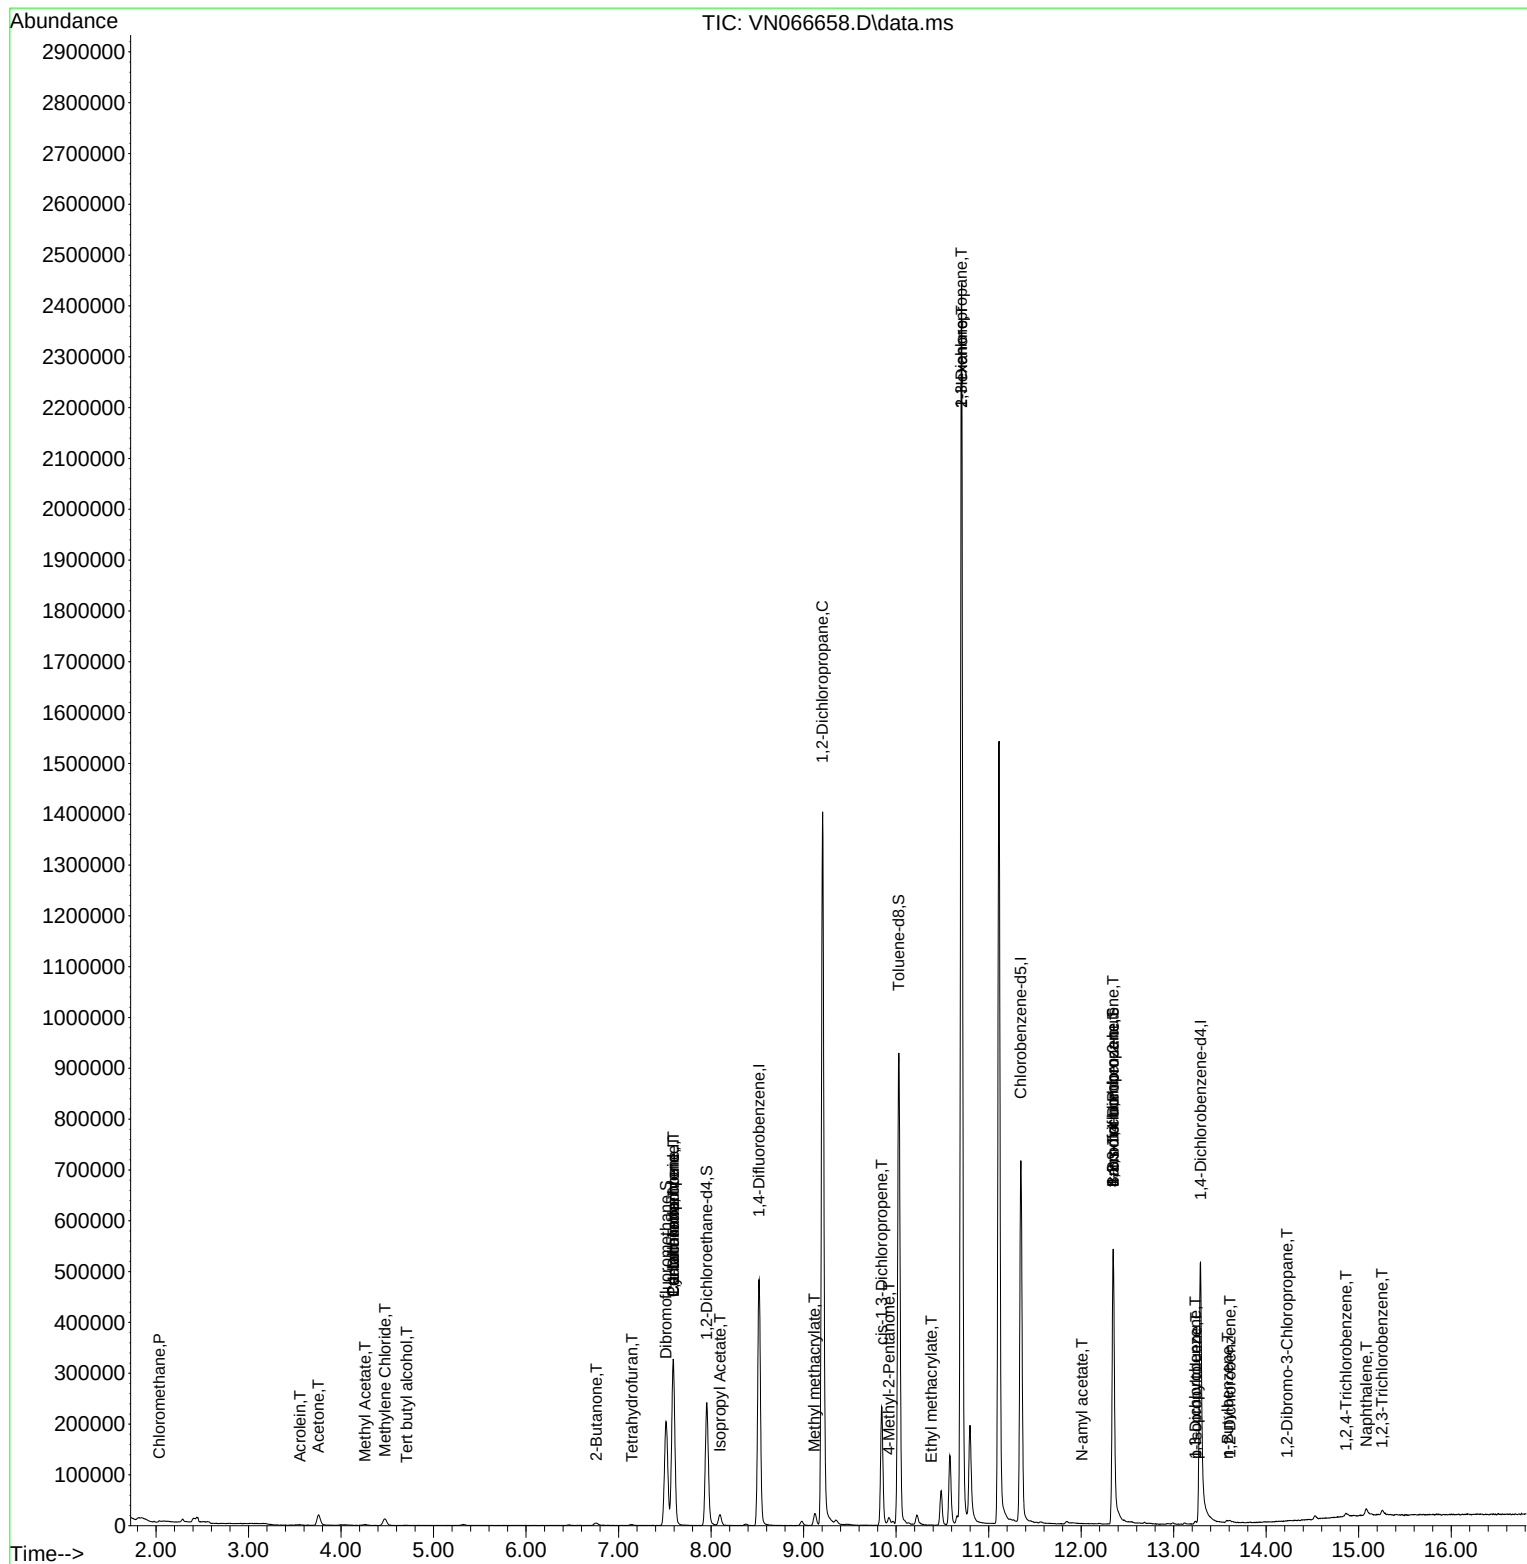




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.591 min Scan# 2188
Delta R.T. 0.003 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 280471
Ion Ratio Lower Upper
168 100
99 52.6 42.6 63.8

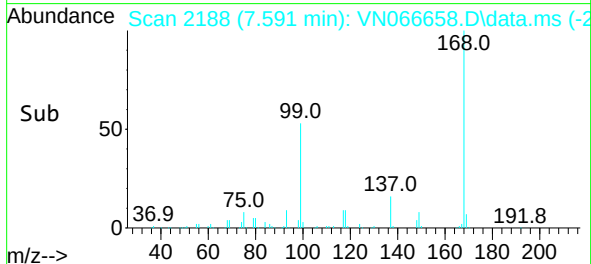

#3
Chloromethane
Concen: 0.31 ug/l
RT: 2.037 min Scan# 117
Delta R.T. 0.006 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31

Tgt Ion: 50 Resp: 1535
Ion Ratio Lower Upper
50 100
52 33.6 25.8 38.8

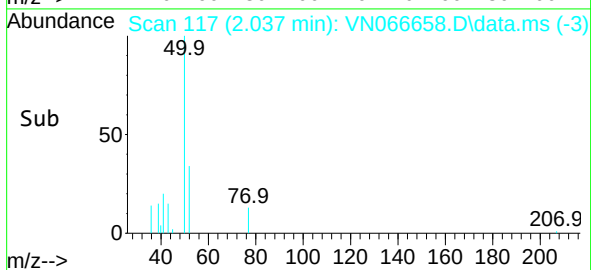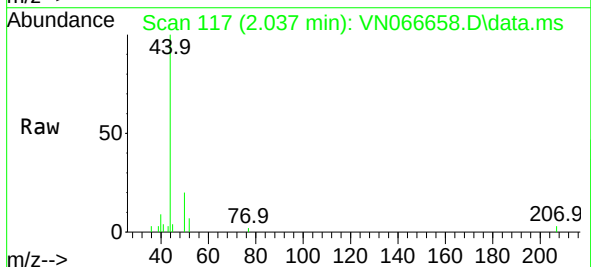


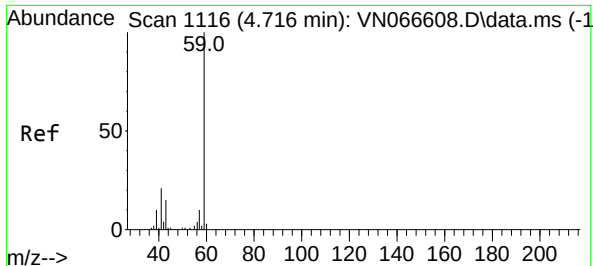




#11

Tert butyl alcohol
Concen: 0.56 ug/l
RT: 4.708 min Scan# 1113
Delta R.T. -0.008 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31

Instrument :
MSVOA_N
ClientSampled :

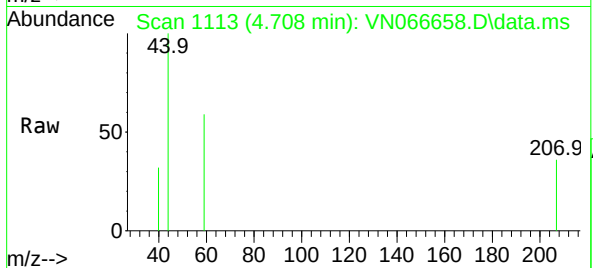


Tgt Ion: 59 Resp: 380
Ion Ratio Lower Upper
59 100
57 0.0 8.0 12.0#

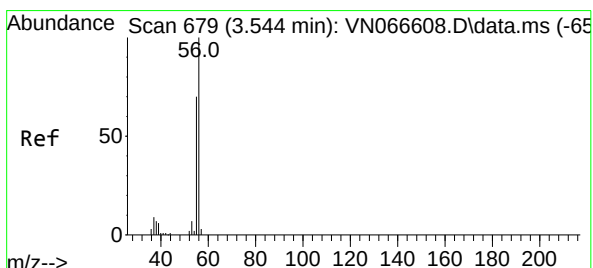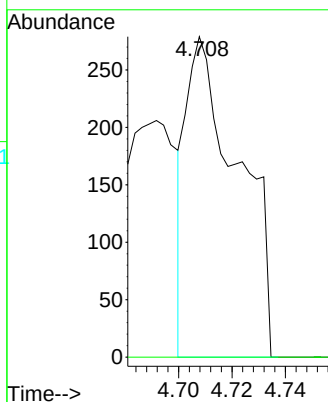
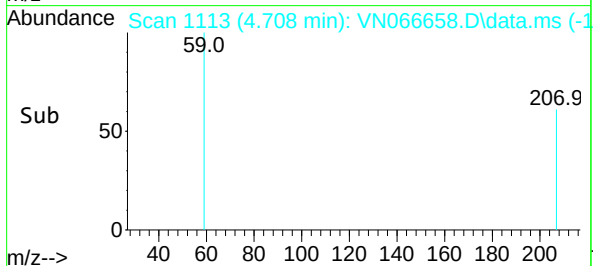



#13

Acrolein
Concen: 2.89 ug/l
RT: 3.555 min Scan# 683
Delta R.T. 0.011 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31

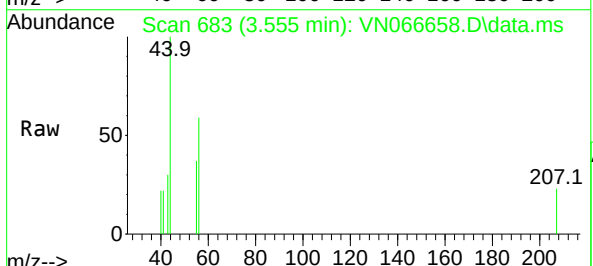

Tgt Ion: 56 Resp: 1045
Ion Ratio Lower Upper
56 100
55 64.3 56.0 84.0



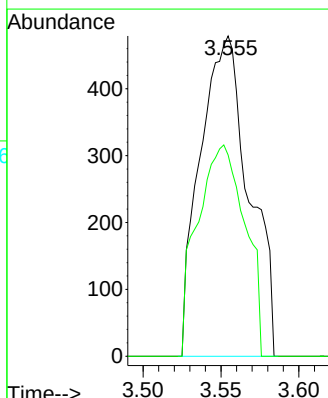
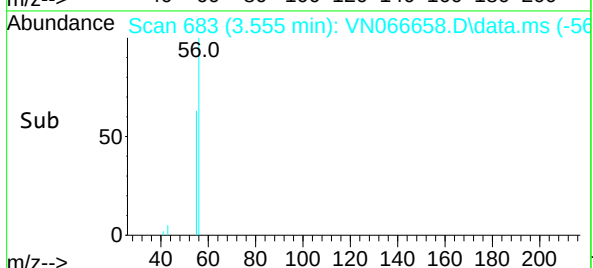


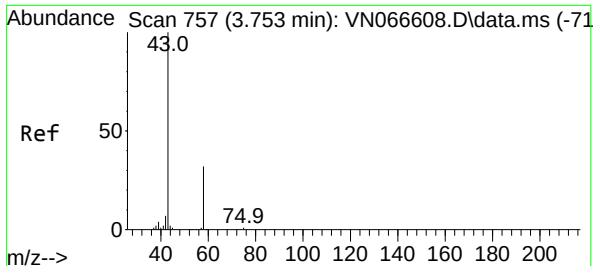

#16
Acetone
Concen: 15.75 ug/l
RT: 3.756 min Scan# 758
Delta R.T. 0.003 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 35862
Ion Ratio Lower Upper
43 100
58 32.4 27.0 40.6

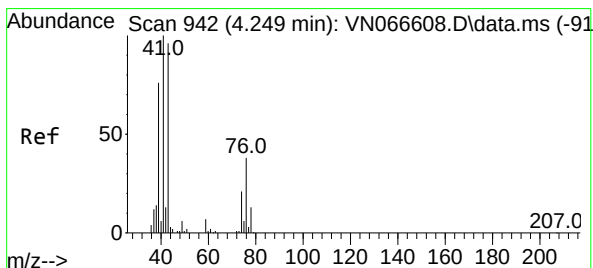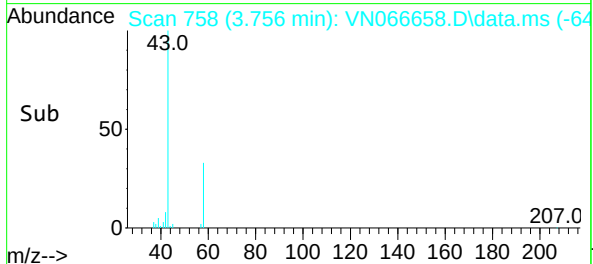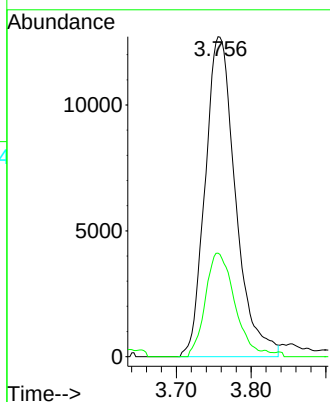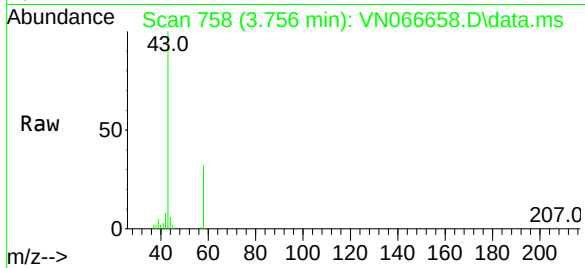

#18
Methyl Acetate
Concen: 0.94 ug/l
RT: 4.260 min Scan# 946
Delta R.T. 0.011 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31


Tgt Ion: 43 Resp: 4305
Ion Ratio Lower Upper
43 100
74 13.8 19.5 29.3#

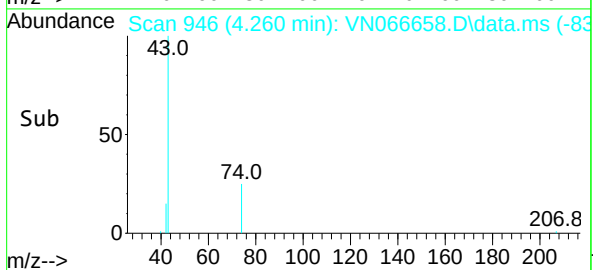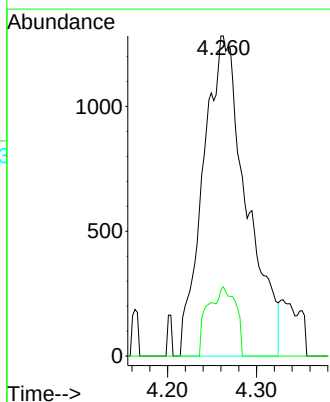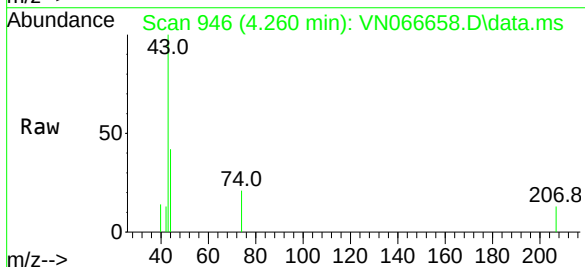



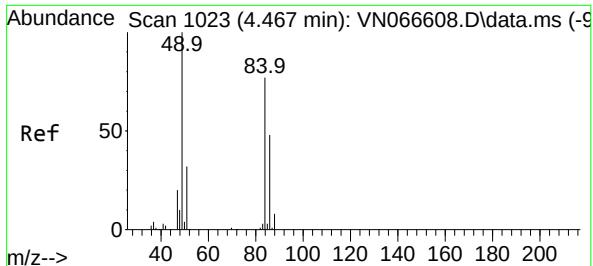


#20
Methylene Chloride
Concen: 2.47 ug/l
RT: 4.474 min Scan# 1026
Delta R.T. 0.007 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31

Instrument :
MSVOA_N
ClientSampleId :



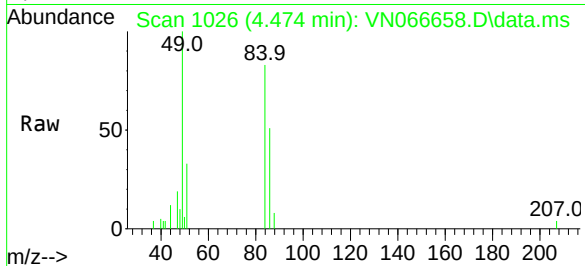



Tgt Ion: 84	Resp: 9878
Ion Ratio	Lower Upper
84 100	
49 120.7	94.6 141.8
51 40.2	29.9 44.9
86 61.9	51.4 77.2

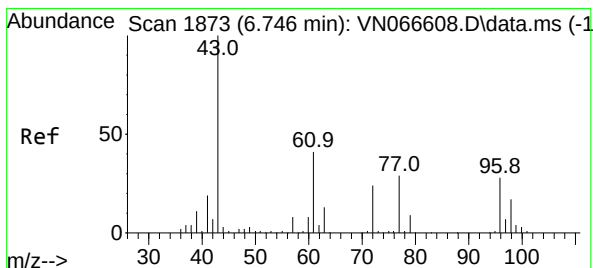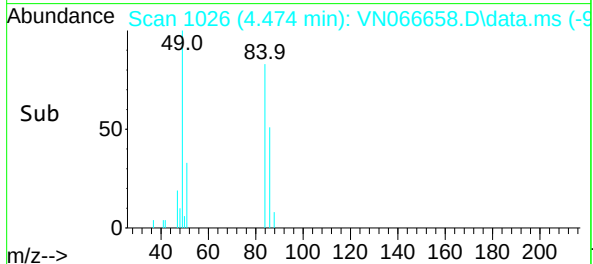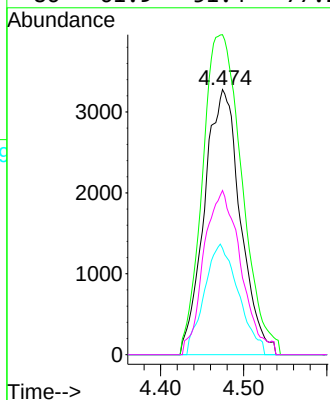

#25
2-Butanone
Concen: 4.35 ug/l
RT: 6.757 min Scan# 1877
Delta R.T. 0.011 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31

Tgt Ion: 43	Resp: 10837		
Ion Ratio	Lower	Upper	
43 100			
72 23.0	23.1	34.7#	

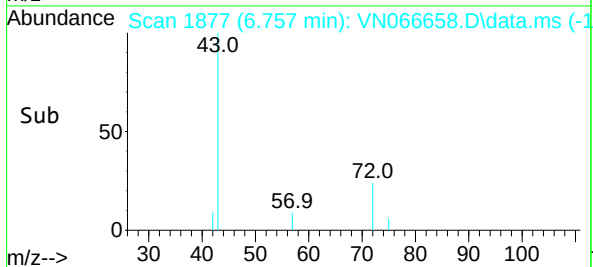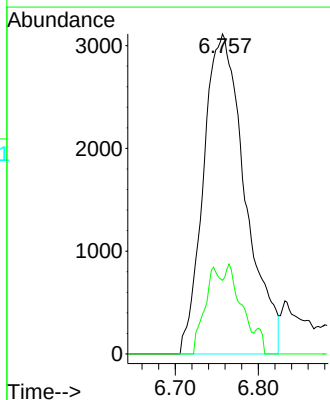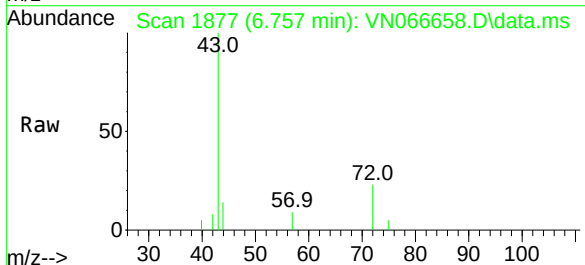

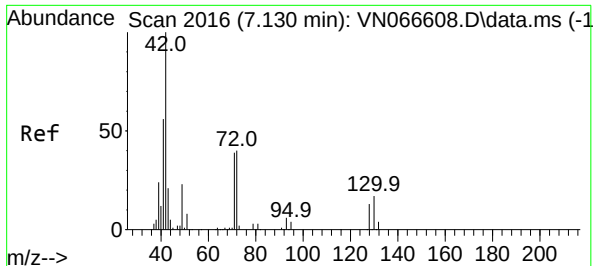

#29

Tetrahydrofuran

Concen: 0.90 ug/l

RT: 7.143 min Scan# 2021





Delta R.T. 0.013 min

Lab File: VN066658.D

Acq: 19 Apr 2021 13:31

Tgt Ion:	42	Resp:	1506
Ion	Ratio	Lower	Upper
42	100		
72	22.9	36.6	55.0#
71	5.1	34.3	51.5#

Instrument :
MSVOA_N
ClientSampleId :

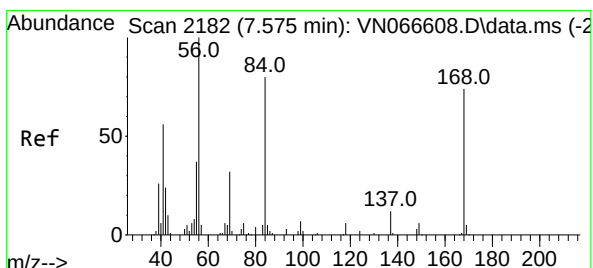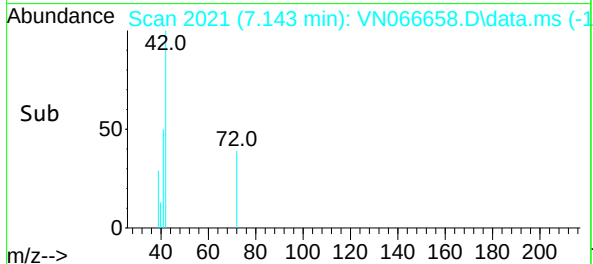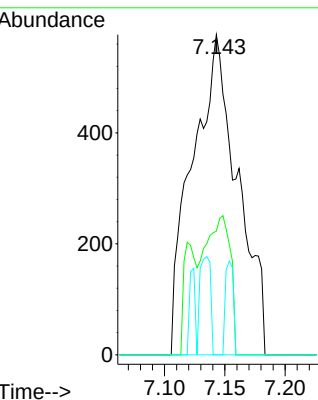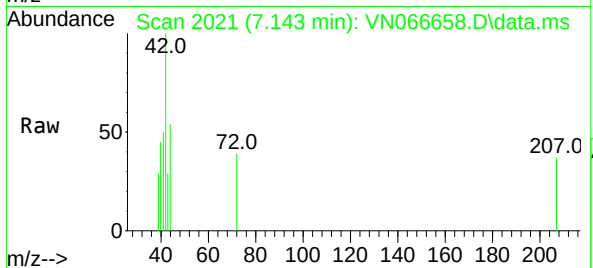

#31

Cyclohexane

Concen: 0.89 ug/l




RT: 7.591 min Scan# 2188


Delta R.T. 0.016 min

Lab File: VN066658.D

Acq: 19 Apr 2021 13:31


Tgt Ion:	56	Resp:	5433
Ion	Ratio	Lower	Upper
56	100		
69	187.6	26.6	39.8#
84	150.1	70.4	105.6#

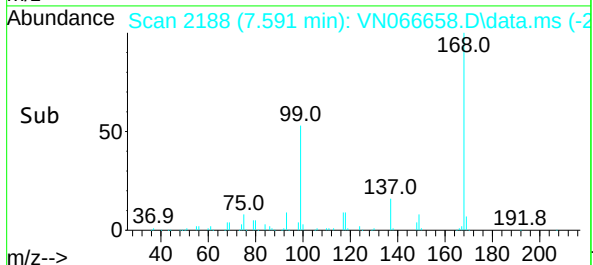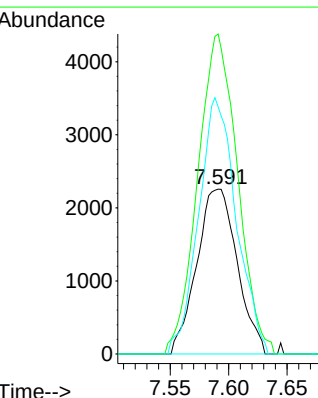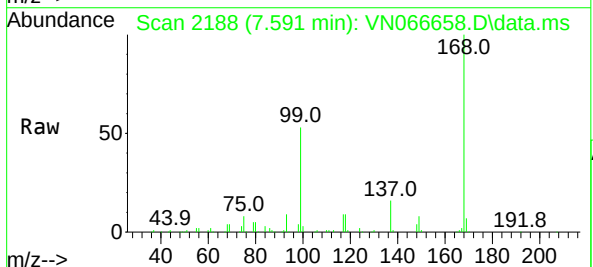






#33
 1,2-Dichloroethane-d4
 Concen: 49.17 ug/l
 RT: 7.953 min Scan# 2323
 Delta R.T. -0.000 min
 Lab File: VN066658.D
 Acq: 19 Apr 2021 13:31

Instrument :
 MSVOA_N
 ClientSampleId :







Tgt Ion: 65 Resp: 208042
 Ion Ratio Lower Upper
 65 100
 67 53.6 0.0 107.2

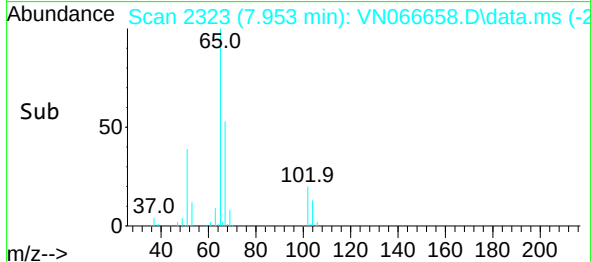

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.519 min Scan# 2534
 Delta R.T. -0.000 min
 Lab File: VN066658.D
 Acq: 19 Apr 2021 13:31

Tgt Ion: 114 Resp: 443913
 Ion Ratio Lower Upper
 114 100
 63 21.2 0.0 38.6
 88 15.0 0.0 30.6


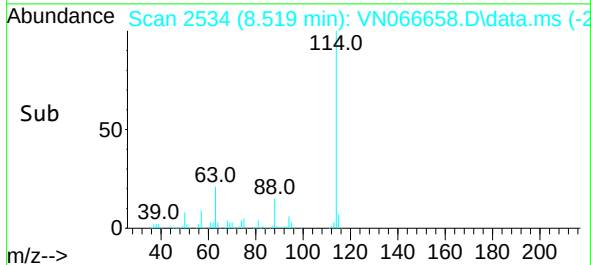

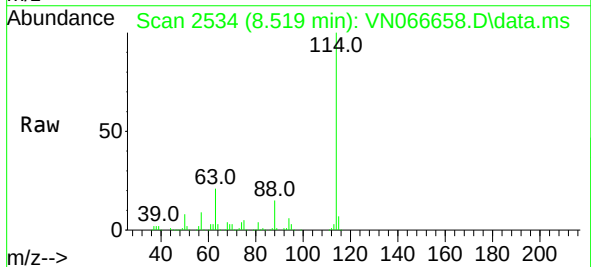




#35
Dibromofluoromethane
Concen: 52.83 ug/l
RT: 7.513 min Scan# 2159
Delta R.T. 0.002 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:	113	Resp:	162634
Ion Ratio	Lower	Upper	
113	100		
111	103.7	82.2	123.2
192	20.8	15.4	23.0

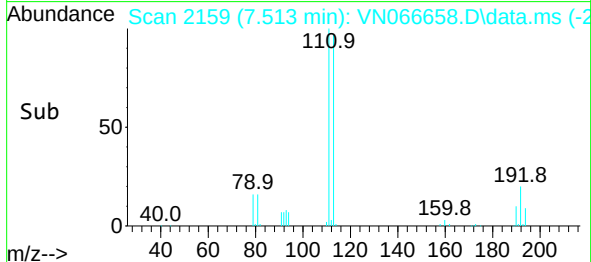

#36
1,1-Dichloropropene
Concen: 4.71 ug/l
RT: 7.591 min Scan# 2188
Delta R.T. -0.126 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31


Tgt Ion:	75	Resp:	21091
Ion Ratio	Lower	Upper	
75	100		
110	7.6	18.2	54.6#
77	0.0	24.9	37.3#

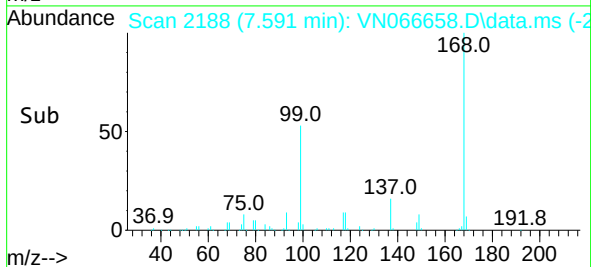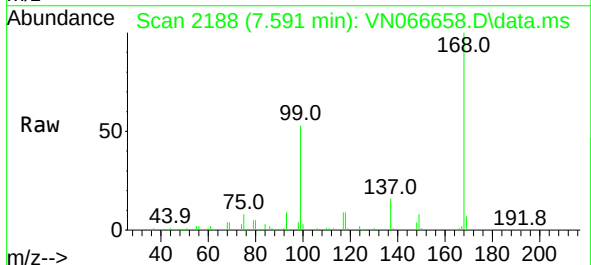






#38
Carbon Tetrachloride
Concen: 5.96 ug/l
RT: 7.591 min Scan# 2188
Delta R.T. -0.105 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:117 Resp: 24982
Ion Ratio Lower Upper
117 100
119 6.7 76.0 114.0#
121 0.0 24.5 36.7#




#43
Isopropyl Acetate
Concen: 3.17 ug/l
RT: 8.095 min Scan# 2376
Delta R.T. 0.000 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31



Tgt Ion: 43 Resp: 26902
Ion Ratio Lower Upper
43 100
61 18.7 22.5 33.7#
87 11.1 11.1 16.7




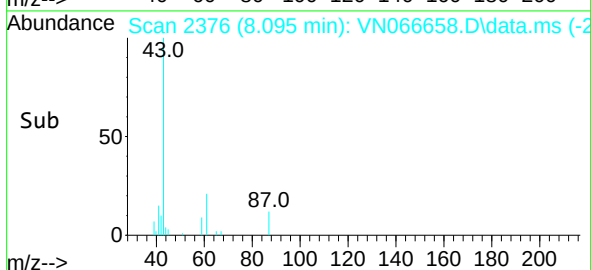


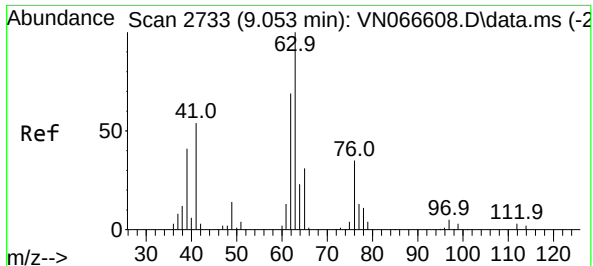

#45
1,2-Dichloropropane
Concen: 0.40 ug/l
RT: 9.203 min Scan# 2789
Delta R.T. 0.150 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 63 Resp: 1612
Ion Ratio Lower Upper
63 100
65 0.0 24.9 37.3#

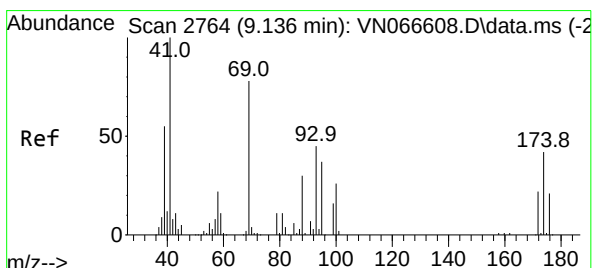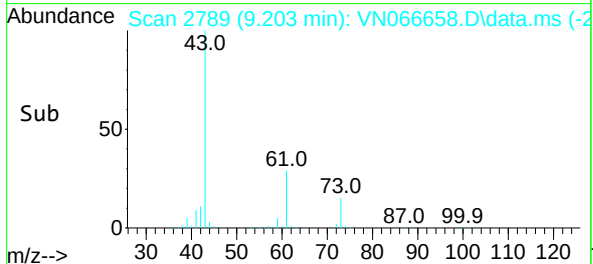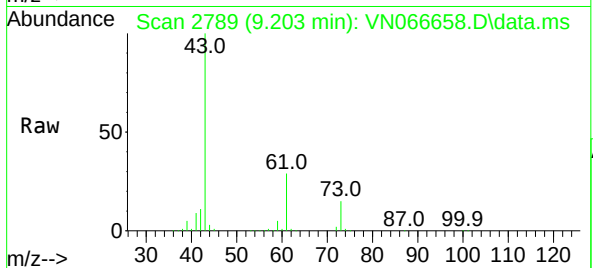

#48
Methyl methacrylate
Concen: 1.72 ug/l
RT: 9.117 min Scan# 2757
Delta R.T. -0.019 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31

Tgt Ion: 41 Resp: 6542
Ion Ratio Lower Upper
41 100
69 0.0 75.9 113.9#
39 0.0 46.6 69.8#


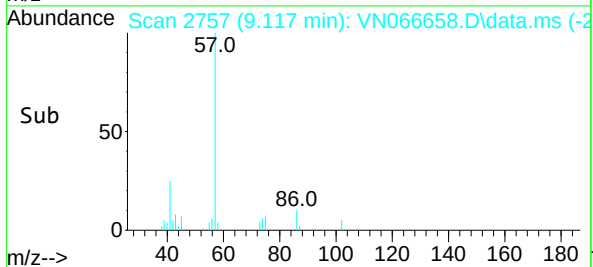

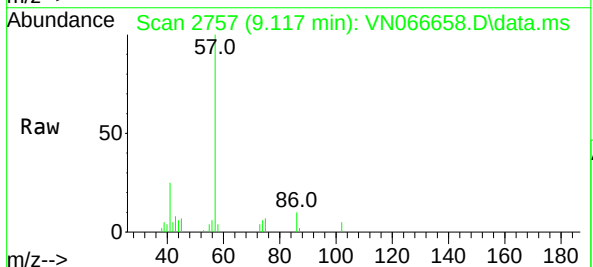




#50
Toluene-d8
Concen: 53.97 ug/l
RT: 10.029 min Scan# 3097
Delta R.T. -0.000 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 651140
Ion Ratio Lower Upper
98 100
100 64.3 50.5 75.7

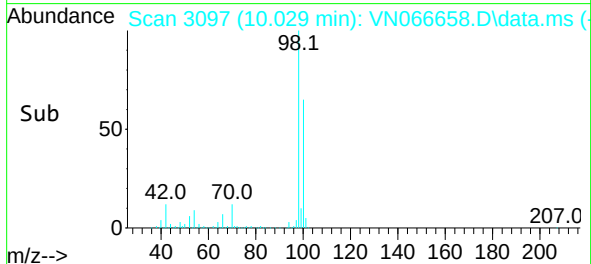

#51
4-Methyl-2-Pentanone
Concen: 2.27 ug/l
RT: 9.924 min Scan# 3058
Delta R.T. 0.002 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31


Tgt Ion: 43 Resp: 11297
Ion Ratio Lower Upper
43 100
58 37.0 32.5 48.7

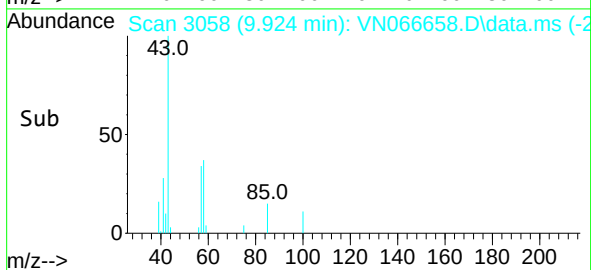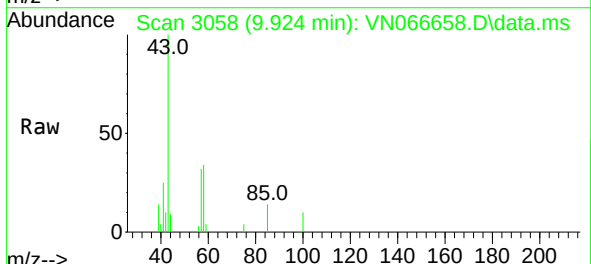






#54
cis-1,3-Dichloropropene
Concen: 7.32 ug/l
RT: 9.844 min Scan# 3028
Delta R.T. 0.067 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 75 Resp: 42815
Ion Ratio Lower Upper
75 100
77 0.7 24.9 37.3#
39 29.5 36.2 54.4#

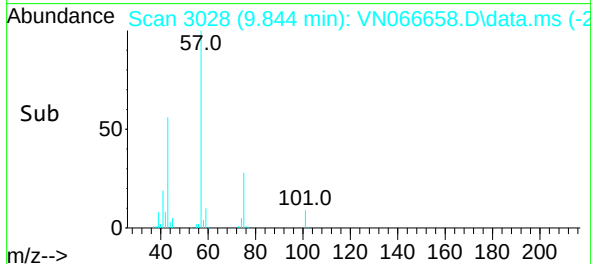

#56
Ethyl methacrylate
Concen: 0.92 ug/l
RT: 10.380 min Scan# 3228
Delta R.T. 0.008 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31

Tgt Ion: 69 Resp: 153
Ion Ratio Lower Upper
69 100
41 0.0 49.6 74.4#
39 0.0 28.0 42.0#


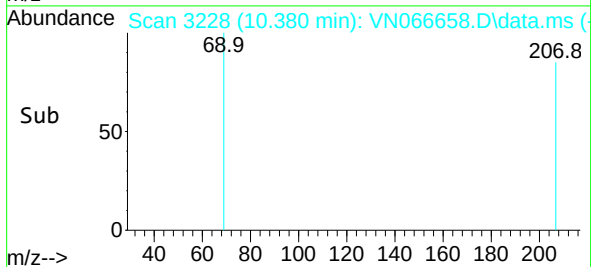

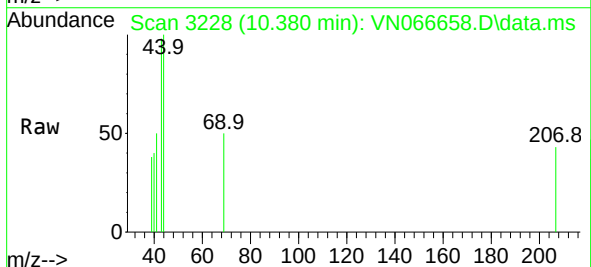


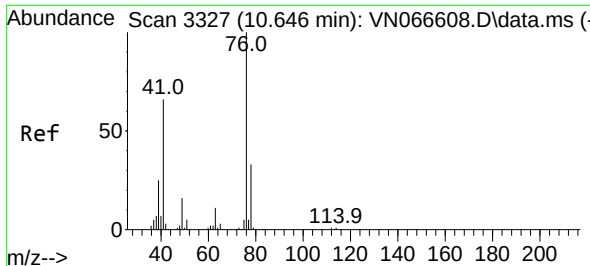

#57
1,3-Dichloropropane
Concen: 4.20 ug/l
RT: 10.705 min Scan# 3349
Delta R.T. 0.059 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 76 Resp: 24584
Ion Ratio Lower Upper
76 100
78 0.0 25.7 38.5#

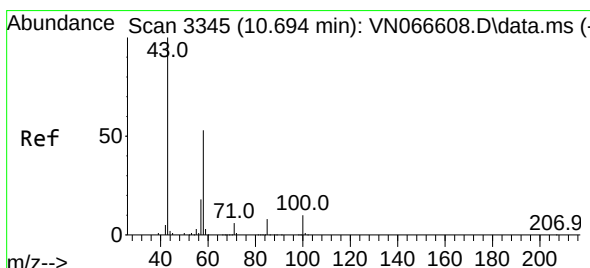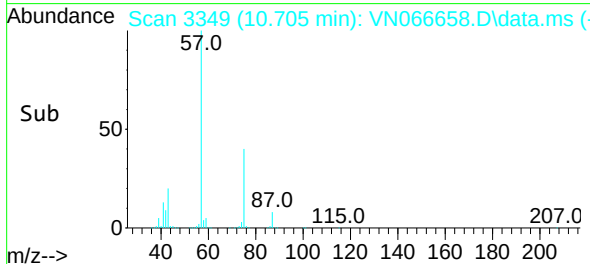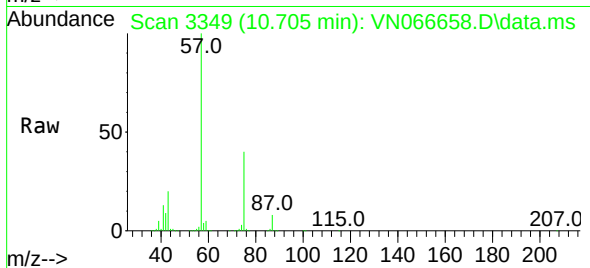

#59
2-Hexanone
Concen: 104.72 ug/l
RT: 10.707 min Scan# 3350
Delta R.T. 0.013 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31

Tgt Ion: 43 Resp: 361818
Ion Ratio Lower Upper
43 100
58 19.4 28.1 84.3#


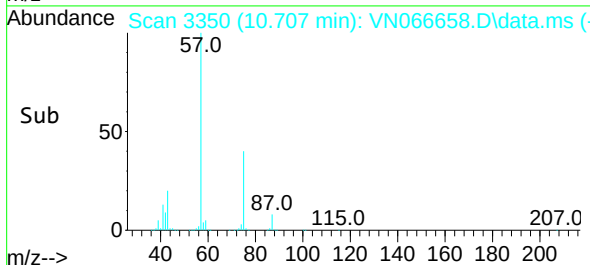

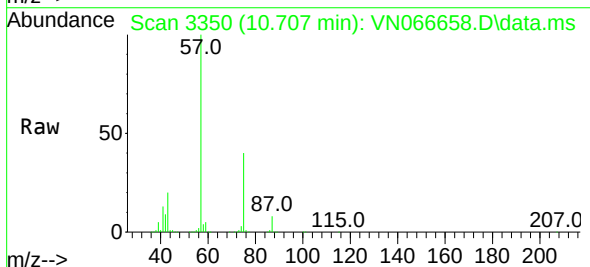


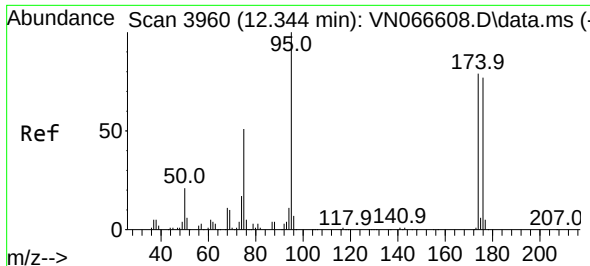

#62
4-Bromofluorobenzene
Concen: 49.97 ug/l
RT: 12.346 min Scan# 3961
Delta R.T. 0.002 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 212012
Ion Ratio Lower Upper
95 100
174 85.0 0.0 169.0
176 81.5 0.0 162.4

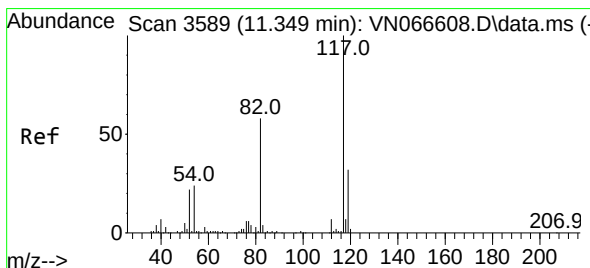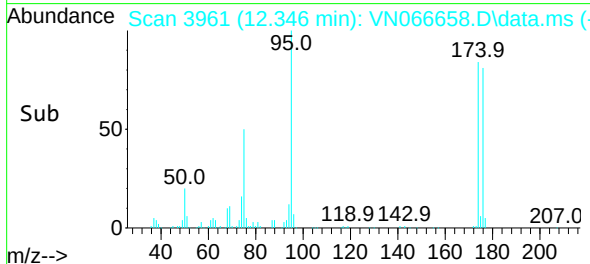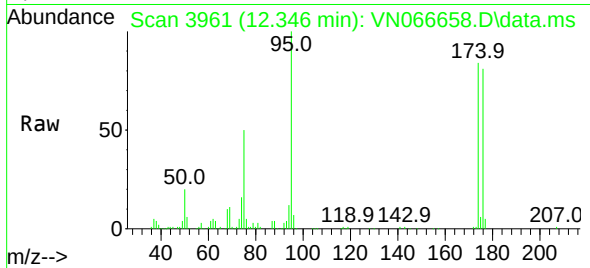

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.348 min Scan# 3589
Delta R.T. -0.001 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31

Tgt Ion: 117 Resp: 427470
Ion Ratio Lower Upper
117 100
82 56.7 43.7 65.5
119 32.3 26.1 39.1


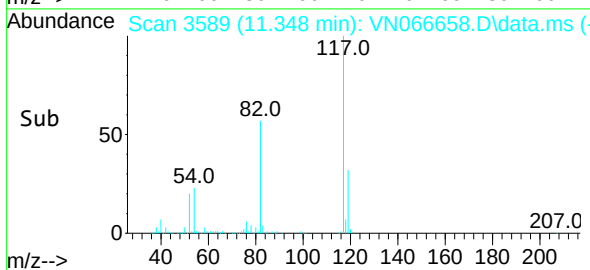

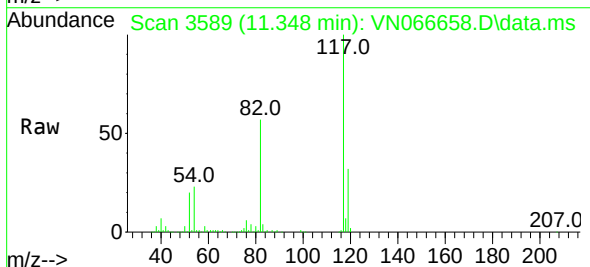


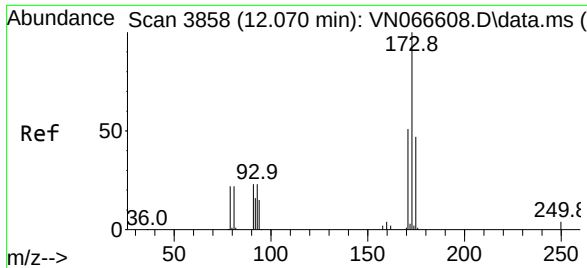

#71
Bromoform
Concen: 0.53 ug/l
RT: 12.346 min Scan# 3961
Delta R.T. 0.276 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:173 Resp: 1353
Ion Ratio Lower Upper
173 100
175 747.9 23.8 71.2#
254 0.0 0.0 0.0

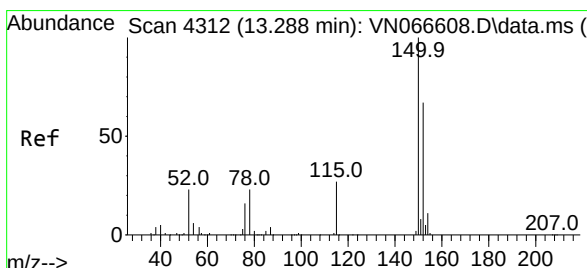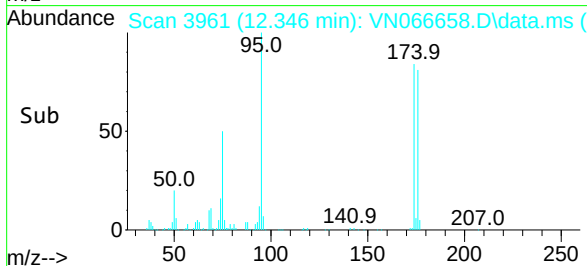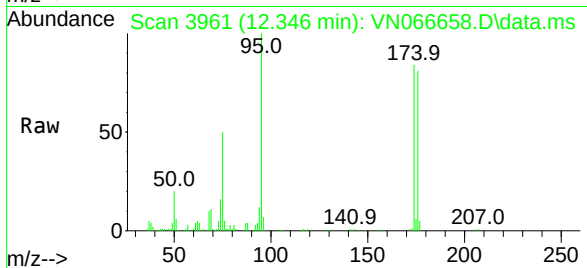

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.290 min Scan# 4313
Delta R.T. 0.002 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31


Tgt Ion:152 Resp: 178224
Ion Ratio Lower Upper
152 100
115 56.8 28.5 85.6
150 163.4 0.0 347.6

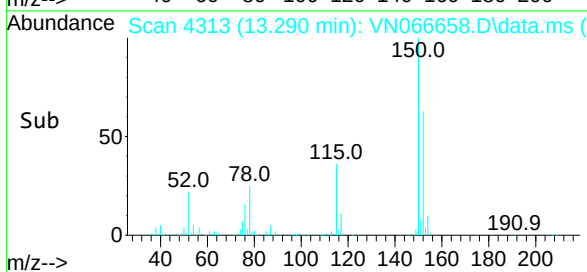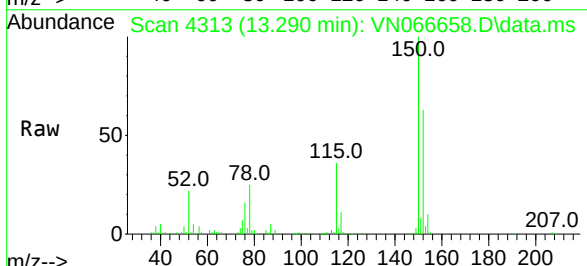



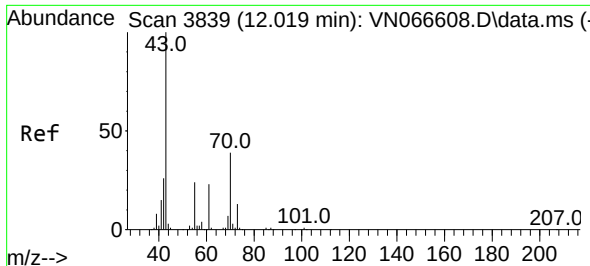


#74
N-amy1 acetate
Concen: 9.76 ug/l
RT: 12.008 min Scan# 3835
Delta R.T. -0.011 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31

Instrument :
MSVOA_N
ClientSampled :



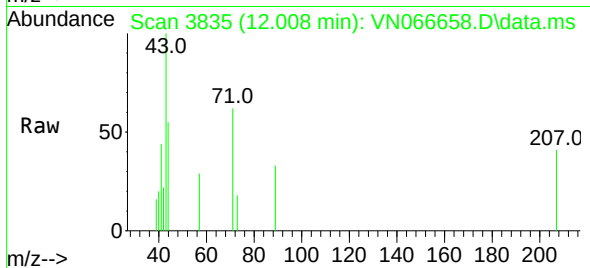



Tgt Ion: 43	Resp: 185
Ion Ratio	Lower Upper
43 100	
70 0.0	34.4 51.6#
55 13.5	20.7 31.1#
61 0.0	19.1 28.7#

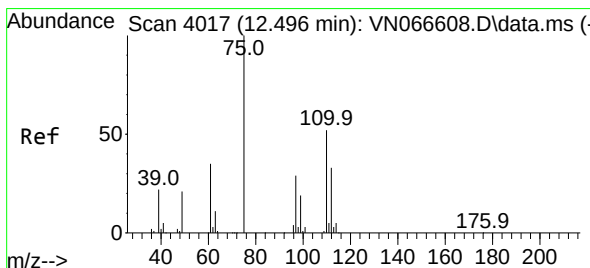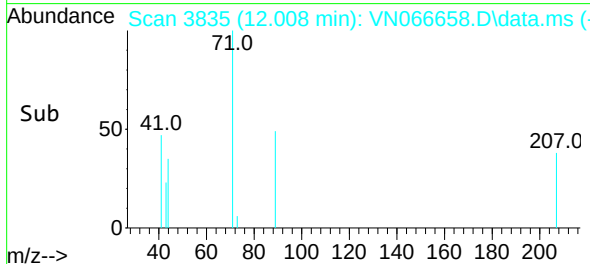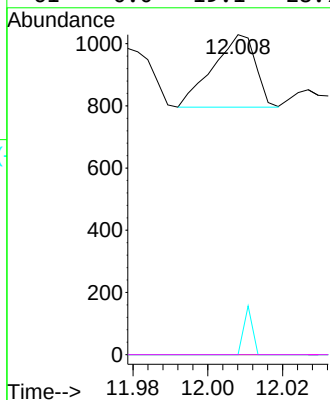

#76
1,2,3-Trichloropropane
Concen: 25.42 ug/l
RT: 12.346 min Scan# 3961
Delta R.T. -0.150 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31

Tgt Ion: 75	Resp: 105959
Ion Ratio	Lower Upper
75 100	
77 1.3	0.0 0.0#


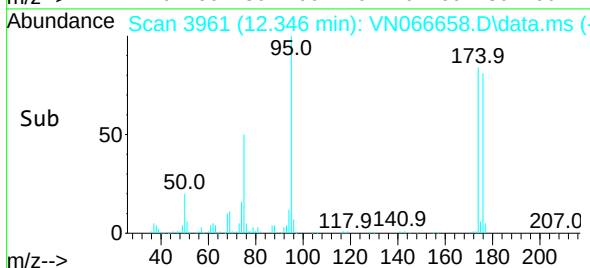
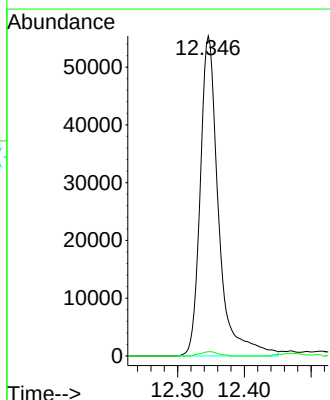
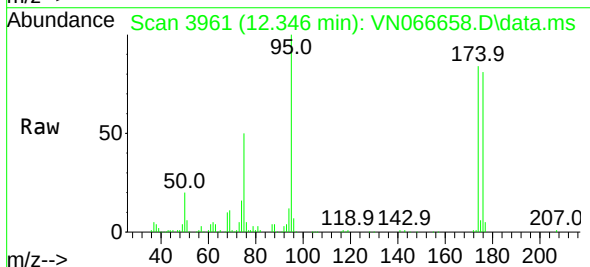




#81
trans-1,4-Dichloro-2-butene
Concen: 78.47 ug/l
RT: 12.346 min Scan# 3961
Delta R.T. 0.102 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 105959
Ion Ratio Lower Upper
75 100
53 0.0 74.6 111.8#
89 0.2 35.8 53.8#

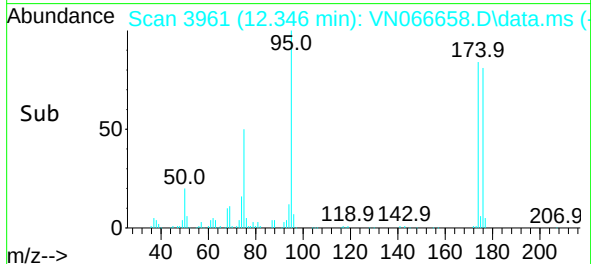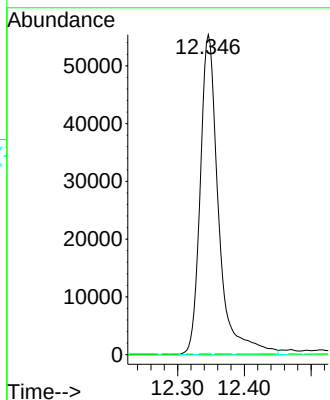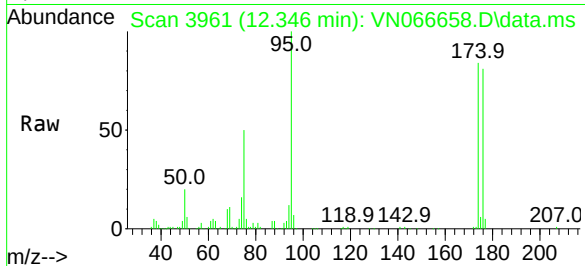

#86
p-Isopropyltoluene
Concen: 0.28 ug/l
RT: 13.239 min Scan# 4294
Delta R.T. 0.005 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31

Tgt Ion: 119 Resp: 2976
Ion Ratio Lower Upper
119 100
134 18.6 13.3 39.8
91 15.5 11.8 35.3


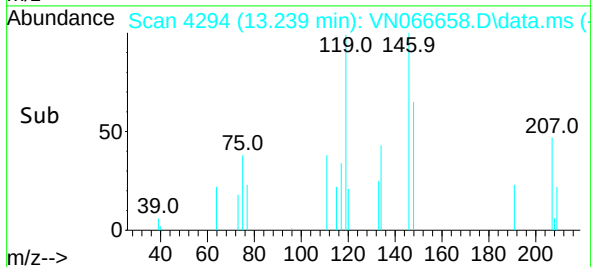
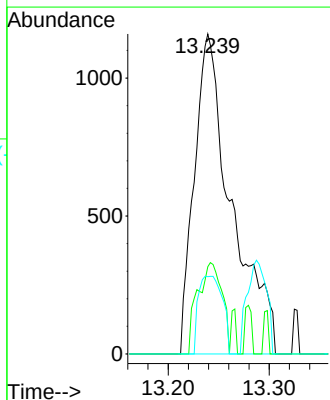
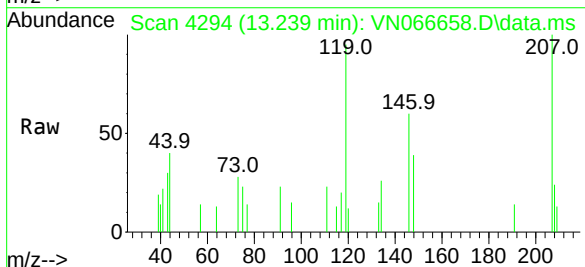




#87
1,3-Dichlorobenzene
Concen: 0.20 ug/l
RT: 13.234 min Scan# 4292
Delta R.T. 0.008 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:	146	Resp:	1211
Ion	Ratio	Lower	Upper
146	100		
111	35.9	19.5	58.5
148	57.6	32.3	96.9

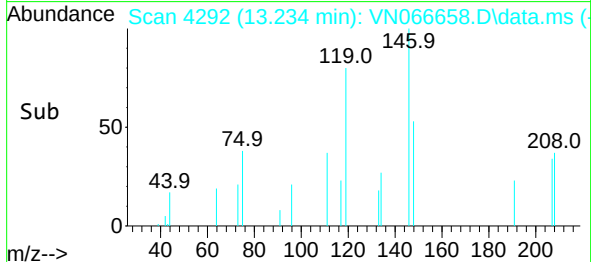

#88
1,4-Dichlorobenzene
Concen: Below Cal
RT: 13.234 min Scan# 4292
Delta R.T. -0.072 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31

Tgt Ion:	146	Resp:	1211
Ion	Ratio	Lower	Upper
146	100		
111	35.9	19.0	57.0
148	57.6	31.8	95.3


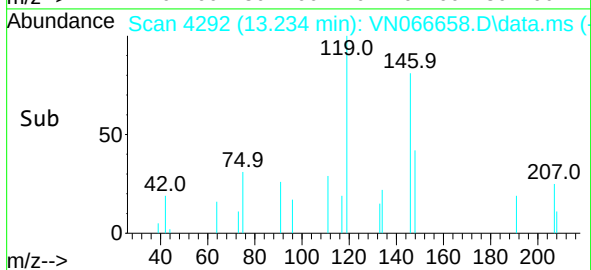

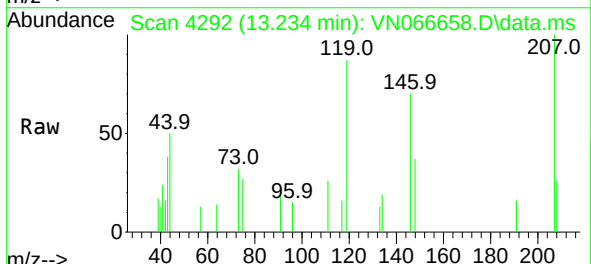




#89
n-Butylbenzene
Concen: 0.23 ug/l
RT: 13.582 min Scan# 4422
Delta R.T. 0.024 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 2098
Ion Ratio Lower Upper
91 100
92 67.7 26.1 78.3
134 7.2 13.0 38.9#

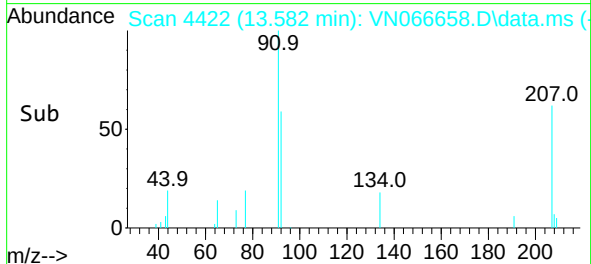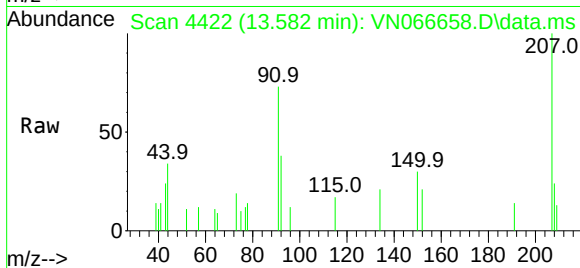

#91
1,2-Dichlorobenzene
Concen: 0.22 ug/l
RT: 13.609 min Scan# 4432
Delta R.T. 0.013 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31

Tgt Ion: 146 Resp: 1264
Ion Ratio Lower Upper
146 100
111 14.6 20.1 60.3#
148 75.0 32.0 96.0


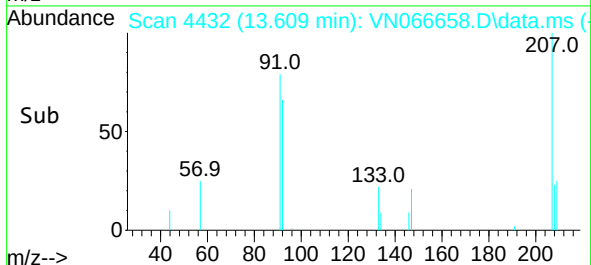

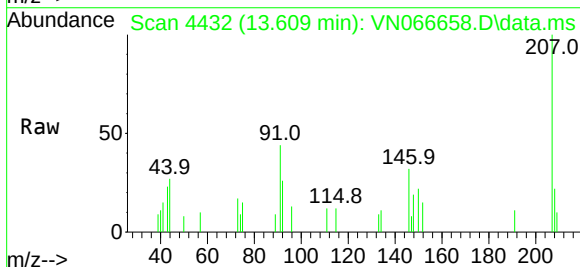


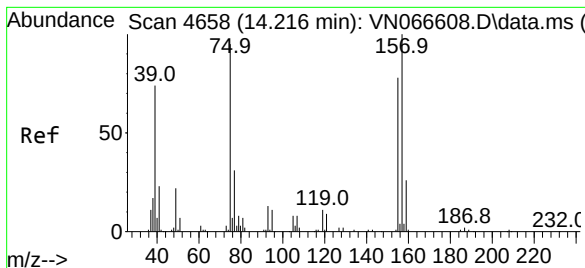

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.29 ug/l
RT: 14.226 min Scan# 4662
Delta R.T. 0.010 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 250
Ion Ratio Lower Upper
75 100
155 0.0 44.1 132.4#
157 0.0 56.0 168.2#

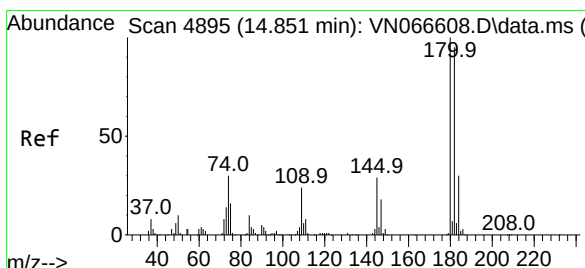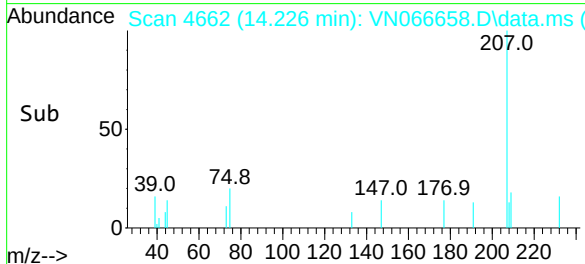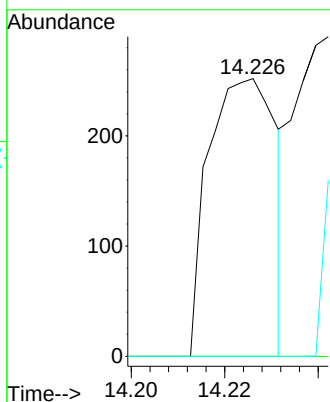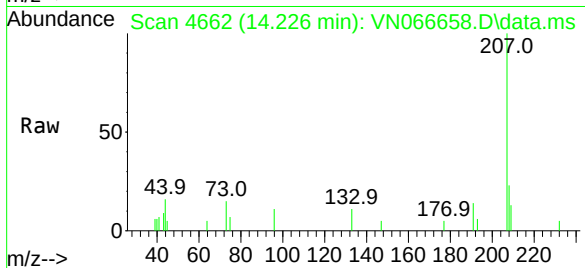

#93
1,2,4-Trichlorobenzene
Concen: 0.90 ug/l
RT: 14.862 min Scan# 4899
Delta R.T. 0.011 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31

Tgt Ion: 180 Resp: 2970
Ion Ratio Lower Upper
180 100
182 110.6 47.3 142.0
145 27.7 15.6 46.8


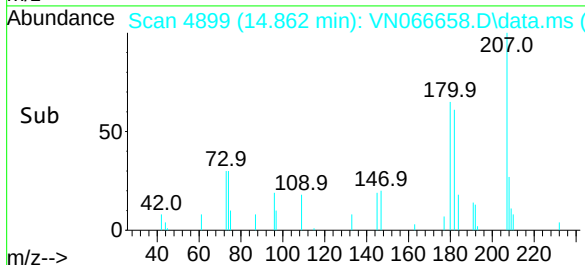
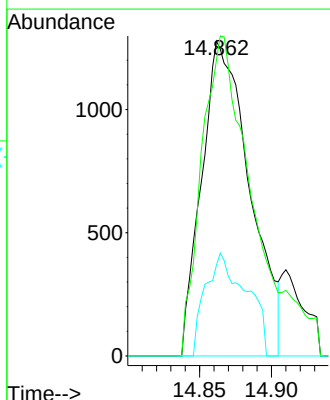
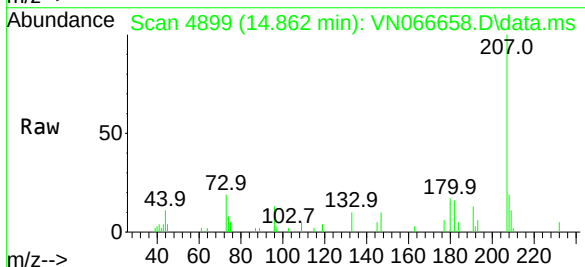


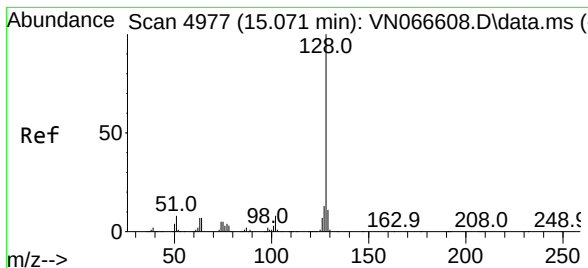

#95
Naphthalene
Concen: 1.94 ug/l
RT: 15.082 min Scan# 4981
Delta R.T. 0.011 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion:	128	Resp:	17625
Ion Ratio	Lower	Upper	
128	100		
127	10.4	10.2	15.2
129	9.1	8.6	13.0

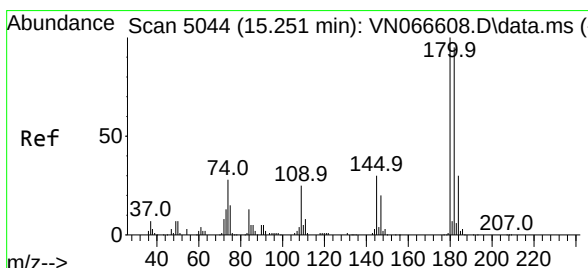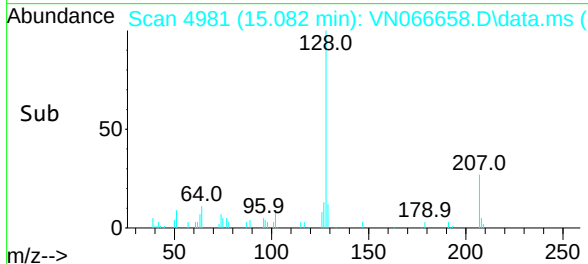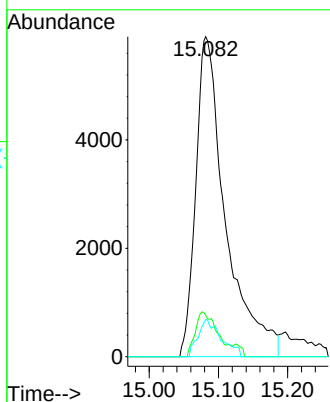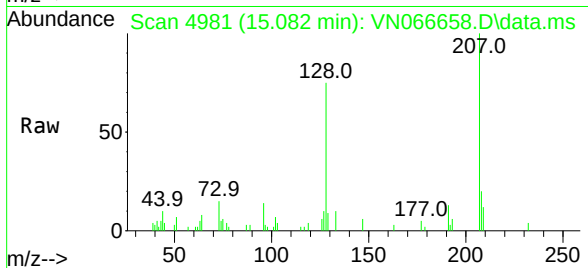

#96
1,2,3-Trichlorobenzene
Concen: 1.28 ug/l
RT: 15.253 min Scan# 5045
Delta R.T. 0.002 min
Lab File: VN066658.D
Acq: 19 Apr 2021 13:31

Tgt Ion:	180	Resp:	4341
Ion Ratio	Lower	Upper	
180	100		
182	90.7	47.4	142.3
145	32.7	16.5	49.5

