

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN041921\  
 Data File : VN066663.D  
 Acq On : 19 Apr 2021 15:29  
 Operator : JC/MD  
 Sample : M2075-20  
 Misc : 5.00mL/MSVOA\_N/WATER  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :

Quant Time: Apr 20 04:56:59 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N041521W.M  
 Quant Title : SW846 8260  
 QLast Update : Thu Apr 15 19:16:35 2021  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response   | Conc    | Units  | Dev(Min) |
|-------------------------------|----------------|------|------------|---------|--------|----------|
| -----                         |                |      |            |         |        |          |
| Internal Standards            |                |      |            |         |        |          |
| 1) Pentafluorobenzene         | 7.591          | 168  | 284533     | 50.00   | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 8.519          | 114  | 445823     | 50.00   | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 11.348         | 117  | 421367     | 50.00   | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 13.287         | 152  | 175089     | 50.00   | ug/l   | 0.00     |
|                               |                |      |            |         |        |          |
| System Monitoring Compounds   |                |      |            |         |        |          |
| 33) 1,2-Dichloroethane-d4     | 7.953          | 65   | 203830     | 47.49   | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 61 - 141 |      | Recovery = | 94.98%  |        |          |
| 35) Dibromofluoromethane      | 7.513          | 113  | 164747     | 53.29   | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 69 - 133 |      | Recovery = | 106.58% |        |          |
| 50) Toluene-d8                | 10.029         | 98   | 650301     | 53.67   | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 65 - 126 |      | Recovery = | 107.34% |        |          |
| 62) 4-Bromofluorobenzene      | 12.346         | 95   | 207044     | 48.59   | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 58 - 135 |      | Recovery = | 97.18%  |        |          |
|                               |                |      |            |         |        |          |
| Target Compounds              |                |      |            |         |        | Qvalue   |
| 3) Chloromethane              | 2.037          | 50   | 1324       | 0.26    | ug/l   | 97       |
| 11) Tert butyl alcohol        | 4.689          | 59   | 200        | 0.29    | ug/l # | 73       |
| 13) Acrolein                  | 3.555          | 56   | 727        | 1.98    | ug/l   | 97       |
| 16) Acetone                   | 3.758          | 43   | 46026      | 22.25   | ug/l   | 96       |
| 18) Methyl Acetate            | 4.255          | 43   | 2943       | 0.64    | ug/l   | 95       |
| 20) Methylene Chloride        | 4.466          | 84   | 3834       | 0.95    | ug/l   | 93       |
| 25) 2-Butanone                | 6.757          | 43   | 10057      | 3.97    | ug/l   | 90       |
| 29) Tetrahydrofuran           | 7.140          | 42   | 1121       | 0.66    | ug/l # | 37       |
| 31) Cyclohexane               | 7.591          | 56   | 5564       | 0.90    | ug/l # | 1        |
| 36) 1,1-Dichloropropene       | 7.591          | 75   | 21196      | 4.72    | ug/l # | 48       |
| 37) Ethyl Acetate             | 6.757          | 43   | 10057      | 1.97    | ug/l # | 68       |
| 38) Carbon Tetrachloride      | 7.591          | 117  | 24999      | 5.94    | ug/l # | 18       |
| 43) Isopropyl Acetate         | 8.095          | 43   | 21513      | 2.53    | ug/l # | 87       |
| 45) 1,2-Dichloropropane       | 9.206          | 63   | 871        | 0.22    | ug/l # | 44       |
| 48) Methyl methacrylate       | 9.114          | 41   | 5045       | 1.32    | ug/l # | 10       |
| 51) 4-Methyl-2-Pentanone      | 9.924          | 43   | 5637       | 1.13    | ug/l # | 73       |
| 54) cis-1,3-Dichloropropene   | 9.844          | 75   | 37627      | 6.41    | ug/l # | 65       |
| 56) Ethyl methacrylate        | 10.321         | 69   | 146        | 0.92    | ug/l # | 27       |
| 57) 1,3-Dichloropropane       | 10.705         | 76   | 15335      | 2.61    | ug/l # | 43       |
| 59) 2-Hexanone                | 10.707         | 43   | 227697     | 67.44   | ug/l # | 49       |
| 71) Bromoform                 | 12.349         | 173  | 1421       | 0.57    | ug/l # | 1        |
| 74) N-amyl acetate            | 12.014         | 43   | 175        | 9.76    | ug/l # | 42       |
| 76) 1,2,3-Trichloropropane    | 12.346         | 75   | 99952      | 24.41   | ug/l # | 100      |
| 81) trans-1,4-Dichloro-2-b... | 12.346         | 75   | 99952      | 75.43   | ug/l # | 12       |
| -----                         |                |      |            |         |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN041921\  
Data File : VN066663.D  
Acq On : 19 Apr 2021 15:29  
Operator : JC/MD  
Sample : M2075-20  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :

Quant Time: Apr 20 04:56:59 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N041521W.M  
Quant Title : SW846 8260  
QLast Update : Thu Apr 15 19:16:35 2021  
Response via : Initial Calibration

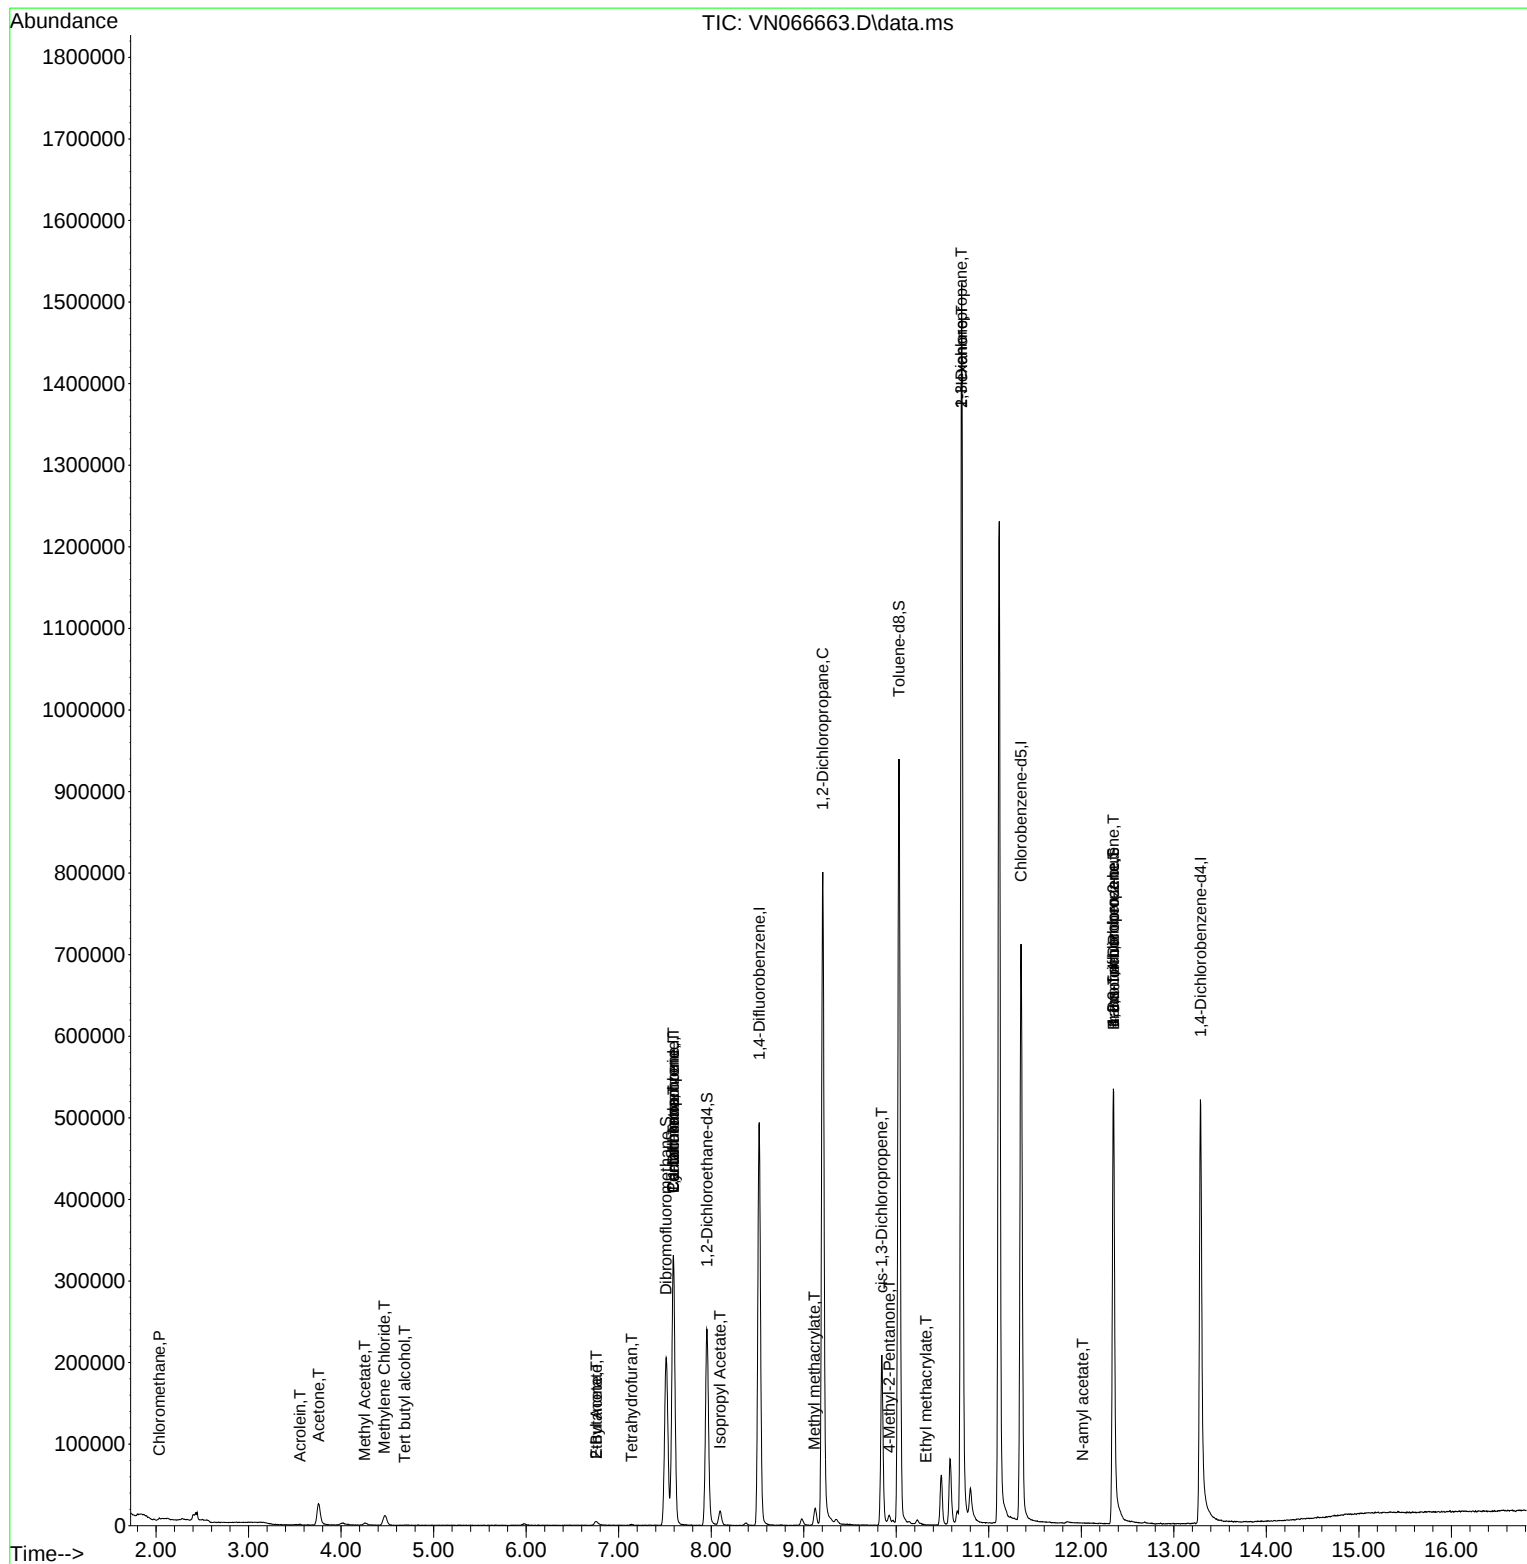

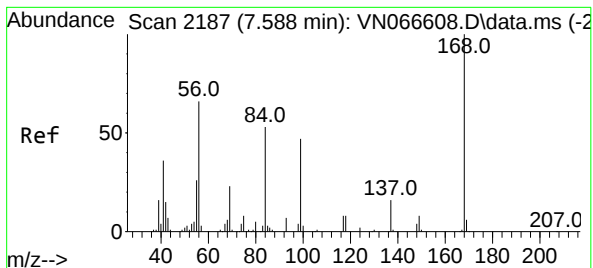

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.591 min Scan# 2188

Delta R.T. 0.003 min





Lab File: VN066663.D

Acq: 19 Apr 2021 15:29

Tgt Ion:168 Resp: 284533

Ion Ratio Lower Upper

|     |      |      |      |
|-----|------|------|------|
| 168 | 100  |      |      |
| 99  | 52.3 | 42.6 | 63.8 |

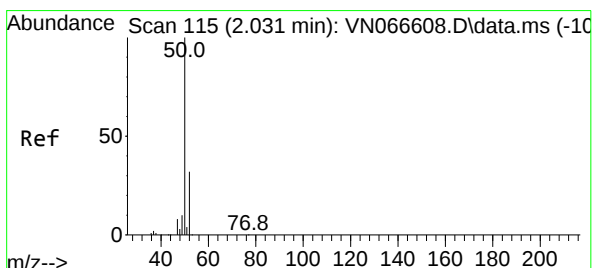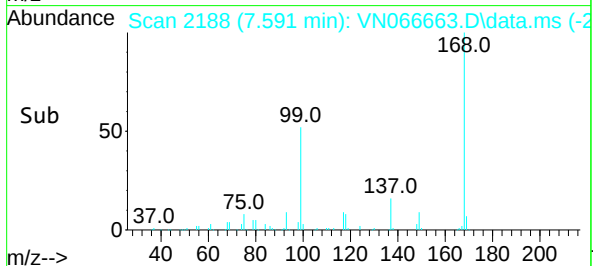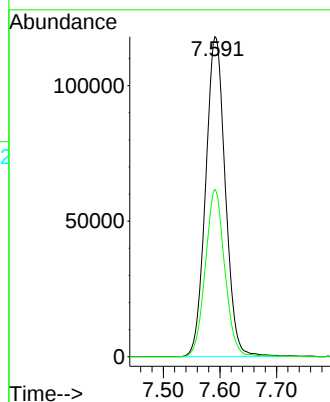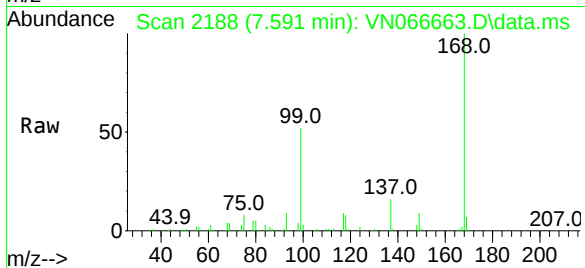

#3

Chloromethane

Concen: 0.26 ug/l

RT: 2.037 min Scan# 117

Delta R.T. 0.006 min




Lab File: VN066663.D


Acq: 19 Apr 2021 15:29

Tgt Ion: 50 Resp: 1324

Ion Ratio Lower Upper

|    |      |      |      |
|----|------|------|------|
| 50 | 100  |      |      |
| 52 | 30.9 | 25.8 | 38.8 |

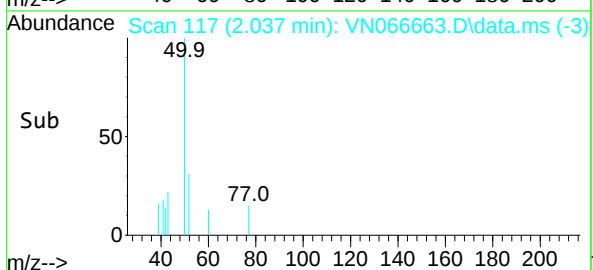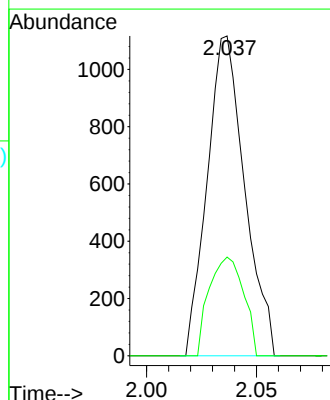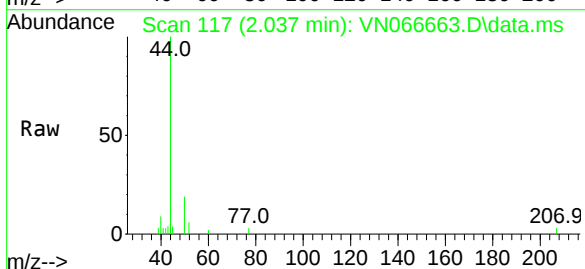




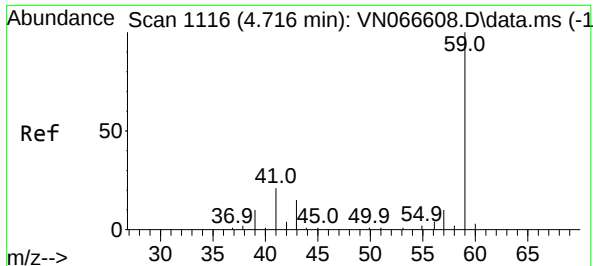


#11

Tert butyl alcohol  
Concen: 0.29 ug/l  
RT: 4.689 min Scan# 1106  
Delta R.T. -0.027 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29

Instrument :  
MSVOA\_N  
ClientSampled :




Tgt Ion: 59 Resp: 200  
Ion Ratio Lower Upper  
59 100  
57 0.0 8.0 12.0#

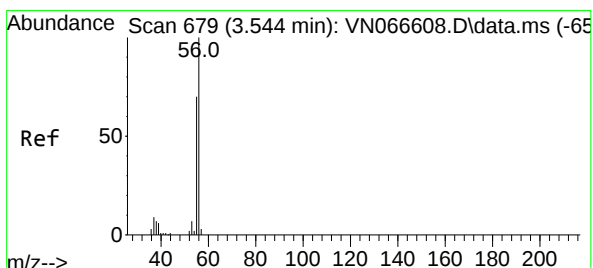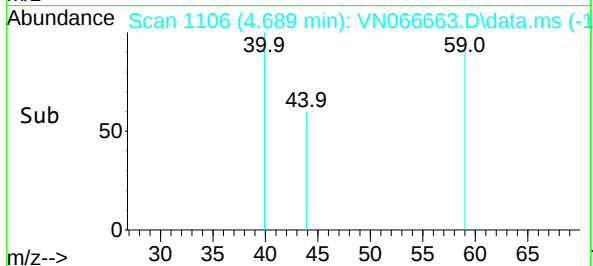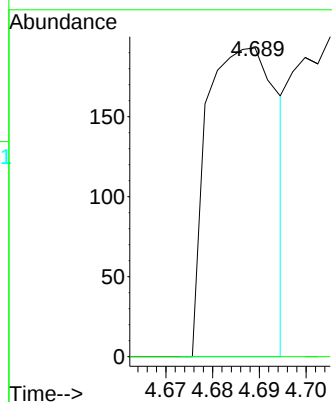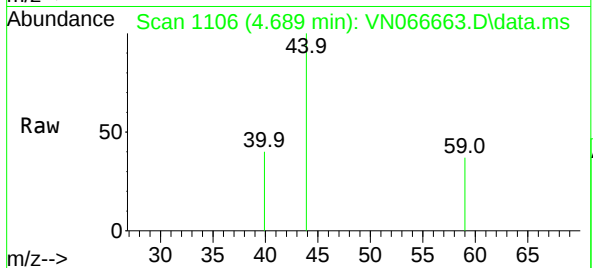


#13

Acrolein  
Concen: 1.98 ug/l  
RT: 3.555 min Scan# 683  
Delta R.T. 0.011 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29

Tgt Ion: 56 Resp: 727  
Ion Ratio Lower Upper  
56 100  
55 72.8 56.0 84.0


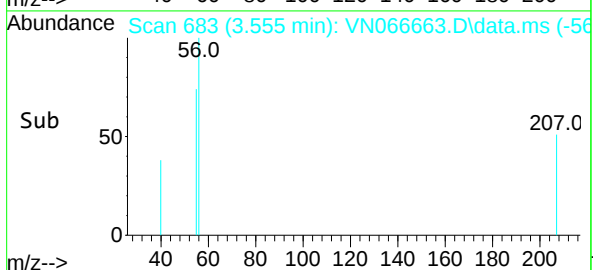

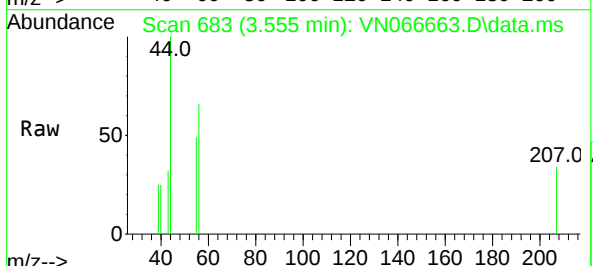




#16  
Acetone  
Concen: 22.25 ug/l  
RT: 3.758 min Scan# 759  
Delta R.T. 0.005 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 43 Resp: 46026  
Ion Ratio Lower Upper  
43 100  
58 31.4 27.0 40.6

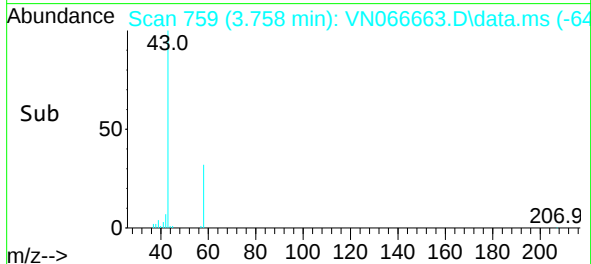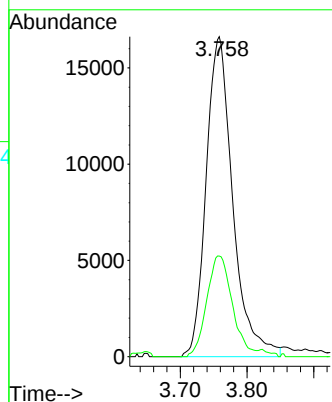

#18  
Methyl Acetate  
Concen: 0.64 ug/l  
RT: 4.255 min Scan# 944  
Delta R.T. 0.006 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29


Tgt Ion: 43 Resp: 2943  
Ion Ratio Lower Upper  
43 100  
74 26.9 19.5 29.3

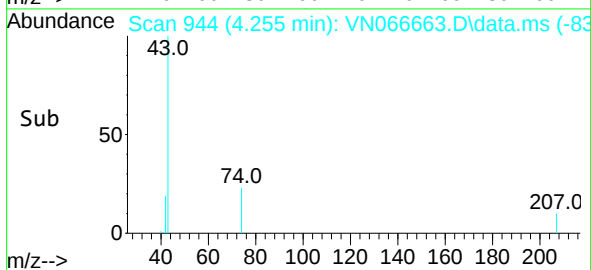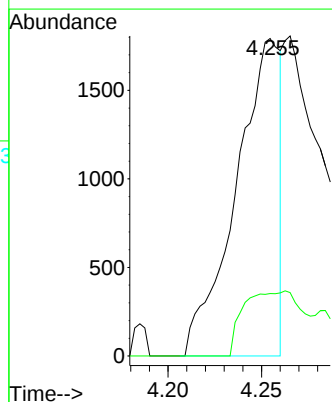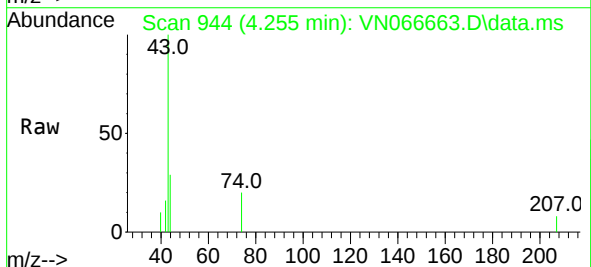



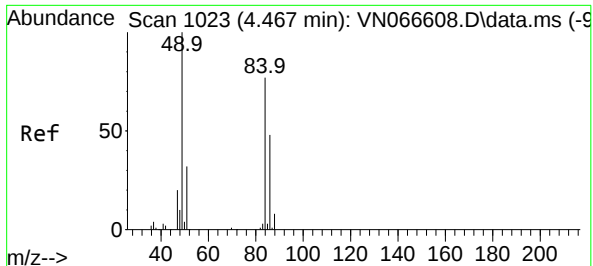


#20  
Methylene Chloride  
Concen: 0.95 ug/l  
RT: 4.466 min Scan# 1023  
Delta R.T. -0.001 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29

Instrument :  
MSVOA\_N  
ClientSampled :



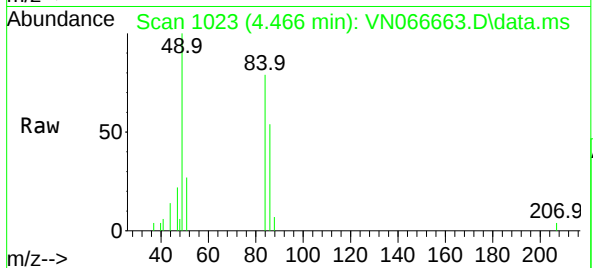



|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 84    | Resp: | 3834  |
| Ion      | Ratio | Lower | Upper |
| 84       | 100   |       |       |
| 49       | 126.2 | 94.6  | 141.8 |
| 51       | 33.8  | 29.9  | 44.9  |
| 86       | 68.7  | 51.4  | 77.2  |

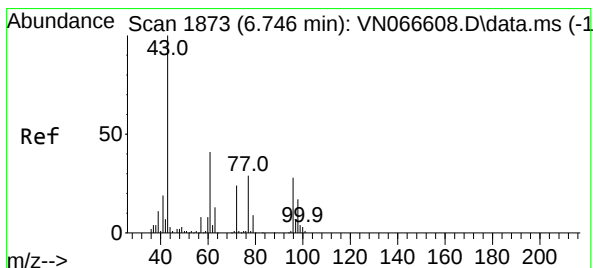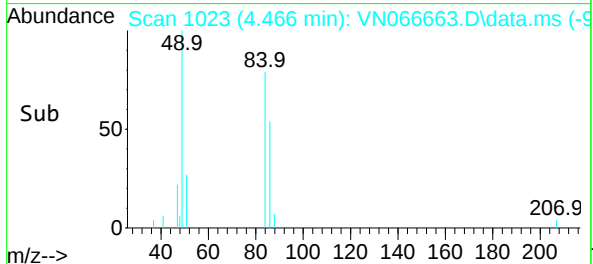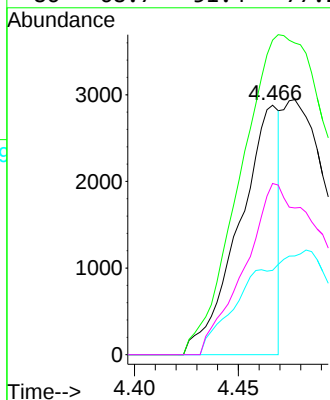

#25  
2-Butanone  
Concen: 3.97 ug/l  
RT: 6.757 min Scan# 1877  
Delta R.T. 0.011 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 43    | Resp: | 10057 |
| Ion      | Ratio | Lower | Upper |
| 43       | 100   |       |       |
| 72       | 23.3  | 23.1  | 34.7  |

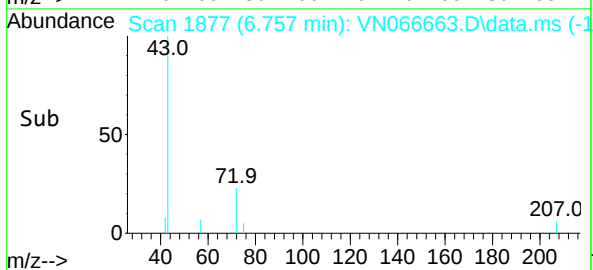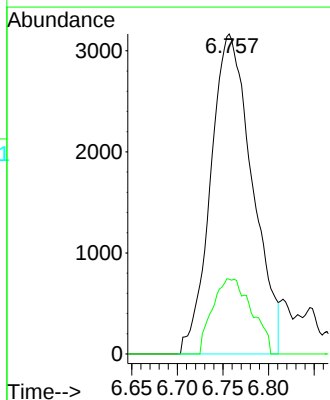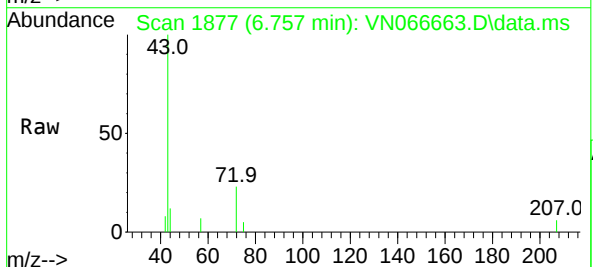

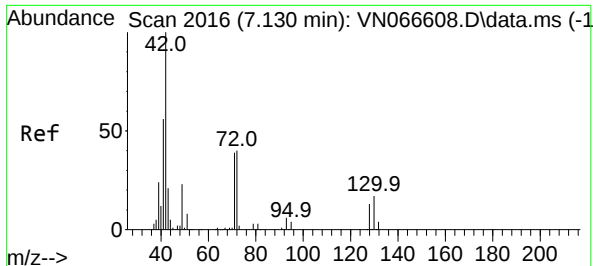

#29

Tetrahydrofuran

Concen: 0.66 ug/l

RT: 7.140 min Scan# 2020





Delta R.T. 0.010 min

Lab File: VN066663.D

Acq: 19 Apr 2021 15:29

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 42    | Resp: | 1121  |
| Ion      | Ratio | Lower | Upper |
| 42       | 100   |       |       |
| 72       | 7.4   | 36.6  | 55.0# |
| 71       | 0.0   | 34.3  | 51.5# |

Instrument :  
MSVOA\_N  
ClientSampled :

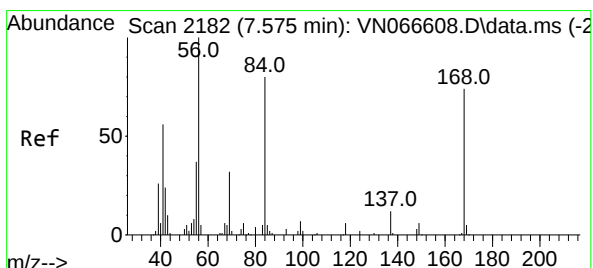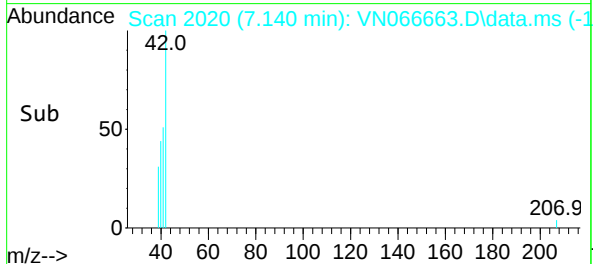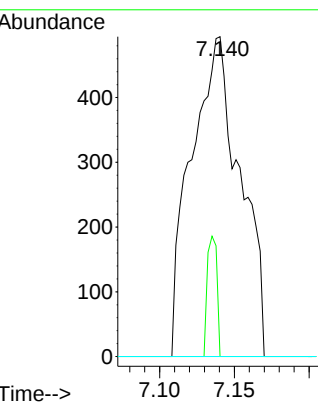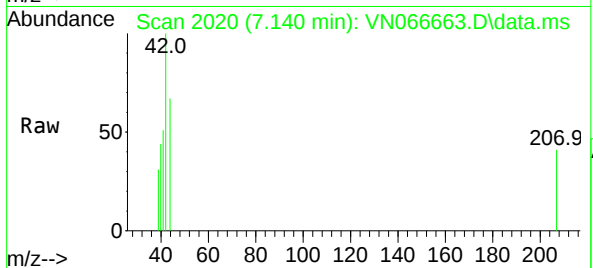

#31

Cyclohexane

Concen: 0.90 ug/l




RT: 7.591 min Scan# 2188


Delta R.T. 0.016 min

Lab File: VN066663.D

Acq: 19 Apr 2021 15:29


|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 56    | Resp: | 5564   |
| Ion      | Ratio | Lower | Upper  |
| 56       | 100   |       |        |
| 69       | 181.7 | 26.6  | 39.8#  |
| 84       | 152.9 | 70.4  | 105.6# |

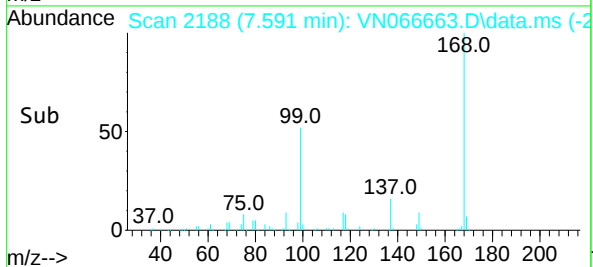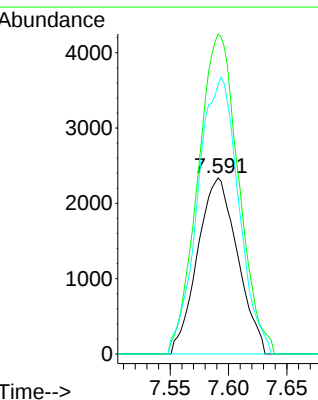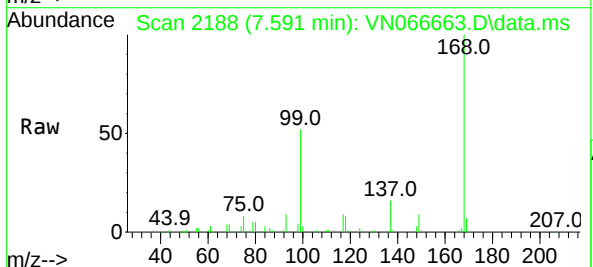






#33  
 1,2-Dichloroethane-d4  
 Concen: 47.49 ug/l  
 RT: 7.953 min Scan# 2323  
 Delta R.T. 0.000 min  
 Lab File: VN066663.D  
 Acq: 19 Apr 2021 15:29

Instrument :  
 MSVOA\_N  
 ClientSampled :







Tgt Ion: 65 Resp: 203830  
 Ion Ratio Lower Upper  
 65 100  
 67 55.1 0.0 107.2

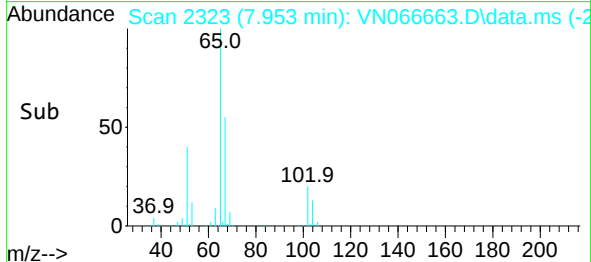

#34  
 1,4-Difluorobenzene  
 Concen: 50.00 ug/l  
 RT: 8.519 min Scan# 2534  
 Delta R.T. -0.000 min  
 Lab File: VN066663.D  
 Acq: 19 Apr 2021 15:29

Tgt Ion: 114 Resp: 445823  
 Ion Ratio Lower Upper  
 114 100  
 63 21.4 0.0 38.6  
 88 15.5 0.0 30.6


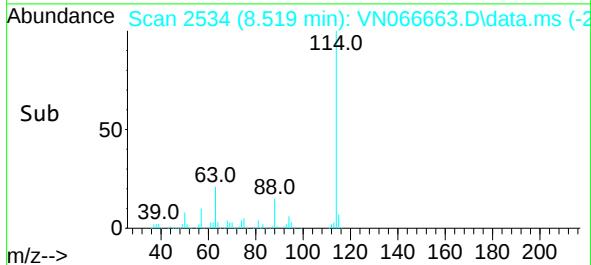

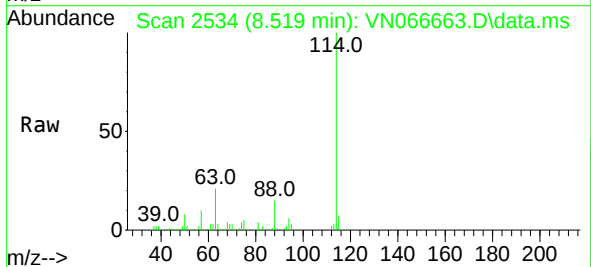




#35  
Dibromofluoromethane  
Concen: 53.29 ug/l  
RT: 7.513 min Scan# 2159  
Delta R.T. 0.002 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion:113 Resp: 164747  
Ion Ratio Lower Upper  
113 100  
111 103.5 82.2 123.2  
192 20.5 15.4 23.0

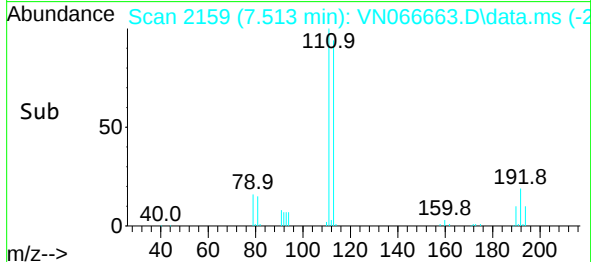

#36  
1,1-Dichloropropene  
Concen: 4.72 ug/l  
RT: 7.591 min Scan# 2188  
Delta R.T. -0.126 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29

Tgt Ion: 75 Resp: 21196  
Ion Ratio Lower Upper  
75 100  
110 8.0 18.2 54.6#  
77 0.0 24.9 37.3#

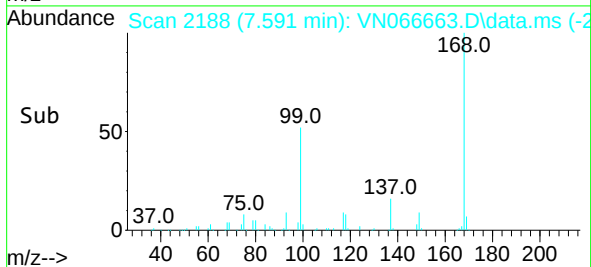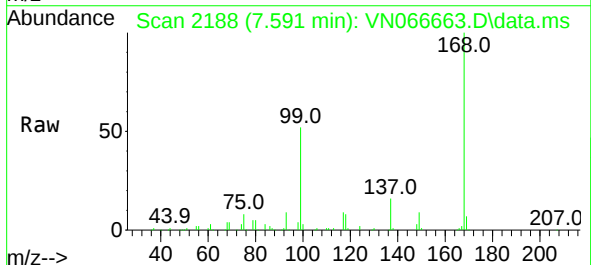

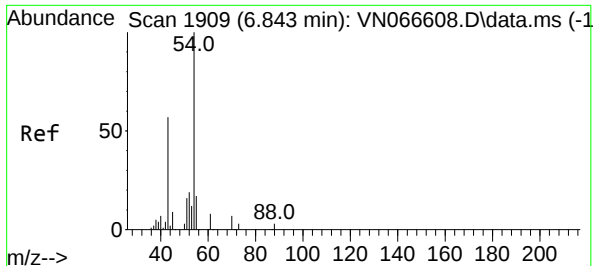

#37

Ethyl Acetate

Concen: 1.97 ug/l

RT: 6.757 min Scan# 1877





Delta R.T. -0.086 min

Lab File: VN066663.D

Acq: 19 Apr 2021 15:29

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 43    | Resp: | 10057 |
| Ion      | Ratio | Lower | Upper |
| 43       | 100   |       |       |
| 61       | 0.0   | 11.6  | 17.4# |
| 70       | 0.0   | 8.6   | 13.0# |

Instrument :  
MSVOA\_N  
ClientSampled :

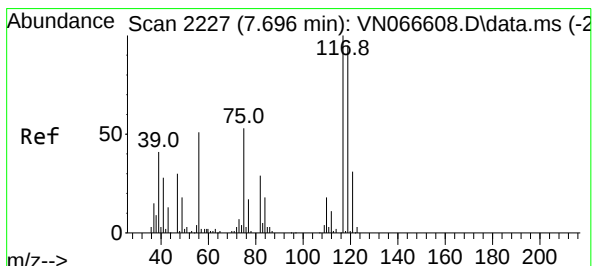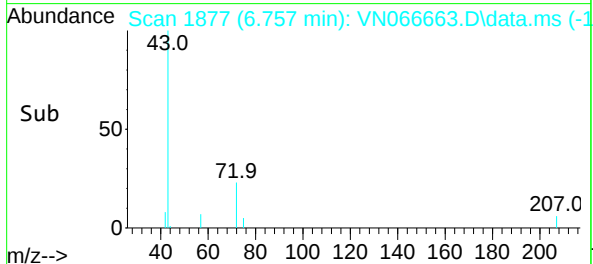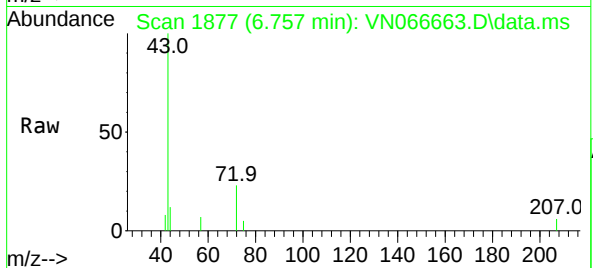

#38

Carbon Tetrachloride

Concen: 5.94 ug/l




RT: 7.591 min Scan# 2188


Delta R.T. -0.105 min

Lab File: VN066663.D

Acq: 19 Apr 2021 15:29


|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 117   | Resp: | 24999  |
| Ion      | Ratio | Lower | Upper  |
| 117      | 100   |       |        |
| 119      | 6.7   | 76.0  | 114.0# |
| 121      | 0.0   | 24.5  | 36.7#  |

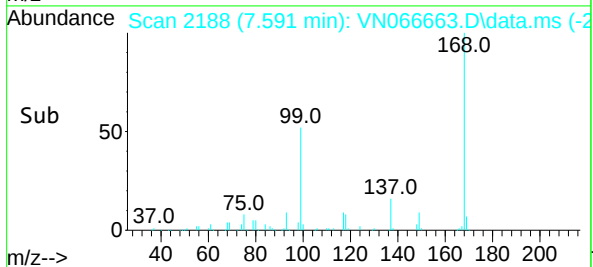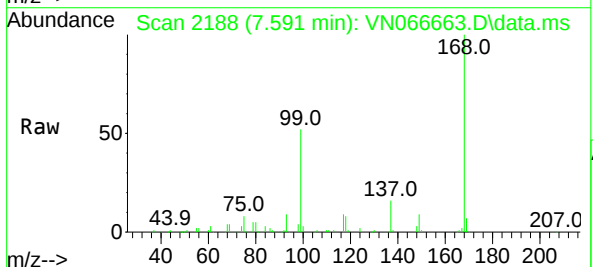






#43  
Isopropyl Acetate  
Concen: 2.53 ug/l  
RT: 8.095 min Scan# 2376  
Delta R.T. 0.000 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29


Instrument :  
MSVOA\_N  
ClientSampled :





Tgt Ion: 43 Resp: 21513  
Ion Ratio Lower Upper  
43 100  
61 19.0 22.5 33.7#  
87 11.6 11.1 16.7

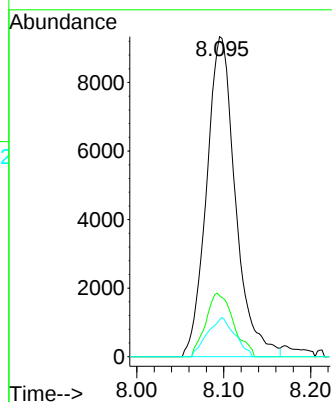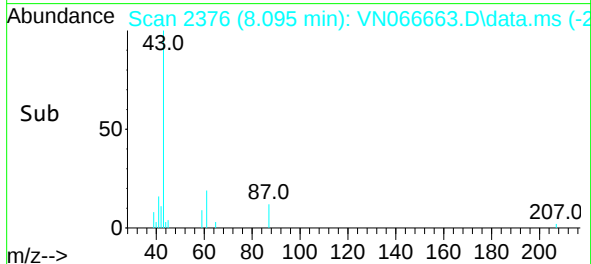


#45  
1,2-Dichloropropane  
Concen: 0.22 ug/l  
RT: 9.206 min Scan# 2790  
Delta R.T. 0.153 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29



Tgt Ion: 63 Resp: 871  
Ion Ratio Lower Upper  
63 100  
65 0.0 24.9 37.3#




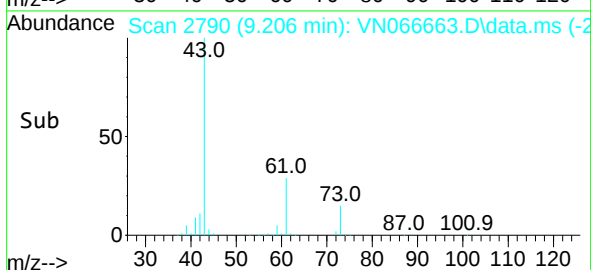




#48  
Methyl methacrylate  
Concen: 1.32 ug/l  
RT: 9.114 min Scan# 2756  
Delta R.T. -0.022 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 41 Resp: 5045  
Ion Ratio Lower Upper  
41 100  
69 0.0 75.9 113.9#  
39 0.0 46.6 69.8#

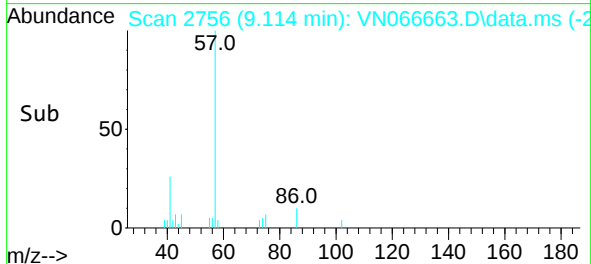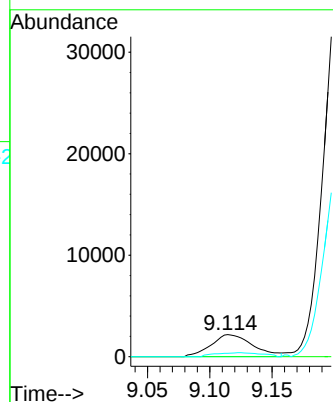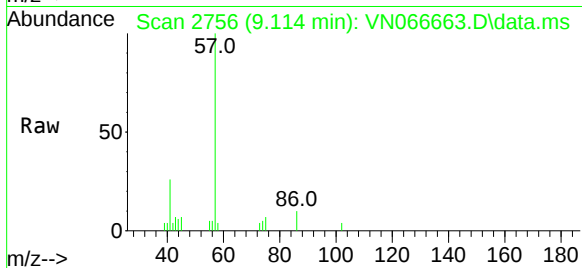

#50  
Toluene-d8  
Concen: 53.67 ug/l  
RT: 10.029 min Scan# 3097  
Delta R.T. -0.000 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29

Tgt Ion: 98 Resp: 650301  
Ion Ratio Lower Upper  
98 100  
100 64.3 50.5 75.7


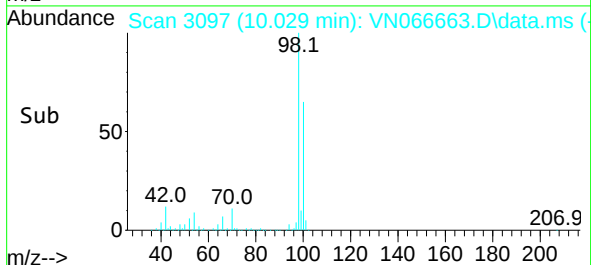
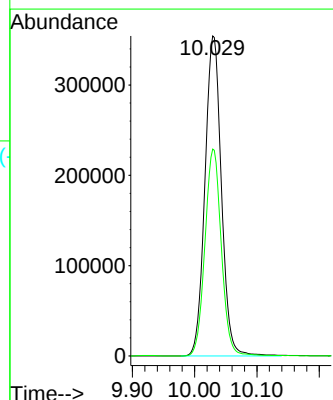
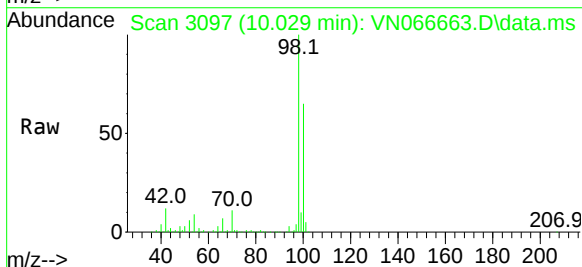




#51  
4-Methyl-2-Pentanone  
Concen: 1.13 ug/l  
RT: 9.924 min Scan# 3058  
Delta R.T. 0.002 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 43 Resp: 5637  
Ion Ratio Lower Upper  
43 100  
58 57.2 32.5 48.7#

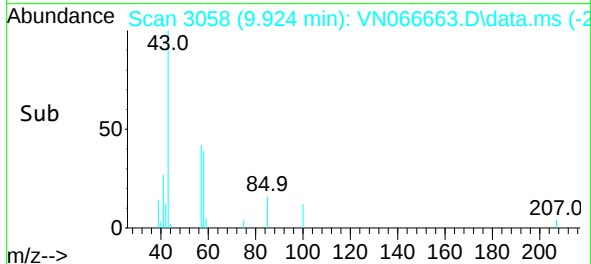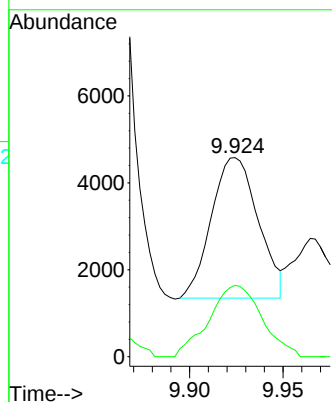

#54  
cis-1,3-Dichloropropene  
Concen: 6.41 ug/l  
RT: 9.844 min Scan# 3028  
Delta R.T. 0.067 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29

Tgt Ion: 75 Resp: 37627  
Ion Ratio Lower Upper  
75 100  
77 0.0 24.9 37.3#  
39 31.9 36.2 54.4#


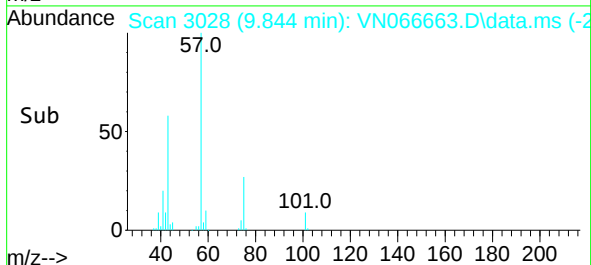

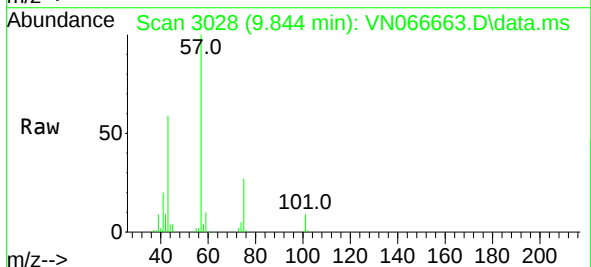


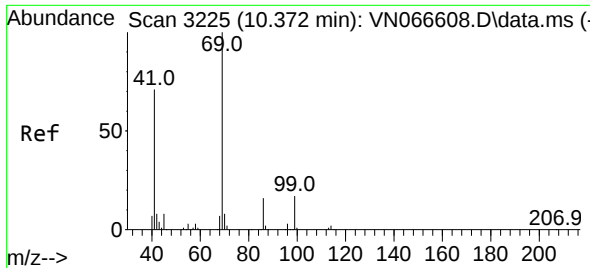

#56  
Ethyl methacrylate  
Concen: 0.92 ug/l  
RT: 10.321 min Scan# 3206  
Delta R.T. -0.051 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 69 Resp: 146  
Ion Ratio Lower Upper  
69 100  
41 0.0 49.6 74.4#  
39 0.0 28.0 42.0#

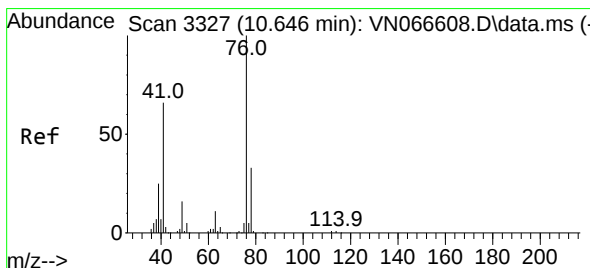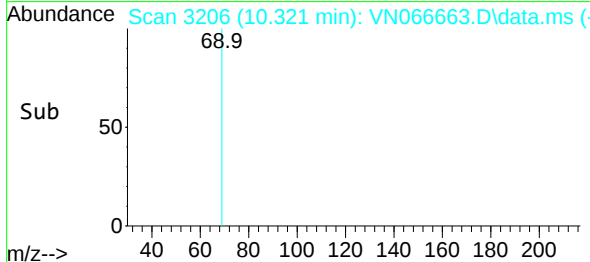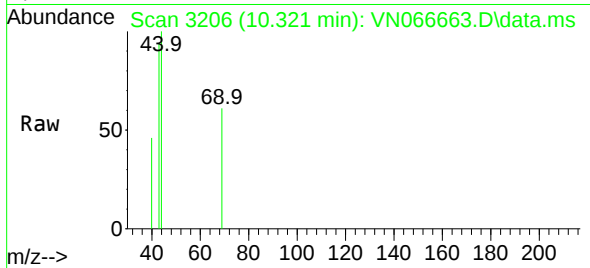

#57  
1,3-Dichloropropane  
Concen: 2.61 ug/l  
RT: 10.705 min Scan# 3349  
Delta R.T. 0.059 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29

Tgt Ion: 76 Resp: 15335  
Ion Ratio Lower Upper  
76 100  
78 0.0 25.7 38.5#


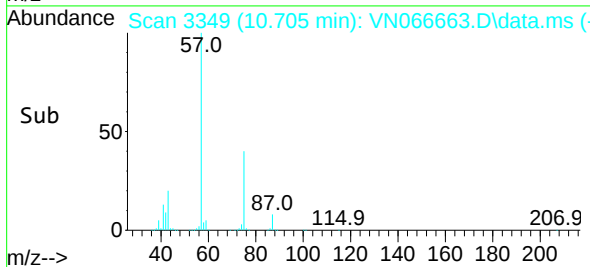

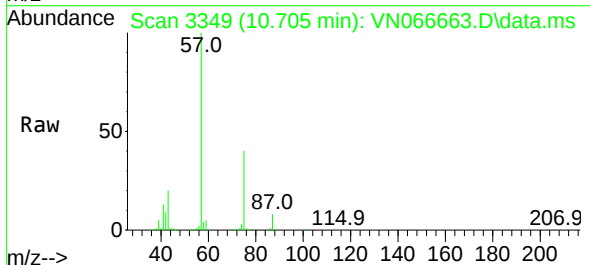


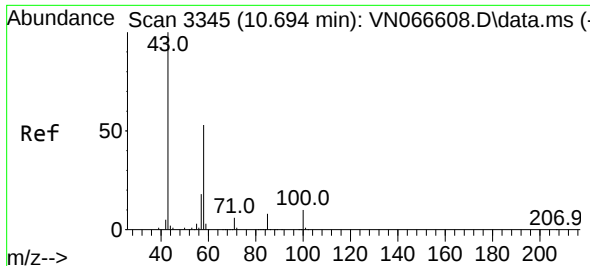

#59  
2-Hexanone  
Concen: 67.44 ug/l  
RT: 10.707 min Scan# 3350  
Delta R.T. 0.013 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 43 Resp: 227697  
Ion Ratio Lower Upper  
43 100  
58 19.1 28.1 84.3#

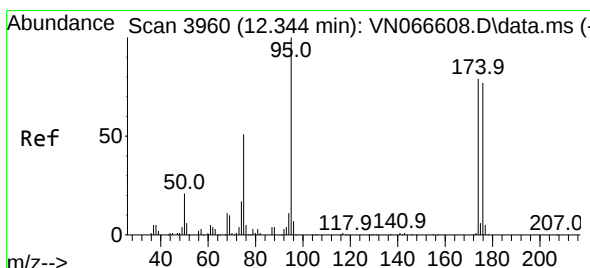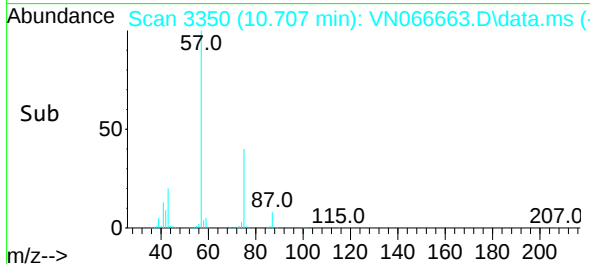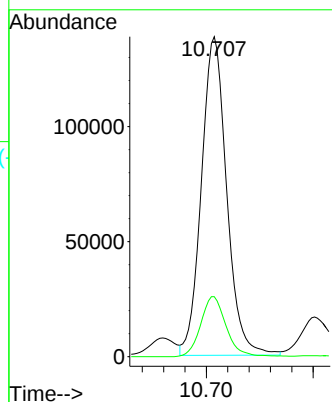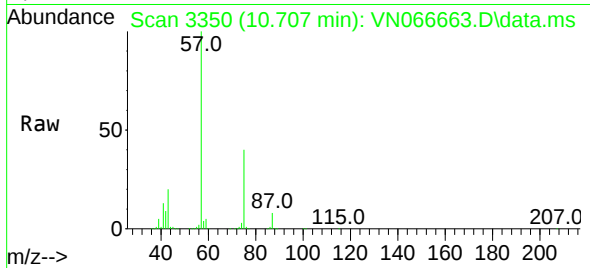

#62  
4-Bromofluorobenzene  
Concen: 48.59 ug/l  
RT: 12.346 min Scan# 3961  
Delta R.T. 0.002 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29

Tgt Ion: 95 Resp: 207044  
Ion Ratio Lower Upper  
95 100  
174 84.9 0.0 169.0  
176 82.3 0.0 162.4


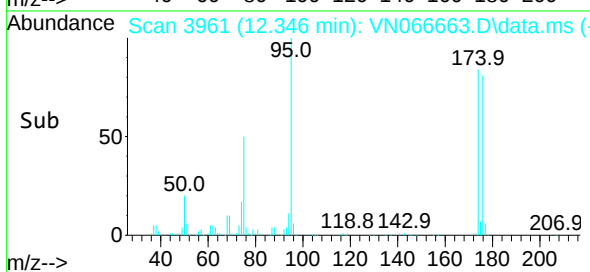
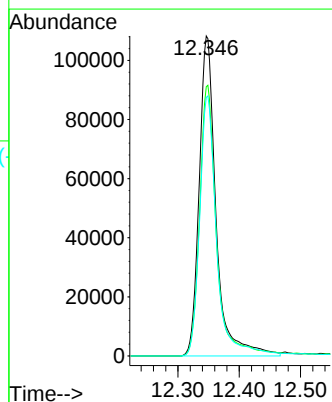
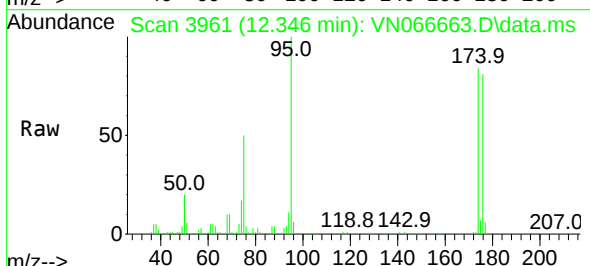


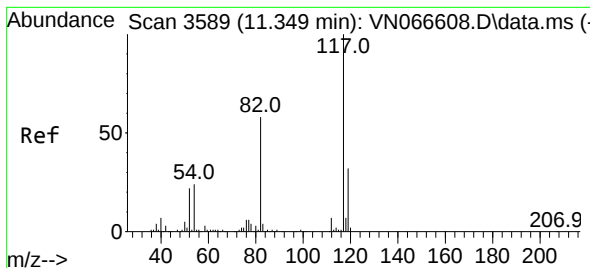

#63  
Chlorobenzene-d5  
Concen: 50.00 ug/l  
RT: 11.348 min Scan# 3589  
Delta R.T. -0.001 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion:117 Resp: 421367  
Ion Ratio Lower Upper  
117 100  
82 56.2 43.7 65.5  
119 32.0 26.1 39.1

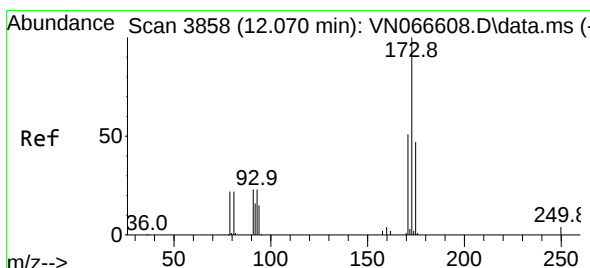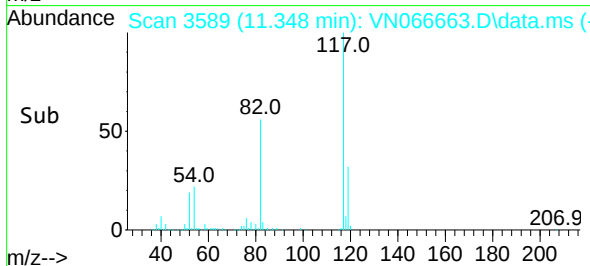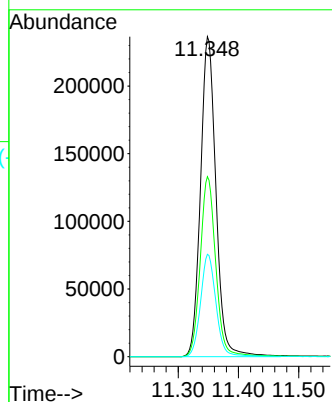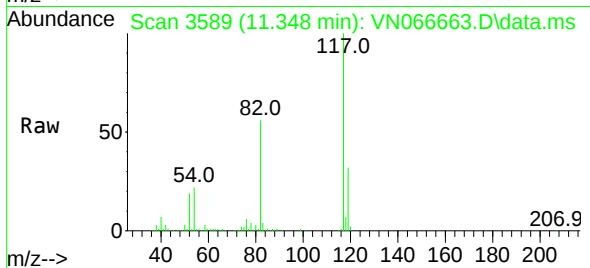

#71  
Bromoform  
Concen: 0.57 ug/l  
RT: 12.349 min Scan# 3962  
Delta R.T. 0.279 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29

Tgt Ion:173 Resp: 1421  
Ion Ratio Lower Upper  
173 100  
175 727.3 23.8 71.2#  
254 0.0 0.0 0.0


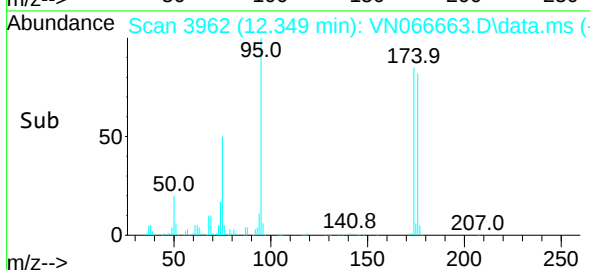

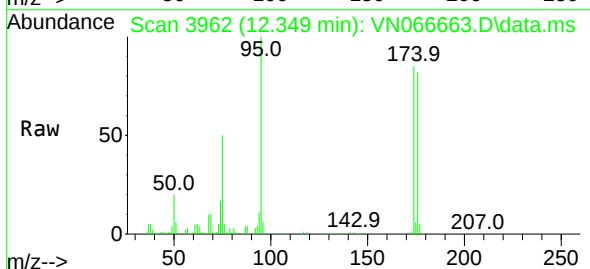




#72  
1,4-Dichlorobenzene-d4  
Concen: 50.00 ug/l  
RT: 13.287 min Scan# 4312  
Delta R.T. -0.001 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion:152 Resp: 175089  
Ion Ratio Lower Upper  
152 100  
115 56.2 28.5 85.6  
150 159.7 0.0 347.6

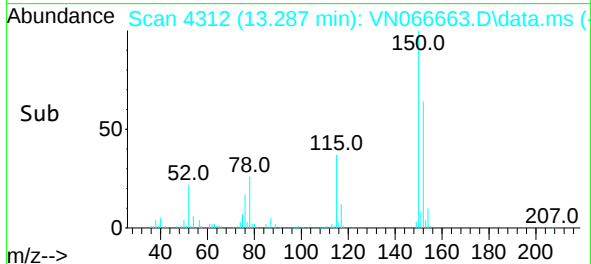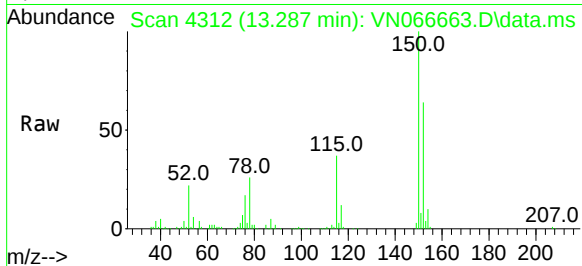

#74  
N-ethyl acetate  
Concen: 9.76 ug/l  
RT: 12.014 min Scan# 3837  
Delta R.T. -0.005 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29

Tgt Ion: 43 Resp: 175  
Ion Ratio Lower Upper  
43 100  
70 0.0 34.4 51.6#  
55 0.0 20.7 31.1#  
61 0.0 19.1 28.7#


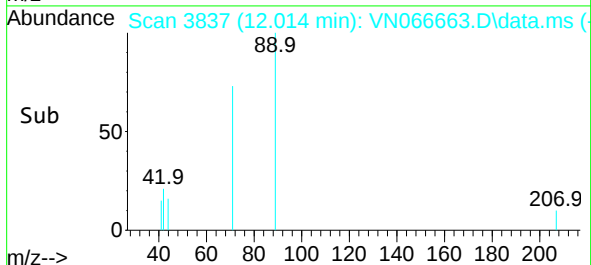
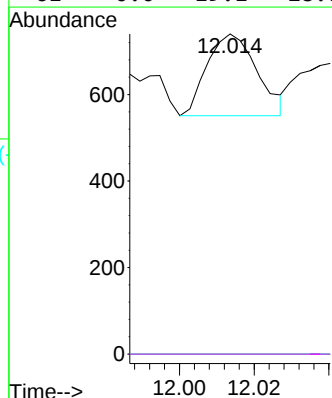
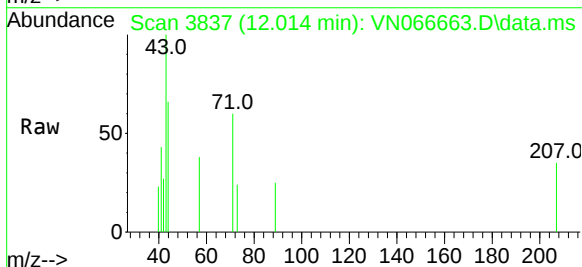




#76  
1,2,3-Trichloropropane  
Concen: 24.41 ug/l  
RT: 12.346 min Scan# 3961  
Delta R.T. -0.150 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29

Instrument :  
MSVOA\_N  
ClientSampled :

Tgt Ion: 75 Resp: 99952  
Ion Ratio Lower Upper  
75 100  
77 1.4 0.0 0.0#

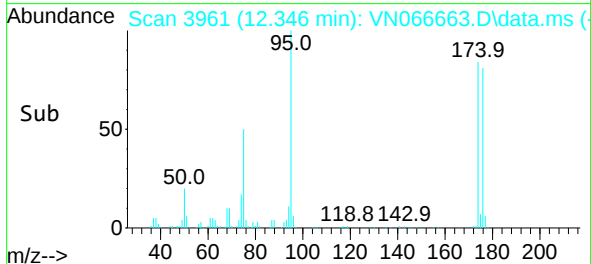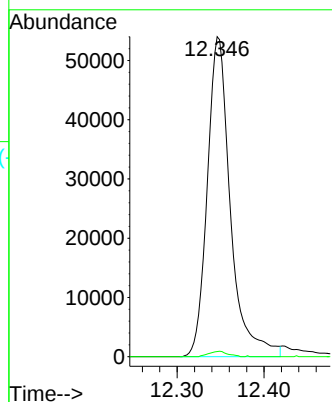

#81  
trans-1,4-Dichloro-2-butene  
Concen: 75.43 ug/l  
RT: 12.346 min Scan# 3961  
Delta R.T. 0.102 min  
Lab File: VN066663.D  
Acq: 19 Apr 2021 15:29

Tgt Ion: 75 Resp: 99952  
Ion Ratio Lower Upper  
75 100  
53 0.0 74.6 111.8#  
89 0.2 35.8 53.8#

