


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041921\
Data File : VN066650.D
Acq On : 19 Apr 2021 9:43
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041521W.M
Title : SW846 8260
Last Update : Thu Apr 15 19:16:35 2021

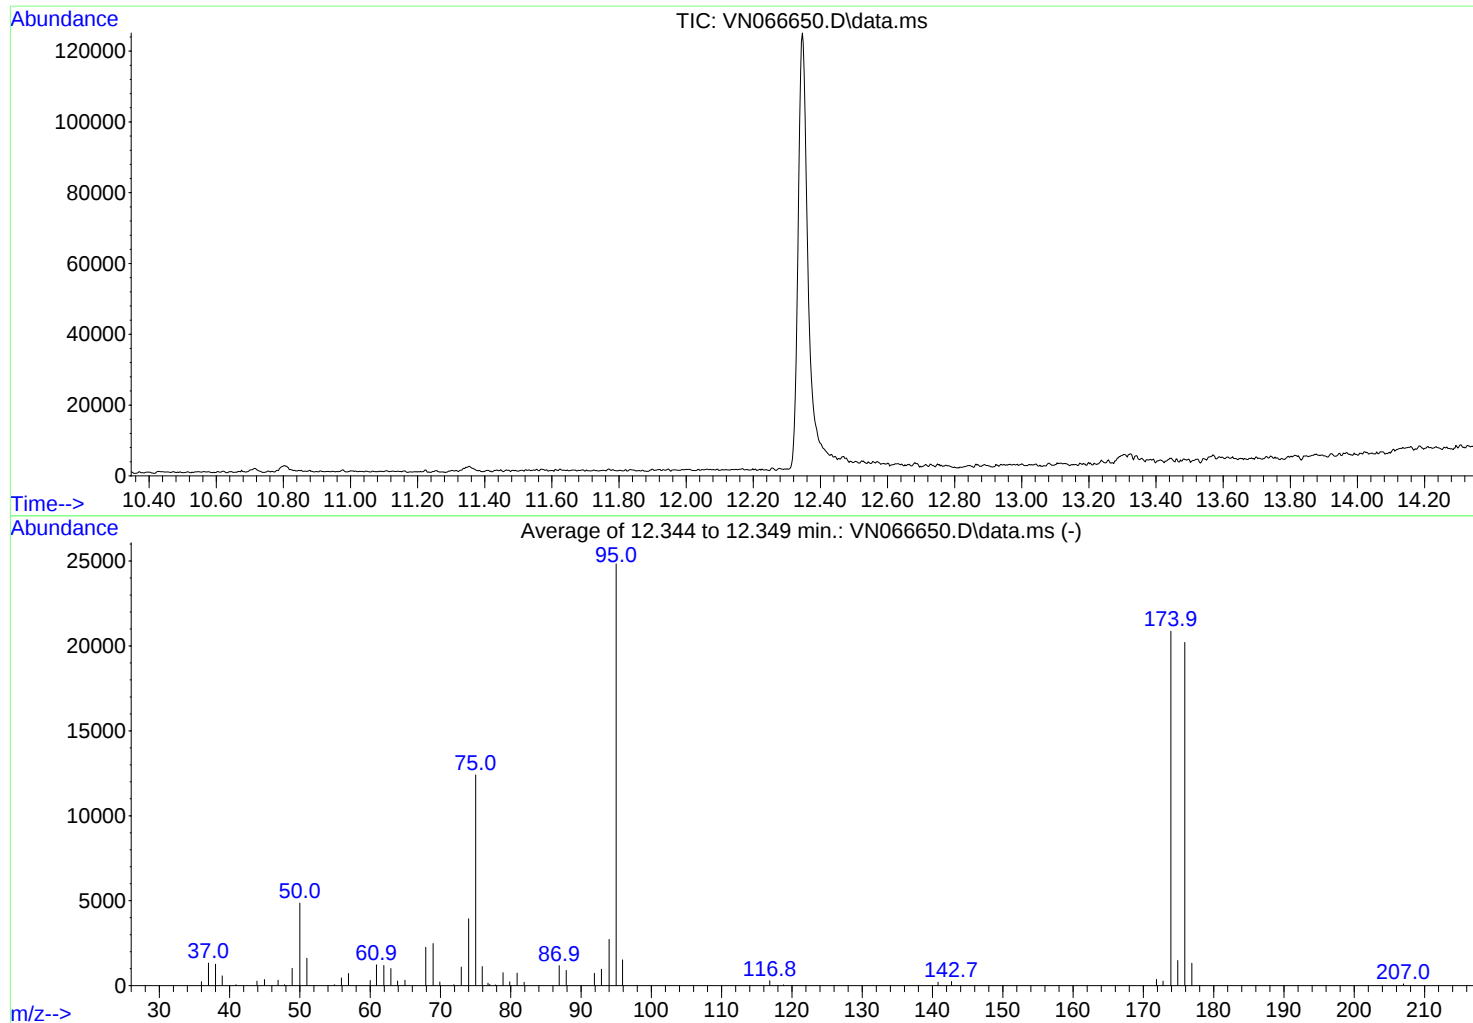

AutoFind: Scans 3960, 3961, 3962; Background Corrected with Scan 3945

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	4863	PASS
75	95	30	60	49.9	12403	PASS
95	95	100	100	100.0	24835	PASS
96	95	5	9	6.1	1513	PASS
173	174	0.00	2	1.3	266	PASS
174	95	50	100	84.0	20867	PASS
175	174	5	9	7.1	1481	PASS
176	174	95	101	96.9	20211	PASS
177	176	5	9	6.5	1318	PASS