

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041922\
 Data File : VN072055.D
 Acq On : 19 Apr 2022 17:26
 Operator : JC\MD
 Sample : N2468-06
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 WC-15-1-7-GR

Quant Time: Apr 20 01:27:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 31 01:57:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.081	168	561490	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	949700	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1138687	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.669	152	432374	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.428	65	296692	46.285	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	92.580%
35) Dibromofluoromethane	8.016	113	258536	46.263	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	92.520%
50) Toluene-d8	10.433	98	1280693	56.021	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	112.040%
62) 4-Bromofluorobenzene	12.727	95	464878	62.876	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	125.760%
Target Compounds						
					Qvalue	
3) Chloromethane	2.293	50	1807	0.319	ug/l #	80
5) Bromomethane	2.816	94	961	0.238	ug/l #	59
11) Tert butyl alcohol	5.363	59	256	0.246	ug/l #	72
13) Acrolein	4.034	56	1185	0.934	ug/l #	75
14) Allyl chloride	5.081	41	10958	1.457	ug/l #	24
16) Acetone	4.293	43	63787	23.285	ug/l	99
17) Carbon Disulfide	4.499	76	6980	0.656	ug/l #	95
18) Methyl Acetate	4.857	43	28154	2.719	ug/l	97
20) Methylene Chloride	5.075	84	336937	58.354	ug/l	97
25) 2-Butanone	7.340	43	20240	5.125	ug/l	94
29) Tetrahydrofuran	7.704	42	682	0.267	ug/l #	54
31) Cyclohexane	8.069	56	9523	1.092	ug/l #	8
36) 1,1-Dichloropropene	8.075	75	37342	4.785	ug/l #	48
37) Ethyl Acetate	7.340	43	20240	2.370	ug/l #	67
38) Carbon Tetrachloride	8.075	117	50019	6.540	ug/l #	17
43) Isopropyl Acetate	8.557	43	106412	7.490	ug/l #	74
45) 1,2-Dichloropropane	9.616	63	3965	0.644	ug/l #	44
48) Methyl methacrylate	9.545	41	15084	2.559	ug/l #	10
49) 1,4-Dioxane	9.616	88	344	Below Cal	#	1
51) 4-Methyl-2-Pentanone	10.333	43	9209	1.127	ug/l #	77
52) Toluene	10.498	92	18927	1.215	ug/l	94
54) cis-1,3-Dichloropropene	10.239	75	98681	10.353	ug/l #	58
57) 1,3-Dichloropropane	11.086	76	55006	5.130	ug/l #	42
59) 2-Hexanone	11.086	43	675150	117.395	ug/l #	48
74) N-amyl acetate	12.357	43	3186	0.305	ug/l #	42
76) 1,2,3-Trichloropropane	12.727	75	225047	22.468	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.727	75	225047	69.628	ug/l #	10
84) 1,2,4-Trimethylbenzene	13.363	105	8035	0.285	ug/l	89
95) Naphthalene	15.504	128	2164	3.904	ug/l #	82
96) 1,2,3-Trichlorobenzene	15.704	180	108	2.430	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041922\
Data File : VN072055.D
Acq On : 19 Apr 2022 17:26
Operator : JC\MD
Sample : N2468-06
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7-GR

Quant Time: Apr 20 01:27:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 31 01:57:54 2022
Response via : Initial Calibration




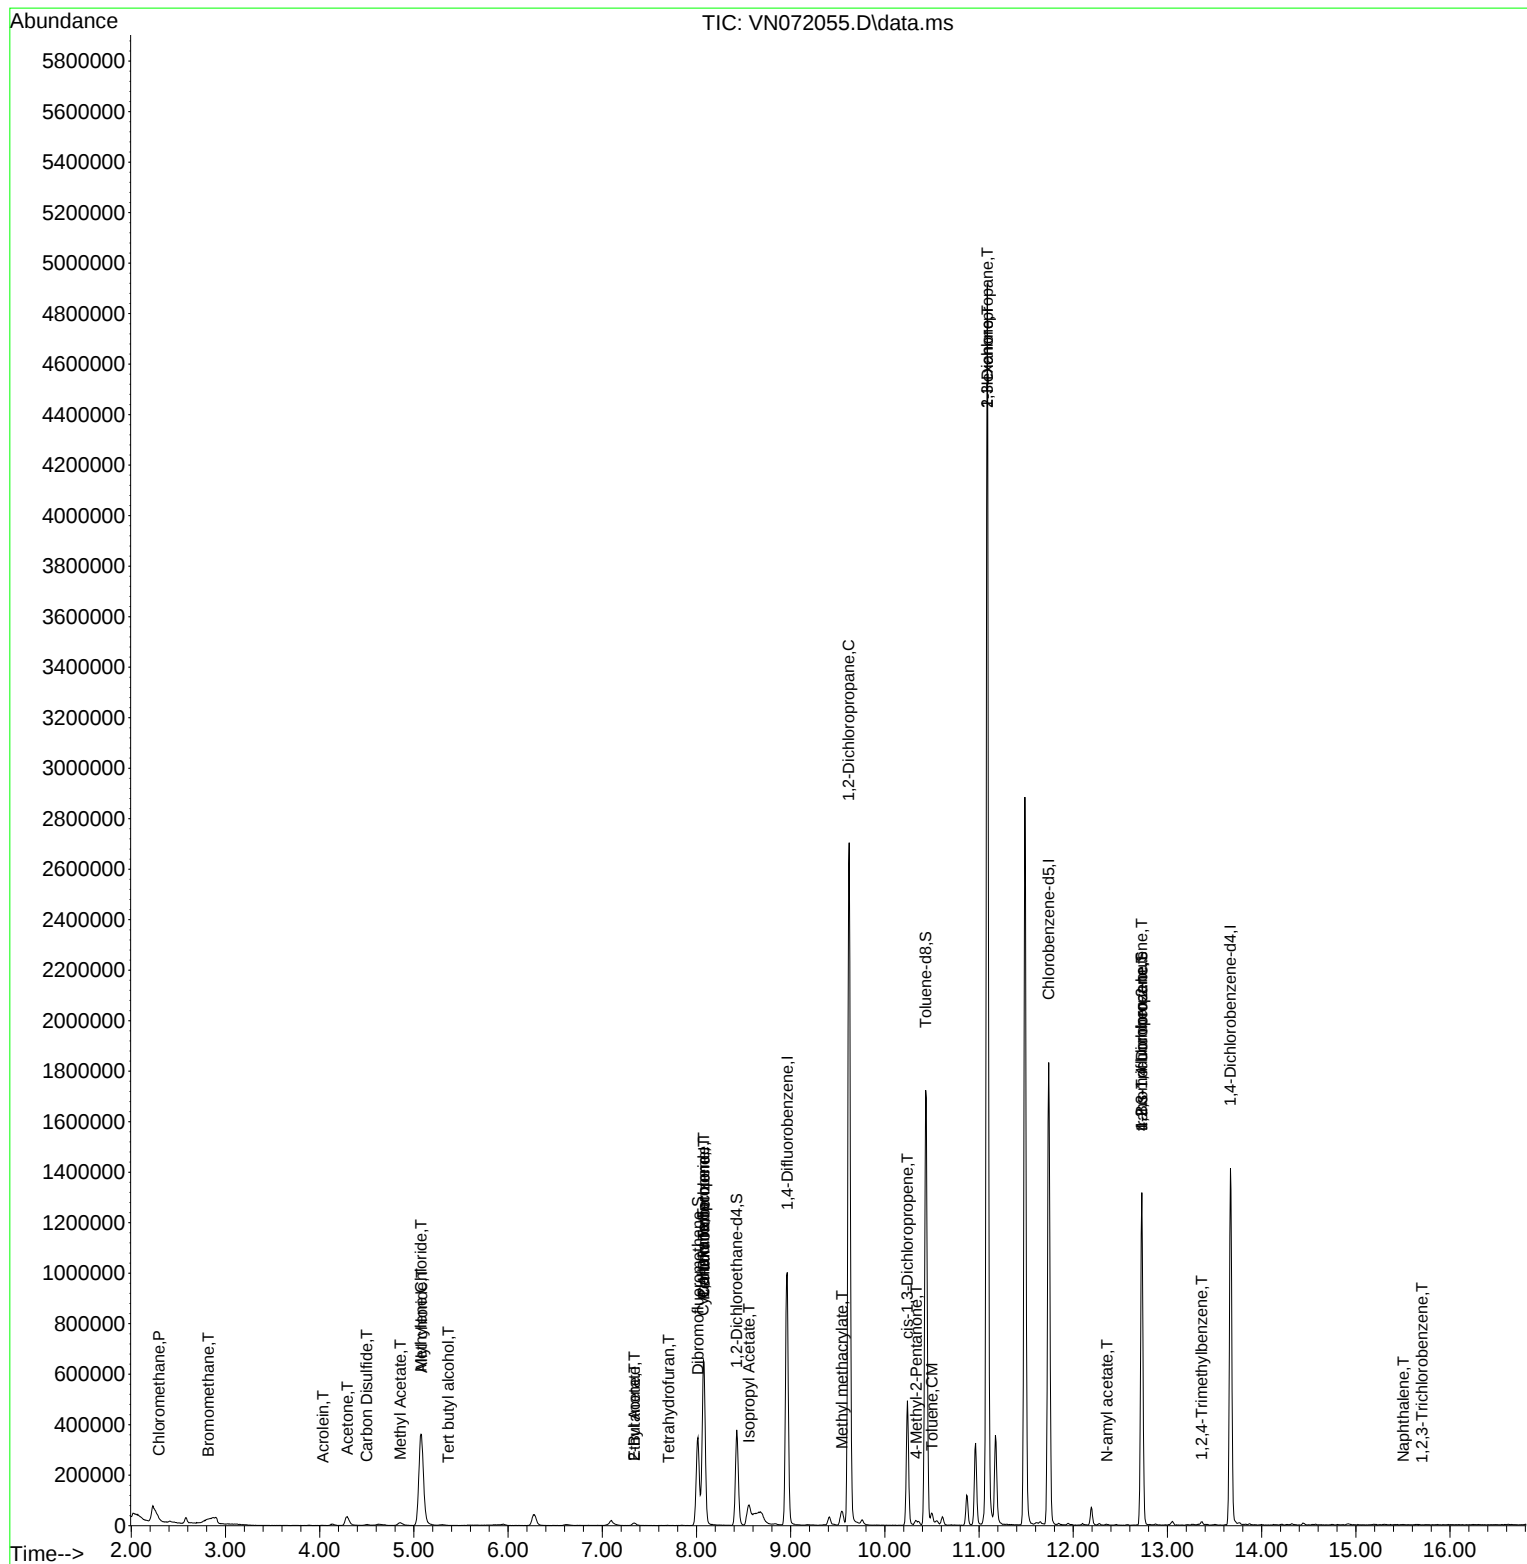




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.000 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7-GR


Tgt Ion:168 Resp: 561490
Ion Ratio Lower Upper
168 100
99 51.0 42.3 63.5

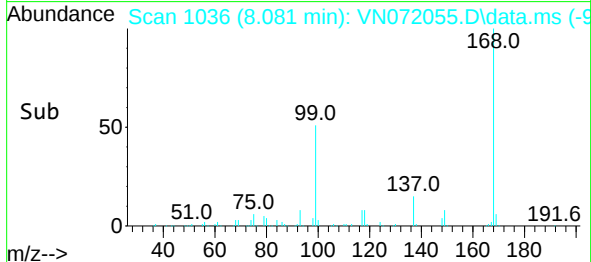

#3
Chloromethane
Concen: 0.319 ug/l
RT: 2.293 min Scan# 52
Delta R.T. -0.006 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26

Tgt Ion: 50 Resp: 1807
Ion Ratio Lower Upper
50 100
52 20.7 25.7 38.5#


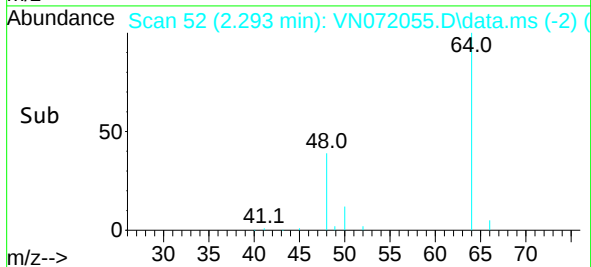

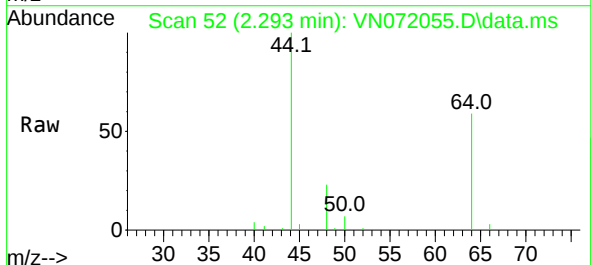


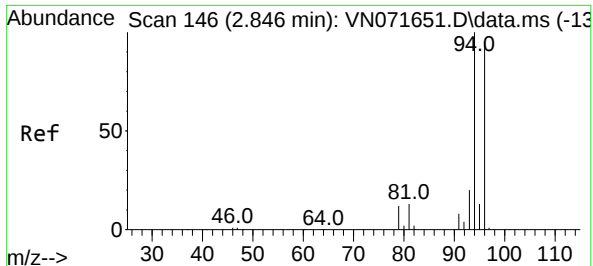

#5
Bromomethane
Concen: 0.238 ug/l
RT: 2.816 min Scan# 146
Delta R.T. -0.030 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7-GR


Tgt Ion: 94 Resp: 961
Ion Ratio Lower Upper
94 100
96 55.3 76.0 114.0#

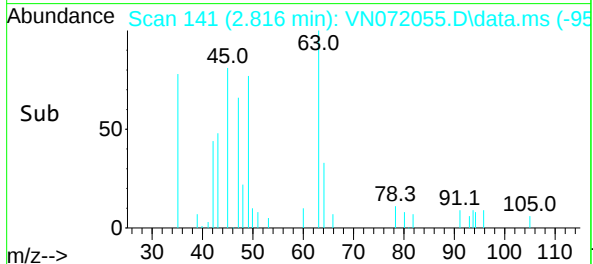

#11
Tert butyl alcohol
Concen: 0.246 ug/l
RT: 5.363 min Scan# 574
Delta R.T. 0.006 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26

Tgt Ion: 59 Resp: 256
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

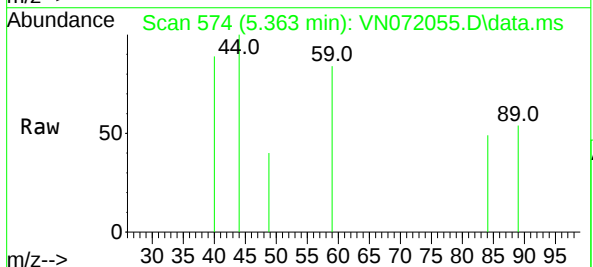



#13

Acrolein

Concen: 0.934 ug/l

RT: 4.034 min Scan# 34

Delta R.T. -0.006 min

Lab File: VN072055.D

Acq: 19 Apr 2022 17:26

Instrument :

MSVOA_N

ClientSampleId :





WC-15-1-7-GR

Tgt Ion: 56 Resp: 1185

Ion Ratio Lower Upper

56 100

55 47.9 54.8 82.2#

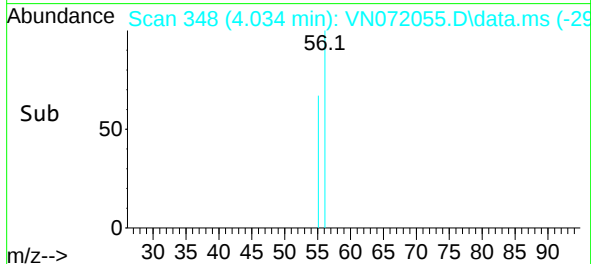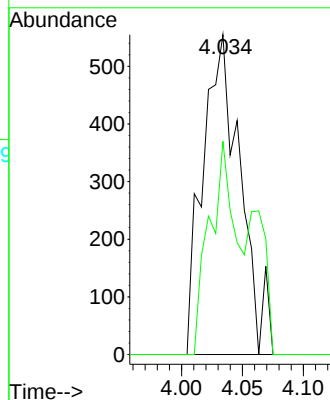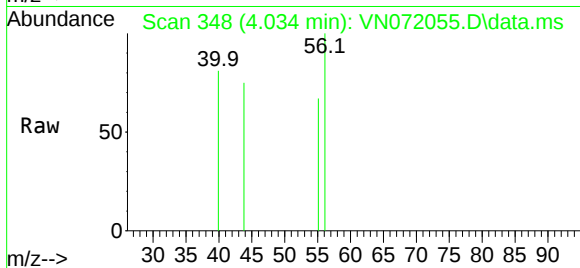

#14

Allyl chloride

Concen: 1.457 ug/l

RT: 5.081 min Scan# 526

Delta R.T. 0.241 min

Lab File: VN072055.D

Acq: 19 Apr 2022 17:26




Tgt Ion: 41 Resp: 10958


Ion Ratio Lower Upper

41 100

39 0.0 53.2 79.8#

76 0.0 29.9 44.9#


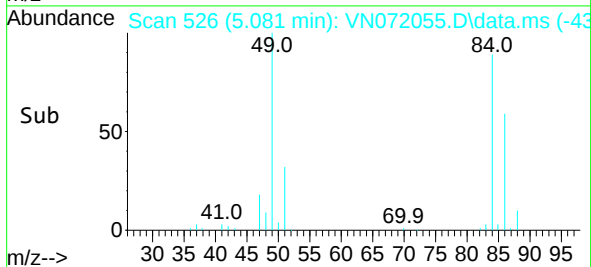
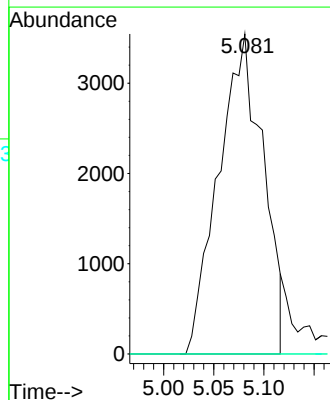
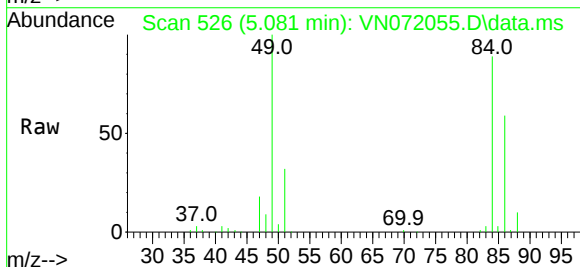




#16
Acetone
Concen: 23.285 ug/l
RT: 4.293 min Scan# 392
Delta R.T. 0.018 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7-GR


Tgt Ion: 43 Resp: 63787
Ion Ratio Lower Upper
43 100
58 32.0 26.0 39.0

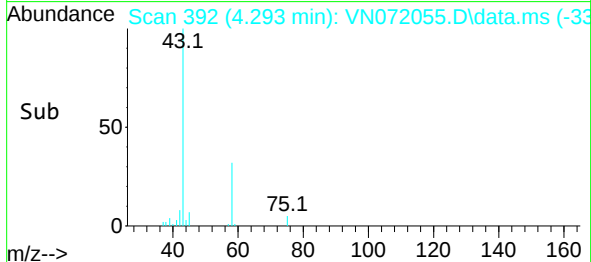

#17
Carbon Disulfide
Concen: 0.656 ug/l
RT: 4.499 min Scan# 427
Delta R.T. -0.035 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26

Tgt Ion: 76 Resp: 6980
Ion Ratio Lower Upper
76 100
78 7.0 7.2 10.8#


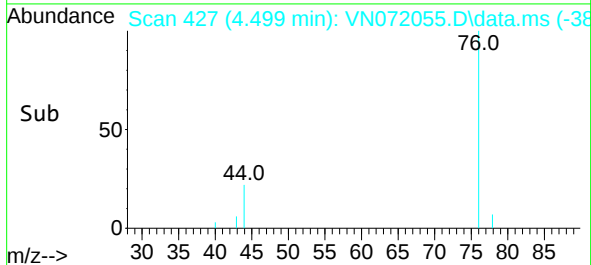

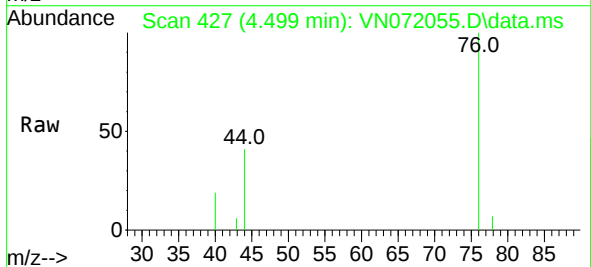




#18
Methyl Acetate
Concen: 2.719 ug/l
RT: 4.857 min Scan# 488
Delta R.T. 0.011 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7-GR


Tgt Ion: 43 Resp: 28154
Ion Ratio Lower Upper
43 100
74 25.7 21.6 32.4

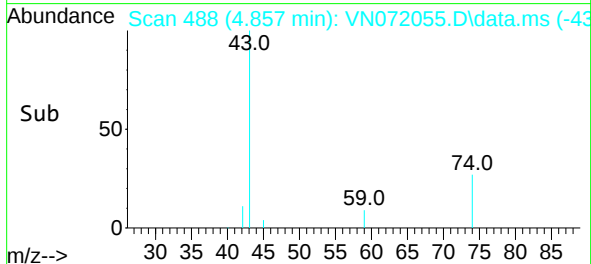

#20
Methylene Chloride
Concen: 58.354 ug/l
RT: 5.075 min Scan# 525
Delta R.T. -0.018 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26

Tgt Ion: 84 Resp: 336937
Ion Ratio Lower Upper
84 100
49 105.7 88.3 132.5
51 33.7 28.2 42.2
86 64.8 50.6 76.0


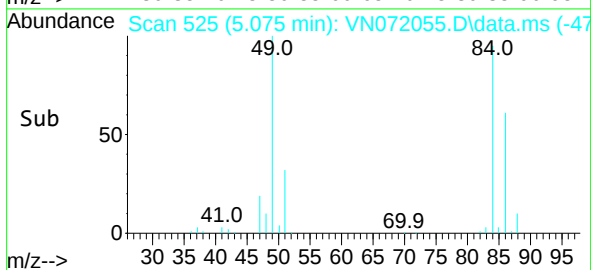

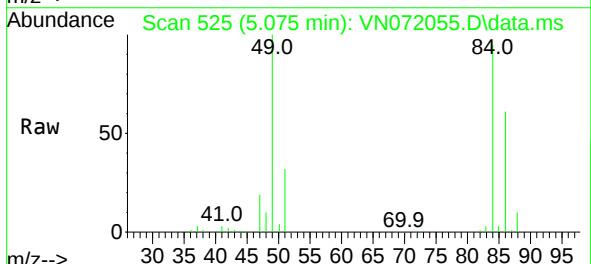




#25
2-Butanone
Concen: 5.125 ug/l
RT: 7.340 min Scan# 910
Delta R.T. 0.012 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7-GR


Tgt Ion: 43 Resp: 20240
Ion Ratio Lower Upper
43 100
72 26.3 23.7 35.5

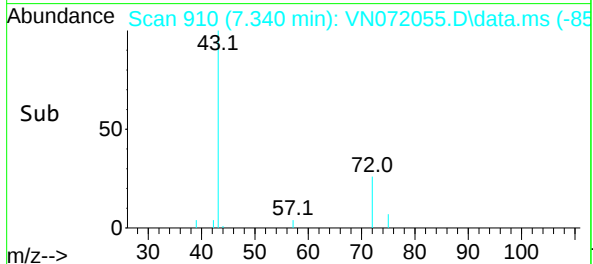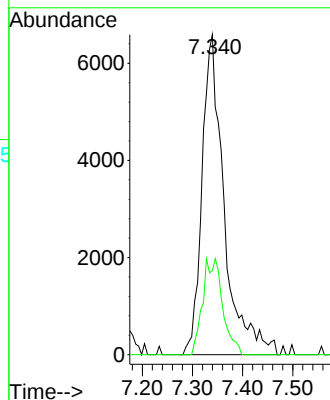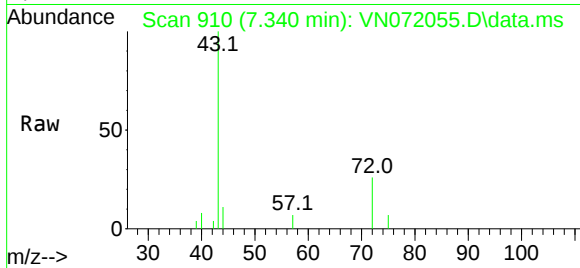

#29
Tetrahydrofuran
Concen: 0.267 ug/l
RT: 7.704 min Scan# 972
Delta R.T. 0.029 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26

Tgt Ion: 42 Resp: 682
Ion Ratio Lower Upper
42 100
72 24.3 39.7 59.5#
71 8.8 36.6 55.0#


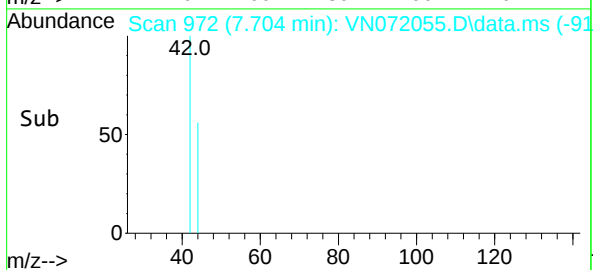
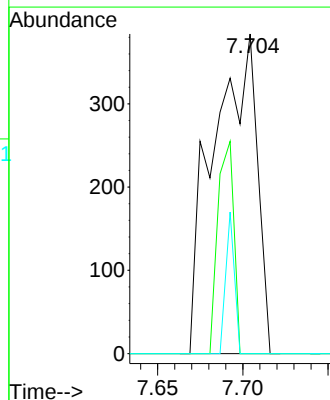
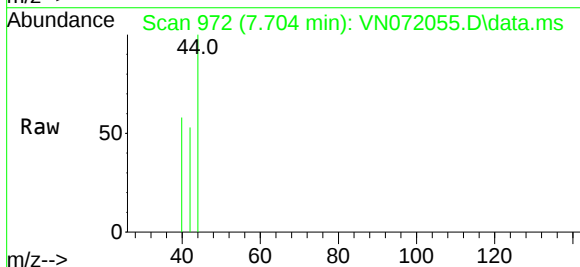




#31
Cyclohexane
Concen: 1.092 ug/l
RT: 8.069 min Scan# 1034
Delta R.T. -0.023 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7-GR


Tgt Ion: 56 Resp: 9523
Ion Ratio Lower Upper
56 100
69 160.9 27.8 41.8#
84 141.4 76.9 115.3#

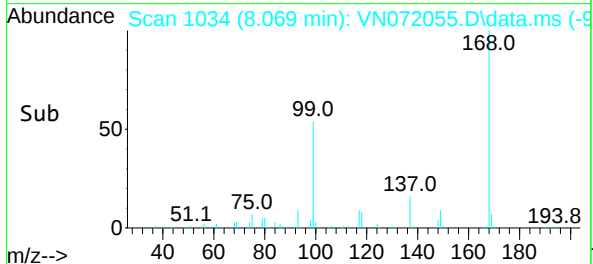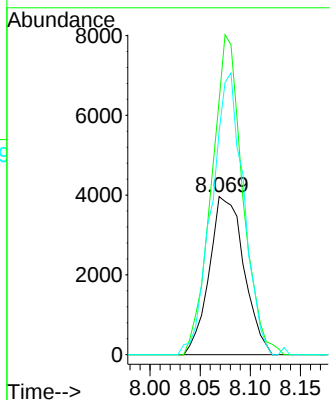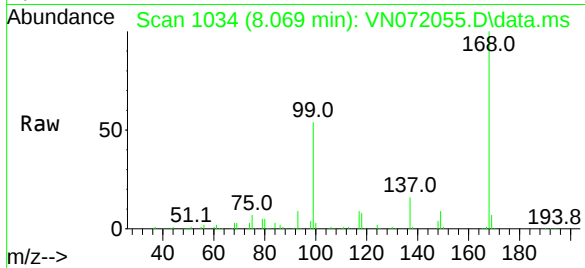

#33
1,2-Dichloroethane-d4
Concen: 46.285 ug/l
RT: 8.428 min Scan# 1095
Delta R.T. -0.006 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26

Tgt Ion: 65 Resp: 296692
Ion Ratio Lower Upper
65 100
67 54.4 0.0 104.8

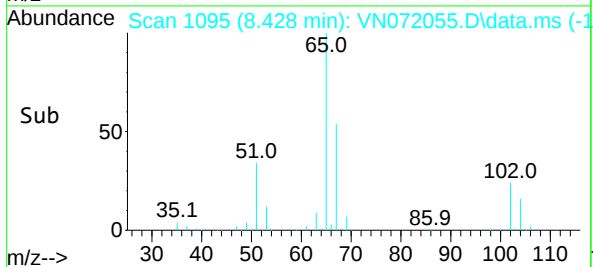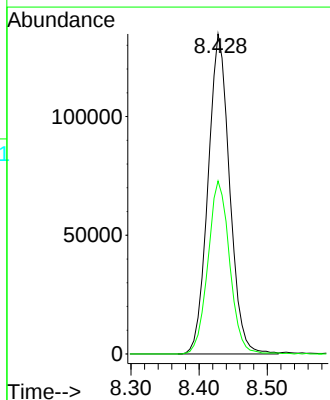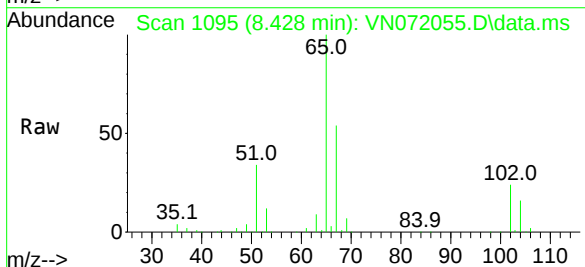

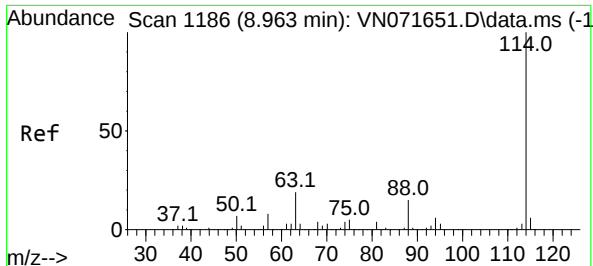

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. -0.000 min

Lab File: VN072055.D

Acq: 19 Apr 2022 17:26

Instrument :

MSVOA_N

ClientSampleId :

WC-15-1-7-GR





Tgt Ion:114 Resp: 949700

Ion Ratio Lower Upper

114 100

63 19.3 0.0 40.0

88 15.4 0.0 32.6

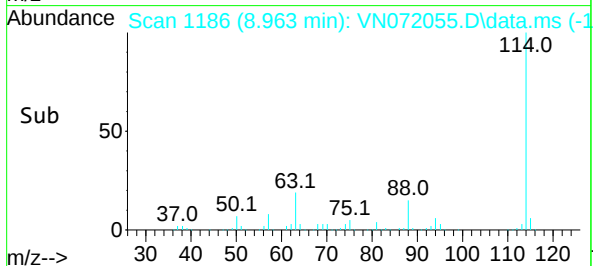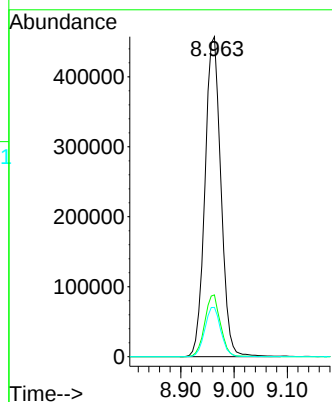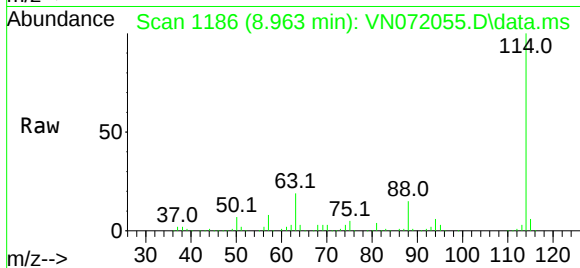

#35

Dibromofluoromethane

Concen: 46.263 ug/l

RT: 8.016 min Scan# 1025

Delta R.T. -0.000 min

Lab File: VN072055.D

Acq: 19 Apr 2022 17:26




Tgt Ion:113 Resp: 258536


Ion Ratio Lower Upper

113 100

111 102.4 81.4 122.0

192 22.3 17.0 25.6


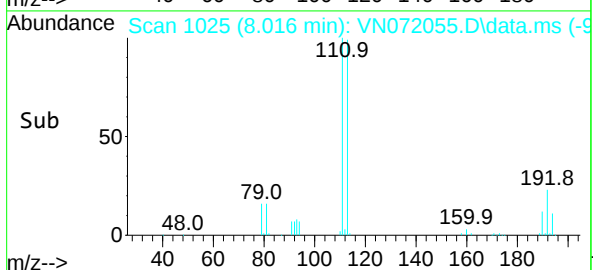

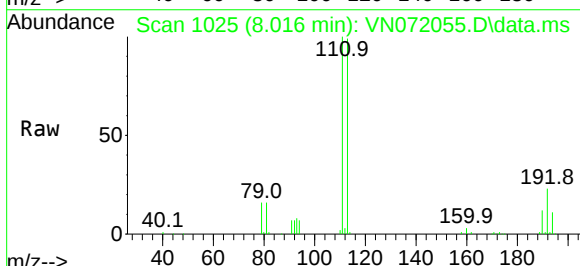




#36
1,1-Dichloropropene
Concen: 4.785 ug/l
RT: 8.075 min Scan# 1059
Delta R.T. -0.141 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7-GR


Tgt Ion: 75 Resp: 37342
Ion Ratio Lower Upper
75 100
110 8.0 18.3 54.8#
77 0.0 25.1 37.7#

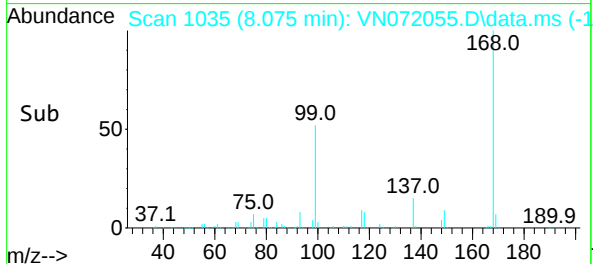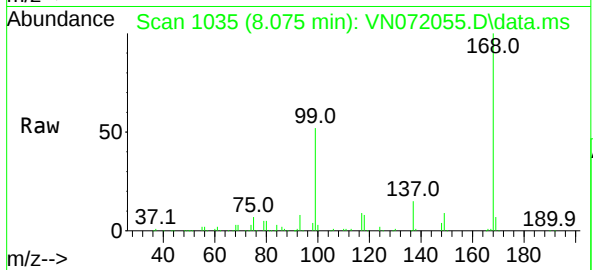

#37
Ethyl Acetate
Concen: 2.370 ug/l
RT: 7.340 min Scan# 910
Delta R.T. -0.064 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26

Tgt Ion: 43 Resp: 20240
Ion Ratio Lower Upper
43 100
61 0.0 11.8 17.6#
70 0.0 9.3 13.9#


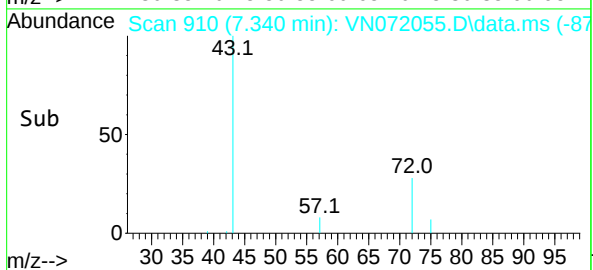

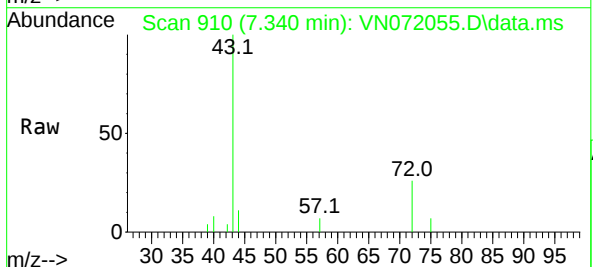


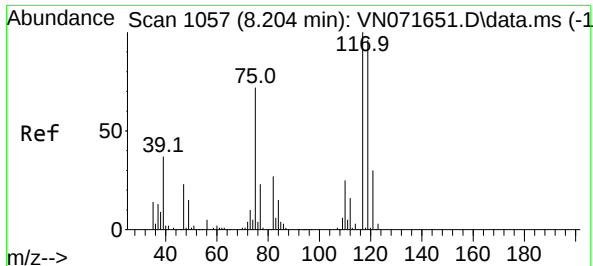

#38
Carbon Tetrachloride
Concen: 6.540 ug/l
RT: 8.075 min Scan# 1107
Delta R.T. -0.129 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7-GR


Tgt Ion:117 Resp: 50019
Ion Ratio Lower Upper
117 100
119 5.7 75.8 113.8#
121 0.0 24.6 37.0#

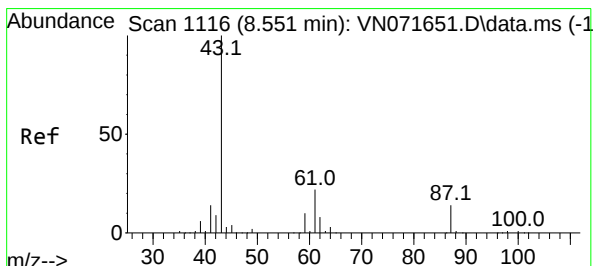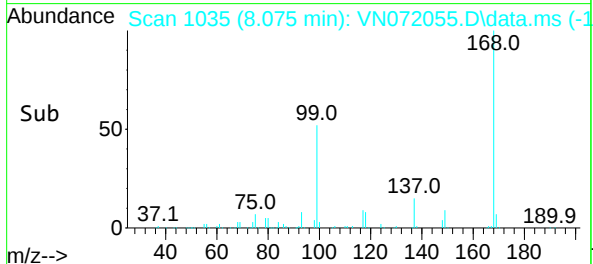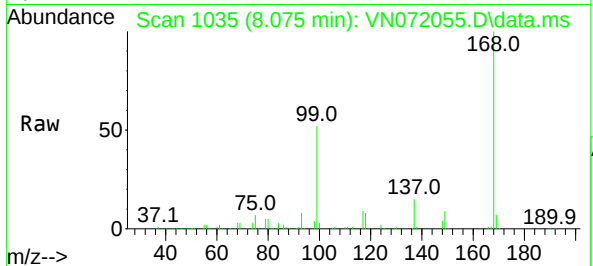

#43
Isopropyl Acetate
Concen: 7.490 ug/l
RT: 8.557 min Scan# 1117
Delta R.T. 0.006 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26

Tgt Ion: 43 Resp: 106412
Ion Ratio Lower Upper
43 100
61 11.7 21.9 32.9#
87 7.3 12.0 18.0#

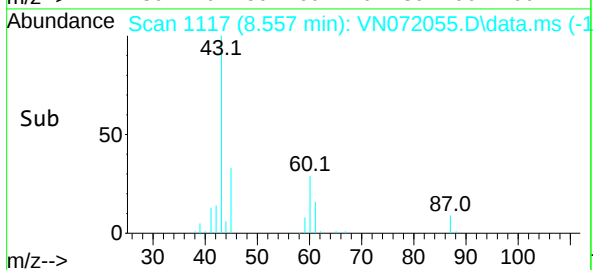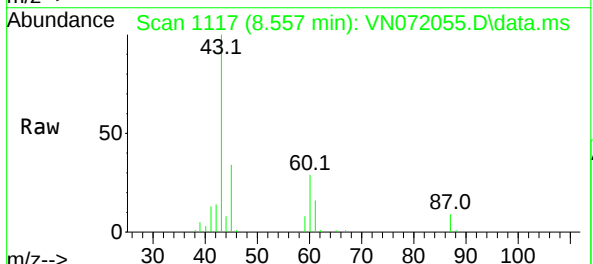

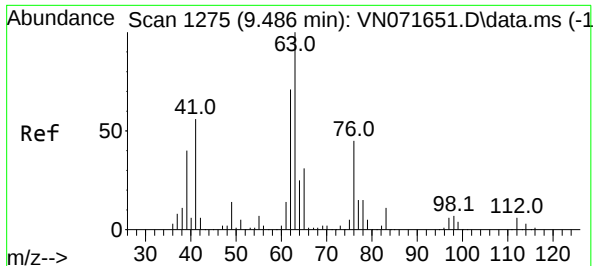

#45

1,2-Dichloropropane

Concen: 0.644 ug/l

RT: 9.616 min Scan# 1297

Delta R.T. 0.130 min

Lab File: VN072055.D

Acq: 19 Apr 2022 17:26

Instrument :

MSVOA_N

ClientSampleId :





WC-15-1-7-GR

Tgt Ion: 63 Resp: 3965

Ion Ratio Lower Upper

63 100

65 0.0 24.9 37.3#

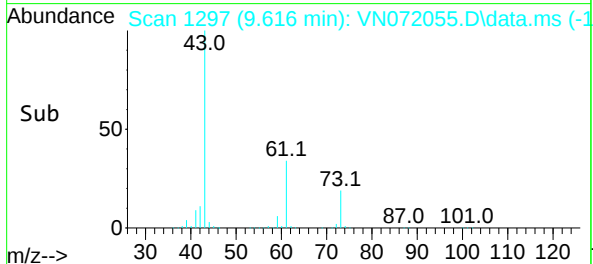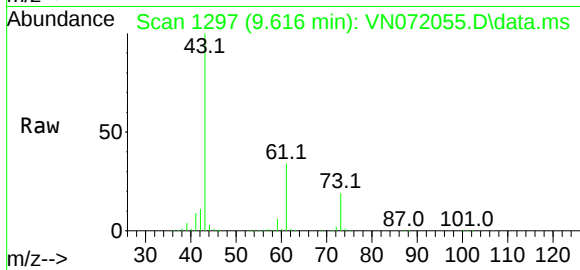

#48

Methyl methacrylate

Concen: 2.559 ug/l

RT: 9.545 min Scan# 1285

Delta R.T. -0.006 min

Lab File: VN072055.D

Acq: 19 Apr 2022 17:26




Tgt Ion: 41 Resp: 15084


Ion Ratio Lower Upper

41 100

69 0.0 74.7 112.1#

39 0.0 45.6 68.4#

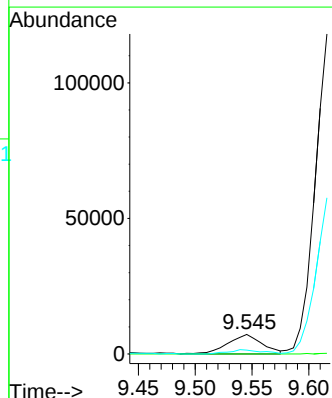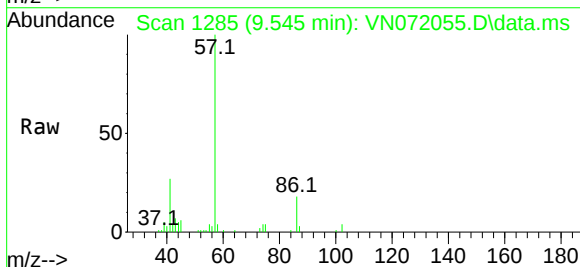

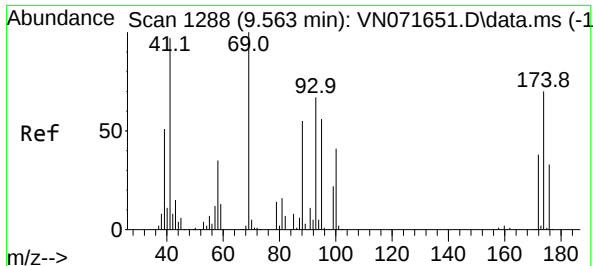

#49

1,4-Dioxane

Concen: Below Cal

RT: 9.616 min Scan# 1

Delta R.T. 0.053 min

Lab File: VN072055.D

Acq: 19 Apr 2022 17:26

Instrument :

MSVOA_N

ClientSampleId :

WC-15-1-7-GR





Tgt Ion: 88 Resp: 344

Ion Ratio Lower Upper

88 100

43 748360.2 20.2 30.4#

58 3523.3 54.2 81.4#

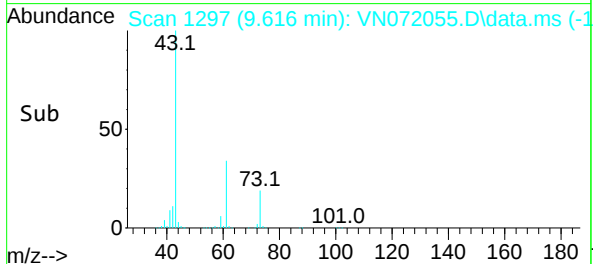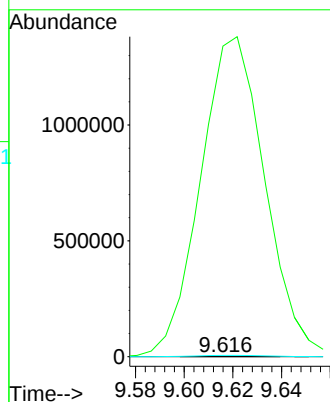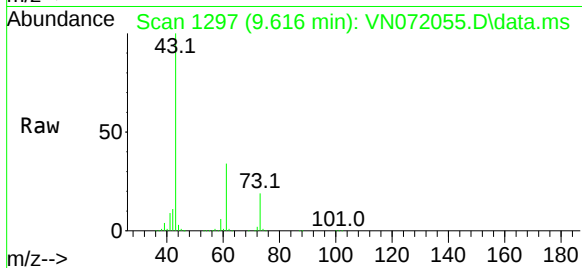

#50

Toluene-d8

Concen: 56.021 ug/l

RT: 10.433 min Scan# 1436

Delta R.T. -0.006 min

Lab File: VN072055.D




Acq: 19 Apr 2022 17:26


Tgt Ion: 98 Resp: 1280693

Ion Ratio Lower Upper

98 100

100 64.8 52.6 78.8

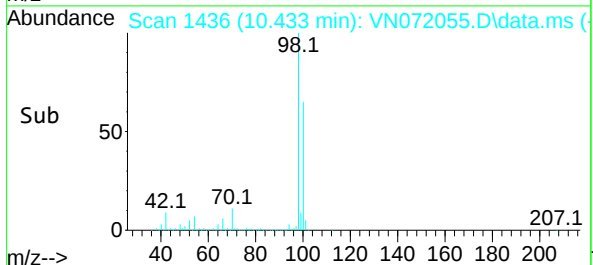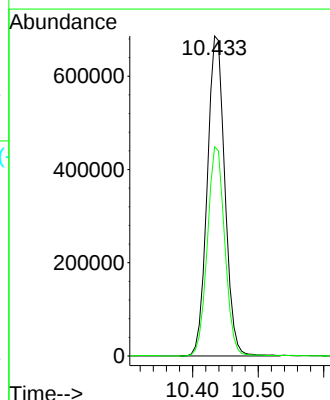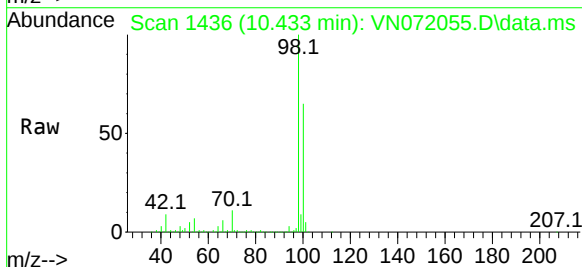



#51

4-Methyl-2-Pentanone

Concen: 1.127 ug/l

RT: 10.333 min Scan# 1419

Delta R.T. 0.011 min

Lab File: VN072055.D

Acq: 19 Apr 2022 17:26

Instrument :

MSVOA_N

ClientSampleId :





WC-15-1-7-GR

Tgt Ion: 43 Resp: 9209

Ion Ratio Lower Upper

43 100

58 57.3 34.1 51.1#

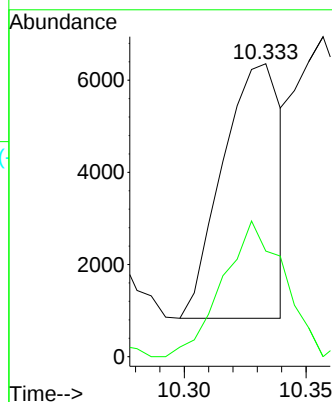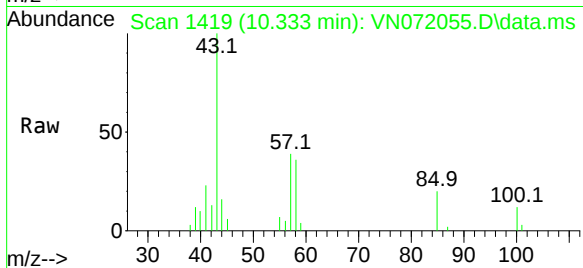

#52

Toluene

Concen: 1.215 ug/l

RT: 10.498 min Scan# 1447

Delta R.T. 0.000 min

Lab File: VN072055.D




Acq: 19 Apr 2022 17:26


Tgt Ion: 92 Resp: 18927

Ion Ratio Lower Upper

92 100

91 181.0 138.6 207.8


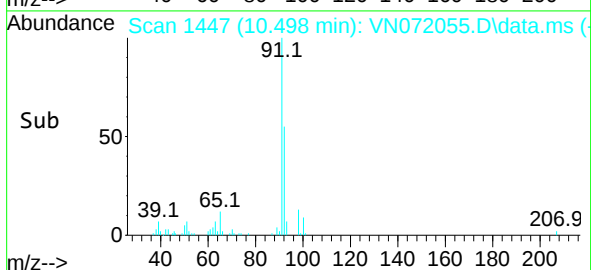

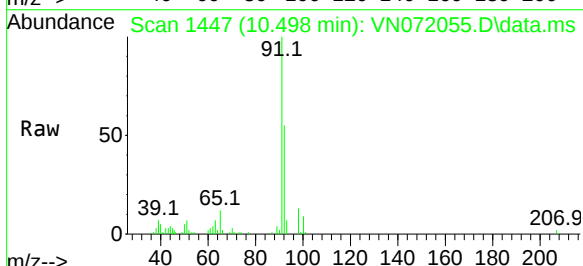




#54
 cis-1,3-Dichloropropene
 Concen: 10.353 ug/l
 RT: 10.239 min Scan# 14
 Delta R.T. 0.053 min
 Lab File: VN072055.D
 Acq: 19 Apr 2022 17:26




Instrument :
 MSVOA_N
 ClientSampleId :
 WC-15-1-7-GR


Tgt Ion: 75 Resp: 98681
 Ion Ratio Lower Upper
 75 100
 77 0.6 25.2 37.8#
 39 23.1 35.7 53.5#

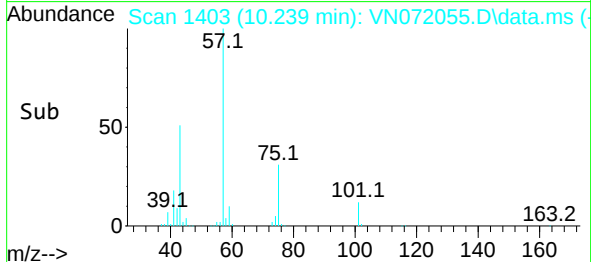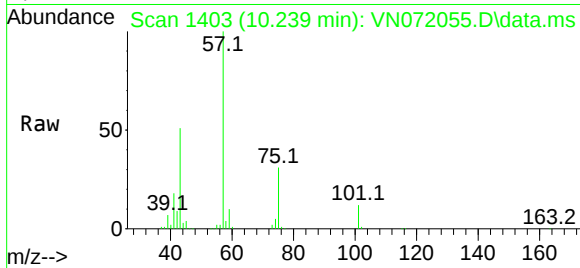

#57
 1,3-Dichloropropane
 Concen: 5.130 ug/l
 RT: 11.086 min Scan# 1547
 Delta R.T. 0.047 min
 Lab File: VN072055.D
 Acq: 19 Apr 2022 17:26

Tgt Ion: 76 Resp: 55006
 Ion Ratio Lower Upper
 76 100
 78 0.3 26.2 39.2#


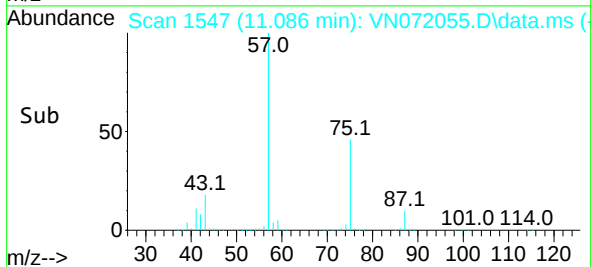

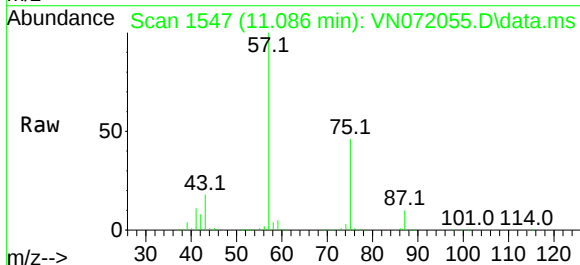




#59
2-Hexanone
Concen: 117.395 ug/l
RT: 11.086 min Scan# 11
Delta R.T. 0.005 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7-GR


Tgt Ion: 43 Resp: 675150
Ion Ratio Lower Upper
43 100
58 20.3 29.7 89.1#

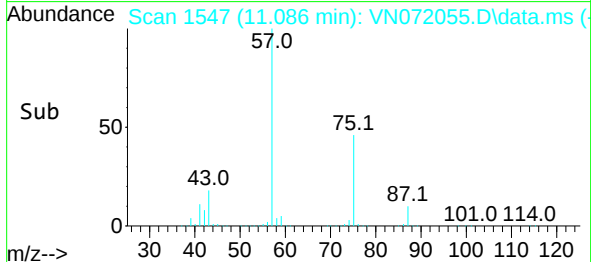

#62
4-Bromofluorobenzene
Concen: 62.876 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26

Tgt Ion: 95 Resp: 464878
Ion Ratio Lower Upper
95 100
174 86.3 0.0 167.6
176 83.4 0.0 163.4


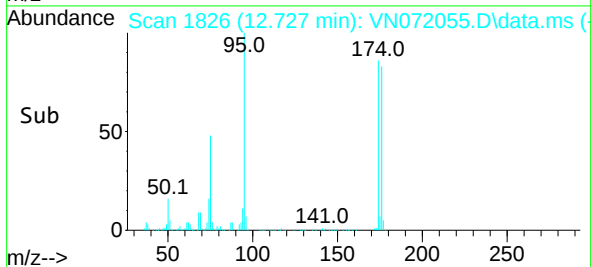

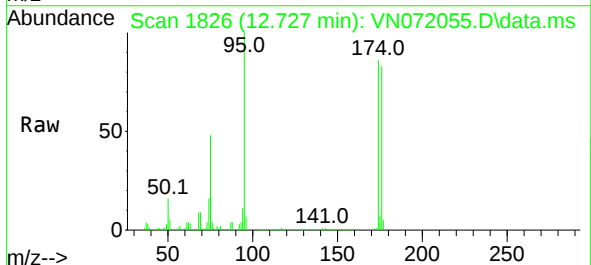




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7-GR


Tgt Ion:117 Resp: 1138687
Ion Ratio Lower Upper
117 100
82 54.4 44.2 66.2
119 31.9 25.4 38.0

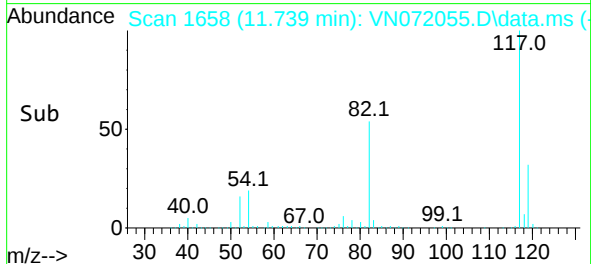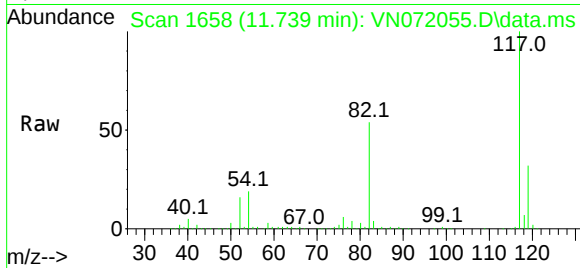

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.669 min Scan# 1986
Delta R.T. -0.000 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26

Tgt Ion:152 Resp: 432374
Ion Ratio Lower Upper
152 100
115 55.8 28.9 86.7
150 156.3 0.0 356.2


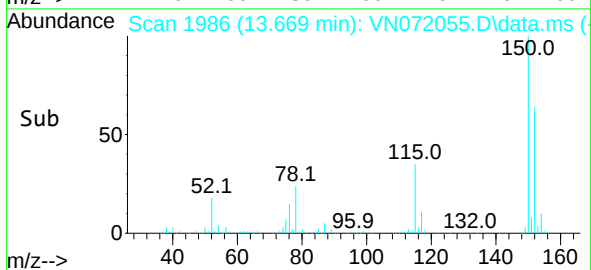

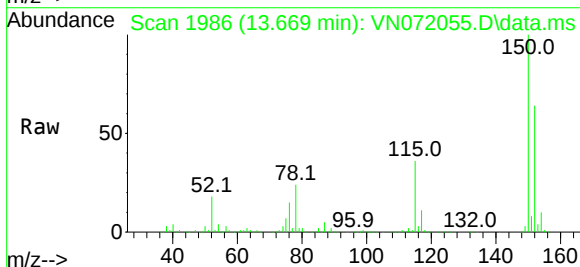




#74
N-amy1 acetate
Concen: 0.305 ug/l
RT: 12.357 min Scan# 1
Delta R.T. -0.023 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7-GR


Tgt Ion: 43	Resp: 3186
Ion Ratio	Lower Upper
43	100
70	0.0 39.0 58.4#
55	5.6 21.1 31.7#
61	0.0 21.1 31.7#

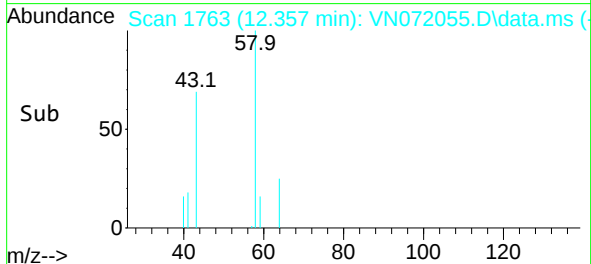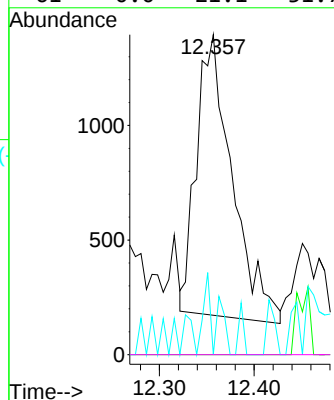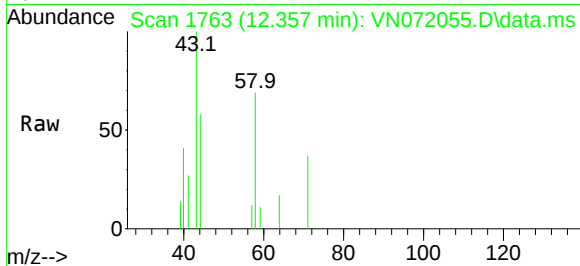

#76
1,2,3-Trichloropropane
Concen: 22.468 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26

Tgt Ion: 75	Resp: 225047
Ion Ratio	Lower Upper
75	100
77	1.5 98.5 295.5#


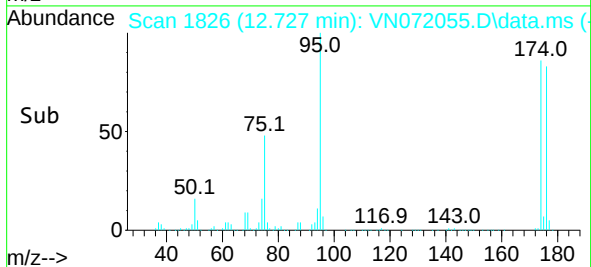
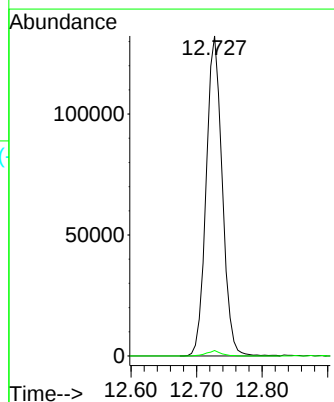
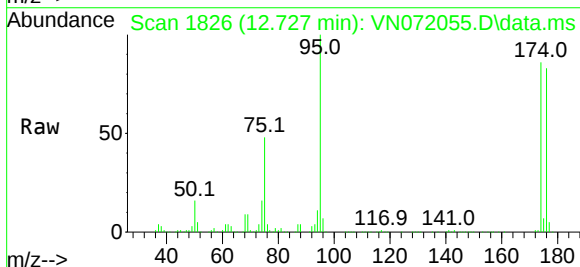




#81
trans-1,4-Dichloro-2-butene
Concen: 69.628 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.105 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7-GR


Tgt Ion: 75 Resp: 225047
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.0 37.2 55.8#

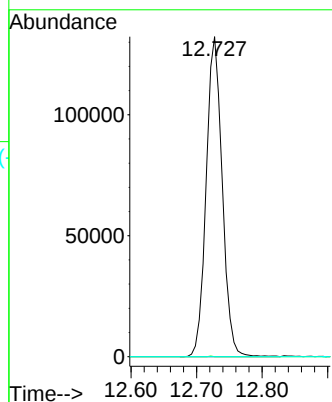

#84
1,2,4-Trimethylbenzene
Concen: 0.285 ug/l
RT: 13.363 min Scan# 1934
Delta R.T. -0.000 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26

Tgt Ion: 105 Resp: 8035
Ion Ratio Lower Upper
105 100
120 39.2 23.3 69.8


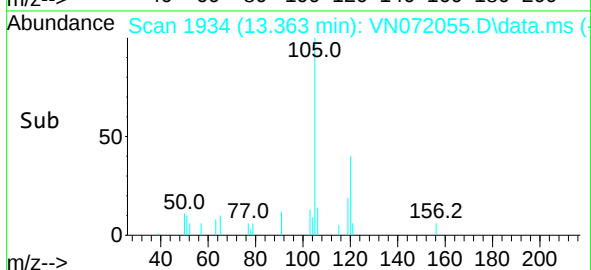




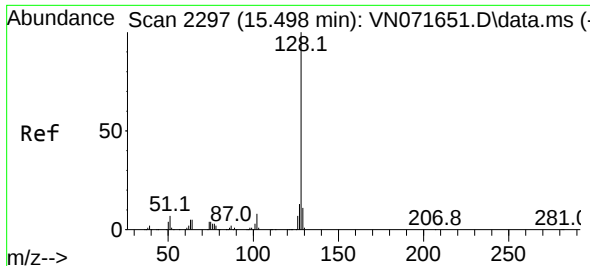

#95
Naphthalene
Concen: 3.904 ug/l
RT: 15.504 min Scan# 2164
Delta R.T. 0.006 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26

Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7-GR

Tgt Ion:128 Resp: 2164
Ion Ratio Lower Upper
128 100
127 6.6 10.3 15.5#
129 3.2 8.6 13.0#

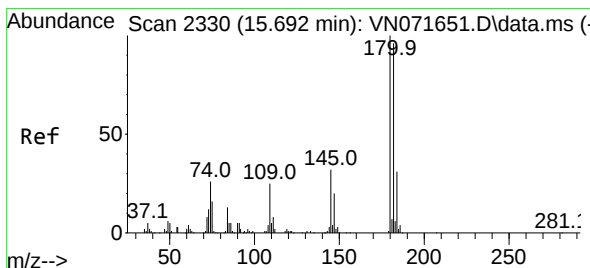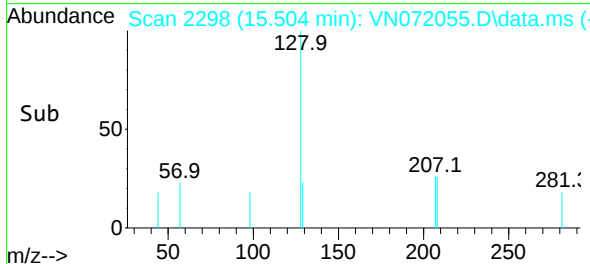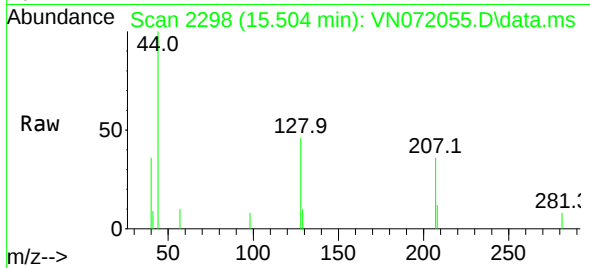

#96
1,2,3-Trichlorobenzene
Concen: 2.430 ug/l
RT: 15.704 min Scan# 2332
Delta R.T. 0.012 min
Lab File: VN072055.D
Acq: 19 Apr 2022 17:26

Tgt Ion:180 Resp: 108
Ion Ratio Lower Upper
180 100
182 0.0 47.8 143.3#
145 0.0 15.5 46.5#

