

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041922\
 Data File : VN072056.D
 Acq On : 19 Apr 2022 17:50
 Operator : JC\MD
 Sample : N2468-08
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 WC-15-1-7

Quant Time: Apr 20 01:27:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 31 01:57:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.081	168	652511	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1117550	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1279478	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.669	152	471373	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.428	65	343848	46.159	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	92.320%
35) Dibromofluoromethane	8.016	113	301787	45.891	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	91.780%
50) Toluene-d8	10.433	98	1479443	54.995	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	109.980%
62) 4-Bromofluorobenzene	12.727	95	522919	60.103	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	120.200%
Target Compounds						
					Qvalue	
3) Chloromethane	2.293	50	1655	0.252	ug/l #	68
11) Tert butyl alcohol	5.369	59	847	0.701	ug/l #	72
13) Acrolein	4.022	56	431	0.292	ug/l #	1
14) Allyl chloride	5.087	41	11983	1.371	ug/l #	25
16) Acetone	4.287	43	86153	27.062	ug/l	99
18) Methyl Acetate	4.857	43	20144	1.074	ug/l	99
20) Methylene Chloride	5.087	84	400027	59.616	ug/l	98
25) 2-Butanone	7.334	43	19422	4.232	ug/l #	88
31) Cyclohexane	8.087	56	18781	1.854	ug/l #	33
36) 1,1-Dichloropropene	8.081	75	43873	4.777	ug/l #	47
37) Ethyl Acetate	7.334	43	19422	1.932	ug/l #	67
38) Carbon Tetrachloride	8.081	117	57224	6.358	ug/l #	16
39) Methylcyclohexane	9.451	83	10803	0.988	ug/l	91
43) Isopropyl Acetate	8.551	43	102078	6.106	ug/l #	76
45) 1,2-Dichloropropane	9.616	63	4570	0.631	ug/l #	44
48) Methyl methacrylate	9.539	41	17115	2.467	ug/l #	23
49) 1,4-Dioxane	9.622	88	541	Below Cal	#	1
51) 4-Methyl-2-Pentanone	10.328	43	12117	1.261	ug/l	91
54) cis-1,3-Dichloropropene	10.239	75	102542	9.142	ug/l #	56
57) 1,3-Dichloropropane	11.086	76	64119	5.081	ug/l #	42
59) 2-Hexanone	11.086	43	754605	111.503	ug/l #	49
68) m/p-Xylenes	11.951	106	6890	0.413	ug/l	96
69) o-Xylene	12.275	106	13704	0.829	ug/l	98
73) Isopropylbenzene	12.575	105	22882	0.576	ug/l	99
74) N-amyl acetate	12.351	43	3409	0.300	ug/l #	41
76) 1,2,3-Trichloropropane	12.727	75	250530	22.943	ug/l #	1
78) n-propylbenzene	12.916	91	10429	0.250	ug/l	92
80) 1,3,5-Trimethylbenzene	13.057	105	92413	2.936	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.727	75	250530	71.099	ug/l #	10
82) 4-Chlorotoluene	13.057	91	9854	0.397	ug/l #	40
84) 1,2,4-Trimethylbenzene	13.363	105	138408	4.507	ug/l	98
85) sec-Butylbenzene	13.492	105	12709	0.341	ug/l	87
86) p-Isopropyltoluene	13.557	119	6868	0.231	ug/l	93
90) Hexachloroethane	14.216	117	3803	0.699	ug/l #	9
95) Naphthalene	15.504	128	5147	4.024	ug/l	96

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041922\
Data File : VN072056.D
Acq On : 19 Apr 2022 17:50
Operator : JC\MD
Sample : N2468-08
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7

Quant Time: Apr 20 01:27:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 31 01:57:54 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041922\
Data File : VN072056.D
Acq On : 19 Apr 2022 17:50
Operator : JC\MD
Sample : N2468-08
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7

Quant Time: Apr 20 01:27:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 31 01:57:54 2022
Response via : Initial Calibration




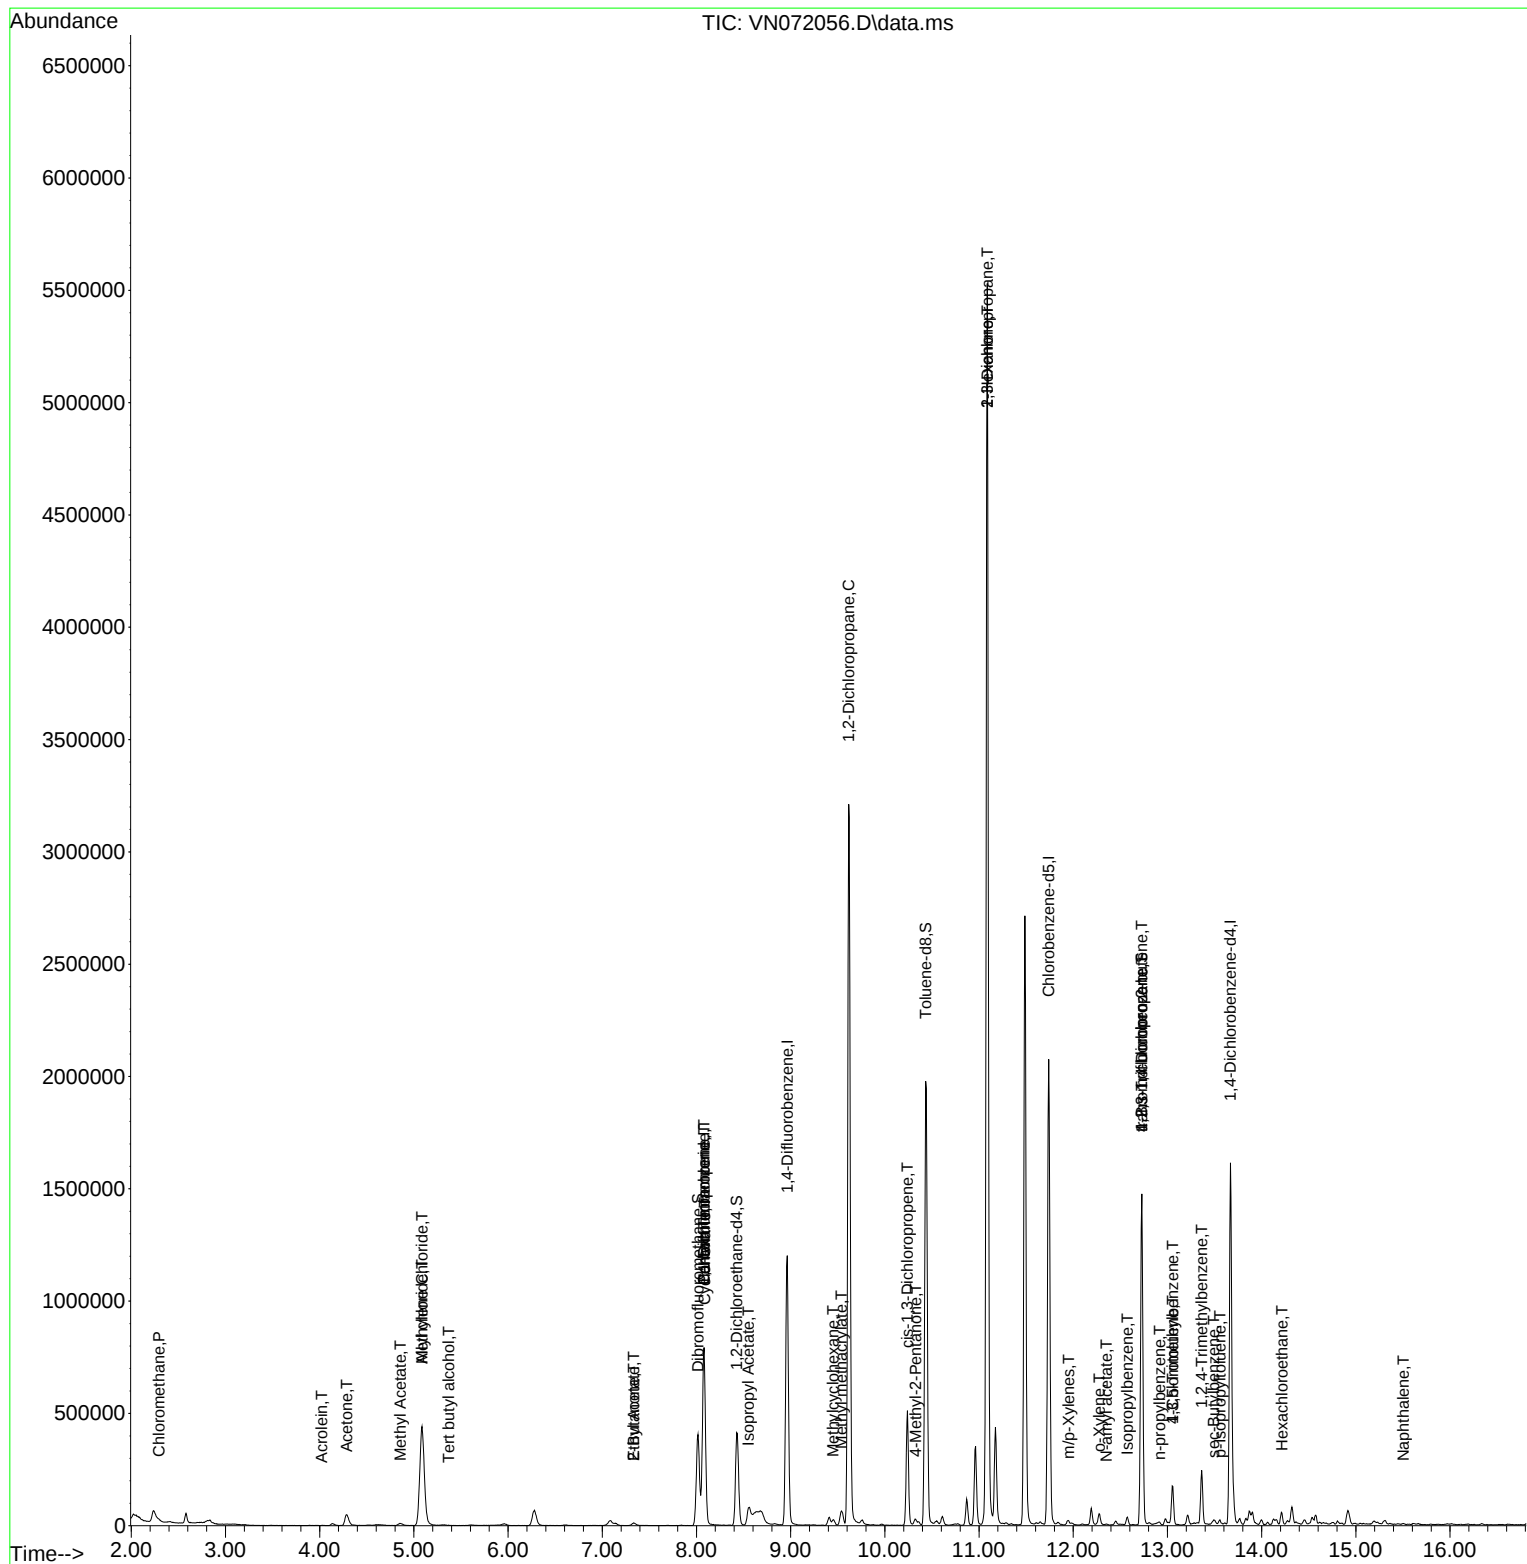




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 1
Delta R.T. -0.000 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7


Tgt Ion:168 Resp: 652511
Ion Ratio Lower Upper
168 100
99 51.8 42.3 63.5

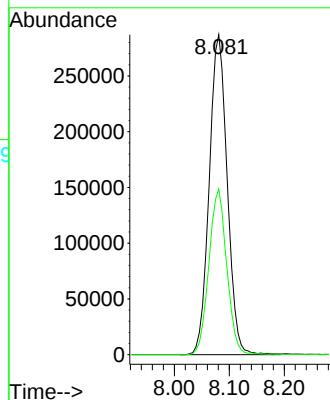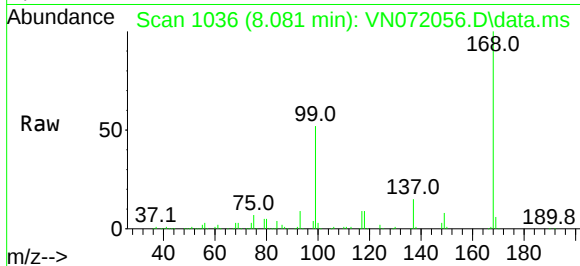

#3
Chloromethane
Concen: 0.252 ug/l
RT: 2.293 min Scan# 52
Delta R.T. -0.006 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50

Tgt Ion: 50 Resp: 1655
Ion Ratio Lower Upper
50 100
52 50.2 25.7 38.5#

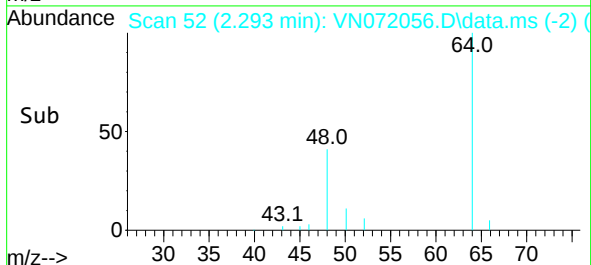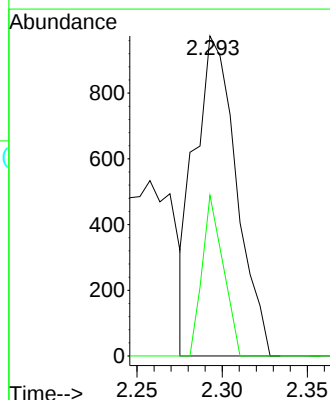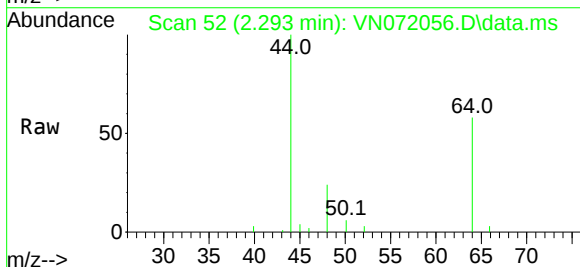



#11

Tert butyl alcohol

Concen: 0.701 ug/l

RT: 5.369 min Scan# 51

Delta R.T. 0.012 min

Lab File: VN072056.D

Acq: 19 Apr 2022 17:50

Instrument :

MSVOA_N

ClientSampleId :





WC-15-1-7

Tgt Ion: 59 Resp: 847

Ion Ratio Lower Upper

59 100

57 0.0 8.3 12.5#

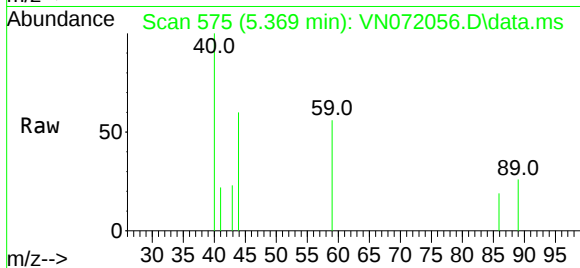

#13

Acrolein

Concen: 0.292 ug/l

RT: 4.022 min Scan# 346

Delta R.T. -0.018 min

Lab File: VN072056.D




Acq: 19 Apr 2022 17:50


Tgt Ion: 56 Resp: 431

Ion Ratio Lower Upper

56 100

55 215.3 54.8 82.2#


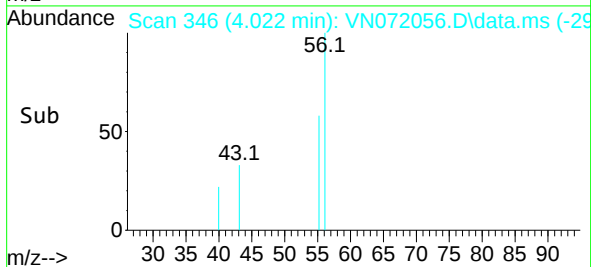

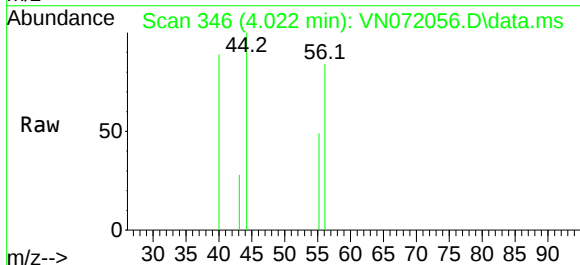




#14
 Allyl chloride
 Concen: 1.371 ug/l
 RT: 5.087 min Scan# 51
 Delta R.T. 0.247 min
 Lab File: VN072056.D
 Acq: 19 Apr 2022 17:50




Instrument :
 MSVOA_N
 ClientSampleId :
 WC-15-1-7


Tgt Ion: 41 Resp: 11983
 Ion Ratio Lower Upper
 41 100
 39 0.9 53.2 79.8#
 76 0.0 29.9 44.9#

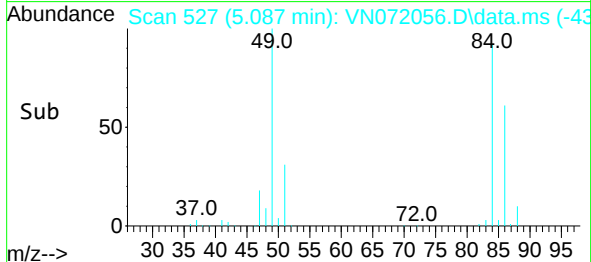

#16
 Acetone
 Concen: 27.062 ug/l
 RT: 4.287 min Scan# 391
 Delta R.T. 0.012 min
 Lab File: VN072056.D
 Acq: 19 Apr 2022 17:50

Tgt Ion: 43 Resp: 86153
 Ion Ratio Lower Upper
 43 100
 58 32.1 26.0 39.0


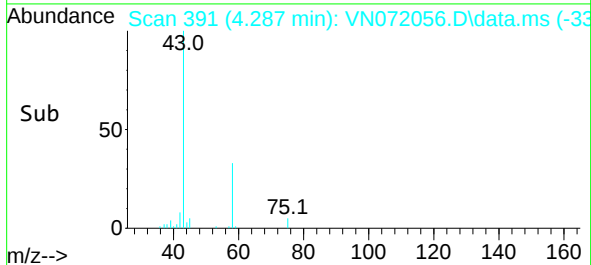

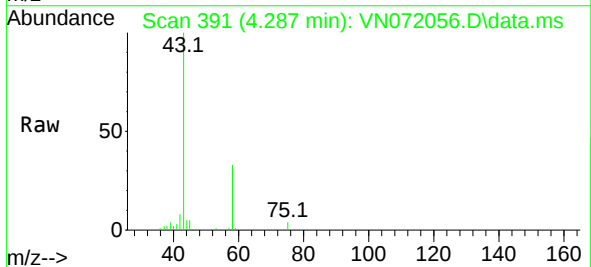




#18
Methyl Acetate
Concen: 1.074 ug/l
RT: 4.857 min Scan# 488
Delta R.T. 0.011 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7


Tgt Ion: 43 Resp: 20144
Ion Ratio Lower Upper
43 100
74 27.5 21.6 32.4



#20
Methylene Chloride
Concen: 59.616 ug/l
RT: 5.087 min Scan# 527
Delta R.T. -0.006 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50

Tgt Ion: 84 Resp: 400027
Ion Ratio Lower Upper
84 100
49 108.3 88.3 132.5
51 33.8 28.2 42.2
86 65.9 50.6 76.0


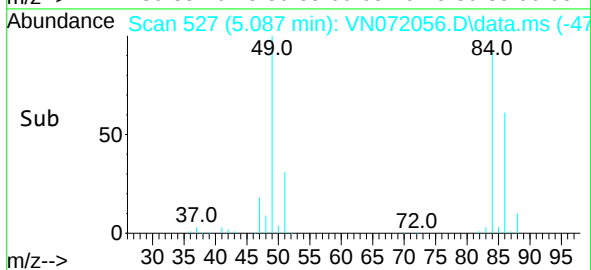






#25
2-Butanone
Concen: 4.232 ug/l
RT: 7.334 min Scan# 908
Delta R.T. 0.006 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7


Tgt Ion: 43 Resp: 19422
Ion Ratio Lower Upper
43 100
72 36.2 23.7 35.5#

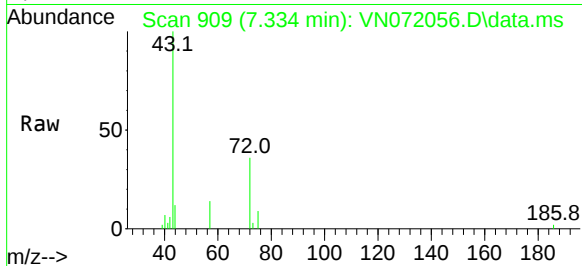

#31
Cyclohexane
Concen: 1.854 ug/l
RT: 8.087 min Scan# 1037
Delta R.T. -0.005 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50

Tgt Ion: 56 Resp: 18781
Ion Ratio Lower Upper
56 100
69 119.8 27.8 41.8#
84 133.9 76.9 115.3#

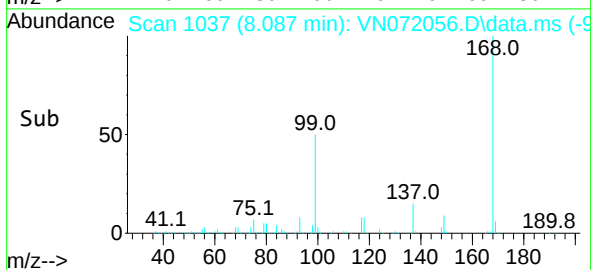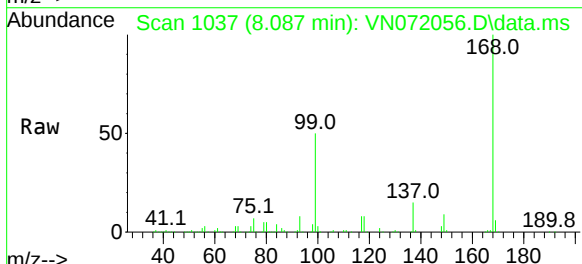

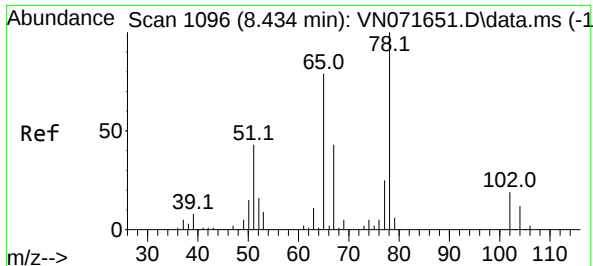

#33

1,2-Dichloroethane-d4

Concen: 46.159 ug/l

RT: 8.428 min Scan# 1095

Delta R.T. -0.006 min

Lab File: VN072056.D

Acq: 19 Apr 2022 17:50

Instrument :

MSVOA_N

ClientSampleId :





WC-15-1-7

Tgt Ion: 65 Resp: 343848

Ion Ratio Lower Upper

65 100

67 53.4 0.0 104.8

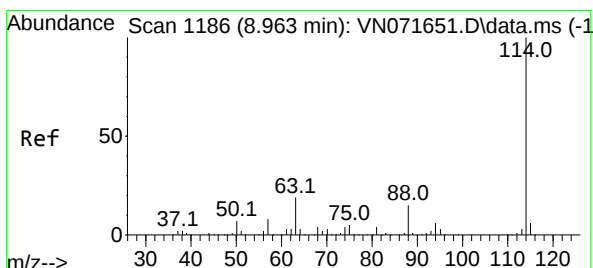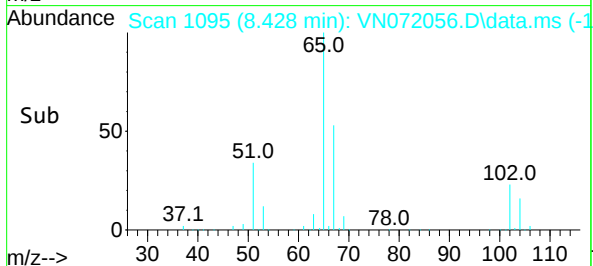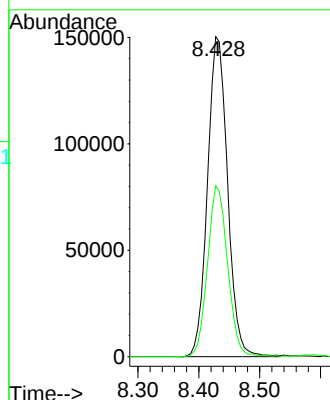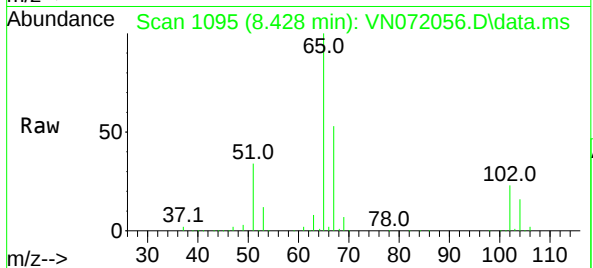

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. -0.000 min

Lab File: VN072056.D

Acq: 19 Apr 2022 17:50




Tgt Ion: 114 Resp: 1117550


Ion Ratio Lower Upper

114 100

63 19.6 0.0 40.0

88 15.5 0.0 32.6

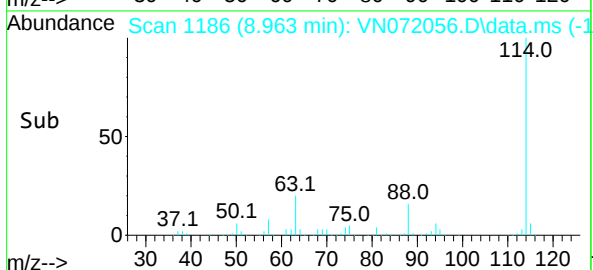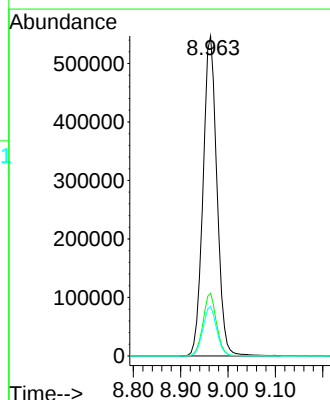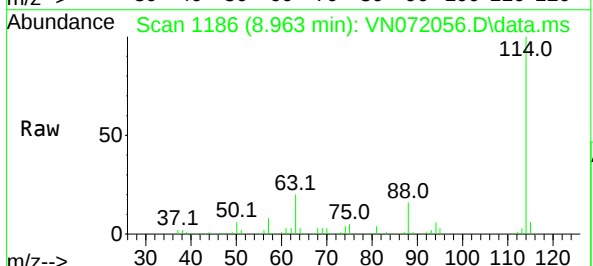

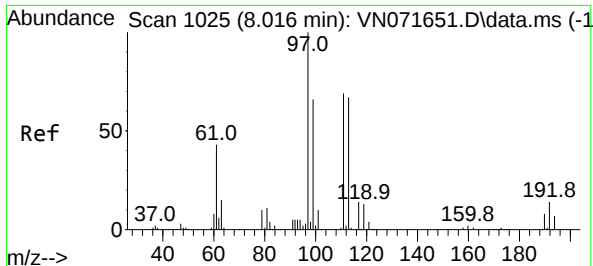

#35

Dibromofluoromethane

Concen: 45.891 ug/l

RT: 8.016 min Scan# 1025

Delta R.T. 0.000 min

Lab File: VN072056.D

Acq: 19 Apr 2022 17:50

Instrument :

MSVOA_N

ClientSampleId :

WC-15-1-7





Tgt Ion:113 Resp: 301787

Ion Ratio Lower Upper

113 100

111 103.6 81.4 122.0

192 22.7 17.0 25.6

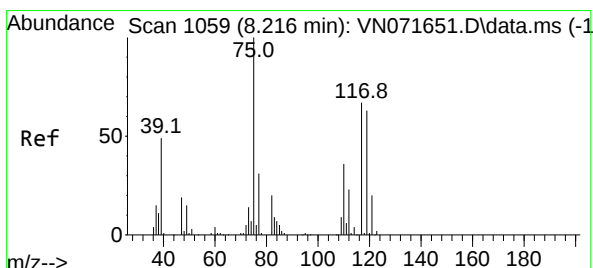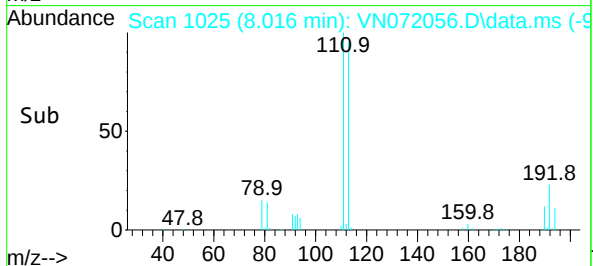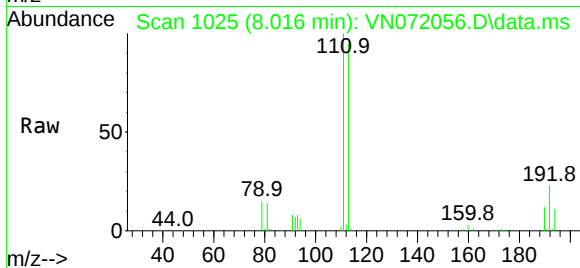

#36

1,1-Dichloropropene

Concen: 4.777 ug/l

RT: 8.081 min Scan# 1036

Delta R.T. -0.135 min

Lab File: VN072056.D

Acq: 19 Apr 2022 17:50




Tgt Ion: 75 Resp: 43873


Ion Ratio Lower Upper

75 100

110 7.4 18.3 54.8#

77 0.0 25.1 37.7#

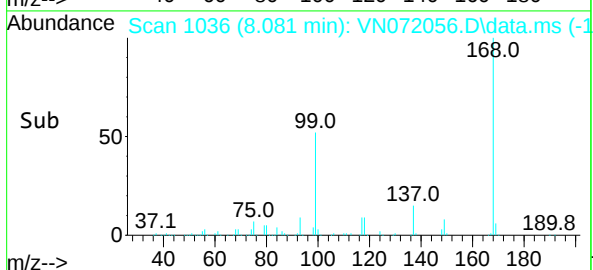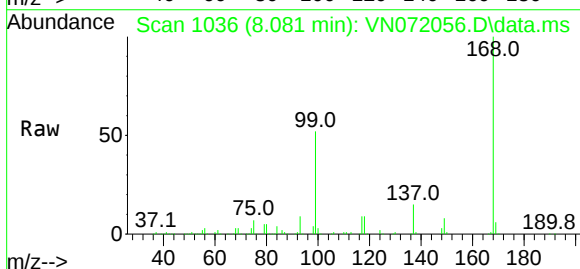



#37

Ethyl Acetate

Concen: 1.932 ug/l

RT: 7.334 min Scan# 909

Delta R.T. -0.070 min

Lab File: VN072056.D

Acq: 19 Apr 2022 17:50

Instrument :

MSVOA_N

ClientSampleId :

WC-15-1-7





Tgt Ion: 43 Resp: 19422

Ion Ratio Lower Upper

43 100

61 0.0 11.8 17.6#

70 0.0 9.3 13.9#

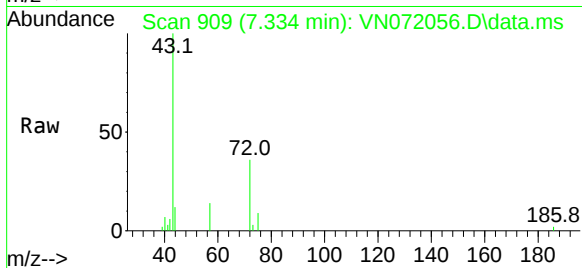

#38

Carbon Tetrachloride

Concen: 6.358 ug/l

RT: 8.081 min Scan# 1036

Delta R.T. -0.123 min

Lab File: VN072056.D

Acq: 19 Apr 2022 17:50




Tgt Ion: 117 Resp: 57224


Ion Ratio Lower Upper

117 100

119 4.8 75.8 113.8#

121 0.0 24.6 37.0#

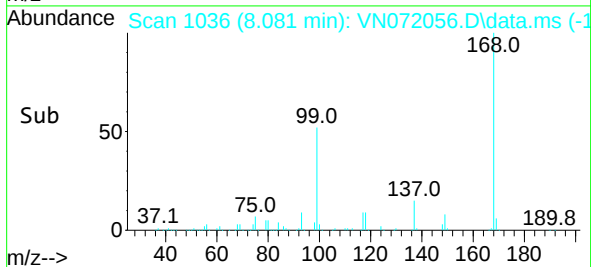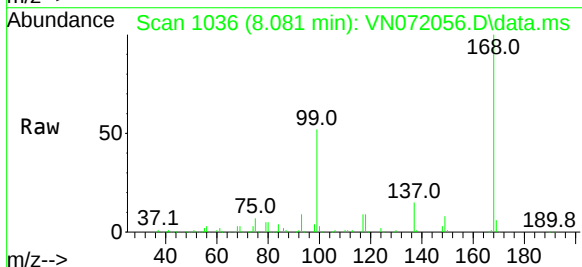

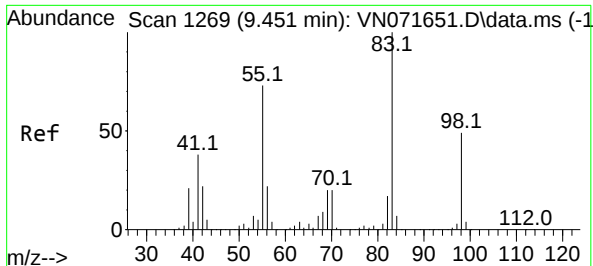

#39

Methylcyclohexane

Concen: 0.988 ug/l

RT: 9.451 min Scan# 1116

Delta R.T. 0.000 min

Lab File: VN072056.D

Acq: 19 Apr 2022 17:50

Instrument :

MSVOA_N

ClientSampleId :

WC-15-1-7





Tgt Ion: 83 Resp: 10803

Ion Ratio Lower Upper

83 100

55 60.0 57.8 86.8

98 48.2 39.4 59.2

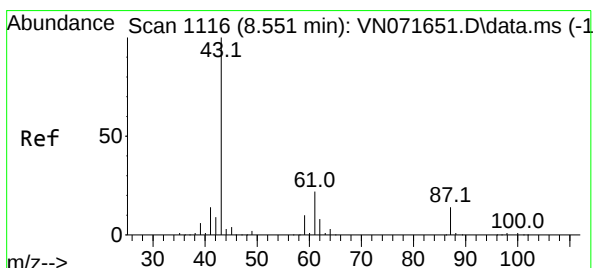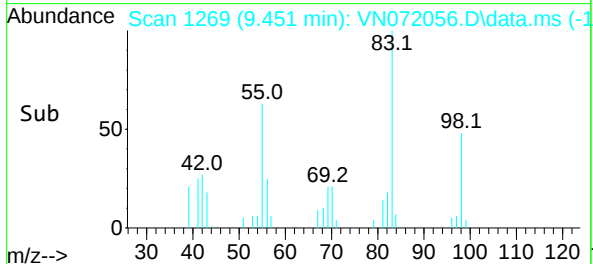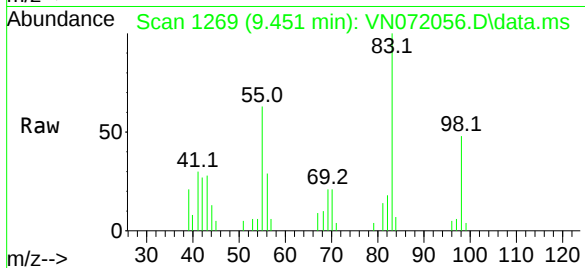

#43

Isopropyl Acetate

Concen: 6.106 ug/l

RT: 8.551 min Scan# 1116

Delta R.T. 0.000 min

Lab File: VN072056.D

Acq: 19 Apr 2022 17:50




Tgt Ion: 43 Resp: 102078


Ion Ratio Lower Upper

43 100

61 12.8 21.9 32.9#

87 8.5 12.0 18.0#

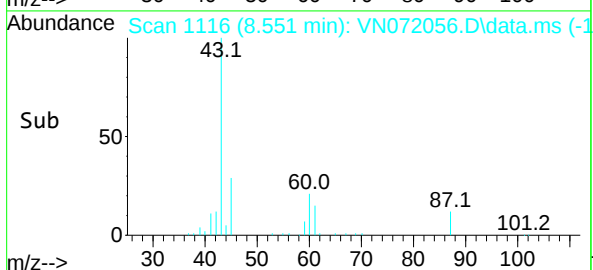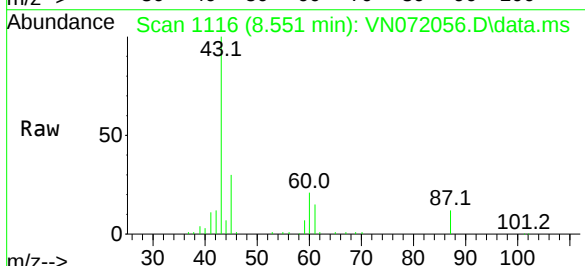

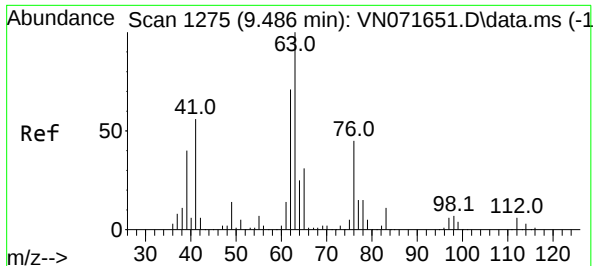

#45

1,2-Dichloropropane

Concen: 0.631 ug/l

RT: 9.616 min Scan# 1297

Delta R.T. 0.130 min

Lab File: VN072056.D

Acq: 19 Apr 2022 17:50

Instrument :

MSVOA_N

ClientSampleId :





WC-15-1-7

Tgt Ion: 63 Resp: 4570

Ion Ratio Lower Upper

63 100

65 0.0 24.9 37.3#

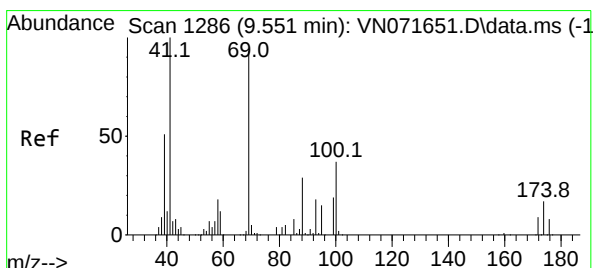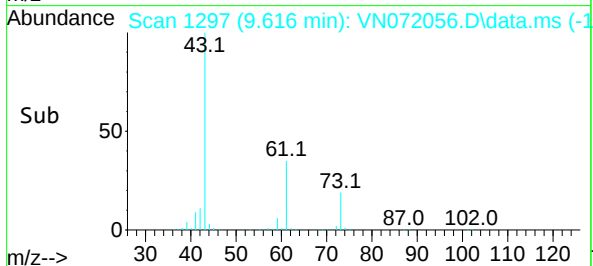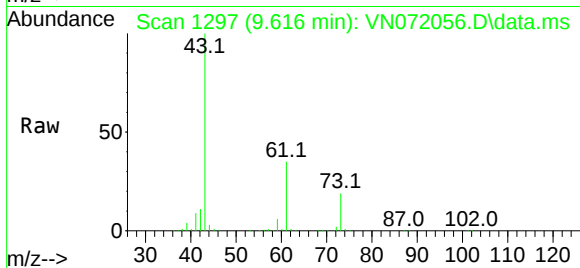

#48

Methyl methacrylate

Concen: 2.467 ug/l

RT: 9.539 min Scan# 1284

Delta R.T. -0.012 min

Lab File: VN072056.D

Acq: 19 Apr 2022 17:50




Tgt Ion: 41 Resp: 17115


Ion Ratio Lower Upper

41 100

69 0.0 74.7 112.1#

39 24.5 45.6 68.4#


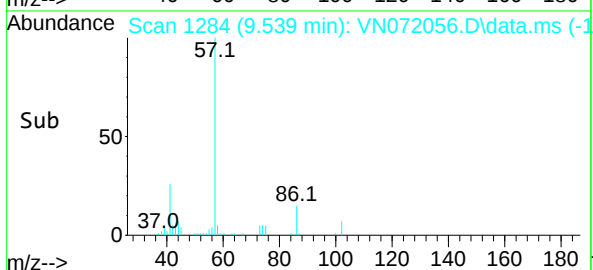

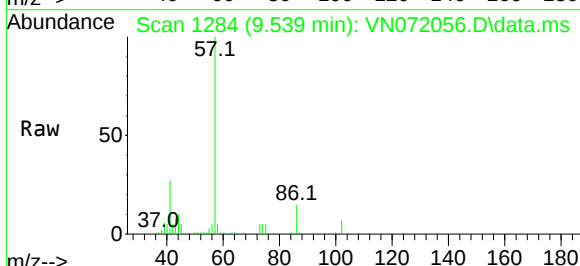


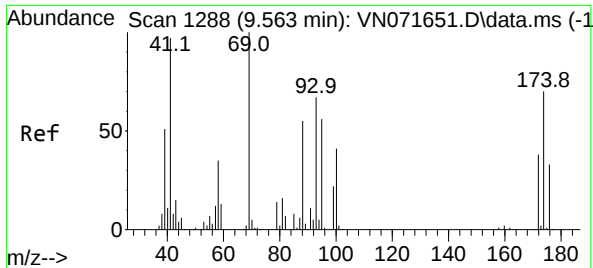

#49
1,4-Dioxane
Concen: Below Cal
RT: 9.622 min Scan# 11
Delta R.T. 0.059 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7


Tgt Ion: 88 Resp: 541
Ion Ratio Lower Upper
88 100
43 556523.3 20.2 30.4#
58 2725.7 54.2 81.4#

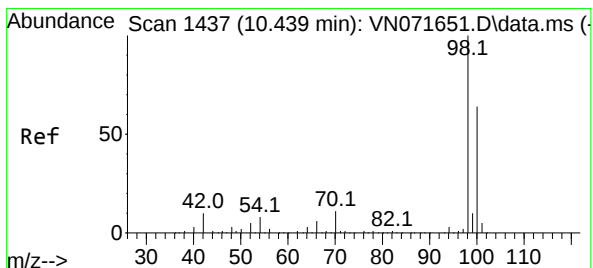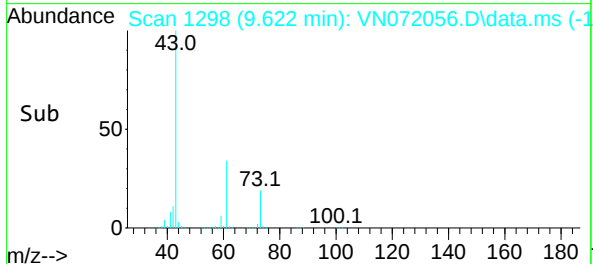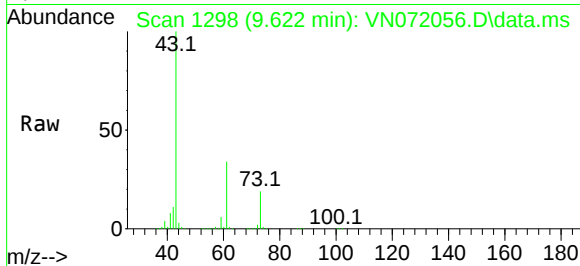

#50
Toluene-d8
Concen: 54.995 ug/l
RT: 10.433 min Scan# 1436
Delta R.T. -0.006 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50

Tgt Ion: 98 Resp: 1479443
Ion Ratio Lower Upper
98 100
100 64.9 52.6 78.8


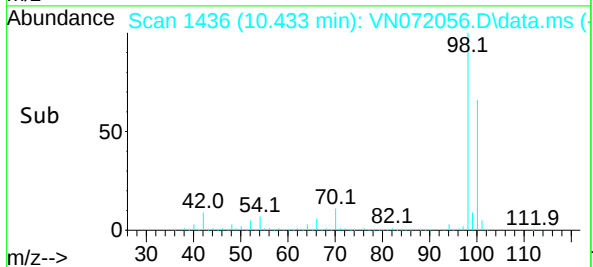

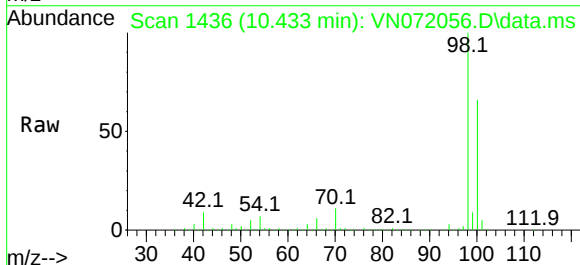




#51
4-Methyl-2-Pentanone
Concen: 1.261 ug/l
RT: 10.328 min Scan# 1417
Delta R.T. 0.006 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7


Tgt Ion: 43 Resp: 12117
Ion Ratio Lower Upper
43 100
58 48.6 34.1 51.1

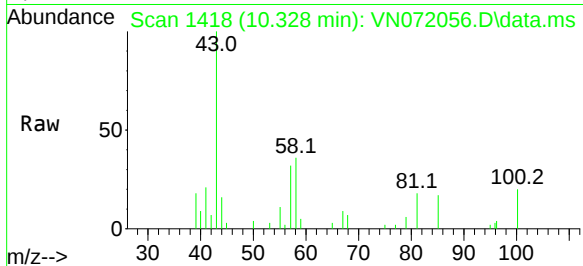

#54
cis-1,3-Dichloropropene
Concen: 9.142 ug/l
RT: 10.239 min Scan# 1403
Delta R.T. 0.053 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50

Tgt Ion: 75 Resp: 102542
Ion Ratio Lower Upper
75 100
77 0.5 25.2 37.8#
39 21.6 35.7 53.5#

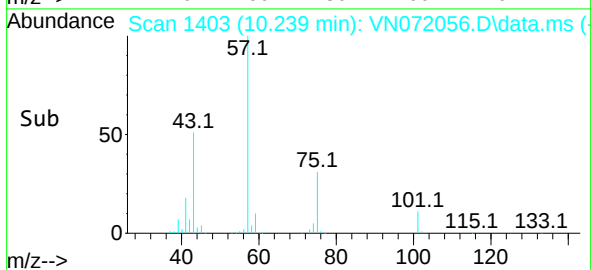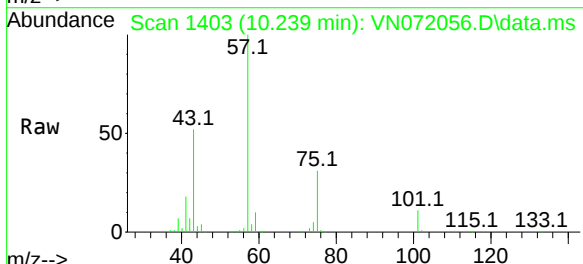



#57

1,3-Dichloropropane

Concen: 5.081 ug/l

RT: 11.086 min Scan# 1547

Delta R.T. 0.047 min

Lab File: VN072056.D

Acq: 19 Apr 2022 17:50

Instrument :

MSVOA_N

ClientSampleId :





WC-15-1-7

Tgt Ion: 76 Resp: 64119

Ion Ratio Lower Upper

76 100

78 0.2 26.2 39.2#

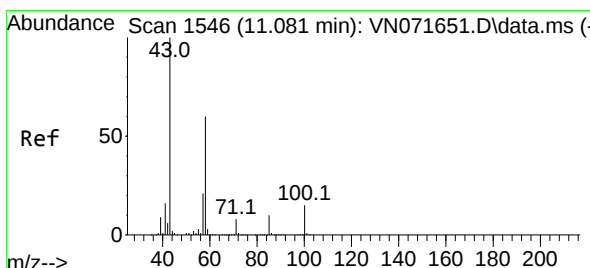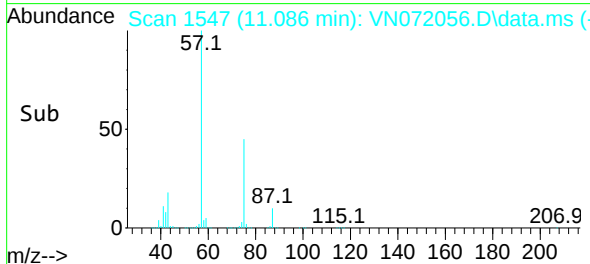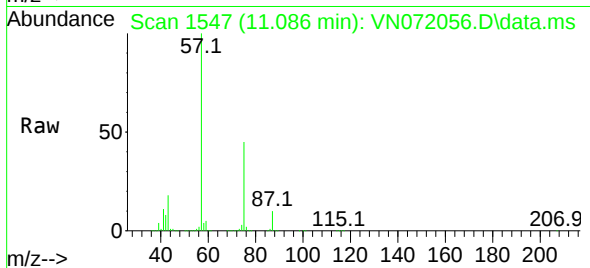

#59

2-Hexanone

Concen: 111.503 ug/l

RT: 11.086 min Scan# 1547

Delta R.T. 0.005 min

Lab File: VN072056.D




Acq: 19 Apr 2022 17:50


Tgt Ion: 43 Resp: 754605

Ion Ratio Lower Upper

43 100

58 20.8 29.7 89.1#


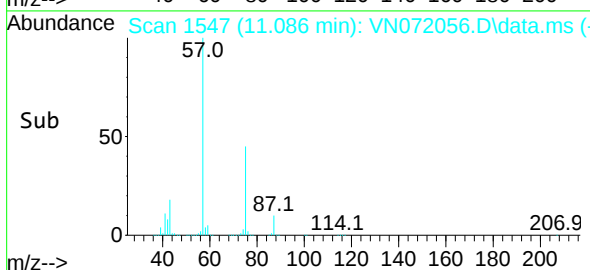






#62
4-Bromofluorobenzene
Concen: 60.103 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7


Tgt Ion: 95 Resp: 522919
Ion Ratio Lower Upper
95 100
174 86.4 0.0 167.6
176 82.2 0.0 163.4

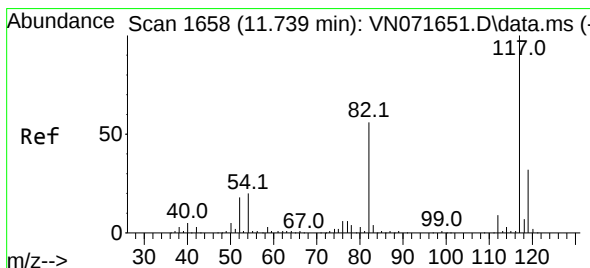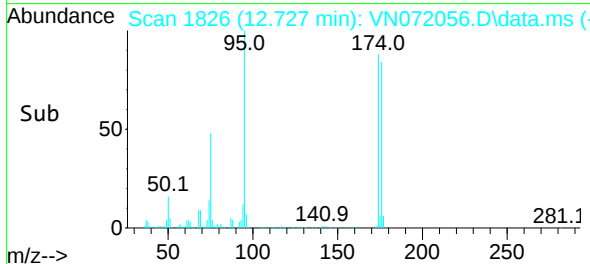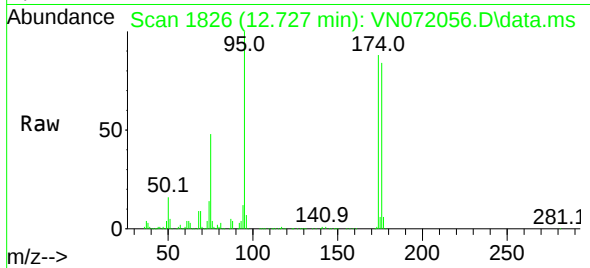

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1658
Delta R.T. 0.000 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50

Tgt Ion: 117 Resp: 1279478
Ion Ratio Lower Upper
117 100
82 55.8 44.2 66.2
119 32.0 25.4 38.0


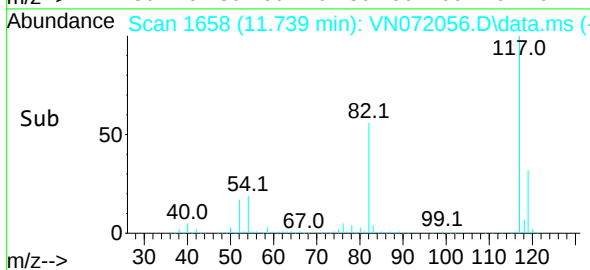

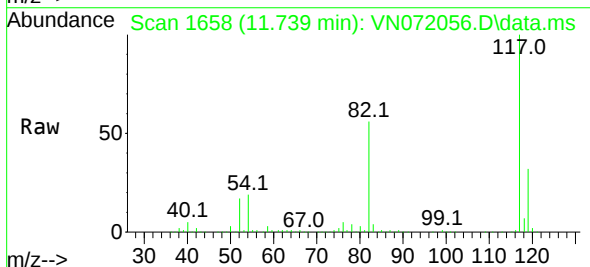




#68
m/p-Xylenes
Concen: 0.413 ug/l
RT: 11.951 min Scan# 1694
Delta R.T. 0.000 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7


Tgt Ion:106 Resp: 6890
Ion Ratio Lower Upper
106 100
91 204.0 158.9 238.3

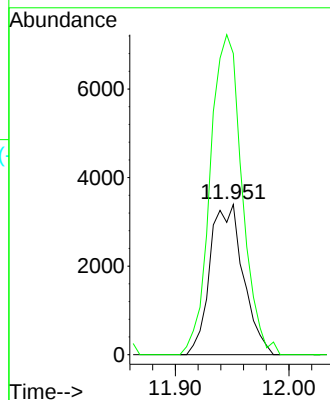

#69
o-Xylene
Concen: 0.829 ug/l
RT: 12.275 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50

Tgt Ion:106 Resp: 13704
Ion Ratio Lower Upper
106 100
91 215.2 106.0 318.0



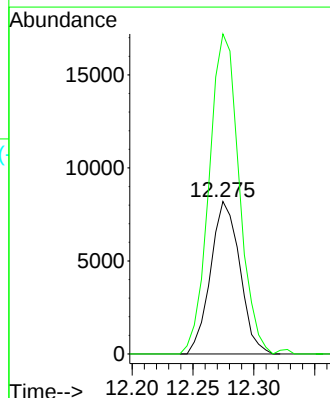
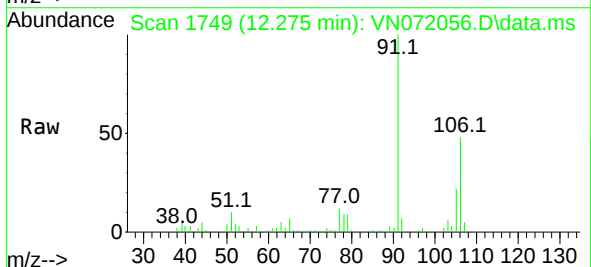




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.669 min Scan# 1986
Delta R.T. -0.000 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7


Tgt Ion:152 Resp: 471373
Ion Ratio Lower Upper
152 100
115 56.7 28.9 86.7
150 157.5 0.0 356.2

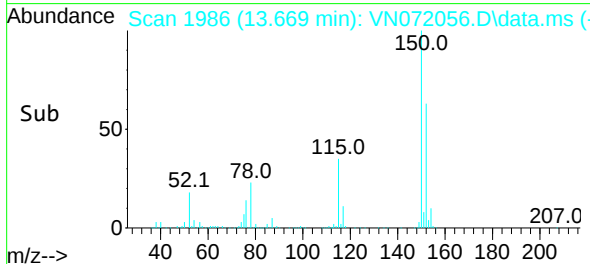

#73
Isopropylbenzene
Concen: 0.576 ug/l
RT: 12.575 min Scan# 1800
Delta R.T. -0.000 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50

Tgt Ion:105 Resp: 22882
Ion Ratio Lower Upper
105 100
120 26.2 13.5 40.4


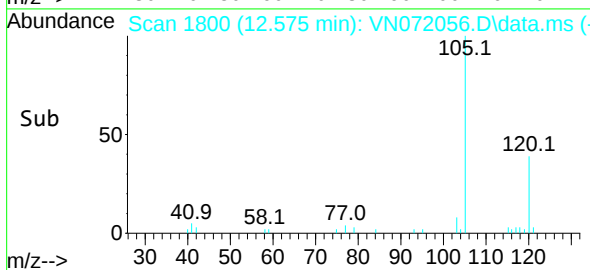

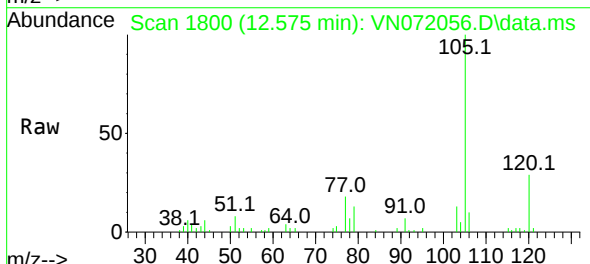




#74
N-amy1 acetate
Concen: 0.300 ug/l
RT: 12.351 min Scan# 11
Delta R.T. -0.029 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7


Tgt Ion: 43	Resp: 3409
Ion Ratio	Lower Upper
43 100	
70 0.0	39.0 58.4#
55 4.0	21.1 31.7#
61 0.0	21.1 31.7#

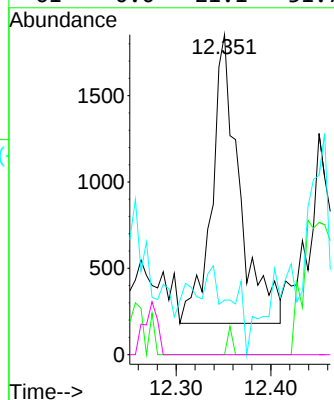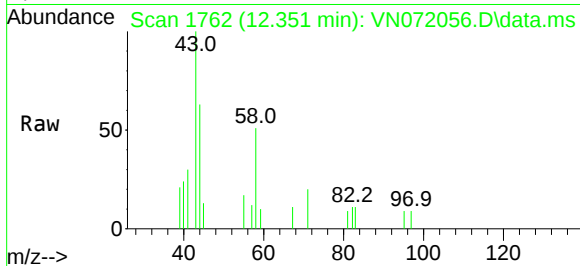

#76
1,2,3-Trichloropropane
Concen: 22.943 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50

Tgt Ion: 75	Resp: 250530
Ion Ratio	Lower Upper
75 100	
77 1.4	98.5 295.5#



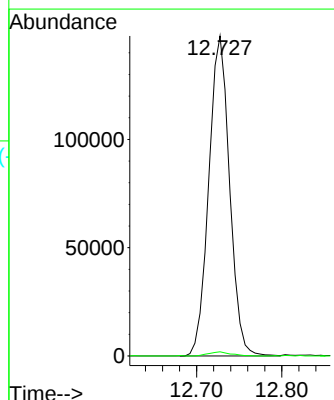
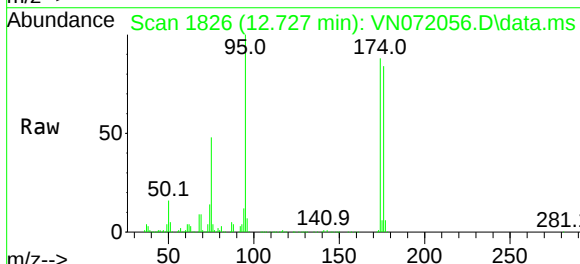




#78
n-propylbenzene
Concen: 0.250 ug/l
RT: 12.916 min Scan# 1858
Delta R.T. -0.000 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7


Tgt Ion: 91 Resp: 10429
Ion Ratio Lower Upper
91 100
120 20.0 11.9 35.5

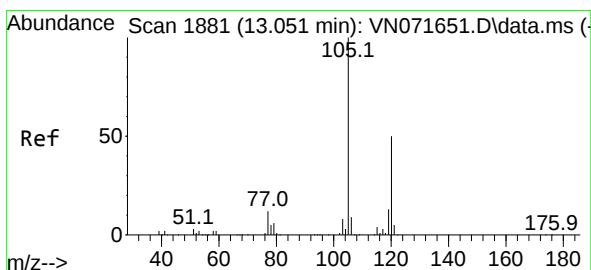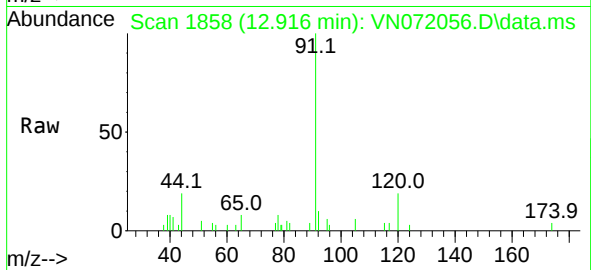

#80
1,3,5-Trimethylbenzene
Concen: 2.936 ug/l
RT: 13.057 min Scan# 1882
Delta R.T. 0.006 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50

Tgt Ion: 105 Resp: 92413
Ion Ratio Lower Upper
105 100
120 50.9 24.9 74.7


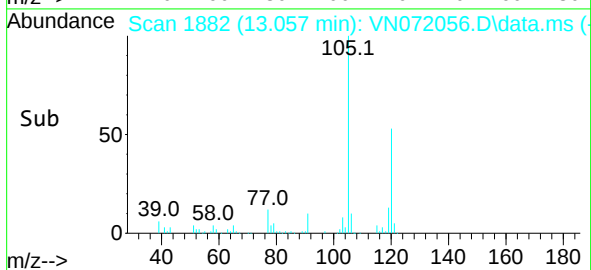

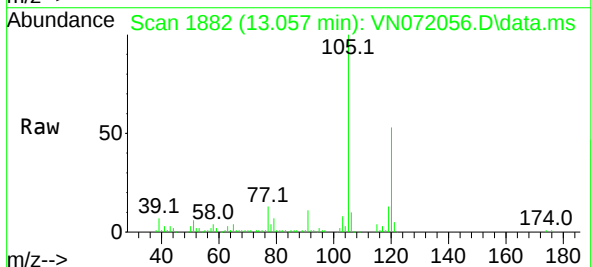




#81
trans-1,4-Dichloro-2-butene
Concen: 71.099 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.105 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7


Tgt Ion: 75 Resp: 250530
Ion Ratio Lower Upper
75 100
53 0.1 78.0 117.0#
89 0.0 37.2 55.8#

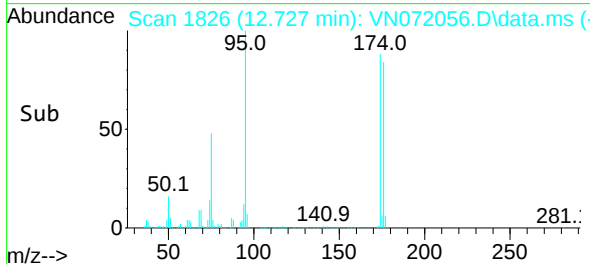

#82
4-Chlorotoluene
Concen: 0.397 ug/l
RT: 13.057 min Scan# 1882
Delta R.T. -0.041 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50

Tgt Ion: 91 Resp: 9854
Ion Ratio Lower Upper
91 100
126 0.0 17.2 51.6#


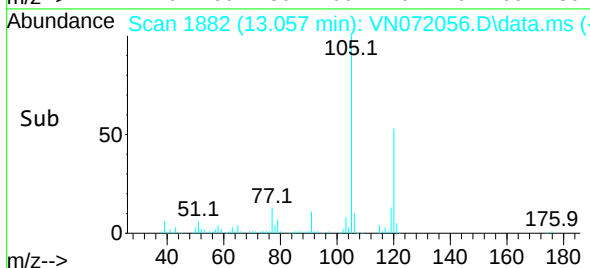

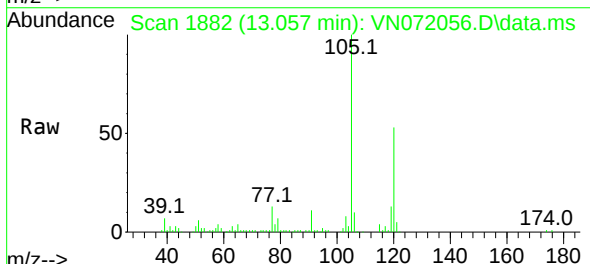




#84
1,2,4-Trimethylbenzene
Concen: 4.507 ug/l
RT: 13.363 min Scan# 1934
Delta R.T. -0.000 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7


Tgt Ion:105 Resp: 138408
Ion Ratio Lower Upper
105 100
120 45.4 23.3 69.8

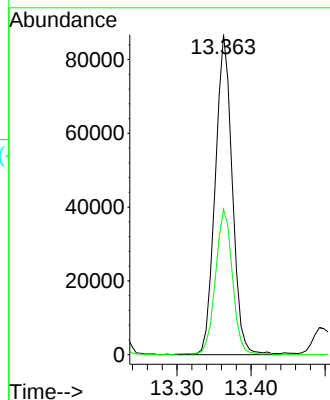

#85
sec-Butylbenzene
Concen: 0.341 ug/l
RT: 13.492 min Scan# 1956
Delta R.T. -0.006 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50

Tgt Ion:105 Resp: 12709
Ion Ratio Lower Upper
105 100
134 26.8 10.4 31.1



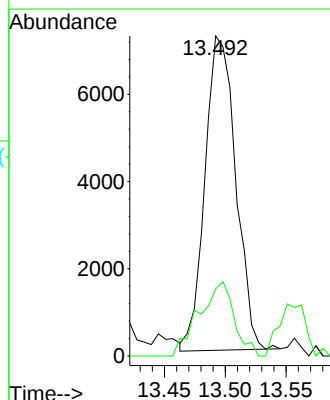
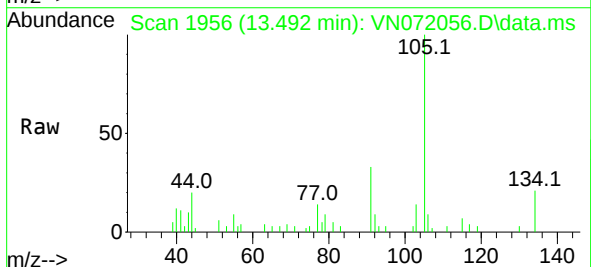




#86
p-Isopropyltoluene
Concen: 0.231 ug/l
RT: 13.557 min Scan# 1976
Delta R.T. -0.053 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50




Instrument :
MSVOA_N
ClientSampleId :
WC-15-1-7


Tgt Ion:119 Resp: 6868
Ion Ratio Lower Upper
119 100
134 27.4 13.3 39.8
91 29.4 11.3 33.9

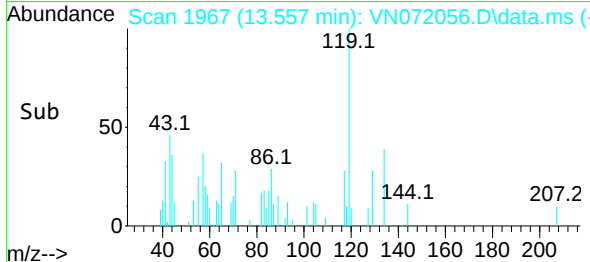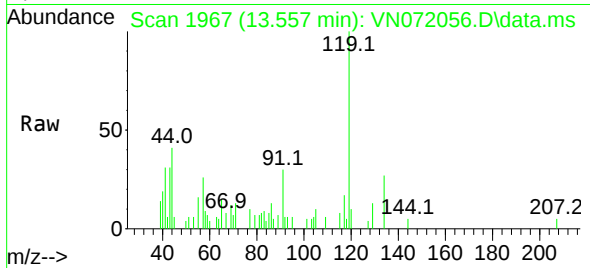

#90
Hexachloroethane
Concen: 0.699 ug/l
RT: 14.216 min Scan# 2079
Delta R.T. 0.012 min
Lab File: VN072056.D
Acq: 19 Apr 2022 17:50

Tgt Ion:117 Resp: 3803
Ion Ratio Lower Upper
117 100
201 0.0 40.6 122.0#

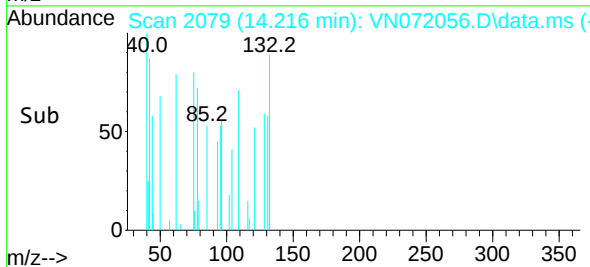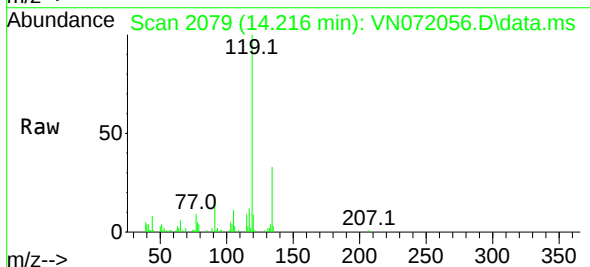



#95

Naphthalene

Concen: 4.024 ug/l

RT: 15.504 min Scan# 21

Delta R.T. 0.006 min

Lab File: VN072056.D


Acq: 19 Apr 2022 17:50

Instrument :

MSVOA_N

ClientSampleId :

WC-15-1-7

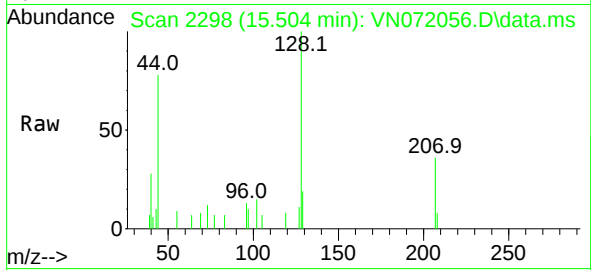

Tgt Ion:128 Resp: 5147

Ion Ratio Lower Upper

128 100

127 14.0 10.3 15.5

129 9.2 8.6 13.0

