
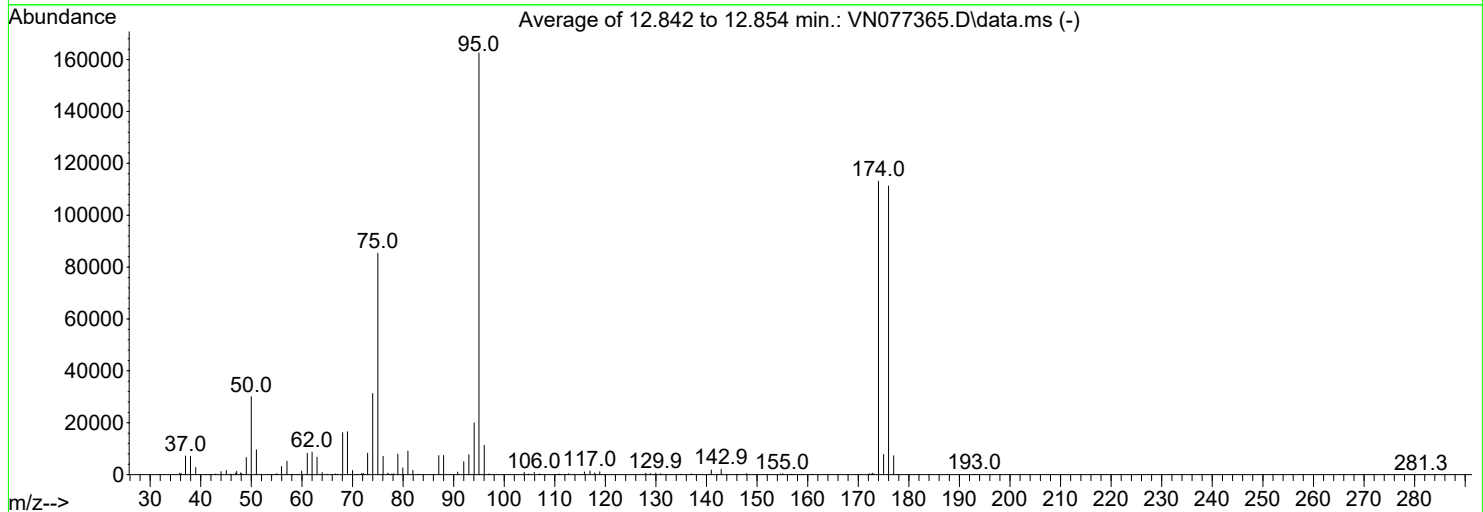


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041923\
Data File : VN077365.D
Acq On : 19 Apr 2023 08:59
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N040523W.M
Title : SW846 8260
Last Update : Thu Apr 06 08:27:03 2023

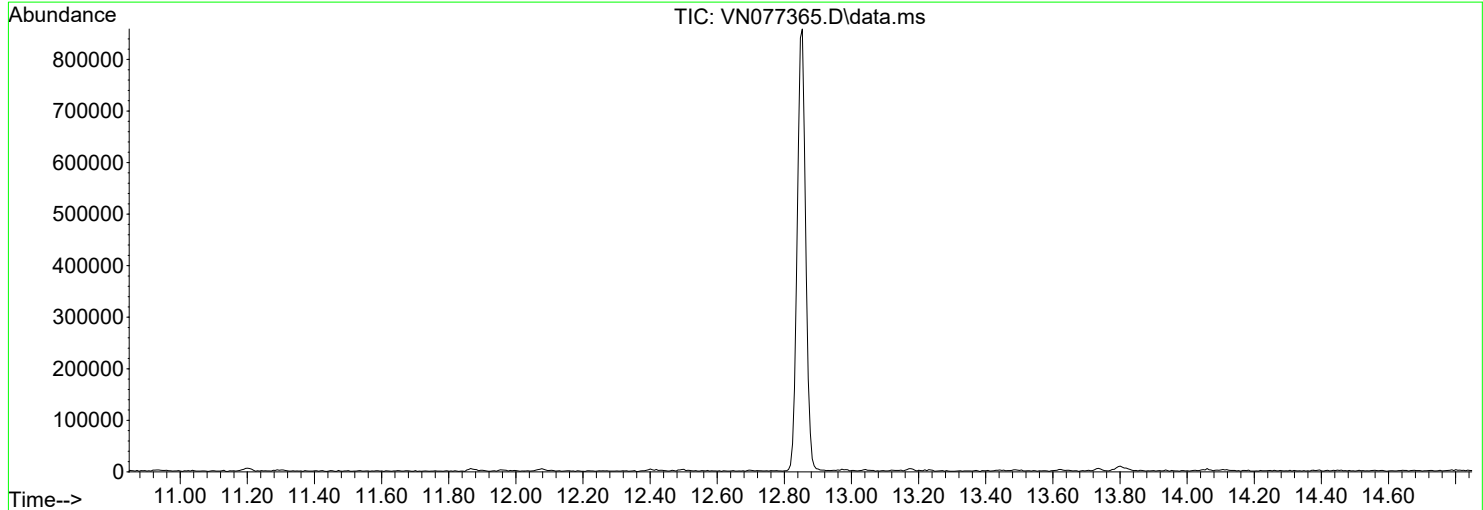

AutoFind: Scans 1854, 1855, 1856; Background Corrected with Scan 1845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	30059	PASS
75	95	30	60	52.5	85341	PASS
95	95	100	100	100.0	162581	PASS
96	95	5	9	6.9	11278	PASS
173	174	0.00	2	0.5	560	PASS
174	95	50	100	69.6	113112	PASS
175	174	5	9	6.9	7764	PASS
176	174	95	101	98.4	111256	PASS
177	176	5	9	6.6	7311	PASS

Average of 12.842 to 12.854 min.: VN077365.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	587	45.95	209	55.05	445	66.65	291
36.10	551	46.90	571	55.95	3142	67.05	163
37.00	7219	47.10	1284	57.05	5175	68.05	1623
37.95	7125	47.90	678	58.15	204	69.00	1654
39.00	2790	48.10	369	59.05	126	70.00	1634
41.10	50	49.00	6590	59.95	1330	70.80	64
41.90	60	50.00	30059	61.05	8291	71.85	488
42.90	261	51.00	9650	62.00	8703	72.15	443
44.00	1151	52.00	204	63.00	6720	73.00	8275
45.05	1612	53.80	63	64.00	776	74.00	31264
45.80	114	54.80	156	64.95	223	75.00	85341

Average of 12.842 to 12.854 min.: VN077365.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.05	7008	86.10	144	104.85	254	118.90	1106
76.90	121	87.05	7312	105.95	845	119.90	54
77.05	645	88.00	7411	106.95	288	127.80	189
77.70	269	90.80	1016	110.75	164	128.00	563
78.15	354	92.00	4975	110.95	185	128.90	409
78.95	7897	93.00	7735	111.90	131	129.80	146
79.95	2623	94.05	19960	112.70	391	129.95	634
80.95	9094	95.00	162581	115.20	60	130.90	356
81.95	1655	96.05	11278	115.85	1051	132.90	50
82.95	189	97.00	323	116.95	1403	134.90	217
84.00	94	103.95	946	117.90	696	137.00	316

Average of 12.842 to 12.854 min.: VN077365.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
140.95	1765	156.90	98	175.00	7764		
142.10	169	158.90	90	176.00	111256		
142.90	2121	160.85	196	177.00	7311		
145.90	204	170.40	55	177.80	117		
146.20	53	171.60	80	190.80	85		
147.85	424	171.90	146	193.00	213		
149.90	147	172.20	349	281.30	100		
154.65	246	172.60	212				
155.00	311	172.80	560				
155.20	153	173.10	323				
156.65	195	174.00	113112				

Instrument :

MSVOA_N

ClientSampleId :

BFB