


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041924\
Data File : VN081801.D
Acq On : 19 Apr 2024 11:03
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N041024W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Apr 11 09:25:01 2024

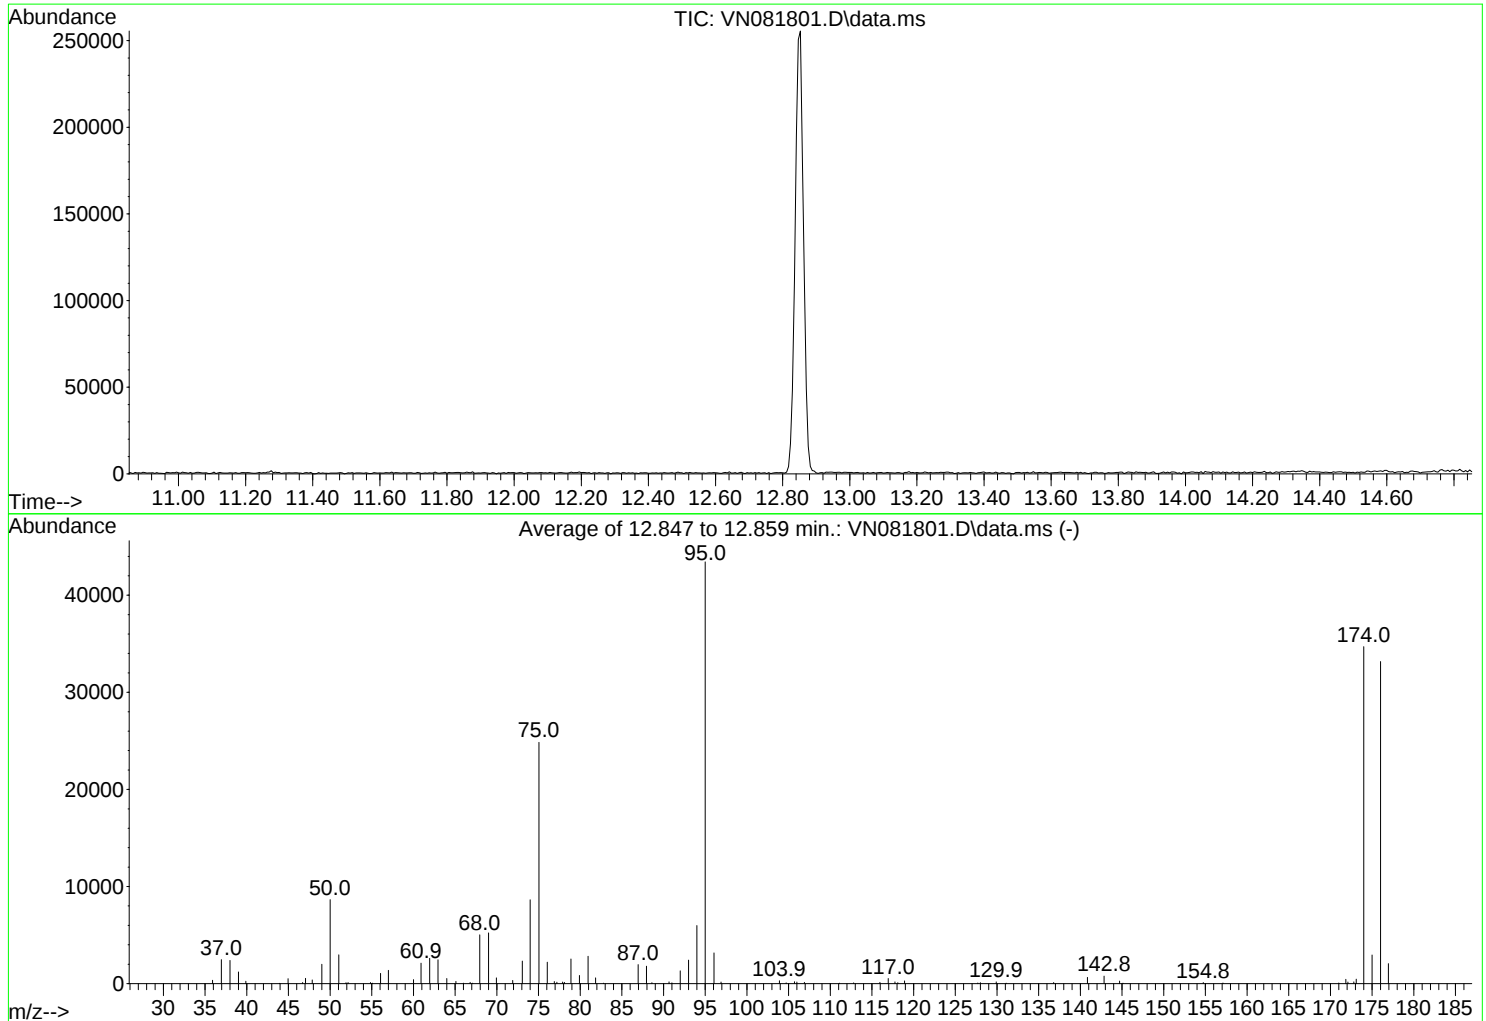

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.9	8654	PASS
75	95	30	60	57.2	24851	PASS
95	95	100	100	100.0	43435	PASS
96	95	5	9	7.3	3156	PASS
173	174	0.00	2	1.3	459	PASS
174	95	50	100	79.9	34699	PASS
175	174	5	9	8.5	2956	PASS
176	174	95	101	95.6	33163	PASS
177	176	5	9	6.2	2059	PASS