


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042021\
 Data File : VN066671.D
 Acq On : 20 Apr 2021 10:13
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N042021W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Apr 21 16:55:39 2021

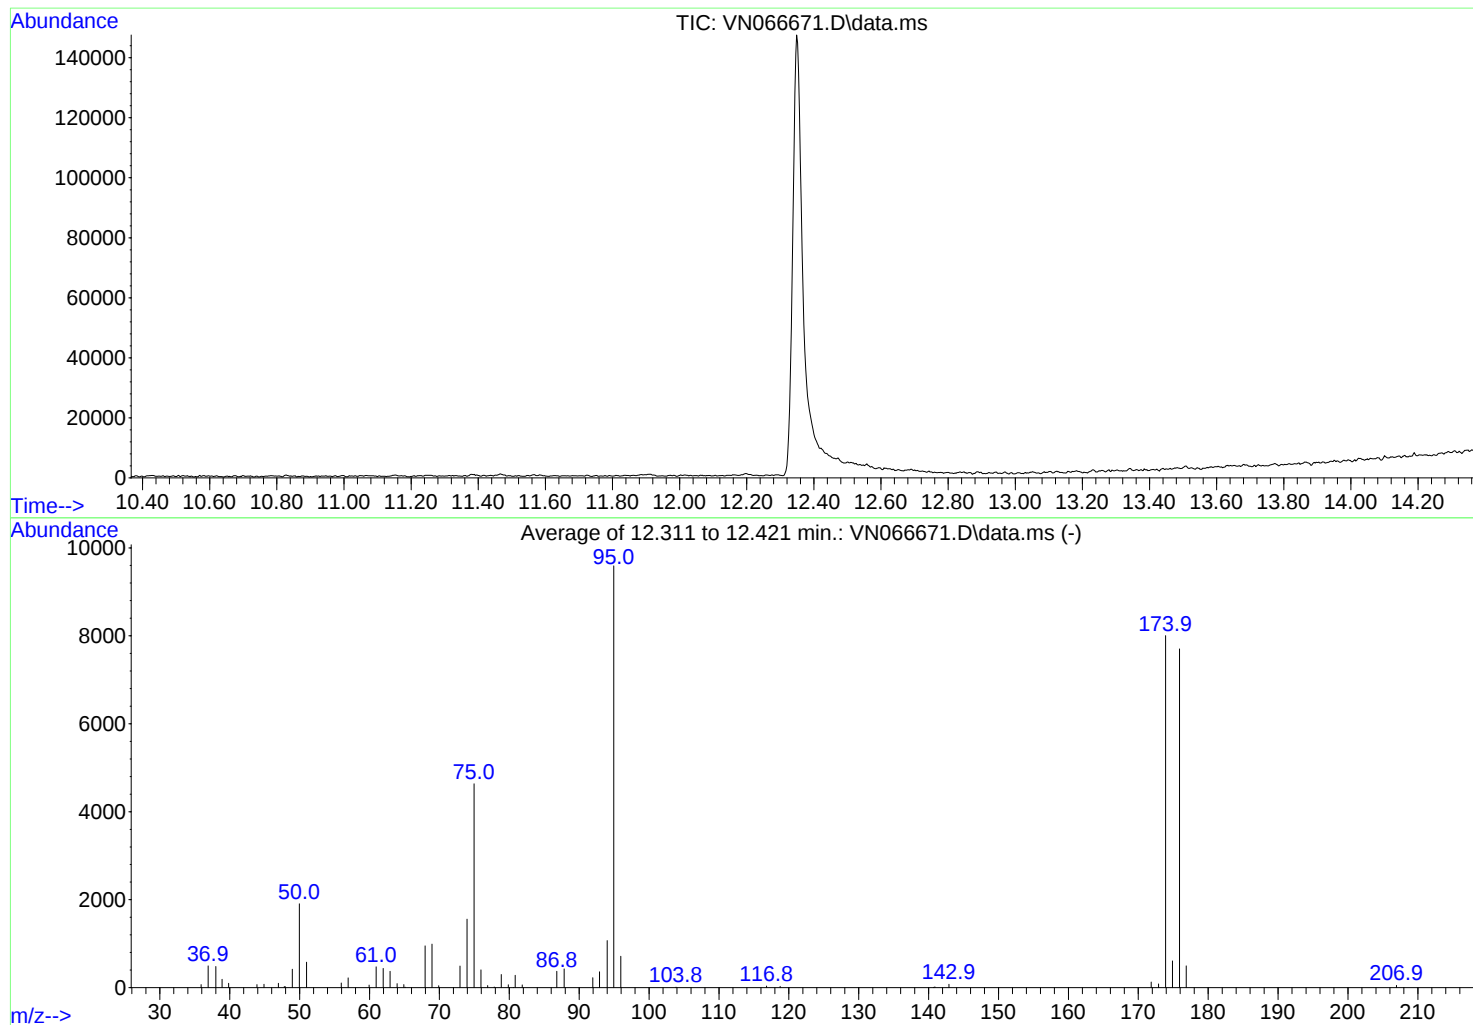

AutoFind: Averaged scan 3948 to 3989; Bkg corrected with scan 3947

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	1906	PASS
75	95	30	60	48.3	4636	PASS
95	95	100	100	100.0	9591	PASS
96	95	5	9	7.4	712	PASS
173	174	0.00	2	1.0	82	PASS
174	95	50	100	83.5	8004	PASS
175	174	5	9	7.6	608	PASS
176	174	95	101	96.3	7704	PASS
177	176	5	9	6.4	494	PASS