

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042022\
 Data File : VN072099.D
 Acq On : 21 Apr 2022 00:41
 Operator : JC\MD
 Sample : N2482-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Apr 21 03:40:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 31 01:57:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.081	168	615335	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1061473	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1134060	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.668	152	435879	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	326906	46.536	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	93.080%
35) Dibromofluoromethane	8.016	113	291930	46.737	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	93.480%
50) Toluene-d8	10.439	98	1317749	51.572	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	103.140%
62) 4-Bromofluorobenzene	12.727	95	491246	59.446	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	118.900%
Target Compounds						
					Qvalue	
3) Chloromethane	2.304	50	2849	0.460	ug/l	93
5) Bromomethane	2.863	94	1656	0.374	ug/l #	77
11) Tert butyl alcohol	5.363	59	2571	2.255	ug/l #	72
13) Acrolein	3.993	56	8296	5.968	ug/l #	1
16) Acetone	4.293	43	50990	16.985	ug/l	97
18) Methyl Acetate	4.857	43	7812	Below Cal	#	89
25) 2-Butanone	7.333	43	7808	1.804	ug/l #	87
29) Tetrahydrofuran	7.686	42	2026	0.723	ug/l #	81
31) Cyclohexane	8.092	56	35357	3.701	ug/l #	72
36) 1,1-Dichloropropene	8.081	75	40458	4.638	ug/l #	48
37) Ethyl Acetate	7.410	43	69753	7.306	ug/l #	95
38) Carbon Tetrachloride	8.081	117	54896	6.422	ug/l #	16
40) Benzene	8.457	78	447955	16.257	ug/l	99
41) Methacrylonitrile	7.704	41	1252	0.268	ug/l #	22
42) 1,2-Dichloroethane	8.445	62	4020	0.422	ug/l	81
43) Isopropyl Acetate	8.598	43	17723	1.116	ug/l #	53
52) Toluene	10.504	92	25289	1.452	ug/l	97
58) 2-Chloroethyl Vinyl ether	9.975	63	73	16.988	ug/l #	44
59) 2-Hexanone	11.086	43	2556	0.398	ug/l	90
67) Ethyl Benzene	11.839	91	65599	1.706	ug/l	96
68) m/p-Xylenes	11.957	106	15708	1.063	ug/l	95
73) Isopropylbenzene	12.574	105	32168	0.876	ug/l	98
76) 1,2,3-Trichloropropane	12.727	75	236938	23.465	ug/l #	1
78) n-propylbenzene	12.915	91	50880	1.317	ug/l	99
79) 2-Chlorotoluene	12.915	91	50880	2.053	ug/l #	40
81) trans-1,4-Dichloro-2-b...	12.727	75	236938	72.717	ug/l #	10
82) 4-Chlorotoluene	12.915	91	50880	2.215	ug/l #	40
90) Hexachloroethane	14.215	117	2247	0.446	ug/l #	9
93) 1,2,4-Trichlorobenzene	15.257	180	1721	2.324	ug/l	95
95) Naphthalene	15.498	128	21820	4.819	ug/l	99
96) 1,2,3-Trichlorobenzene	15.692	180	2058	2.706	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042022\
Data File : VN072099.D
Acq On : 21 Apr 2022 00:41
Operator : JC\MD
Sample : N2482-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Apr 21 03:40:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 31 01:57:54 2022
Response via : Initial Calibration

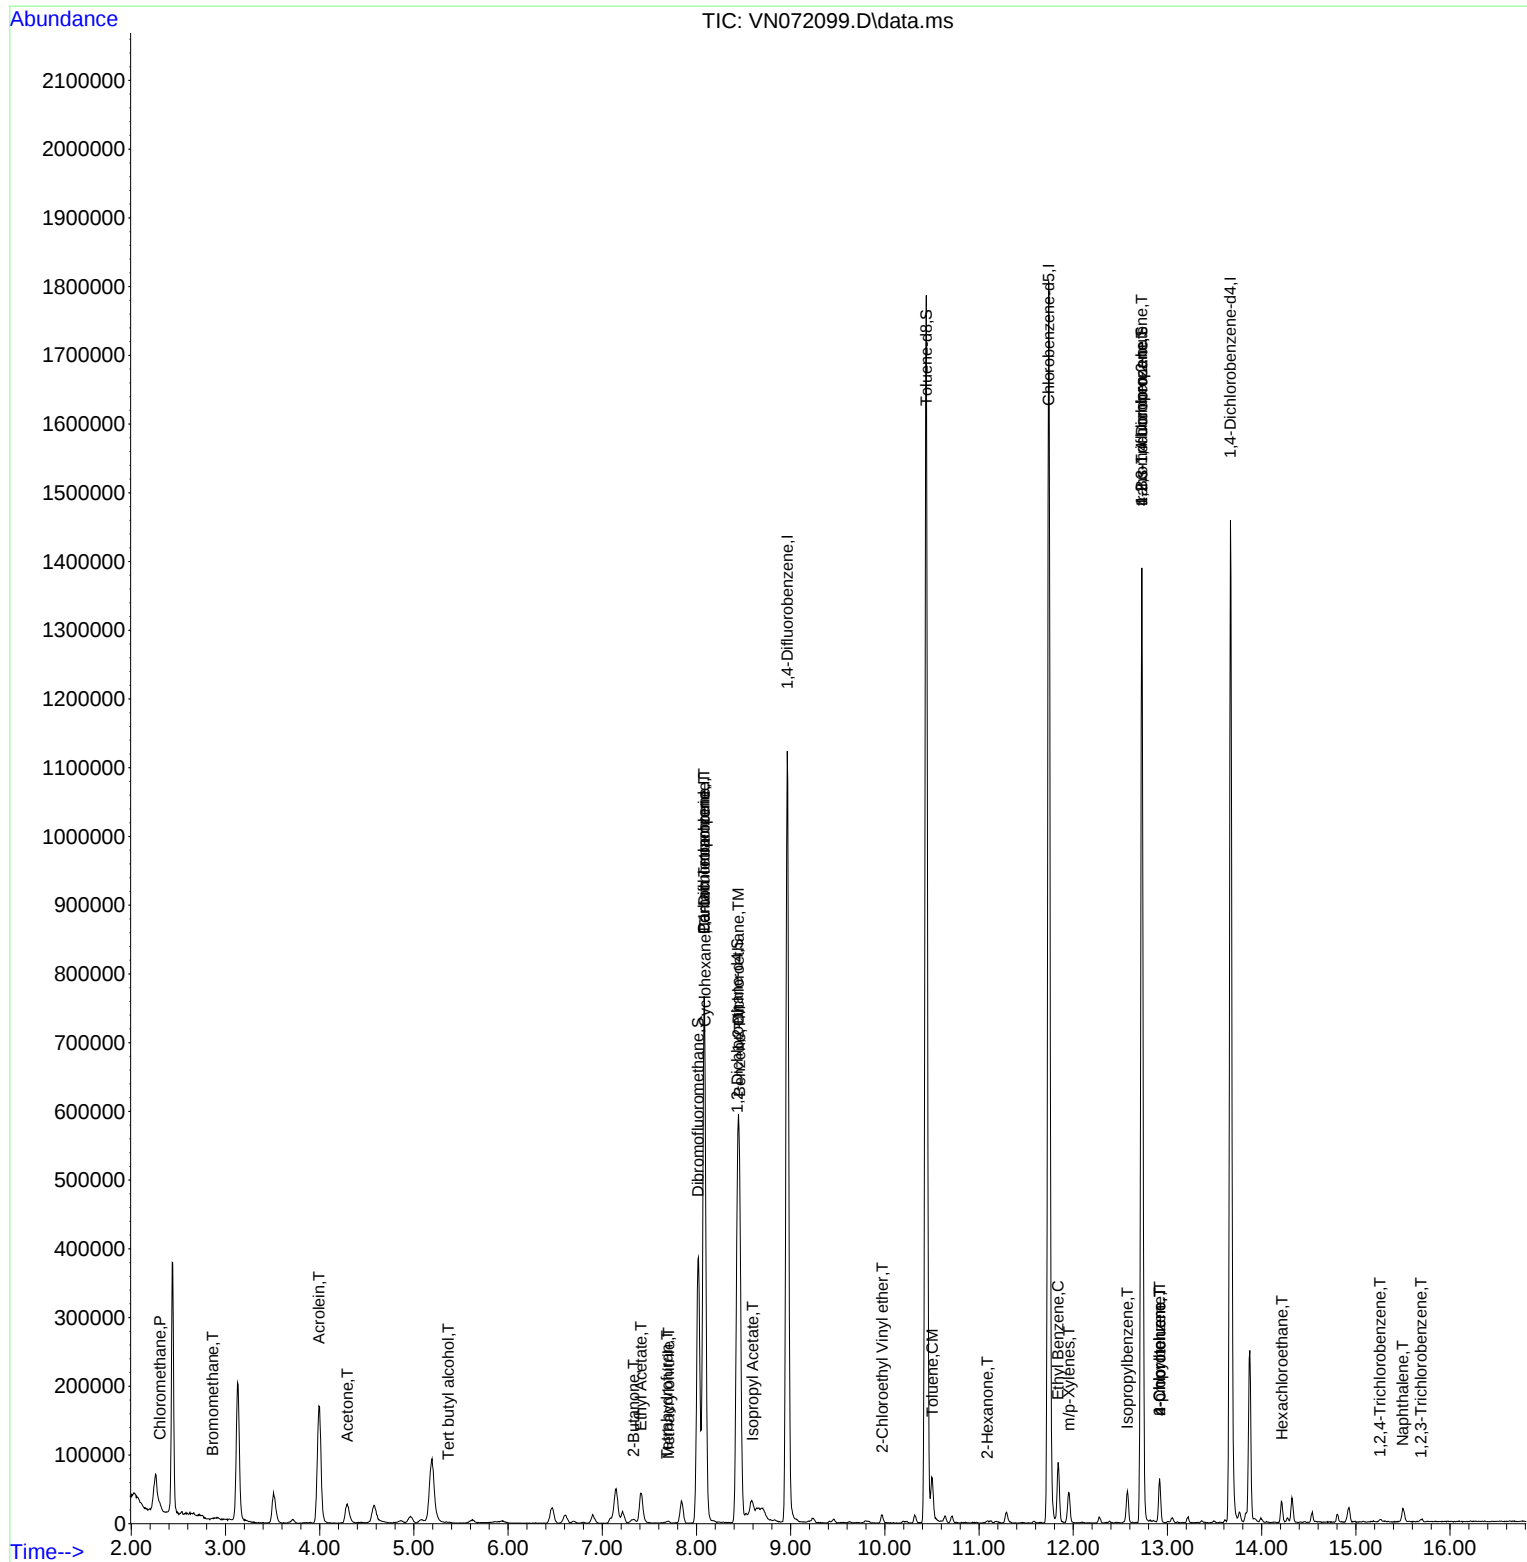






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41

Instrument :
MSVOA_N
ClientSampleId :



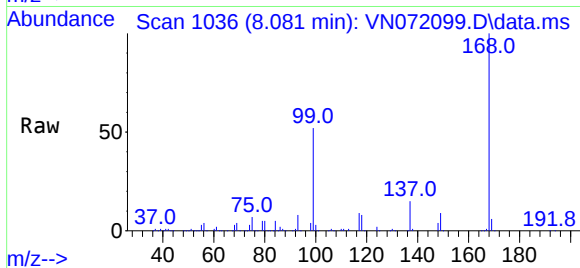



Tgt Ion:168 Resp: 615335
Ion Ratio Lower Upper
168 100
99 51.9 42.3 63.5

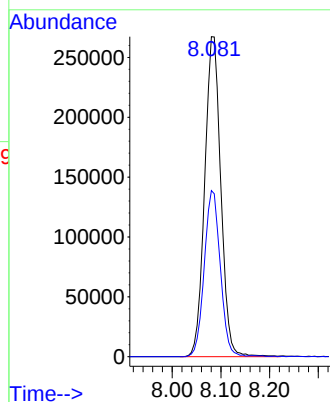

#3
Chloromethane
Concen: 0.460 ug/l
RT: 2.304 min Scan# 54
Delta R.T. 0.005 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41

Tgt Ion: 50 Resp: 2849
Ion Ratio Lower Upper
50 100
52 28.2 25.7 38.5


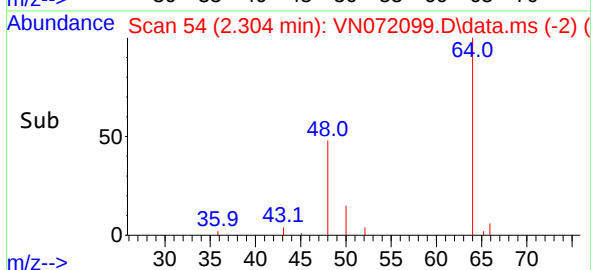

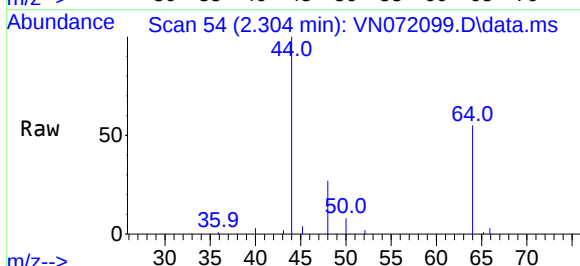




#5
Bromomethane
Concen: 0.374 ug/l
RT: 2.863 min Scan# 146
Delta R.T. 0.017 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 94 Resp: 1656
Ion Ratio Lower Upper
94 100
96 72.8 76.0 114.0#

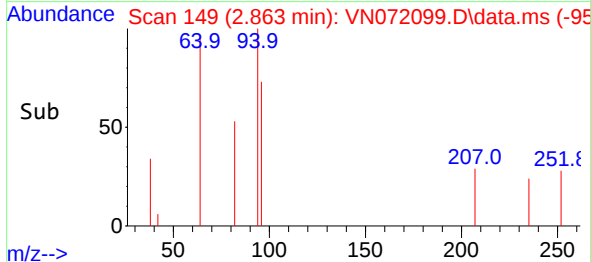

#11
Tert butyl alcohol
Concen: 2.255 ug/l
RT: 5.363 min Scan# 574
Delta R.T. 0.006 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41

Tgt Ion: 59 Resp: 2571
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#


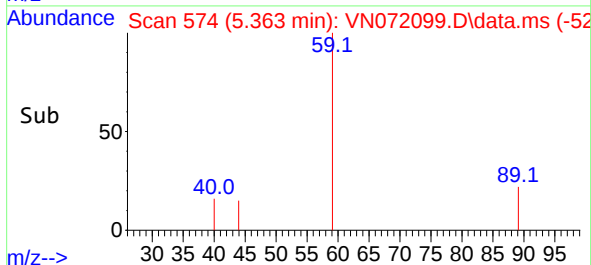
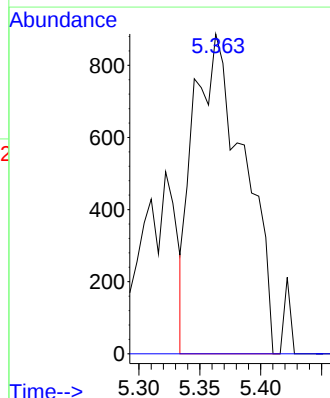
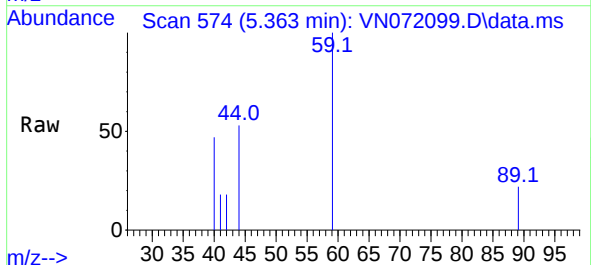




#13
Acrolein
Concen: 5.968 ug/l
RT: 3.993 min Scan# 341
Delta R.T. -0.047 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 56 Resp: 8296
Ion Ratio Lower Upper
56 100
55 2033.6 54.8 82.2#



#16
Acetone
Concen: 16.985 ug/l
RT: 4.293 min Scan# 392
Delta R.T. 0.018 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41


Tgt Ion: 43 Resp: 50990
Ion Ratio Lower Upper
43 100
58 34.4 26.0 39.0

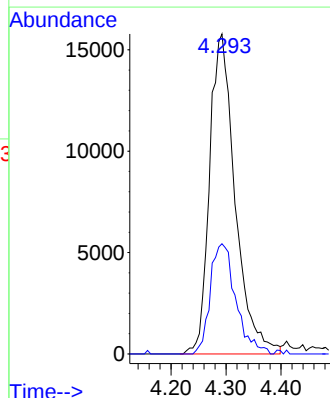






#18
Methyl Acetate
Concen: Below Cal
RT: 4.857 min Scan# 41
Delta R.T. 0.011 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43 Resp: 7812
Ion Ratio Lower Upper
43 100
74 21.3 21.6 32.4#



#25
2-Butanone
Concen: 1.804 ug/l
RT: 7.333 min Scan# 909
Delta R.T. 0.005 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41


Tgt Ion: 43 Resp: 7808
Ion Ratio Lower Upper
43 100
72 22.5 23.7 35.5#

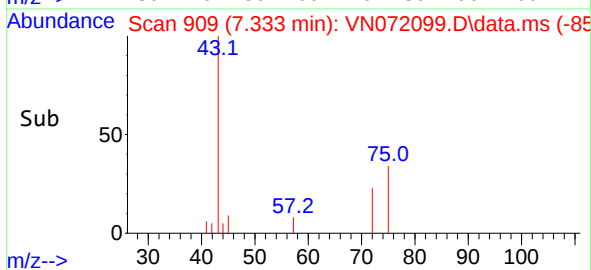



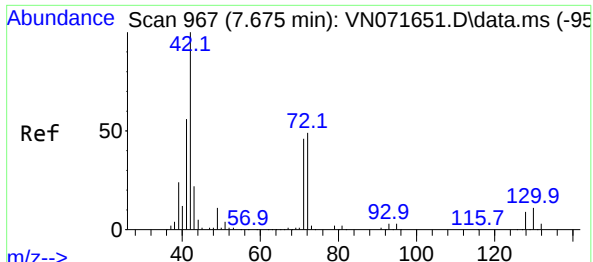


#29
Tetrahydrofuran
Concen: 0.723 ug/l
RT: 7.686 min Scan# 967
Delta R.T. 0.011 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41

Instrument :
MSVOA_N
ClientSampleId :



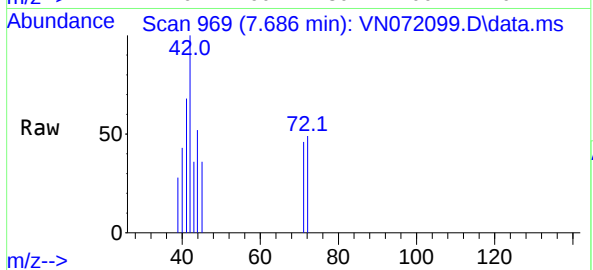



Tgt Ion: 42 Resp: 2026
Ion Ratio Lower Upper
42 100
72 31.5 39.7 59.5#
71 38.6 36.6 55.0

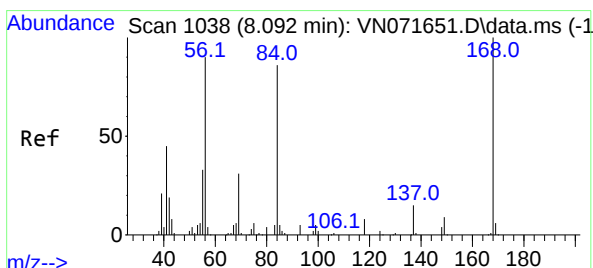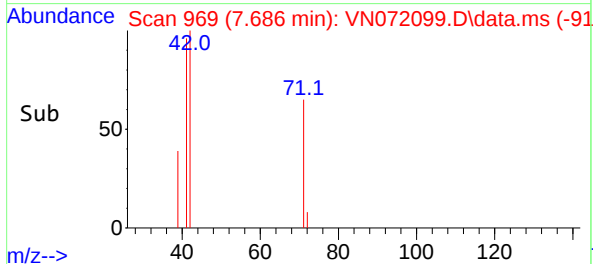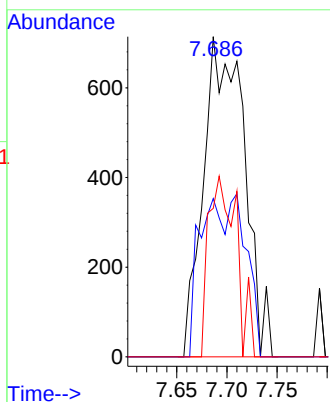

#31
Cyclohexane
Concen: 3.701 ug/l
RT: 8.092 min Scan# 1038
Delta R.T. 0.000 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41

Tgt Ion: 56 Resp: 35357
Ion Ratio Lower Upper
56 100
69 76.1 27.8 41.8#
84 108.5 76.9 115.3


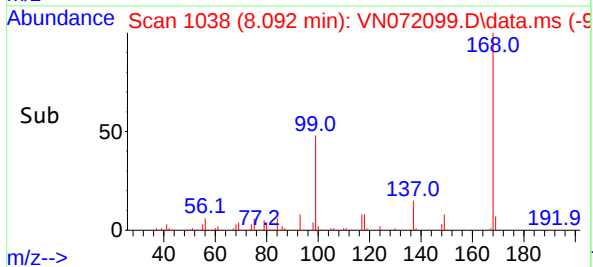
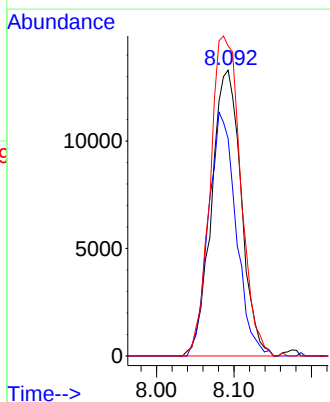
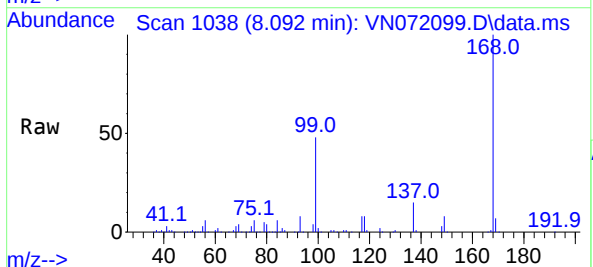




#33
1,2-Dichloroethane-d4
Concen: 46.536 ug/l
RT: 8.433 min Scan# 1096
Delta R.T. -0.001 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 65 Resp: 326906
Ion Ratio Lower Upper
65 100
67 53.1 0.0 104.8

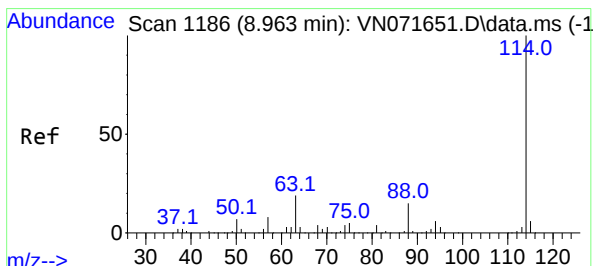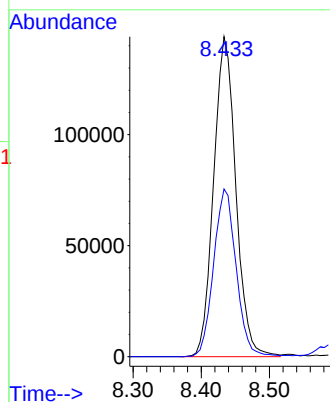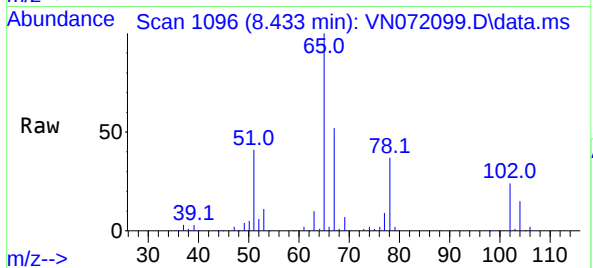

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.963 min Scan# 1186
Delta R.T. -0.000 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41


Tgt Ion:114 Resp: 1061473
Ion Ratio Lower Upper
114 100
63 18.5 0.0 40.0
88 15.4 0.0 32.6

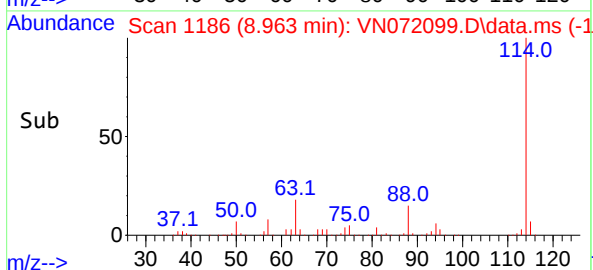



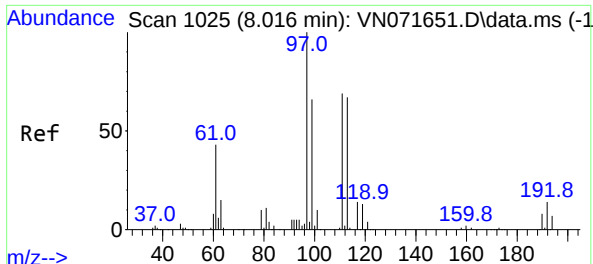


#35
Dibromofluoromethane
Concen: 46.737 ug/l
RT: 8.016 min Scan# 1035
Delta R.T. -0.000 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41

Instrument :
MSVOA_N
ClientSampleId :



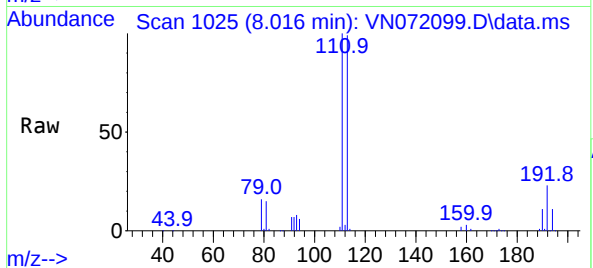



Tgt Ion:113 Resp: 291930
Ion Ratio Lower Upper
113 100
111 104.2 81.4 122.0
192 22.7 17.0 25.6

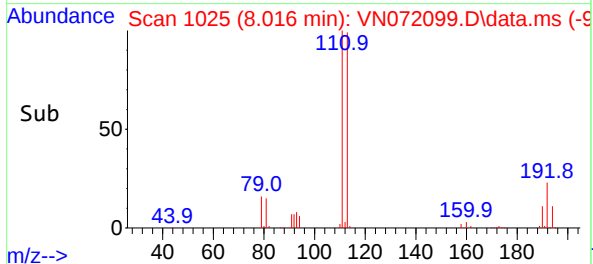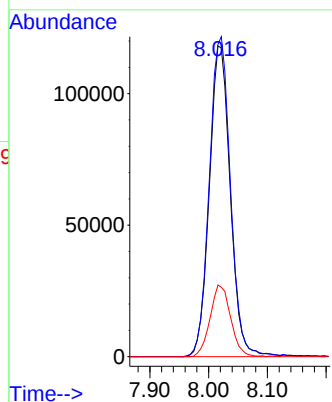

#36
1,1-Dichloropropene
Concen: 4.638 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.135 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41


Tgt Ion: 75 Resp: 40458
Ion Ratio Lower Upper
75 100
110 8.4 18.3 54.8#
77 0.0 25.1 37.7#

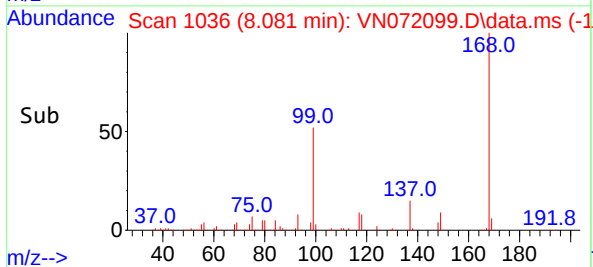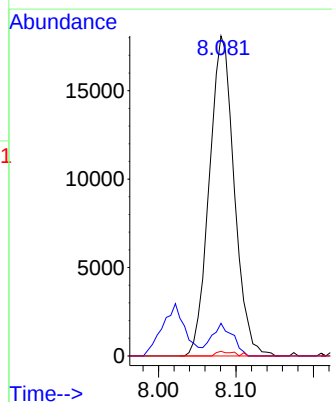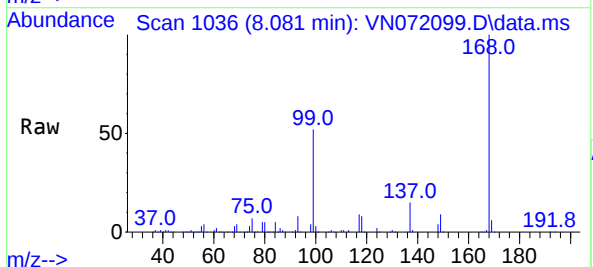






#37
Ethyl Acetate
Concen: 7.306 ug/l
RT: 7.410 min Scan# 91
Delta R.T. 0.006 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43 Resp: 69753
Ion Ratio Lower Upper
43 100
61 16.3 11.8 17.6
70 14.1 9.3 13.9#



#38
Carbon Tetrachloride
Concen: 6.422 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.123 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41

Tgt Ion: 117 Resp: 54896
Ion Ratio Lower Upper
117 100
119 4.3 75.8 113.8#
121 0.0 24.6 37.0#


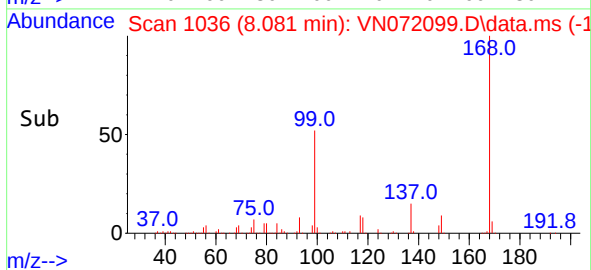






#40
Benzene
Concen: 16.257 ug/l
RT: 8.457 min Scan# 1100
Delta R.T. -0.000 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 78 Resp: 447955
Ion Ratio Lower Upper
78 100
77 23.9 19.4 29.0

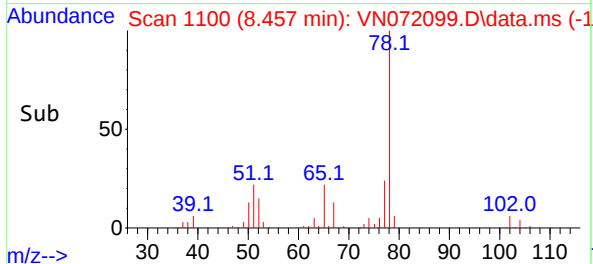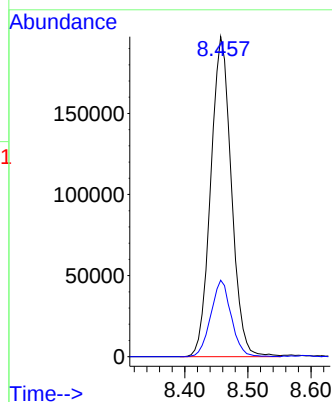

#41
Methacrylonitrile
Concen: 0.268 ug/l
RT: 7.704 min Scan# 972
Delta R.T. 0.076 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41

Tgt Ion: 41 Resp: 1252
Ion Ratio Lower Upper
41 100
39 15.6 48.6 73.0#
67 0.0 73.4 110.2#
52 0.0 27.7 41.5#


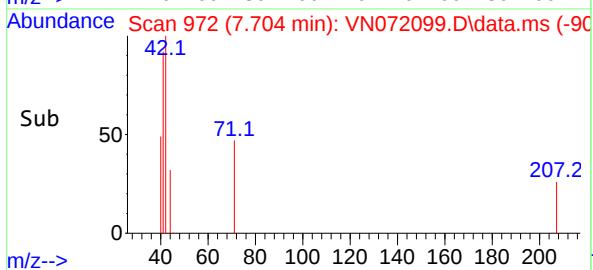

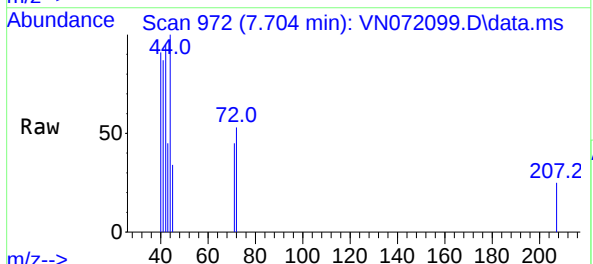




#42
1,2-Dichloroethane
Concen: 0.422 ug/l
RT: 8.445 min Scan# 1109
Delta R.T. -0.083 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 62 Resp: 4020
Ion Ratio Lower Upper
62 100
98 2.7 0.0 19.4

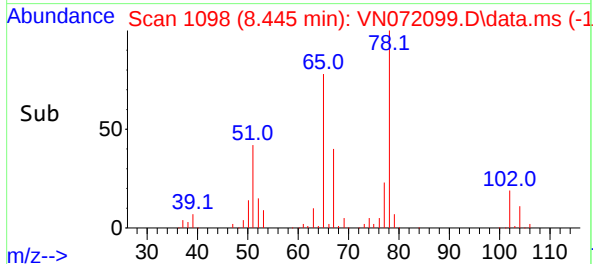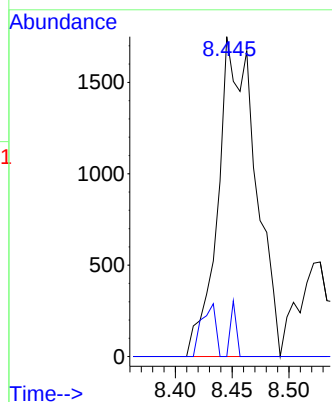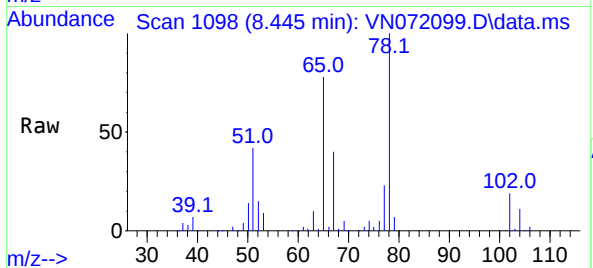

#43
Isopropyl Acetate
Concen: 1.116 ug/l
RT: 8.598 min Scan# 1124
Delta R.T. 0.047 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41

Tgt Ion: 43 Resp: 17723
Ion Ratio Lower Upper
43 100
61 0.0 21.9 32.9#
87 0.0 12.0 18.0#


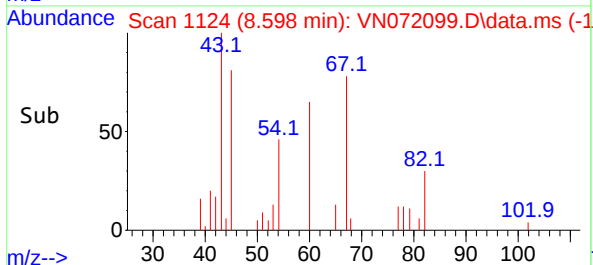

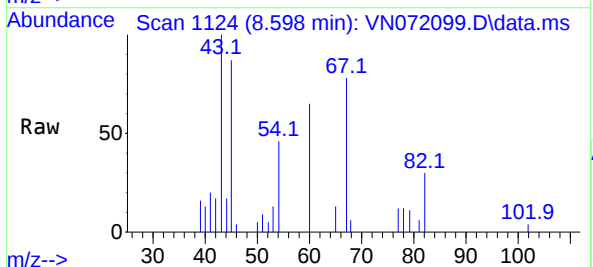




#50
Toluene-d8
Concen: 51.572 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 1317749
Ion Ratio Lower Upper
98 100
100 64.6 52.6 78.8



#52
Toluene
Concen: 1.452 ug/l
RT: 10.504 min Scan# 1448
Delta R.T. 0.006 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41

Tgt Ion: 92 Resp: 25289
Ion Ratio Lower Upper
92 100
91 176.9 138.6 207.8


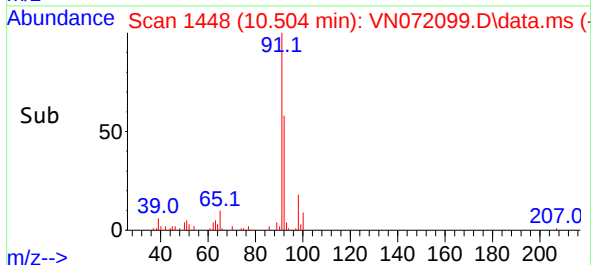
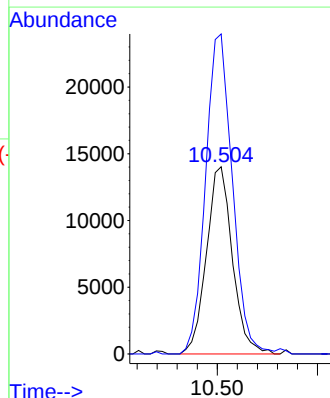
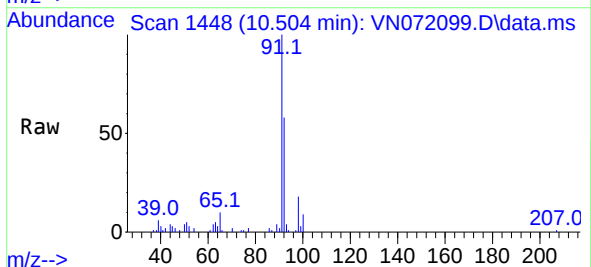




#58
2-Chloroethyl Vinyl ether
Concen: 16.988 ug/l
RT: 9.975 min Scan# 11
Delta R.T. -0.059 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 63 Resp: 73
Ion Ratio Lower Upper
63 100
106 0.0 24.6 36.8#

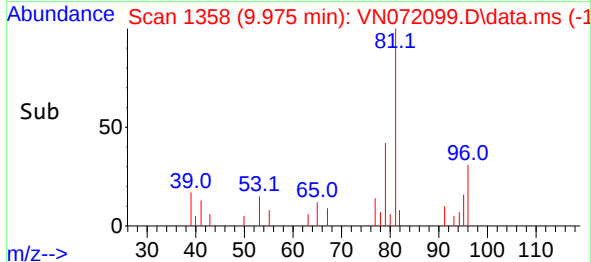

#59
2-Hexanone
Concen: 0.398 ug/l
RT: 11.086 min Scan# 1547
Delta R.T. 0.005 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41

Tgt Ion: 43 Resp: 2556
Ion Ratio Lower Upper
43 100
58 52.1 29.7 89.1


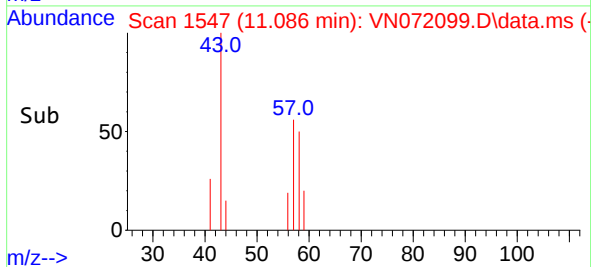

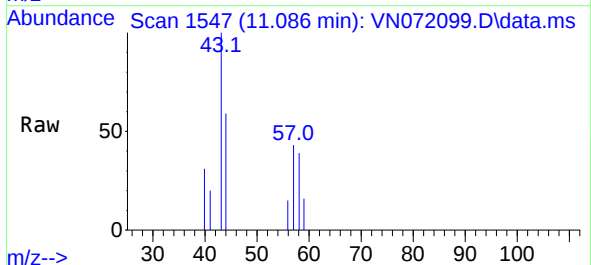




#62
4-Bromofluorobenzene
Concen: 59.446 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 491246
Ion Ratio Lower Upper
95 100
174 87.4 0.0 167.6
176 84.9 0.0 163.4

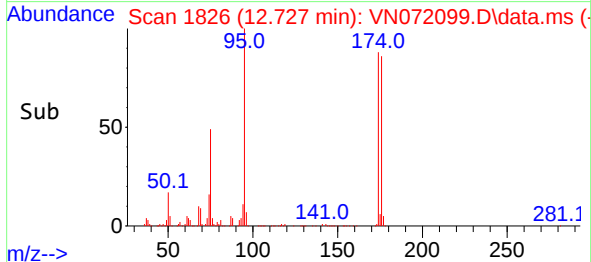

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1658
Delta R.T. 0.000 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41

Tgt Ion: 117 Resp: 1134060
Ion Ratio Lower Upper
117 100
82 54.5 44.2 66.2
119 32.0 25.4 38.0


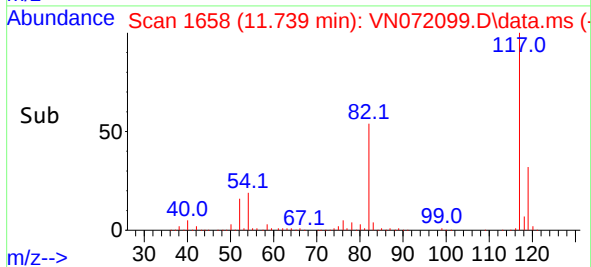

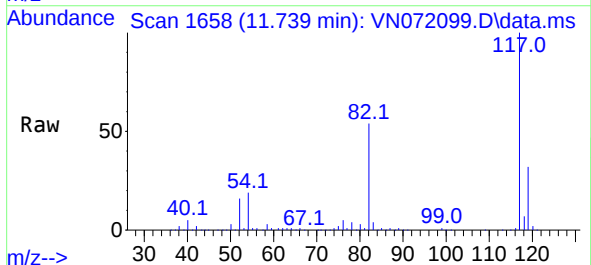




#67
Ethyl Benzene
Concen: 1.706 ug/l
RT: 11.839 min Scan# 1675
Delta R.T. 0.000 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 65599
Ion Ratio Lower Upper
91 100
106 33.1 24.9 37.3

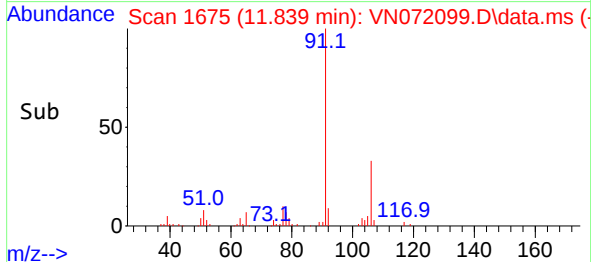

#68
m/p-Xylenes
Concen: 1.063 ug/l
RT: 11.957 min Scan# 1695
Delta R.T. 0.006 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41


Tgt Ion: 106 Resp: 15708
Ion Ratio Lower Upper
106 100
91 191.7 158.9 238.3

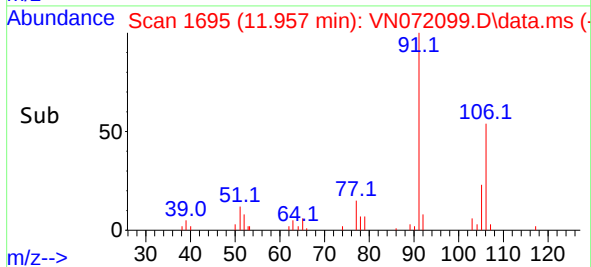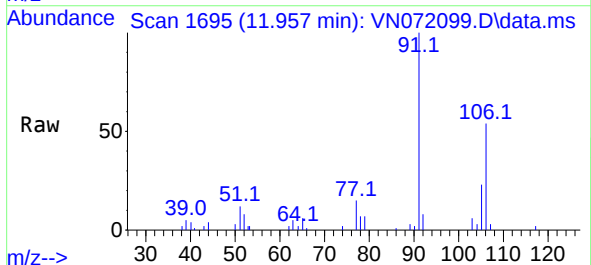






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.668 min Scan# 1986
Delta R.T. -0.001 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:152 Resp: 435879
Ion Ratio Lower Upper
152 100
115 56.2 28.9 86.7
150 157.3 0.0 356.2



#73
Isopropylbenzene
Concen: 0.876 ug/l
RT: 12.574 min Scan# 1800
Delta R.T. -0.001 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41

Tgt Ion:105 Resp: 32168
Ion Ratio Lower Upper
105 100
120 25.6 13.5 40.4


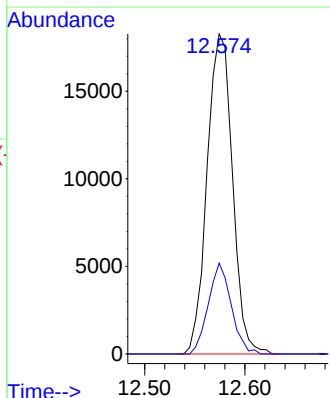
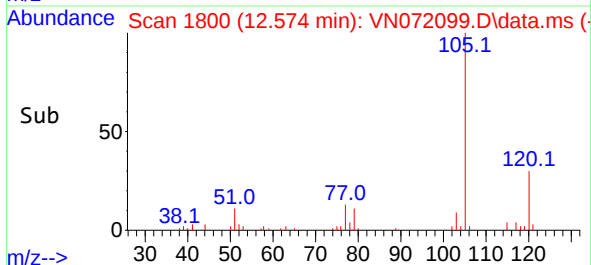
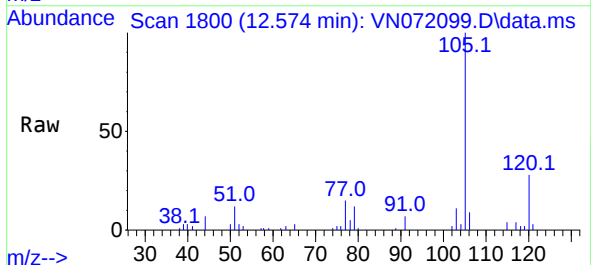


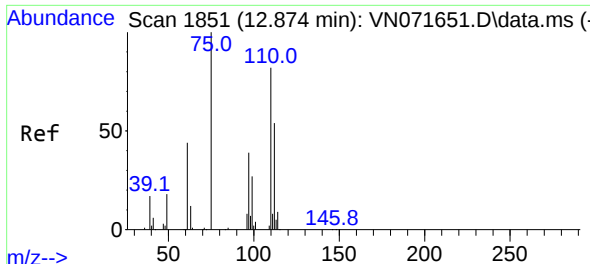

#76
1,2,3-Trichloropropane
Concen: 23.465 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 236938
Ion Ratio Lower Upper
75 100
77 1.2 98.5 295.5#

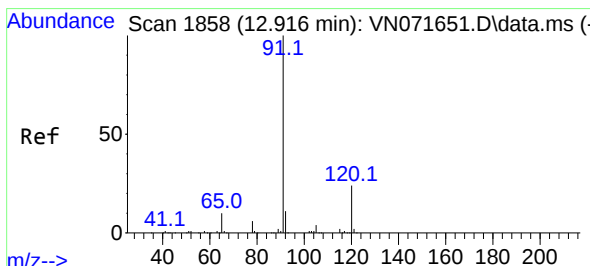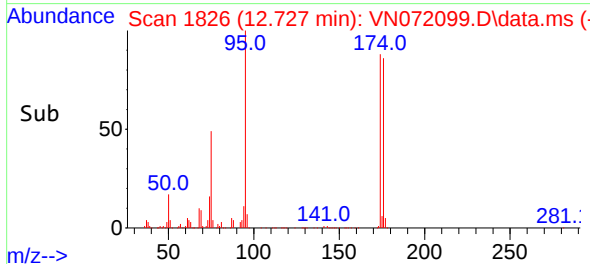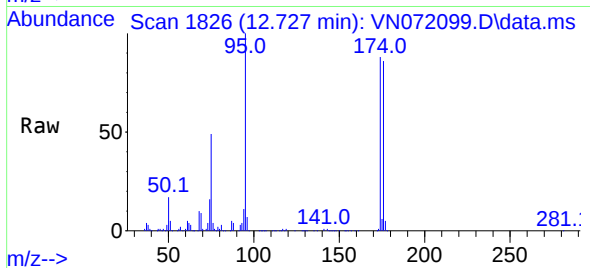

#78
n-propylbenzene
Concen: 1.317 ug/l
RT: 12.915 min Scan# 1858
Delta R.T. -0.001 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41

Tgt Ion: 91 Resp: 50880
Ion Ratio Lower Upper
91 100
120 24.2 11.9 35.5


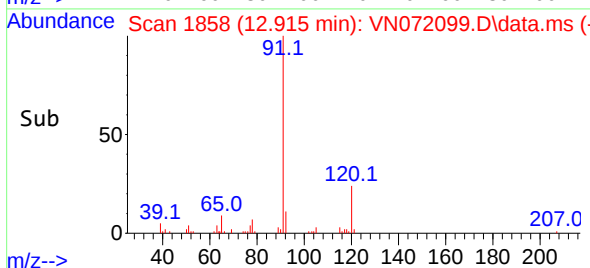

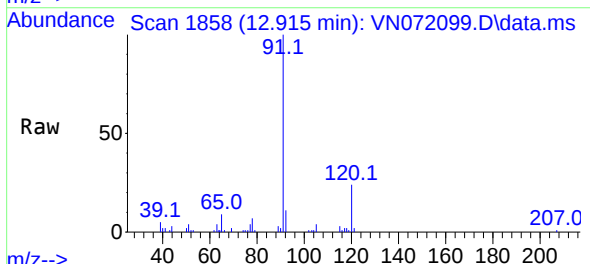




#79
2-Chlorotoluene
Concen: 2.053 ug/l
RT: 12.915 min Scan# 11
Delta R.T. -0.089 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 50880
Ion Ratio Lower Upper
91 100
126 0.0 17.3 51.9#

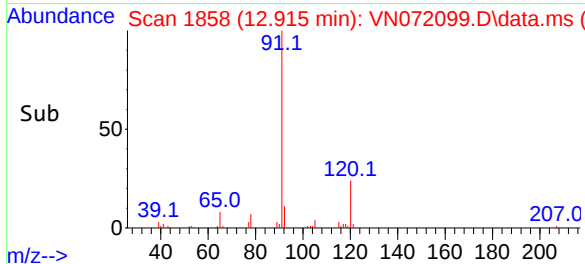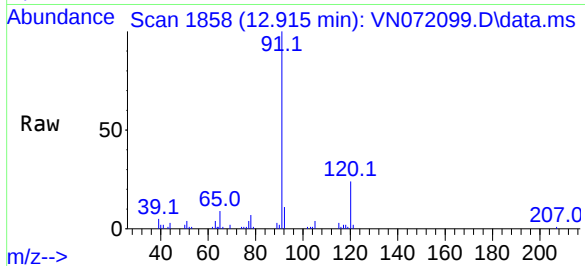

#81
trans-1,4-Dichloro-2-butene
Concen: 72.717 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.105 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41

Tgt Ion: 75 Resp: 236938
Ion Ratio Lower Upper
75 100
53 0.1 78.0 117.0#
89 0.0 37.2 55.8#


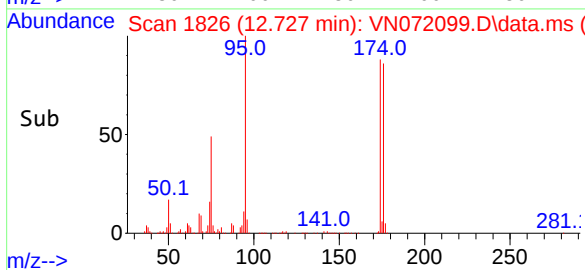

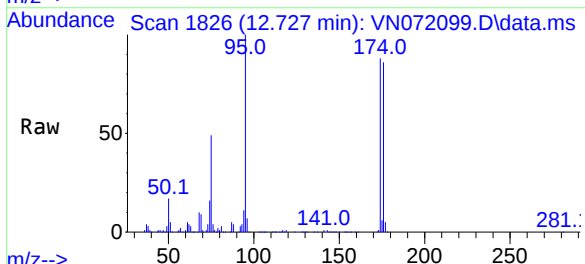




#82
4-Chlorotoluene
Concen: 2.215 ug/l
RT: 12.915 min Scan# 11
Delta R.T. -0.183 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 50880
Ion Ratio Lower Upper
91 100
126 0.0 17.2 51.6#



#90
Hexachloroethane
Concen: 0.446 ug/l
RT: 14.215 min Scan# 2079
Delta R.T. 0.011 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41


Tgt Ion: 117 Resp: 2247
Ion Ratio Lower Upper
117 100
201 0.0 40.6 122.0#

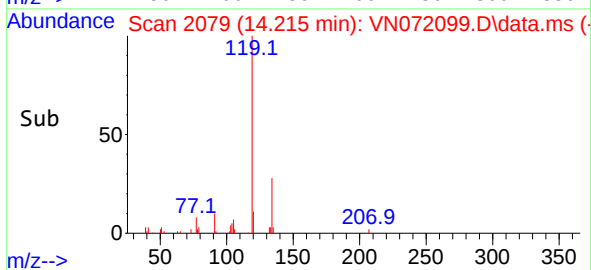






#93
1,2,4-Trichlorobenzene
Concen: 2.324 ug/l
RT: 15.257 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:180 Resp: 1721
Ion Ratio Lower Upper
180 100
182 99.4 47.5 142.5
145 24.4 14.5 43.5

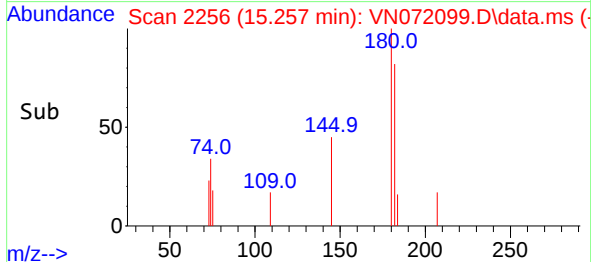

#95
Naphthalene
Concen: 4.819 ug/l
RT: 15.498 min Scan# 2297
Delta R.T. -0.000 min
Lab File: VN072099.D
Acq: 21 Apr 2022 00:41


Tgt Ion:128 Resp: 21820
Ion Ratio Lower Upper
128 100
127 12.8 10.3 15.5
129 11.2 8.6 13.0

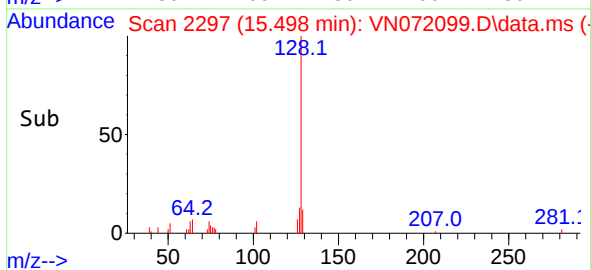



#96
 1,2,3-Trichlorobenzene
 Concen: 2.706 ug/l
 RT: 15.692 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN072099.D
 Acq: 21 Apr 2022 00:41

Instrument :
 MSVOA_N
 ClientSampleId :



Tgt Ion:	180	Resp:	2058
Ion	Ratio	Lower	Upper
180	100		
182	93.5	47.8	143.3
145	16.0	15.5	46.5

