

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042022\
 Data File : VN072101.D
 Acq On : 21 Apr 2022 01:29
 Operator : JC\MD
 Sample : N2482-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 COP-1R

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Title : SW846 8260

Signal : TIC: VN072101.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.257	38	46	62	rVB4	33688	126340	3.84%	0.641%
2	2.434	73	76	86	rVB3	17810	34205	1.04%	0.173%
3	3.128	186	194	205	rVB	46198	108788	3.30%	0.552%
4	4.287	382	391	408	rBV	41278	129744	3.94%	0.658%
5	4.581	425	441	453	rBV	44203	153562	4.66%	0.779%
6	7.145	871	877	886	rVB	13068	35981	1.09%	0.182%
7	7.410	915	922	936	rVB	38900	98364	2.99%	0.499%
8	8.022	1016	1026	1031	rBV	386605	964576	29.29%	4.890%
9	8.081	1031	1036	1050	rVB	736027	1653977	50.22%	8.386%
10	8.434	1086	1096	1112	rBV	400466	961618	29.20%	4.875%
11	8.963	1177	1186	1199	rBV	1109157	2245577	68.19%	11.385%
12	10.439	1428	1437	1443	rBV	1798311	3293169	100.00%	16.696%
13	10.504	1443	1448	1458	rVB	309727	578833	17.58%	2.935%
14	11.739	1650	1658	1670	rBV	1807426	3191466	96.91%	16.181%
15	11.839	1670	1675	1684	rVV	71814	124183	3.77%	0.630%
16	11.945	1686	1693	1710	rVB	254555	489045	14.85%	2.479%
17	12.274	1743	1749	1758	rBV	233155	391759	11.90%	1.986%
18	12.727	1818	1826	1837	rBV	1362007	2298721	69.80%	11.655%
19	12.980	1863	1869	1872	rBV	39390	70271	2.13%	0.356%
20	13.051	1877	1881	1888	rVB	51009	85326	2.59%	0.433%
21	13.216	1902	1909	1918	rBV2	29885	48136	1.46%	0.244%
22	13.363	1928	1934	1940	rBV	53731	86469	2.63%	0.438%
23	13.668	1979	1986	1998	rBV	1390382	2463956	74.82%	12.492%
24	13.763	1998	2002	2009	rVB	27829	48596	1.48%	0.246%
25	13.868	2016	2020	2031	rVB4	19776	41121	1.25%	0.208%


Sum of corrected areas: 19723783

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042022\
Data File : VN072101.D
Acq On : 21 Apr 2022 01:29
Operator : JC\MD
Sample : N2482-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
COP-1R

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

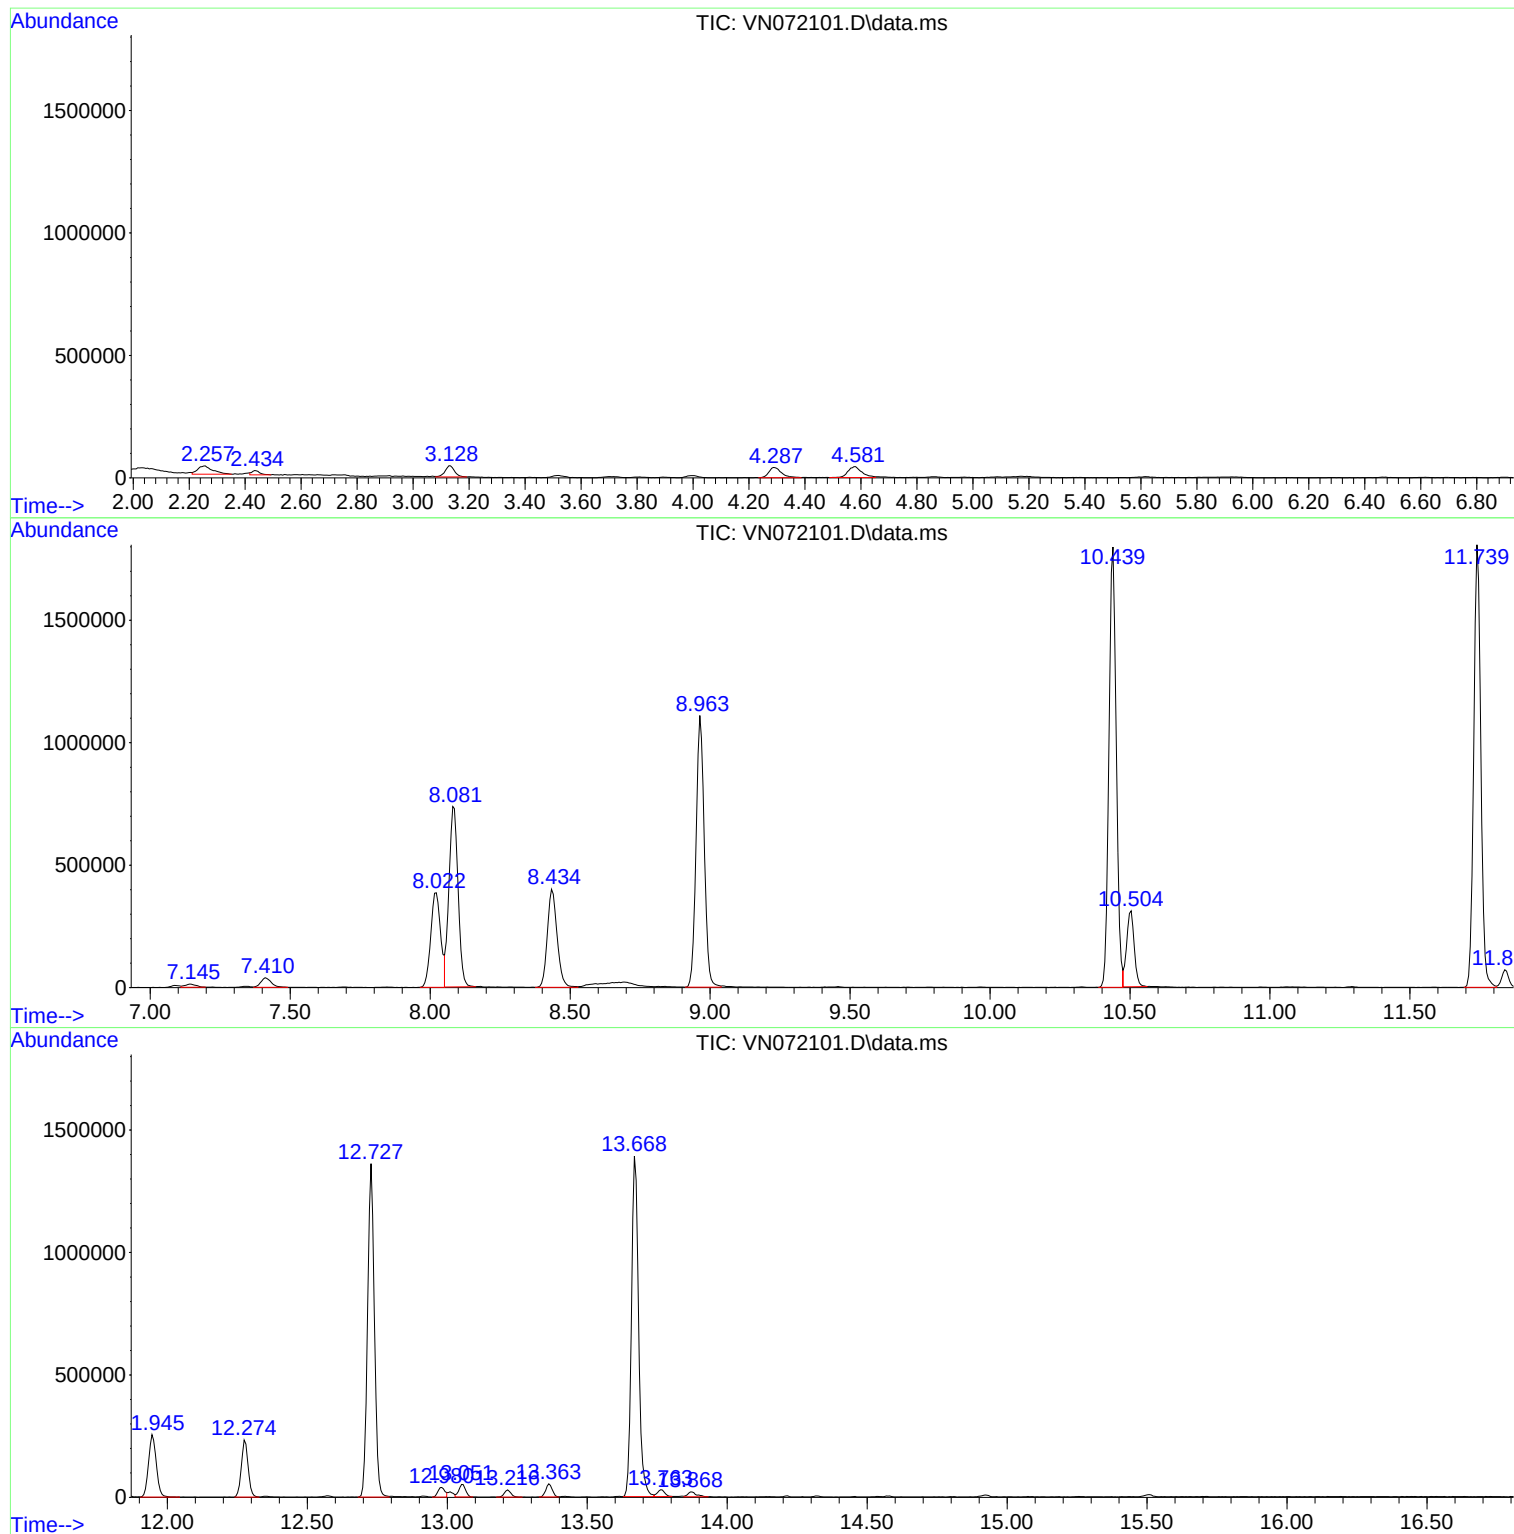

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042022\
Data File : VN072101.D
Acq On : 21 Apr 2022 01:29
Operator : JC\MD
Sample : N2482-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
COP-1R

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042022\
Data File : VN072101.D
Acq On : 21 Apr 2022 01:29
Operator : JC\MD
Sample : N2482-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
COP-1R

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc