

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042023\
 Data File : VN077391.D
 Acq On : 20 Apr 2023 11:20
 Operator : JC\MD
 Sample : VN0420WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0420WBL01

Quant Time: Apr 21 02:54:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N040523W.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 06 08:27:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.231	168	588712	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.107	114	1092776	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.866	117	946850	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.795	152	338042	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	358199	44.518	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	89.040%
35) Dibromofluoromethane	8.166	113	327385	46.799	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	93.600%
50) Toluene-d8	10.572	98	1301411	46.212	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	92.420%
62) 4-Bromofluorobenzene	12.854	95	413582	44.156	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	88.320%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042023\
Data File : VN077391.D
Acq On : 20 Apr 2023 11:20
Operator : JC\MD
Sample : VN0420WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0420WBL01

Quant Time: Apr 21 02:54:51 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N040523W.M
Quant Title : SW846 8260
QLast Update : Thu Apr 06 08:27:03 2023
Response via : Initial Calibration




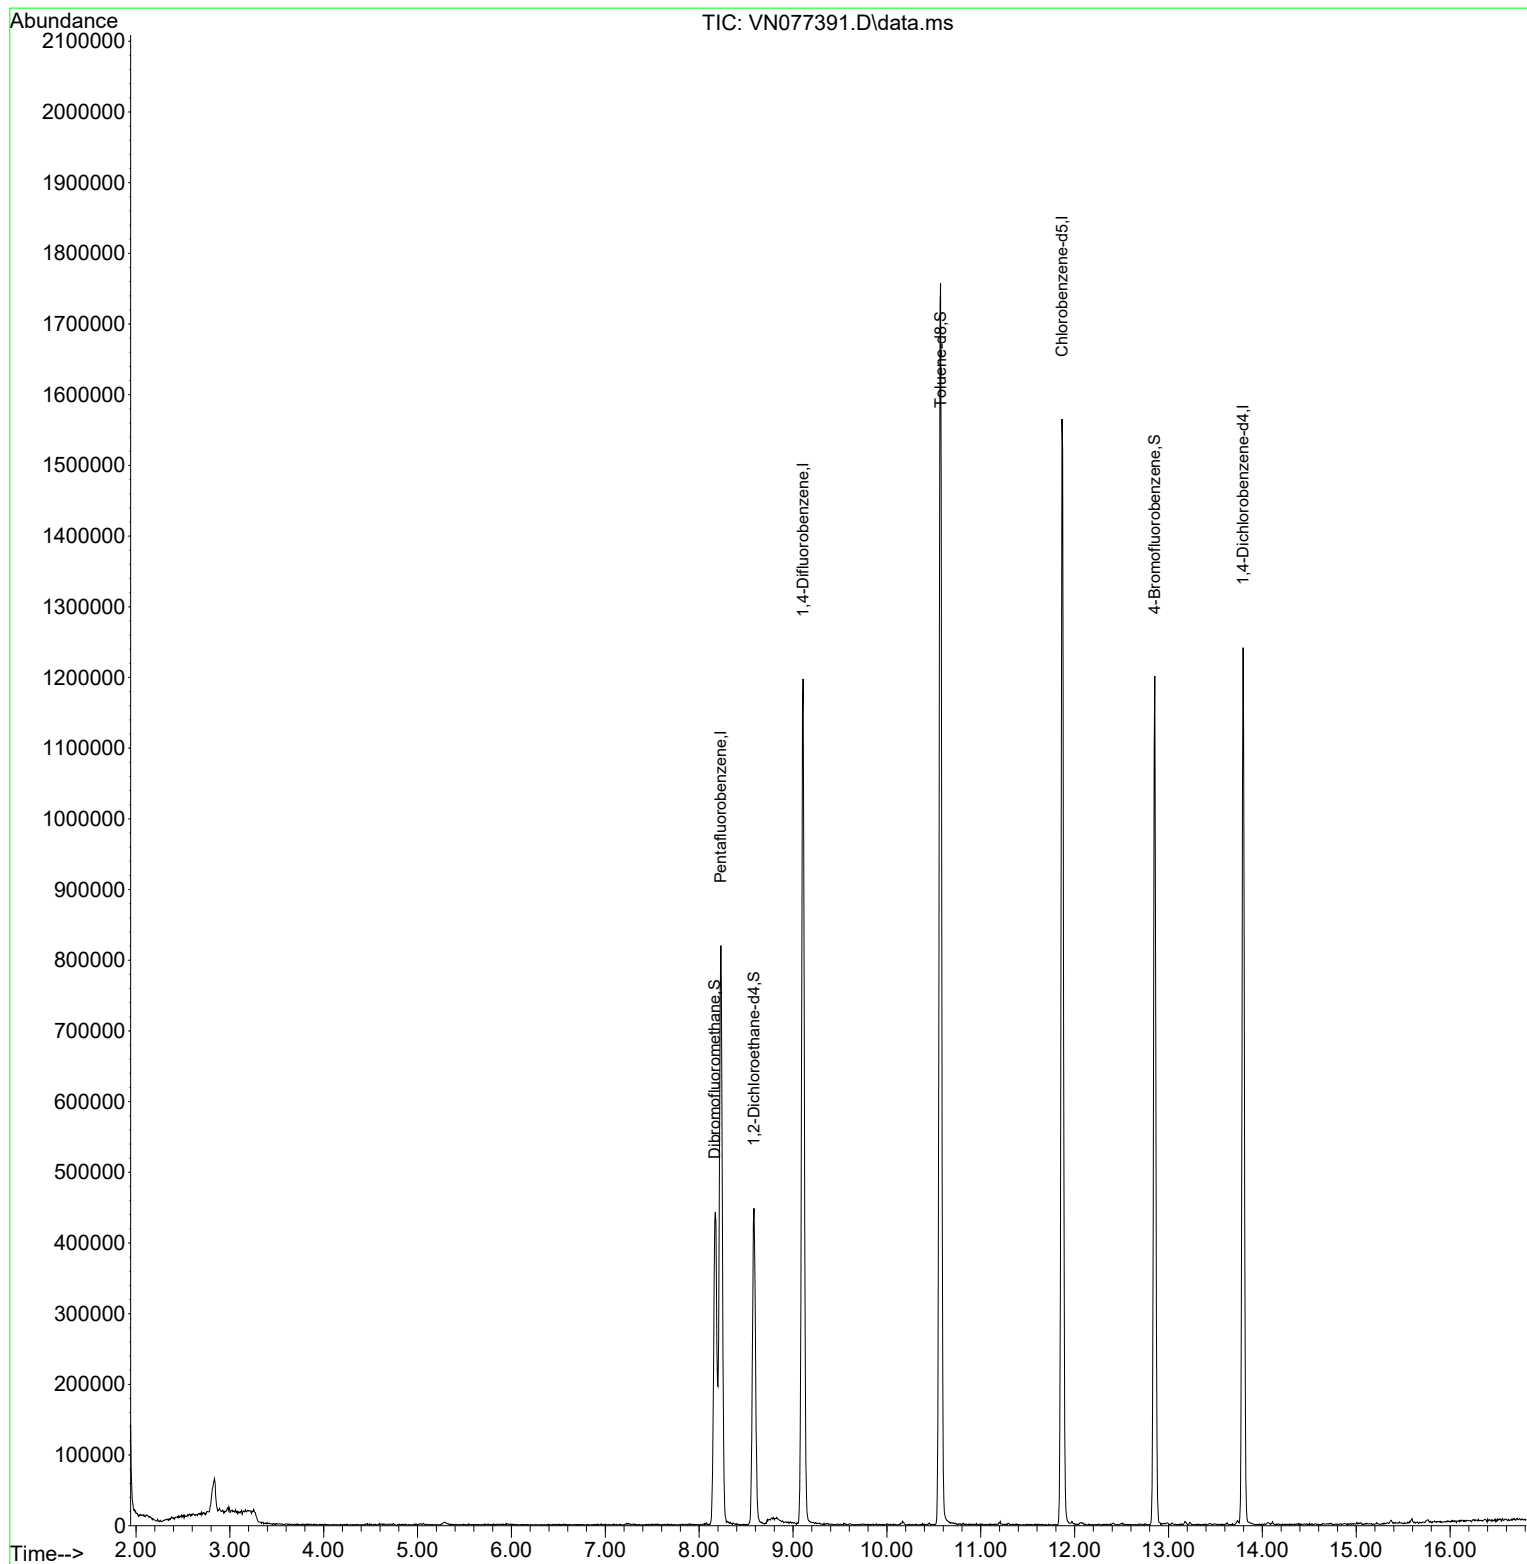


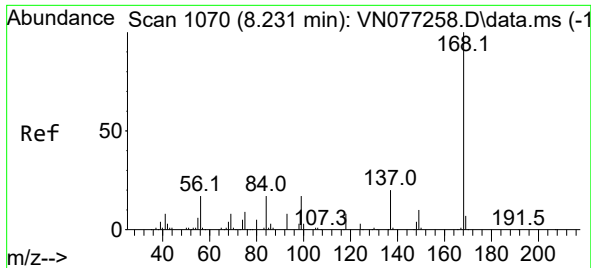

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.231 min Scan# 110
Delta R.T. -0.000 min
Lab File: VN077391.D
Acq: 20 Apr 2023 11:20




Instrument :
MSVOA_N
ClientSampleId :
VN0420WBL01


Tgt Ion:168 Resp: 588712
Ion Ratio Lower Upper
168 100
99 63.5 50.6 75.8

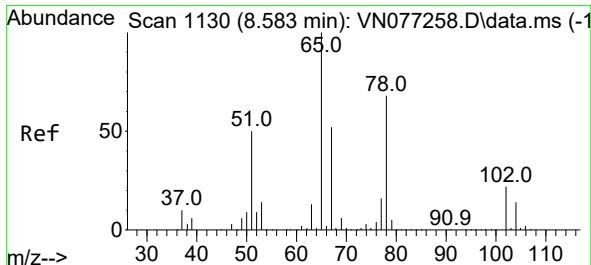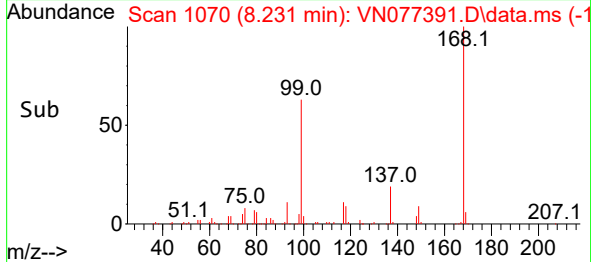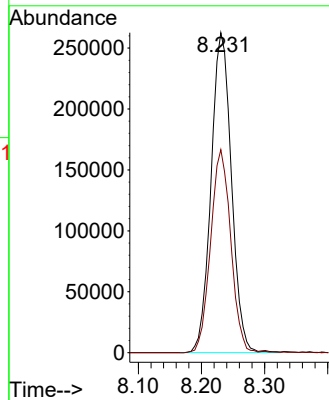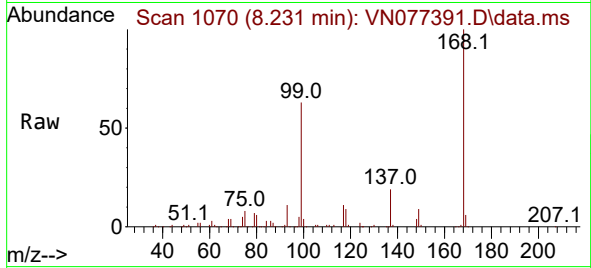

#33
1,2-Dichloroethane-d4
Concen: 44.518 ug/l
RT: 8.583 min Scan# 1130
Delta R.T. 0.000 min
Lab File: VN077391.D
Acq: 20 Apr 2023 11:20

Tgt Ion: 65 Resp: 358199
Ion Ratio Lower Upper
65 100
67 52.3 0.0 108.8

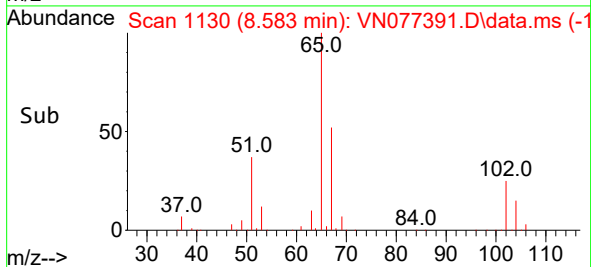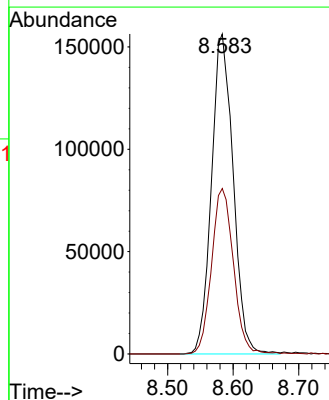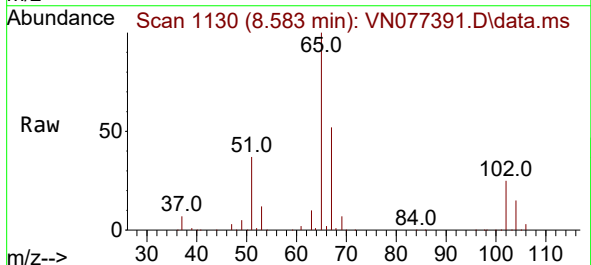

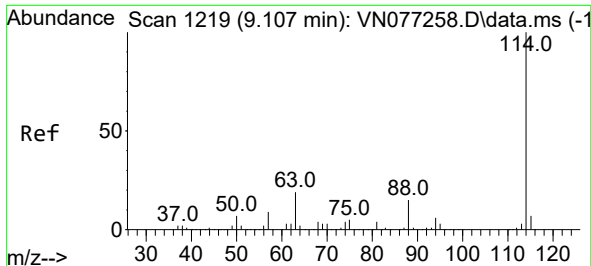

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.107 min Scan# 11

Delta R.T. -0.000 min

Lab File: VN077391.D

Acq: 20 Apr 2023 11:20

Instrument :

MSVOA_N

ClientSampleId :

VN0420WBL01





Tgt Ion:114 Resp: 1092776

Ion Ratio Lower Upper

114 100

63 18.1 0.0 37.8

88 15.3 0.0 29.4

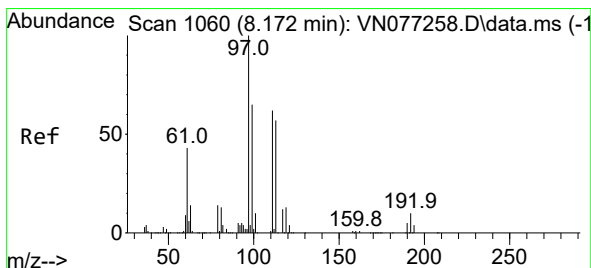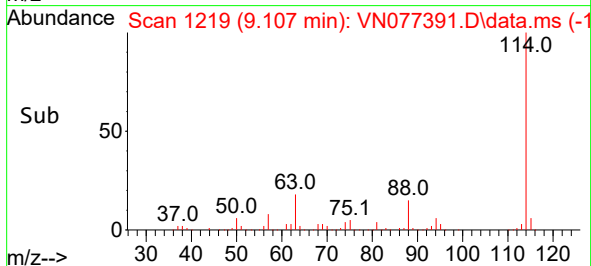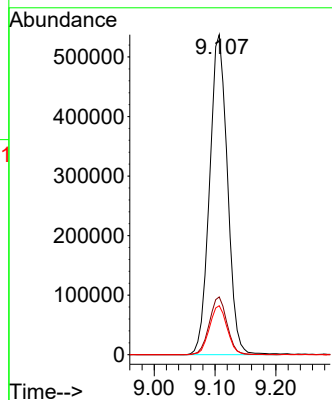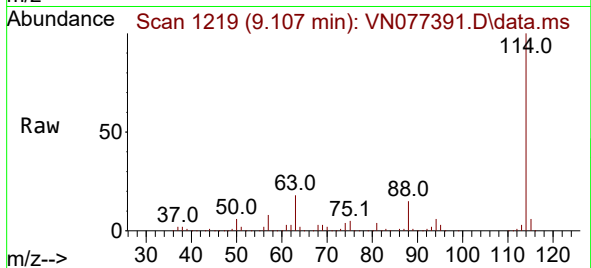

#35

Dibromofluoromethane

Concen: 46.799 ug/l

RT: 8.166 min Scan# 1059

Delta R.T. -0.006 min

Lab File: VN077391.D

Acq: 20 Apr 2023 11:20




Tgt Ion:113 Resp: 327385


Ion Ratio Lower Upper

113 100

111 101.9 83.4 125.0

192 16.0 13.5 20.3


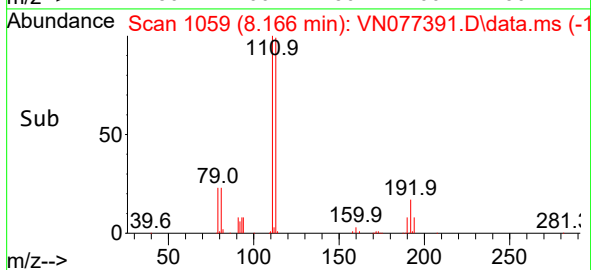
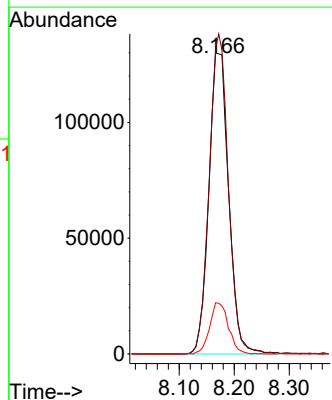
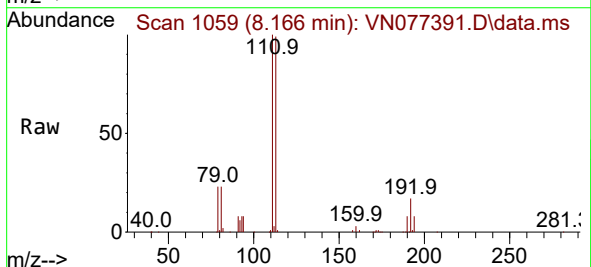


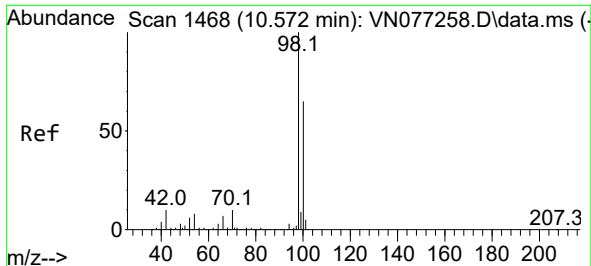

#50
Toluene-d8
Concen: 46.212 ug/l
RT: 10.572 min Scan# 1468
Delta R.T. -0.000 min
Lab File: VN077391.D
Acq: 20 Apr 2023 11:20




Instrument :
MSVOA_N
ClientSampleId :
VN0420WBL01


Tgt Ion: 98 Resp: 1301411
Ion Ratio Lower Upper
98 100
100 65.3 51.3 76.9

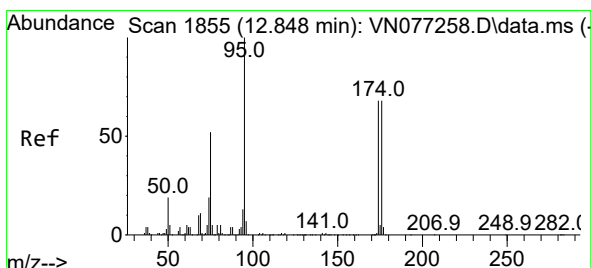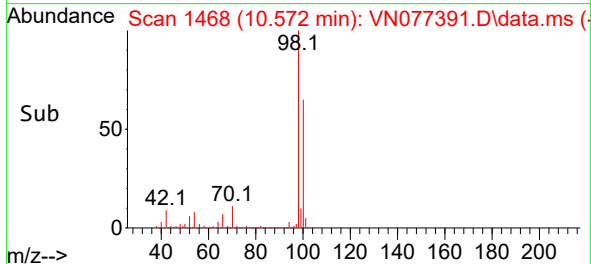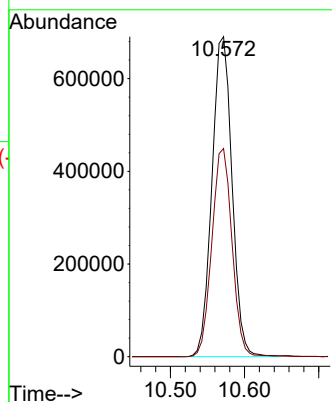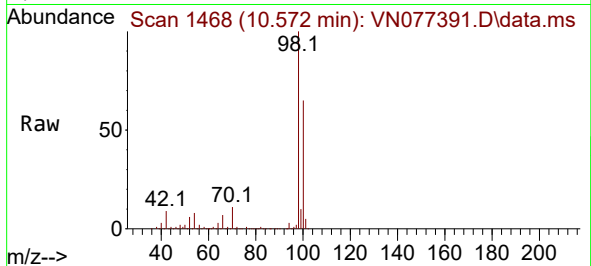

#62
4-Bromofluorobenzene
Concen: 44.156 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. 0.006 min
Lab File: VN077391.D
Acq: 20 Apr 2023 11:20

Tgt Ion: 95 Resp: 413582
Ion Ratio Lower Upper
95 100
174 73.0 0.0 146.8
176 70.1 0.0 139.6


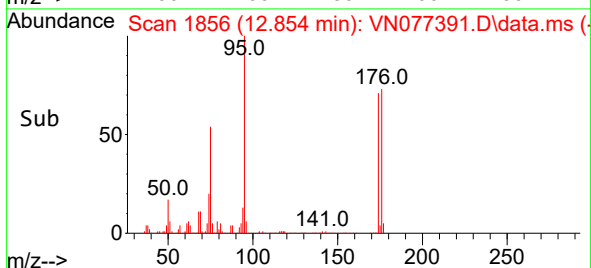
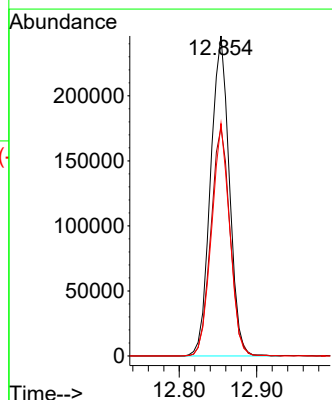
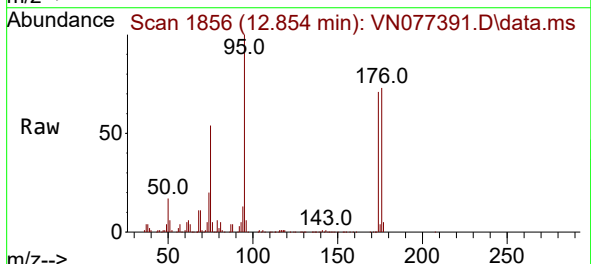


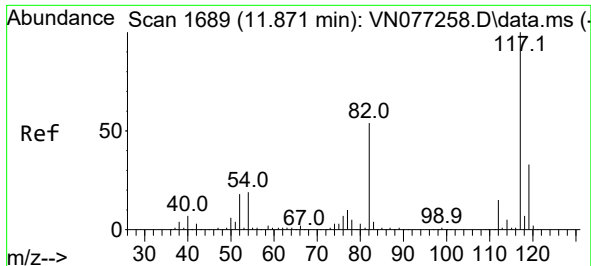

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.866 min Scan# 11
Delta R.T. -0.005 min
Lab File: VN077391.D
Acq: 20 Apr 2023 11:20

Instrument :
MSVOA_N
ClientSampleId :
VN0420WBL01

Tgt Ion:117 Resp: 946850
Ion Ratio Lower Upper
117 100
82 56.9 42.9 64.3
119 32.5 26.2 39.4

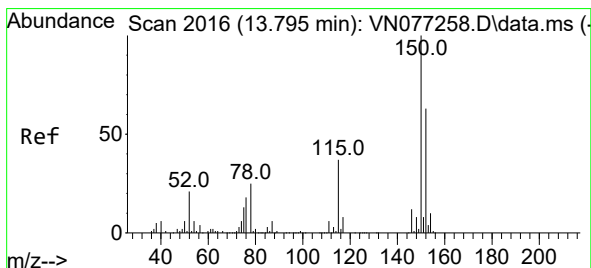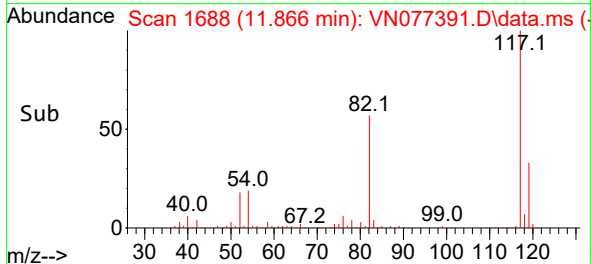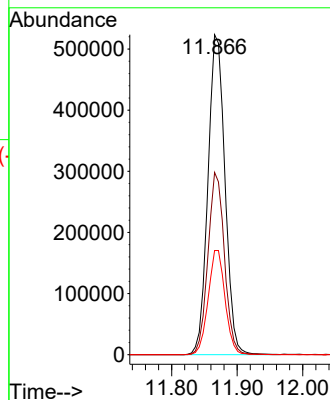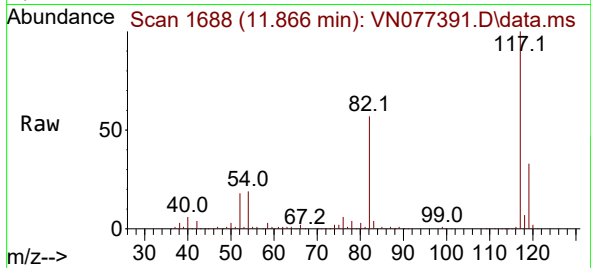

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.795 min Scan# 2016
Delta R.T. -0.000 min
Lab File: VN077391.D
Acq: 20 Apr 2023 11:20

Tgt Ion:152 Resp: 338042
Ion Ratio Lower Upper
152 100
115 63.9 32.1 96.3
150 157.3 0.0 354.8

