


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042121\
Data File : VN066689.D
Acq On : 21 Apr 2021 9:29
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042121W.M
Title : SW846 8260
Last Update : Thu Apr 22 08:25:55 2021

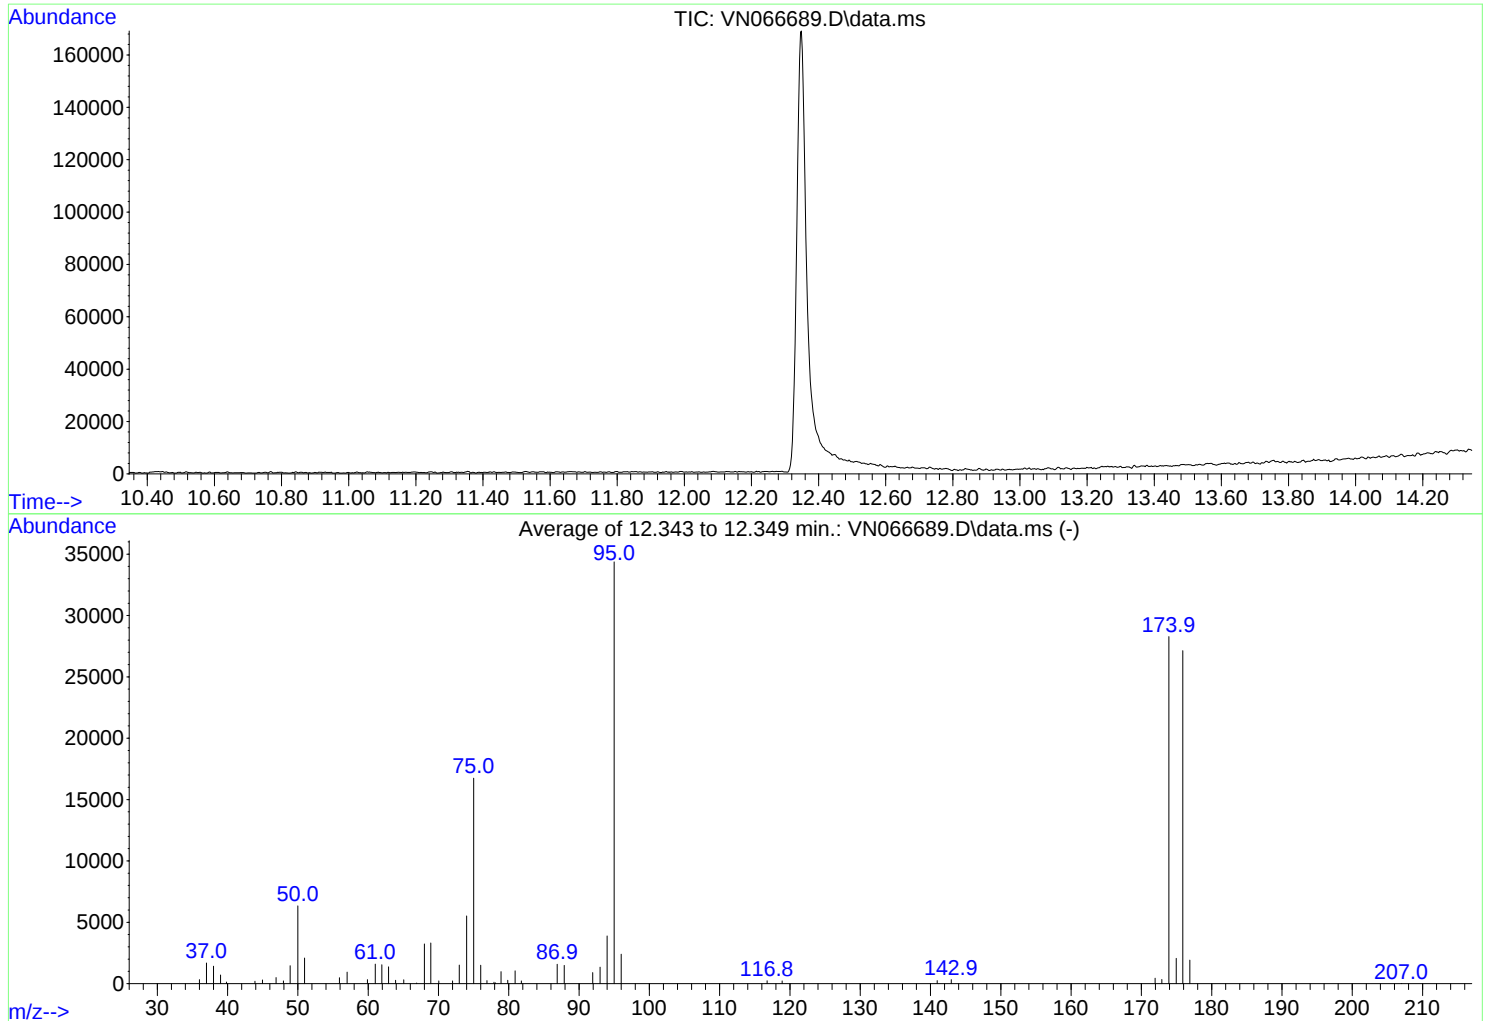

AutoFind: Scans 3960, 3961, 3962; Background Corrected with Scan 3945

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	6334	PASS
75	95	30	60	48.7	16743	PASS
95	95	100	100	100.0	34373	PASS
96	95	5	9	7.0	2406	PASS
173	174	0.00	2	1.2	334	PASS
174	95	50	100	82.3	28280	PASS
175	174	5	9	7.3	2060	PASS
176	174	95	101	96.0	27136	PASS
177	176	5	9	7.1	1915	PASS