

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042123\
 Data File : VN077420.D
 Acq On : 21 Apr 2023 11:44
 Operator : JC\MD
 Sample : VN0421WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0421WBL01

Quant Time: Apr 22 02:39:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N040723W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri Apr 07 13:04:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.819	128	60090	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.107	114	437709	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.866	117	440938	30.000	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.583	65	150271	29.486	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	98.300%
60) 4-Bromofluorobenzene	12.854	95	199076	26.110	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	87.033%
63) Toluene-d8	10.572	98	464999	29.998	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	100.000%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042123\
Data File : VN077420.D
Acq On : 21 Apr 2023 11:44
Operator : JC\MD
Sample : VN0421WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0421WBL01

Quant Time: Apr 22 02:39:39 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N040723W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri Apr 07 13:04:49 2023
Response via : Initial Calibration




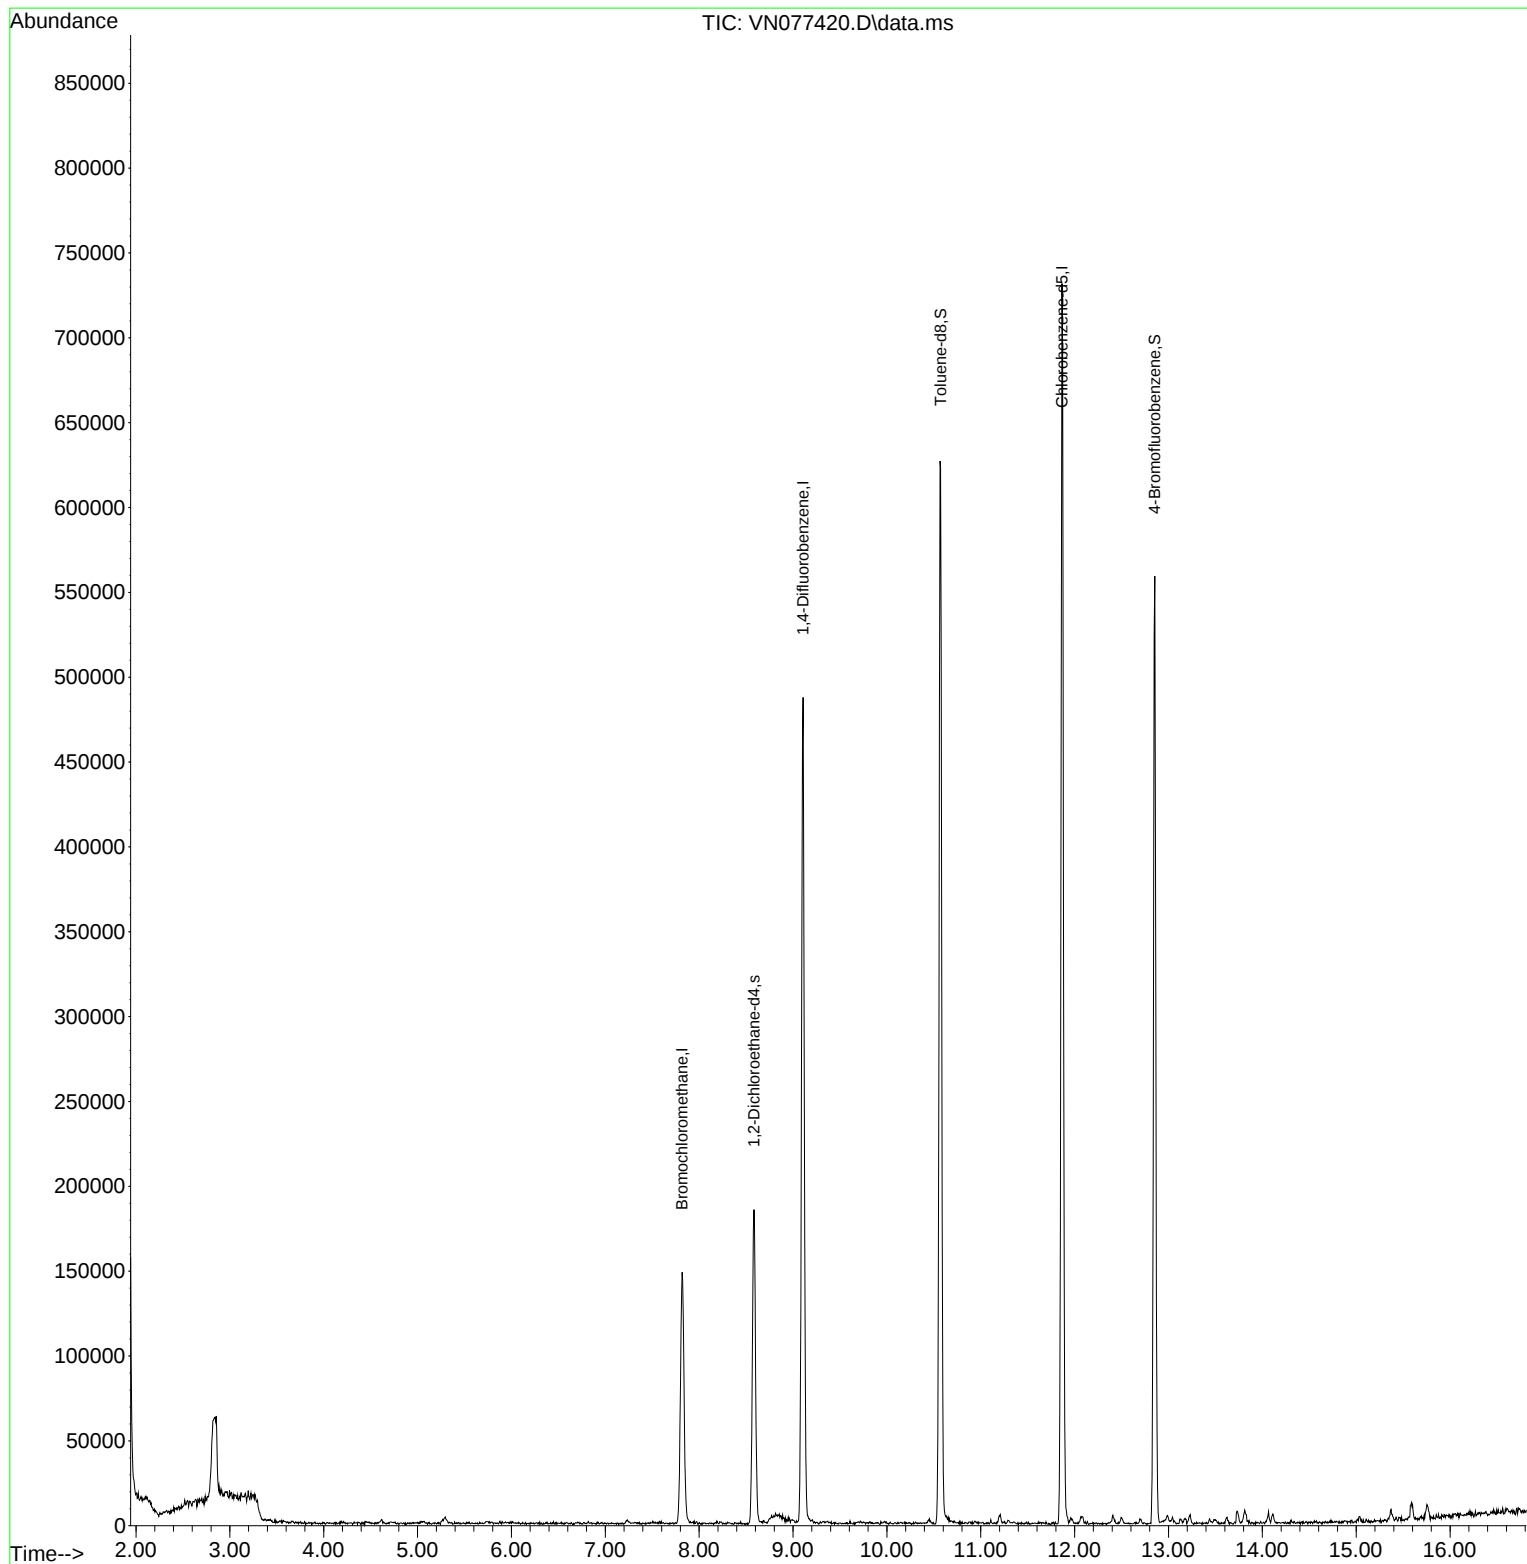


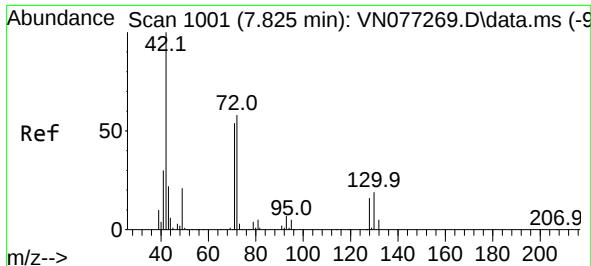

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.819 min Scan# 1000
Delta R.T. -0.006 min
Lab File: VN077420.D
Acq: 21 Apr 2023 11:44




Instrument :
MSVOA_N
ClientSampleId :
VN0421WBL01


Tgt Ion:128 Resp: 60090
Ion Ratio Lower Upper
128 100
49 125.8 0.0 379.5
130 124.6 0.0 322.8

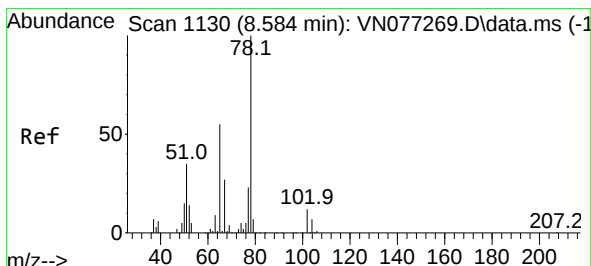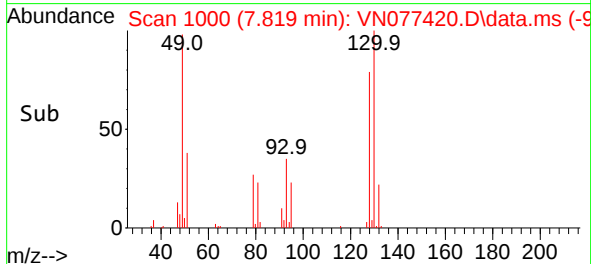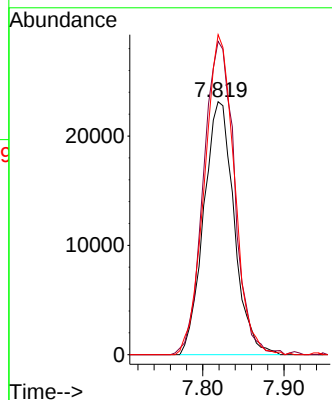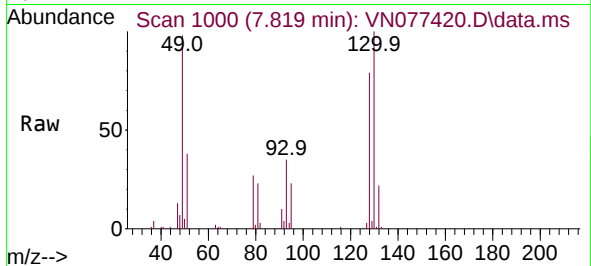

#27
1,2-Dichloroethane-d4
Concen: 29.486 ug/l
RT: 8.583 min Scan# 1130
Delta R.T. -0.001 min
Lab File: VN077420.D
Acq: 21 Apr 2023 11:44

Tgt Ion: 65 Resp: 150271
Ion Ratio Lower Upper
65 100
67 51.5 41.8 62.6


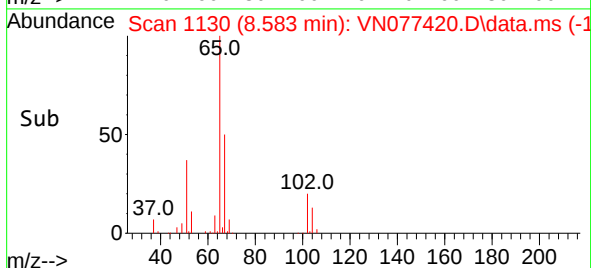
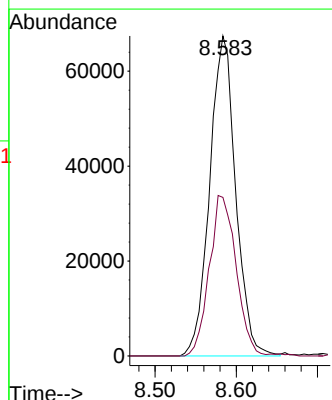
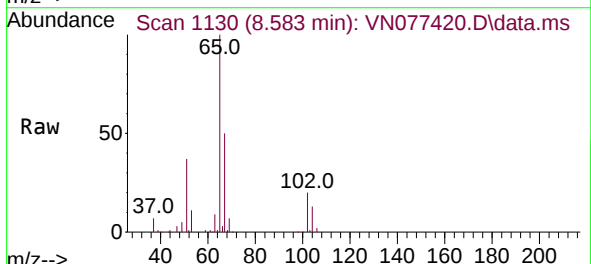


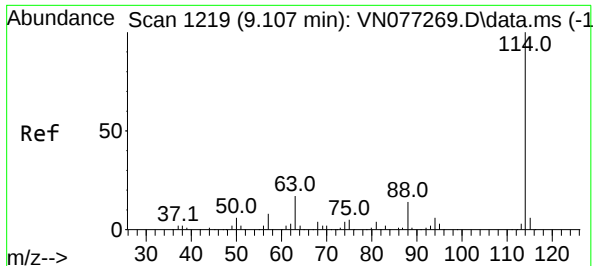

#28
1,4-Difluorobenzene
Concen: 30.000 ug/l
RT: 9.107 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN077420.D
Acq: 21 Apr 2023 11:44




Instrument :
MSVOA_N
ClientSampleId :
VN0421WBL01


Tgt Ion:114 Resp: 437709
Ion Ratio Lower Upper
114 100
63 18.0 15.0 22.4
88 14.9 11.9 17.9

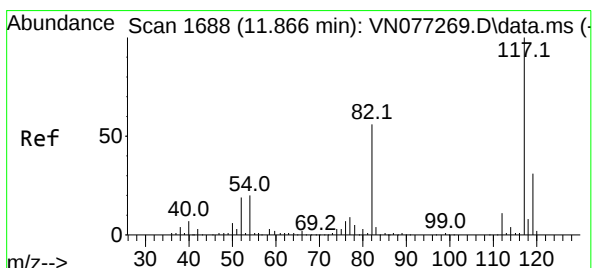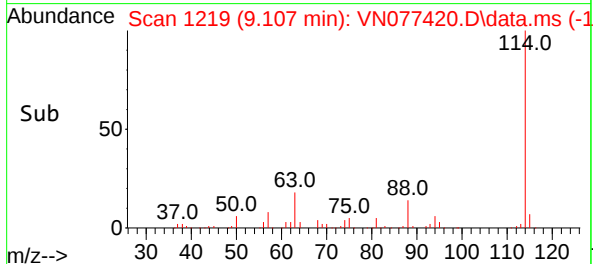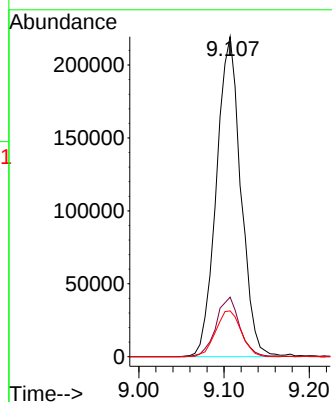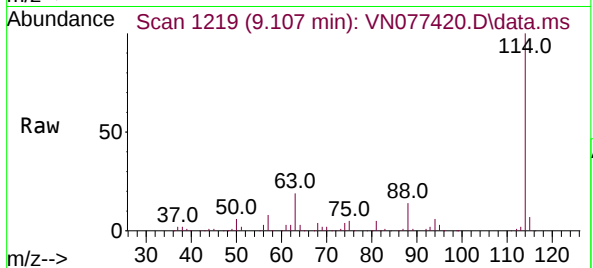

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 11.866 min Scan# 1688
Delta R.T. -0.000 min
Lab File: VN077420.D
Acq: 21 Apr 2023 11:44

Tgt Ion:117 Resp: 440938
Ion Ratio Lower Upper
117 100
82 54.5 43.8 65.8
119 31.7 25.4 38.0


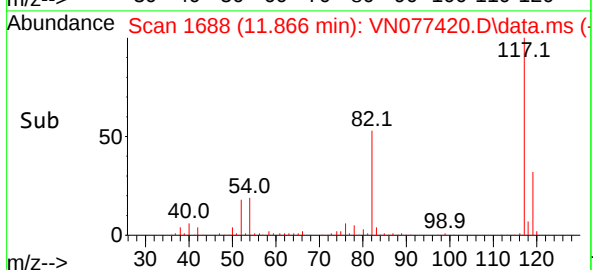
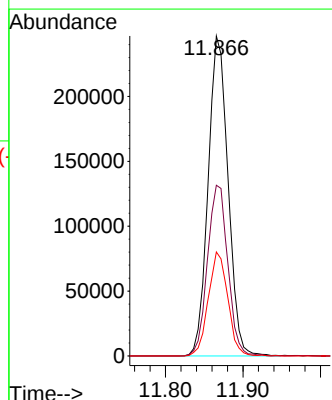
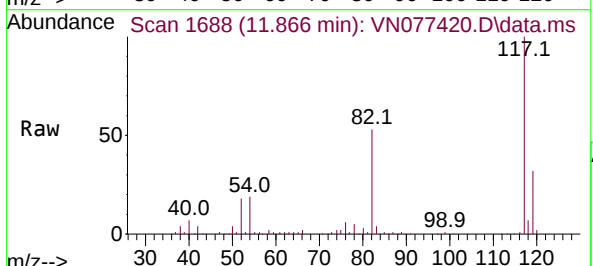


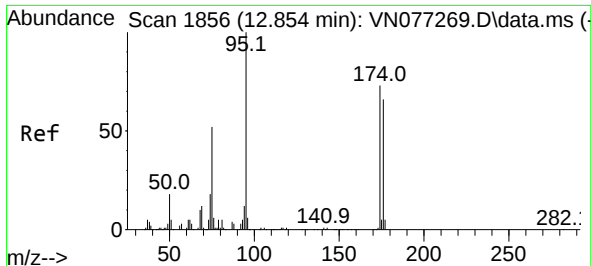

#60
4-Bromofluorobenzene
Concen: 26.110 ug/l
RT: 12.854 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN077420.D
Acq: 21 Apr 2023 11:44

Instrument :
MSVOA_N
ClientSampleId :
VN0421WBL01

Tgt Ion: 95 Resp: 199076
Ion Ratio Lower Upper
95 100
174 72.6 57.8 86.8
176 69.5 54.6 81.8

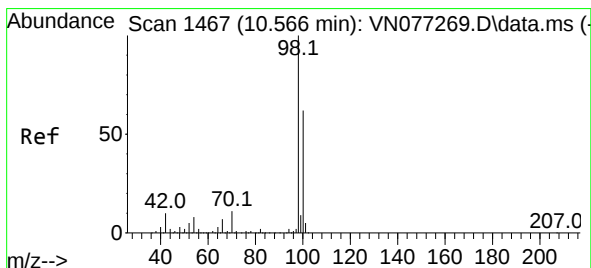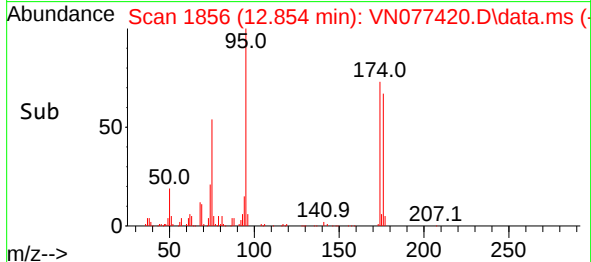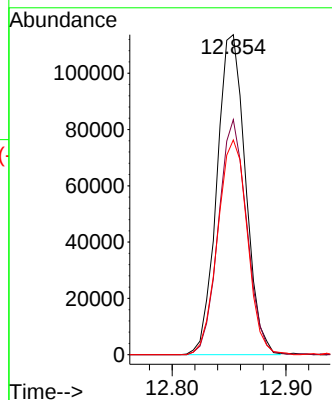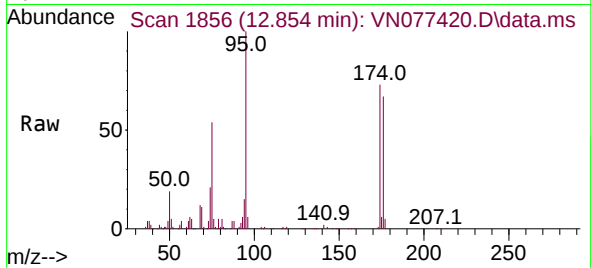

#63
Toluene-d8
Concen: 29.998 ug/l
RT: 10.572 min Scan# 1468
Delta R.T. 0.006 min
Lab File: VN077420.D
Acq: 21 Apr 2023 11:44

Tgt Ion: 98 Resp: 464999
Ion Ratio Lower Upper
98 100
100 65.4 51.4 77.2

