


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042123\
Data File : VN077416.D
Acq On : 21 Apr 2023 08:27
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N040723W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Apr 07 13:04:49 2023

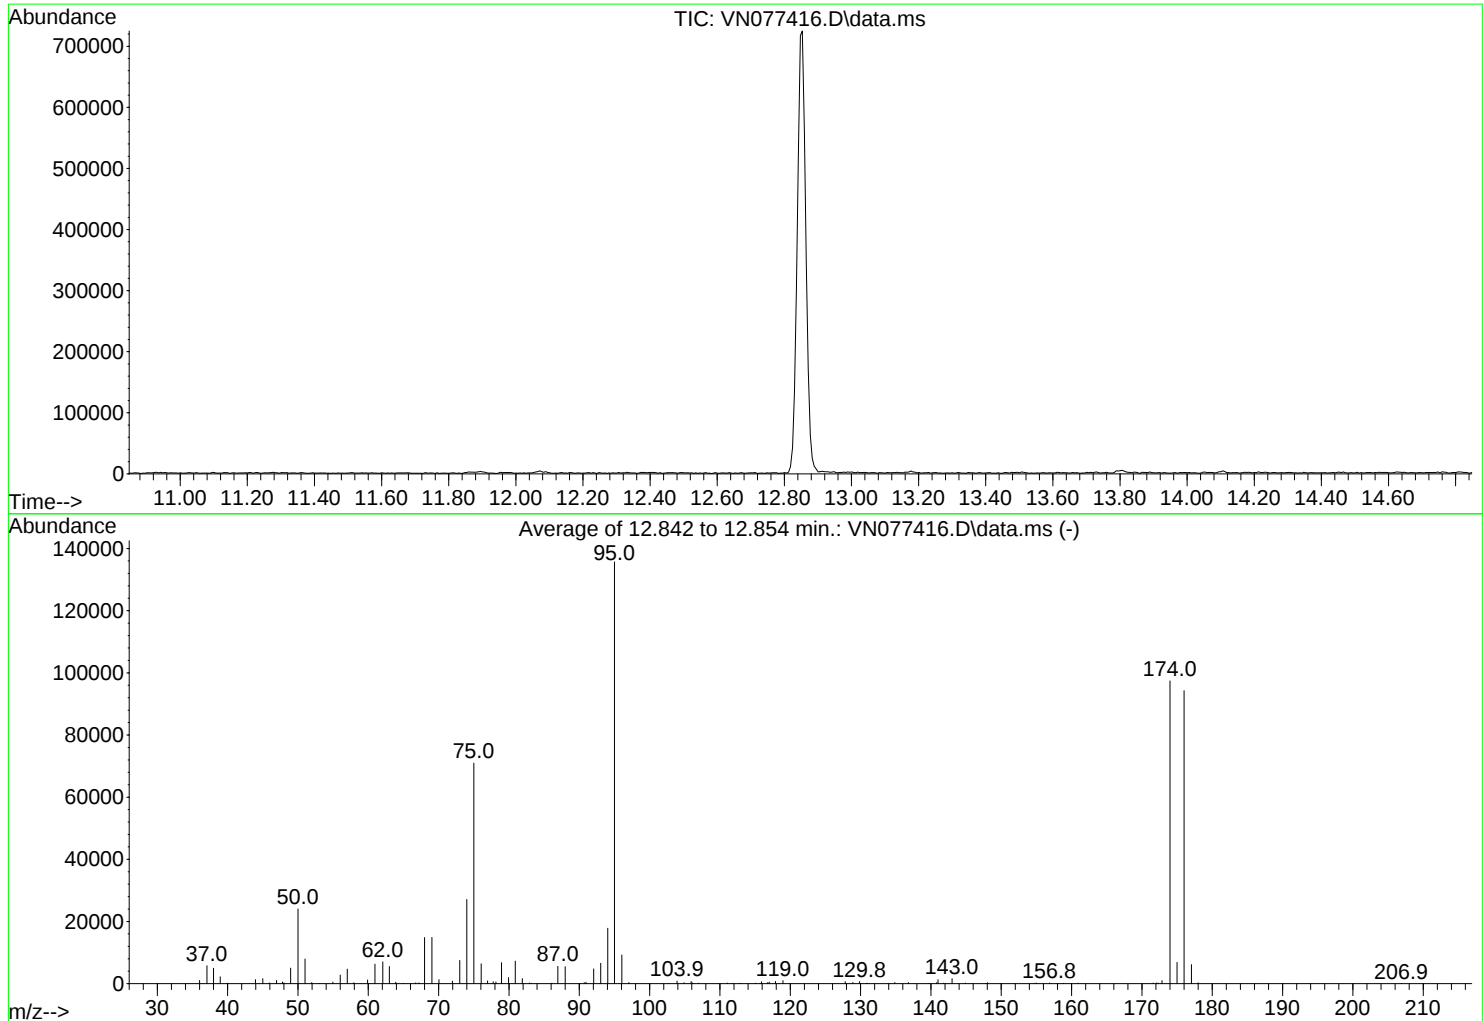

AutoFind: Scans 1854, 1855, 1856; Background Corrected with Scan 1847

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.7	24056	PASS
75	95	30	60	52.3	70947	PASS
95	95	100	100	100.0	135723	PASS
96	95	5	9	6.8	9227	PASS
173	174	0.00	2	1.0	974	PASS
174	95	50	100	71.8	97435	PASS
175	174	5	9	7.0	6834	PASS
176	174	95	101	96.8	94269	PASS
177	176	5	9	6.5	6116	PASS