



2-Chloroethyl Vinyl ether

Response Ratio

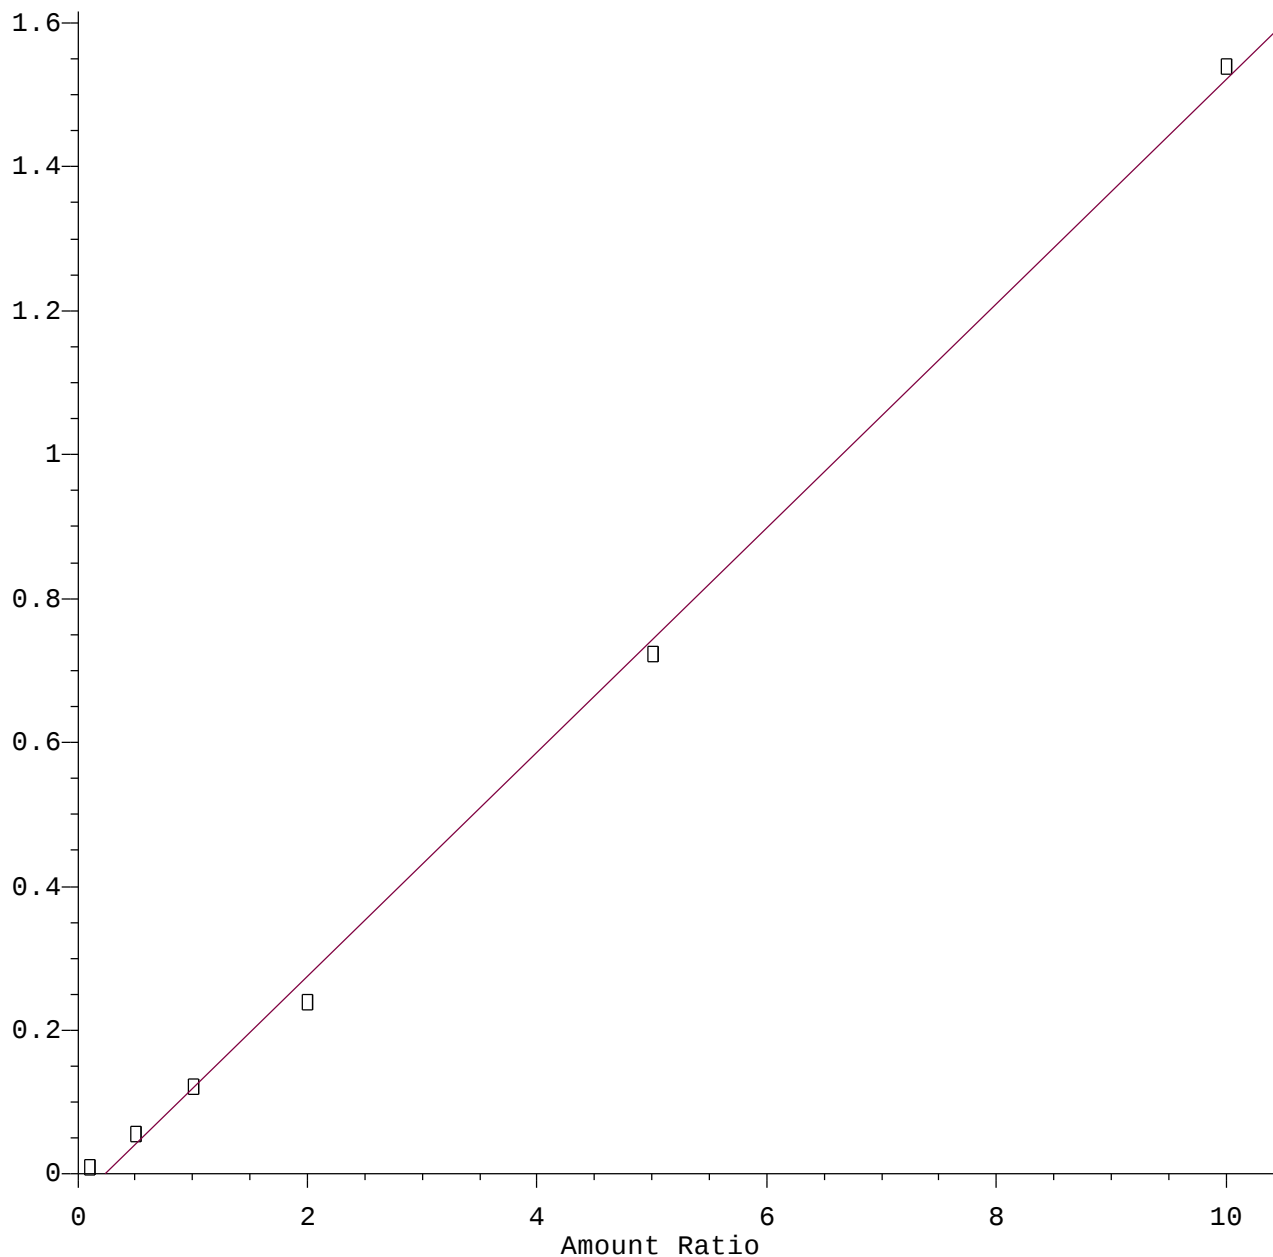

Resp Ratio = $1.56 \times 10^{-1} \times \text{Amt} - 3.51 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042219W.M
Calibration Table Last Updated: Tue Apr 23 05:52:53 2019

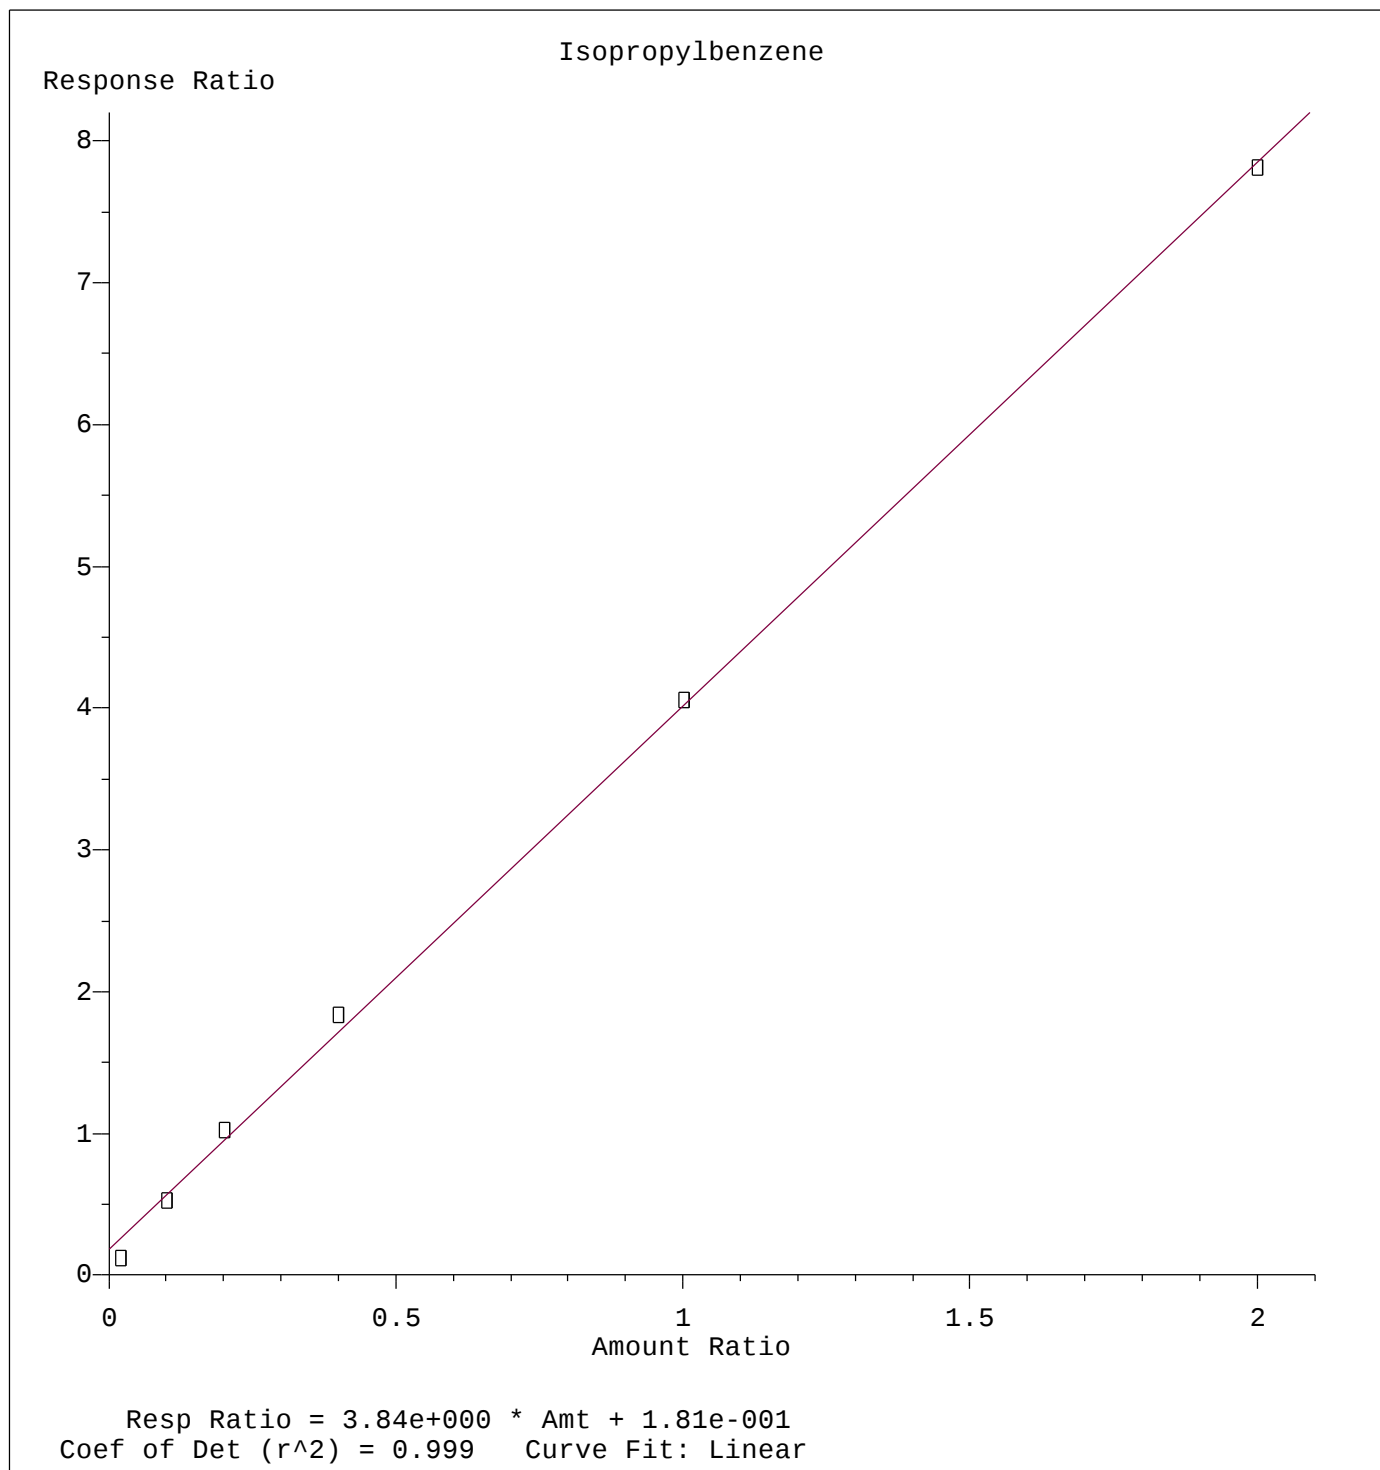

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042219W.M
Calibration Table Last Updated: Tue Apr 23 05:52:53 2019

1,1,2,2-Tetrachloroethane

Response Ratio

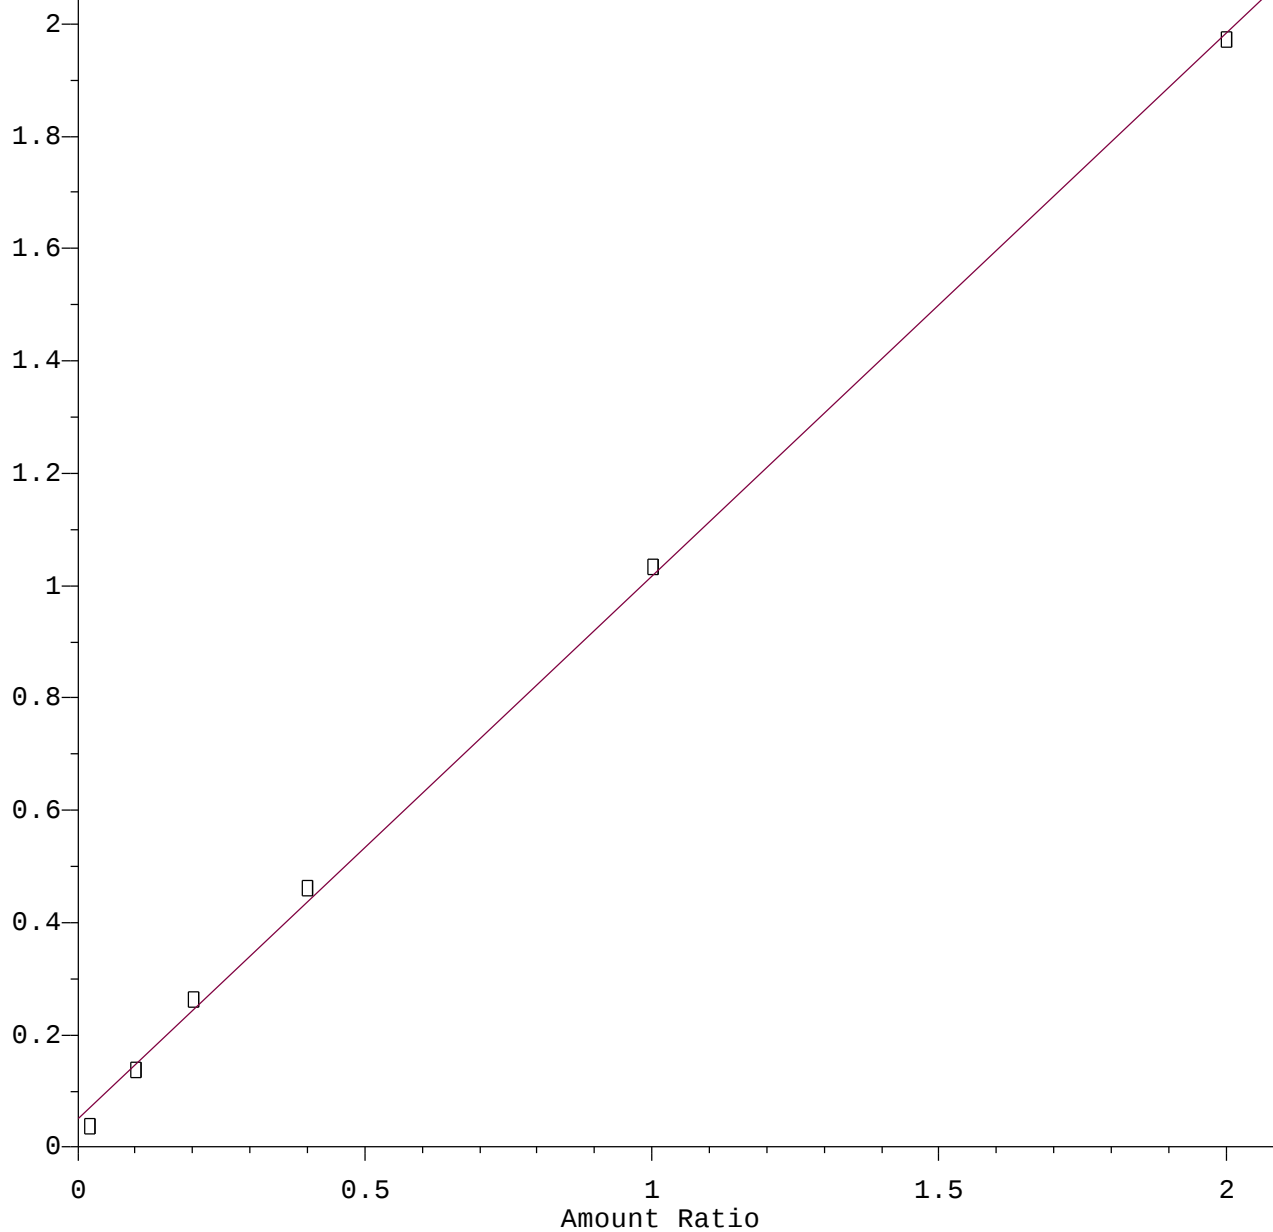


Resp Ratio = $9.67 \times 10^{-1} \times \text{Amt} + 4.97 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042219W.M
Calibration Table Last Updated: Tue Apr 23 05:52:53 2019

tert-Butylbenzene

Response Ratio

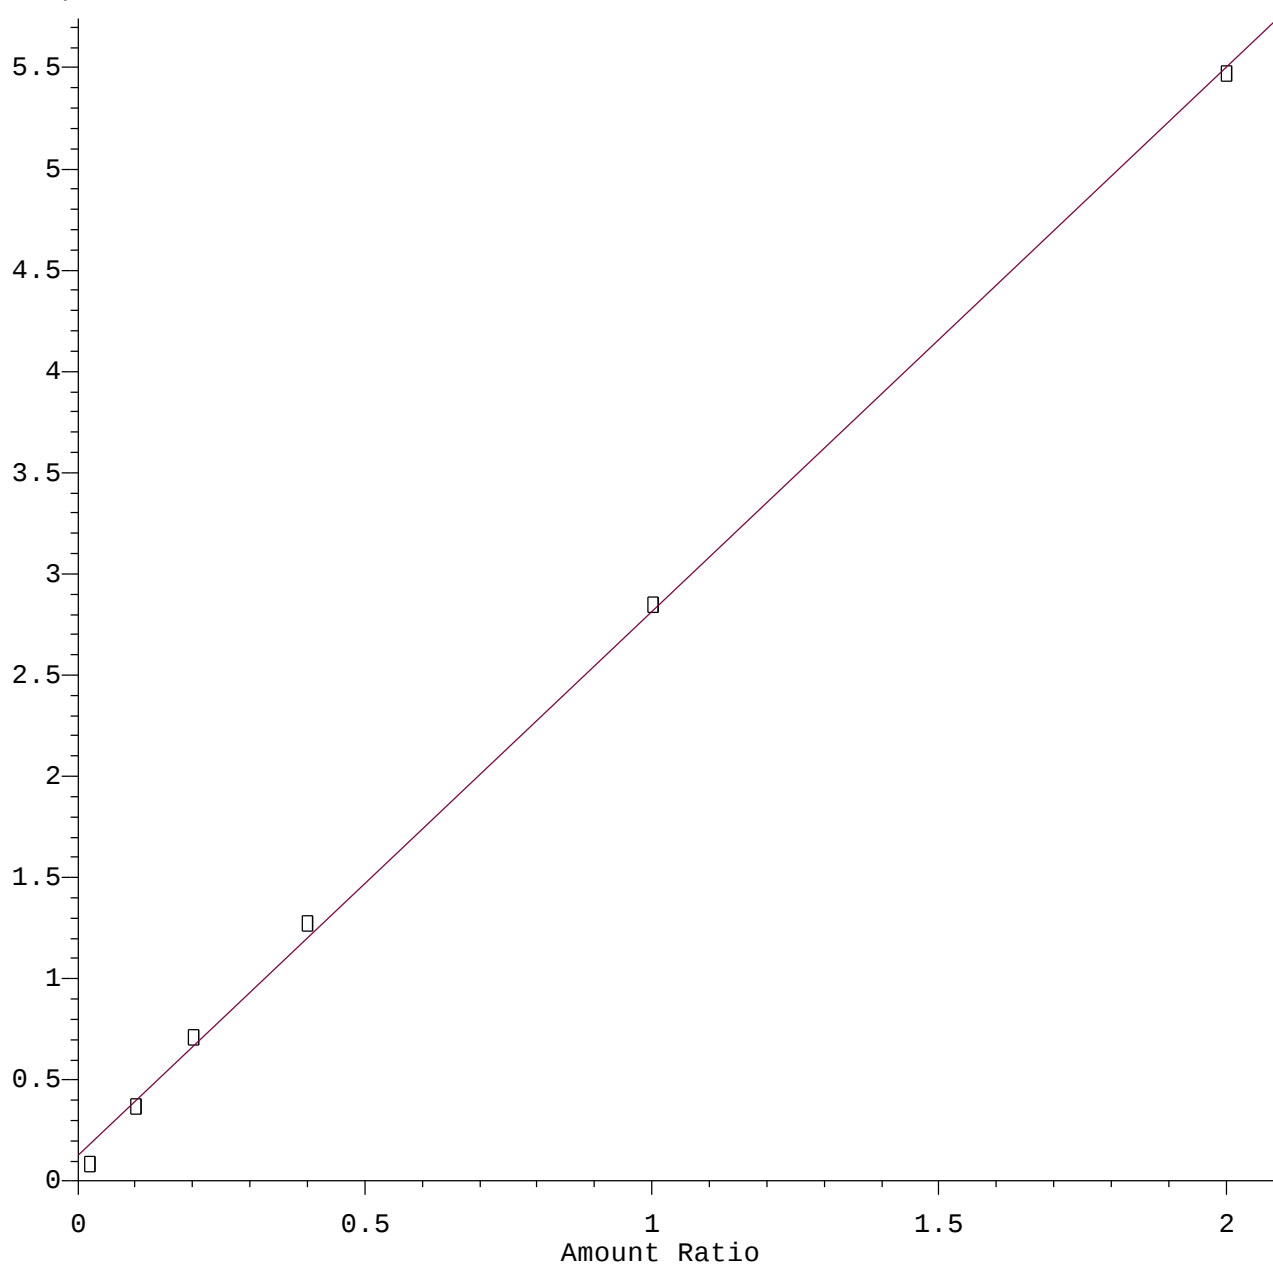


Resp Ratio = 2.69e+000 * Amt + 1.24e-001
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042219W.M
Calibration Table Last Updated: Tue Apr 23 05:52:53 2019


1,2,4-Trichlorobenzene

Response Ratio

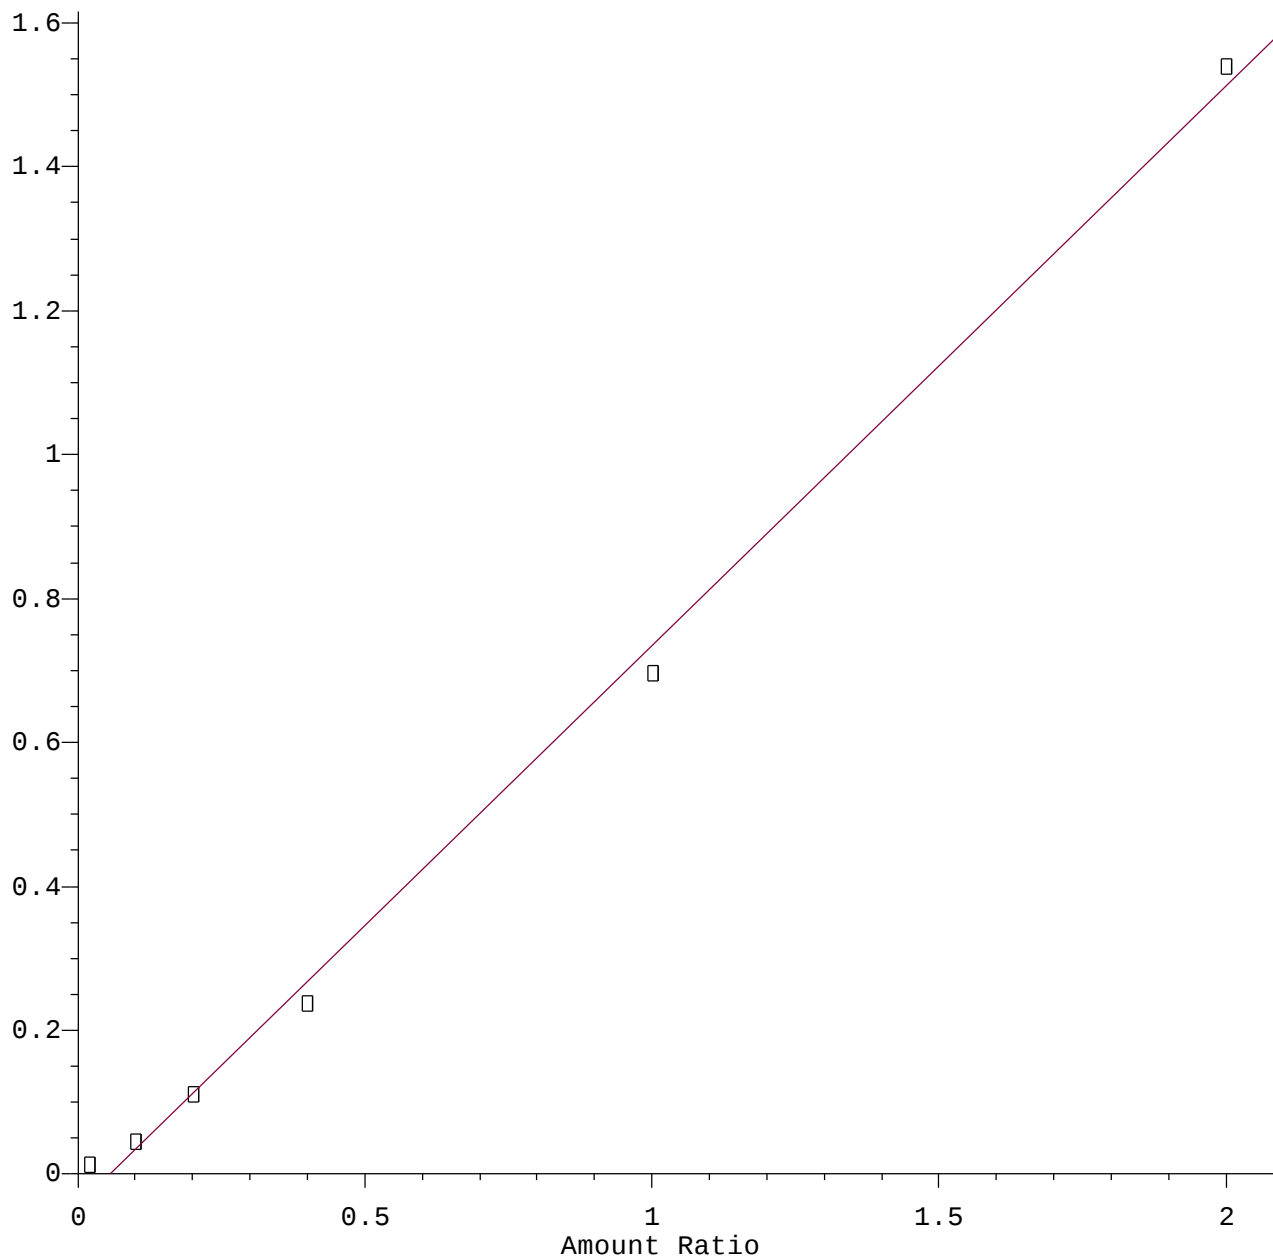

Resp Ratio = $7.78 \times 10^{-1} \times \text{Amt} - 4.26 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042219W.M
Calibration Table Last Updated: Tue Apr 23 05:52:53 2019

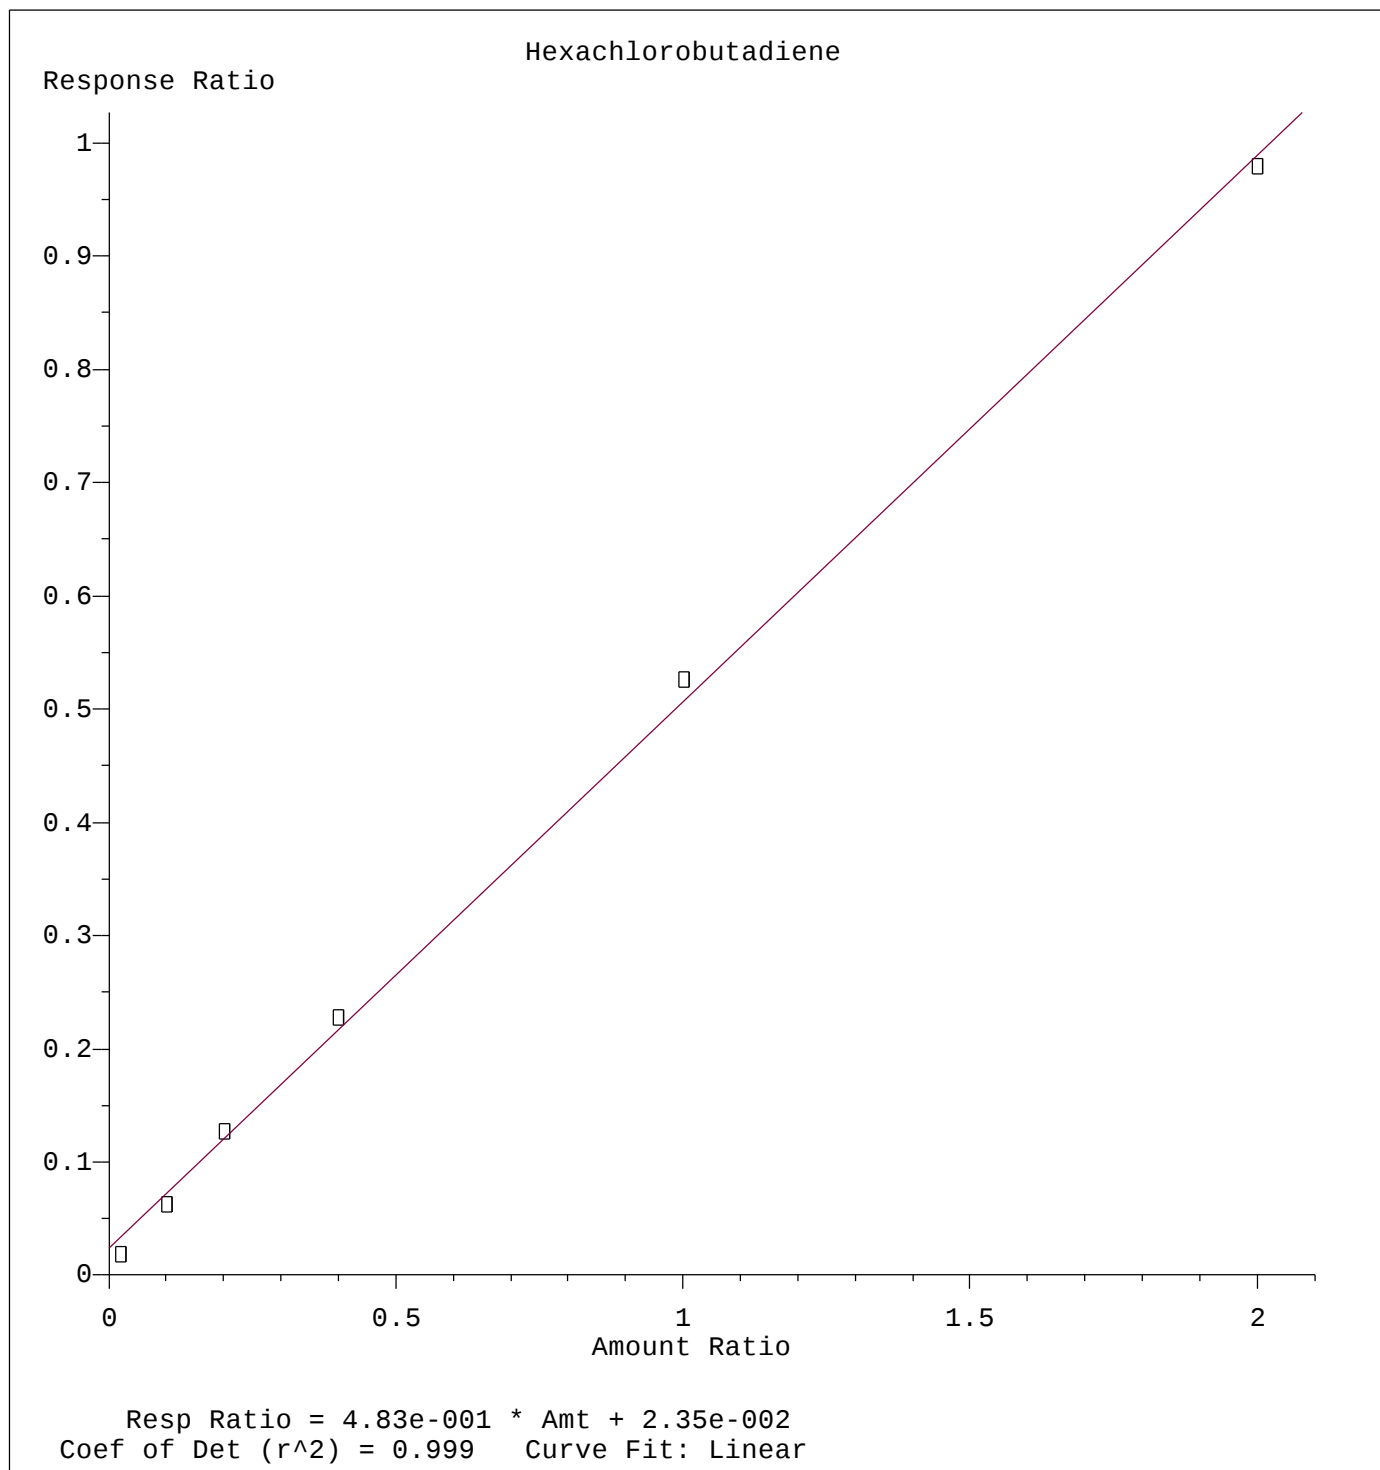

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042219W.M
Calibration Table Last Updated: Tue Apr 23 05:52:53 2019

Naphthalene

Response Ratio

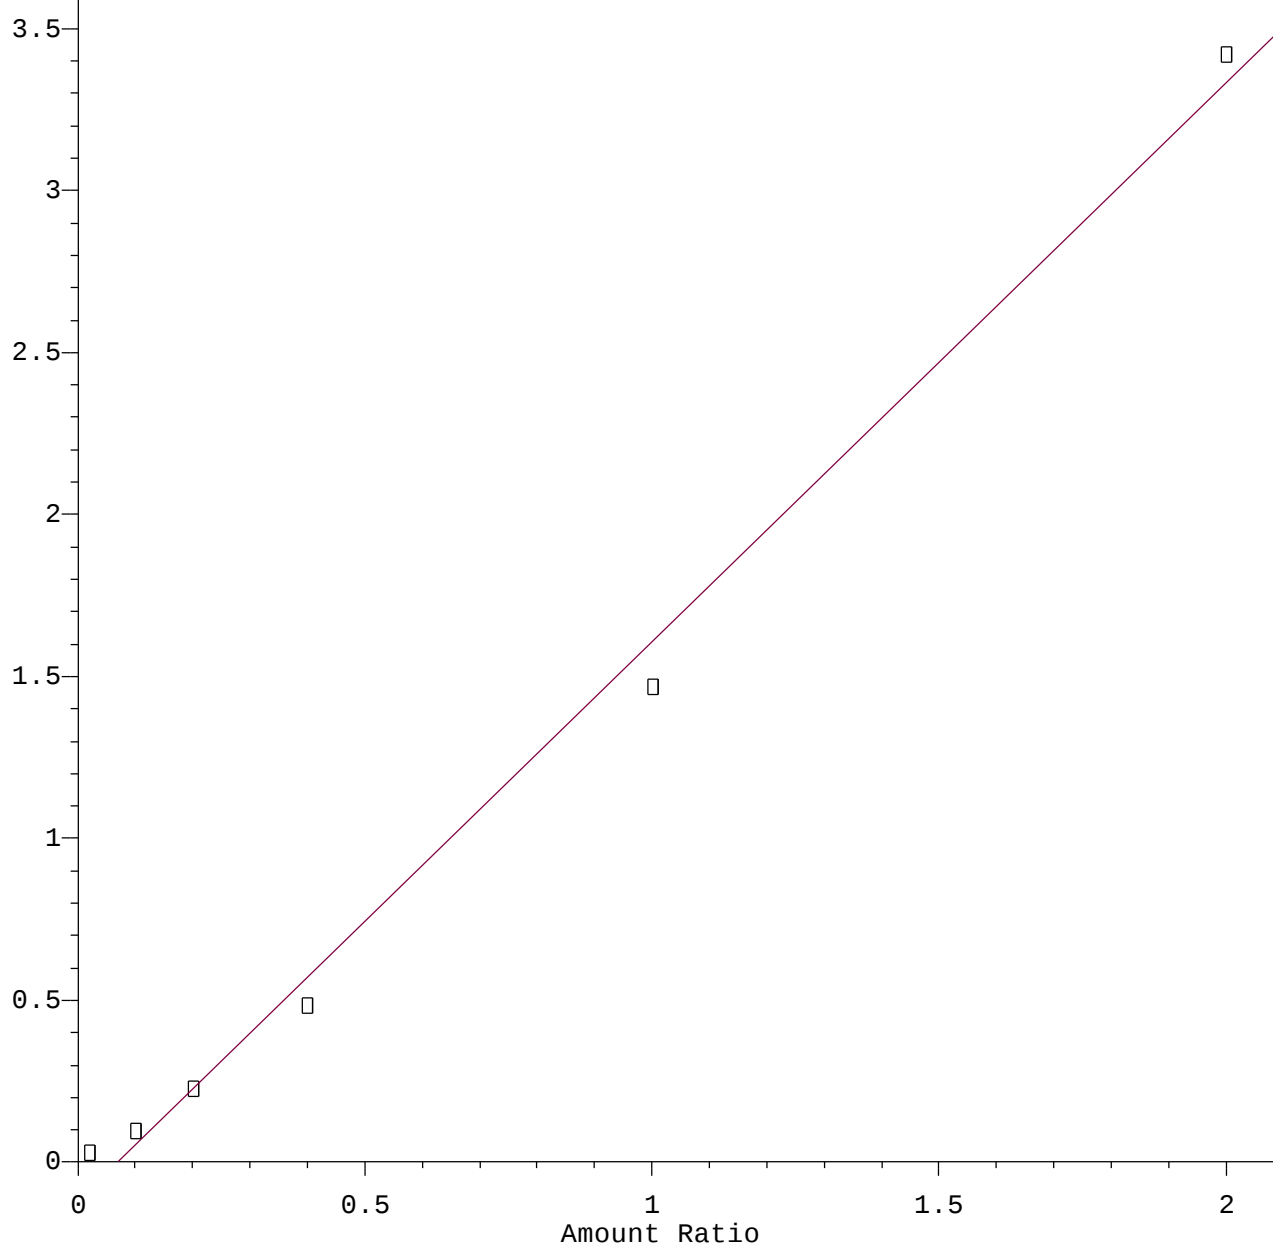


Resp Ratio = $1.72 \times 10^0 \times \text{Amt} - 1.17 \times 10^{-1}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042219W.M
Calibration Table Last Updated: Tue Apr 23 05:52:53 2019


1,2,3-Trichlorobenzene

Response Ratio

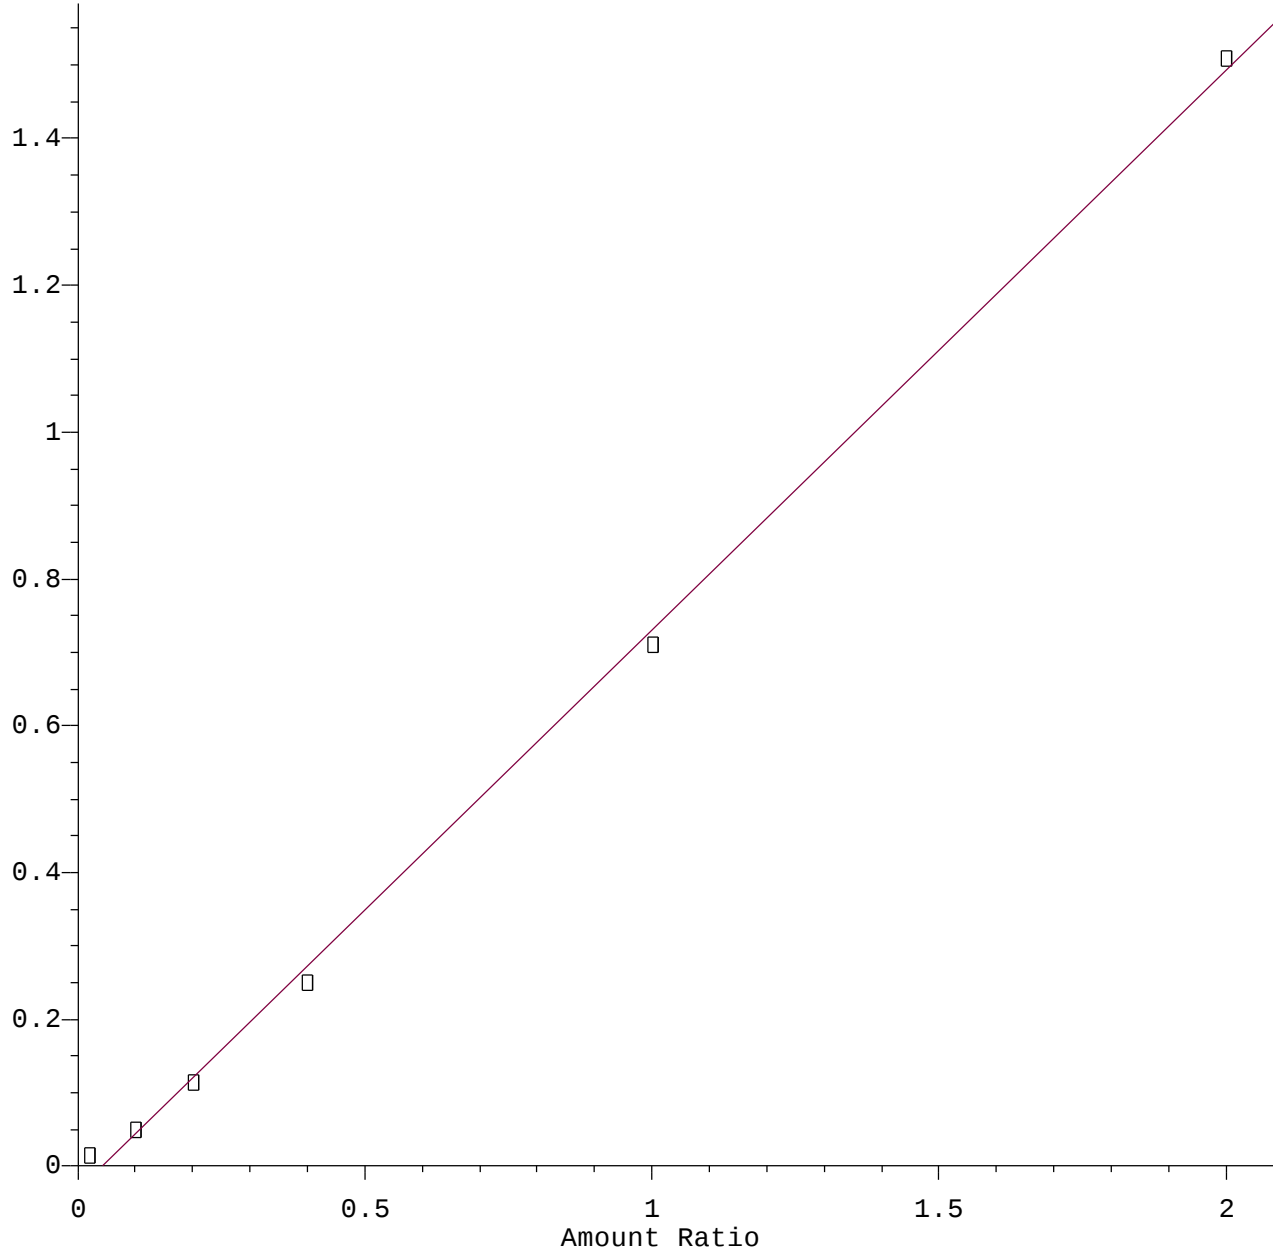


Resp Ratio = 7.63e-001 * Amt - 3.24e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042219W.M
Calibration Table Last Updated: Tue Apr 23 05:52:53 2019

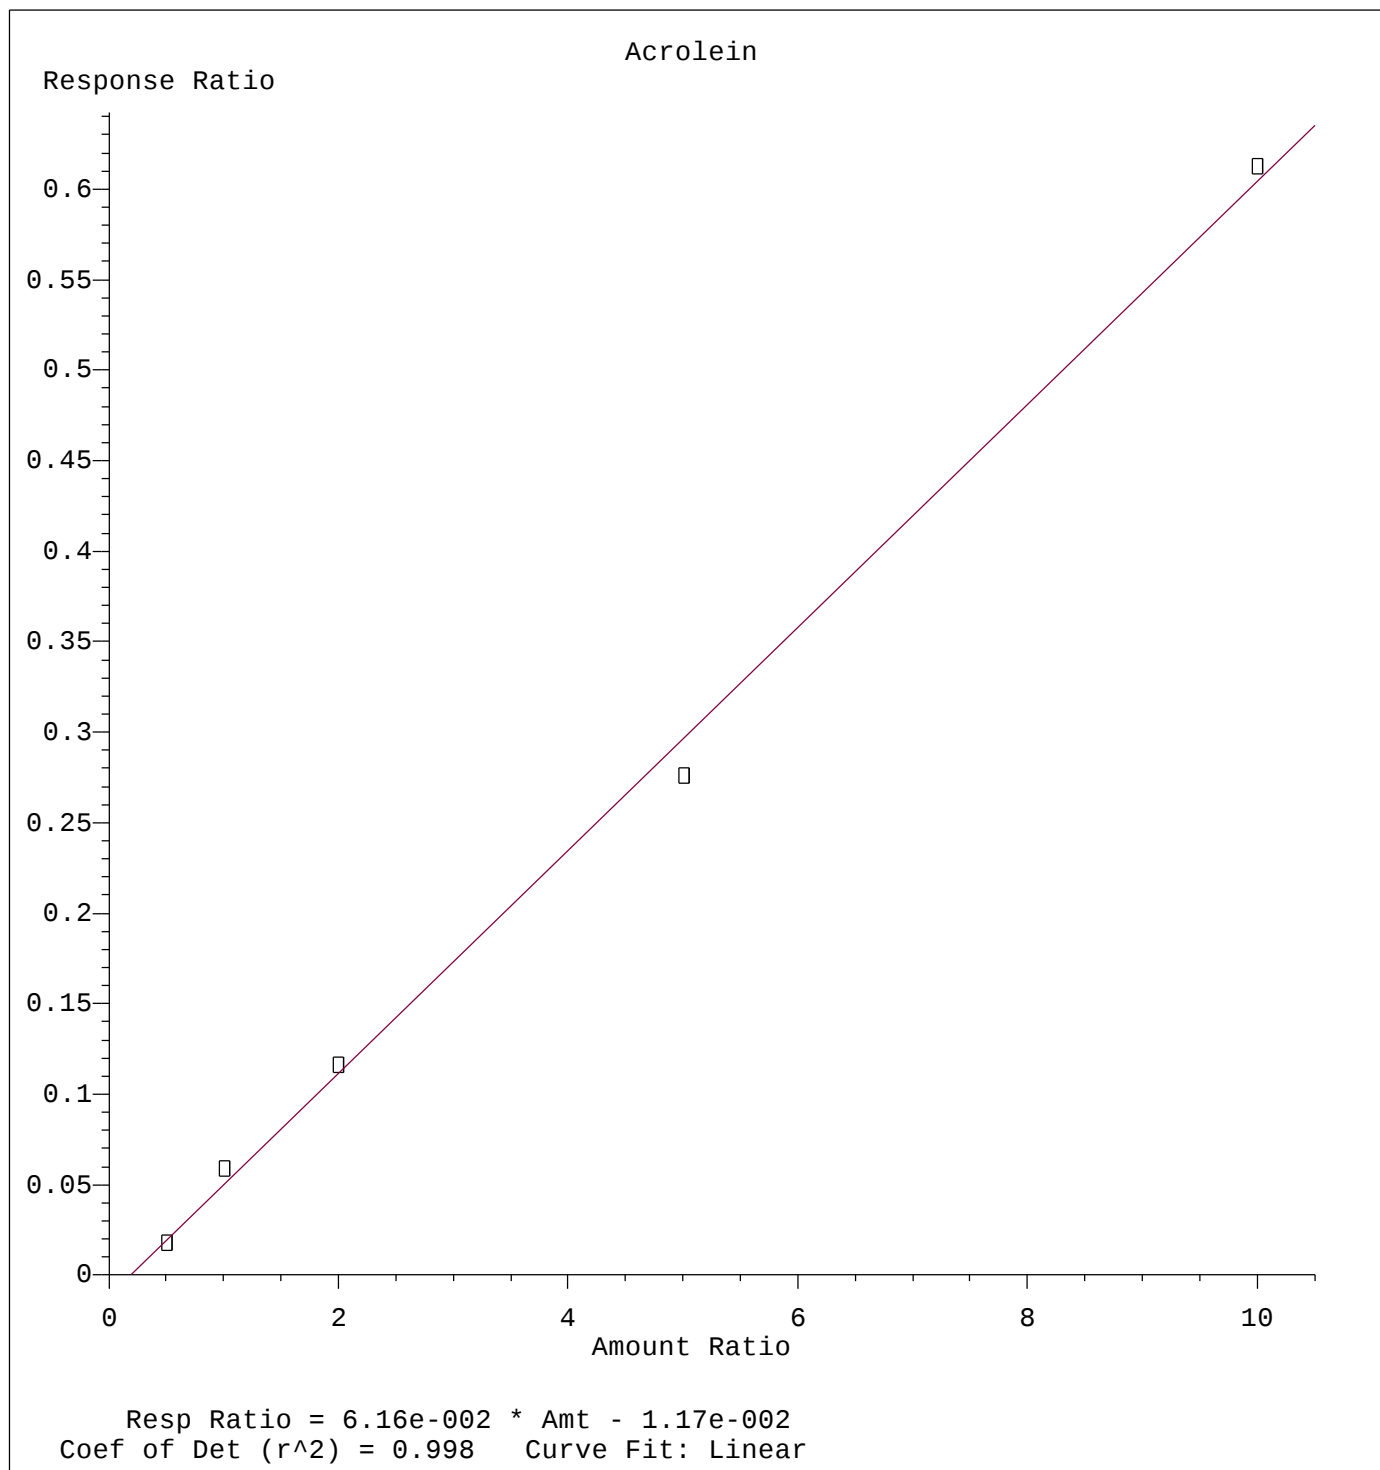

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042219W.M
Calibration Table Last Updated: Tue Apr 23 05:52:53 2019

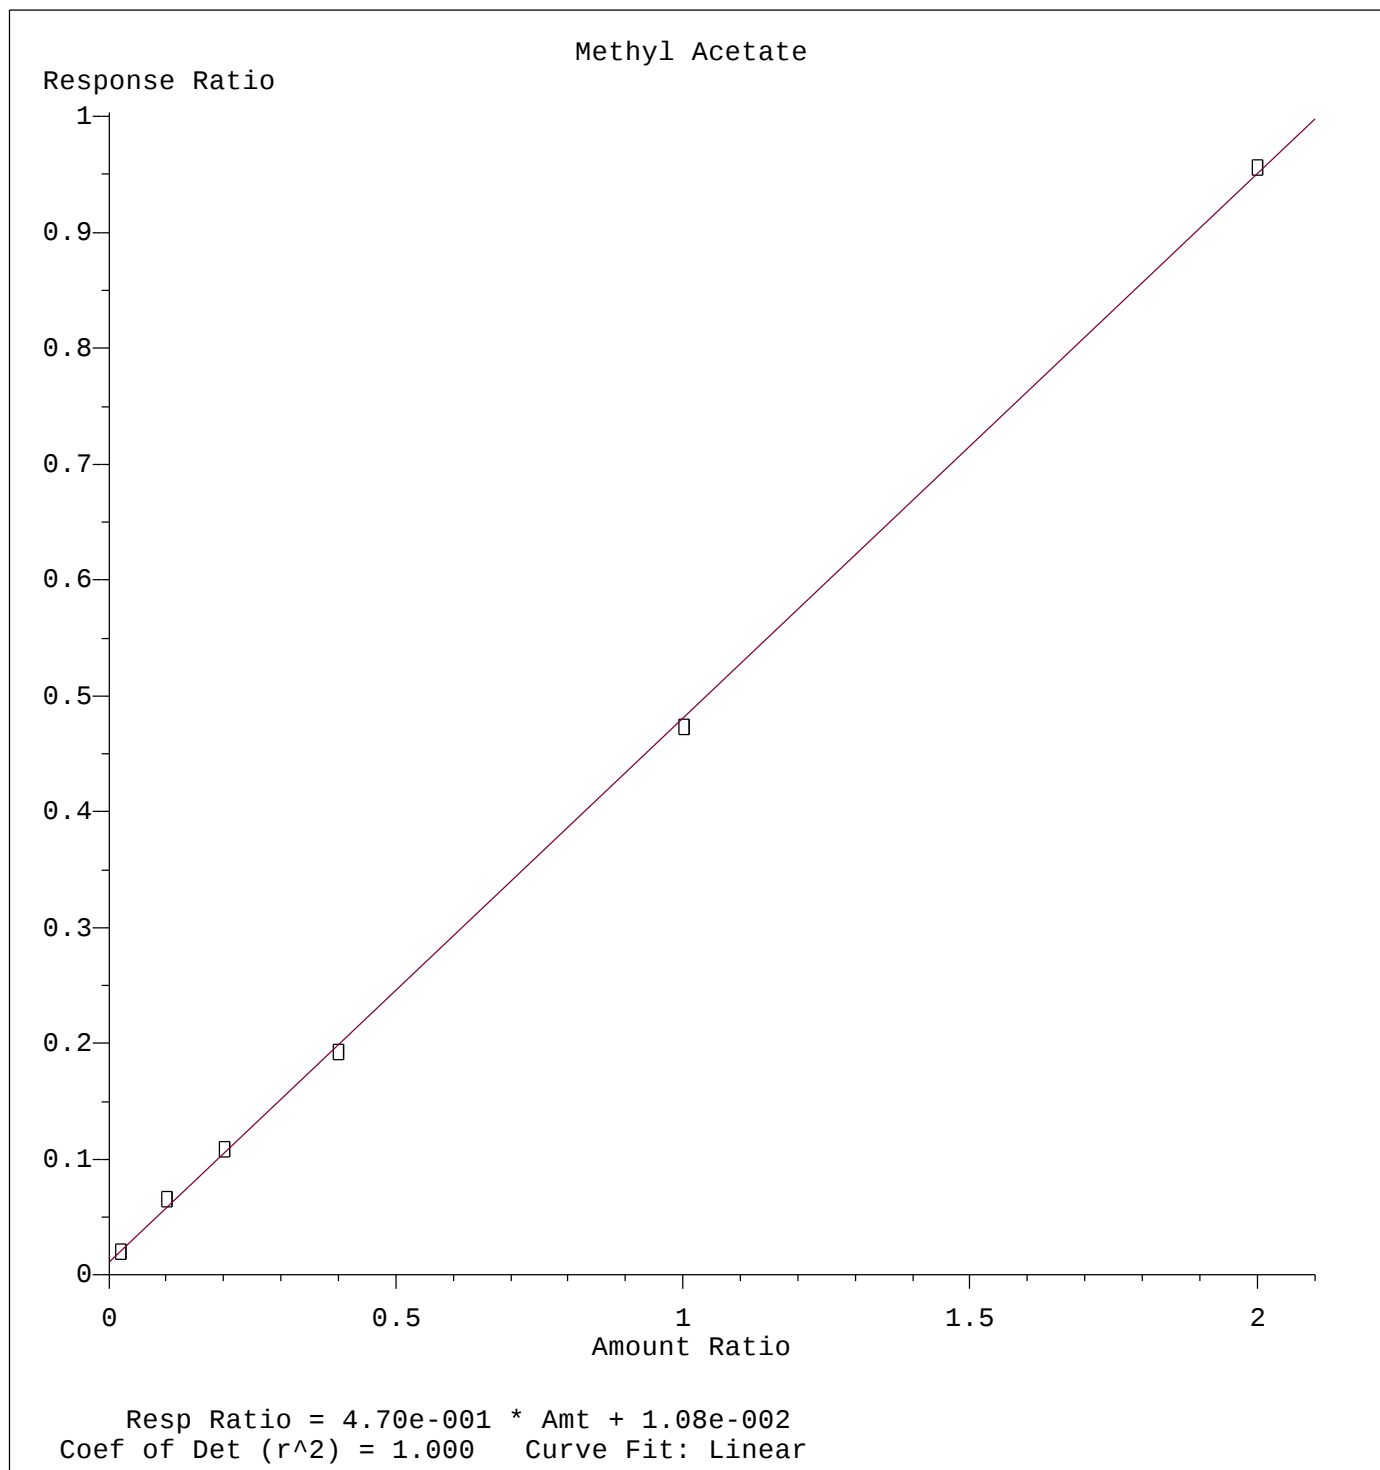

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042219W.M
Calibration Table Last Updated: Tue Apr 23 05:52:53 2019

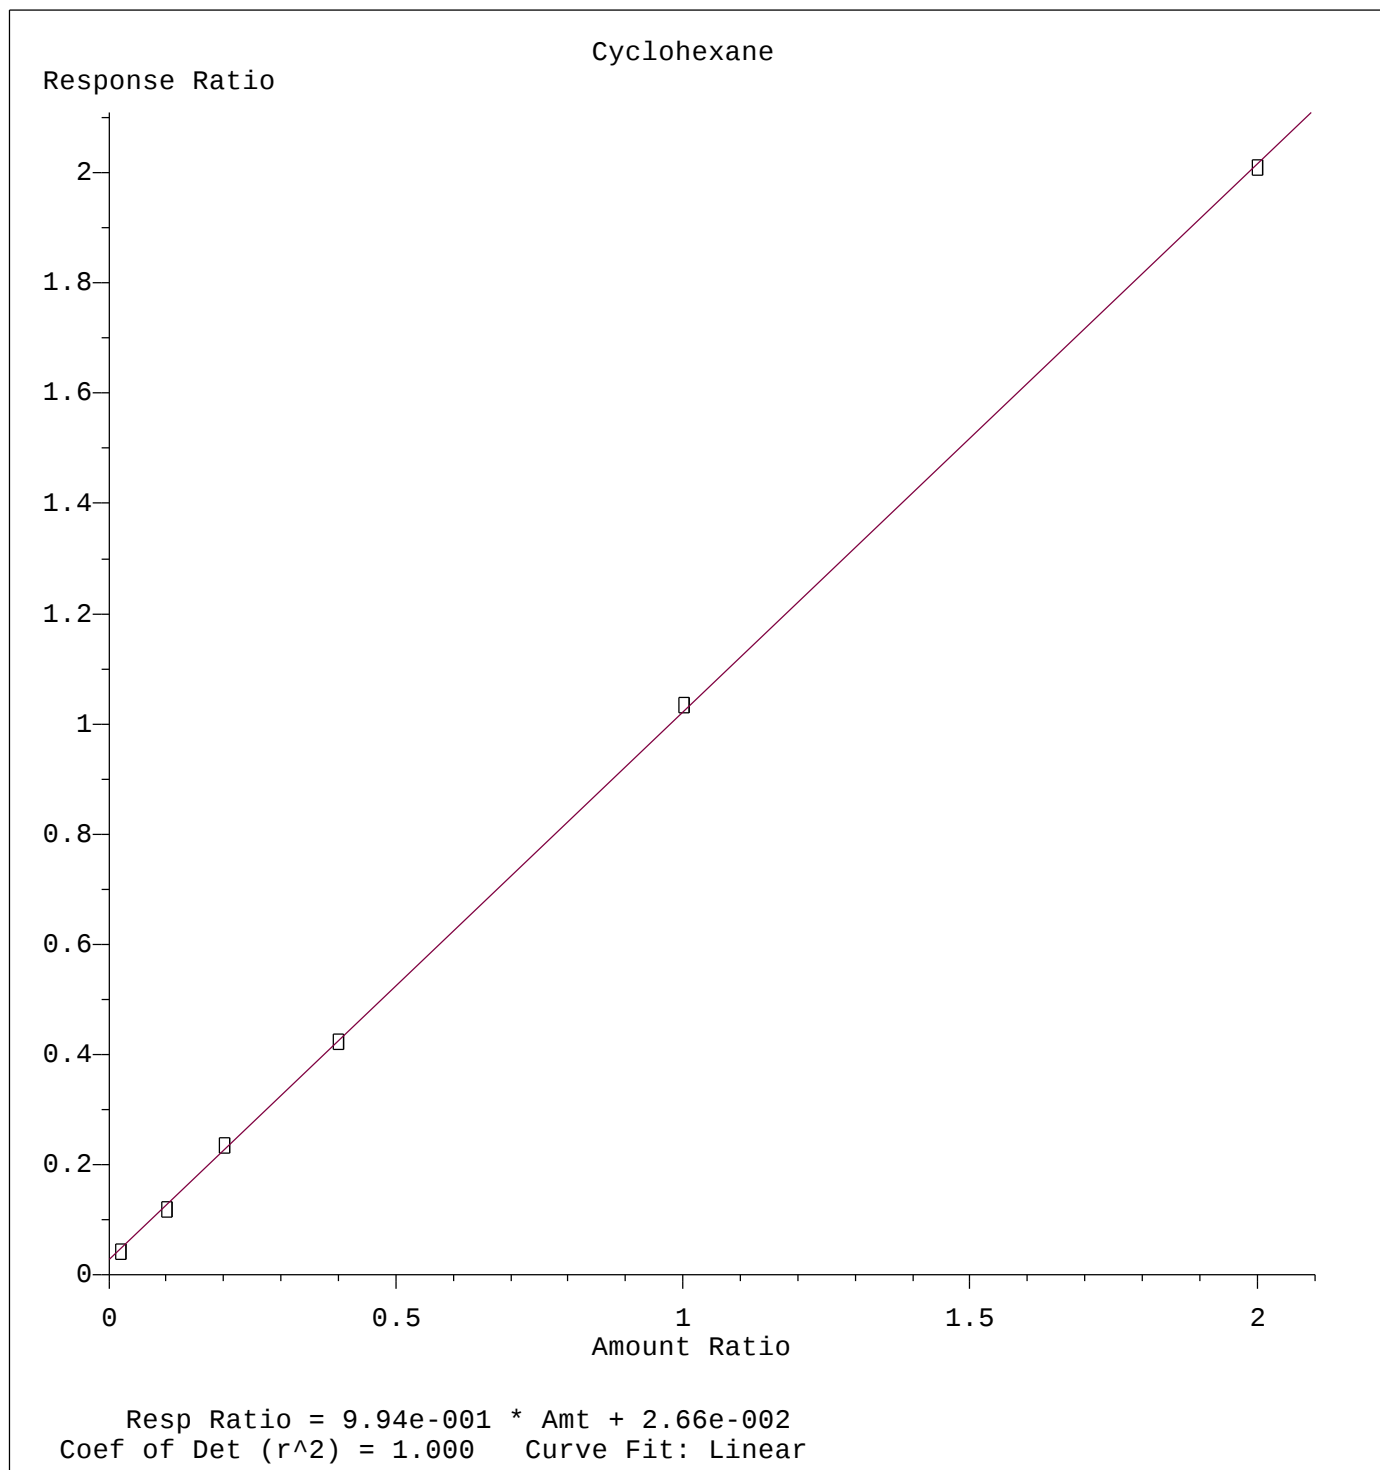

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042219W.M
Calibration Table Last Updated: Tue Apr 23 05:52:53 2019