


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN042220\
 Data File : VN061124.D
 Acq On : 22 Apr 2020 12:38
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042220W.M
 Title : SW846 8260
 Last Update : Wed Apr 22 15:26:40 2020

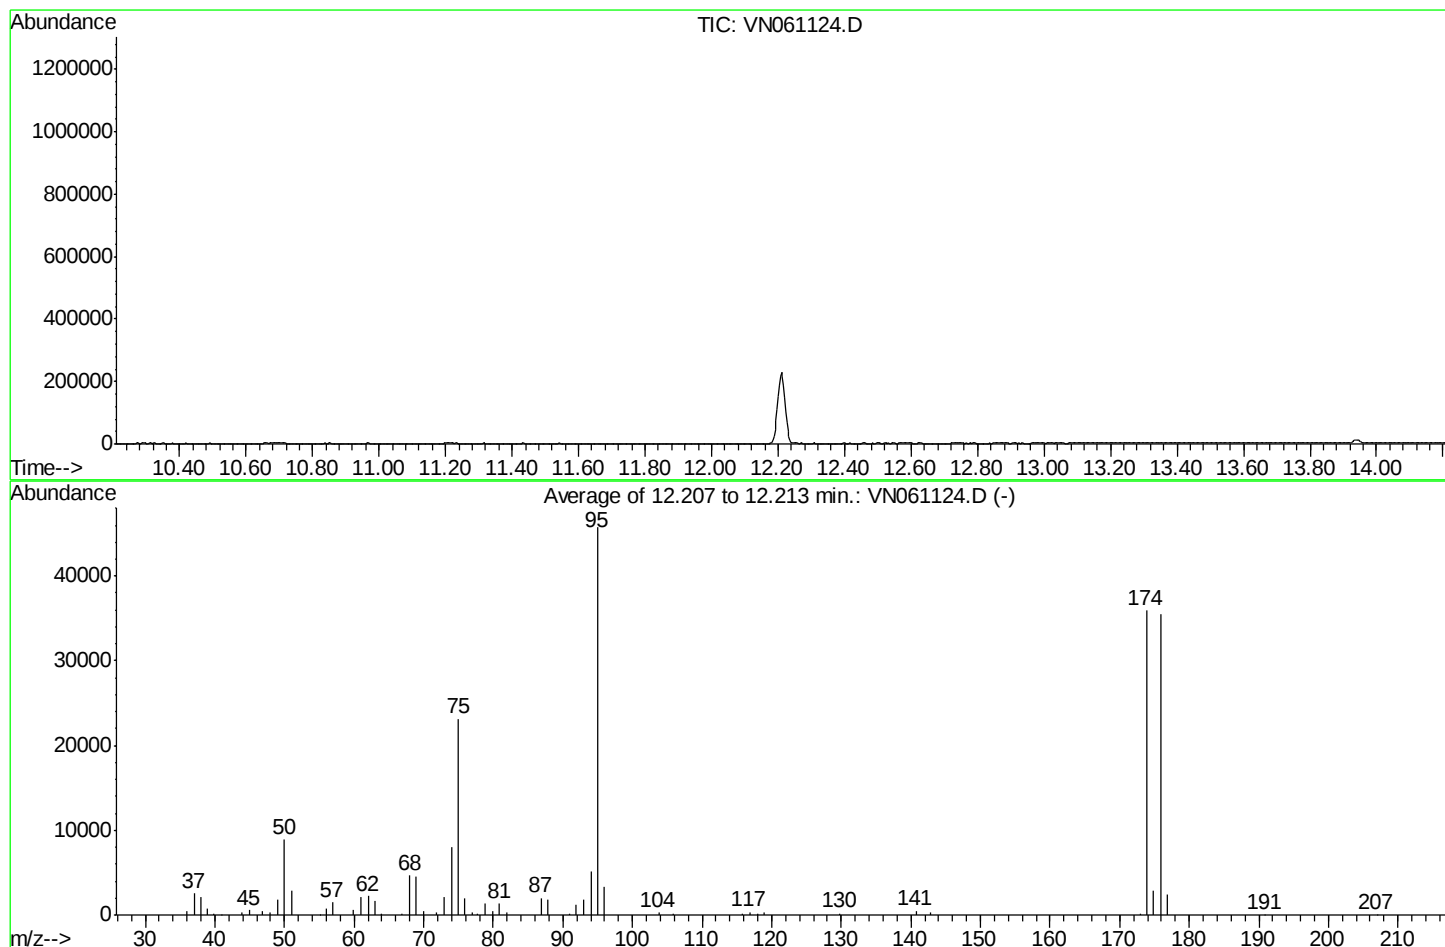

AutoFind: Scans 3302, 3303, 3304; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	8860	PASS
75	95	30	60	50.6	23128	PASS
95	95	100	100	100.0	45749	PASS
96	95	5	9	7.1	3265	PASS
173	174	0.00	2	0.3	107	PASS
174	95	50	100	78.4	35885	PASS
175	174	5	9	8.0	2887	PASS
176	174	95	101	99.0	35522	PASS
177	176	5	9	7.0	2482	PASS