

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042222\
 Data File : VN072160.D
 Acq On : 22 Apr 2022 16:34
 Operator : JC\MD
 Sample : N2514-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Apr 23 03:20:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 31 01:57:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.087	168	541057	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	919865	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	996989	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.669	152	385669	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	278351	45.064	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	90.120%
35) Dibromofluoromethane	8.016	113	258936	47.837	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	95.680%
50) Toluene-d8	10.439	98	1184831	53.509	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	107.020%
62) 4-Bromofluorobenzene	12.727	95	410415	57.310	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	114.620%
Target Compounds						
					Qvalue	
3) Chloromethane	2.305	50	1508	0.277	ug/l #	76
5) Bromomethane	2.875	94	1353	0.348	ug/l #	67
14) Allyl chloride	5.093	41	2837	0.391	ug/l #	24
16) Acetone	4.287	43	58964	22.337	ug/l	92
17) Carbon Disulfide	4.546	76	2637	0.257	ug/l #	75
18) Methyl Acetate	4.869	43	6283	Below Cal		99
20) Methylene Chloride	5.098	84	105664	18.991	ug/l	93
25) 2-Butanone	7.340	43	18678	4.908	ug/l	99
31) Cyclohexane	8.081	56	13490	1.606	ug/l #	11
36) 1,1-Dichloropropene	8.081	75	34958	4.625	ug/l #	50
37) Ethyl Acetate	7.340	43	18678	2.258	ug/l #	67
38) Carbon Tetrachloride	8.087	117	47401	6.399	ug/l #	17
39) Methylcyclohexane	9.457	83	14633	1.626	ug/l	92
43) Isopropyl Acetate	8.557	43	45412	3.300	ug/l #	85
45) 1,2-Dichloropropane	9.622	63	1965	0.329	ug/l #	44
48) Methyl methacrylate	9.545	41	8606	1.507	ug/l #	21
49) 1,4-Dioxane	9.616	88	73	Below Cal	#	1
51) 4-Methyl-2-Pentanone	10.333	43	5171	0.654	ug/l #	64
54) cis-1,3-Dichloropropene	10.239	75	53613	5.807	ug/l #	57
55) 1,1,2-Trichloroethane	10.875	97	1886	0.304	ug/l #	16
57) 1,3-Dichloropropane	11.086	76	24995	2.406	ug/l #	43
59) 2-Hexanone	11.086	43	295854	53.111	ug/l #	49
68) m/p-Xylenes	11.945	106	2823	0.217	ug/l	83
69) o-Xylene	12.280	106	3227	0.250	ug/l	93
73) Isopropylbenzene	12.574	105	25163	0.774	ug/l	98
76) 1,2,3-Trichloropropane	12.727	75	193640	21.674	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.727	75	193640	67.166	ug/l #	10
84) 1,2,4-Trimethylbenzene	13.363	105	24912	0.992	ug/l	97
85) sec-Butylbenzene	13.492	105	12957	0.425	ug/l #	72
89) n-Butylbenzene	13.933	91	4502	0.249	ug/l #	79
90) Hexachloroethane	14.216	117	2900	0.651	ug/l #	9
93) 1,2,4-Trichlorobenzene	15.263	180	429	2.153	ug/l #	57
95) Naphthalene	15.504	128	4037	4.015	ug/l #	81
96) 1,2,3-Trichlorobenzene	15.680	180	422	2.482	ug/l #	1

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042222\
Data File : VN072160.D
Acq On : 22 Apr 2022 16:34
Operator : JC\MD
Sample : N2514-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Apr 23 03:20:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 31 01:57:54 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#) = qualifier out of range (m) = manual integration (+) = signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042222\
Data File : VN072160.D
Acq On : 22 Apr 2022 16:34
Operator : JC\MD
Sample : N2514-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Apr 23 03:20:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 31 01:57:54 2022
Response via : Initial Calibration




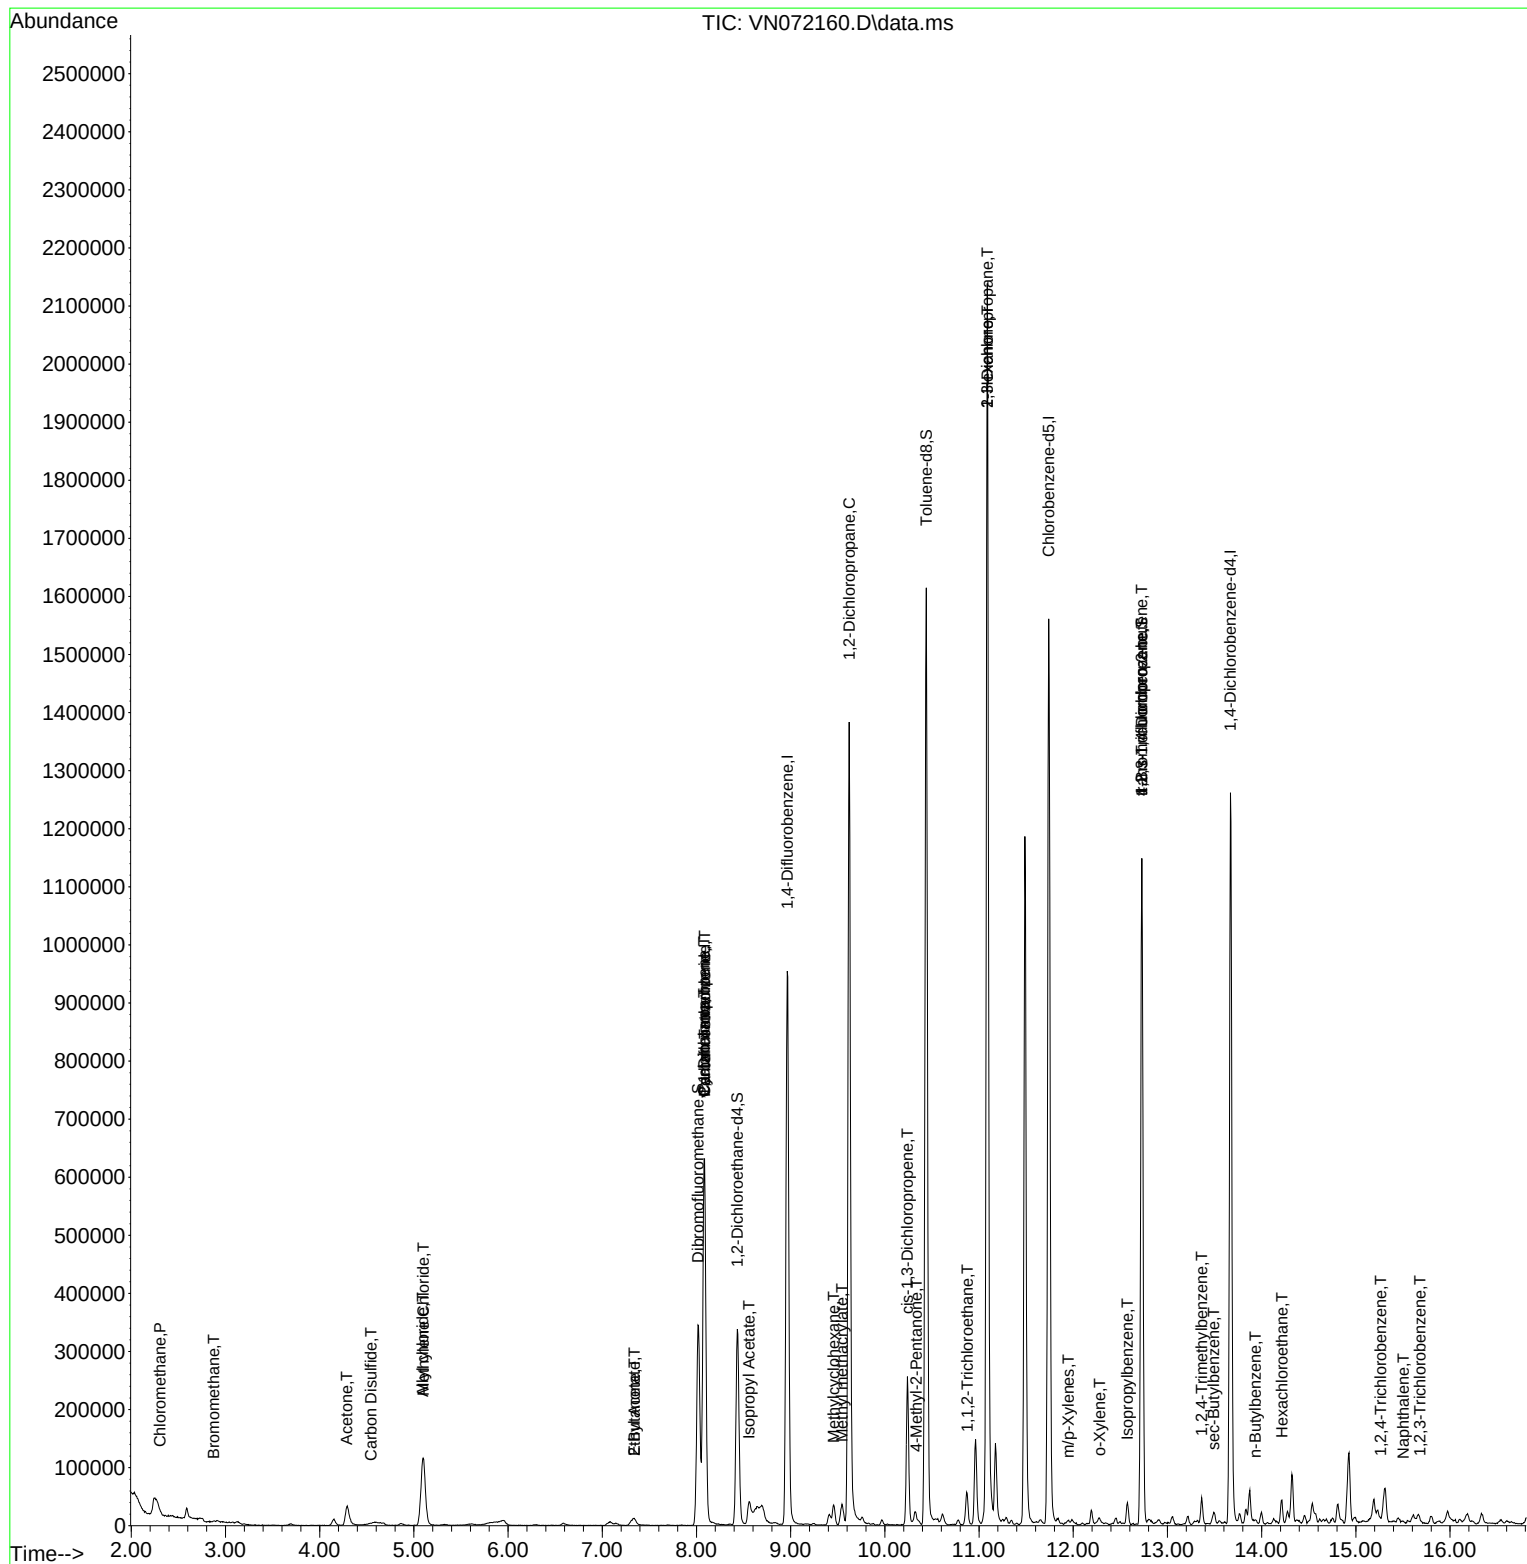




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.087 min Scan# 10
Delta R.T. 0.006 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 541057
Ion Ratio Lower Upper
168 100
99 48.9 42.3 63.5

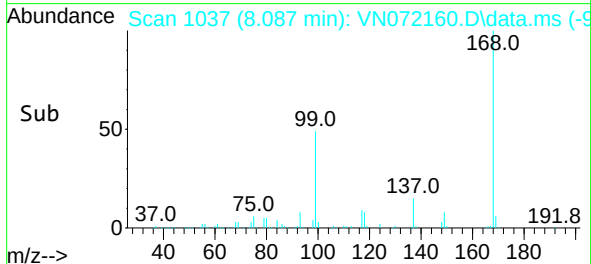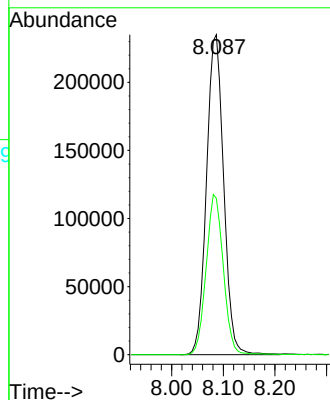

#3
Chloromethane
Concen: 0.277 ug/l
RT: 2.305 min Scan# 54
Delta R.T. 0.006 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34


Tgt Ion: 50 Resp: 1508
Ion Ratio Lower Upper
50 100
52 18.8 25.7 38.5#

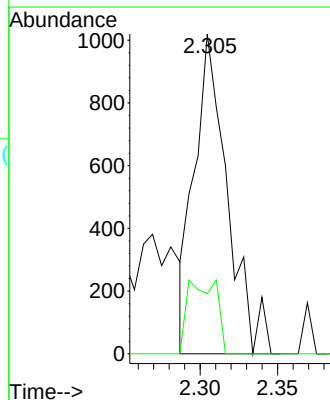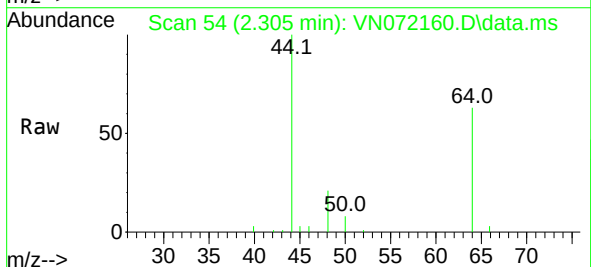



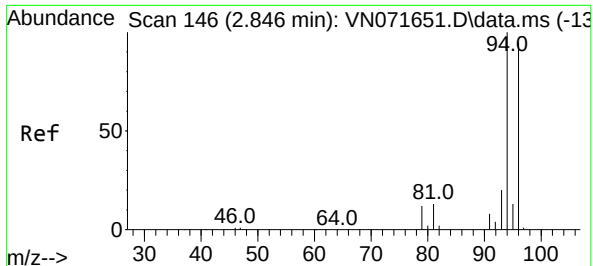


#5
Bromomethane
Concen: 0.348 ug/l
RT: 2.875 min Scan# 11
Delta R.T. 0.029 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34

Instrument :
MSVOA_N
ClientSampleId :



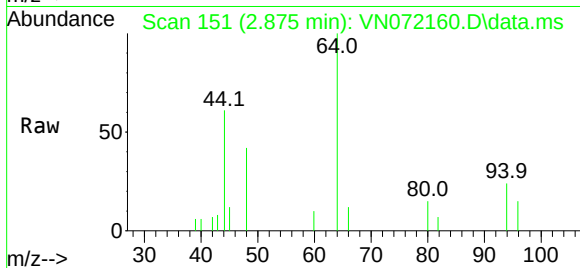



Tgt Ion: 94 Resp: 1353
Ion Ratio Lower Upper
94 100
96 62.6 76.0 114.0#

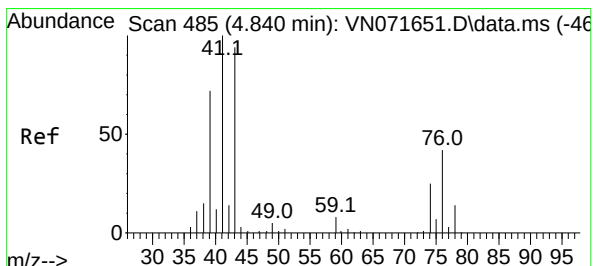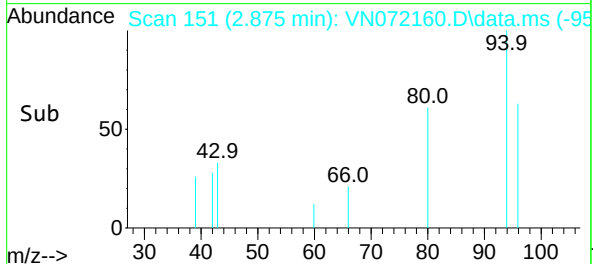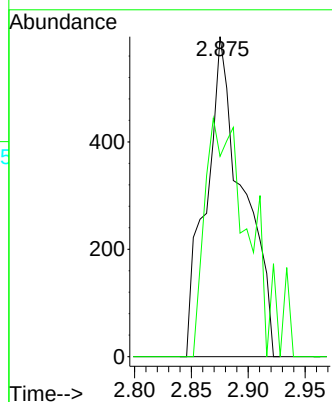

#14
Allyl chloride
Concen: 0.391 ug/l
RT: 5.093 min Scan# 528
Delta R.T. 0.253 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34

Tgt Ion: 41 Resp: 2837
Ion Ratio Lower Upper
41 100
39 0.0 53.2 79.8#
76 0.0 29.9 44.9#


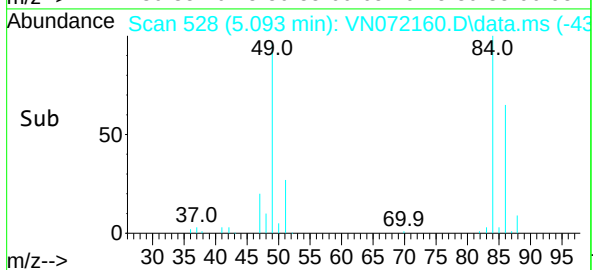

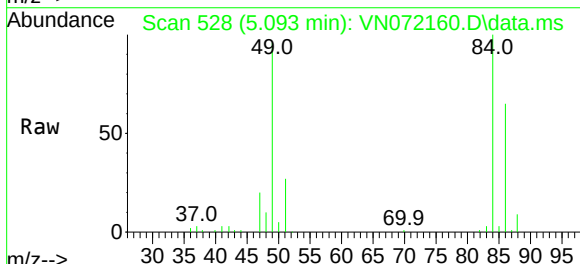




#16
Acetone
Concen: 22.337 ug/l
RT: 4.287 min Scan# 391
Delta R.T. 0.012 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 58964
Ion Ratio Lower Upper
43 100
58 36.9 26.0 39.0

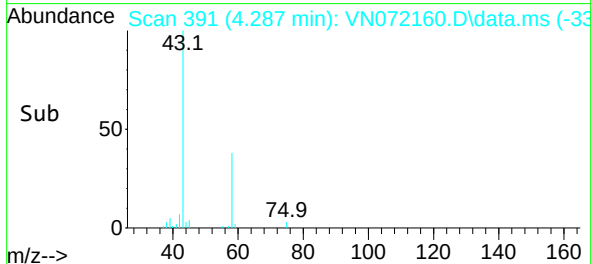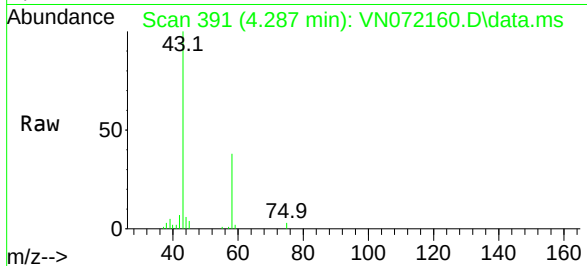

#17
Carbon Disulfide
Concen: 0.257 ug/l
RT: 4.546 min Scan# 435
Delta R.T. 0.012 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34

Tgt Ion: 76 Resp: 2637
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#




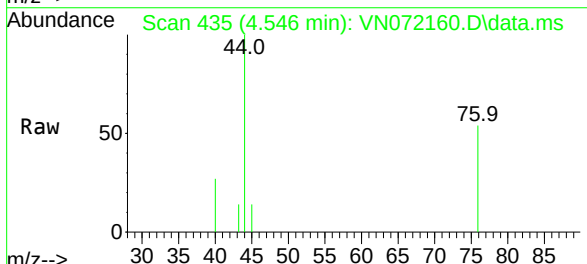




#18
Methyl Acetate
Concen: Below Cal
RT: 4.869 min Scan# 49
Delta R.T. 0.023 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 6283
Ion Ratio Lower Upper
43 100
74 26.4 21.6 32.4

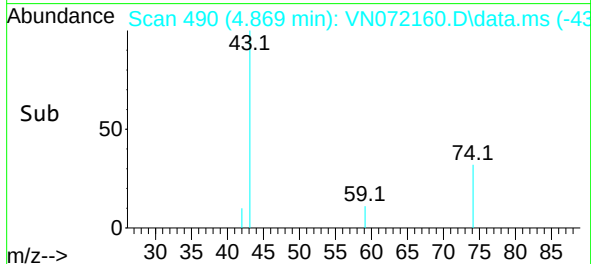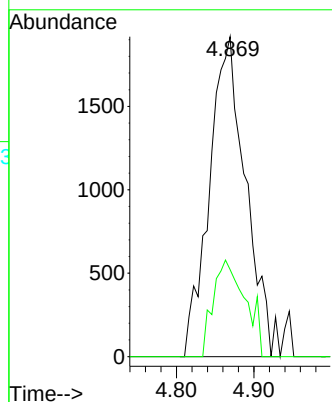

#20
Methylene Chloride
Concen: 18.991 ug/l
RT: 5.098 min Scan# 529
Delta R.T. 0.005 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34

Tgt Ion: 84 Resp: 105664
Ion Ratio Lower Upper
84 100
49 99.7 88.3 132.5
51 32.3 28.2 42.2
86 65.4 50.6 76.0

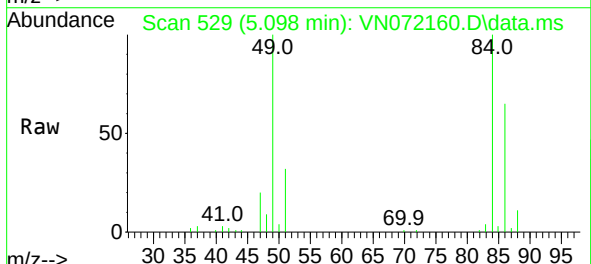

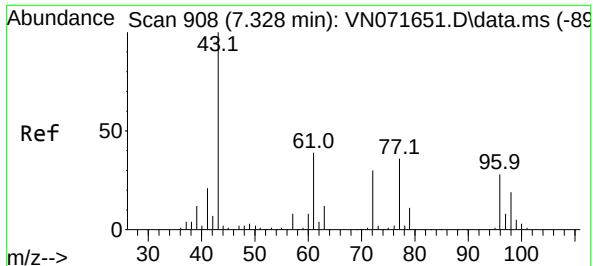

#25

2-Butanone

Concen: 4.908 ug/l

RT: 7.340 min Scan# 91

Delta R.T. 0.012 min

Lab File: VN072160.D

Acq: 22 Apr 2022 16:34

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 43 Resp: 18678

Ion Ratio Lower Upper

43 100

72 29.3 23.7 35.5

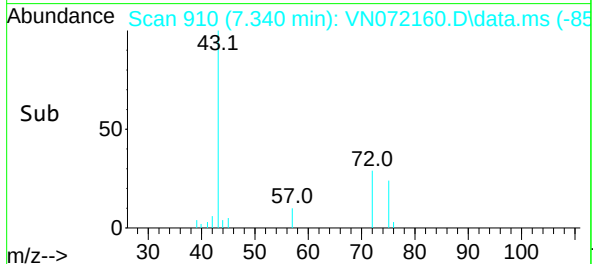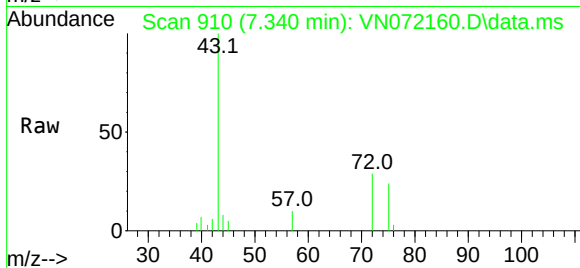

#31

Cyclohexane

Concen: 1.606 ug/l

RT: 8.081 min Scan# 1036

Delta R.T. -0.011 min

Lab File: VN072160.D

Acq: 22 Apr 2022 16:34




Tgt Ion: 56 Resp: 13490


Ion Ratio Lower Upper

56 100

69 153.3 27.8 41.8#

84 142.2 76.9 115.3#

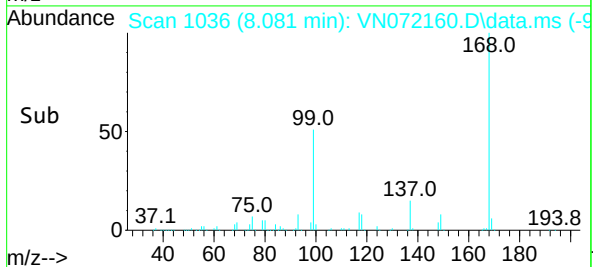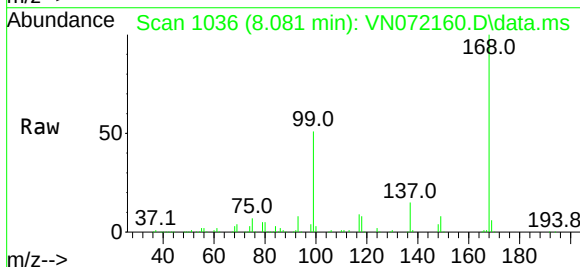



#33

1,2-Dichloroethane-d4

Concen: 45.064 ug/l

RT: 8.434 min Scan# 1096

Delta R.T. -0.000 min

Lab File: VN072160.D

Acq: 22 Apr 2022 16:34

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 278351

Ion Ratio Lower Upper

65 100

67 54.4 0.0 104.8

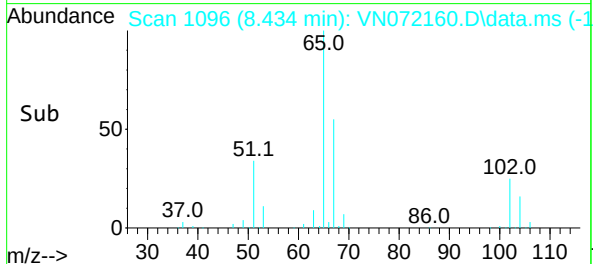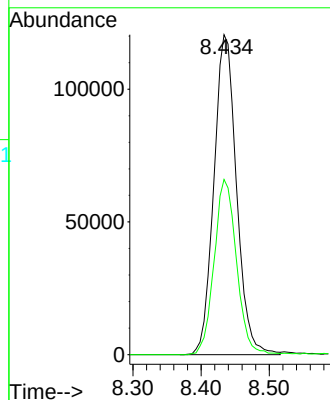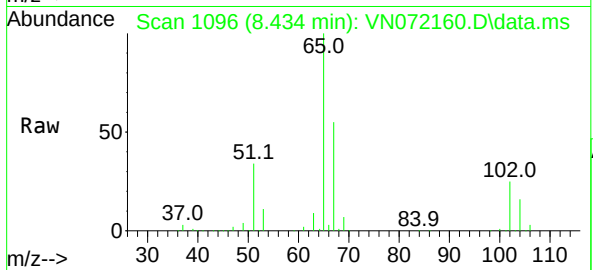

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. -0.000 min

Lab File: VN072160.D

Acq: 22 Apr 2022 16:34




Tgt Ion: 114 Resp: 919865


Ion Ratio Lower Upper

114 100

63 18.5 0.0 40.0

88 15.2 0.0 32.6

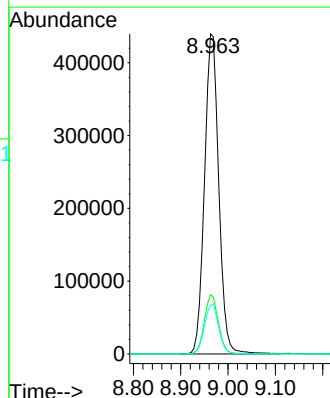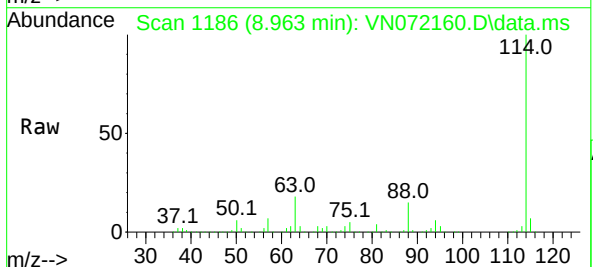

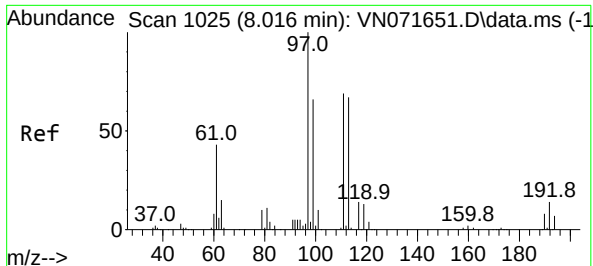

#35

Dibromofluoromethane

Concen: 47.837 ug/l

RT: 8.016 min Scan# 1025

Delta R.T. -0.000 min

Lab File: VN072160.D

Acq: 22 Apr 2022 16:34

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:113 Resp: 258936

Ion Ratio Lower Upper

113 100

111 103.8 81.4 122.0

192 23.0 17.0 25.6

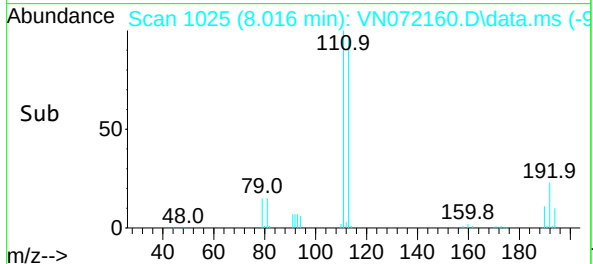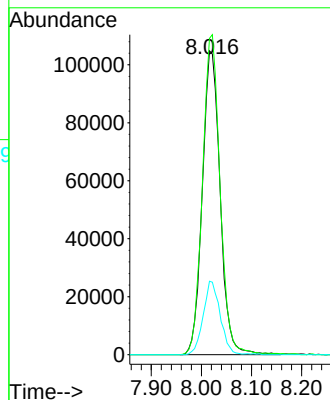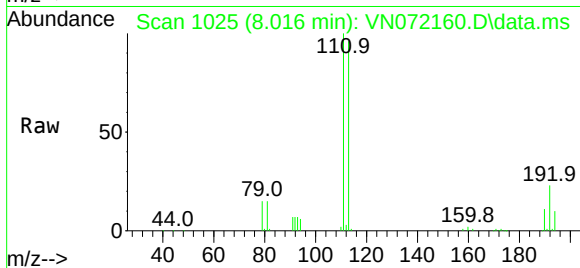

#36

1,1-Dichloropropene

Concen: 4.625 ug/l

RT: 8.081 min Scan# 1036

Delta R.T. -0.135 min

Lab File: VN072160.D

Acq: 22 Apr 2022 16:34




Tgt Ion: 75 Resp: 34958


Ion Ratio Lower Upper

75 100

110 9.8 18.3 54.8#

77 0.2 25.1 37.7#

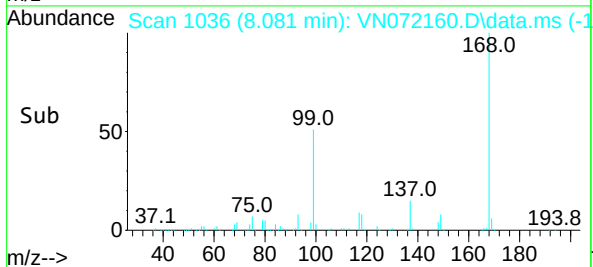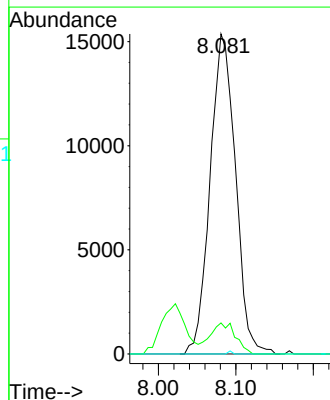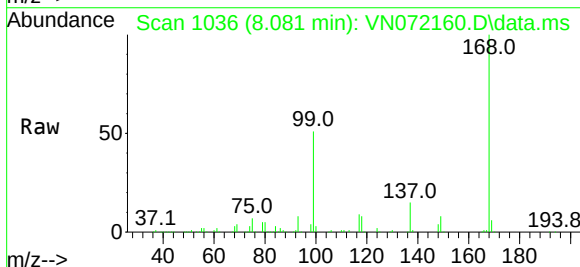



#37

Ethyl Acetate

Concen: 2.258 ug/l

RT: 7.340 min Scan# 91

Delta R.T. -0.064 min


Lab File: VN072160.D

Acq: 22 Apr 2022 16:34




Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion:	43	Resp:	18678
Ion	Ratio	Lower	Upper
43	100		
61	0.0	11.8	17.6#
70	0.0	9.3	13.9#

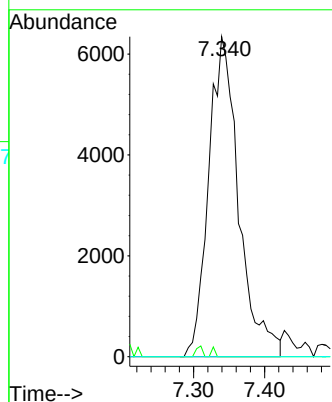

#38

Carbon Tetrachloride

Concen: 6.399 ug/l




RT: 8.087 min Scan# 1037


Delta R.T. -0.117 min

Lab File: VN072160.D

Acq: 22 Apr 2022 16:34

Tgt Ion:	117	Resp:	47401
Ion	Ratio	Lower	Upper
117	100		
119	6.2	75.8	113.8#
121	0.0	24.6	37.0#

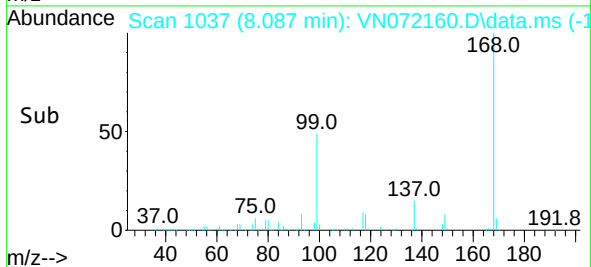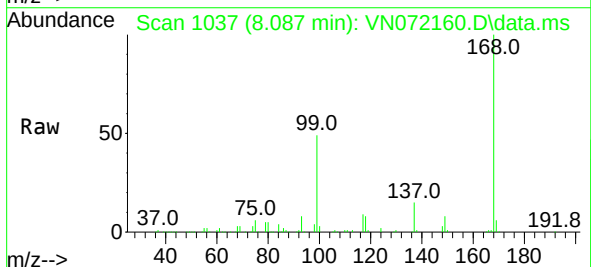

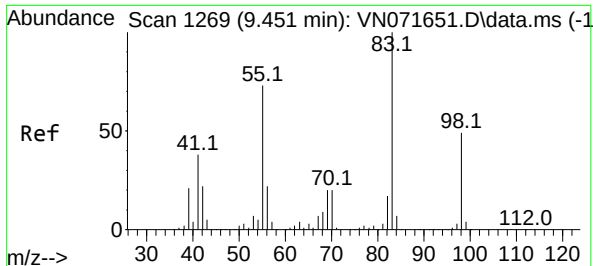

#39

Methylcyclohexane

Concen: 1.626 ug/l

RT: 9.457 min Scan# 1117

Delta R.T. 0.006 min

Lab File: VN072160.D

Acq: 22 Apr 2022 16:34

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion: 83 Resp: 14633

Ion Ratio Lower Upper

83 100

55 77.2 57.8 86.8

98 57.7 39.4 59.2

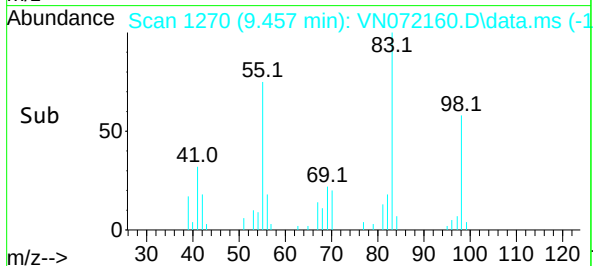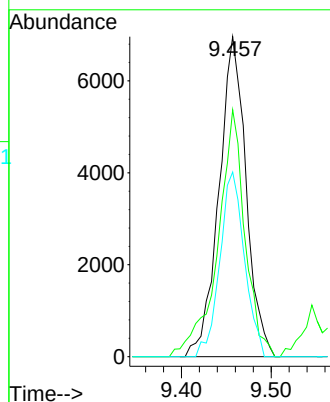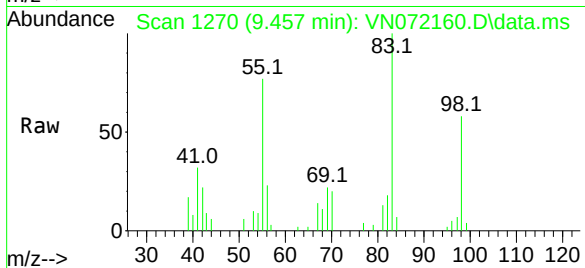

#43

Isopropyl Acetate

Concen: 3.300 ug/l

RT: 8.557 min Scan# 1117

Delta R.T. 0.006 min

Lab File: VN072160.D

Acq: 22 Apr 2022 16:34




Tgt Ion: 43 Resp: 45412


Ion Ratio Lower Upper

43 100

61 17.2 21.9 32.9#

87 12.2 12.0 18.0

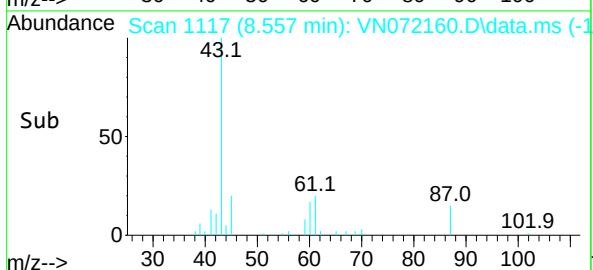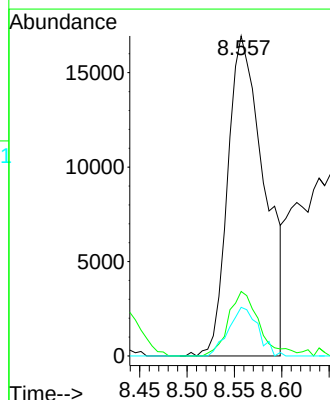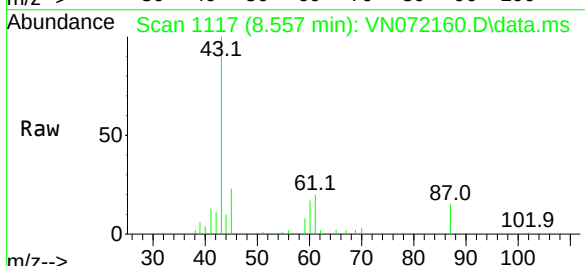

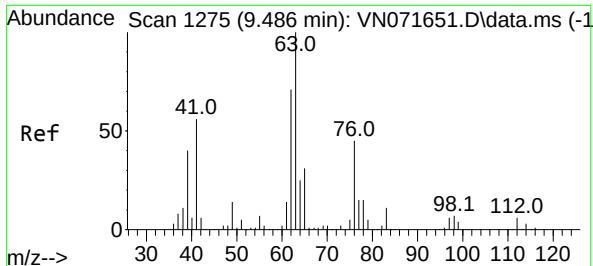

#45

1,2-Dichloropropane

Concen: 0.329 ug/l

RT: 9.622 min Scan# 1298

Delta R.T. 0.136 min

Lab File: VN072160.D

Acq: 22 Apr 2022 16:34

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 63 Resp: 1965

Ion Ratio Lower Upper

63 100

65 0.0 24.9 37.3#

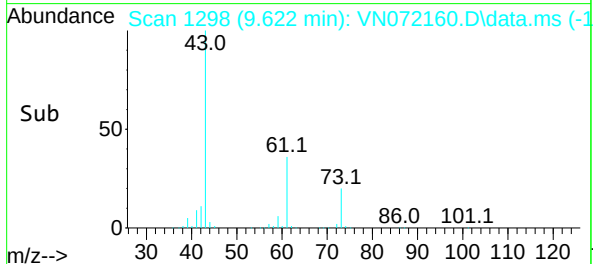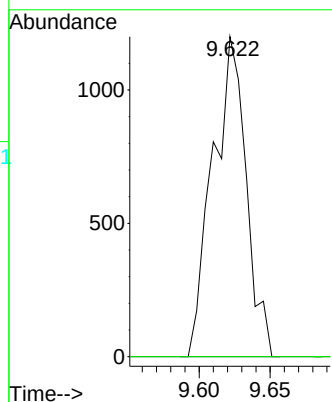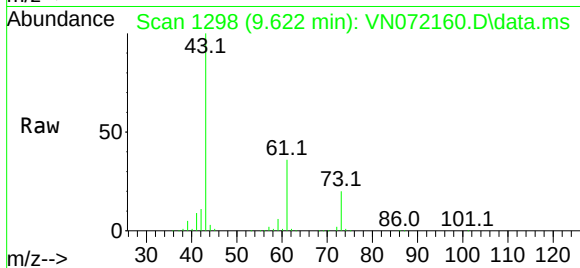

#48

Methyl methacrylate

Concen: 1.507 ug/l

RT: 9.545 min Scan# 1285

Delta R.T. -0.006 min

Lab File: VN072160.D

Acq: 22 Apr 2022 16:34




Tgt Ion: 41 Resp: 8606


Ion Ratio Lower Upper

41 100

69 0.0 74.7 112.1#


39 21.6 45.6 68.4#

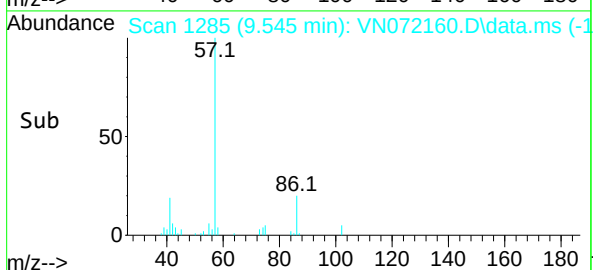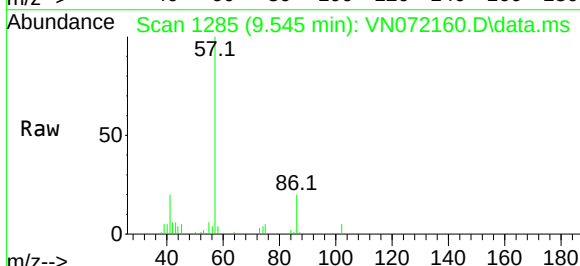






#49
1,4-Dioxane
Concen: Below Cal
RT: 9.616 min Scan# 11
Delta R.T. 0.053 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 88 Resp: 73
Ion Ratio Lower Upper
88 100
43 1772513.7 20.2 30.4#
58 9884.9 54.2 81.4#

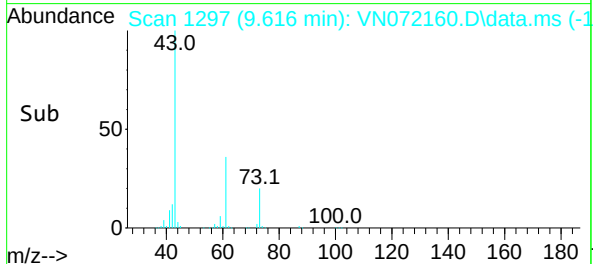

#50
Toluene-d8
Concen: 53.509 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34

Tgt Ion: 98 Resp: 1184831
Ion Ratio Lower Upper
98 100
100 64.8 52.6 78.8

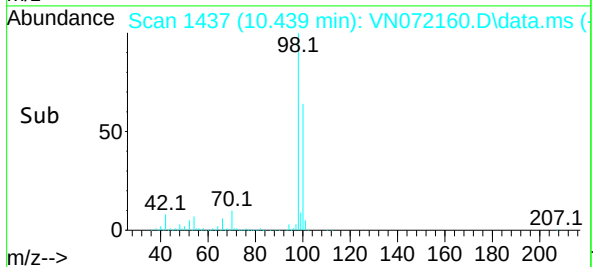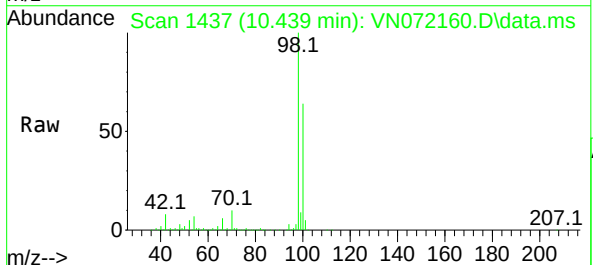



#51

4-Methyl-2-Pentanone

Concen: 0.654 ug/l

RT: 10.333 min Scan# 1419

Delta R.T. 0.011 min

Lab File: VN072160.D

Acq: 22 Apr 2022 16:34

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 43 Resp: 5171

Ion Ratio Lower Upper

43 100

58 65.5 34.1 51.1#

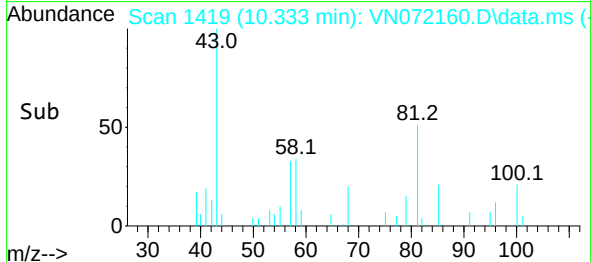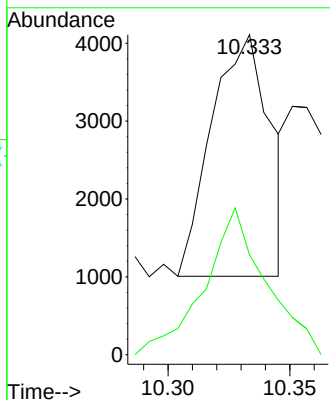

#54

cis-1,3-Dichloropropene

Concen: 5.807 ug/l

RT: 10.239 min Scan# 1403

Delta R.T. 0.053 min

Lab File: VN072160.D

Acq: 22 Apr 2022 16:34




Tgt Ion: 75 Resp: 53613


Ion Ratio Lower Upper

75 100

77 0.0 25.2 37.8#

39 23.2 35.7 53.5#


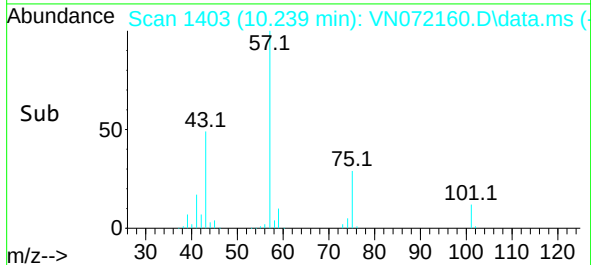
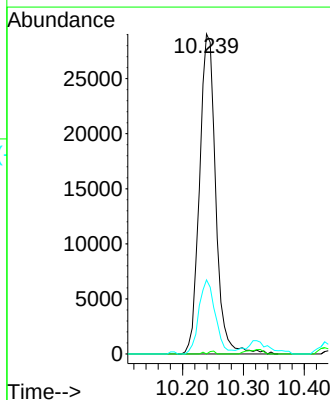
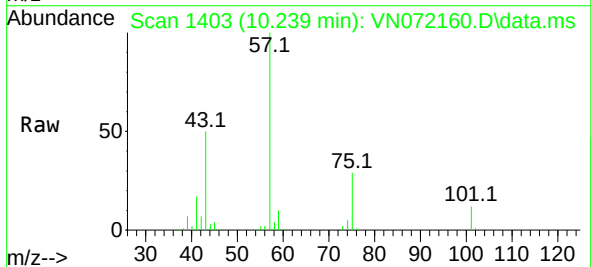




#55
 1,1,2-Trichloroethane
 Concen: 0.304 ug/l
 RT: 10.875 min Scan# 1511
 Delta R.T. -0.017 min
 Lab File: VN072160.D
 Acq: 22 Apr 2022 16:34




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 97	Resp: 1886
Ion Ratio	Lower Upper
97 100	
83 0.0	66.2 99.4#
85 0.0	43.9 65.9#
99 0.0	50.6 76.0#

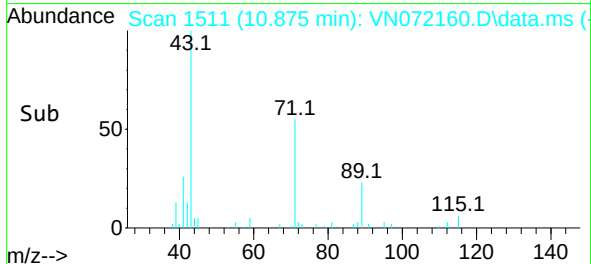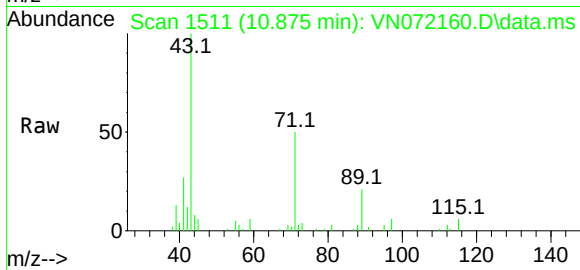

#57
 1,3-Dichloropropane
 Concen: 2.406 ug/l
 RT: 11.086 min Scan# 1547
 Delta R.T. 0.047 min
 Lab File: VN072160.D
 Acq: 22 Apr 2022 16:34

Tgt Ion: 76	Resp: 24995
Ion Ratio	Lower Upper
76 100	
78 0.6	26.2 39.2#




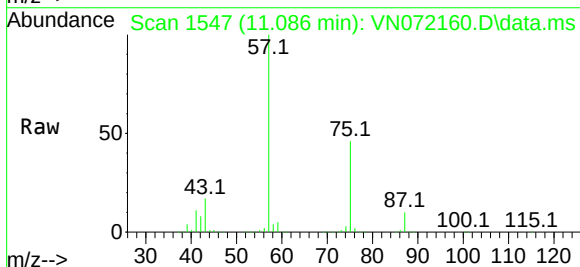




#59
2-Hexanone
Concen: 53.111 ug/l
RT: 11.086 min Scan# 11
Delta R.T. 0.005 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 295854
Ion Ratio Lower Upper
43 100
58 21.1 29.7 89.1#

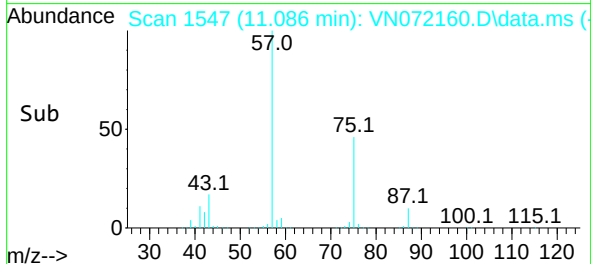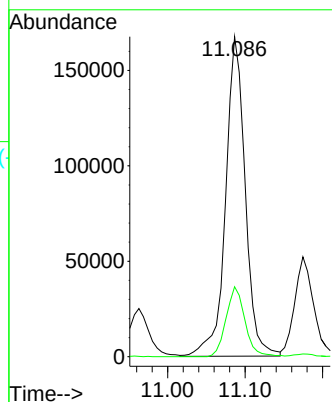

#62
4-Bromofluorobenzene
Concen: 57.310 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34

Tgt Ion: 95 Resp: 410415
Ion Ratio Lower Upper
95 100
174 89.4 0.0 167.6
176 86.9 0.0 163.4




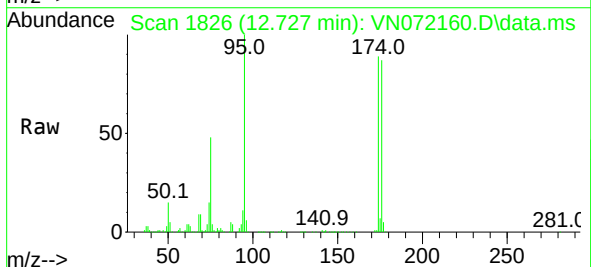




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 996989
Ion Ratio Lower Upper
117 100
82 54.1 44.2 66.2
119 32.0 25.4 38.0

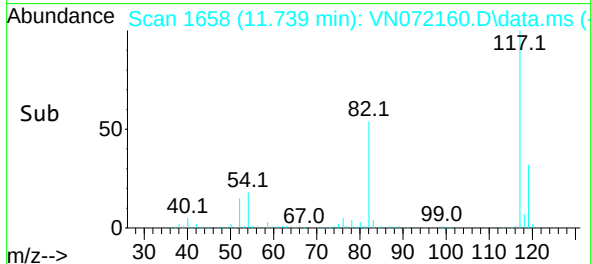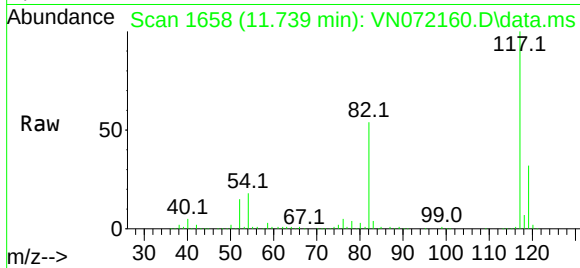

#68
m/p-Xylenes
Concen: 0.217 ug/l
RT: 11.945 min Scan# 1693
Delta R.T. -0.006 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34

Tgt Ion:106 Resp: 2823
Ion Ratio Lower Upper
106 100
91 173.7 158.9 238.3




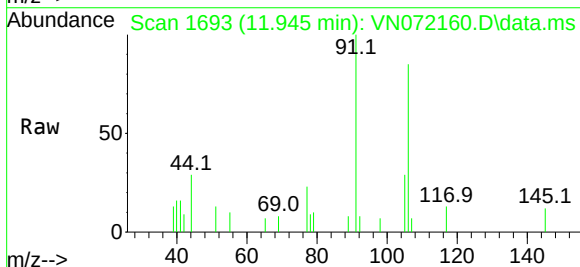




#69
o-Xylene
Concen: 0.250 ug/l
RT: 12.280 min Scan# 11
Delta R.T. 0.005 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:106 Resp: 3227
Ion Ratio Lower Upper
106 100
91 201.7 106.0 318.0

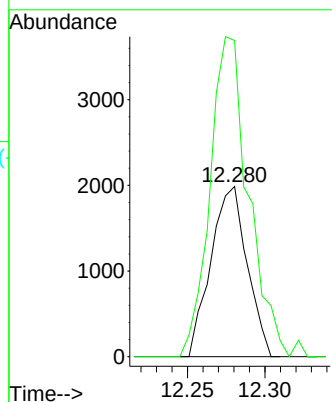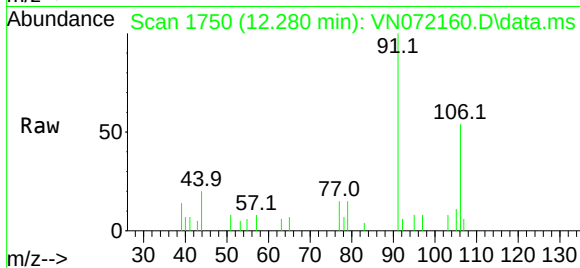

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.669 min Scan# 1986
Delta R.T. -0.000 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34

Tgt Ion:152 Resp: 385669
Ion Ratio Lower Upper
152 100
115 55.1 28.9 86.7
150 155.4 0.0 356.2

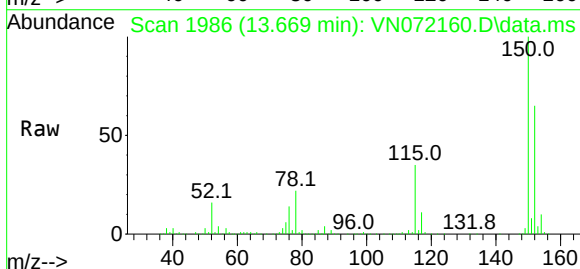



#73

Isopropylbenzene

Concen: 0.774 ug/l

RT: 12.574 min Scan# 1800

Delta R.T. -0.001 min

Lab File: VN072160.D

Acq: 22 Apr 2022 16:34

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:105 Resp: 25163

Ion Ratio Lower Upper

105 100

120 27.8 13.5 40.4

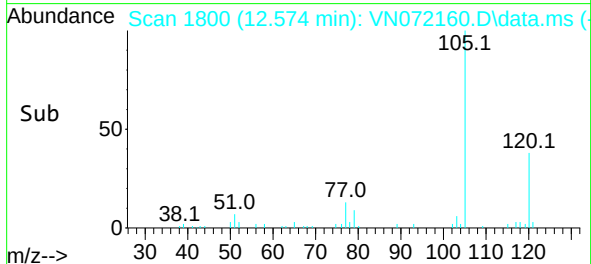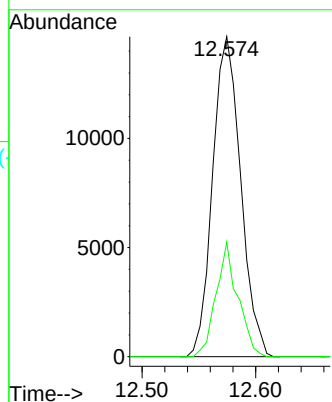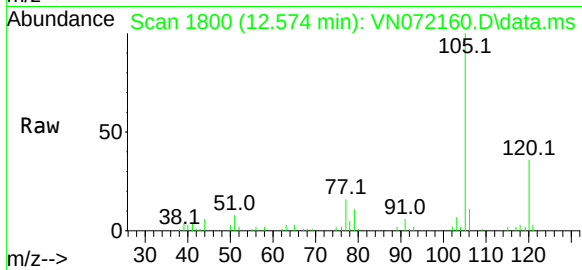

#76

1,2,3-Trichloropropane

Concen: 21.674 ug/l

RT: 12.727 min Scan# 1826

Delta R.T. -0.147 min

Lab File: VN072160.D




Acq: 22 Apr 2022 16:34


Tgt Ion: 75 Resp: 193640

Ion Ratio Lower Upper

75 100


77 1.5 98.5 295.5#

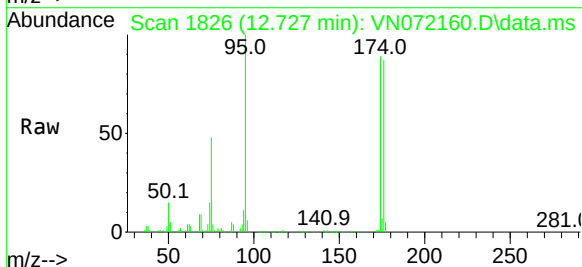



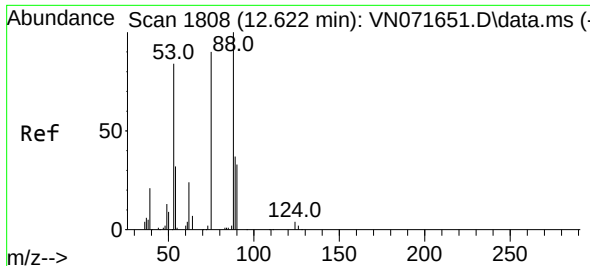


#81
trans-1,4-Dichloro-2-butene
Concen: 67.166 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.105 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34


Instrument :
MSVOA_N
ClientSampleId :

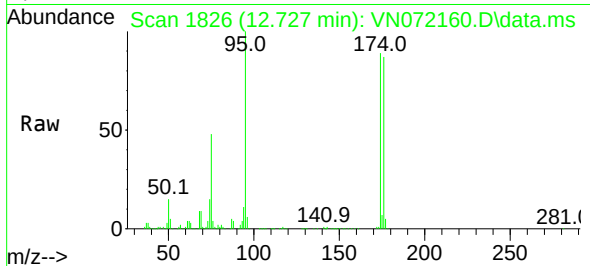



Tgt Ion: 75 Resp: 193640
Ion Ratio Lower Upper
75 100
53 0.1 78.0 117.0#
89 0.0 37.2 55.8#

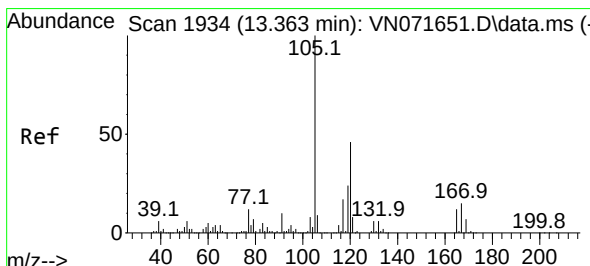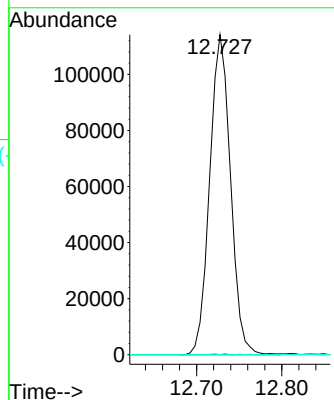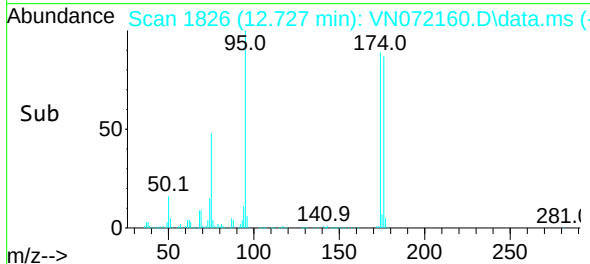


#84
1,2,4-Trimethylbenzene
Concen: 0.992 ug/l
RT: 13.363 min Scan# 1934
Delta R.T. -0.000 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34

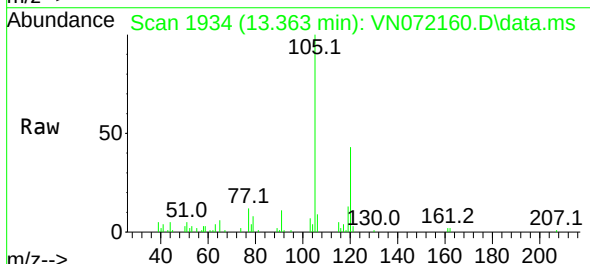

Tgt Ion: 105 Resp: 24912
Ion Ratio Lower Upper
105 100
120 44.5 23.3 69.8



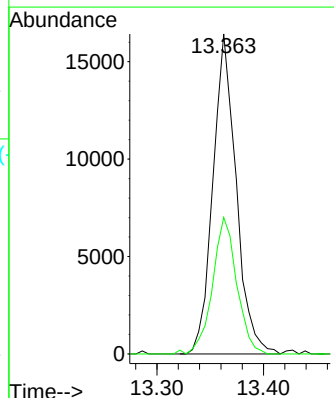
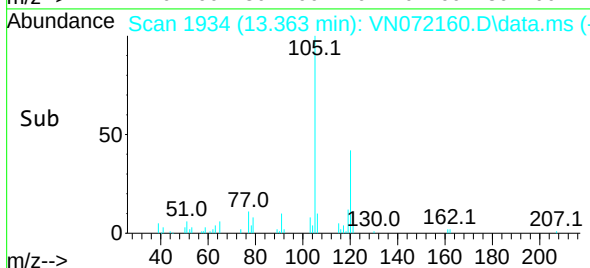


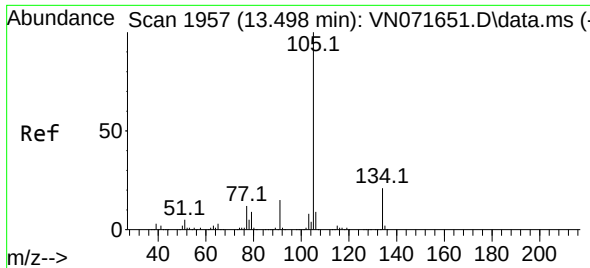

#85
 sec-Butylbenzene
 Concen: 0.425 ug/l
 RT: 13.492 min Scan# 1956
 Delta R.T. -0.006 min
 Lab File: VN072160.D
 Acq: 22 Apr 2022 16:34




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion:105 Resp: 12957
 Ion Ratio Lower Upper
 105 100
 134 33.7 10.4 31.1#

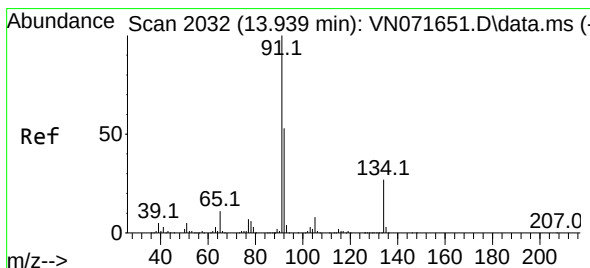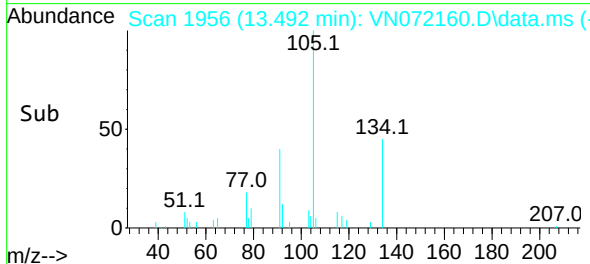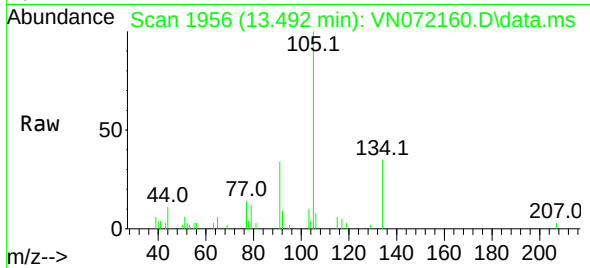

#89
 n-Butylbenzene
 Concen: 0.249 ug/l
 RT: 13.933 min Scan# 2031
 Delta R.T. -0.006 min
 Lab File: VN072160.D
 Acq: 22 Apr 2022 16:34

Tgt Ion: 91 Resp: 4502
 Ion Ratio Lower Upper
 91 100
 92 57.1 26.9 80.7
 134 0.0 13.6 40.8#


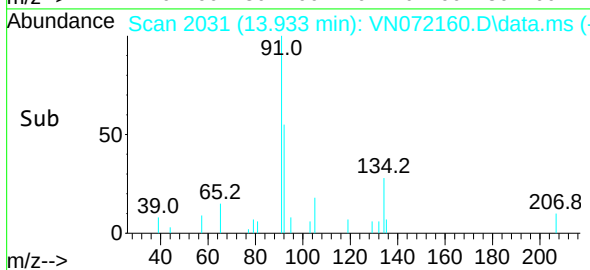

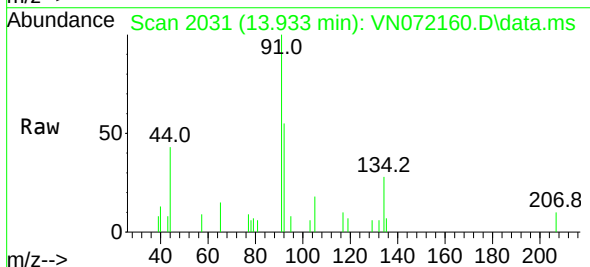




#90
Hexachloroethane
Concen: 0.651 ug/l
RT: 14.216 min Scan# 2077
Delta R.T. 0.012 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 2900
Ion Ratio Lower Upper
117 100
201 0.0 40.6 122.0#

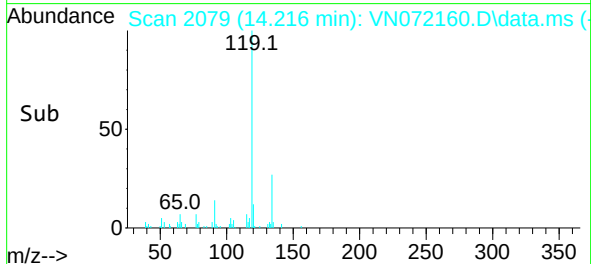

#93
1,2,4-Trichlorobenzene
Concen: 2.153 ug/l
RT: 15.263 min Scan# 2257
Delta R.T. 0.006 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34


Tgt Ion:180 Resp: 429
Ion Ratio Lower Upper
180 100
182 56.9 47.5 142.5
145 0.0 14.5 43.5#

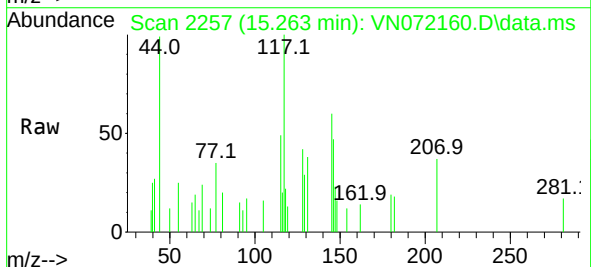



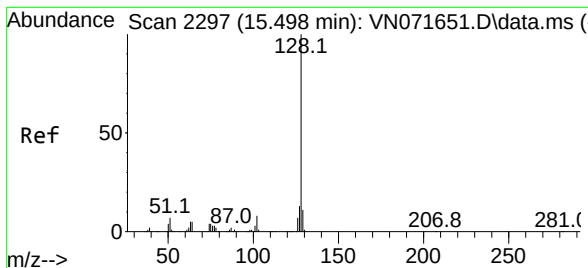


#95
Naphthalene
Concen: 4.015 ug/l
RT: 15.504 min Scan# 21
Delta R.T. 0.006 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34


Instrument :
MSVOA_N
ClientSampleId :

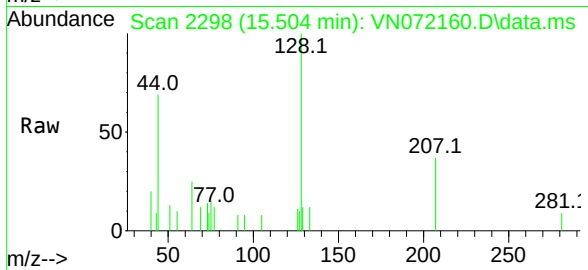

Tgt Ion:128 Resp: 4037
Ion Ratio Lower Upper
128 100
127 0.0 10.3 15.5#
129 9.7 8.6 13.0

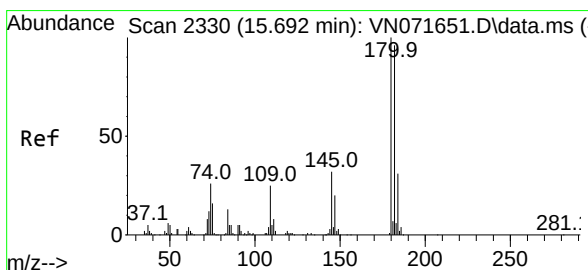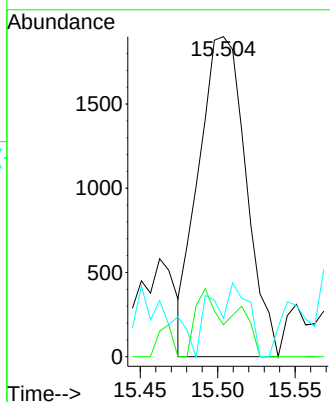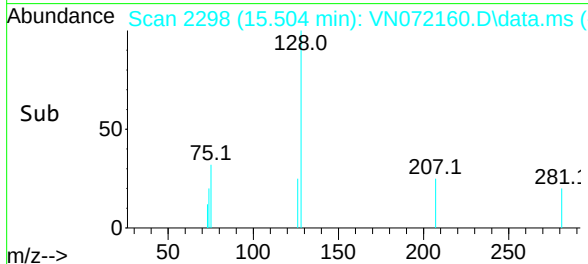

#96
1,2,3-Trichlorobenzene
Concen: 2.482 ug/l
RT: 15.680 min Scan# 2328
Delta R.T. -0.012 min
Lab File: VN072160.D
Acq: 22 Apr 2022 16:34

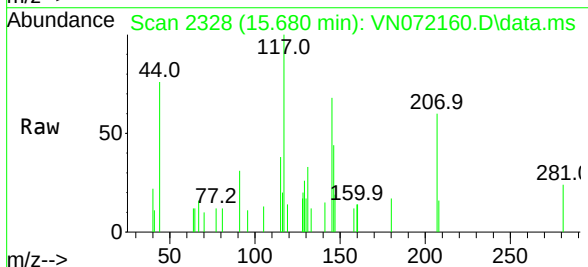

Tgt Ion:180 Resp: 422
Ion Ratio Lower Upper
180 100
182 90.3 47.8 143.3
145 1283.9 15.5 46.5#

